

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040422\
 Data File : PL073806.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Apr 2022 17:42
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 05 01:27:34 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 04:12:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.640	5.492	6989131	35142942	21.822	21.412
28)	SA Decachlor...	10.413	11.334	8597712	26841263	16.908	15.010
Target Compounds							
2)	A alpha-BHC	5.375f	0.000	7359	0	0.018	N.D. #
6)	B beta-BHC	0.000	6.678	0	545828	N.D.	0.524 #
7)	B delta-BHC	0.000	6.958	0	1837340	N.D.	0.853 #
10)	B gamma-Chl...	0.000	8.199	0	217308	N.D.	0.106 #
11)	B alpha-Chl...	0.000	8.259f	0	1792	N.D.	0.001 #
14)	MA Endrin	8.088f	0.000	368020	0	0.948	N.D. #
15)	B Endosulfa...	8.354f	0.000	36752	0	0.094	N.D. #
16)	A 4,4'-DDD	0.000	8.991	0	39991	N.D.	0.027 #
18)	B Endrin al...	8.559	9.202	28540	118595	0.090	0.097
23)	Chlordane-1	0.000	6.856	0	735291	N.D.	10.764 #
25)	Chlordane-3	0.000	8.199	0	217308	N.D.	0.801 #
26)	Chlordane-4	0.000	8.259f	0	1792	N.D.	0.005 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040422\
Data File : PL073806.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Apr 2022 17:42
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 05 01:27:34 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 04:12:46 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

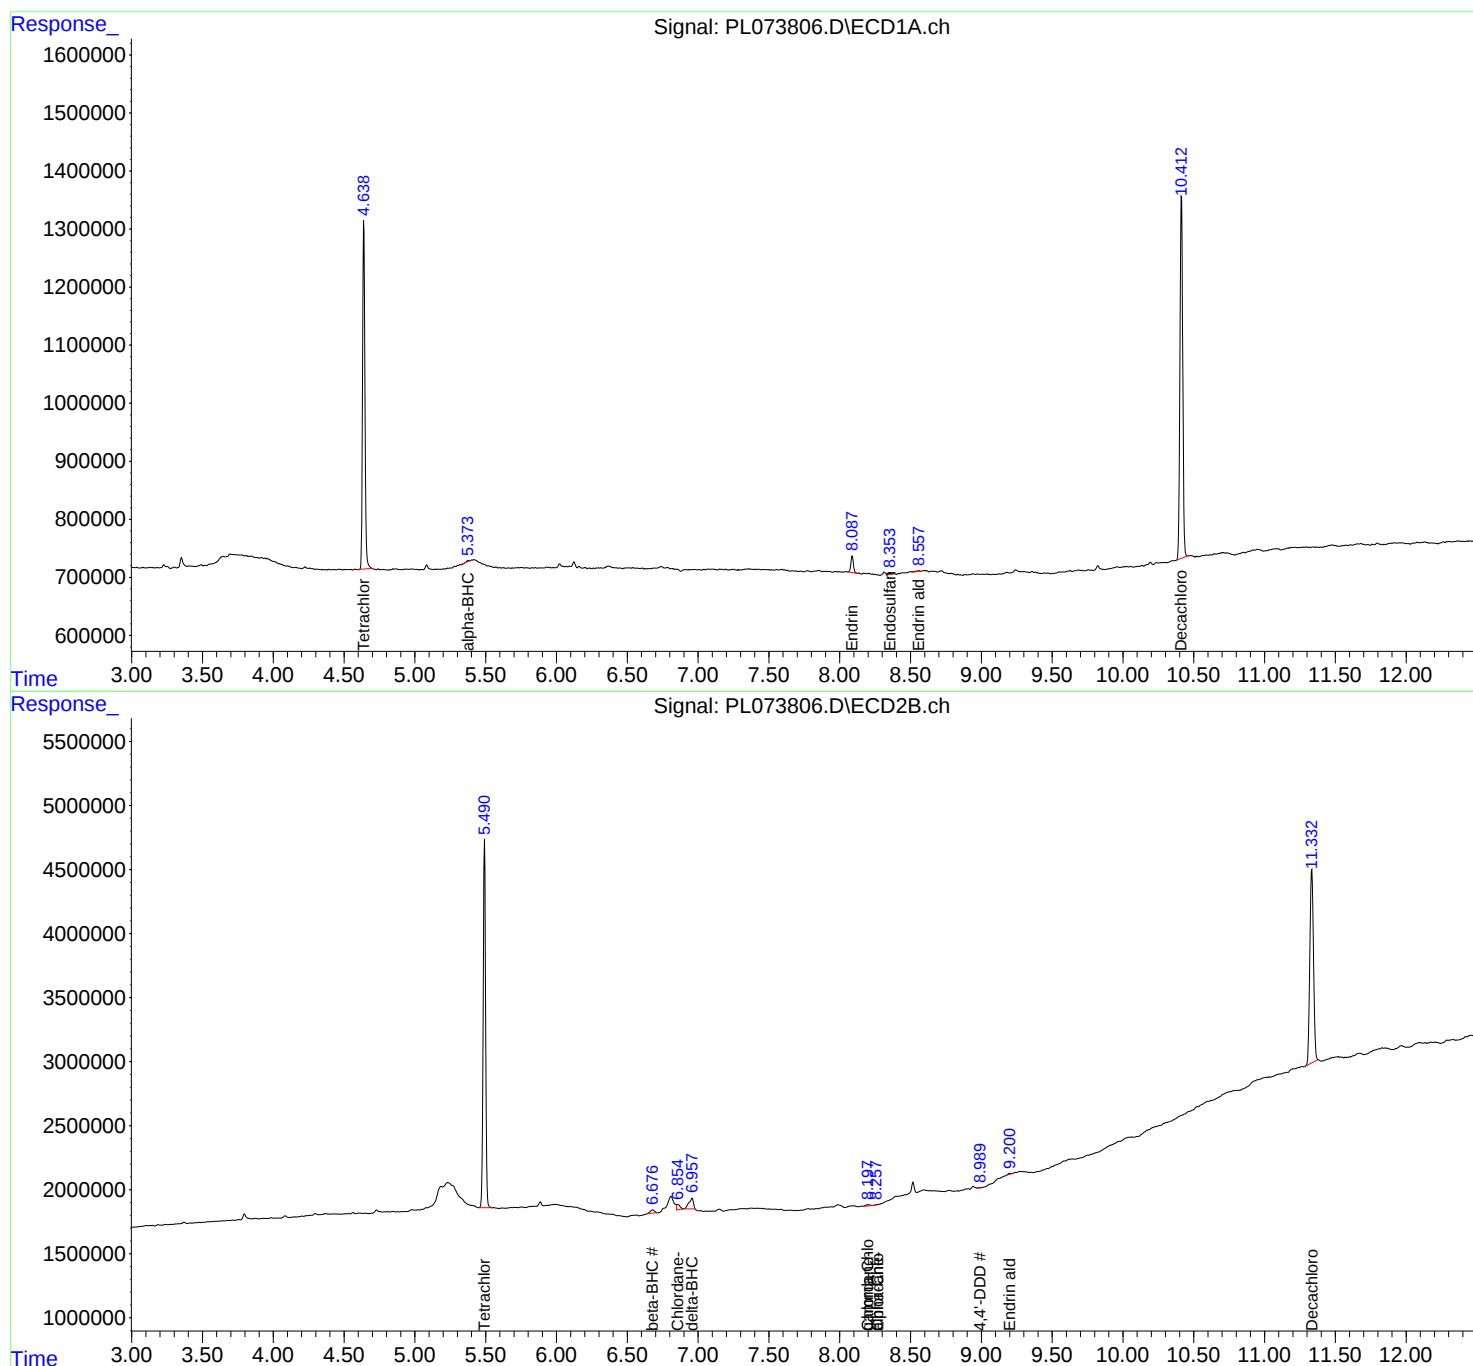


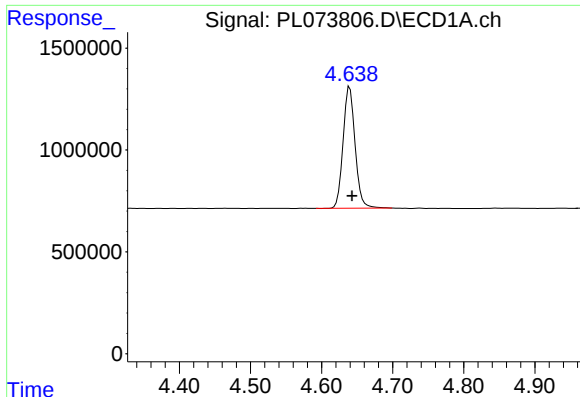

#1 Tetrachloro-m-xylene


R.T.: 4.640 min
Delta R.T.: -0.003 min
Response: 6989131
Conc: 21.82 ng/ml

Instrument :
ECD_L
ClientSampleId :

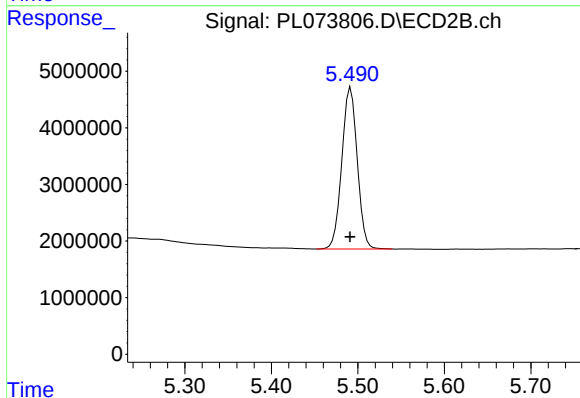


#1 Tetrachloro-m-xylene

R.T.: 5.492 min
Delta R.T.: 0.000 min
Response: 35142942
Conc: 21.41 ng/ml

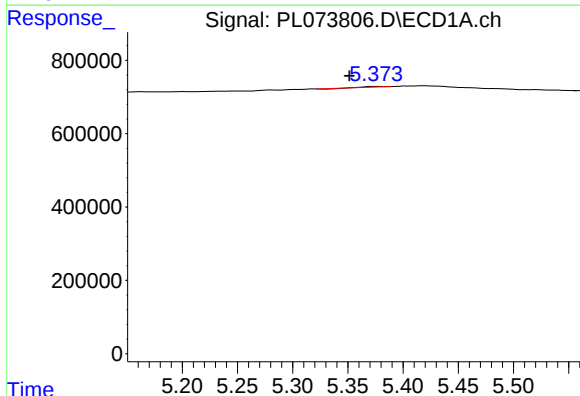


#2 alpha-BHC

R.T.: 5.375 min
Delta R.T.: 0.023 min
Response: 7359
Conc: 0.02 ng/ml

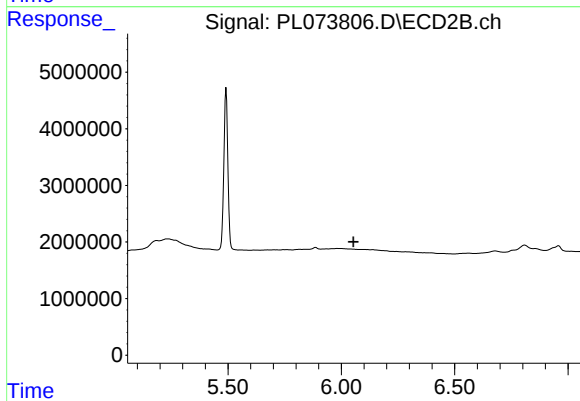

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 6.054 min
Response: 0
Conc: N.D.

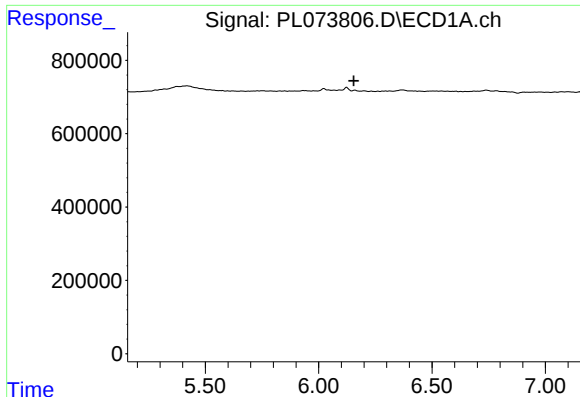

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 6.155 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

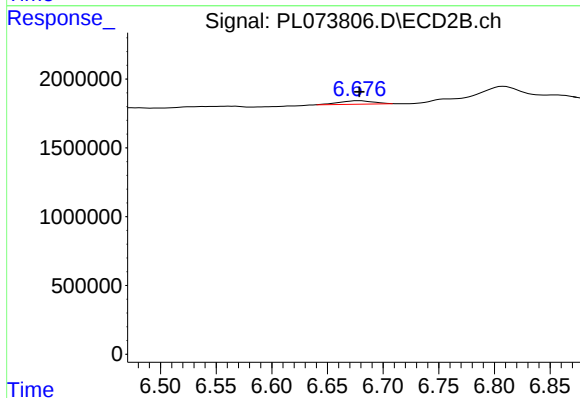


#6 beta-BHC

R.T.: 6.678 min
Delta R.T.: 0.000 min
Response: 545828
Conc: 0.52 ng/ml

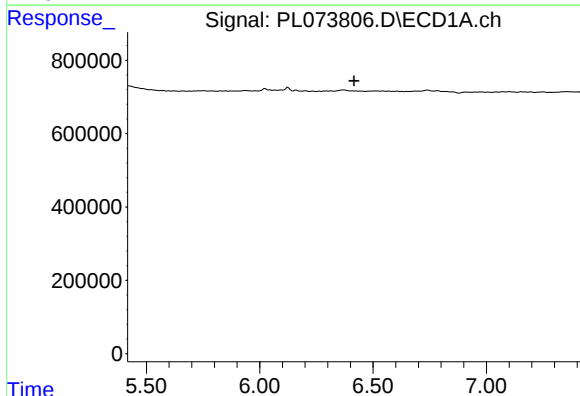


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 6.416 min
Response: 0
Conc: N.D.

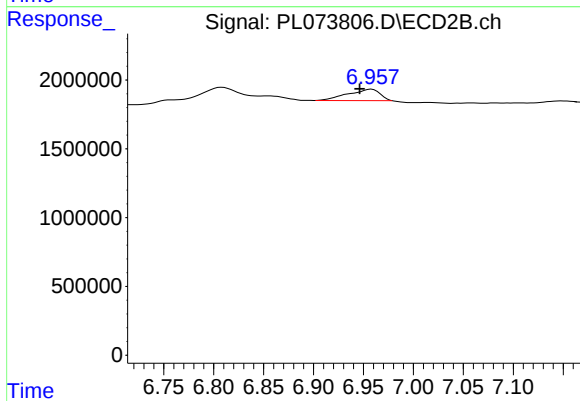

#7 delta-BHC


R.T.: 6.958 min
Delta R.T.: 0.012 min
Response: 1837340
Conc: 0.85 ng/ml

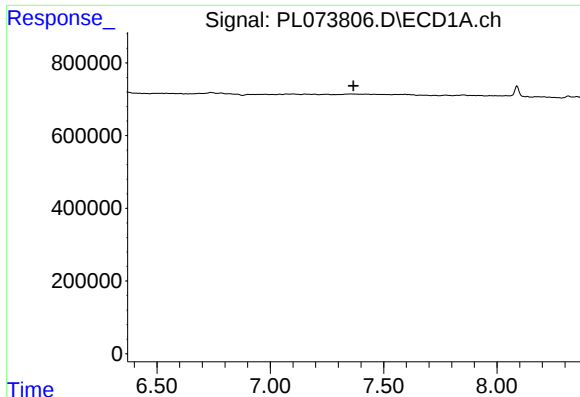

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.368 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

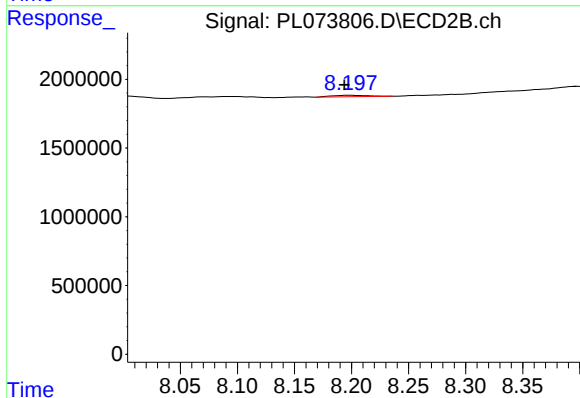


#10 gamma-Chlordane

R.T.: 8.199 min
Delta R.T.: 0.005 min
Response: 217308
Conc: 0.11 ng/ml

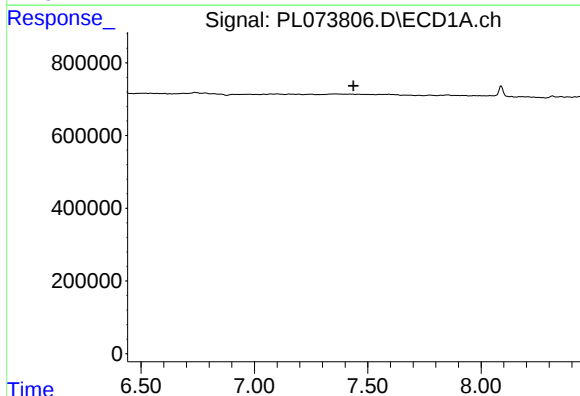


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.437 min
Response: 0
Conc: N.D.

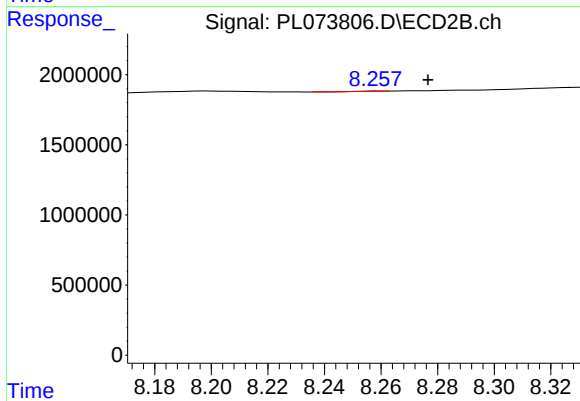

#11 alpha-Chlordane


R.T.: 8.259 min
Delta R.T.: -0.018 min
Response: 1792
Conc: 0.00 ng/ml

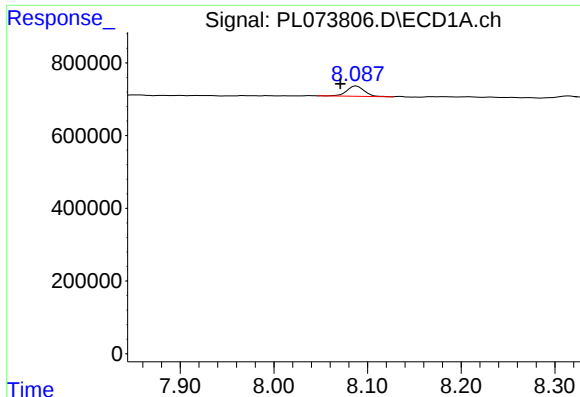

#14 Endrin


R.T.: 8.088 min
Delta R.T.: 0.017 min
Response: 368020
Conc: 0.95 ng/ml

Instrument :
ECD_L
ClientSampleId :

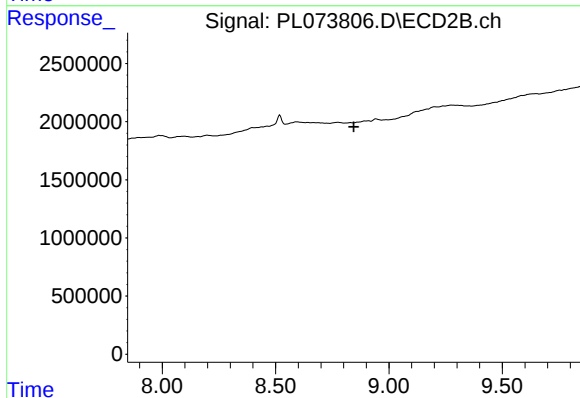


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 8.845 min
Response: 0
Conc: N.D.

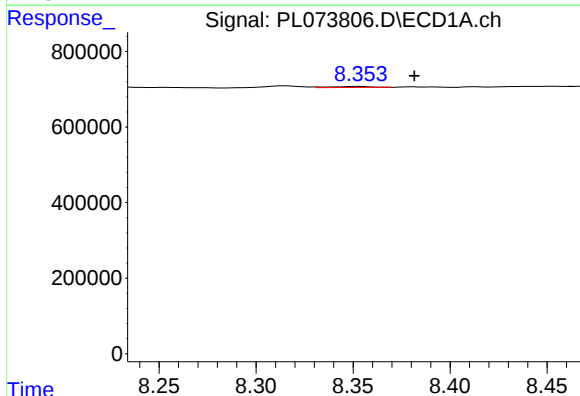


#15 Endosulfan II

R.T.: 8.354 min
Delta R.T.: -0.028 min
Response: 36752
Conc: 0.09 ng/ml

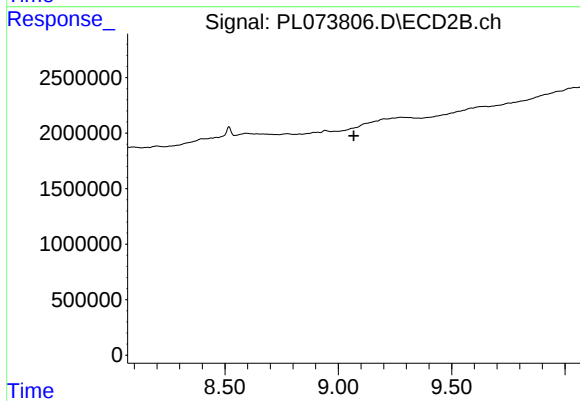

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 9.069 min
Response: 0
Conc: N.D.

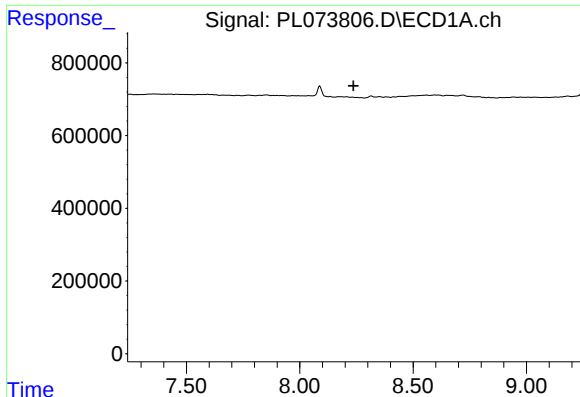

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 8.237 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

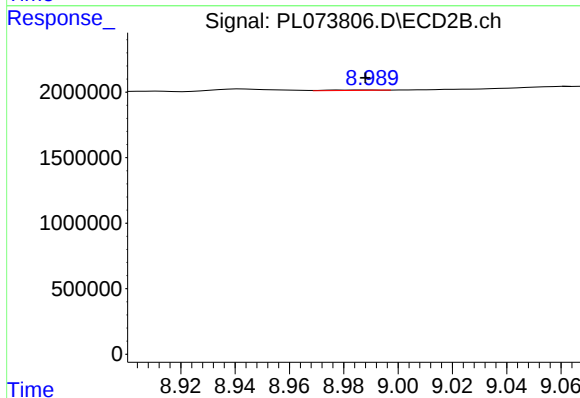


#16 4,4'-DDD

R.T.: 8.991 min
Delta R.T.: 0.003 min
Response: 39991
Conc: 0.03 ng/ml

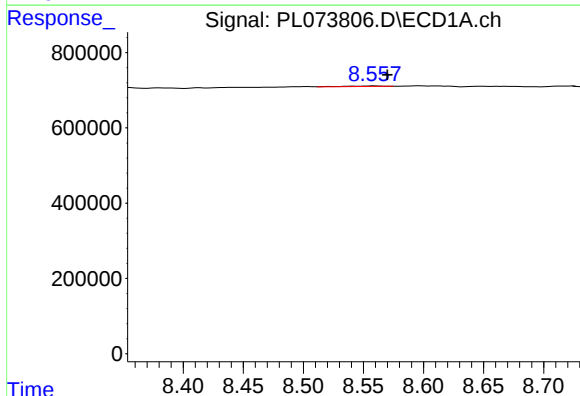


#18 Endrin aldehyde

R.T.: 8.559 min
Delta R.T.: -0.011 min
Response: 28540
Conc: 0.09 ng/ml

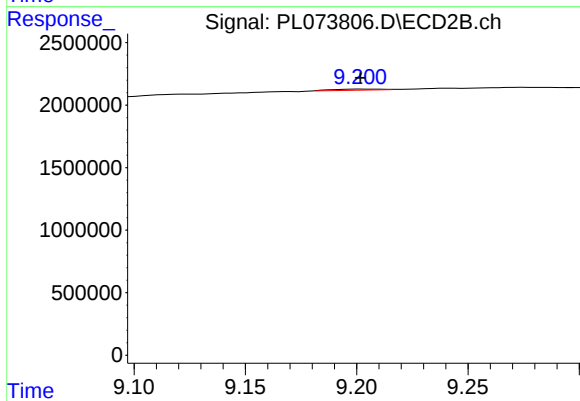

#18 Endrin aldehyde


R.T.: 9.202 min
Delta R.T.: 0.000 min
Response: 118595
Conc: 0.10 ng/ml

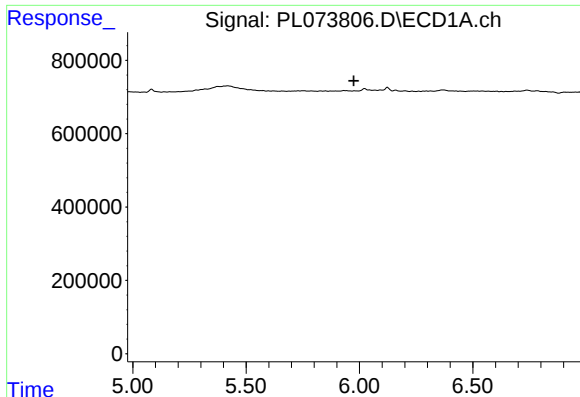

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.976 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

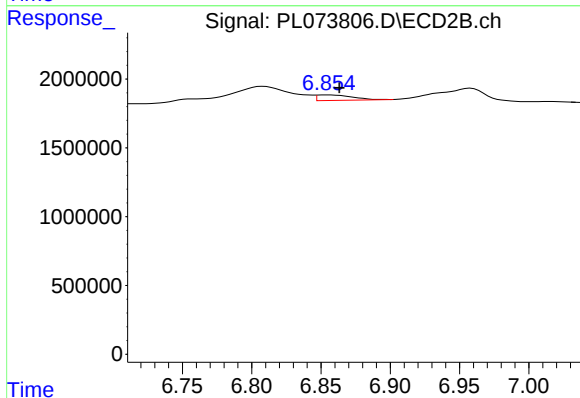


#23 Chlordane-1

R.T.: 6.856 min
Delta R.T.: -0.008 min
Response: 735291
Conc: 10.76 ng/ml

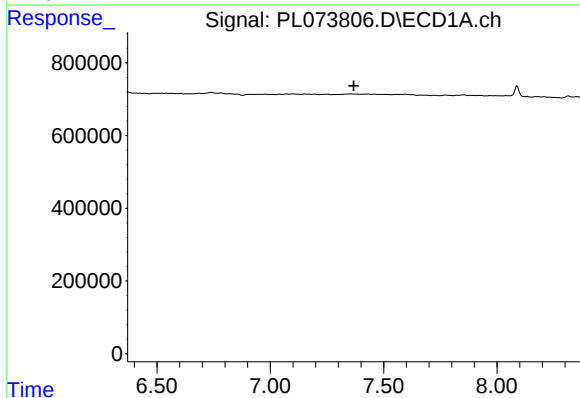


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.368 min
Response: 0
Conc: N.D.

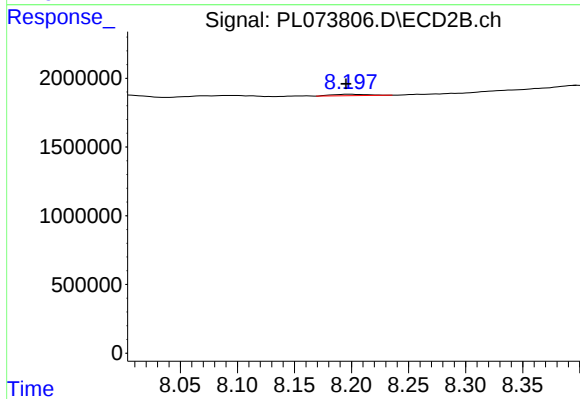

#25 Chlordane-3


R.T.: 8.199 min
Delta R.T.: 0.003 min
Response: 217308
Conc: 0.80 ng/ml

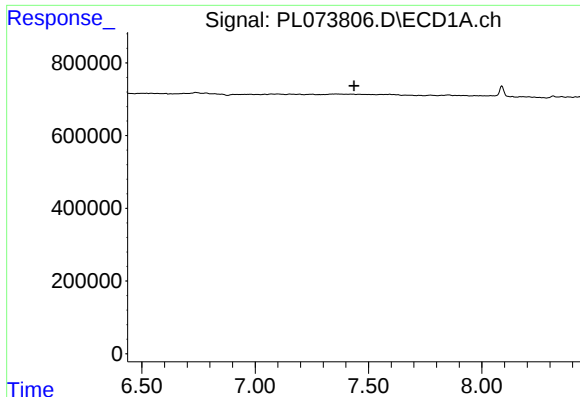

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.437 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

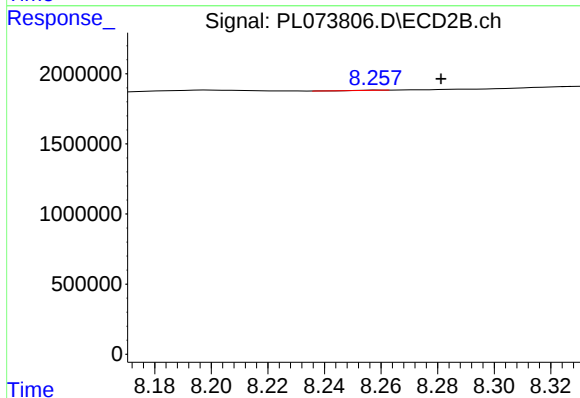


#26 Chlordane-4

R.T.: 8.259 min
Delta R.T.: -0.023 min
Response: 1792
Conc: 0.01 ng/ml

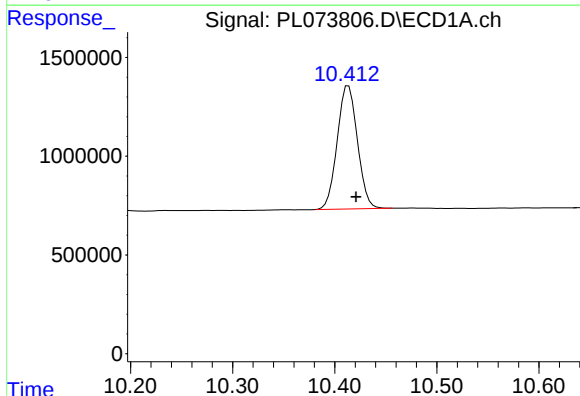

#28 Decachlorobiphenyl

R.T.: 10.413 min
Delta R.T.: -0.008 min
Response: 8597712
Conc: 16.91 ng/ml

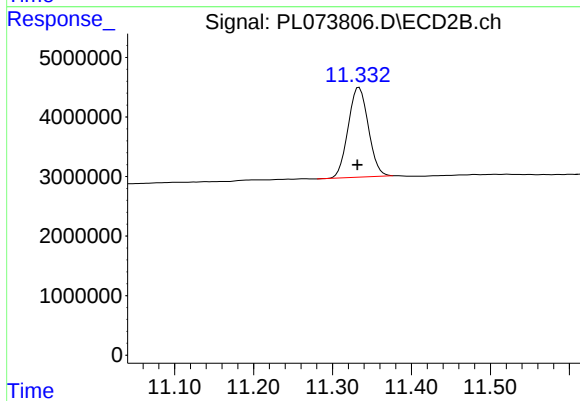

#28 Decachlorobiphenyl

R.T.: 11.334 min
Delta R.T.: 0.002 min
Response: 26841263
Conc: 15.01 ng/ml