

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040519\
 Data File : PL047071.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Apr 2019 14:40
 Operator : AJ\SJ
 Sample : PB118635BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB118635BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 05 23:10:11 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:40:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.362	3.973	137.6E6	40679843	18.911	17.767
28)	SA Decachlor...	8.040	9.028	160.3E6	46615198	19.054	20.106
Target Compounds							
14)	MA Endrin	0.000	6.710f	0	4559894	N.D.	1.908 #
27)	Chlordane-5	0.000	6.984f	0	2441502	N.D.	27.177 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040519\
Data File : PL047071.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Apr 2019 14:40
Operator : AJ\SJ
Sample : PB118635BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB118635BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 05 23:10:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

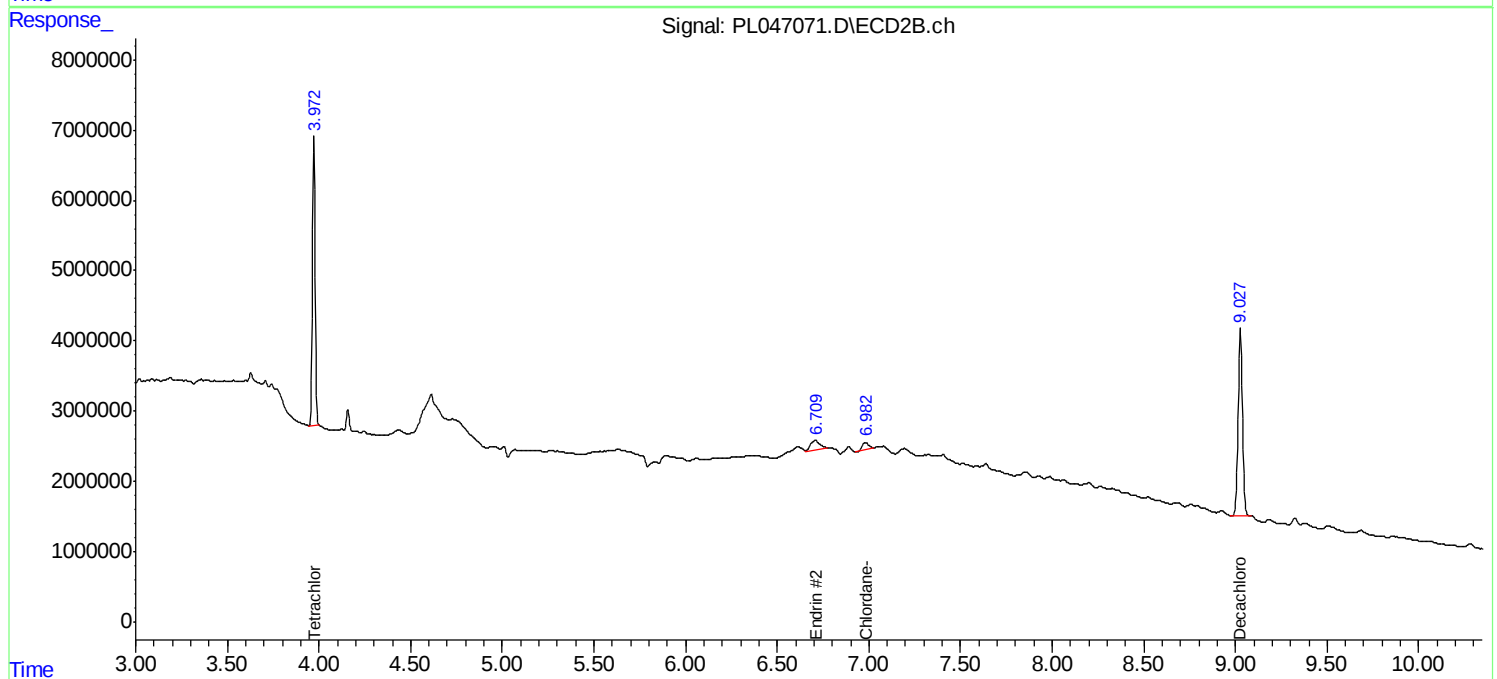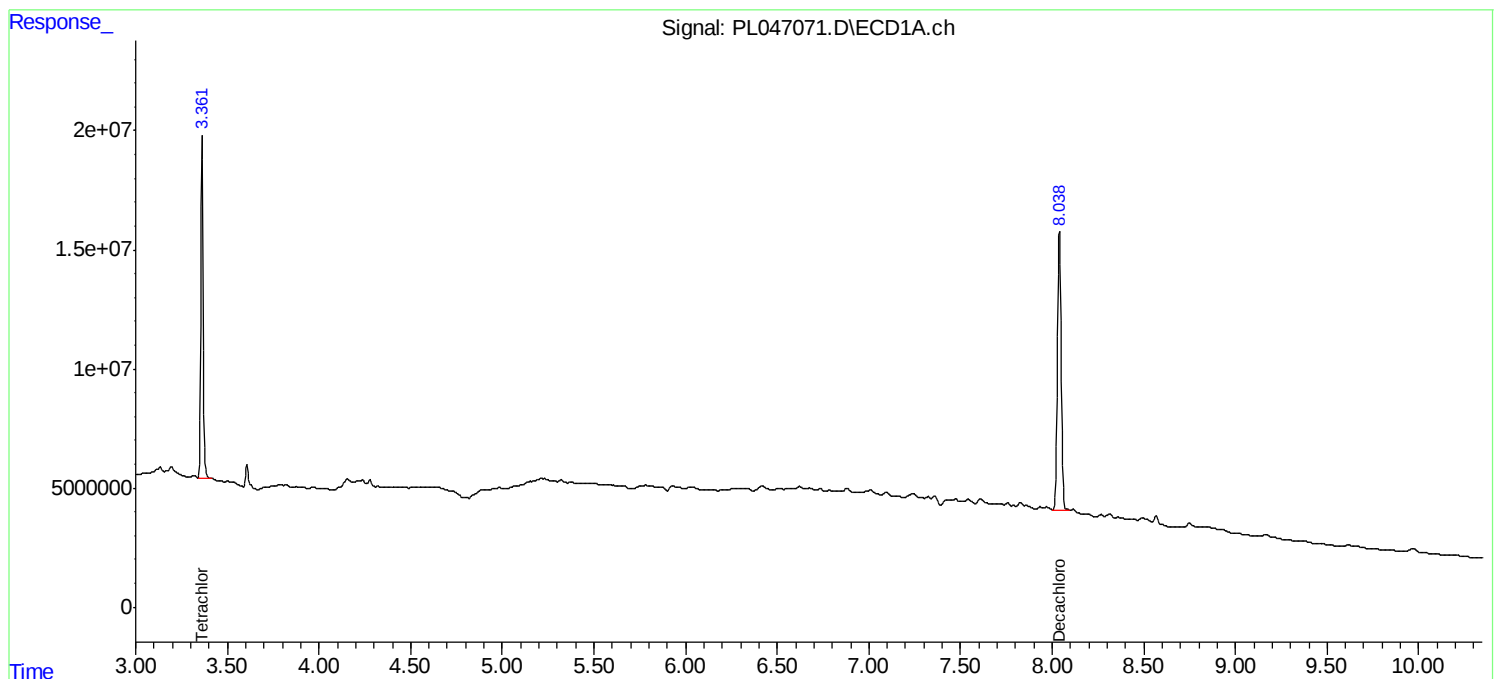


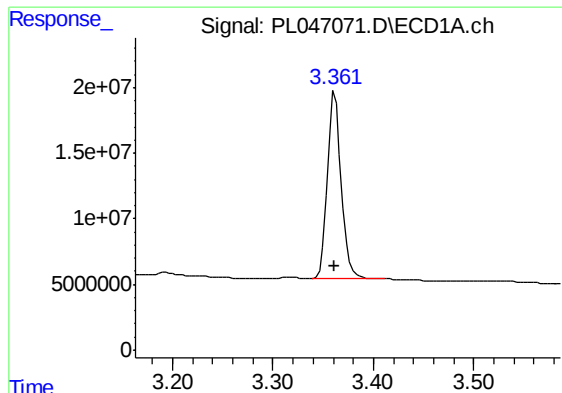

#1 Tetrachloro-m-xylene


R.T.: 3.362 min
Delta R.T.: 0.000 min
Response: 137568076
Conc: 18.91 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB118635BL

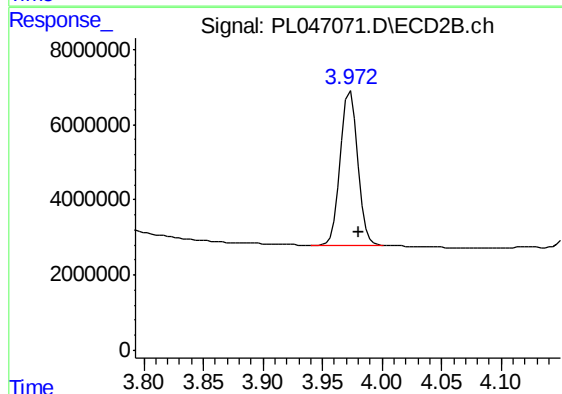


#1 Tetrachloro-m-xylene

R.T.: 3.973 min
Delta R.T.: -0.007 min
Response: 40679843
Conc: 17.77 ng/ml

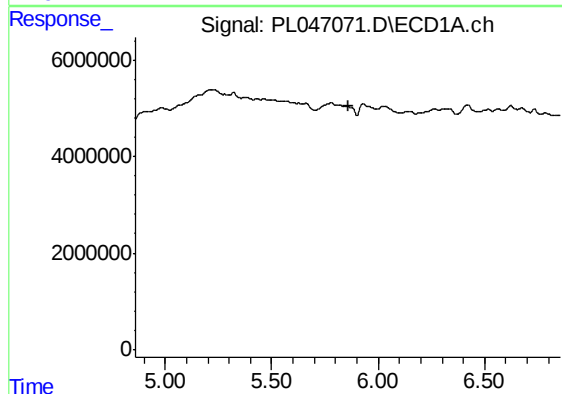


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 5.860 min
Response: 0
Conc: N.D.

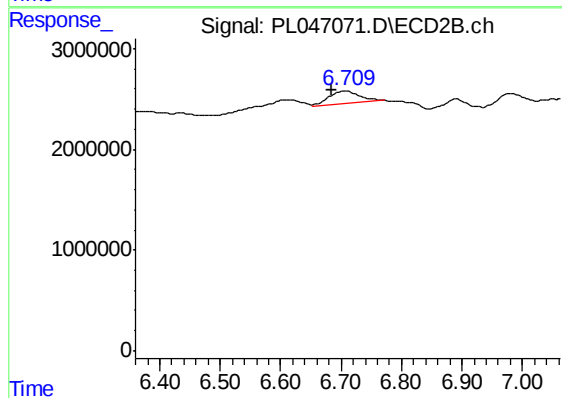

#14 Endrin


R.T.: 6.710 min
Delta R.T.: 0.025 min
Response: 4559894
Conc: 1.91 ng/ml

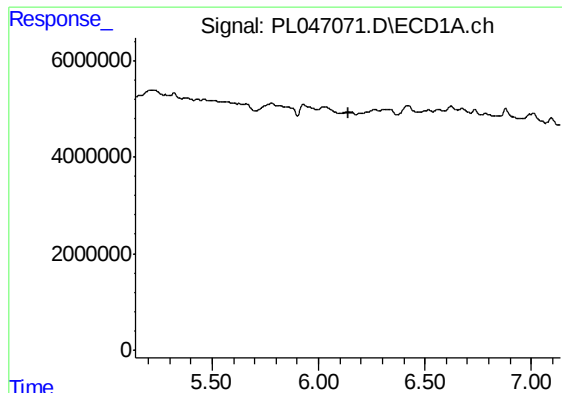

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.139 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB118635BL

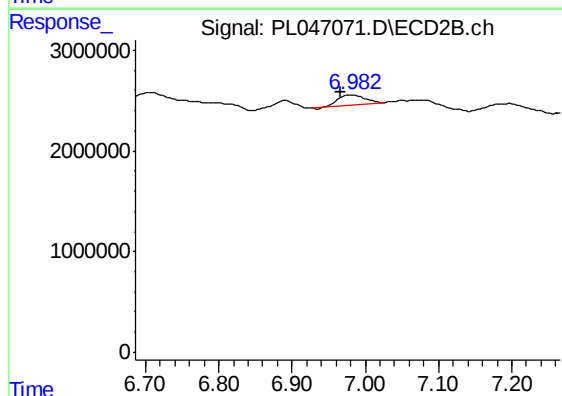


#27 Chlordane-5

R.T.: 6.984 min
Delta R.T.: 0.016 min
Response: 2441502
Conc: 27.18 ng/ml

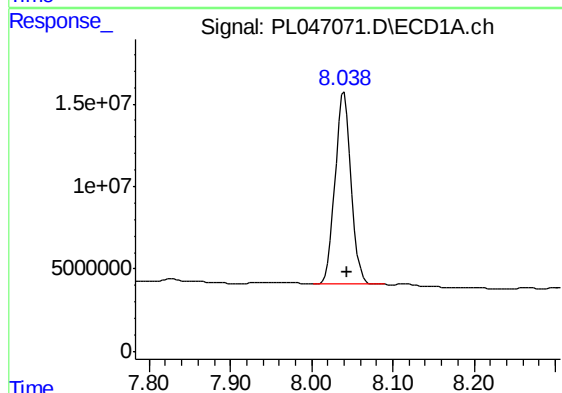

#28 Decachlorobiphenyl

R.T.: 8.040 min
Delta R.T.: -0.004 min
Response: 160265660
Conc: 19.05 ng/ml

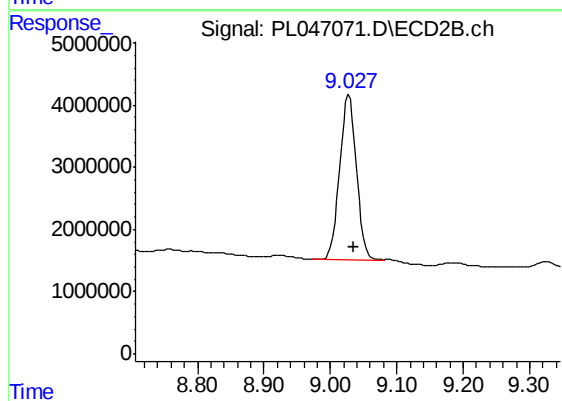

#28 Decachlorobiphenyl

R.T.: 9.028 min
Delta R.T.: -0.007 min
Response: 46615198
Conc: 20.11 ng/ml