

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040519\
 Data File : PL047074.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Apr 2019 15:23
 Operator : AJ\SJ
 Sample : K2193-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HR-06-040319-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 05 23:11:07 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:40:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.357	3.976	151.9E6	46632049	20.887	20.367
28)	SA Decachlor...	8.032	9.026	168.7E6	49177706	20.056	21.211
Target Compounds							
23)	Chlordane-1	4.231f	0.000	8824547	0	26.240	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040519\
Data File : PL047074.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Apr 2019 15:23
Operator : AJ\SJ
Sample : K2193-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HR-06-040319-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 05 23:11:07 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

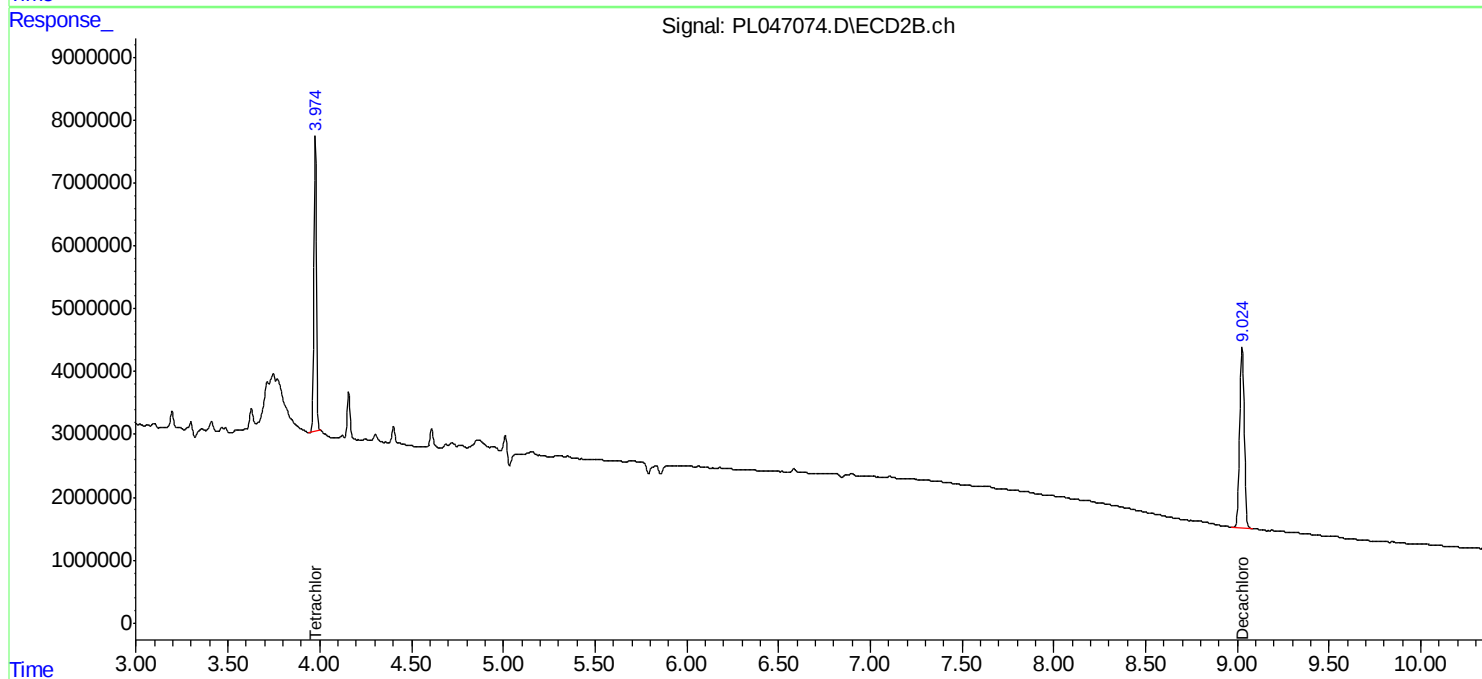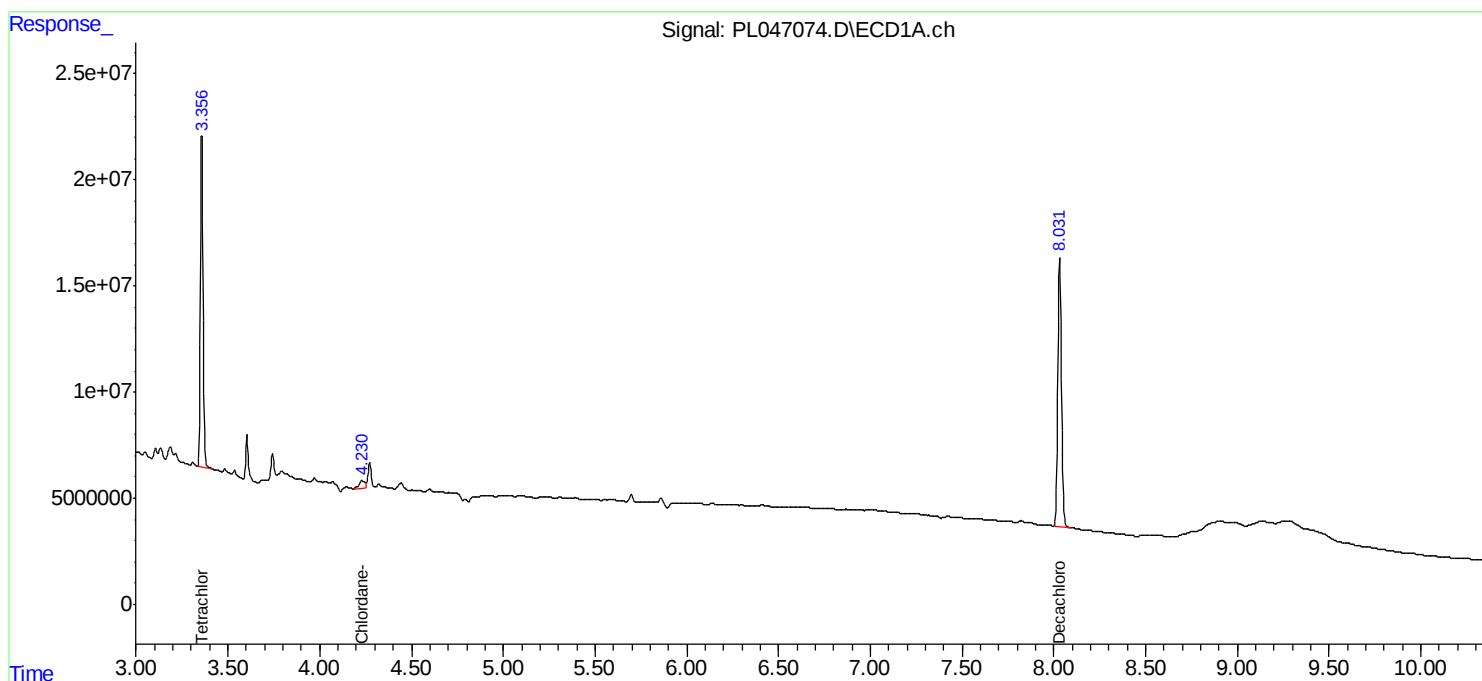


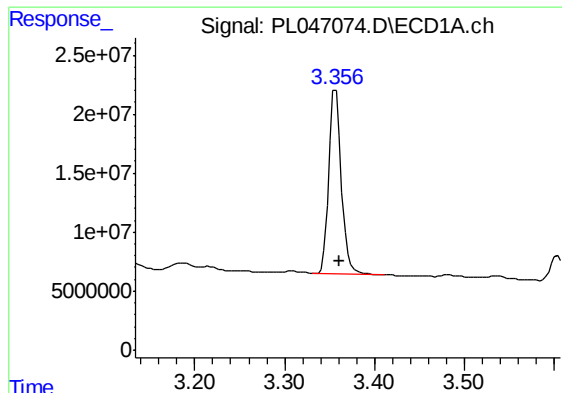

#1 Tetrachloro-m-xylene


R.T.: 3.357 min
Delta R.T.: -0.004 min
Response: 151945781
Conc: 20.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
HR-06-040319-A

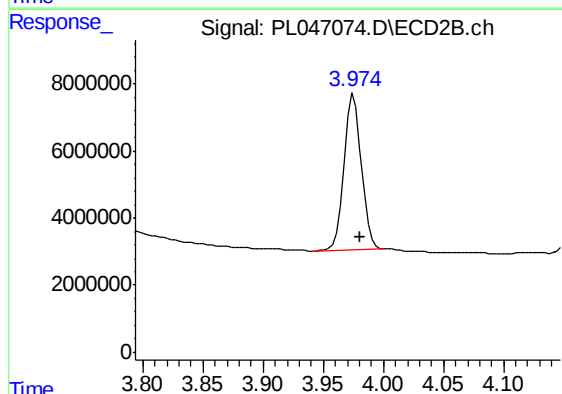


#1 Tetrachloro-m-xylene

R.T.: 3.976 min
Delta R.T.: -0.005 min
Response: 46632049
Conc: 20.37 ng/ml

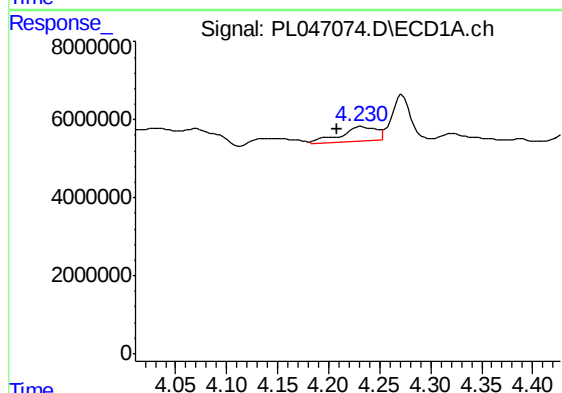


#23 Chlordane-1

R.T.: 4.231 min
Delta R.T.: 0.023 min
Response: 8824547
Conc: 26.24 ng/ml

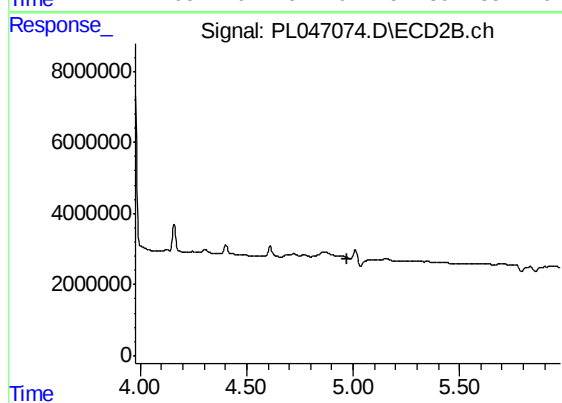

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.975 min
Response: 0
Conc: N.D.

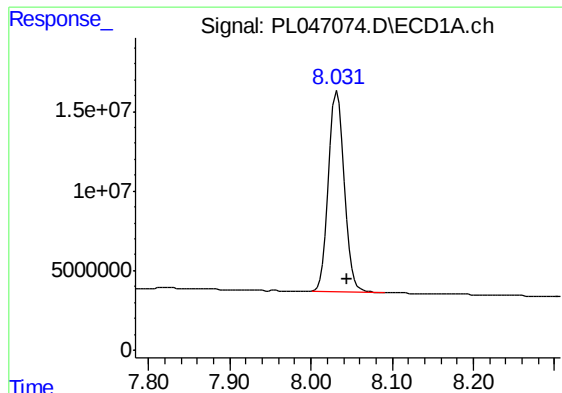

#28 Decachlorobiphenyl

R.T.: 8.032 min
Delta R.T.: -0.012 min
Response: 168695227
Conc: 20.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
HR-06-040319-A

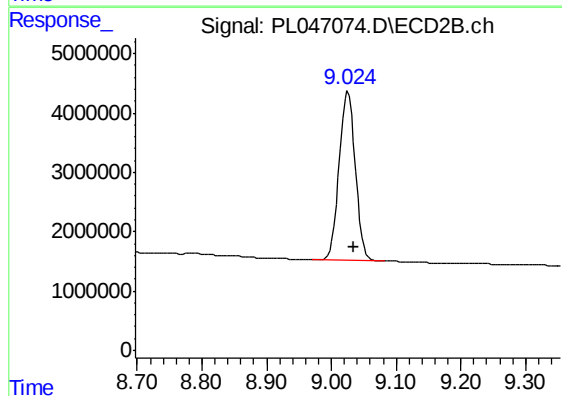

#28 Decachlorobiphenyl

R.T.: 9.026 min
Delta R.T.: -0.009 min
Response: 49177706
Conc: 21.21 ng/ml