

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040521\
 Data File : PL065876.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Apr 2021 14:24
 Operator : AR\AJ
 Sample : M1911-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 05 15:18:46 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 31 15:57:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.276	3.780	29249332	32029958	11.228	11.669
28)	SA Decachlor...	7.909	8.728	26836806	25632385	11.587	11.369
Target Compounds							
2)	A alpha-BHC	0.000	4.192f	0	1867806	N.D.	0.460 #
4)	MA Heptachlor	0.000	4.941	0	858029	N.D.	0.243 #
6)	B beta-BHC	0.000	4.630	0	5185165	N.D.	2.977 #
12)	B 4,4'-DDE	5.369	6.074	450433	599691	0.163	0.230 #
14)	MA Endrin	5.752	0.000	344907	0	0.128	N.D. #
15)	B Endosulfa...	0.000	6.677f	0	489697	N.D.	0.207 #
18)	B Endrin al...	0.000	6.753f	0	136542	N.D.	0.072 #
21)	B Endrin ke...	6.866	0.000	119849	0	0.044	N.D. #
23)	Chlordane-1	4.109	0.000	771572	0	8.551	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040521\
Data File : PL065876.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Apr 2021 14:24
Operator : AR\AJ
Sample : M1911-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 05 15:18:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
Quant Title : GC Extractables
QLast Update : Wed Mar 31 15:57:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

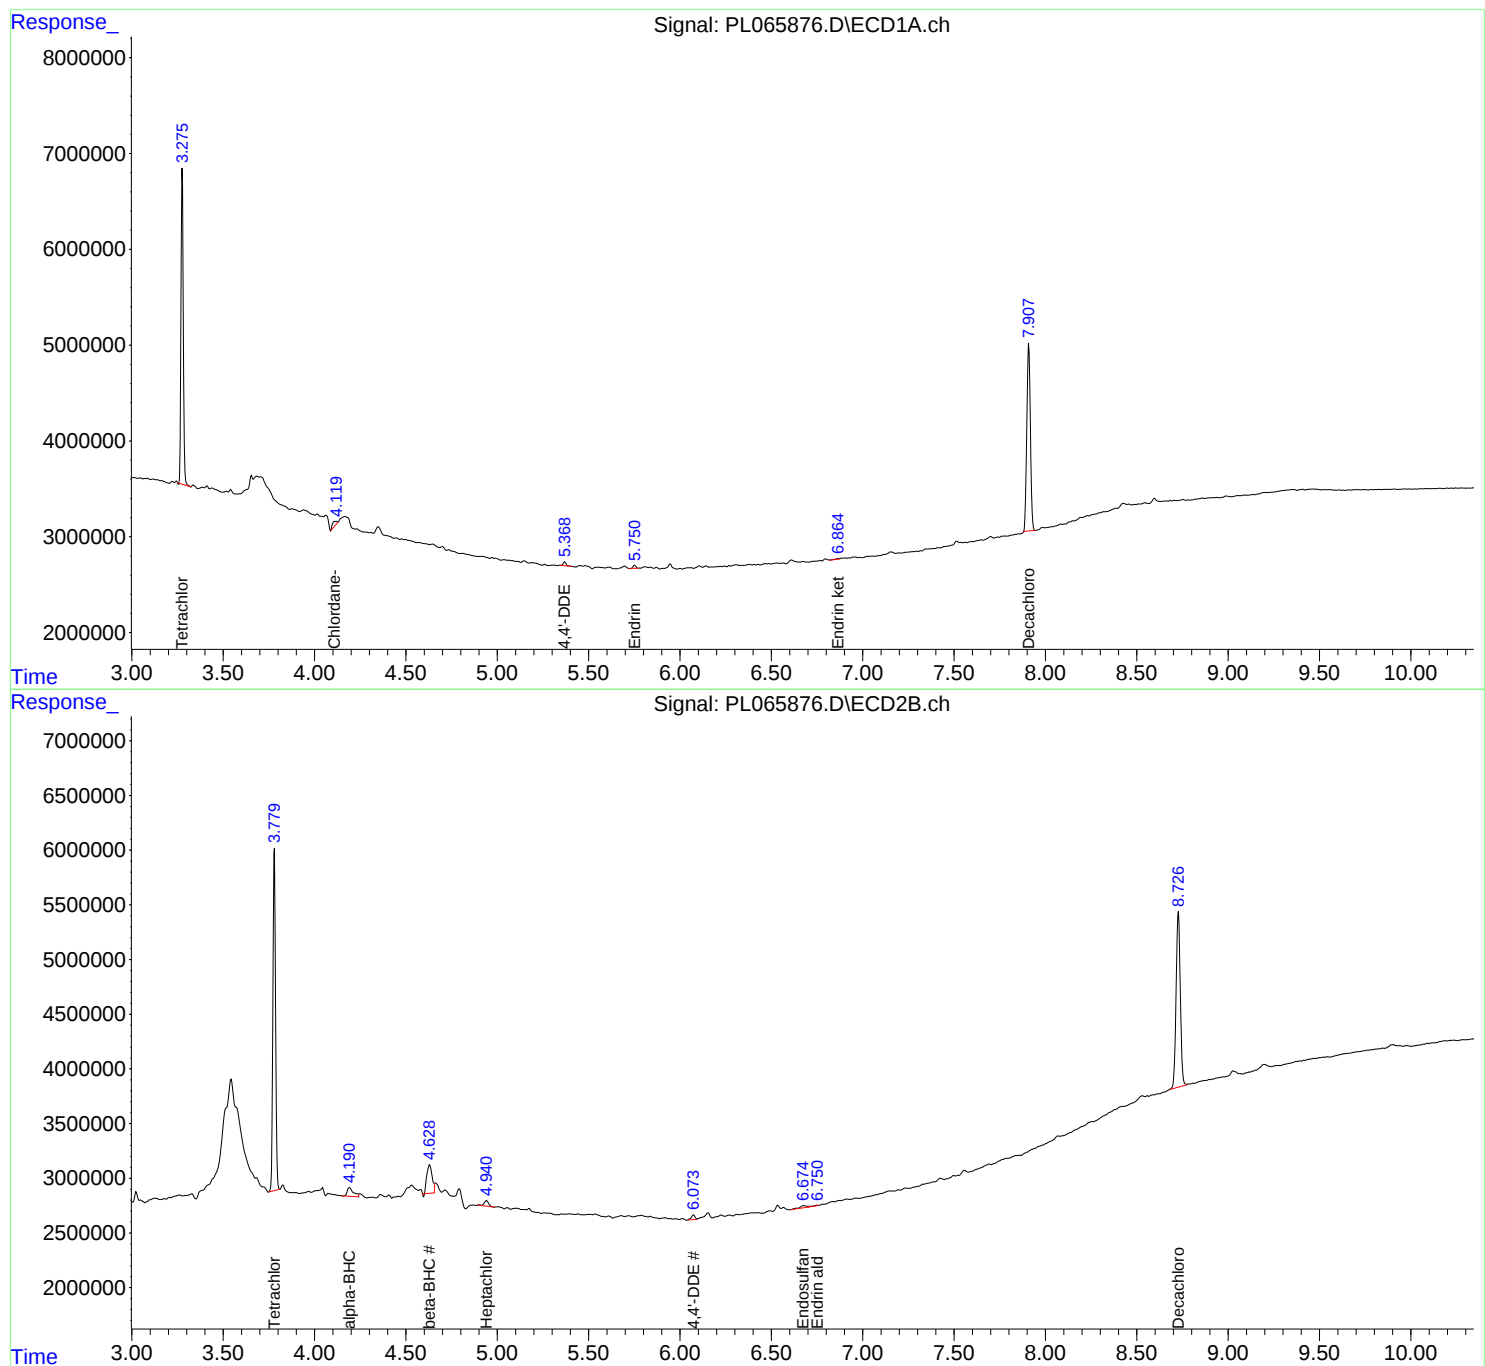


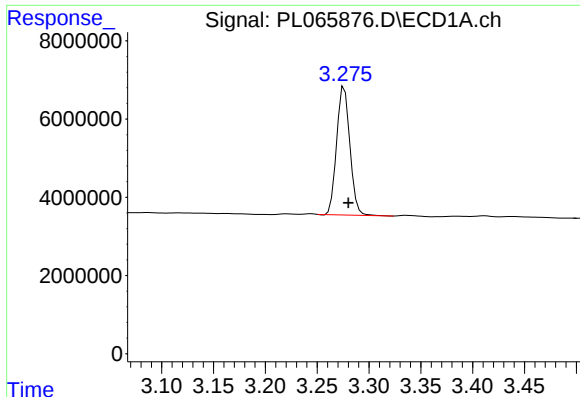

#1 Tetrachloro-m-xylene


R.T.: 3.276 min
Delta R.T.: -0.004 min
Response: 29249332
Conc: 11.23 ng/ml

Instrument :
ECD_L
ClientSampleId :

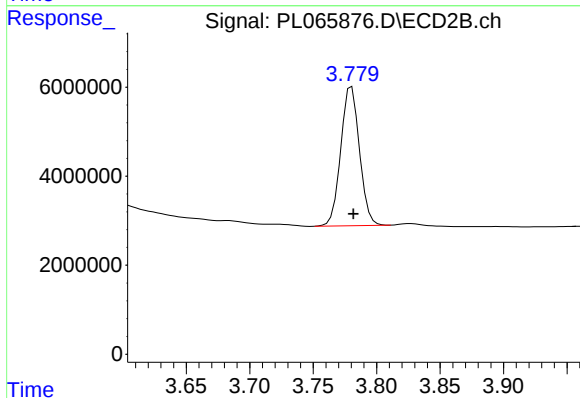


#1 Tetrachloro-m-xylene

R.T.: 3.780 min
Delta R.T.: -0.001 min
Response: 32029958
Conc: 11.67 ng/ml

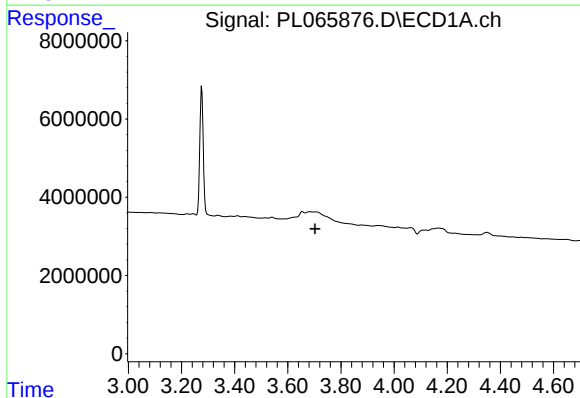


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.703 min
Response: 0
Conc: N.D.

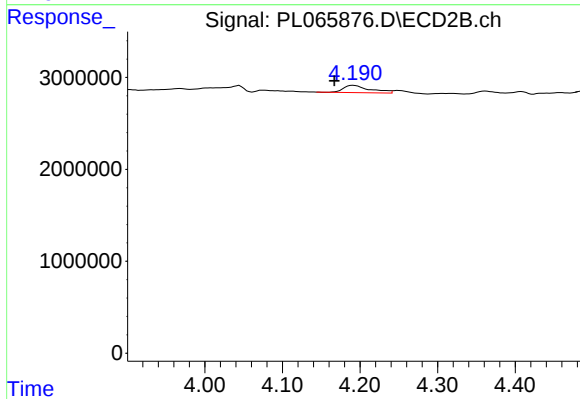

#2 alpha-BHC


R.T.: 4.192 min
Delta R.T.: 0.024 min
Response: 1867806
Conc: 0.46 ng/ml

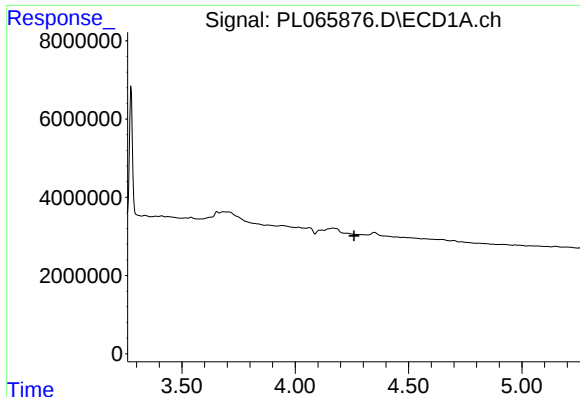

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.260 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

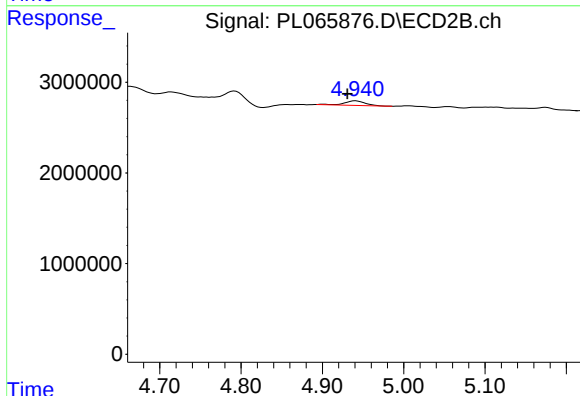


#4 Heptachlor

R.T.: 4.941 min
Delta R.T.: 0.010 min
Response: 858029
Conc: 0.24 ng/ml

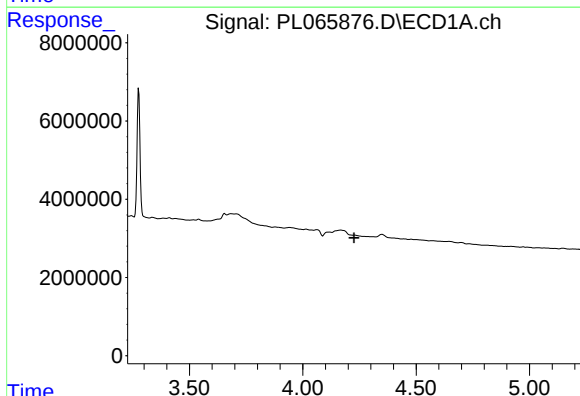


#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 4.226 min
Response: 0
Conc: N.D.

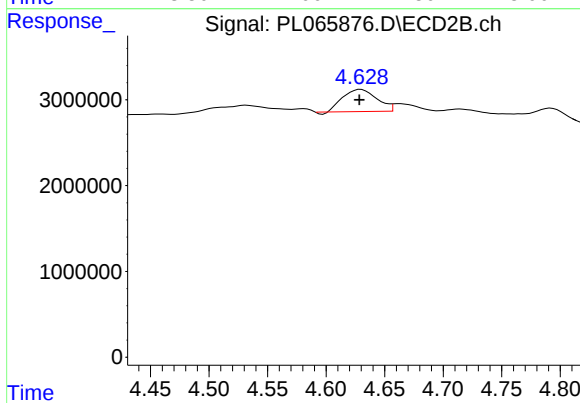

#6 beta-BHC


R.T.: 4.630 min
Delta R.T.: 0.001 min
Response: 5185165
Conc: 2.98 ng/ml

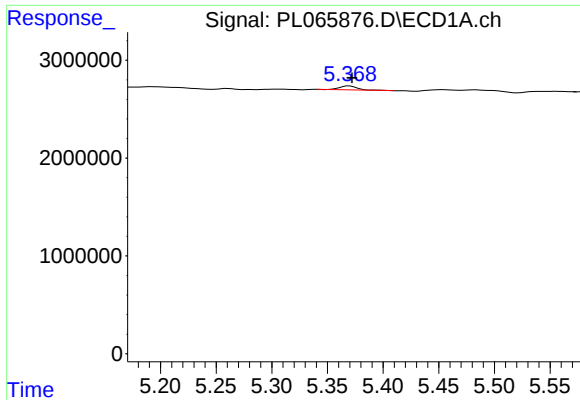

#12 4,4'-DDE


R.T.: 5.369 min
Delta R.T.: -0.003 min
Response: 450433
Conc: 0.16 ng/ml

Instrument :
ECD_L
ClientSampleId :

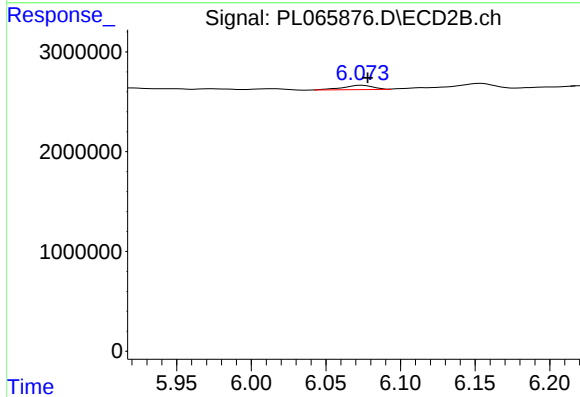


#12 4,4'-DDE

R.T.: 6.074 min
Delta R.T.: -0.004 min
Response: 599691
Conc: 0.23 ng/ml

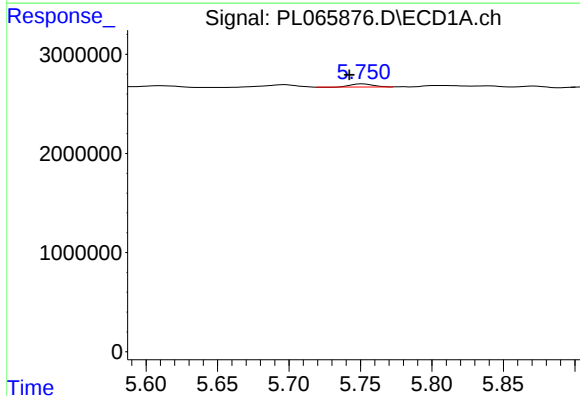


#14 Endrin

R.T.: 5.752 min
Delta R.T.: 0.009 min
Response: 344907
Conc: 0.13 ng/ml

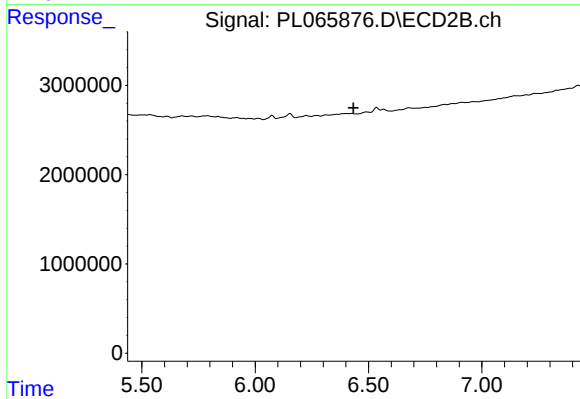

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.434 min
Response: 0
Conc: N.D.

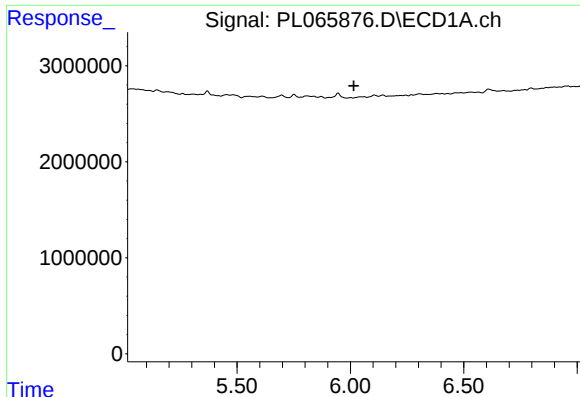

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.015 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

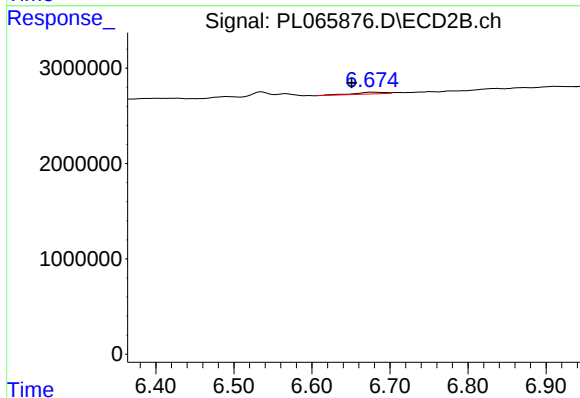


#15 Endosulfan II

R.T.: 6.677 min
Delta R.T.: 0.026 min
Response: 489697
Conc: 0.21 ng/ml

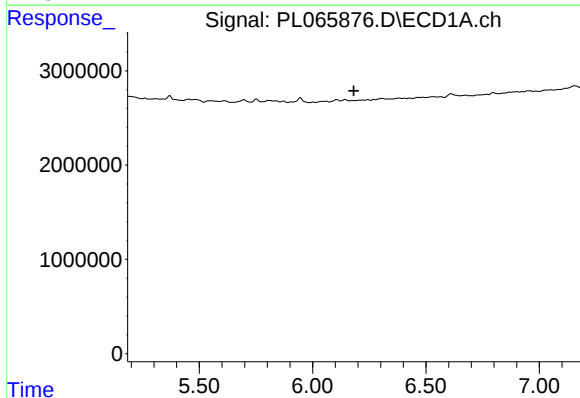


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 6.181 min
Response: 0
Conc: N.D.

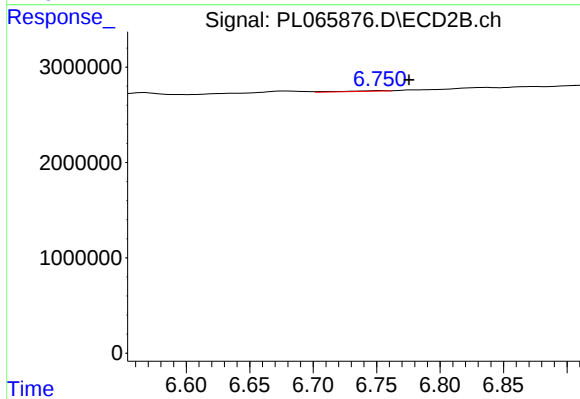

#18 Endrin aldehyde


R.T.: 6.753 min
Delta R.T.: -0.023 min
Response: 136542
Conc: 0.07 ng/ml

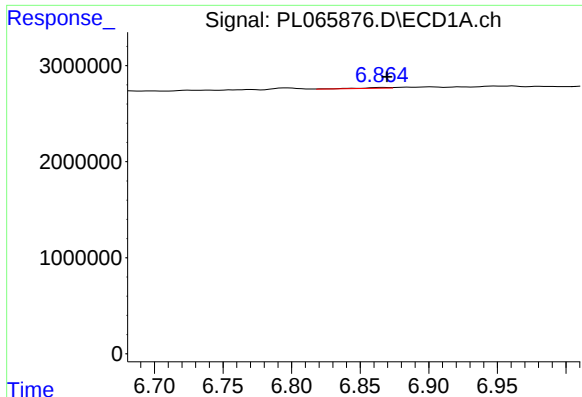

#21 Endrin ketone


R.T.: 6.866 min
Delta R.T.: -0.004 min
Response: 119849
Conc: 0.04 ng/ml

Instrument :
ECD_L
ClientSampleId :

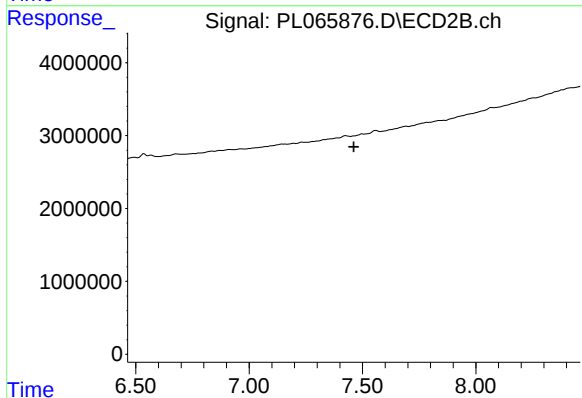


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.462 min
Response: 0
Conc: N.D.

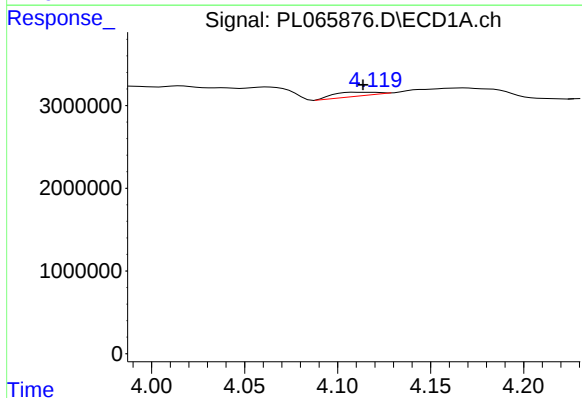


#23 Chlordane-1

R.T.: 4.109 min
Delta R.T.: -0.005 min
Response: 771572
Conc: 8.55 ng/ml

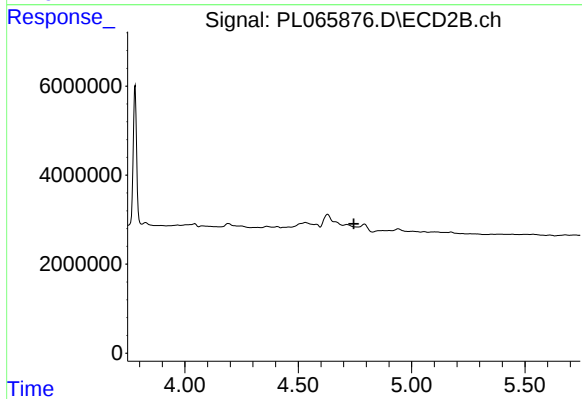

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.745 min
Response: 0
Conc: N.D.

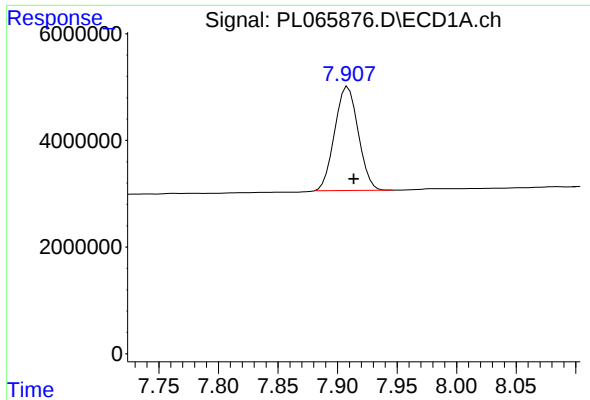

#28 Decachlorobiphenyl

R.T.: 7.909 min
Delta R.T.: -0.005 min
Response: 26836806
Conc: 11.59 ng/ml

Instrument :
ECD_L
ClientSampleId :

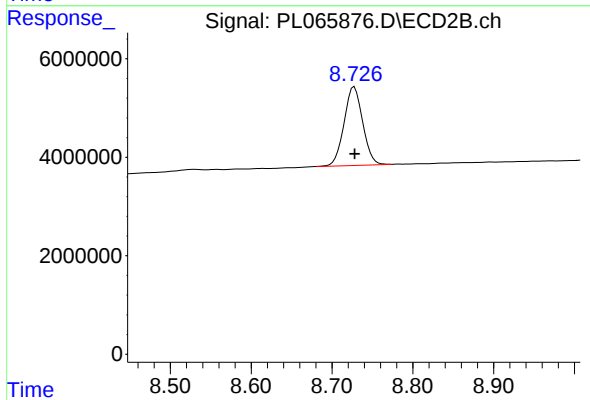

#28 Decachlorobiphenyl

R.T.: 8.728 min
Delta R.T.: 0.000 min
Response: 25632385
Conc: 11.37 ng/ml