

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040521\
 Data File : PL065874.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Apr 2021 13:55
 Operator : AR\AJ
 Sample : M1909-02
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 FS-SB-10-26-27

Manual Integrations
 APPROVED

Ankita
 4/7/2021 4:47:12 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 06 10:49:45 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 31 15:57:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.282	3.780	105.5E6	60016502	40.500	21.864 #
28)	SA Decachlor...	7.908	8.727	25946082	25002392	11.203	11.090
Target Compounds							
12)	B 4,4'-DDE	5.381	6.070	5068.6E6	1732.4E6	1837.090m	663.118m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040521\
Data File : PL065874.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Apr 2021 13:55
Operator : AR\AJ
Sample : M1909-02
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
FS-SB-10-26-27


Manual Integrations
APPROVED

Ankita
4/7/2021 4:47:12 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 06 10:49:45 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
Quant Title : GC Extractables
QLast Update : Wed Mar 31 15:57:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

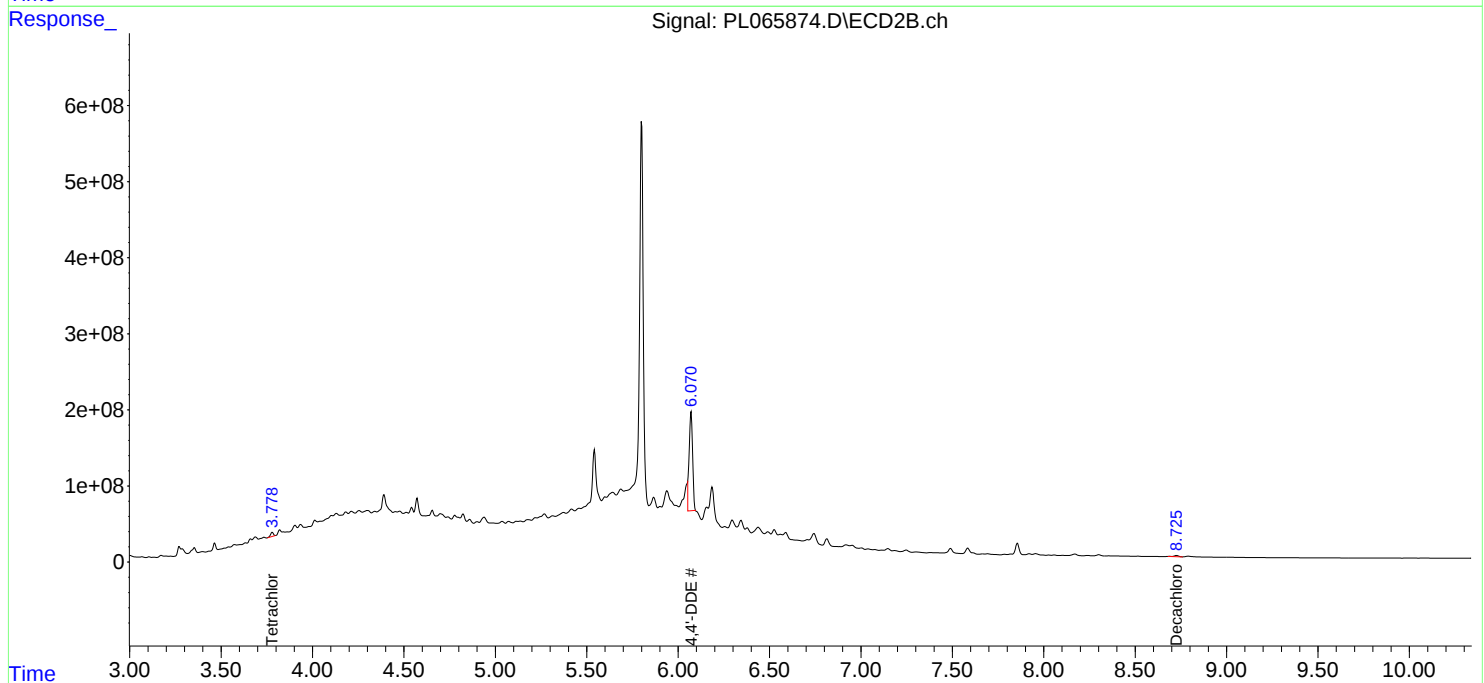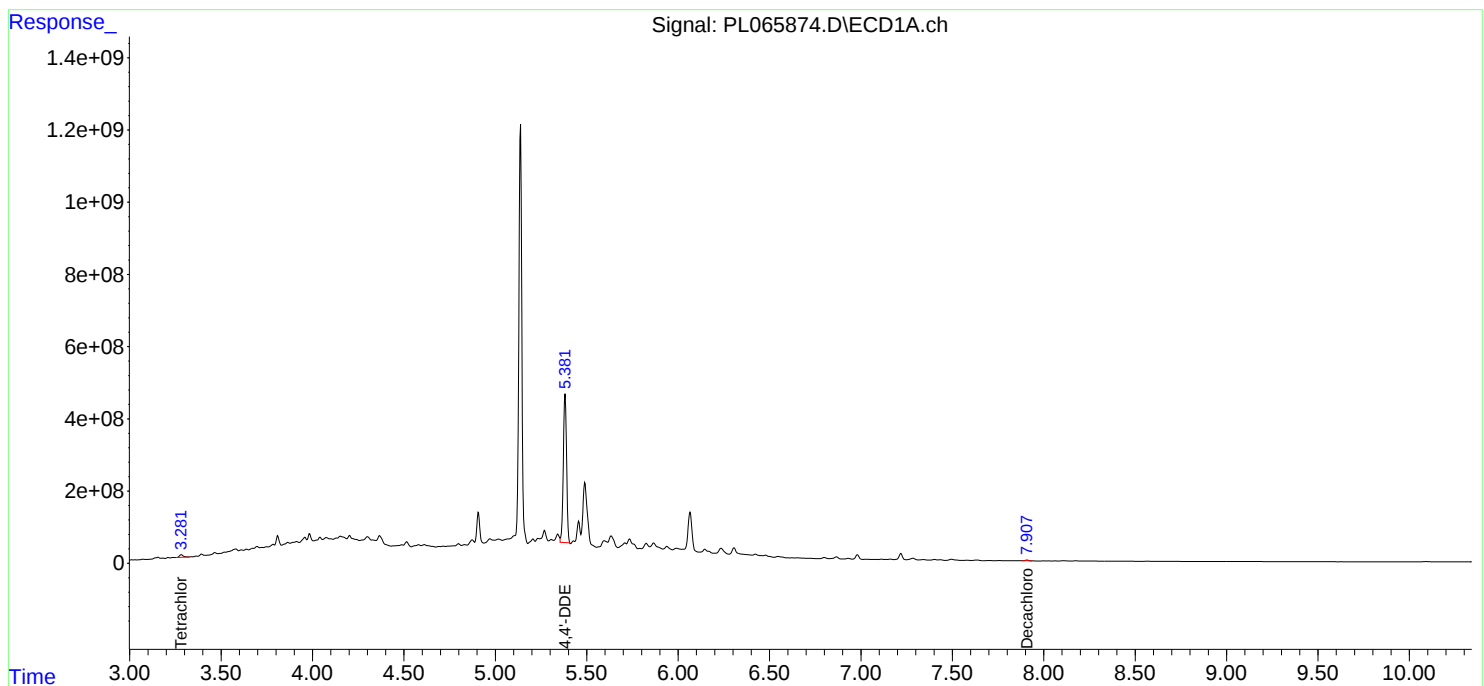

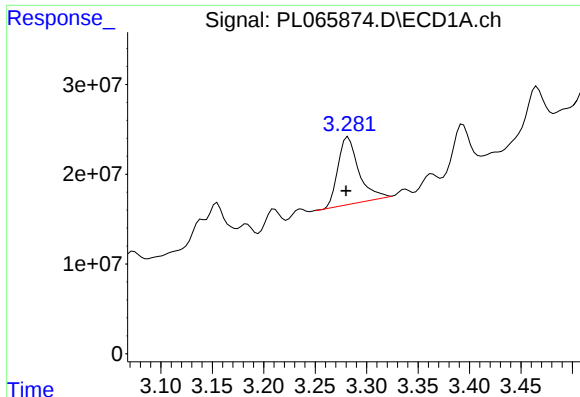


#1 Tetrachloro-m-xylene

R.T.: 3.282 min
Delta R.T.: 0.002 min
Response: 105502339
Conc: 40.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
FS-SB-10-26-27


Manual Integrations
APPROVED

Ankita
4/7/2021 4:47:12 PM

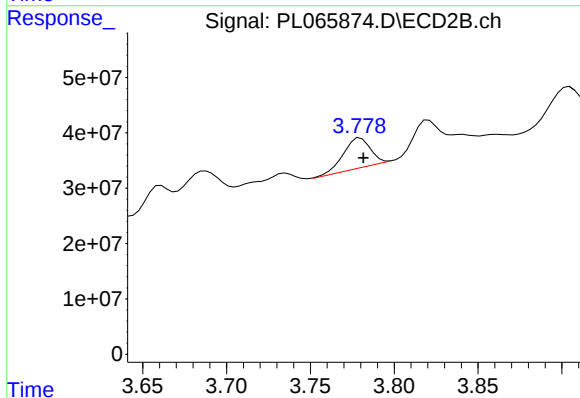


#1 Tetrachloro-m-xylene

R.T.: 3.780 min
Delta R.T.: -0.002 min
Response: 60016502
Conc: 21.86 ng/ml

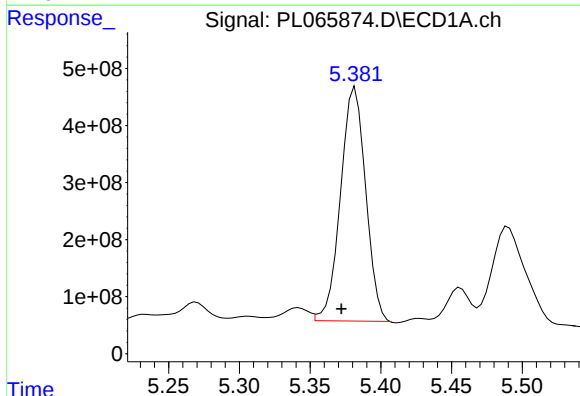


#12 4,4'-DDE

R.T.: 5.381 min
Delta R.T.: 0.008 min
Response: 5068582514
Conc: 1837.09 ng/ml m

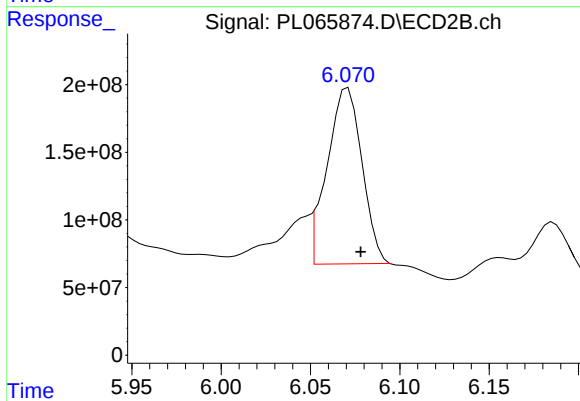

#12 4,4'-DDE

R.T.: 6.070 min
Delta R.T.: -0.008 min
Response: 1732418490
Conc: 663.12 ng/ml m

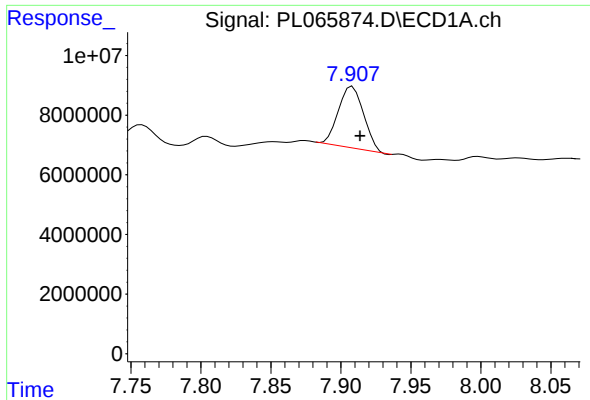


#28 Decachlorobiphenyl

R.T.: 7.908 min
Delta R.T.: -0.005 min
Response: 25946082
Conc: 11.20 ng/ml

Instrument :
ECD_L
ClientSampleId :
FS-SB-10-26-27

Manual Integrations
APPROVED

Ankita
4/7/2021 4:47:12 PM

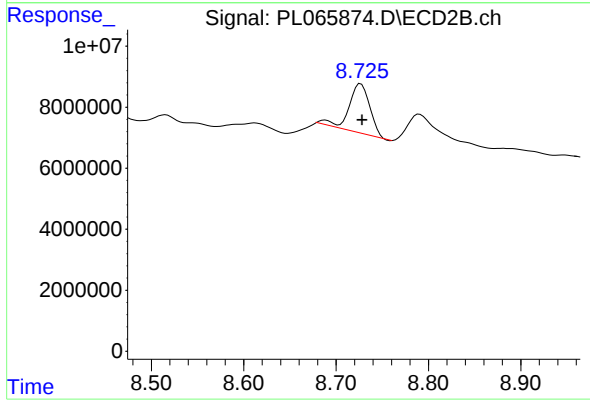

#28 Decachlorobiphenyl

R.T.: 8.727 min
Delta R.T.: -0.001 min
Response: 25002392
Conc: 11.09 ng/ml