

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040521\
 Data File : PL065884.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Apr 2021 17:22
 Operator : AR\AJ
 Sample : M1894-04
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 0156-AMENDED-CP-COMP

Manual Integrations
 APPROVED

Ankita
 4/6/2021 2:57:50 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 06 02:35:21 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 31 15:57:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.275	3.780	61470496	58317543	23.597m	21.245
28)	SA Decachlor...	7.908	8.727	39959212	38497136	17.253	17.076

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040521\
Data File : PL065884.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Apr 2021 17:22
Operator : AR\AJ
Sample : M1894-04
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
0156-AMENDED-CP-COMP


Manual Integrations
APPROVED

Ankita
4/6/2021 2:57:50 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 06 02:35:21 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
Quant Title : GC Extractables
QLast Update : Wed Mar 31 15:57:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

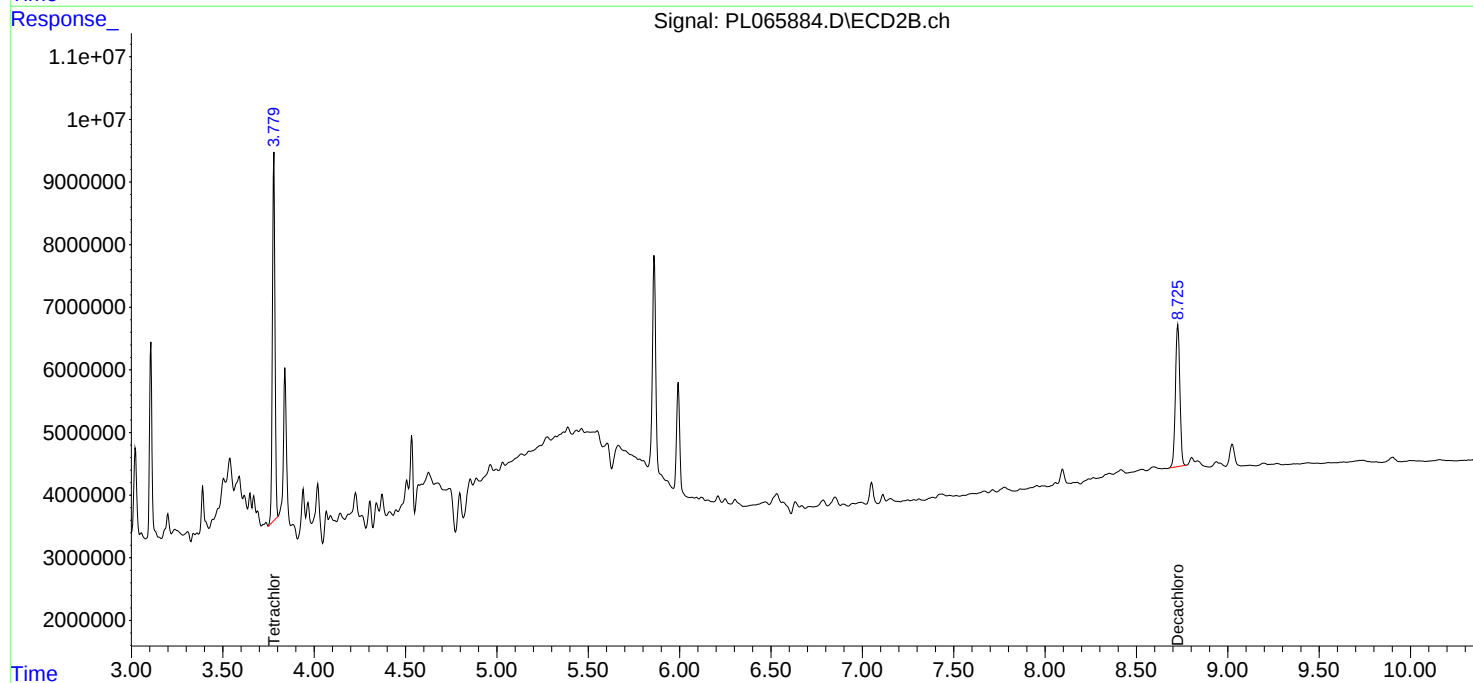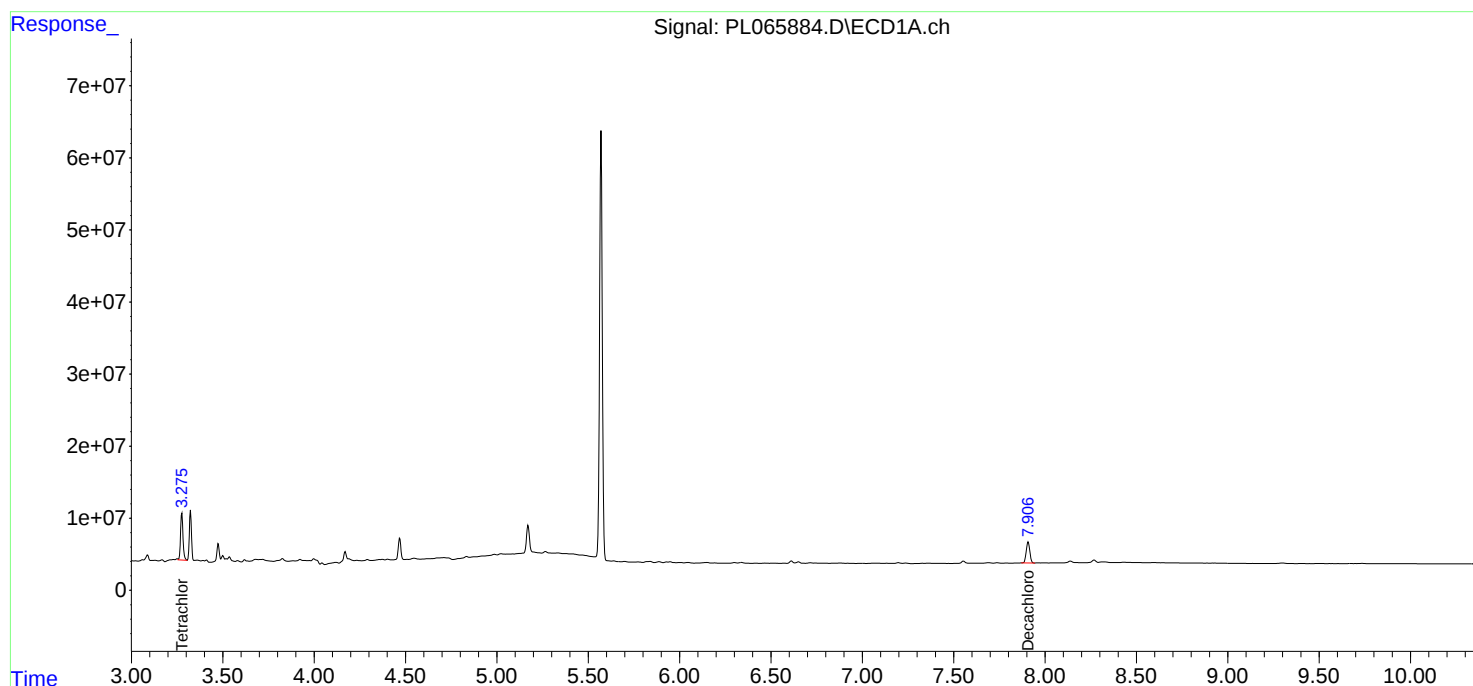

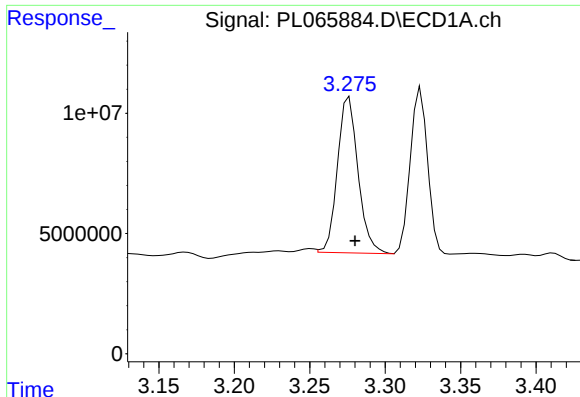


#1 Tetrachloro-m-xylene

R.T.: 3.275 min
Delta R.T.: -0.005 min
Response: 61470496
Conc: 23.60 ng/ml m

Instrument :
ECD_L
ClientSampleId :
0156-AMENDED-CP-COMP


Manual Integrations
APPROVED

Ankita
4/6/2021 2:57:50 PM

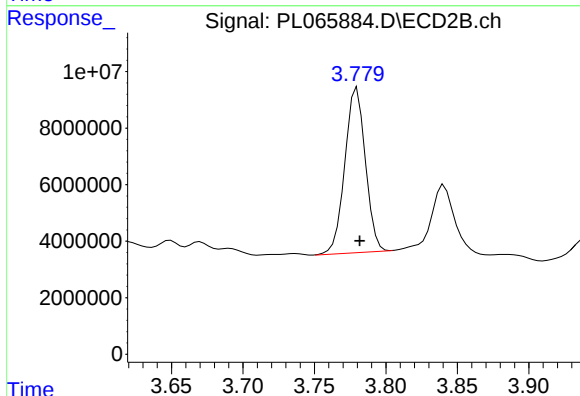


#1 Tetrachloro-m-xylene

R.T.: 3.780 min
Delta R.T.: -0.002 min
Response: 58317543
Conc: 21.25 ng/ml

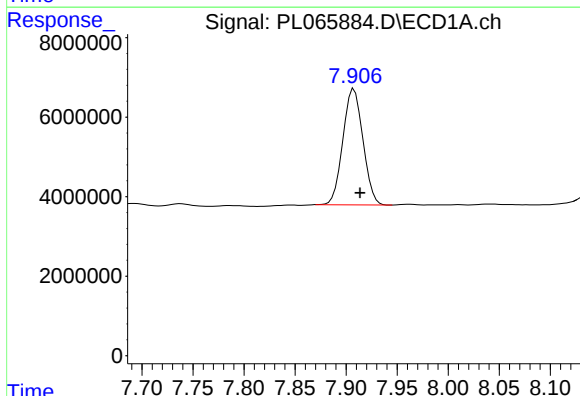

#28 Decachlorobiphenyl

R.T.: 7.908 min
Delta R.T.: -0.006 min
Response: 39959212
Conc: 17.25 ng/ml

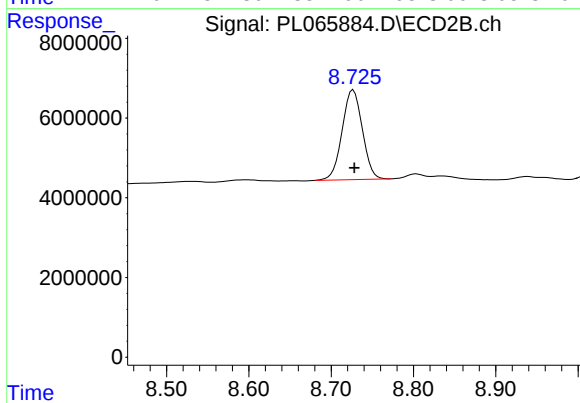

#28 Decachlorobiphenyl

R.T.: 8.727 min
Delta R.T.: -0.001 min
Response: 38497136
Conc: 17.08 ng/ml