

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040620\
 Data File : PL057816.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Apr 2020 17:12
 Operator : AJ\MA
 Sample : L2166-05
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 07 01:08:58 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 04 06:41:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.457	3.956	86305227	19085218	8.561	8.794
28)	SA Decachlor...	8.203	8.976	105.9E6	25686847	10.277	11.499
Target Compounds							
2)	A alpha-BHC	3.898	0.000	4637427	0	0.267	N.D. #
4)	MA Heptachlor	0.000	5.138	0	256051	N.D.	0.076 #
9)	A Endosulfan I	5.495	0.000	973537	0	0.079	N.D. #
12)	B 4,4'-DDE	5.615	6.277	2586972	490270	0.197	0.166
14)	MA Endrin	6.000	0.000	1229908	0	0.105	N.D. #
15)	B Endosulfa...	0.000	6.869f	0	649154	N.D.	0.250 #
17)	MA 4,4'-DDT	6.369	0.000	486568	0	0.048	N.D. #
23)	Chlordane-1	4.348f	0.000	896552	0	2.424	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040620\
Data File : PL057816.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Apr 2020 17:12
Operator : AJ\MA
Sample : L2166-05
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 07 01:08:58 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
Quant Title : GC Extractables
QLast Update : Sat Apr 04 06:41:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

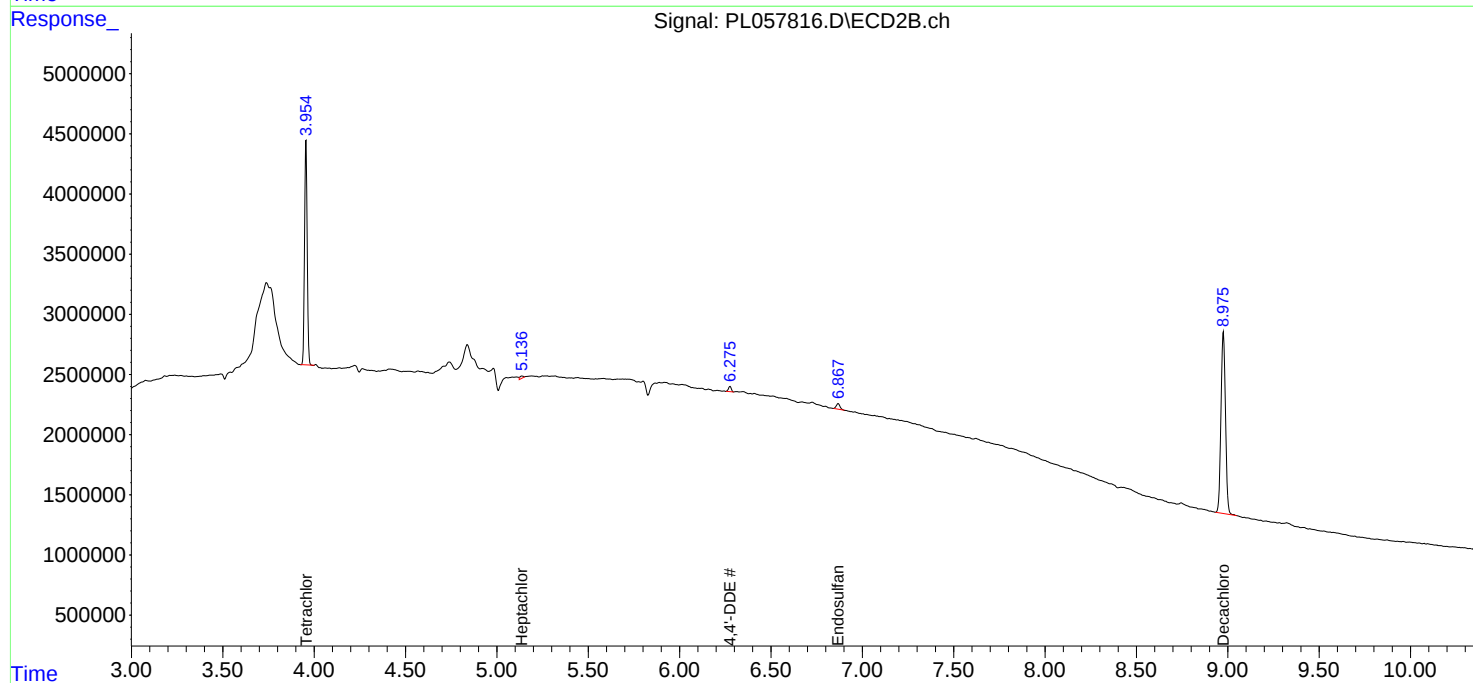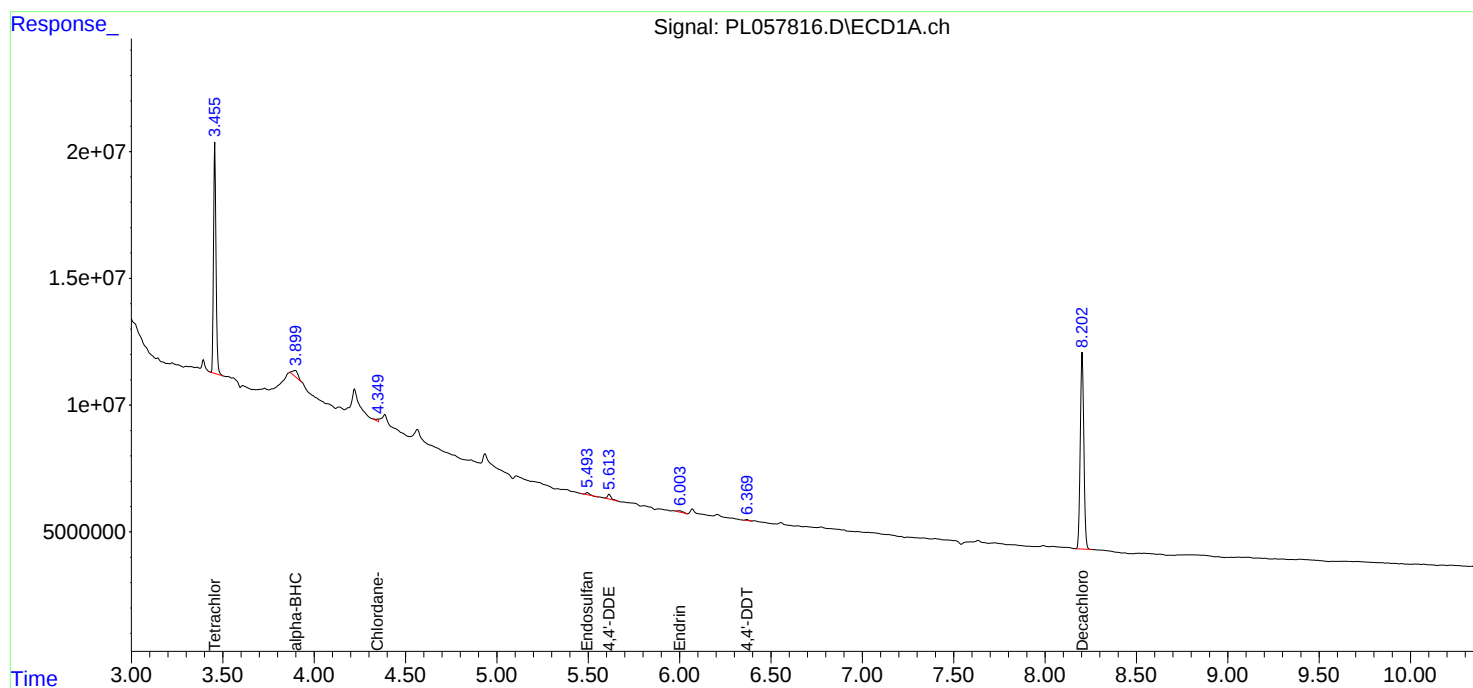


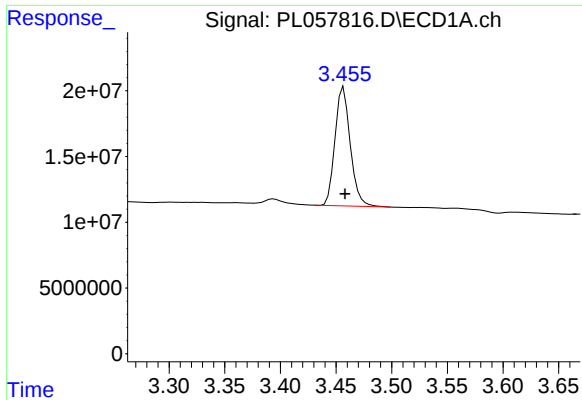

#1 Tetrachloro-m-xylene


R.T.: 3.457 min
Delta R.T.: -0.001 min
Response: 86305227
Conc: 8.56 ng/ml

Instrument :
ECD_L
ClientSampleId :

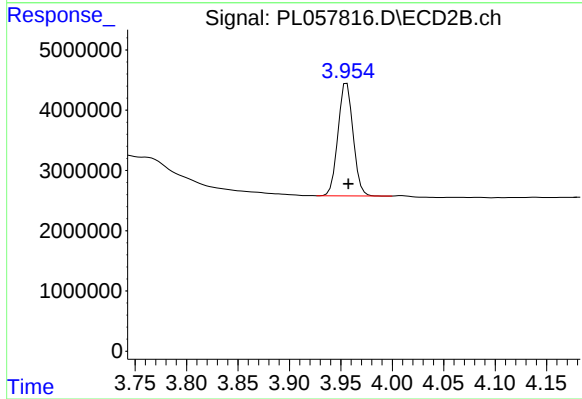


#1 Tetrachloro-m-xylene

R.T.: 3.956 min
Delta R.T.: -0.001 min
Response: 19085218
Conc: 8.79 ng/ml

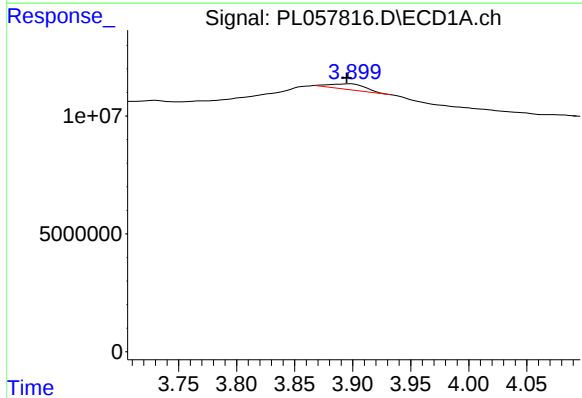


#2 alpha-BHC

R.T.: 3.898 min
Delta R.T.: 0.003 min
Response: 4637427
Conc: 0.27 ng/ml

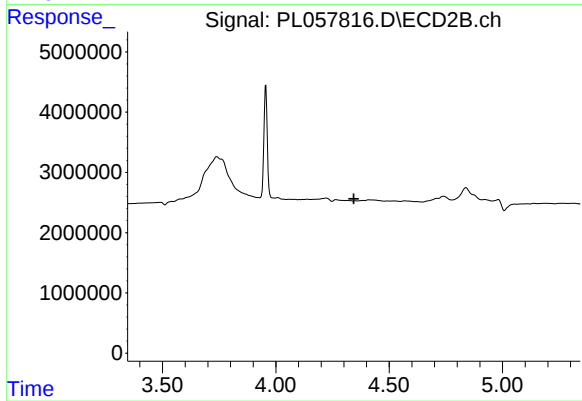

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.345 min
Response: 0
Conc: N.D.

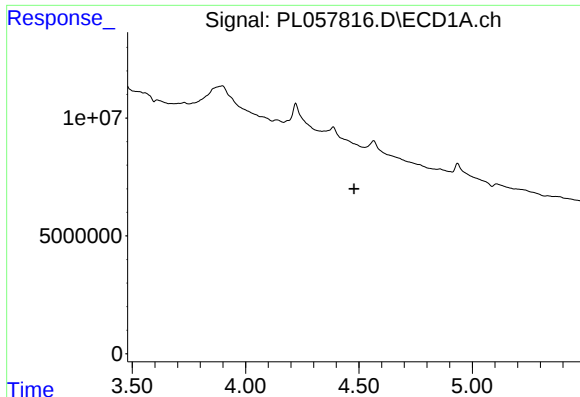

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.479 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

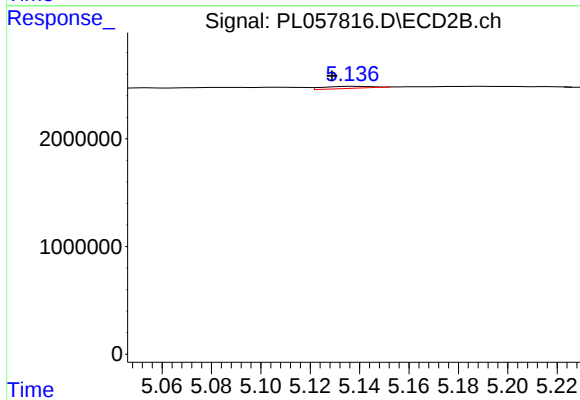


#4 Heptachlor

R.T.: 5.138 min
Delta R.T.: 0.009 min
Response: 256051
Conc: 0.08 ng/ml

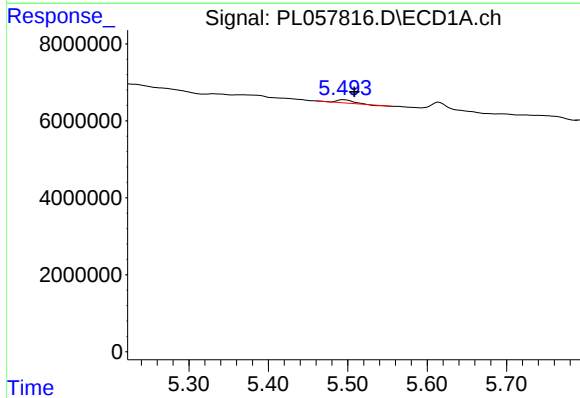


#9 Endosulfan I

R.T.: 5.495 min
Delta R.T.: -0.013 min
Response: 973537
Conc: 0.08 ng/ml

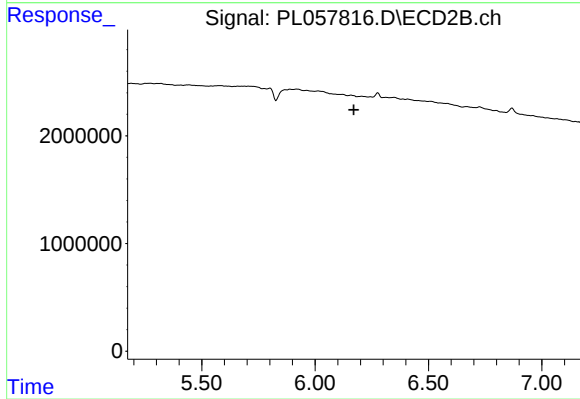

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.170 min
Response: 0
Conc: N.D.

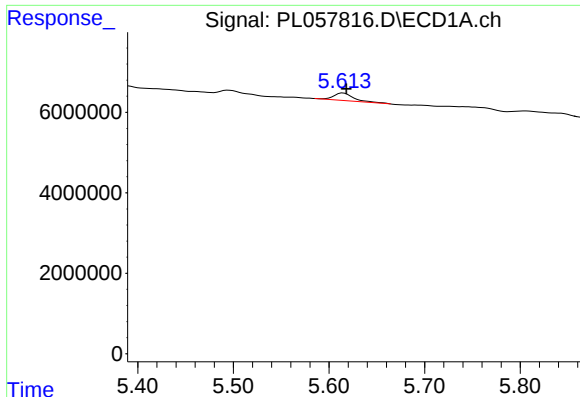

#12 4,4'-DDE


R.T.: 5.615 min
Delta R.T.: -0.003 min
Response: 2586972
Conc: 0.20 ng/ml

Instrument :
ECD_L
ClientSampleId :

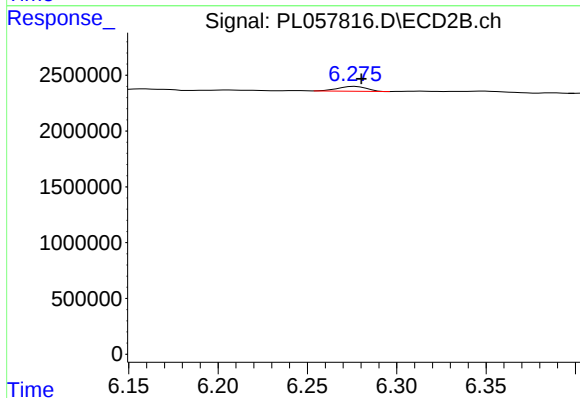


#12 4,4'-DDE

R.T.: 6.277 min
Delta R.T.: -0.004 min
Response: 490270
Conc: 0.17 ng/ml

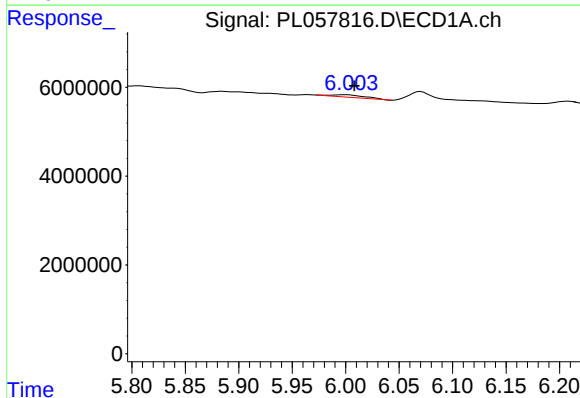


#14 Endrin

R.T.: 6.000 min
Delta R.T.: -0.008 min
Response: 1229908
Conc: 0.11 ng/ml

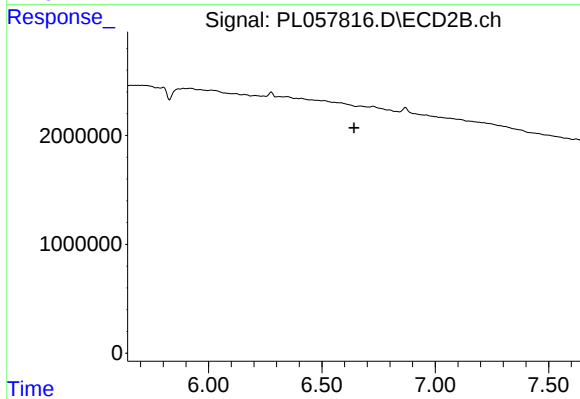

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.642 min
Response: 0
Conc: N.D.

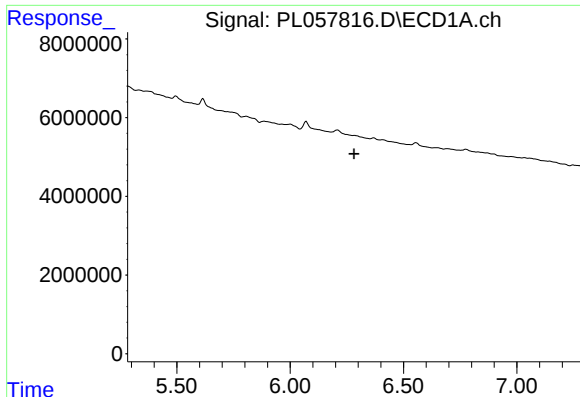

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.282 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

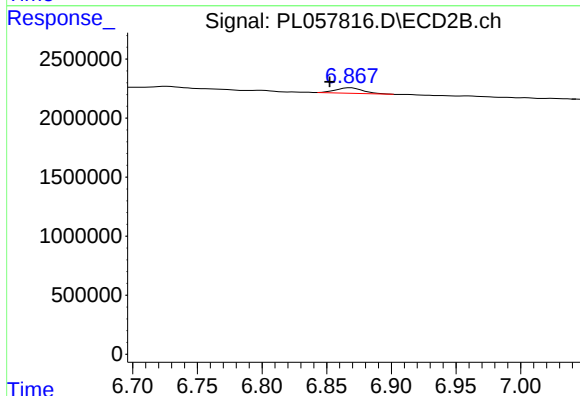


#15 Endosulfan II

R.T.: 6.869 min
Delta R.T.: 0.016 min
Response: 649154
Conc: 0.25 ng/ml

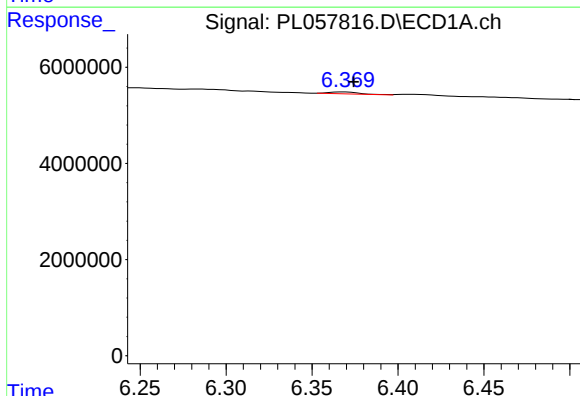


#17 4,4'-DDT

R.T.: 6.369 min
Delta R.T.: -0.005 min
Response: 486568
Conc: 0.05 ng/ml

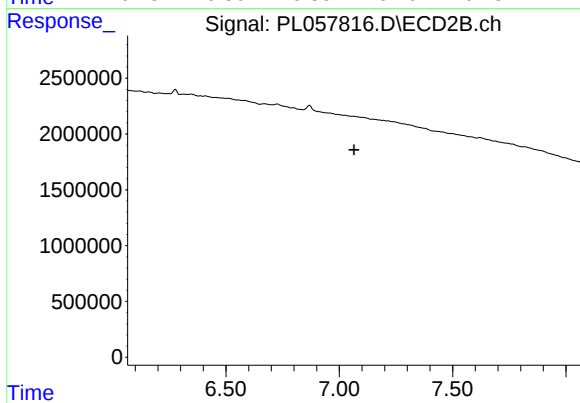

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 7.066 min
Response: 0
Conc: N.D.

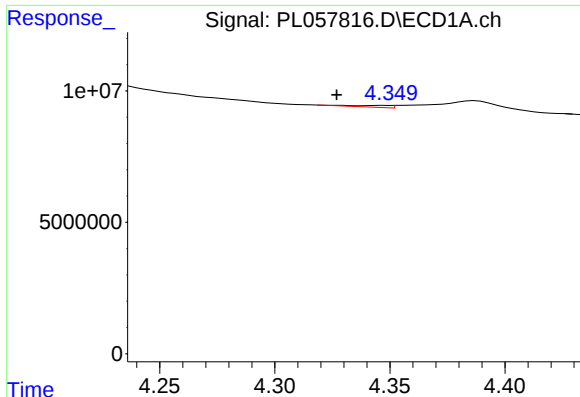

#23 Chlordane-1


R.T.: 4.348 min
Delta R.T.: 0.021 min
Response: 896552
Conc: 2.42 ng/ml

Instrument :
ECD_L
ClientSampleId :

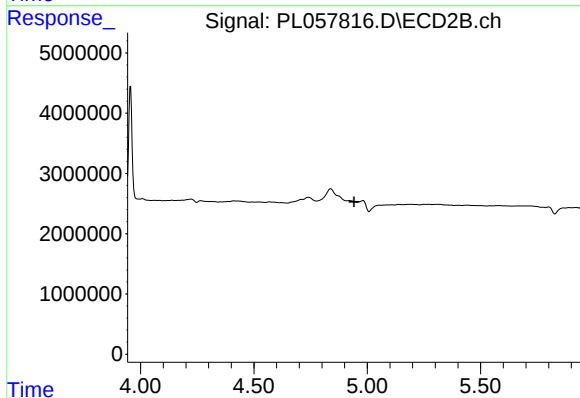


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.942 min
Response: 0
Conc: N.D.

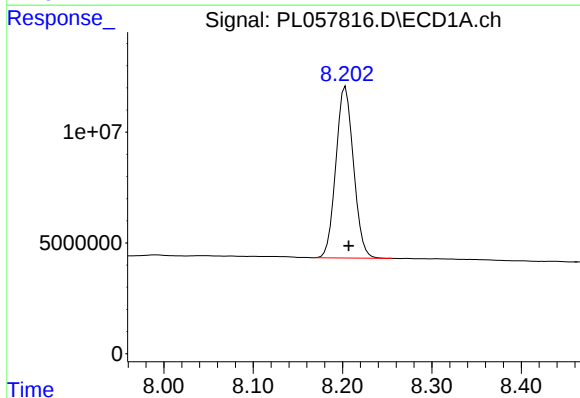

#28 Decachlorobiphenyl

R.T.: 8.203 min
Delta R.T.: -0.003 min
Response: 105942571
Conc: 10.28 ng/ml

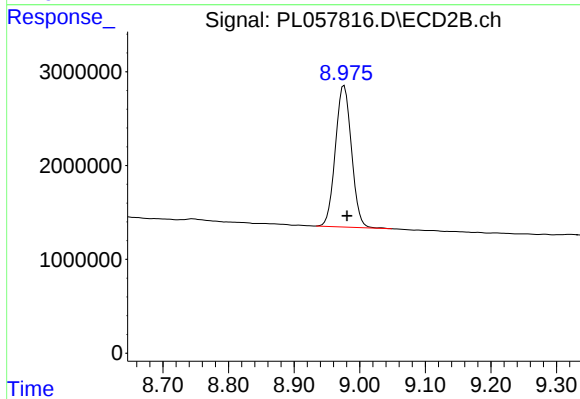

#28 Decachlorobiphenyl

R.T.: 8.976 min
Delta R.T.: -0.005 min
Response: 25686847
Conc: 11.50 ng/ml