

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040620\
 Data File : PL057831.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Apr 2020 20:44
 Operator : AJ\MA
 Sample : L2166-06
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 07 01:13:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 04 06:41:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.458	3.956	225.4E6	48062445	22.361	22.147
28)	SA Decachlor...	8.203	8.977	204.9E6	46346441	19.876	20.748
Target Compounds							
4)	MA Heptachlor	0.000	5.140	0	985431	N.D.	0.294 #
7)	B delta-BHC	0.000	4.985f	0	9931898	N.D.	5.837 #
8)	B Heptachlo...	0.000	5.797f	0	10317822	N.D.	3.821 #
15)	B Endosulfa...	0.000	6.867	0	799348	N.D.	0.308 #
23)	Chlordane-1	4.355f	0.000	13654039	0	36.918	N.D. #
24)	Chlordane-2	4.846f	0.000	21227693	0	52.581	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040620\
Data File : PL057831.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Apr 2020 20:44
Operator : AJ\MA
Sample : L2166-06
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 07 01:13:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
Quant Title : GC Extractables
QLast Update : Sat Apr 04 06:41:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

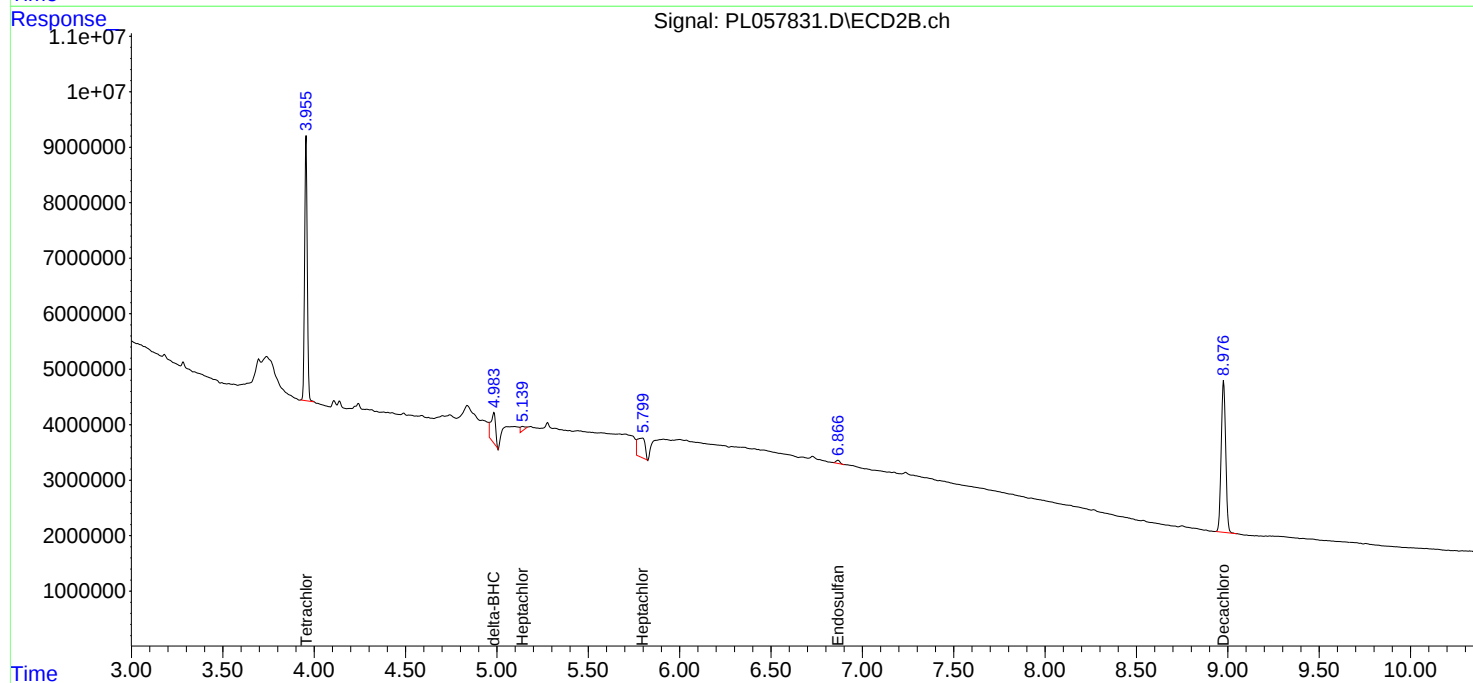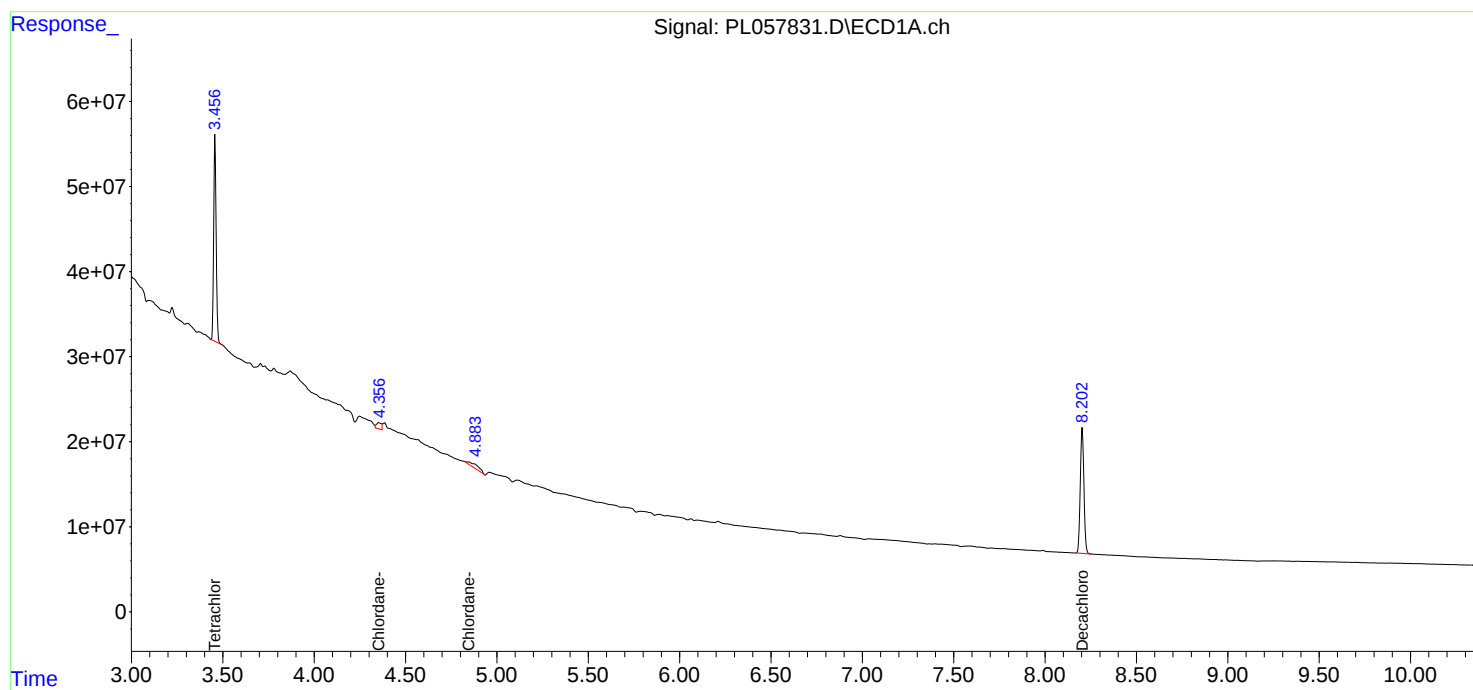


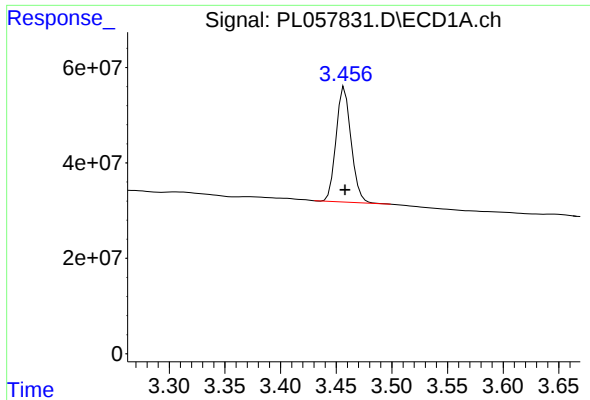

#1 Tetrachloro-m-xylene


R.T.: 3.458 min
Delta R.T.: 0.000 min
Response: 225425514
Conc: 22.36 ng/ml

Instrument :
ECD_L
ClientSampleId :

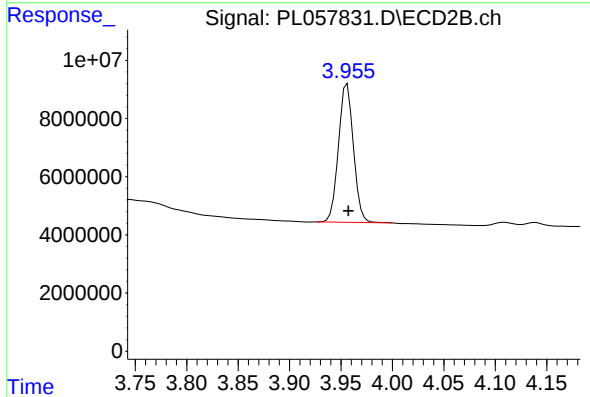


#1 Tetrachloro-m-xylene

R.T.: 3.956 min
Delta R.T.: -0.001 min
Response: 48062445
Conc: 22.15 ng/ml

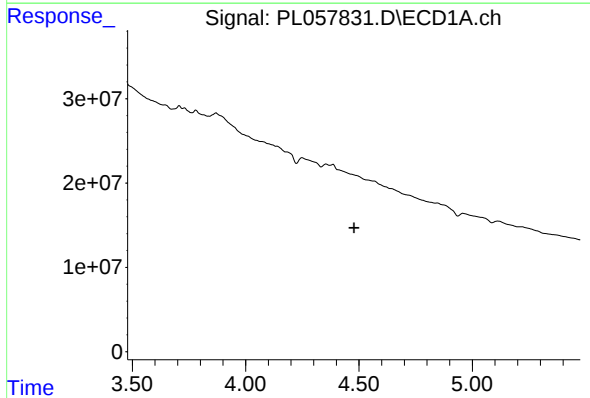


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.479 min
Response: 0
Conc: N.D.

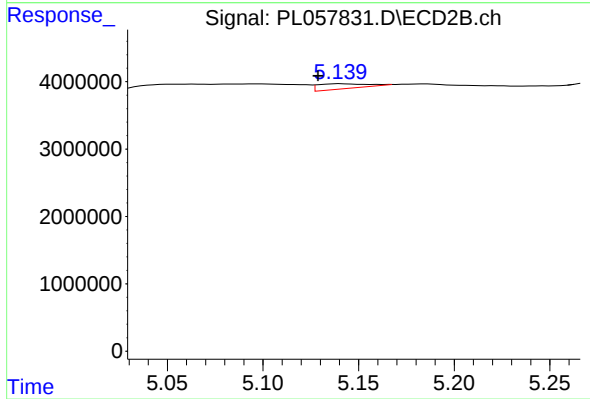

#4 Heptachlor


R.T.: 5.140 min
Delta R.T.: 0.012 min
Response: 985431
Conc: 0.29 ng/ml

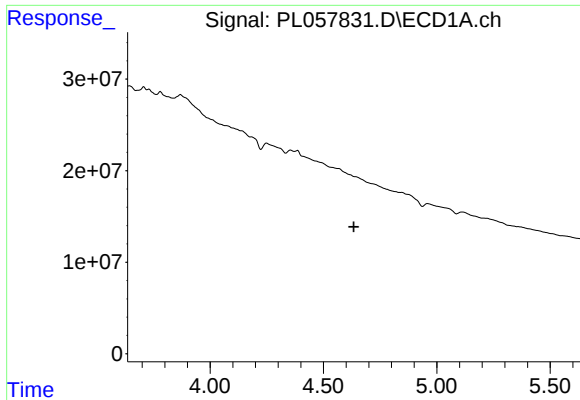

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.634 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

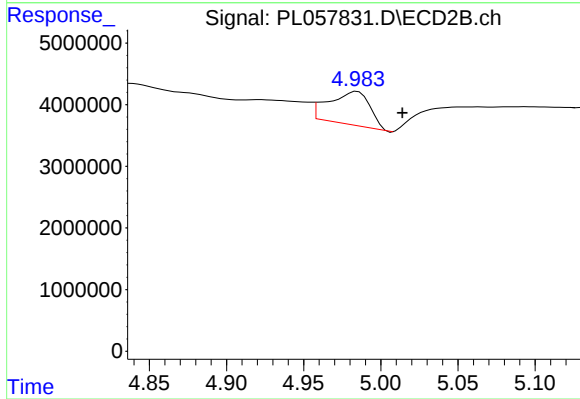


#7 delta-BHC

R.T.: 4.985 min
Delta R.T.: -0.029 min
Response: 9931898
Conc: 5.84 ng/ml

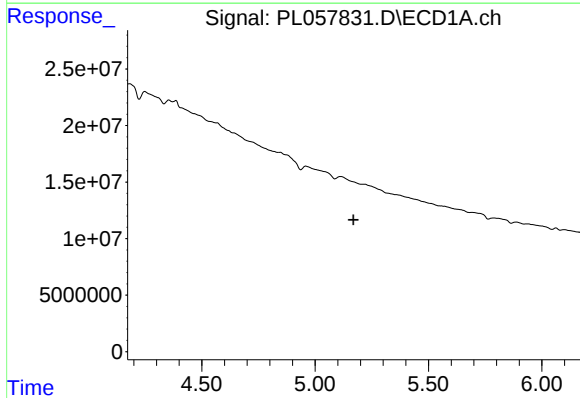


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.169 min
Response: 0
Conc: N.D.

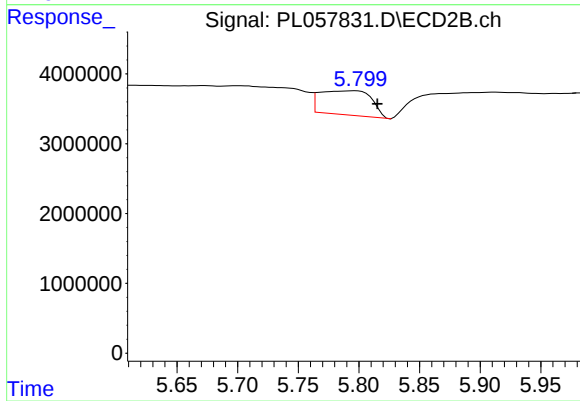

#8 Heptachlor epoxide


R.T.: 5.797 min
Delta R.T.: -0.018 min
Response: 10317822
Conc: 3.82 ng/ml

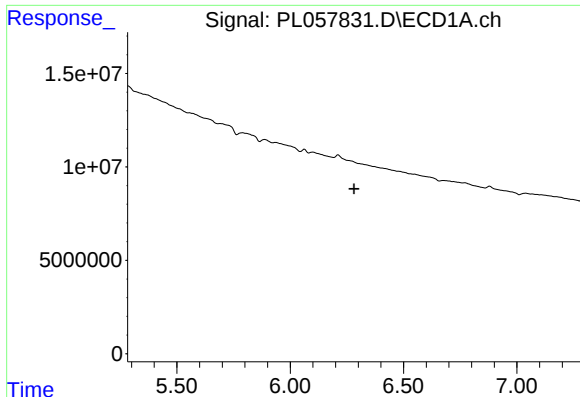

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.282 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

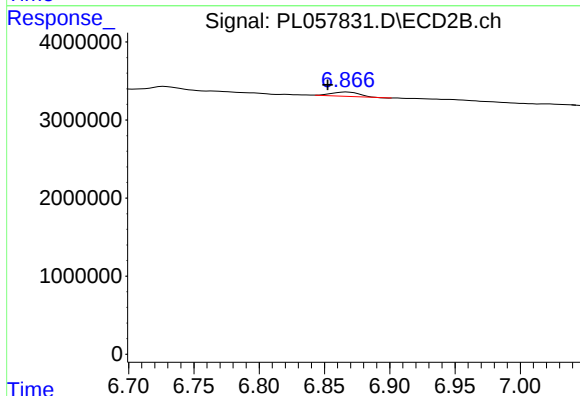


#15 Endosulfan II

R.T.: 6.867 min
Delta R.T.: 0.015 min
Response: 799348
Conc: 0.31 ng/ml

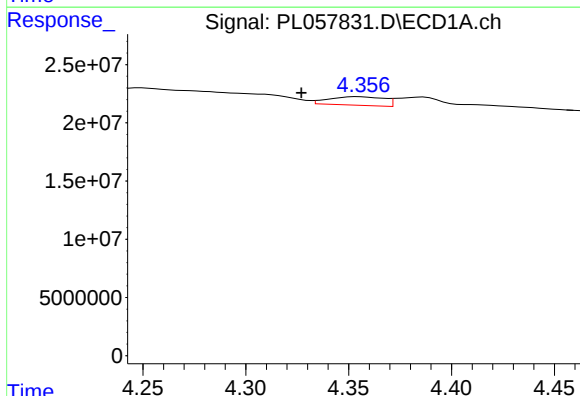


#23 Chlordane-1

R.T.: 4.355 min
Delta R.T.: 0.028 min
Response: 13654039
Conc: 36.92 ng/ml

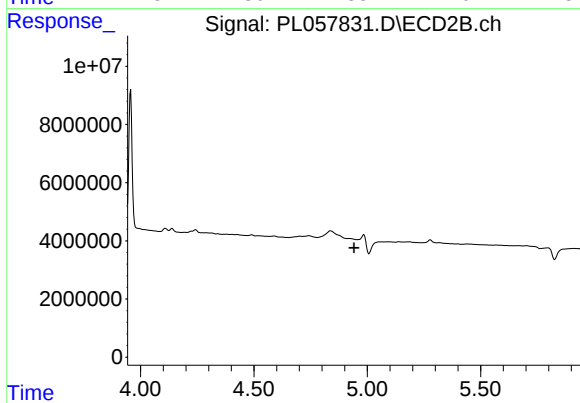

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.942 min
Response: 0
Conc: N.D.

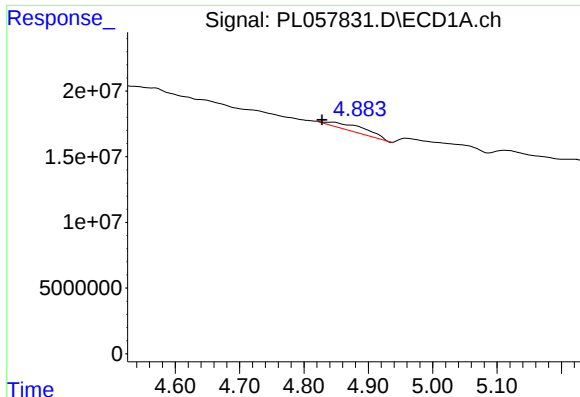

#24 Chlordane-2


R.T.: 4.846 min
Delta R.T.: 0.018 min
Response: 21227693
Conc: 52.58 ng/ml

Instrument :
ECD_L
ClientSampleId :

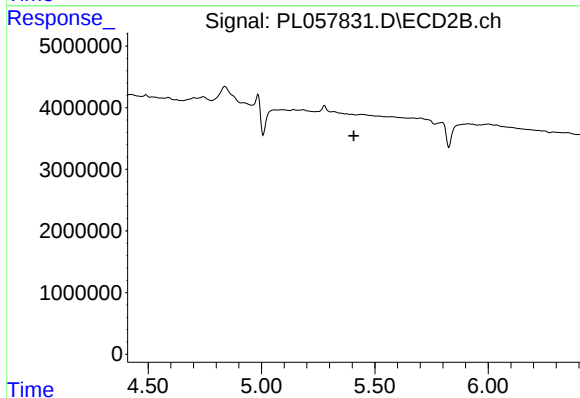


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.407 min
Response: 0
Conc: N.D.

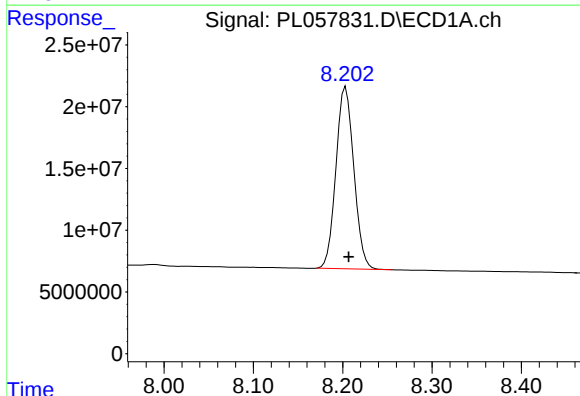

#28 Decachlorobiphenyl

R.T.: 8.203 min
Delta R.T.: -0.003 min
Response: 204890094
Conc: 19.88 ng/ml

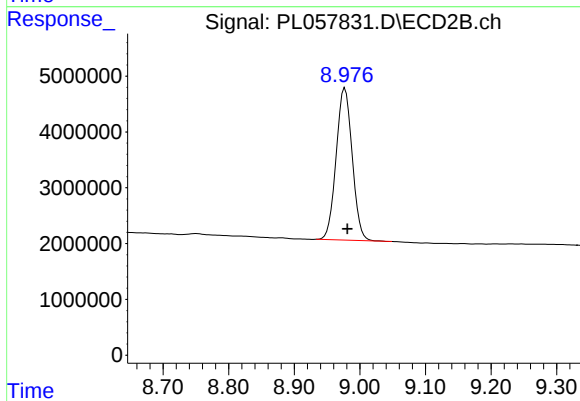

#28 Decachlorobiphenyl

R.T.: 8.977 min
Delta R.T.: -0.004 min
Response: 46346441
Conc: 20.75 ng/ml