

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040620\
 Data File : PL057832.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Apr 2020 20:58
 Operator : AJ\MA
 Sample : L2166-13
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 07 01:13:39 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 04 06:41:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.458	3.956	228.2E6	48918379	22.635	22.542
28)	SA Decachlor...	8.205	8.978	217.6E6	49792608	21.109	22.291
Target Compounds							
4)	MA Heptachlor	0.000	5.139	0	1292809	N.D.	0.385 #
7)	B delta-BHC	0.000	4.985f	0	8423805	N.D.	5.258 #
8)	B Heptachlo...	0.000	5.799f	0	9020667	N.D.	3.341 #
12)	B 4,4'-DDE	0.000	6.307f	0	649103	N.D.	0.219 #
15)	B Endosulfa...	6.287	6.869f	356018	1054431	0.032	0.407 #
23)	Chlordane-1	4.357f	0.000	9970628	0	26.959	N.D. #
24)	Chlordane-2	4.849f	0.000	19872101	0	49.223	N.D. #
27)	Chlordane-5	6.287	0.000	356018	0	0.941	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040620\
Data File : PL057832.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Apr 2020 20:58
Operator : AJ\MA
Sample : L2166-13
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 07 01:13:39 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
Quant Title : GC Extractables
QLast Update : Sat Apr 04 06:41:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

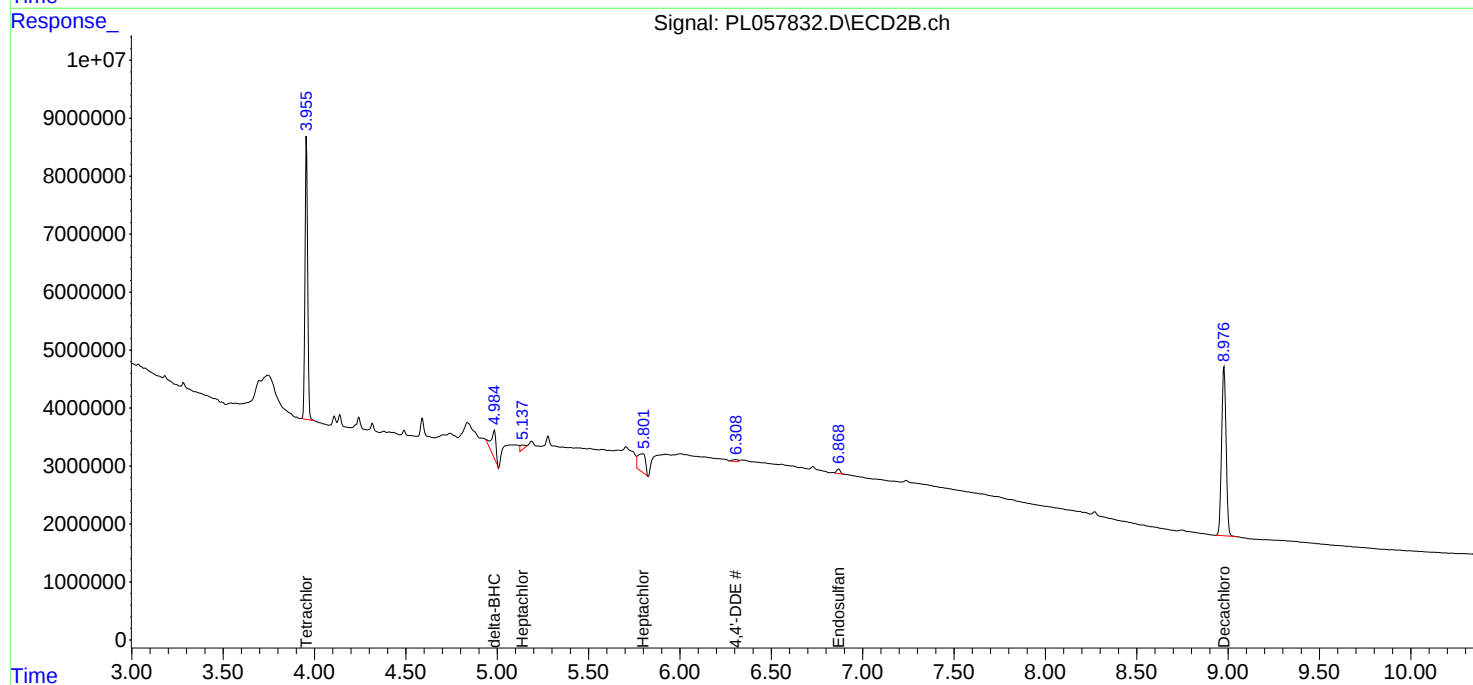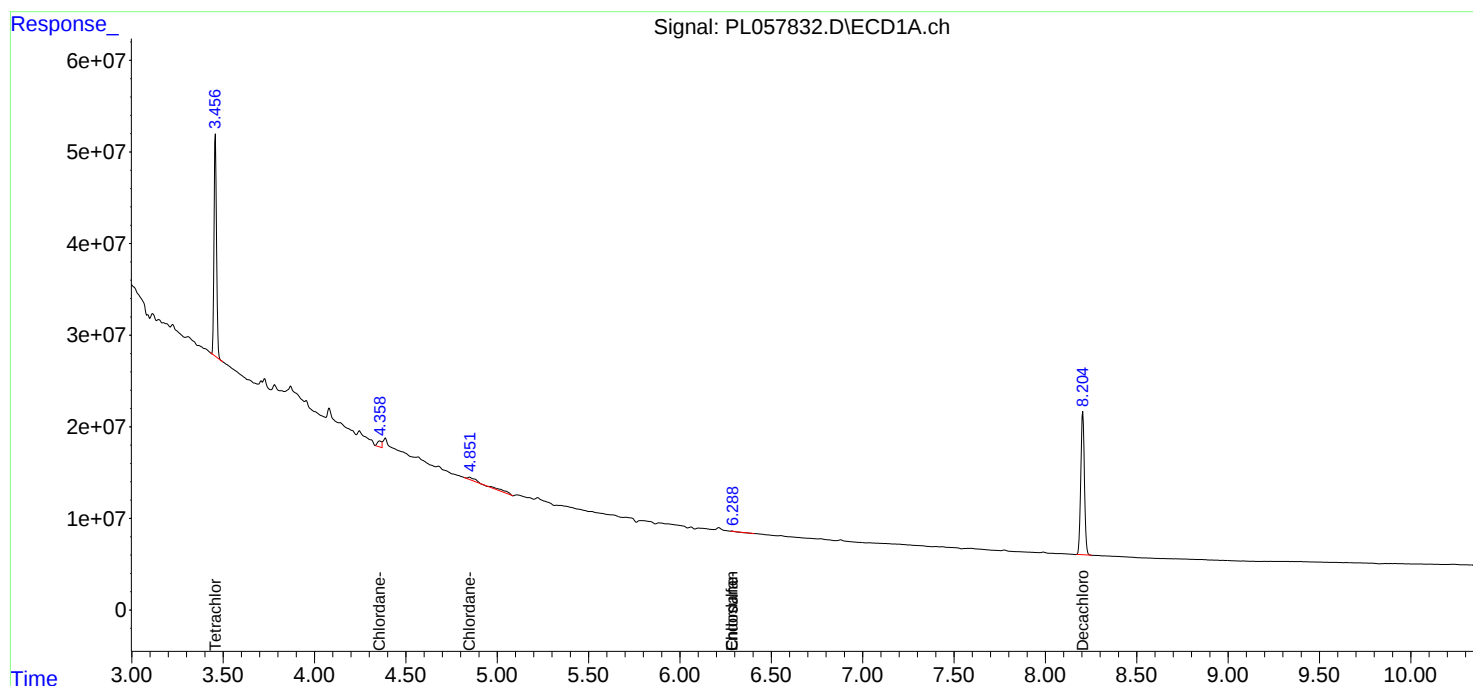


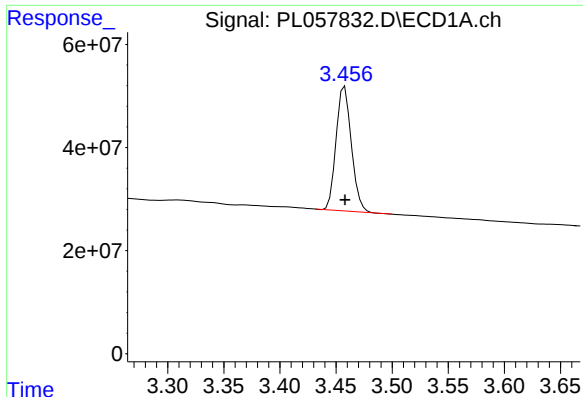

#1 Tetrachloro-m-xylene


R.T.: 3.458 min
Delta R.T.: 0.000 min
Response: 228179365
Conc: 22.63 ng/ml

Instrument :
ECD_L
ClientSampleId :

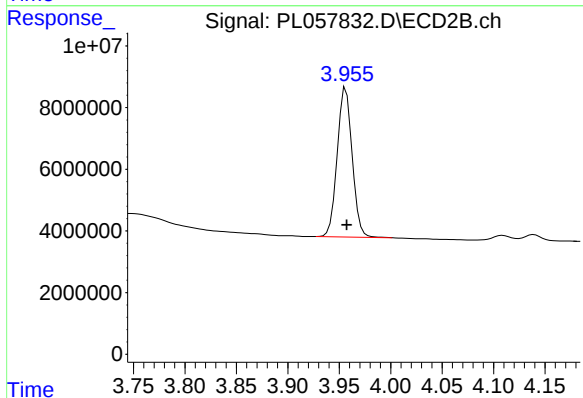


#1 Tetrachloro-m-xylene

R.T.: 3.956 min
Delta R.T.: 0.000 min
Response: 48918379
Conc: 22.54 ng/ml

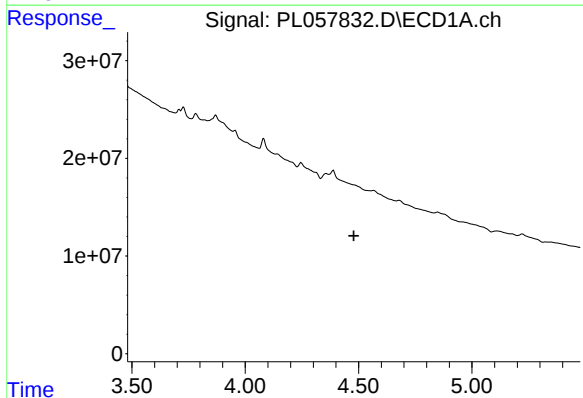


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.479 min
Response: 0
Conc: N.D.

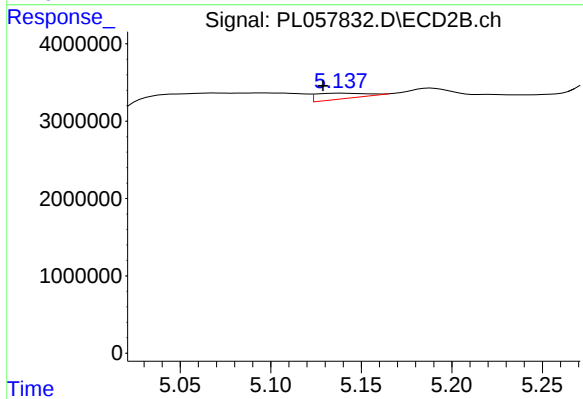

#4 Heptachlor


R.T.: 5.139 min
Delta R.T.: 0.010 min
Response: 1292809
Conc: 0.39 ng/ml

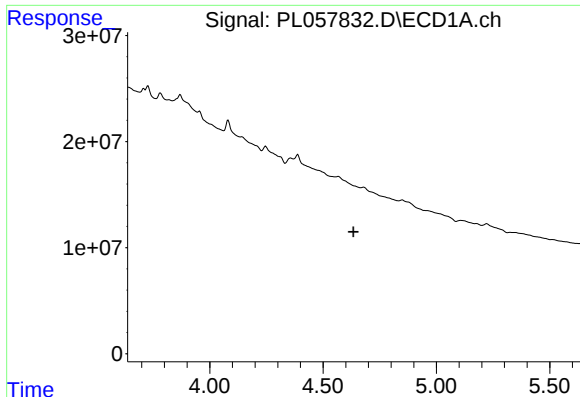

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.634 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

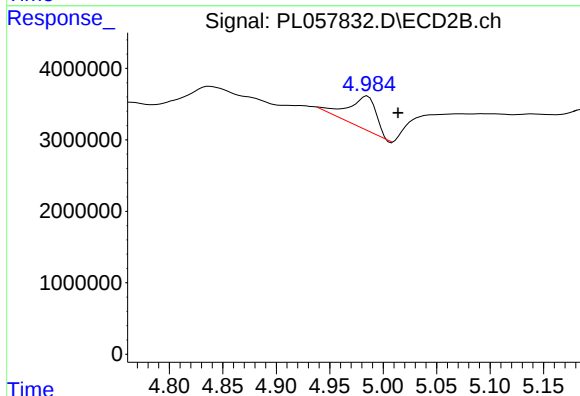


#7 delta-BHC

R.T.: 4.985 min
Delta R.T.: -0.029 min
Response: 8423805
Conc: 5.26 ng/ml

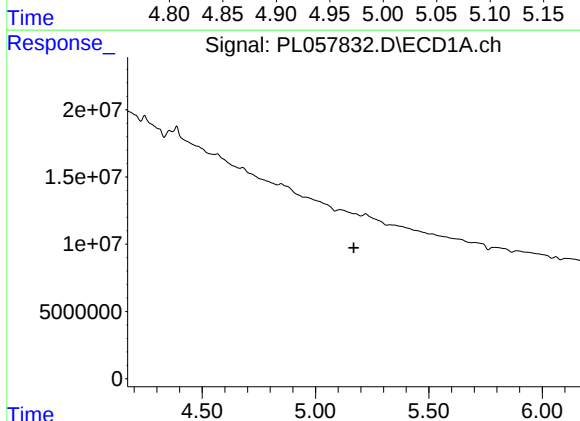


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.169 min
Response: 0
Conc: N.D.

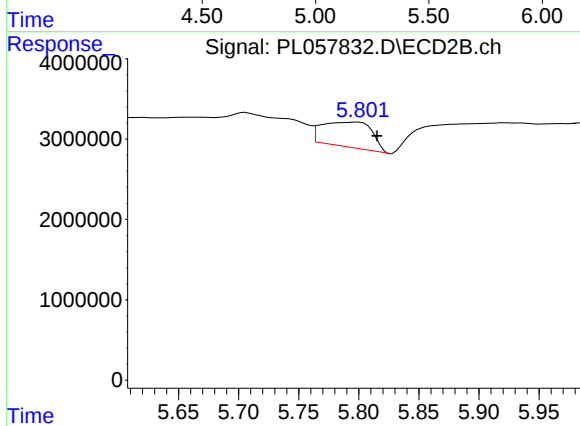

#8 Heptachlor epoxide


R.T.: 5.799 min
Delta R.T.: -0.016 min
Response: 9020667
Conc: 3.34 ng/ml

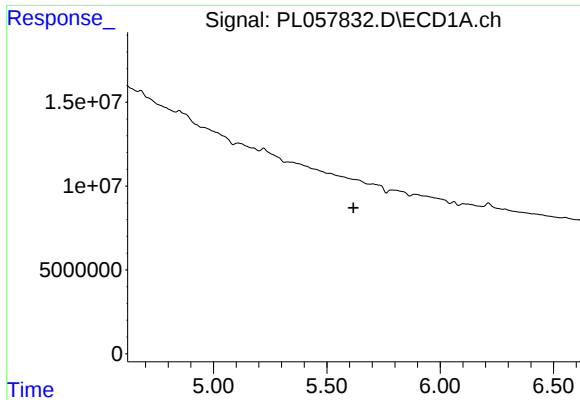

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 5.618 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

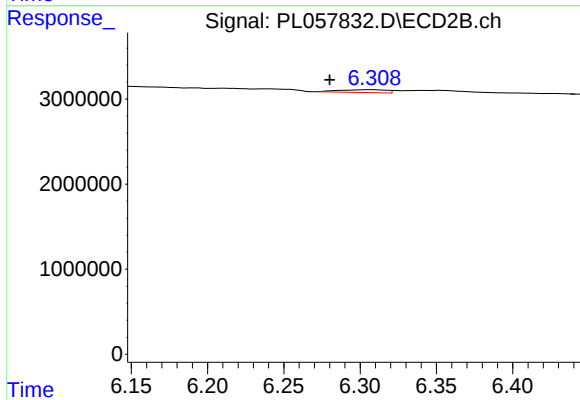


#12 4,4'-DDE

R.T.: 6.307 min
Delta R.T.: 0.027 min
Response: 649103
Conc: 0.22 ng/ml

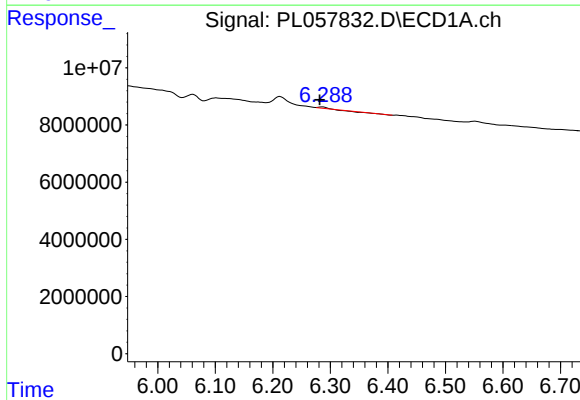


#15 Endosulfan II

R.T.: 6.287 min
Delta R.T.: 0.005 min
Response: 356018
Conc: 0.03 ng/ml

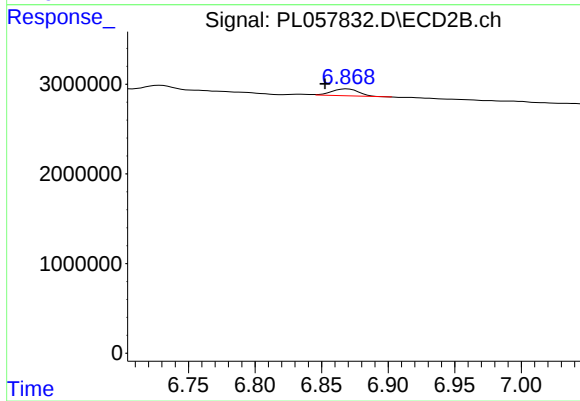

#15 Endosulfan II


R.T.: 6.869 min
Delta R.T.: 0.017 min
Response: 1054431
Conc: 0.41 ng/ml

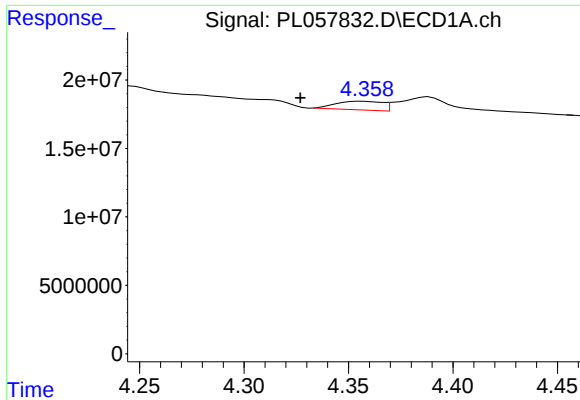

#23 Chlordane-1


R.T.: 4.357 min
Delta R.T.: 0.030 min
Response: 9970628
Conc: 26.96 ng/ml

Instrument :
ECD_L
ClientSampleId :

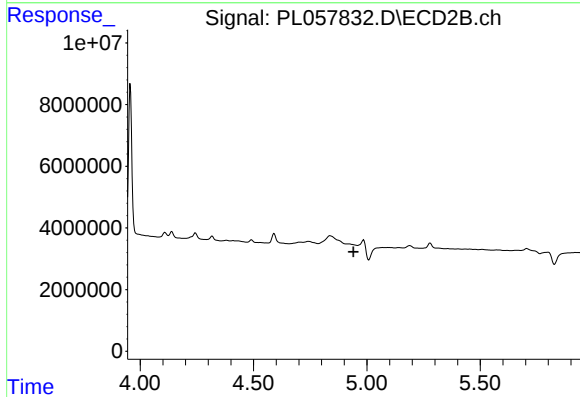


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.942 min
Response: 0
Conc: N.D.

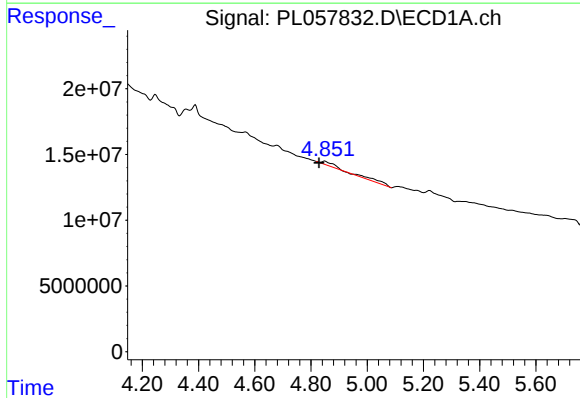


#24 Chlordane-2

R.T.: 4.849 min
Delta R.T.: 0.021 min
Response: 19872101
Conc: 49.22 ng/ml

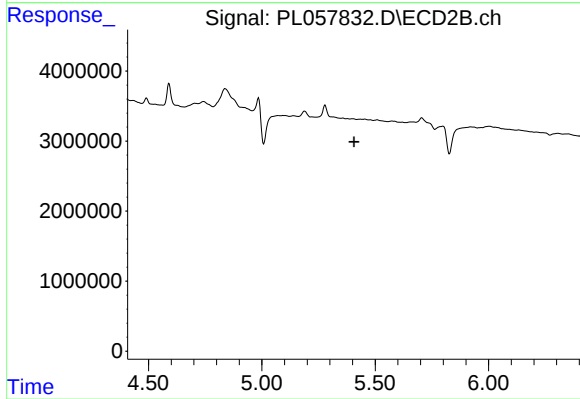

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.407 min
Response: 0
Conc: N.D.

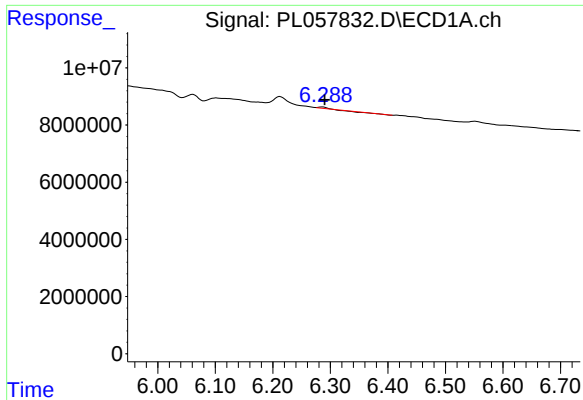

#27 Chlordane-5


R.T.: 6.287 min
Delta R.T.: -0.004 min
Response: 356018
Conc: 0.94 ng/ml

Instrument :
ECD_L
ClientSampleId :

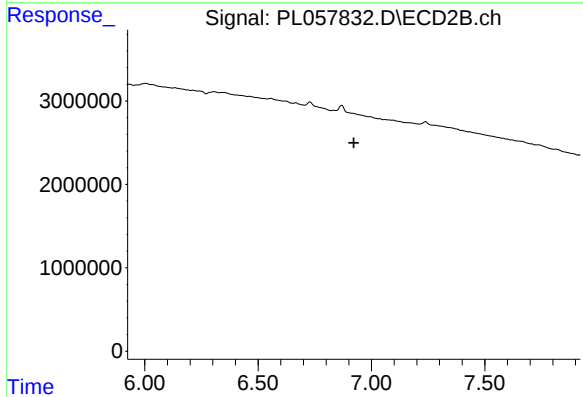


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.922 min
Response: 0
Conc: N.D.

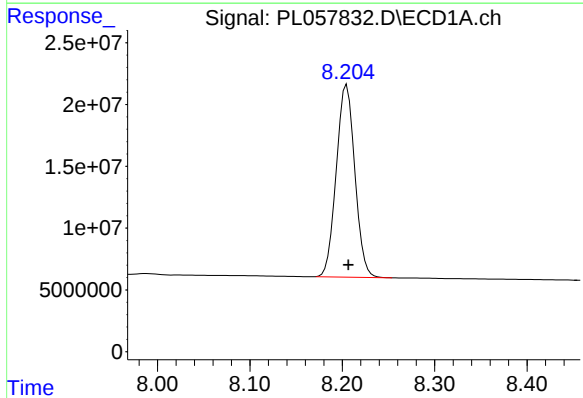

#28 Decachlorobiphenyl

R.T.: 8.205 min
Delta R.T.: -0.002 min
Response: 217598993
Conc: 21.11 ng/ml

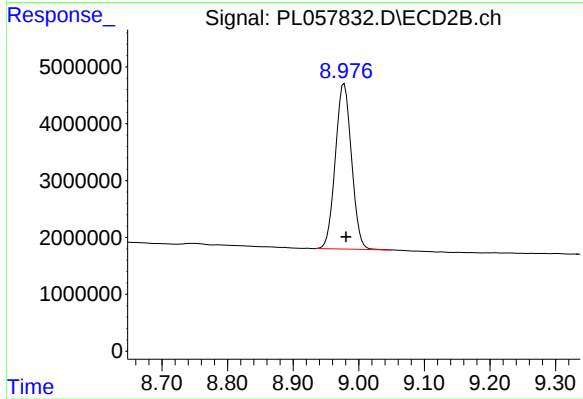

#28 Decachlorobiphenyl

R.T.: 8.978 min
Delta R.T.: -0.003 min
Response: 49792608
Conc: 22.29 ng/ml