

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040620\
 Data File : PL057835.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Apr 2020 21:41
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 07 01:14:29 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 04 06:41:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.457	3.956	228.1E6	47599788	22.630	21.934
28)	SA Decachlor...	8.204	8.977	215.2E6	49128090	20.880	21.993
Target Compounds							
2)	A alpha-BHC	3.896	0.000	4642456	0	0.267	N.D. #
4)	MA Heptachlor	0.000	5.142	0	551874	N.D.	0.164 #
8)	B Heptachlo...	0.000	5.803	0	2390317	N.D.	0.885 #
15)	B Endosulfa...	0.000	6.868f	0	674439	N.D.	0.260 #
20)	A Methoxychlor	6.902f	0.000	937730	0	0.170	N.D. #
23)	Chlordane-1	4.352f	0.000	2927563	0	7.916	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040620\
Data File : PL057835.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Apr 2020 21:41
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 07 01:14:29 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
Quant Title : GC Extractables
QLast Update : Sat Apr 04 06:41:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

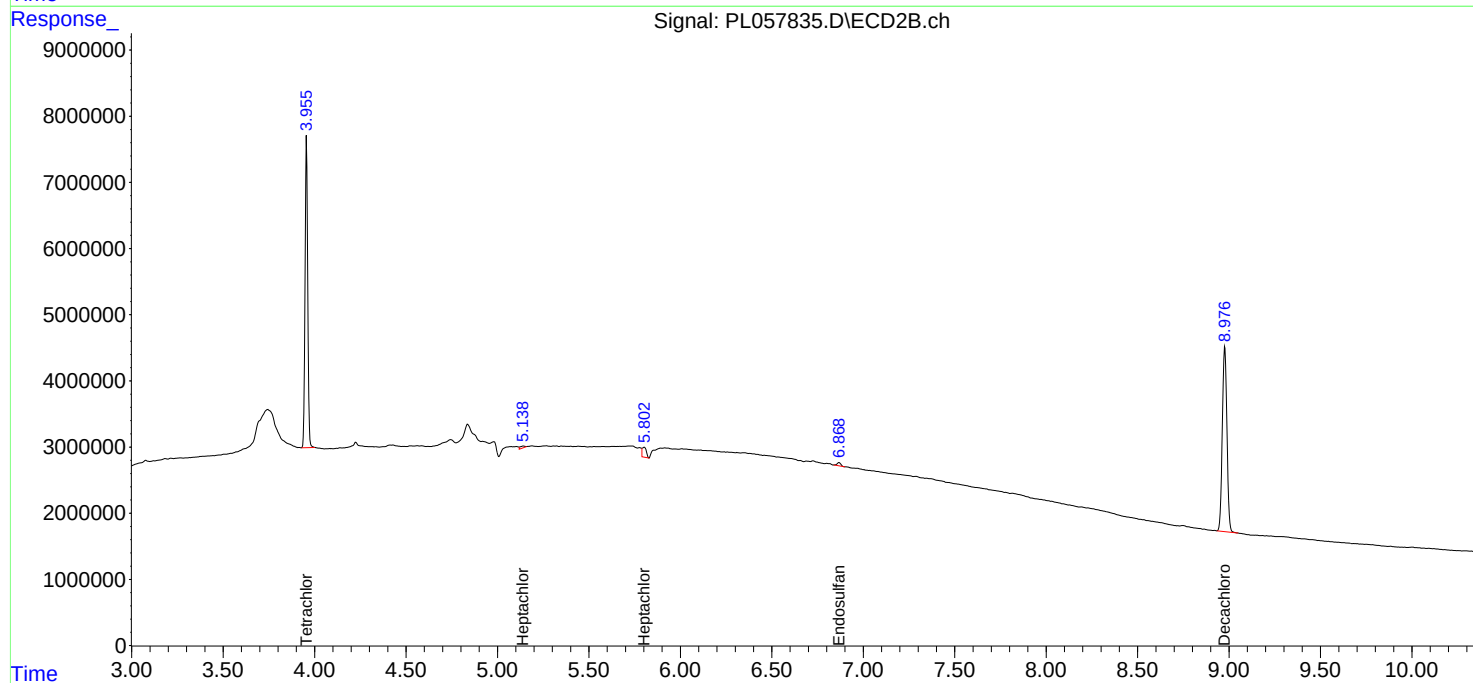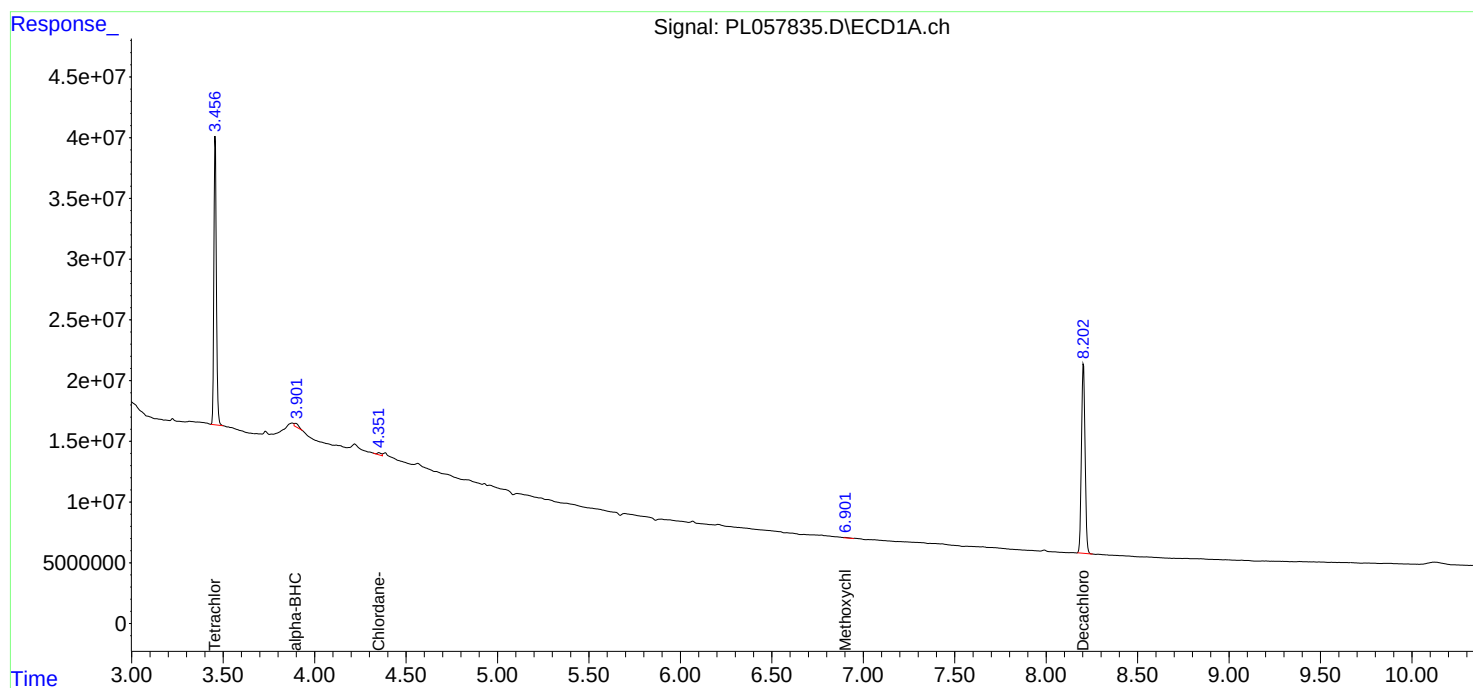


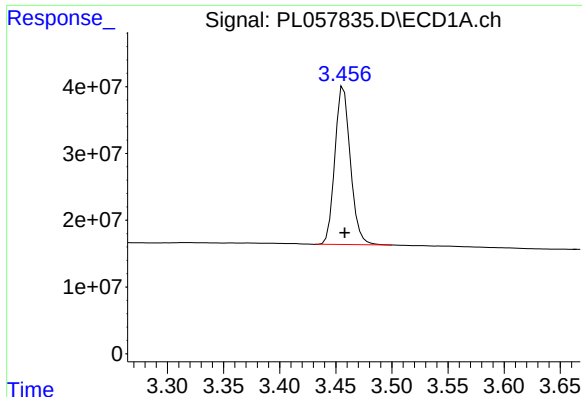

#1 Tetrachloro-m-xylene


R.T.: 3.457 min
Delta R.T.: 0.000 min
Response: 228129024
Conc: 22.63 ng/ml

Instrument :
ECD_L
ClientSampleId :

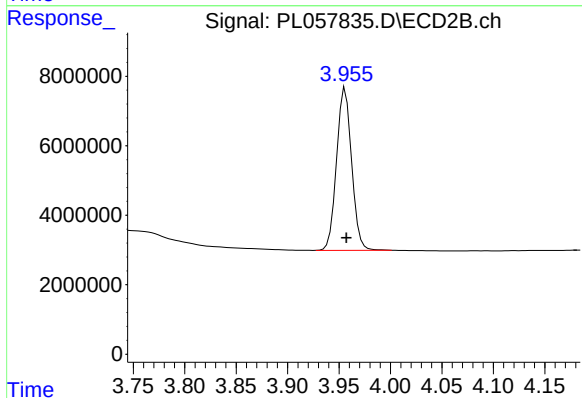


#1 Tetrachloro-m-xylene

R.T.: 3.956 min
Delta R.T.: -0.001 min
Response: 47599788
Conc: 21.93 ng/ml

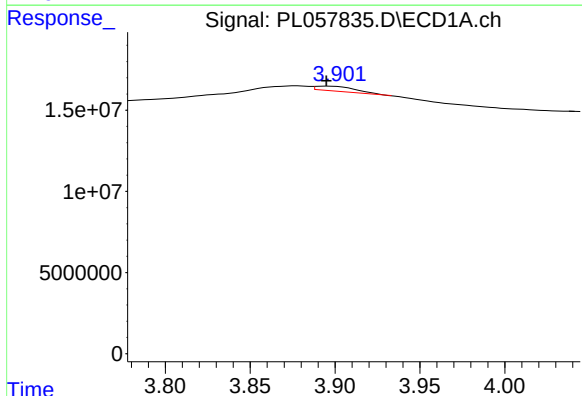


#2 alpha-BHC

R.T.: 3.896 min
Delta R.T.: 0.001 min
Response: 4642456
Conc: 0.27 ng/ml

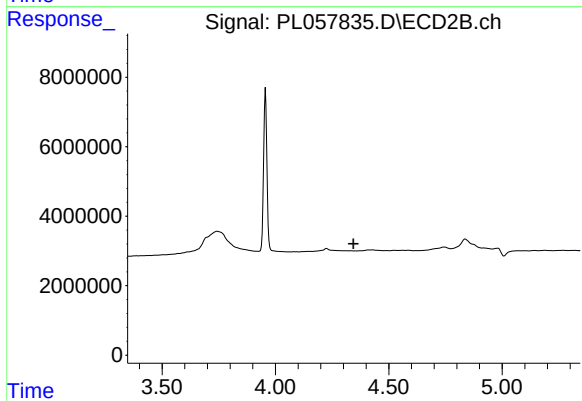

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.345 min
Response: 0
Conc: N.D.

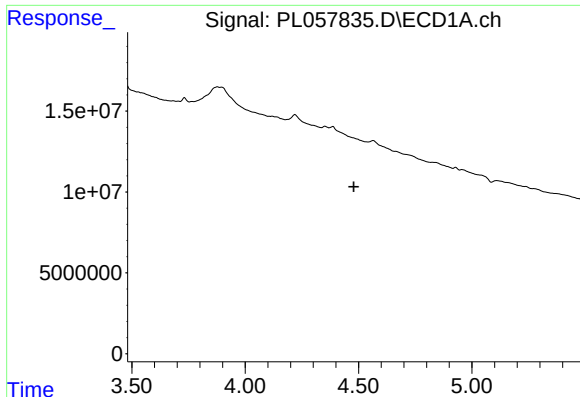

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.479 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

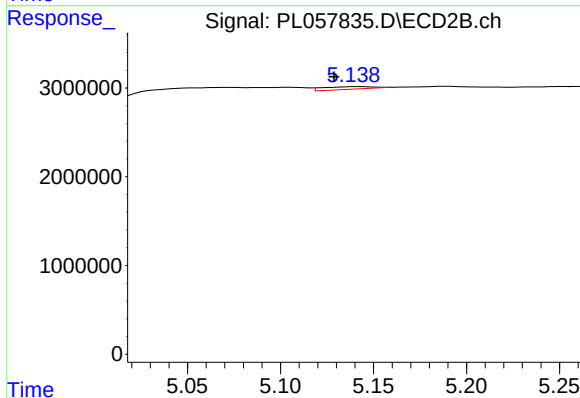


#4 Heptachlor

R.T.: 5.142 min
Delta R.T.: 0.013 min
Response: 551874
Conc: 0.16 ng/ml

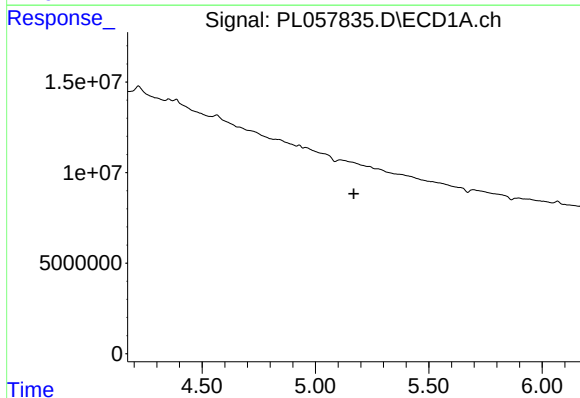


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.169 min
Response: 0
Conc: N.D.

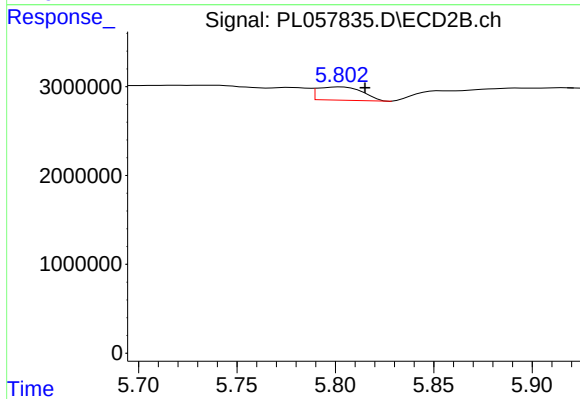

#8 Heptachlor epoxide


R.T.: 5.803 min
Delta R.T.: -0.012 min
Response: 2390317
Conc: 0.89 ng/ml

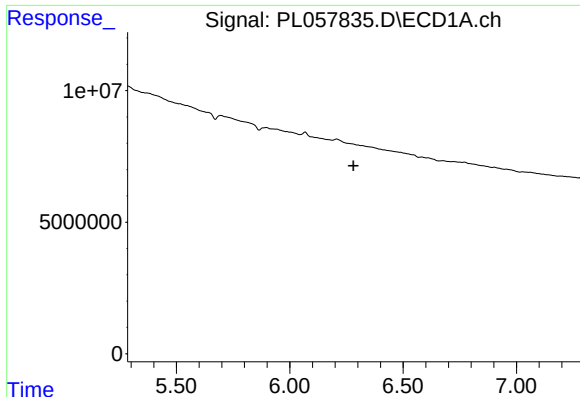

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.282 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

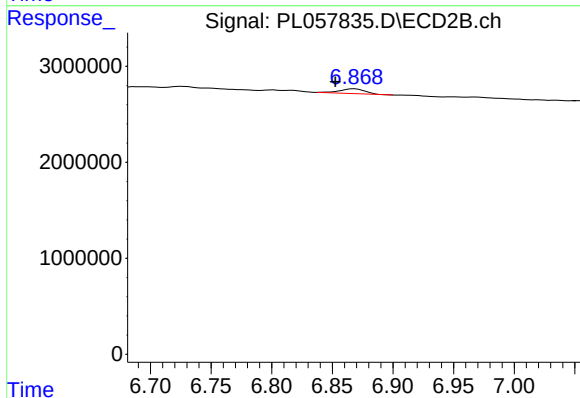


#15 Endosulfan II

R.T.: 6.868 min
Delta R.T.: 0.016 min
Response: 674439
Conc: 0.26 ng/ml

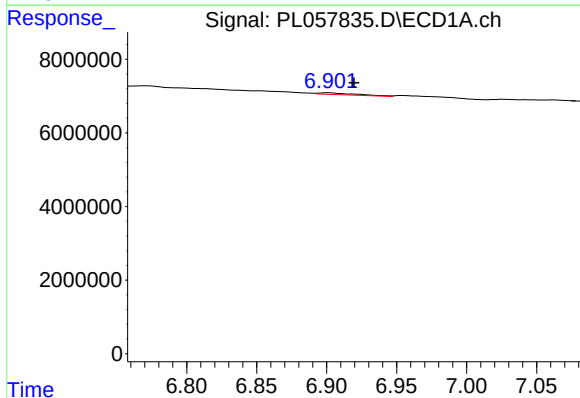


#20 Methoxychlor

R.T.: 6.902 min
Delta R.T.: -0.017 min
Response: 937730
Conc: 0.17 ng/ml

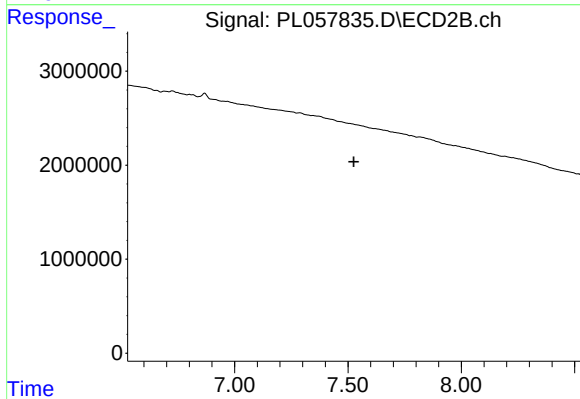

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 7.525 min
Response: 0
Conc: N.D.

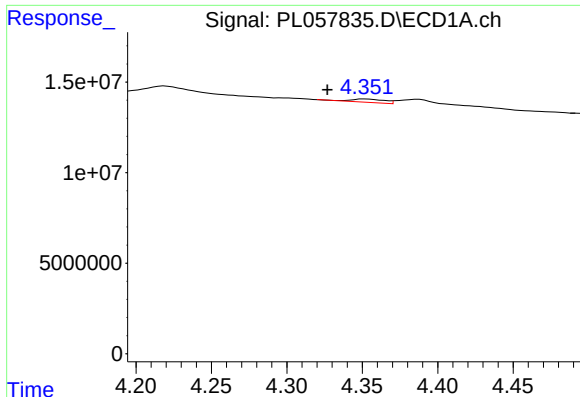

#23 Chlordane-1


R.T.: 4.352 min
Delta R.T.: 0.025 min
Response: 2927563
Conc: 7.92 ng/ml

Instrument :
ECD_L
ClientSampleId :

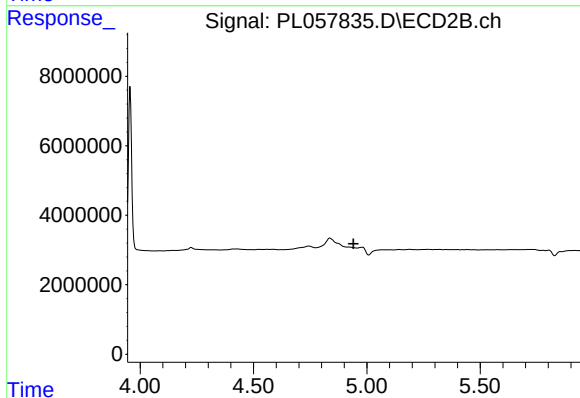


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.942 min
Response: 0
Conc: N.D.

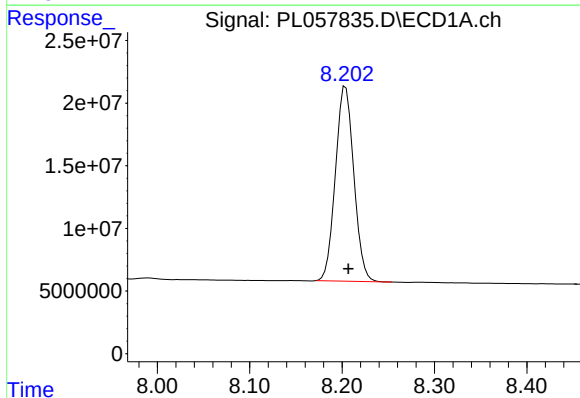

#28 Decachlorobiphenyl

R.T.: 8.204 min
Delta R.T.: -0.003 min
Response: 215243647
Conc: 20.88 ng/ml

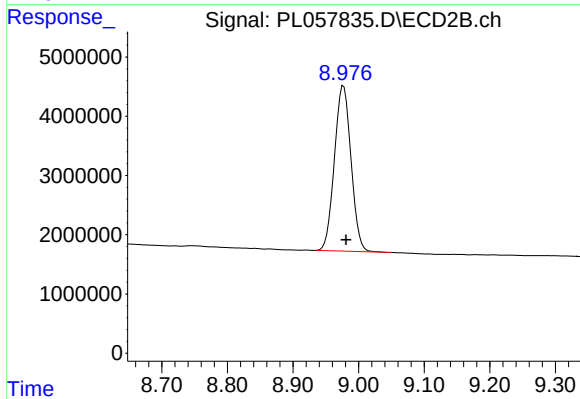

#28 Decachlorobiphenyl

R.T.: 8.977 min
Delta R.T.: -0.004 min
Response: 49128090
Conc: 21.99 ng/ml