

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040620\
 Data File : PL057815.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Apr 2020 16:58
 Operator : AJ\MA
 Sample : L2164-02
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ROLL-OFF-COMP

Manual Integrations
 APPROVED

mohammad
 4/7/2020 2:32:02 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 07 01:08:39 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 04 06:41:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.459	3.956	101.4E6	23144487	10.057	10.665
28)	SA Decachlor...	8.205	8.979	114.8E6	27215832	11.132	12.184
Target Compounds							
12)	B 4,4'-DDE	5.616	6.277	7295292	2549175	0.557m	0.861m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040620\
Data File : PL057815.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Apr 2020 16:58
Operator : AJ\MA
Sample : L2164-02
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
ROLL-OFF-COMP


Manual Integrations
APPROVED

mohammad
4/7/2020 2:32:02 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 07 01:08:39 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
Quant Title : GC Extractables
QLast Update : Sat Apr 04 06:41:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

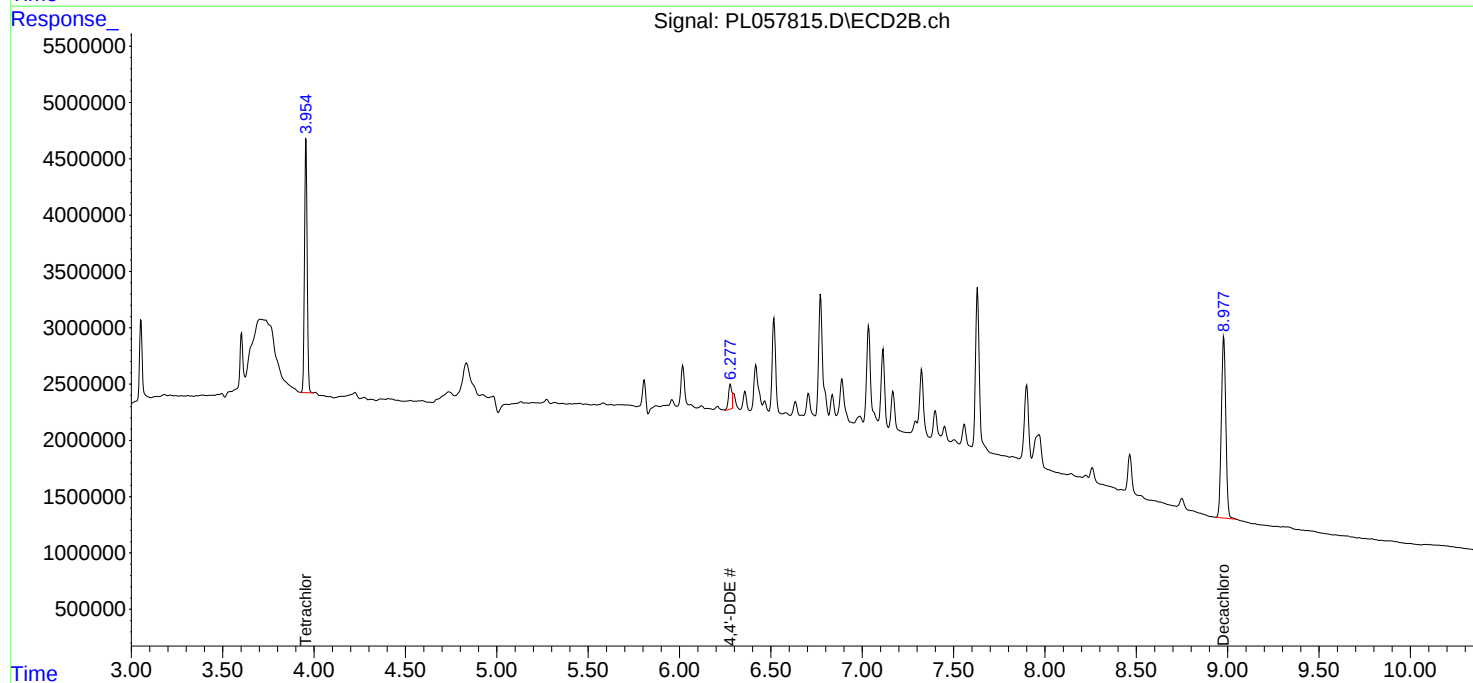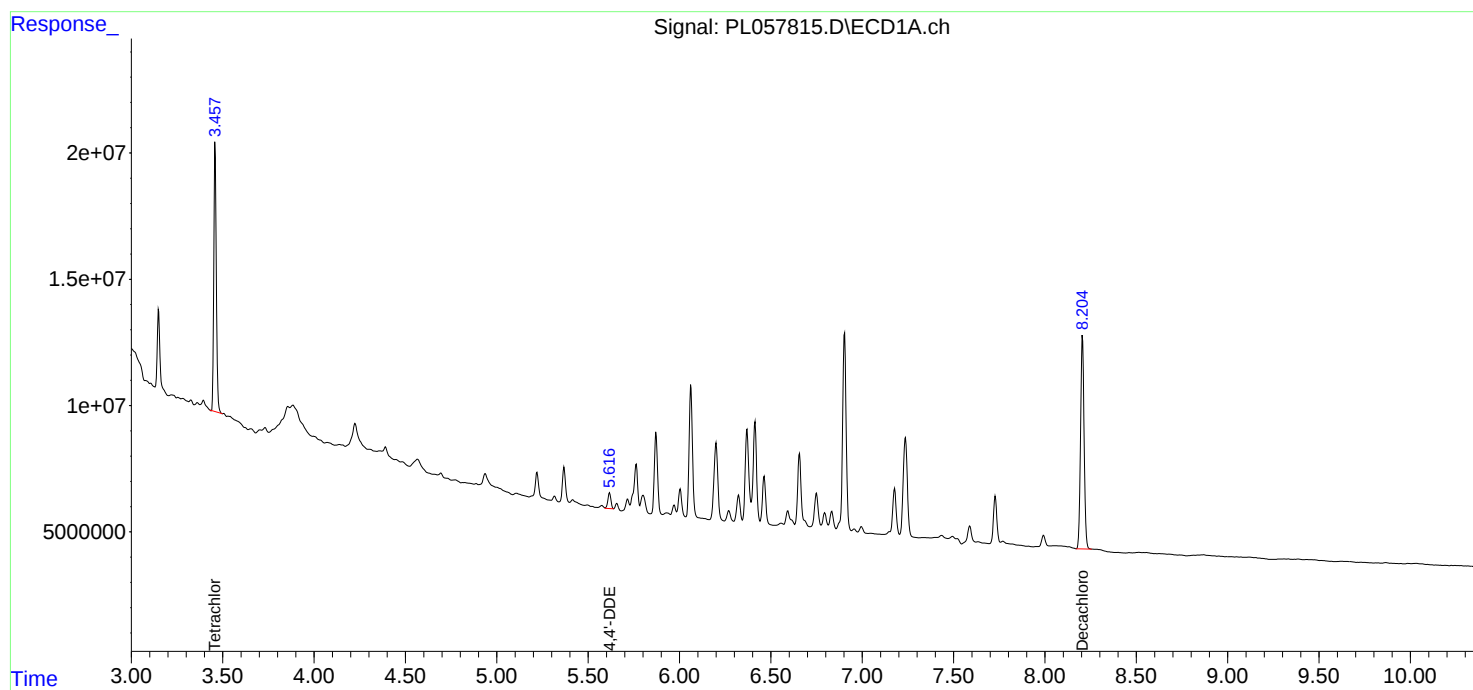

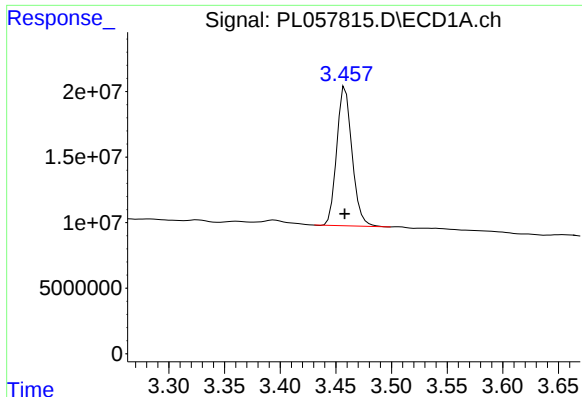


#1 Tetrachloro-m-xylene

R.T.: 3.459 min
Delta R.T.: 0.000 min
Response: 101387302
Conc: 10.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
ROLL-OFF-COMP


Manual Integrations
APPROVED

mohammad
4/7/2020 2:32:02 PM

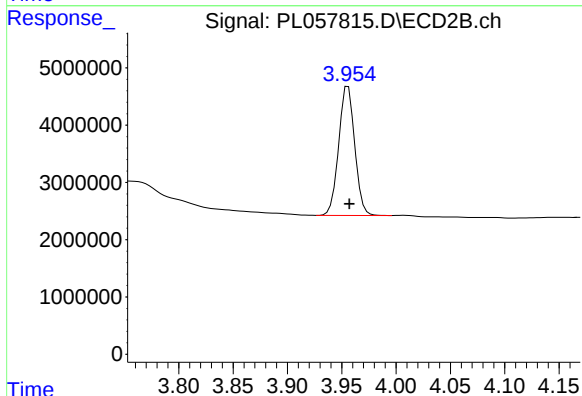


#1 Tetrachloro-m-xylene

R.T.: 3.956 min
Delta R.T.: -0.001 min
Response: 23144487
Conc: 10.66 ng/ml

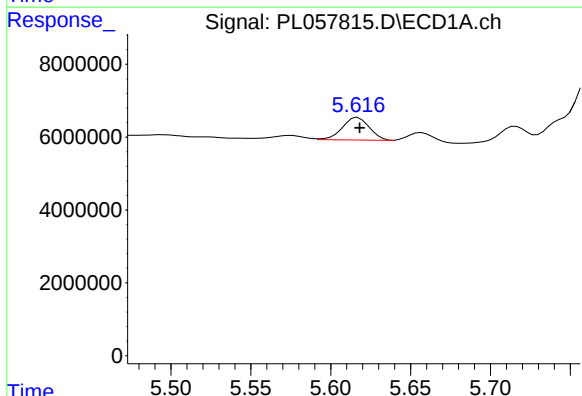


#12 4,4'-DDE

R.T.: 5.616 min
Delta R.T.: -0.003 min
Response: 7295292
Conc: 0.56 ng/ml m

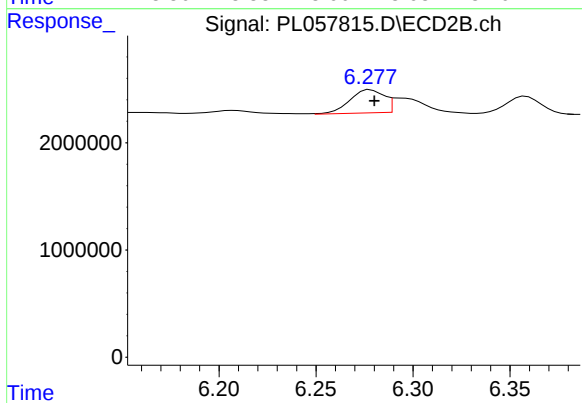

#12 4,4'-DDE

R.T.: 6.277 min
Delta R.T.: -0.003 min
Response: 2549175
Conc: 0.86 ng/ml m

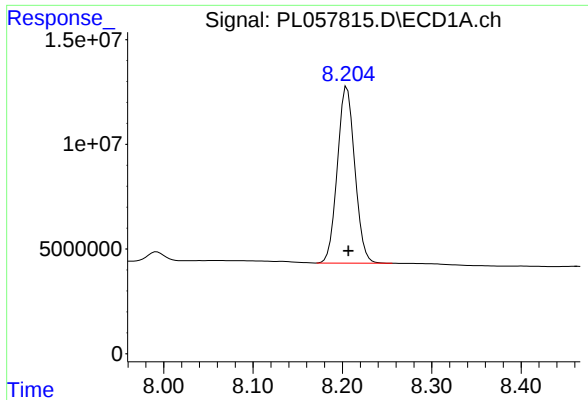


#28 Decachlorobiphenyl

R.T.: 8.205 min
Delta R.T.: -0.002 min
Response: 114757119
Conc: 11.13 ng/ml

Instrument :
ECD_L
ClientSampleId :
ROLL-OFF-COMP

Manual Integrations
APPROVED

mohammad
4/7/2020 2:32:02 PM

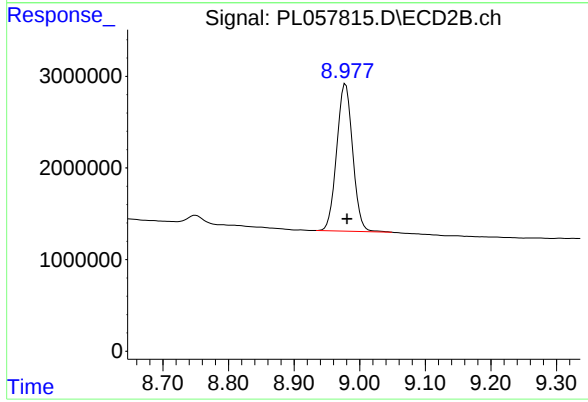

#28 Decachlorobiphenyl

R.T.: 8.979 min
Delta R.T.: -0.002 min
Response: 27215832
Conc: 12.18 ng/ml