

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040621\
 Data File : PL065890.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Apr 2021 09:24
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 07 04:27:41 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 31 15:57:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
28)	SA Decachlor...	7.904	0.000	2815060	0	1.215	N.D. #
Target Compounds							
4)	MA Heptachlor	0.000	4.941	0	1352753	N.D.	0.383 #
6)	B beta-BHC	4.223	4.629	-3730349	14313423	N.D.	8.218
8)	B Heptachlo...	0.000	5.601	0	7076674	N.D.	2.279 #
11)	B alpha-Chl...	0.000	5.923	0	307267	N.D.	0.104 #
14)	MA Endrin	5.750	0.000	526605	0	0.195	N.D. #
15)	B Endosulfa...	0.000	6.670f	0	406110	N.D.	0.172 #
18)	B Endrin al...	0.000	6.766	0	284940	N.D.	0.150 #
21)	B Endrin ke...	0.000	7.442f	0	113841	N.D.	0.044 #
26)	Chlordane-4	0.000	5.923	0	307267	N.D.	0.607 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040621\
Data File : PL065890.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Apr 2021 09:24
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 07 04:27:41 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
Quant Title : GC Extractables
QLast Update : Wed Mar 31 15:57:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

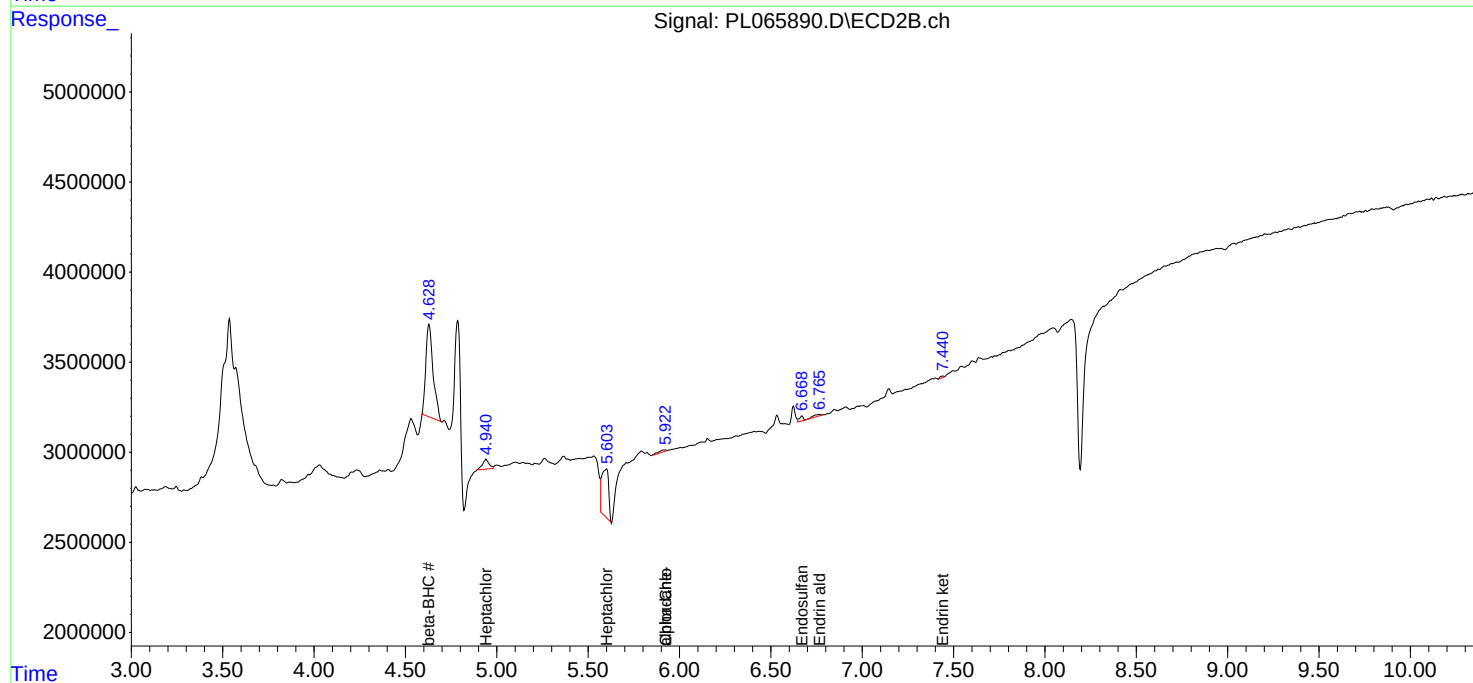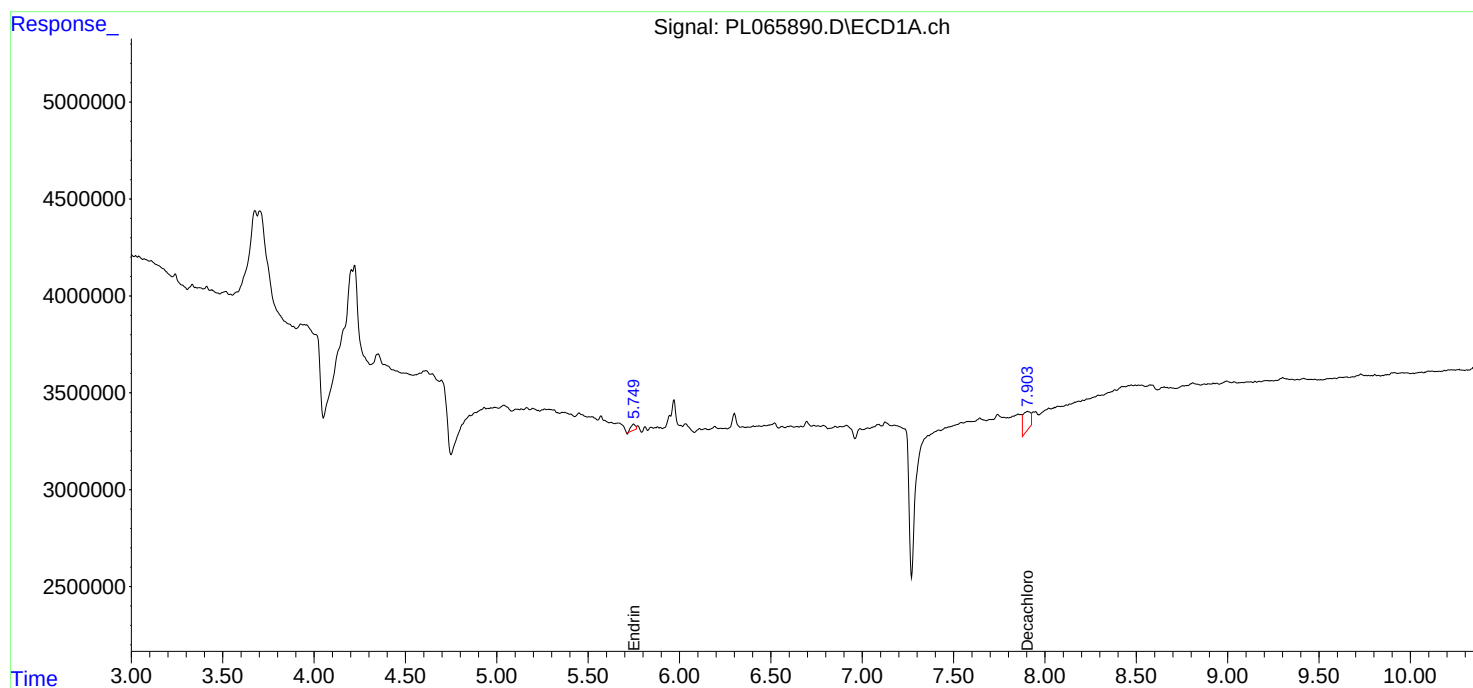


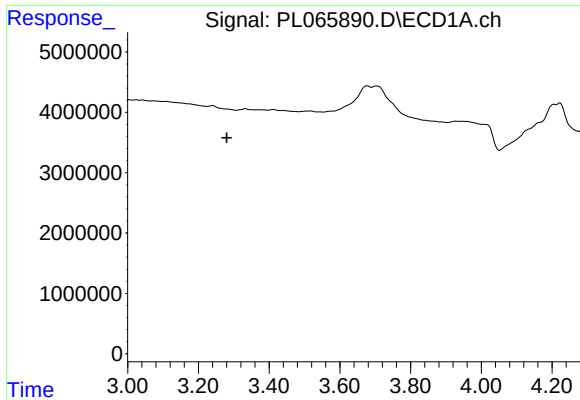

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.280 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

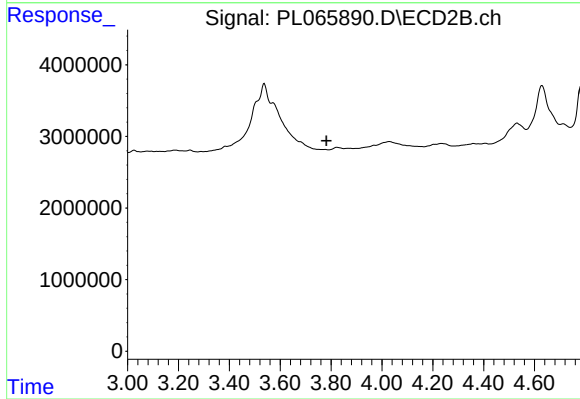


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.782 min
Response: 0
Conc: N.D.

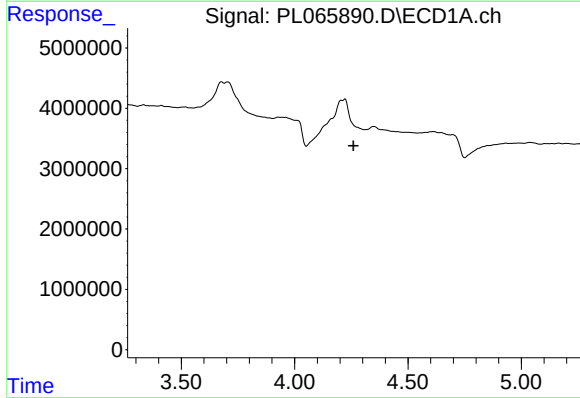


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.260 min
Response: 0
Conc: N.D.

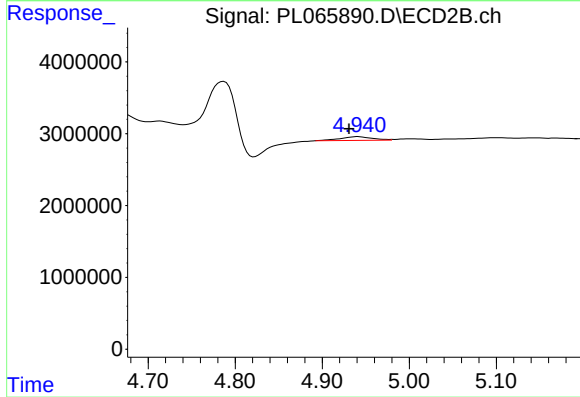

#4 Heptachlor


R.T.: 4.941 min
Delta R.T.: 0.010 min
Response: 1352753
Conc: 0.38 ng/ml

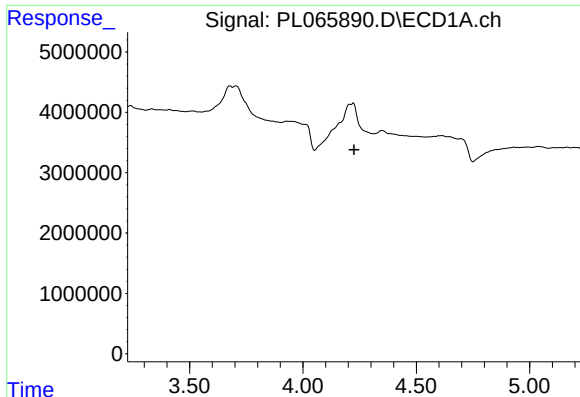

#6 beta-BHC


R.T.: 4.223 min
Delta R.T.: -0.004 min
Response: -3730349
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

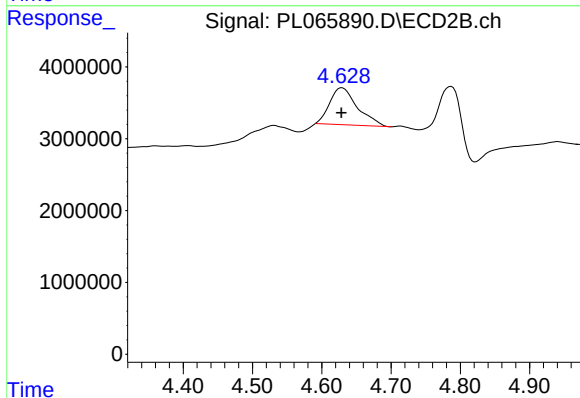


#6 beta-BHC

R.T.: 4.629 min
Delta R.T.: 0.000 min
Response: 14313423
Conc: 8.22 ng/ml

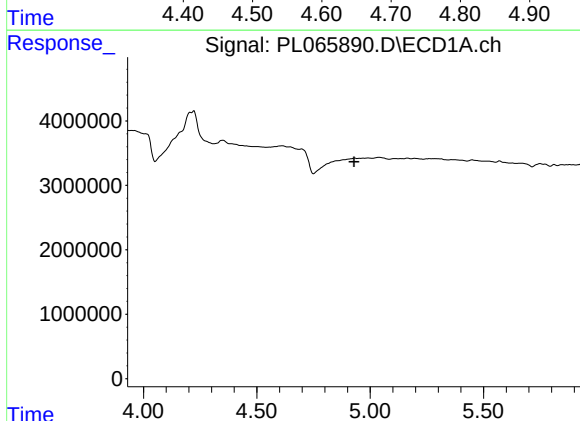


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.929 min
Response: 0
Conc: N.D.

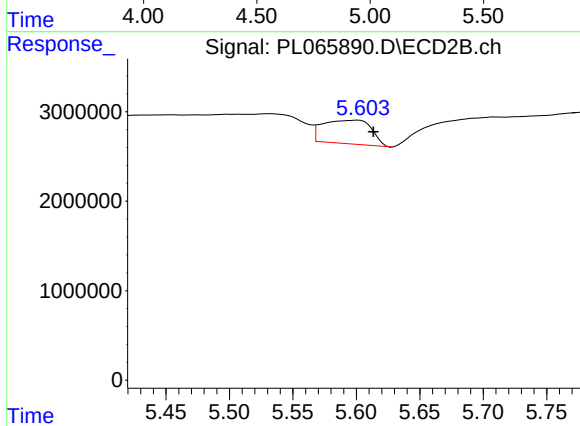

#8 Heptachlor epoxide


R.T.: 5.601 min
Delta R.T.: -0.012 min
Response: 7076674
Conc: 2.28 ng/ml

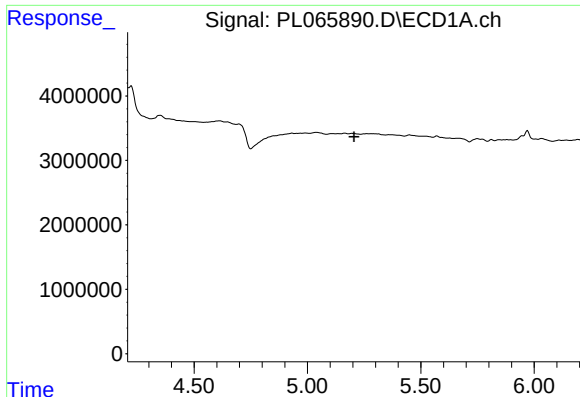

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.206 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

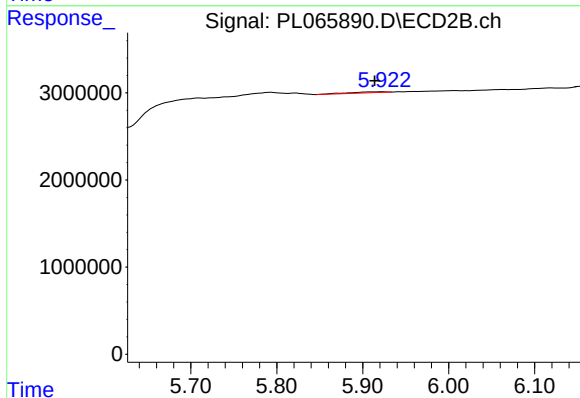


#11 alpha-Chlordane

R.T.: 5.923 min
Delta R.T.: 0.009 min
Response: 307267
Conc: 0.10 ng/ml

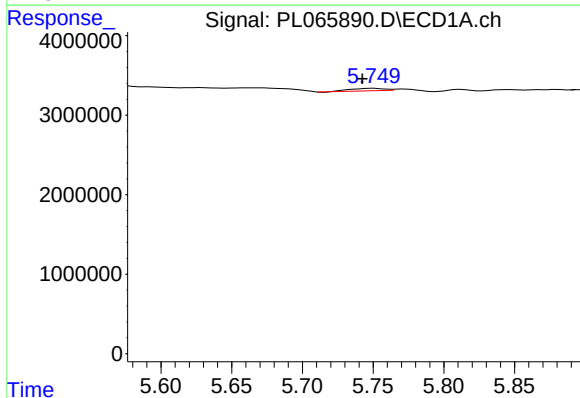


#14 Endrin

R.T.: 5.750 min
Delta R.T.: 0.007 min
Response: 526605
Conc: 0.20 ng/ml

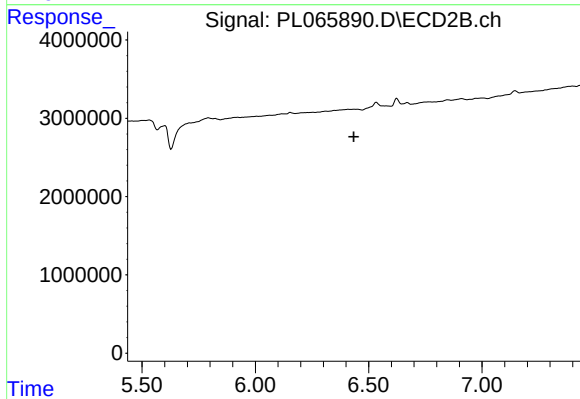

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.434 min
Response: 0
Conc: N.D.

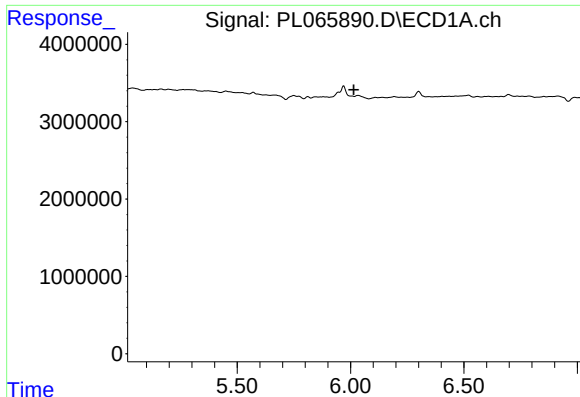

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.015 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

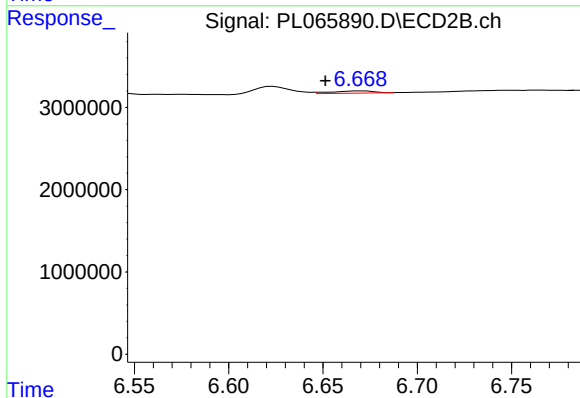


#15 Endosulfan II

R.T.: 6.670 min
Delta R.T.: 0.019 min
Response: 406110
Conc: 0.17 ng/ml

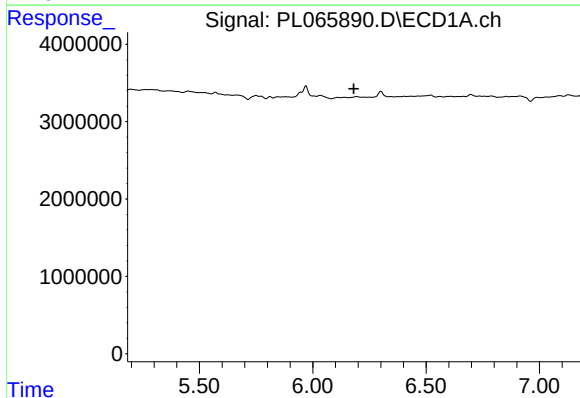


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 6.181 min
Response: 0
Conc: N.D.

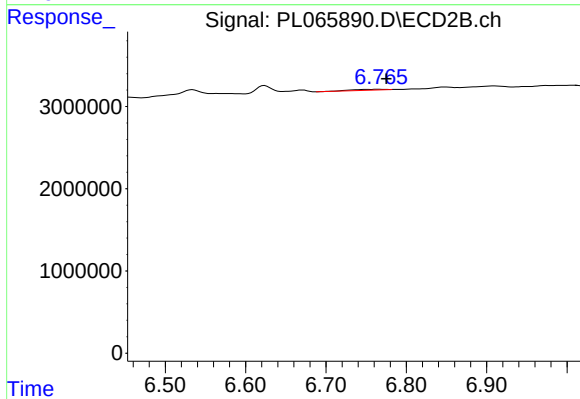

#18 Endrin aldehyde


R.T.: 6.766 min
Delta R.T.: -0.010 min
Response: 284940
Conc: 0.15 ng/ml

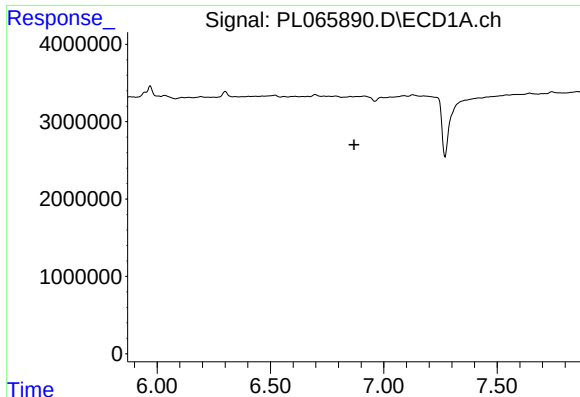

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 6.870 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

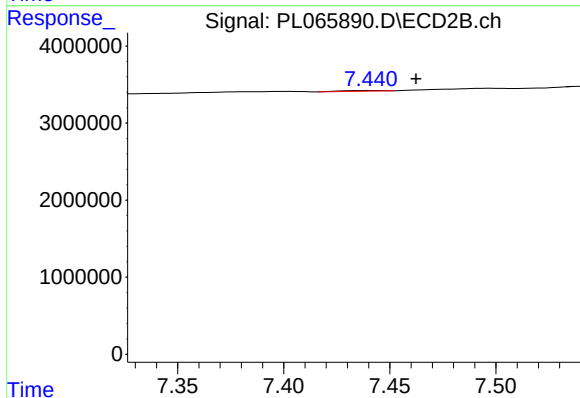


#21 Endrin ketone

R.T.: 7.442 min
Delta R.T.: -0.020 min
Response: 113841
Conc: 0.04 ng/ml

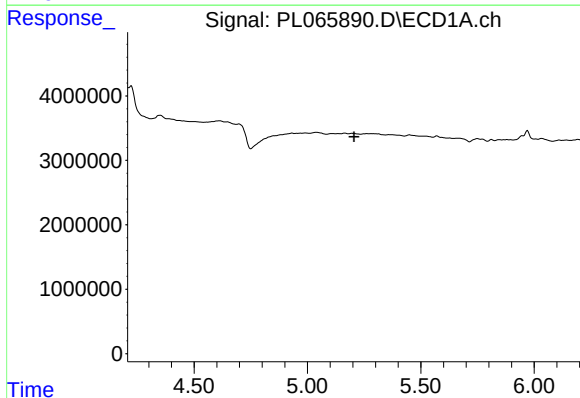


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.205 min
Response: 0
Conc: N.D.

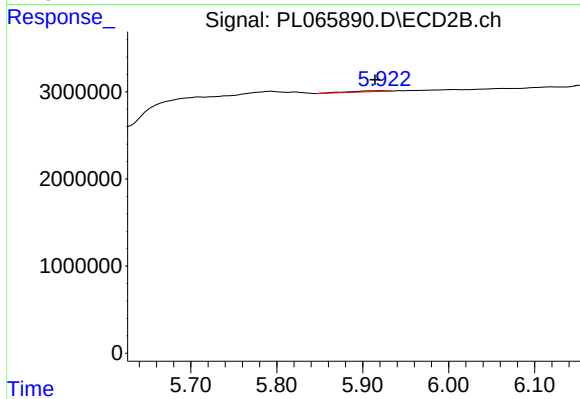

#26 Chlordane-4


R.T.: 5.923 min
Delta R.T.: 0.009 min
Response: 307267
Conc: 0.61 ng/ml

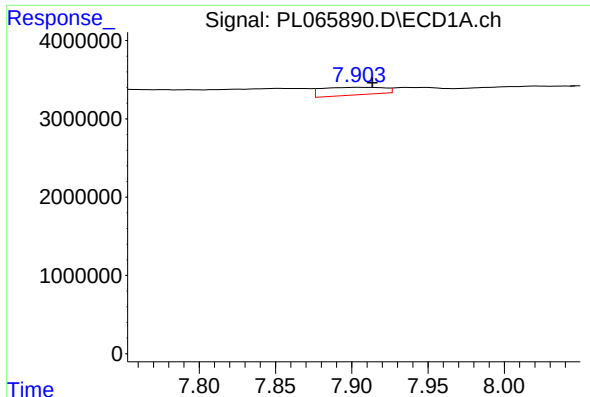

#28 Decachlorobiphenyl

R.T.: 7.904 min
Delta R.T.: -0.009 min
Response: 2815060
Conc: 1.22 ng/ml

Instrument :
ECD_L
ClientSampleId :

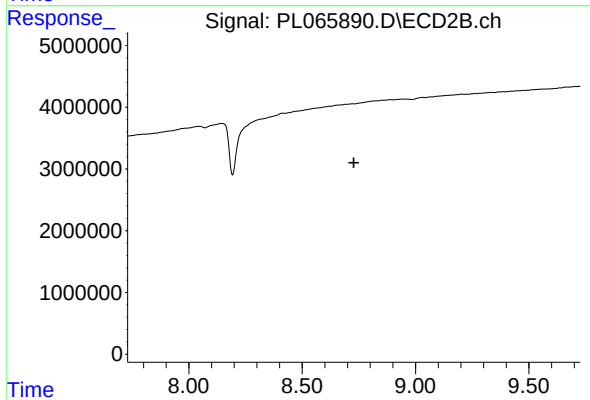

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.728 min
Response: 0
Conc: N.D.