

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040621\
 Data File : PL065899.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Apr 2021 12:07
 Operator : AR\AJ
 Sample : PB135502BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 07 04:30:06 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 31 15:57:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.276	3.780	47879417	50731536	18.380	18.482
28)	SA Decachlor...	7.908	8.727	51194243	46494924	22.104	20.623
Target Compounds							
4)	MA Heptachlor	0.000	4.947f	0	1054022	N.D.	0.299 #
6)	B beta-BHC	4.228	4.630	-411442	4920790	N.D.	2.825
8)	B Heptachlo...	0.000	5.612	0	2407455	N.D.	0.775 #
14)	MA Endrin	5.752	0.000	1195232	0	0.443	N.D. #
15)	B Endosulfa...	0.000	6.673f	0	319988	N.D.	0.135 #
17)	MA 4,4'-DDT	0.000	6.887f	0	159695	N.D.	0.071 #
18)	B Endrin al...	0.000	6.775	0	59603	N.D.	0.031 #
20)	A Methoxychlor	0.000	7.322	0	290044	N.D.	0.229 #
21)	B Endrin ke...	0.000	7.468	0	90242	N.D.	0.035 #
24)	Chlordane-2	4.616f	0.000	1724501	0	15.004	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040621\
Data File : PL065899.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Apr 2021 12:07
Operator : AR\AJ
Sample : PB135502BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 07 04:30:06 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
Quant Title : GC Extractables
QLast Update : Wed Mar 31 15:57:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

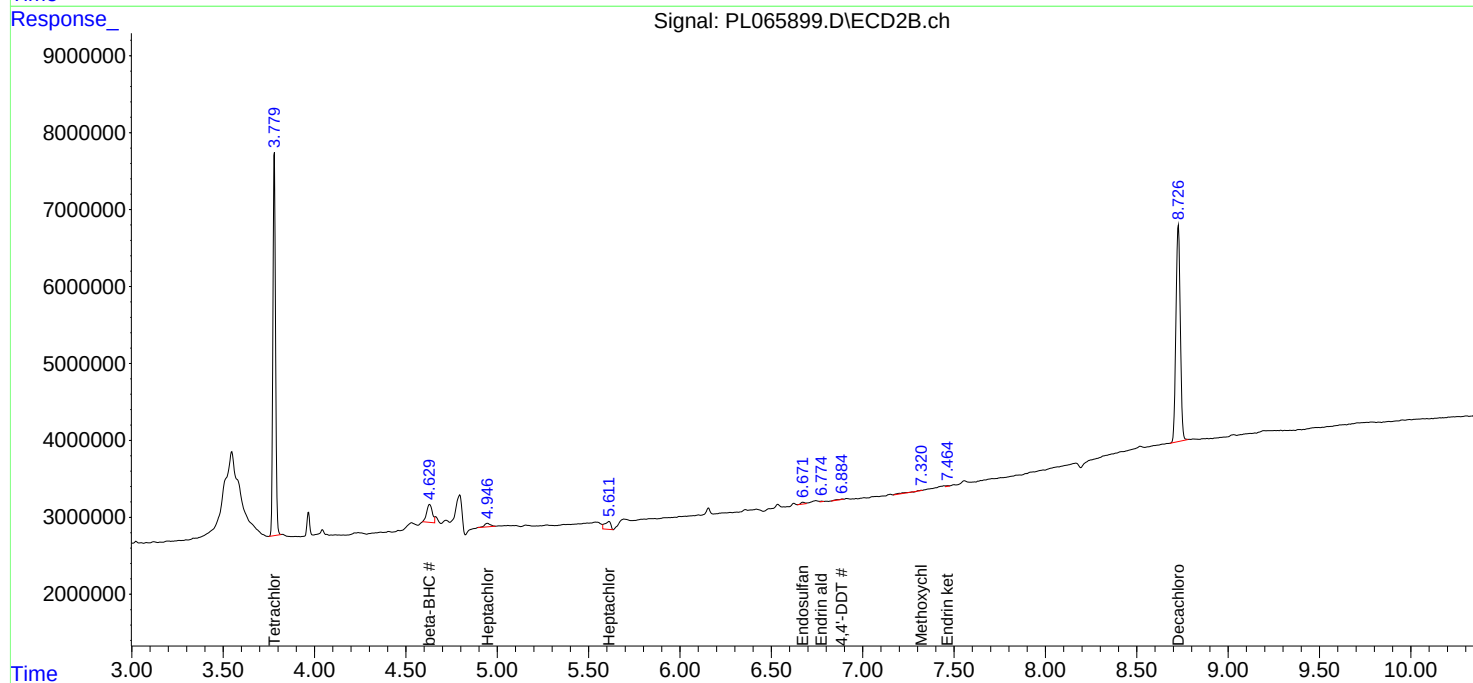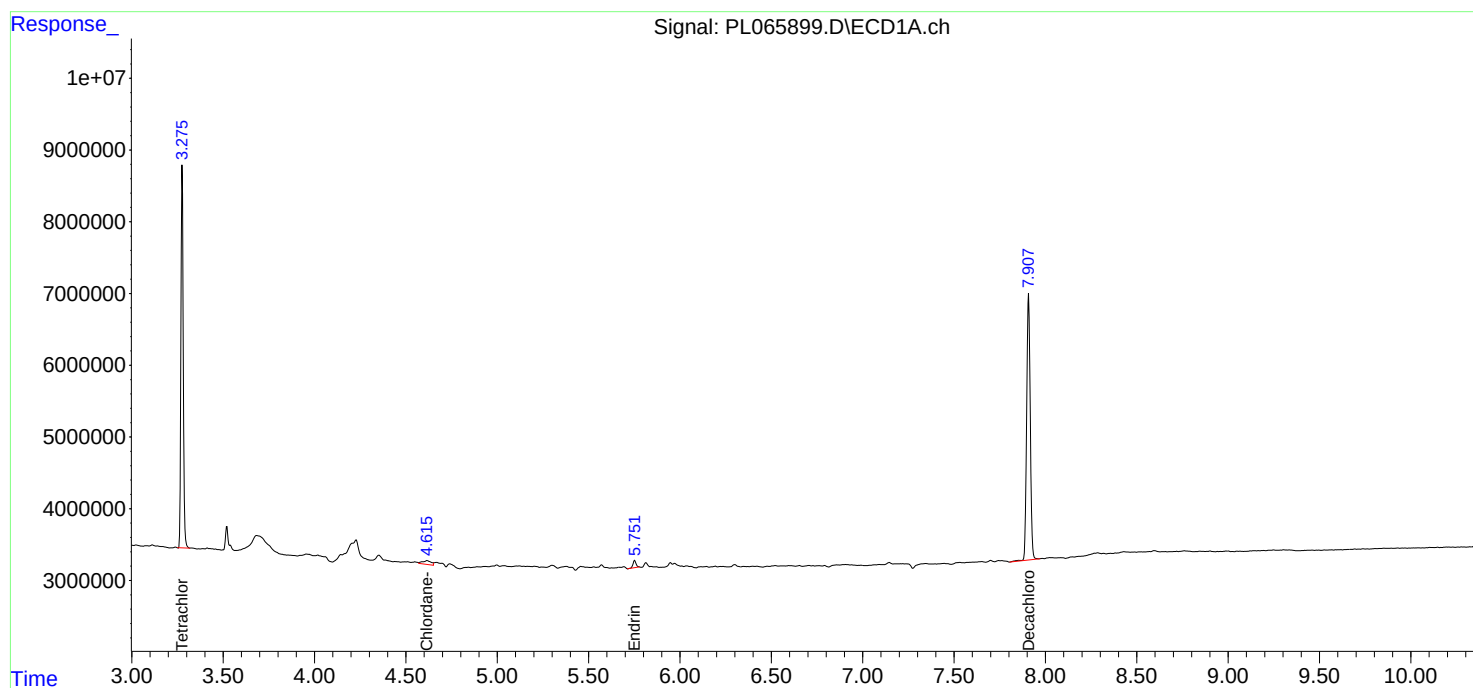


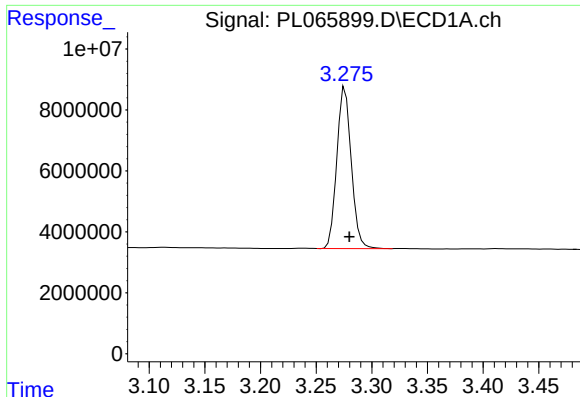

#1 Tetrachloro-m-xylene


R.T.: 3.276 min
Delta R.T.: -0.004 min
Response: 47879417
Conc: 18.38 ng/ml

Instrument :
ECD_L
ClientSampleId :

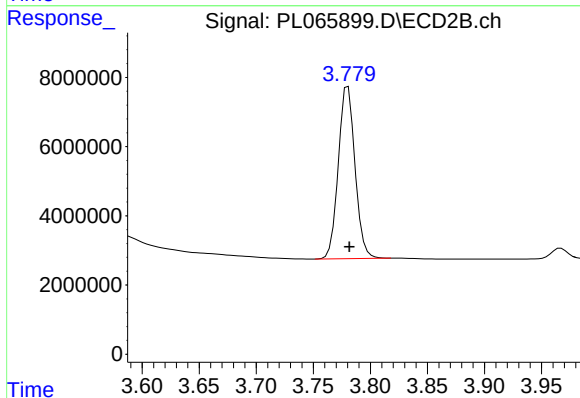


#1 Tetrachloro-m-xylene

R.T.: 3.780 min
Delta R.T.: -0.001 min
Response: 50731536
Conc: 18.48 ng/ml

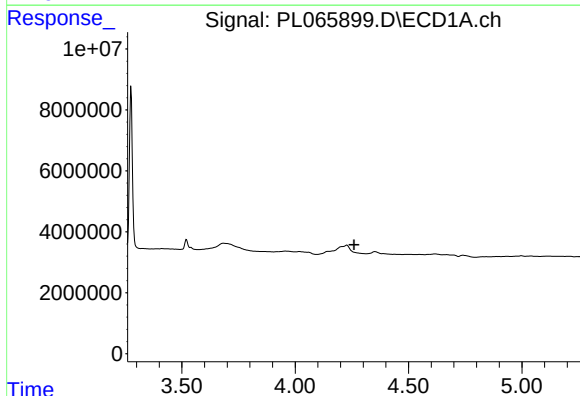


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.260 min
Response: 0
Conc: N.D.

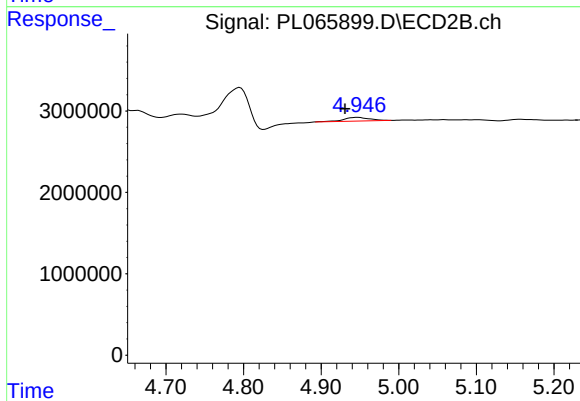

#4 Heptachlor


R.T.: 4.947 min
Delta R.T.: 0.016 min
Response: 1054022
Conc: 0.30 ng/ml

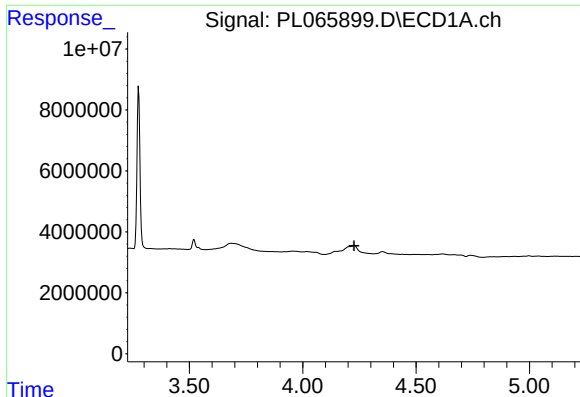

#6 beta-BHC


R.T.: 4.228 min
Delta R.T.: 0.001 min
Response: -411442
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

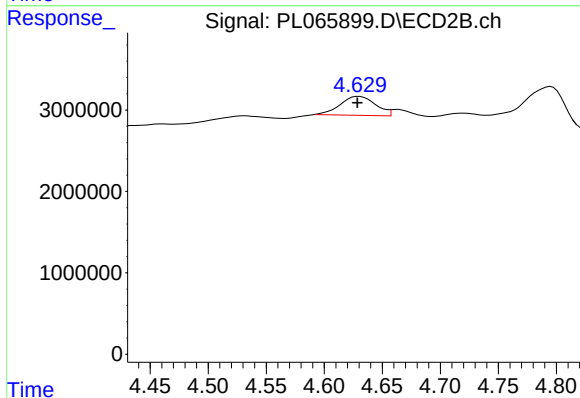


#6 beta-BHC

R.T.: 4.630 min
Delta R.T.: 0.001 min
Response: 4920790
Conc: 2.83 ng/ml

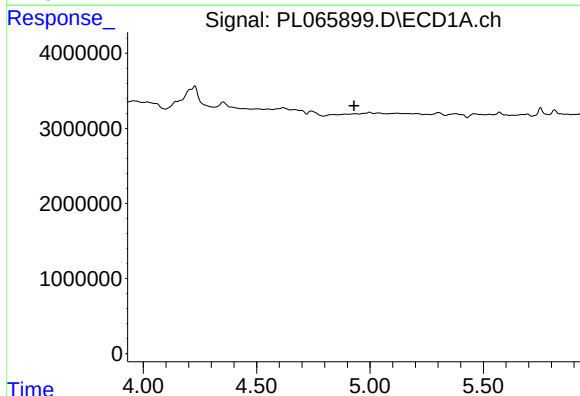


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.929 min
Response: 0
Conc: N.D.

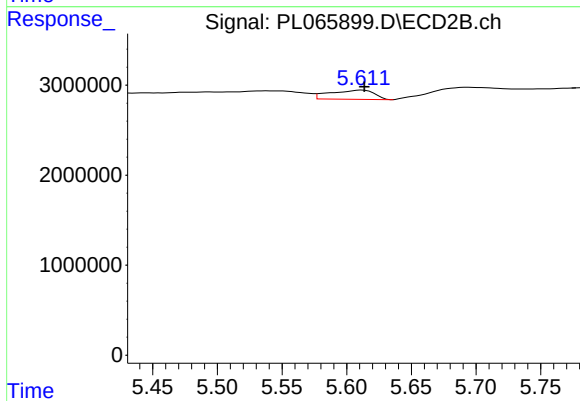

#8 Heptachlor epoxide


R.T.: 5.612 min
Delta R.T.: -0.001 min
Response: 2407455
Conc: 0.78 ng/ml

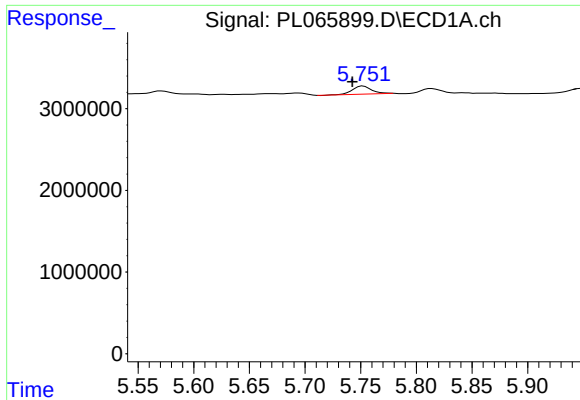

#14 Endrin


R.T.: 5.752 min
Delta R.T.: 0.010 min
Response: 1195232
Conc: 0.44 ng/ml

Instrument :
ECD_L
ClientSampleId :

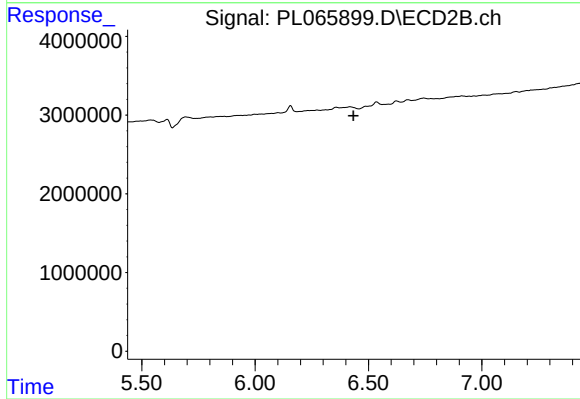


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.434 min
Response: 0
Conc: N.D.

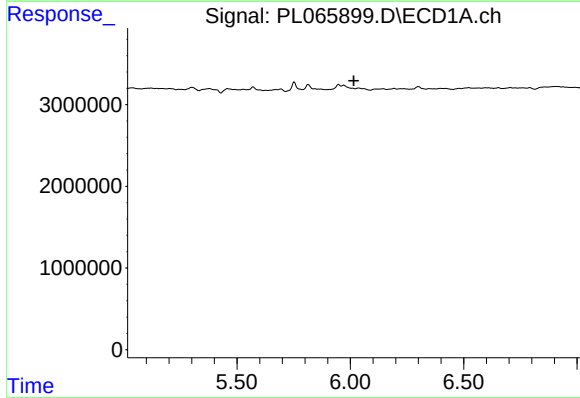


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.015 min
Response: 0
Conc: N.D.

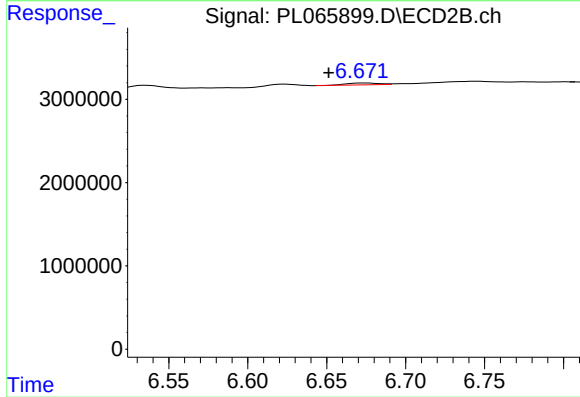

#15 Endosulfan II


R.T.: 6.673 min
Delta R.T.: 0.022 min
Response: 319988
Conc: 0.14 ng/ml

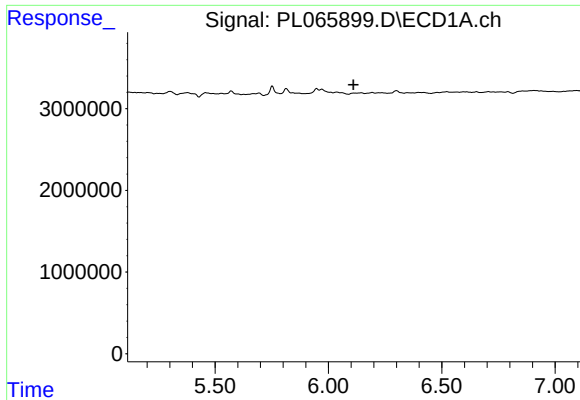

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.111 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

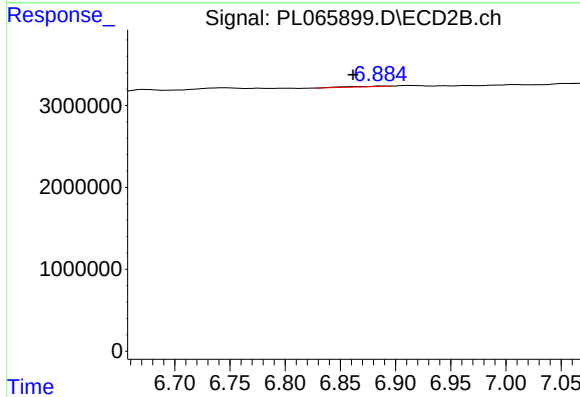


#17 4,4'-DDT

R.T.: 6.887 min
Delta R.T.: 0.025 min
Response: 159695
Conc: 0.07 ng/ml

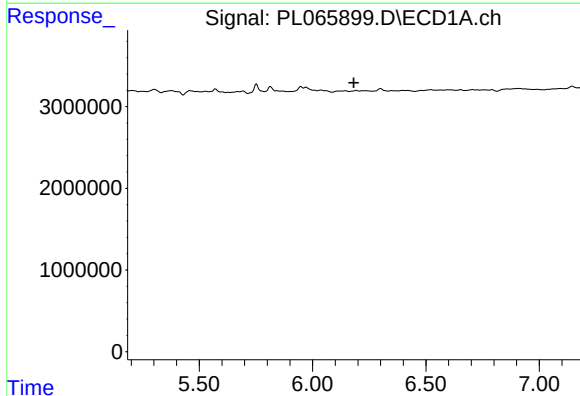


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 6.181 min
Response: 0
Conc: N.D.

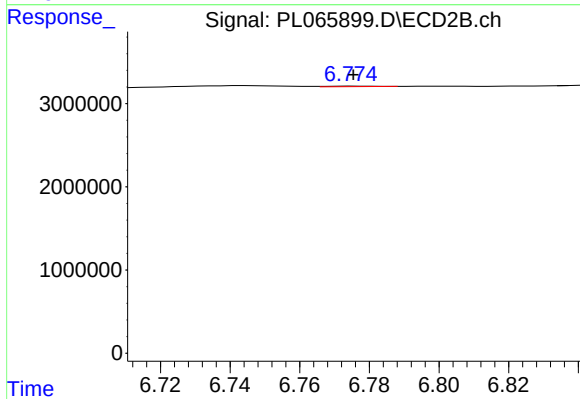

#18 Endrin aldehyde


R.T.: 6.775 min
Delta R.T.: 0.000 min
Response: 59603
Conc: 0.03 ng/ml

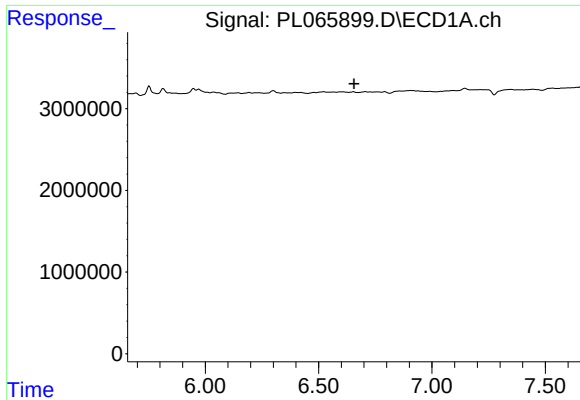

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 6.656 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

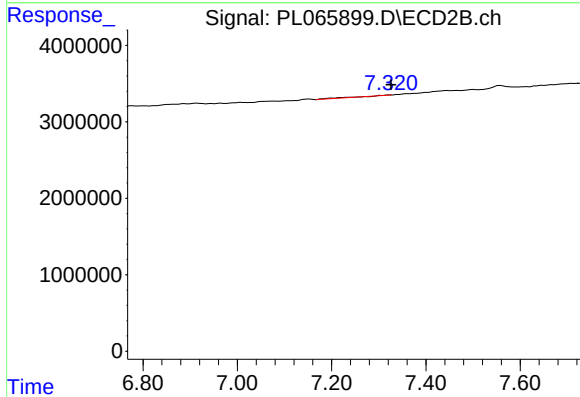


#20 Methoxychlor

R.T.: 7.322 min
Delta R.T.: -0.005 min
Response: 290044
Conc: 0.23 ng/ml

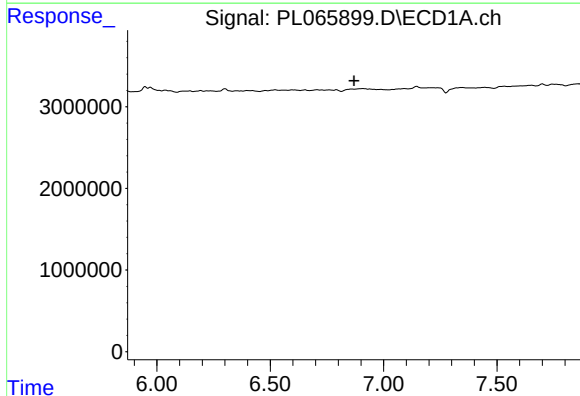


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 6.870 min
Response: 0
Conc: N.D.

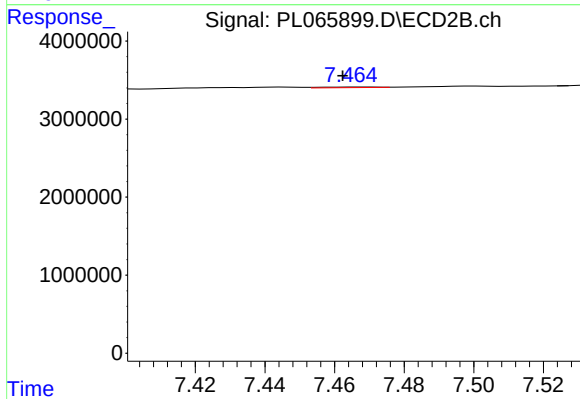

#21 Endrin ketone


R.T.: 7.468 min
Delta R.T.: 0.005 min
Response: 90242
Conc: 0.04 ng/ml

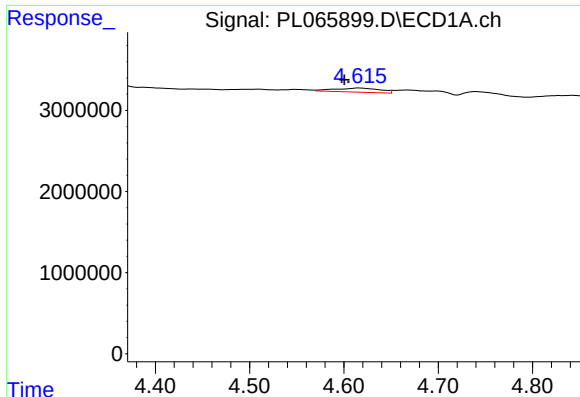

#24 Chlordane-2


R.T.: 4.616 min
Delta R.T.: 0.016 min
Response: 1724501
Conc: 15.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

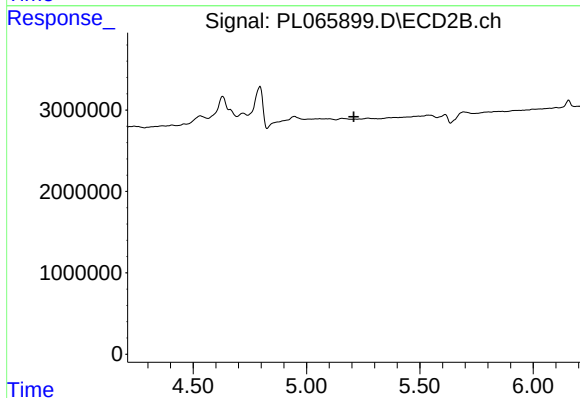


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.208 min
Response: 0
Conc: N.D.

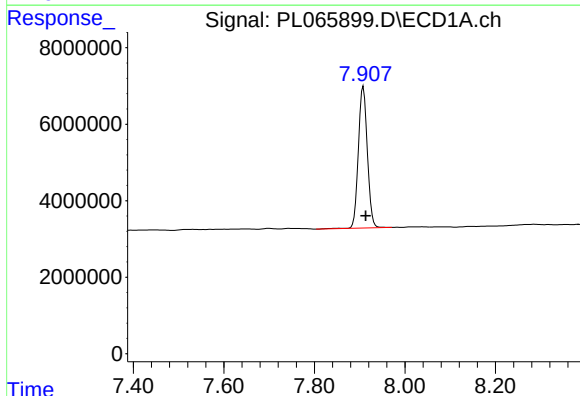

#28 Decachlorobiphenyl

R.T.: 7.908 min
Delta R.T.: -0.006 min
Response: 51194243
Conc: 22.10 ng/ml

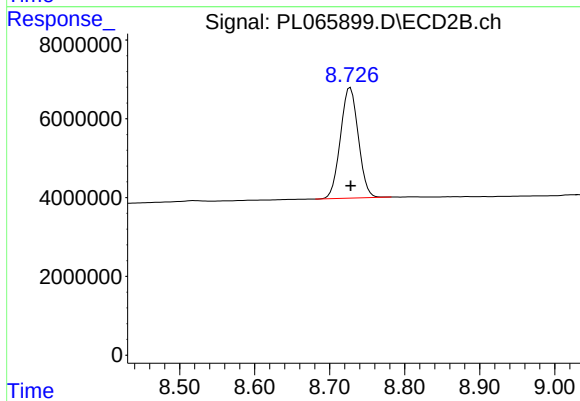

#28 Decachlorobiphenyl

R.T.: 8.727 min
Delta R.T.: 0.000 min
Response: 46494924
Conc: 20.62 ng/ml