

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040621\
 Data File : PL065902.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Apr 2021 12:50
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 07 04:31:01 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 31 15:57:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.275	3.779	47762960	50071986	18.335	18.241
28)	SA Decachlor...	7.906	8.726	49269454	44945327	21.273	19.936
Target Compounds							
4)	MA Heptachlor	0.000	4.944	0	908079	N.D.	0.257 #
6)	B beta-BHC	4.229	4.628	144369	5468376	0.091	3.139 #
8)	B Heptachlo...	0.000	5.609	0	4234642	N.D.	1.364 #
14)	MA Endrin	5.751	0.000	657010	0	0.243	N.D. #
15)	B Endosulfa...	0.000	6.671f	0	233799	N.D.	0.099 #
18)	B Endrin al...	0.000	6.780	0	191491	N.D.	0.101 #
20)	A Methoxychlor	0.000	7.328	0	19637	N.D.	0.016 #
21)	B Endrin ke...	6.863	7.434f	385009	642519	0.140	0.250 #
23)	Chlordane-1	4.142f	0.000	3245953	0	35.975	N.D. #
24)	Chlordane-2	4.617f	0.000	2692975	0	23.431	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040621\
Data File : PL065902.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Apr 2021 12:50
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 07 04:31:01 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
Quant Title : GC Extractables
QLast Update : Wed Mar 31 15:57:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

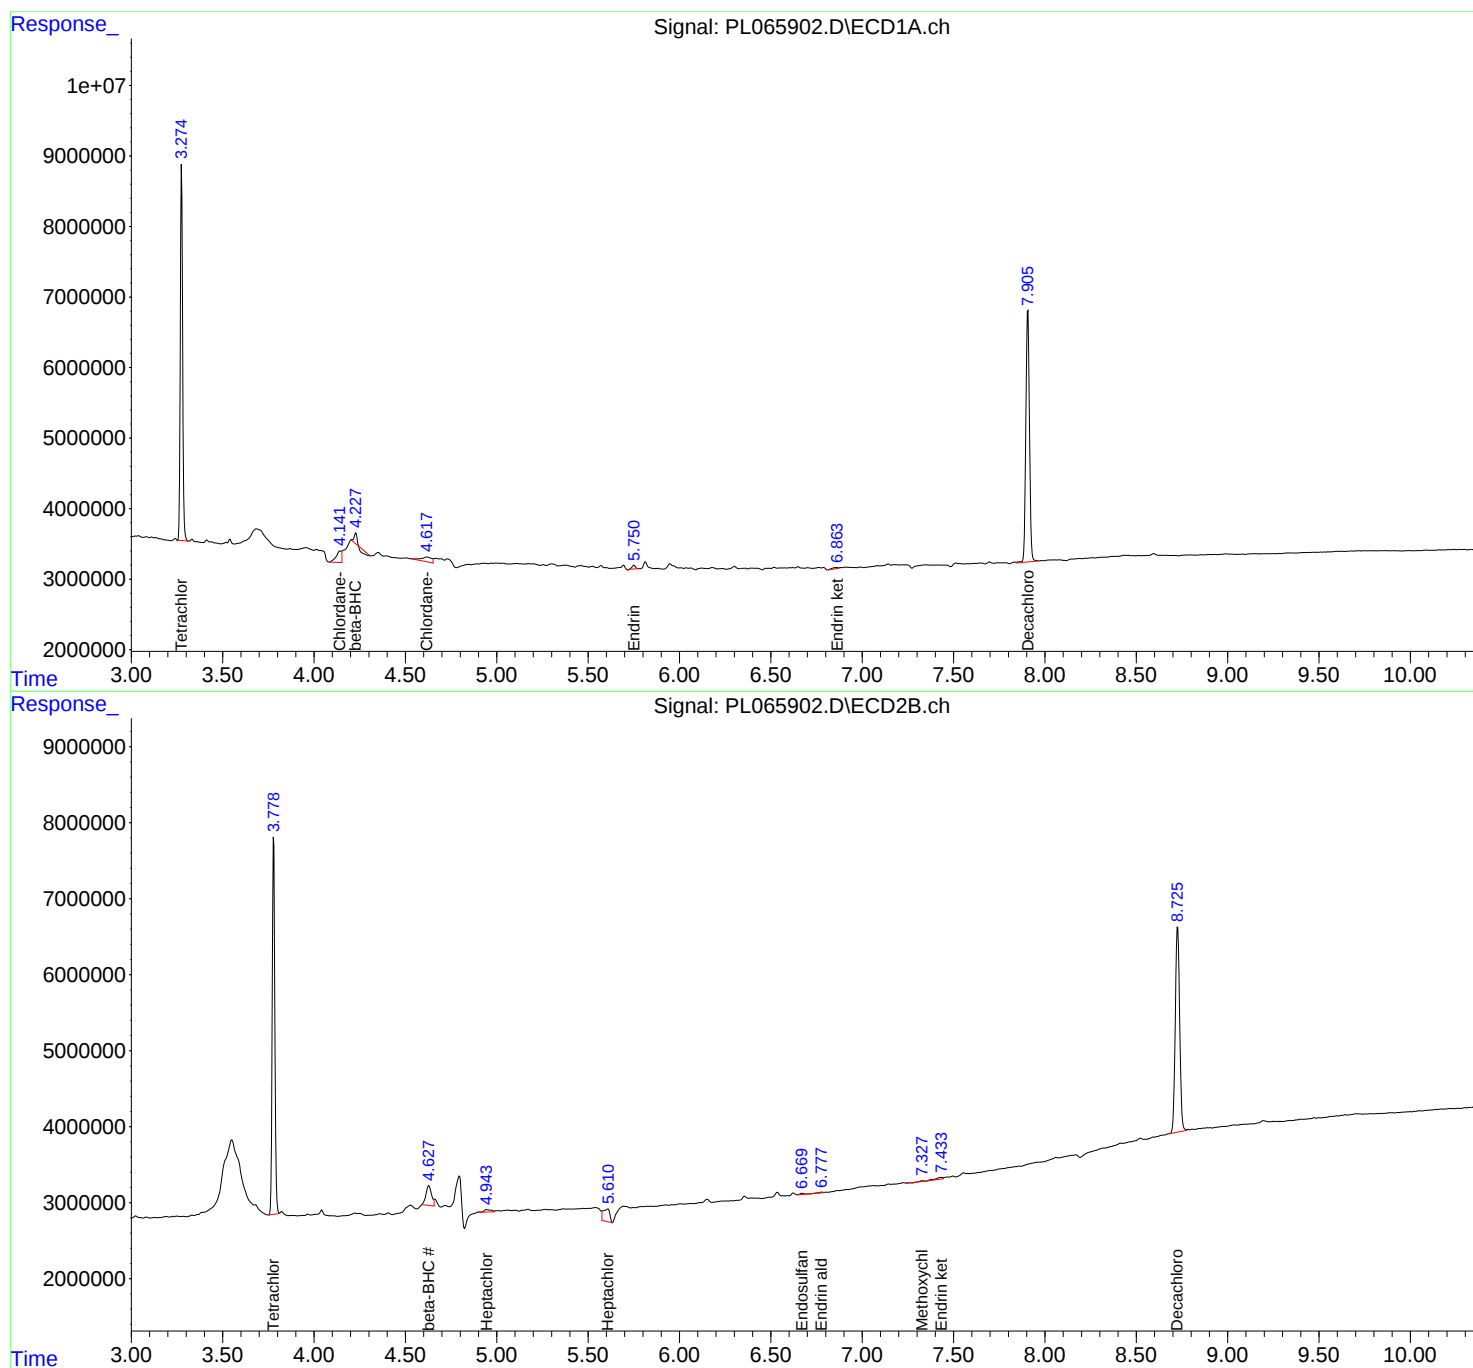


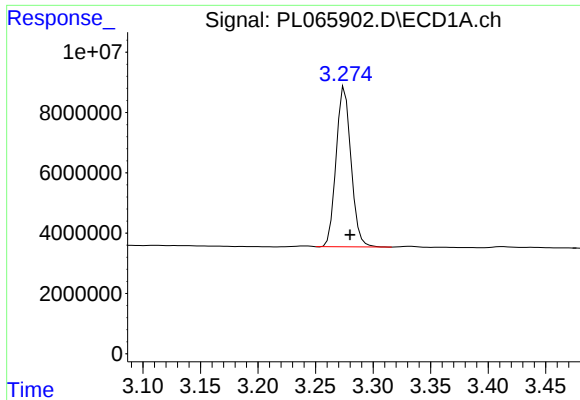

#1 Tetrachloro-m-xylene


R.T.: 3.275 min
Delta R.T.: -0.005 min
Response: 47762960
Conc: 18.34 ng/ml

Instrument :
ECD_L
ClientSampleId :

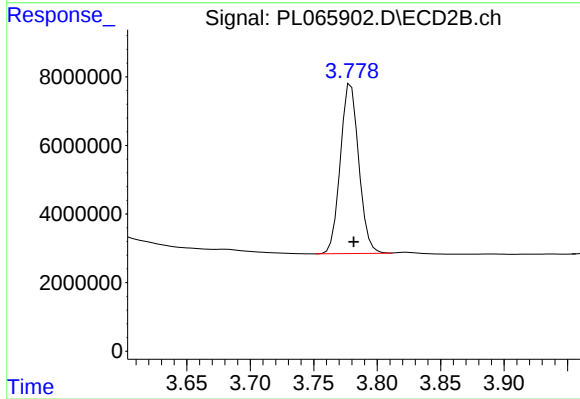


#1 Tetrachloro-m-xylene

R.T.: 3.779 min
Delta R.T.: -0.002 min
Response: 50071986
Conc: 18.24 ng/ml

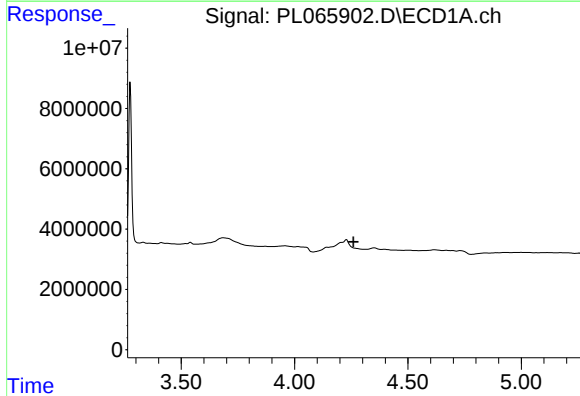


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.260 min
Response: 0
Conc: N.D.

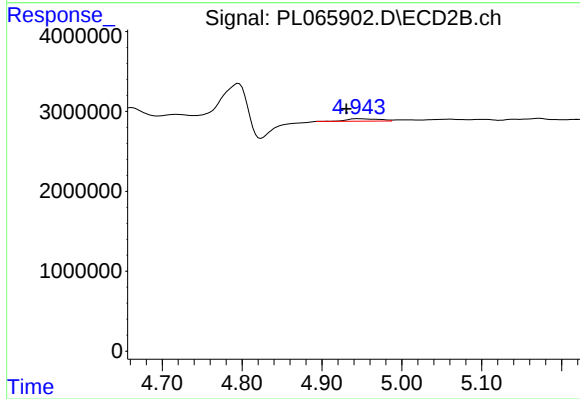

#4 Heptachlor


R.T.: 4.944 min
Delta R.T.: 0.013 min
Response: 908079
Conc: 0.26 ng/ml

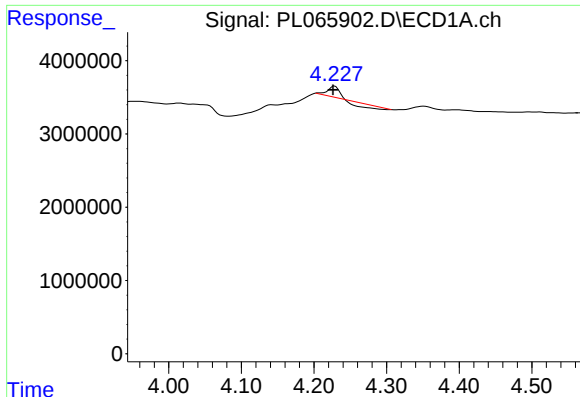

#6 beta-BHC


R.T.: 4.229 min
Delta R.T.: 0.002 min
Response: 144369
Conc: 0.09 ng/ml

Instrument :
ECD_L
ClientSampleId :

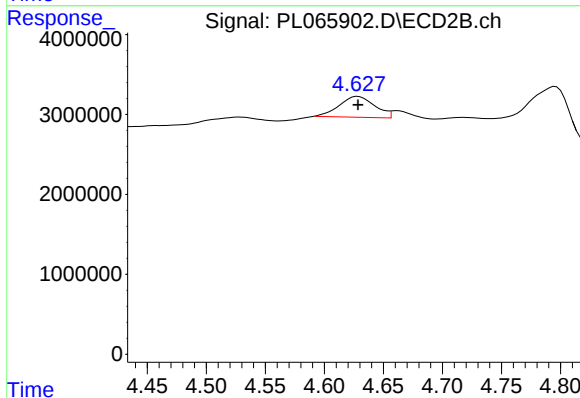


#6 beta-BHC

R.T.: 4.628 min
Delta R.T.: 0.000 min
Response: 5468376
Conc: 3.14 ng/ml

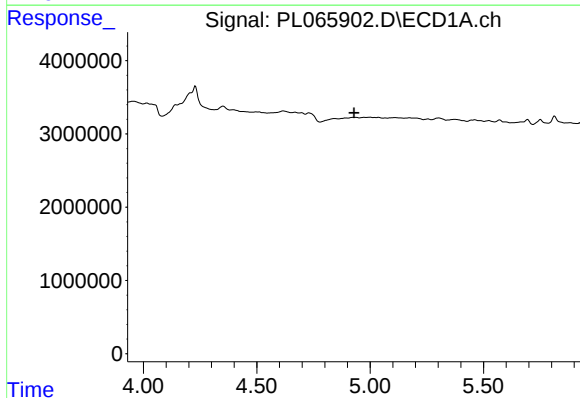


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.929 min
Response: 0
Conc: N.D.

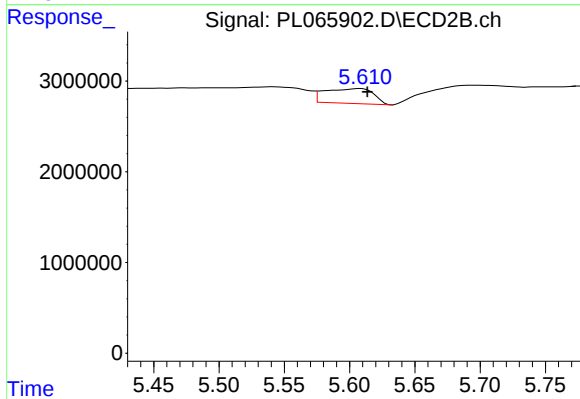

#8 Heptachlor epoxide


R.T.: 5.609 min
Delta R.T.: -0.005 min
Response: 4234642
Conc: 1.36 ng/ml

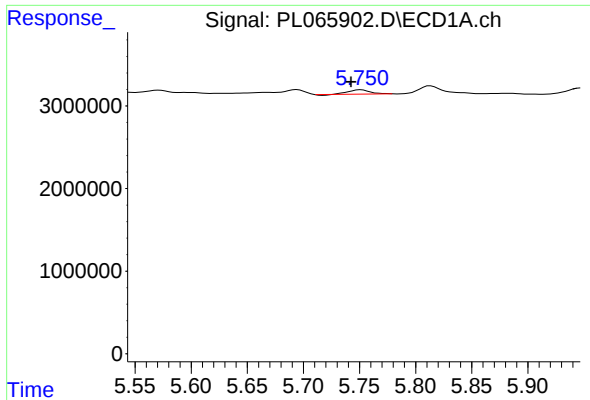

#14 Endrin


R.T.: 5.751 min
Delta R.T.: 0.009 min
Response: 657010
Conc: 0.24 ng/ml

Instrument :
ECD_L
ClientSampleId :

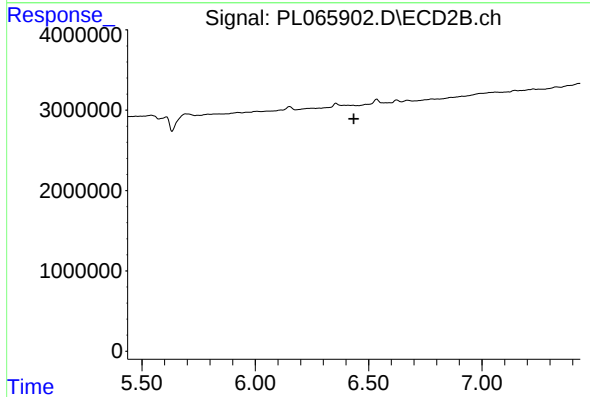


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.434 min
Response: 0
Conc: N.D.

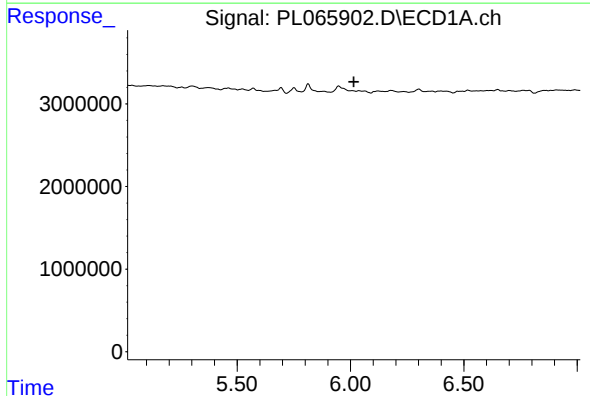


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.015 min
Response: 0
Conc: N.D.

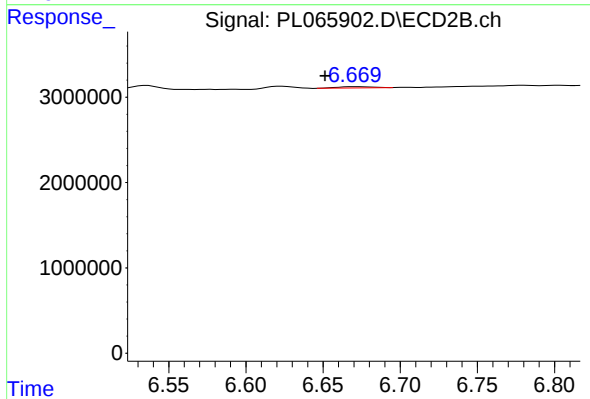

#15 Endosulfan II


R.T.: 6.671 min
Delta R.T.: 0.019 min
Response: 233799
Conc: 0.10 ng/ml

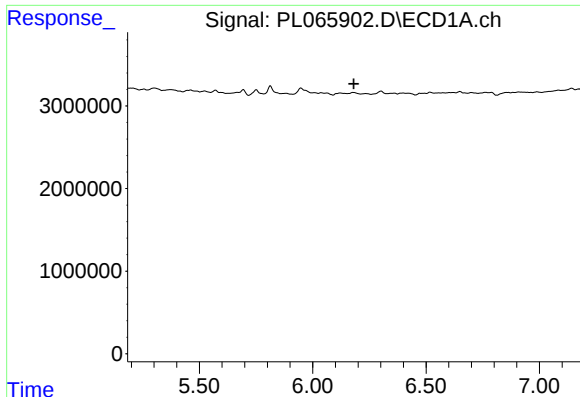

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 6.181 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

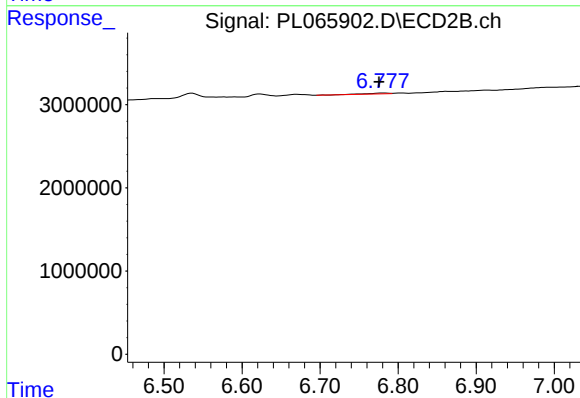


#18 Endrin aldehyde

R.T.: 6.780 min
Delta R.T.: 0.004 min
Response: 191491
Conc: 0.10 ng/ml

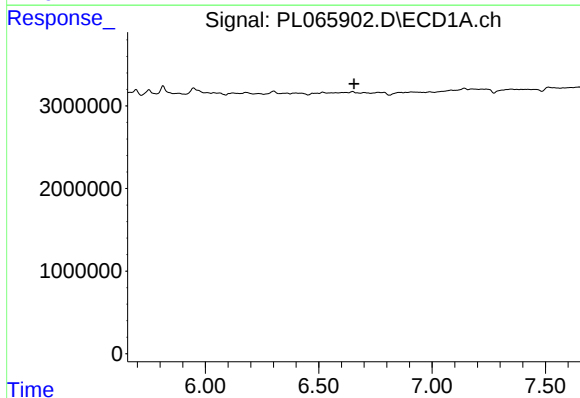


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.656 min
Response: 0
Conc: N.D.

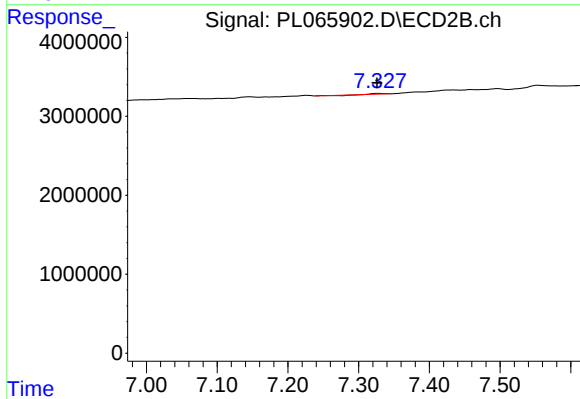

#20 Methoxychlor


R.T.: 7.328 min
Delta R.T.: 0.001 min
Response: 19637
Conc: 0.02 ng/ml

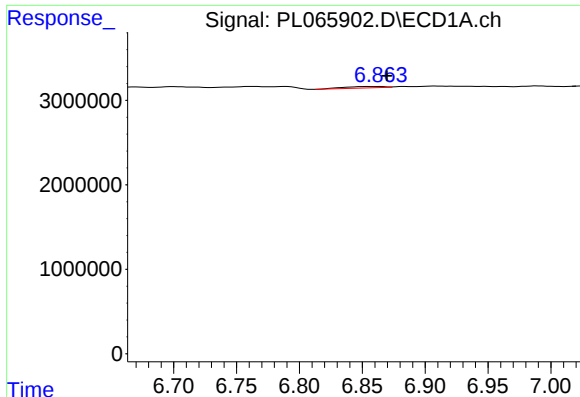

#21 Endrin ketone


R.T.: 6.863 min
Delta R.T.: -0.006 min
Response: 385009
Conc: 0.14 ng/ml

Instrument :
ECD_L
ClientSampleId :

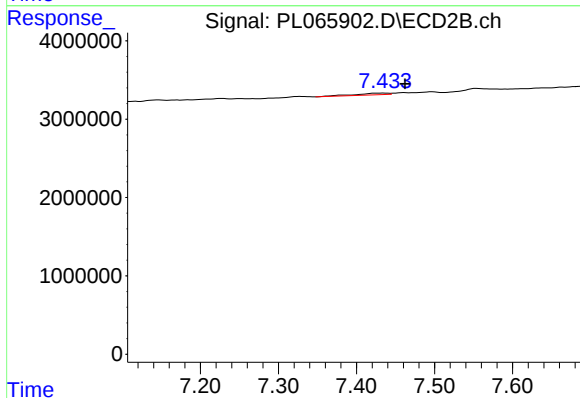


#21 Endrin ketone

R.T.: 7.434 min
Delta R.T.: -0.028 min
Response: 642519
Conc: 0.25 ng/ml

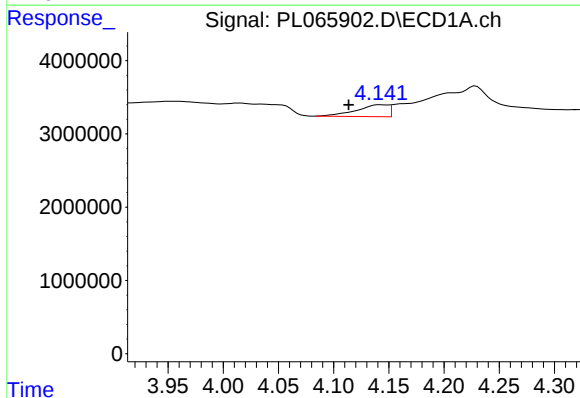


#23 Chlordane-1

R.T.: 4.142 min
Delta R.T.: 0.028 min
Response: 3245953
Conc: 35.98 ng/ml

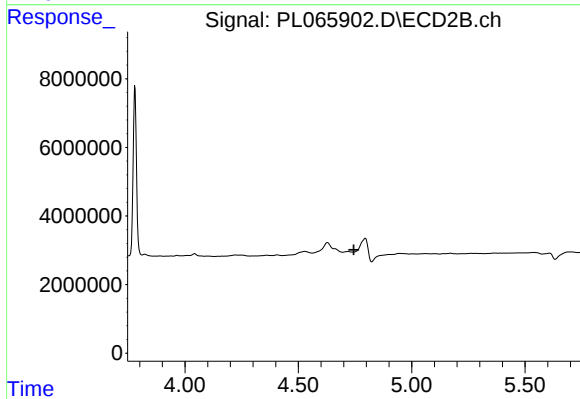

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.745 min
Response: 0
Conc: N.D.

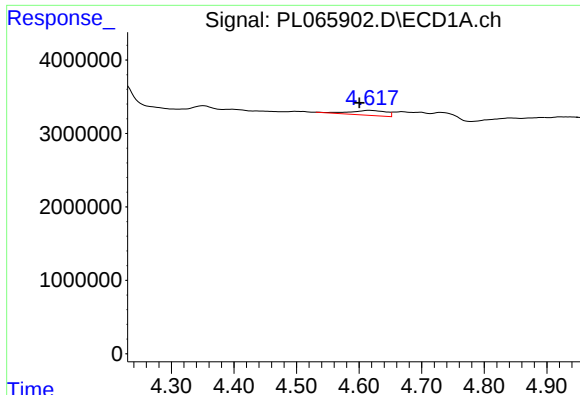

#24 Chlordane-2


R.T.: 4.617 min
Delta R.T.: 0.016 min
Response: 2692975
Conc: 23.43 ng/ml

Instrument :
ECD_L
ClientSampleId :

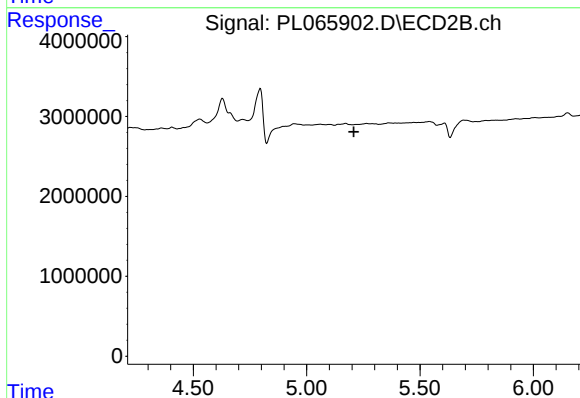


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.208 min
Response: 0
Conc: N.D.

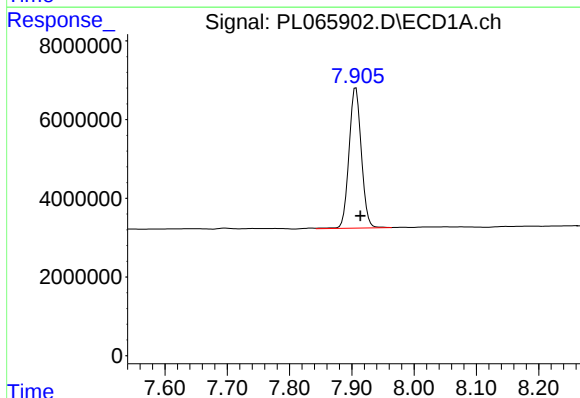

#28 Decachlorobiphenyl

R.T.: 7.906 min
Delta R.T.: -0.007 min
Response: 49269454
Conc: 21.27 ng/ml

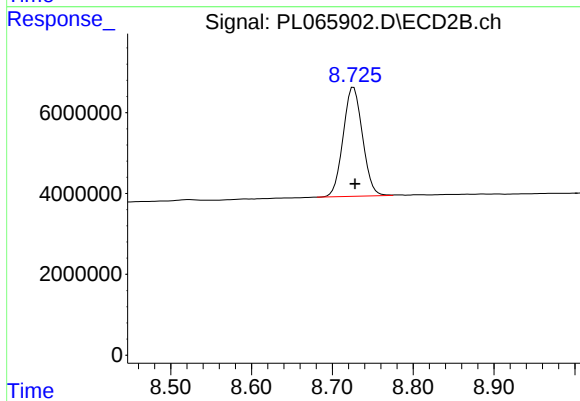

#28 Decachlorobiphenyl

R.T.: 8.726 min
Delta R.T.: -0.002 min
Response: 44945327
Conc: 19.94 ng/ml