

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040621\
 Data File : PL065904.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Apr 2021 13:18
 Operator : AR\AJ
 Sample : PB135554BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 07 04:31:32 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 31 15:57:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.276	3.780	47130331	50152172	18.092	18.271
28)	SA Decachlor...	7.907	8.728	50406646	46168293	21.764	20.478
Target Compounds							
4)	MA Heptachlor	0.000	4.943	0	405301	N.D.	0.115 #
6)	B beta-BHC	4.229	4.628	-61185	8337718	N.D.	4.787
7)	B delta-BHC	0.000	4.862f	0	491919	N.D.	0.165 #
8)	B Heptachlo...	0.000	5.609	0	2461349	N.D.	0.793 #
9)	A Endosulfan I	0.000	5.966	0	345552	N.D.	0.126 #
18)	B Endrin al...	0.000	6.789	0	88409	N.D.	0.047 #
20)	A Methoxychlor	0.000	7.301f	0	272300	N.D.	0.215 #
21)	B Endrin ke...	6.862	0.000	305456	0	0.111	N.D. #
23)	Chlordane-1	4.140f	0.000	1813904	0	20.104	N.D. #
24)	Chlordane-2	4.572f	0.000	398597	0	3.468	N.D. #
27)	Chlordane-5	0.000	6.713	0	17116	N.D.	0.205 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040621\
Data File : PL065904.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Apr 2021 13:18
Operator : AR\AJ
Sample : PB135554BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 07 04:31:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
Quant Title : GC Extractables
QLast Update : Wed Mar 31 15:57:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

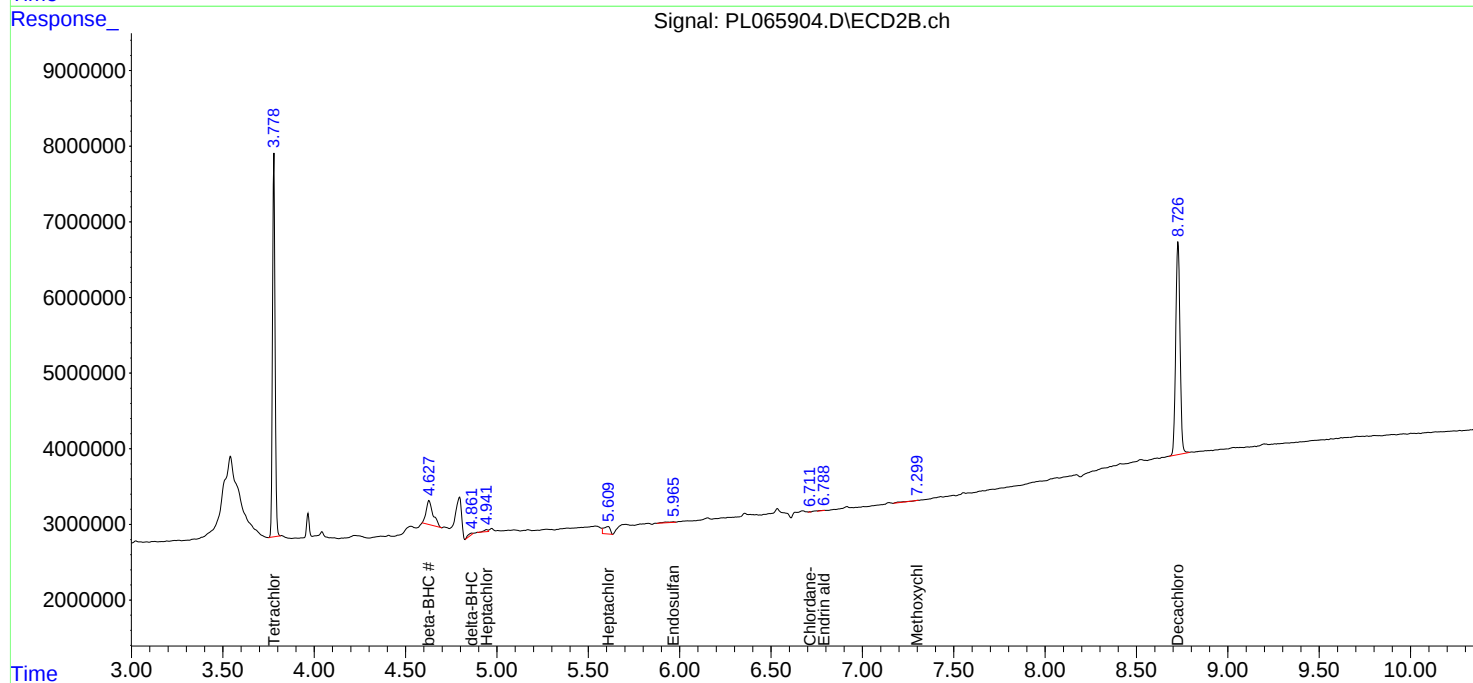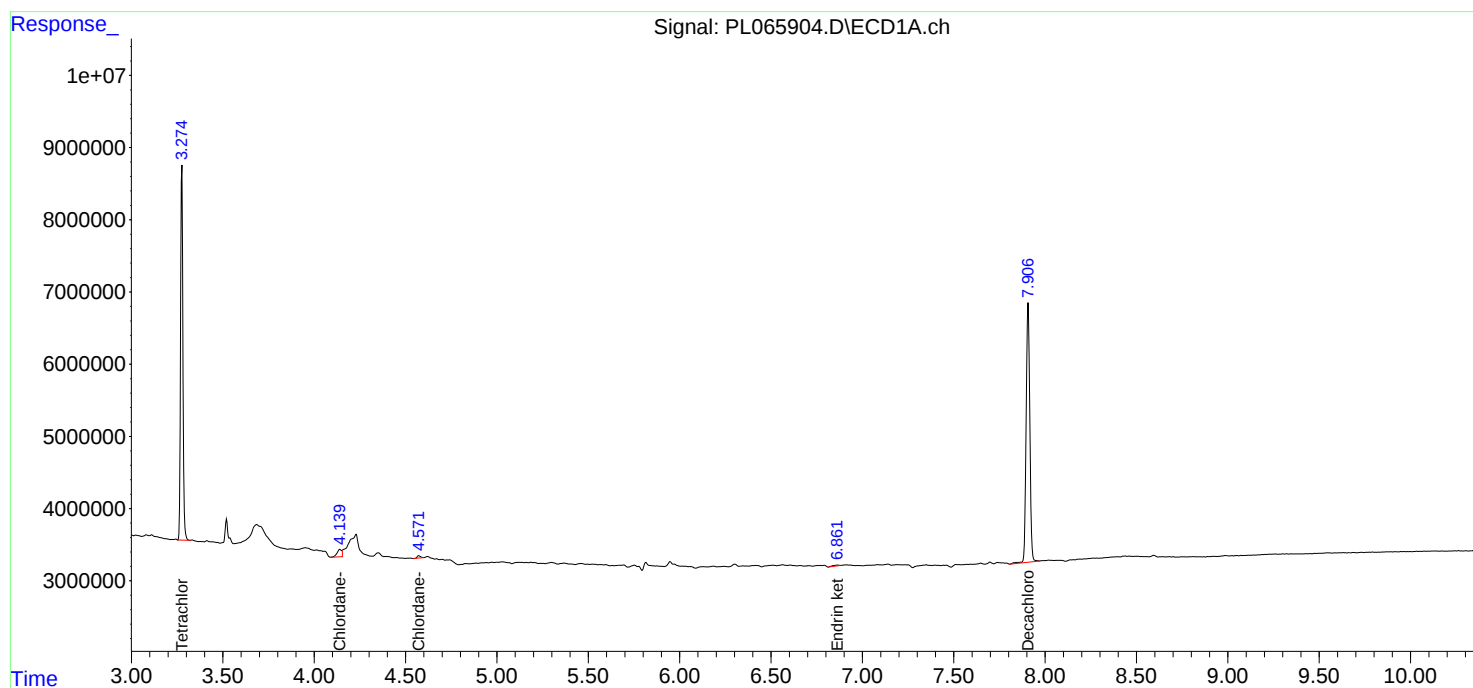


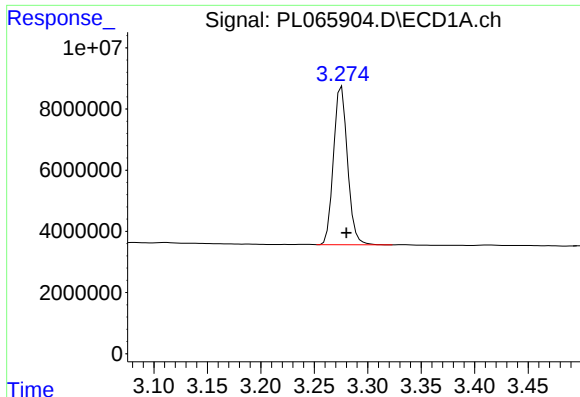

#1 Tetrachloro-m-xylene


R.T.: 3.276 min
Delta R.T.: -0.004 min
Response: 47130331
Conc: 18.09 ng/ml

Instrument :
ECD_L
ClientSampleId :

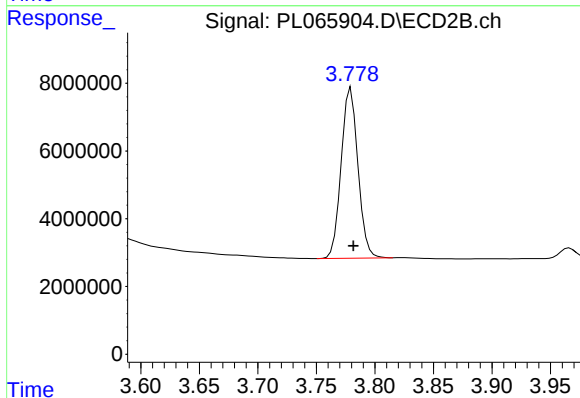


#1 Tetrachloro-m-xylene

R.T.: 3.780 min
Delta R.T.: -0.002 min
Response: 50152172
Conc: 18.27 ng/ml

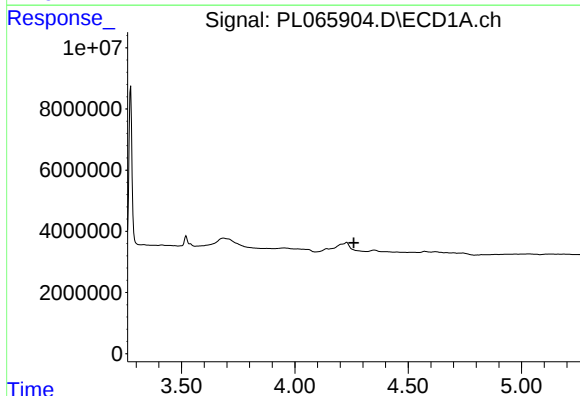


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.260 min
Response: 0
Conc: N.D.

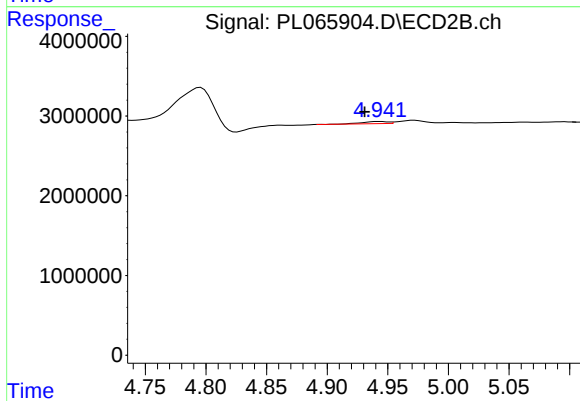

#4 Heptachlor


R.T.: 4.943 min
Delta R.T.: 0.012 min
Response: 405301
Conc: 0.11 ng/ml

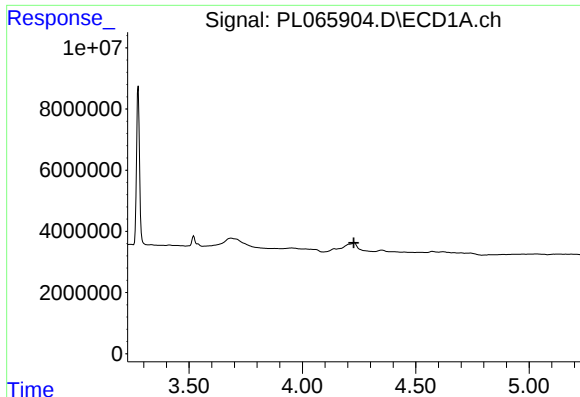

#6 beta-BHC


R.T.: 4.229 min
Delta R.T.: 0.003 min
Response: -61185
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

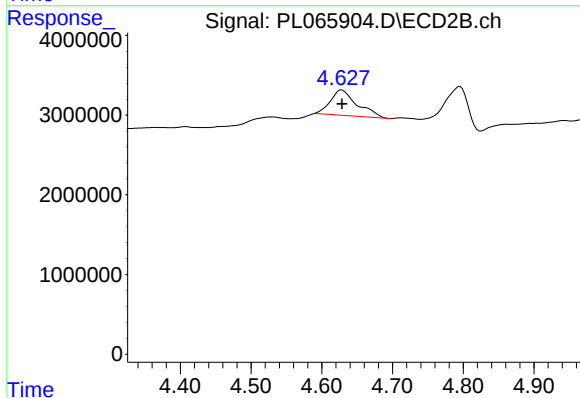


#6 beta-BHC

R.T.: 4.628 min
Delta R.T.: 0.000 min
Response: 8337718
Conc: 4.79 ng/ml

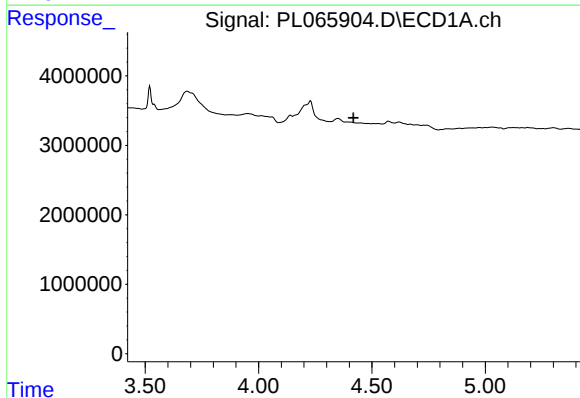


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.419 min
Response: 0
Conc: N.D.

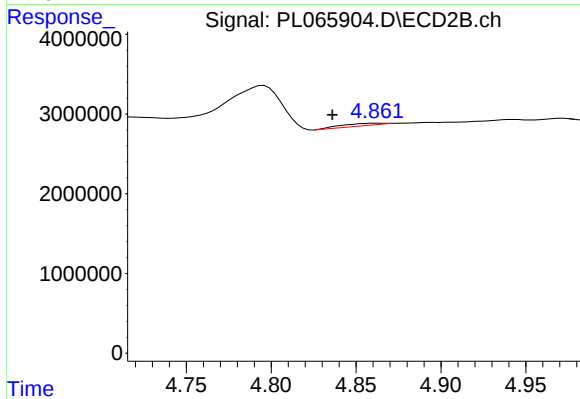

#7 delta-BHC


R.T.: 4.862 min
Delta R.T.: 0.026 min
Response: 491919
Conc: 0.16 ng/ml

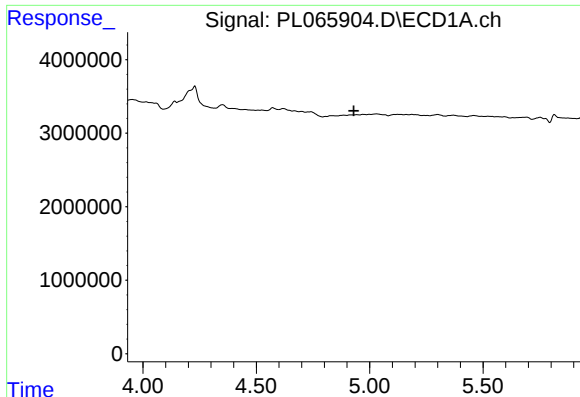

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.929 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

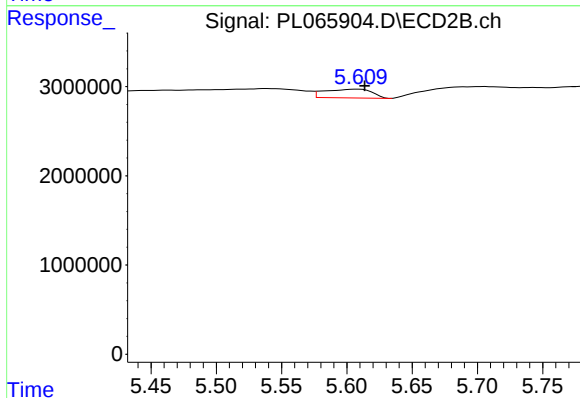


#8 Heptachlor epoxide

R.T.: 5.609 min
Delta R.T.: -0.004 min
Response: 2461349
Conc: 0.79 ng/ml

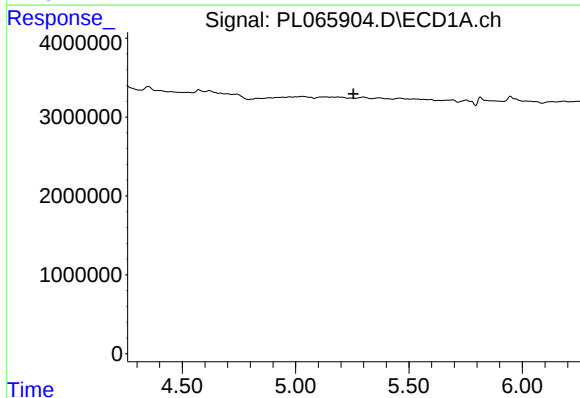


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.255 min
Response: 0
Conc: N.D.

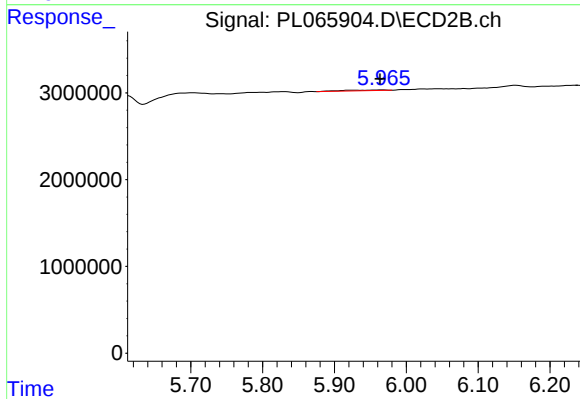

#9 Endosulfan I


R.T.: 5.966 min
Delta R.T.: 0.003 min
Response: 345552
Conc: 0.13 ng/ml

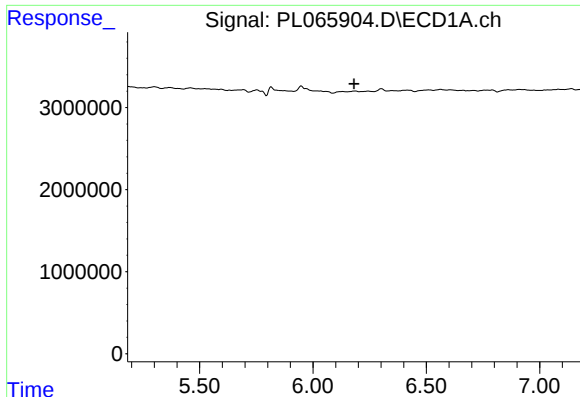

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 6.181 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

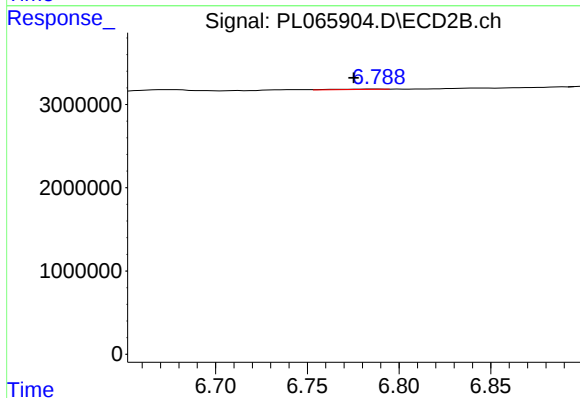


#18 Endrin aldehyde

R.T.: 6.789 min
Delta R.T.: 0.013 min
Response: 88409
Conc: 0.05 ng/ml

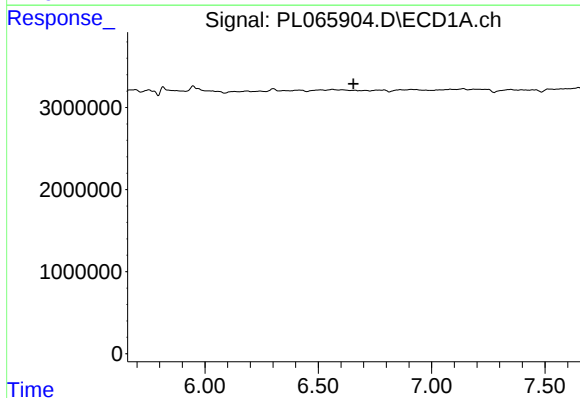


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.656 min
Response: 0
Conc: N.D.

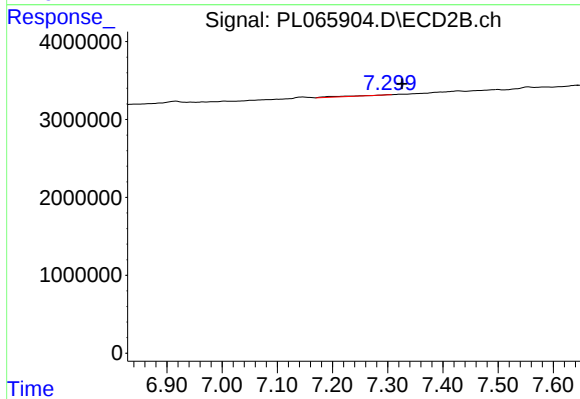

#20 Methoxychlor


R.T.: 7.301 min
Delta R.T.: -0.025 min
Response: 272300
Conc: 0.21 ng/ml

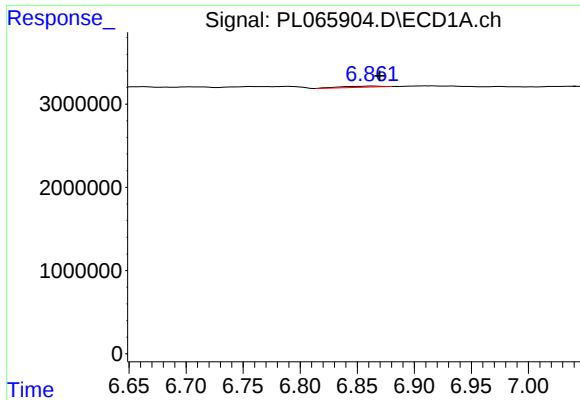

#21 Endrin ketone


R.T.: 6.862 min
Delta R.T.: -0.008 min
Response: 305456
Conc: 0.11 ng/ml

Instrument :
ECD_L
ClientSampleId :

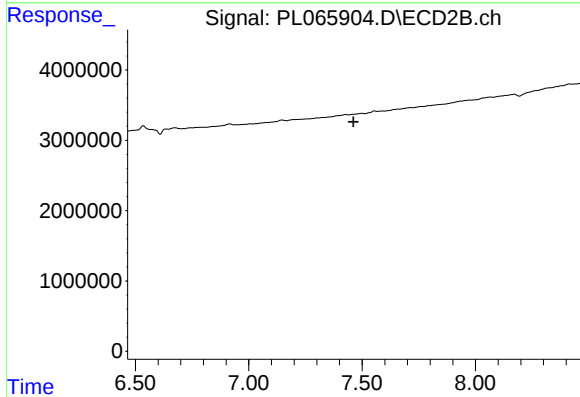


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.462 min
Response: 0
Conc: N.D.

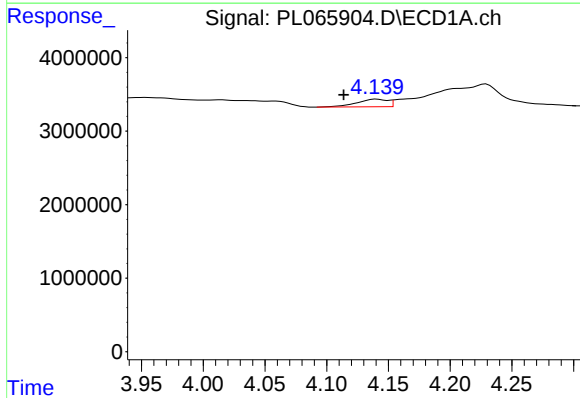


#23 Chlordane-1

R.T.: 4.140 min
Delta R.T.: 0.027 min
Response: 1813904
Conc: 20.10 ng/ml

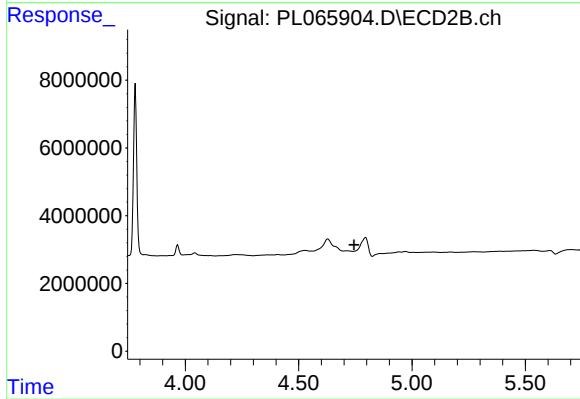

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.745 min
Response: 0
Conc: N.D.

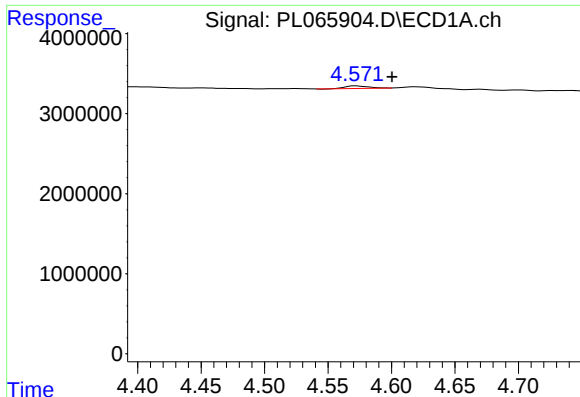

#24 Chlordane-2


R.T.: 4.572 min
Delta R.T.: -0.028 min
Response: 398597
Conc: 3.47 ng/ml

Instrument :
ECD_L
ClientSampleId :

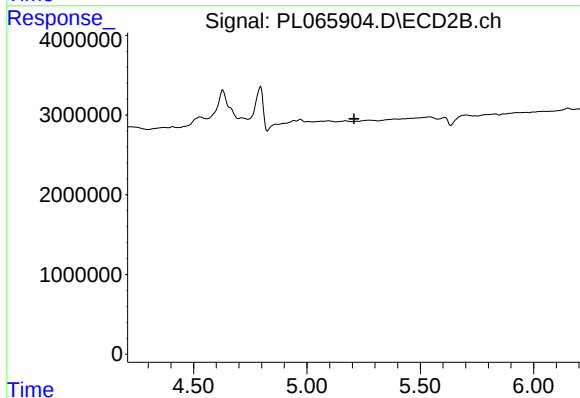


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.208 min
Response: 0
Conc: N.D.

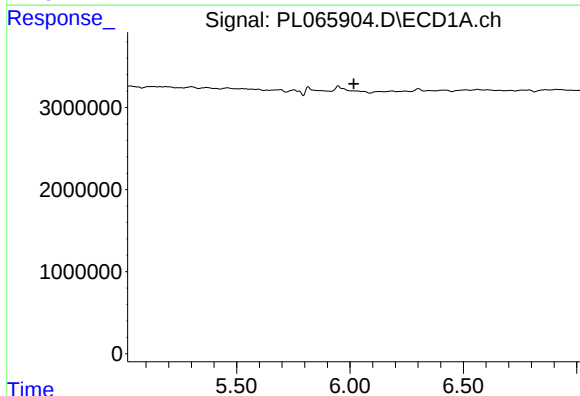


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.017 min
Response: 0
Conc: N.D.

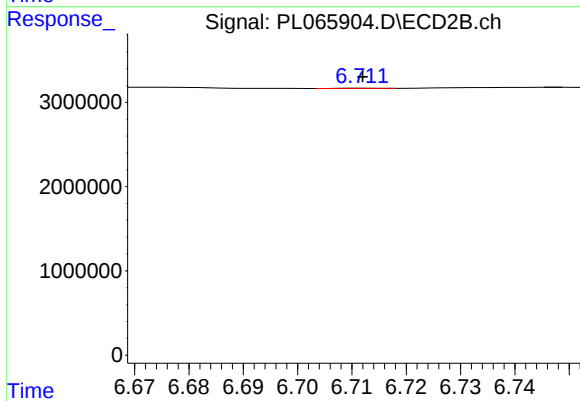

#27 Chlordane-5


R.T.: 6.713 min
Delta R.T.: 0.000 min
Response: 17116
Conc: 0.21 ng/ml

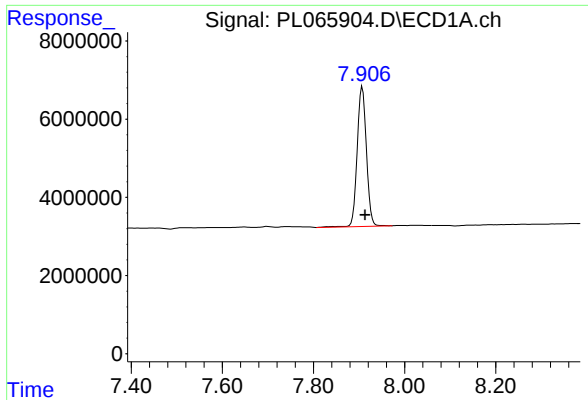

#28 Decachlorobiphenyl

R.T.: 7.907 min
Delta R.T.: -0.007 min
Response: 50406646
Conc: 21.76 ng/ml

Instrument :
ECD_L
ClientSampleId :

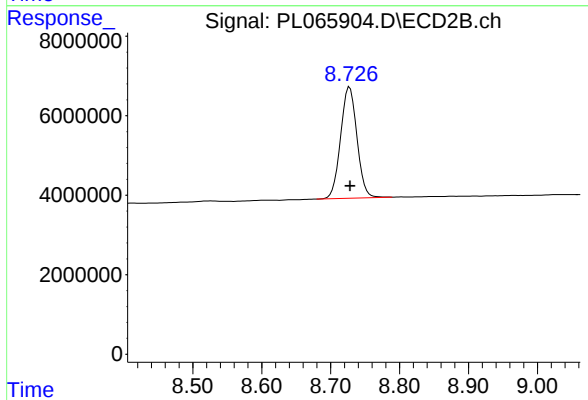

#28 Decachlorobiphenyl

R.T.: 8.728 min
Delta R.T.: 0.000 min
Response: 46168293
Conc: 20.48 ng/ml