

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040621\
 Data File : PL065926.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Apr 2021 19:08
 Operator : AR\AJ
 Sample : PB135567BSD
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 07 04:37:21 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 31 15:57:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.276	3.780	49364506	52225240	18.950	19.026
28)	SA Decachlor...	7.907	8.727	52892575	48493955	22.838	21.510
Target Compounds							
4)	MA Heptachlor	0.000	4.945	0	623517	N.D.	0.177 #
6)	B beta-BHC	4.228	4.630	-148198	7868751	N.D.	4.518
8)	B Heptachlo...	0.000	5.612	0	1056217	N.D.	0.340 #
14)	MA Endrin	5.750	0.000	257754	0	0.095	N.D. #
15)	B Endosulfa...	0.000	6.675f	0	355908	N.D.	0.151 #
18)	B Endrin al...	0.000	6.794f	0	285607	N.D.	0.151 #
20)	A Methoxychlor	0.000	7.345f	0	583782	N.D.	0.461 #
21)	B Endrin ke...	0.000	7.437f	0	903941	N.D.	0.352 #
23)	Chlordane-1	4.141f	0.000	1164035	0	12.901	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040621\
Data File : PL065926.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Apr 2021 19:08
Operator : AR\AJ
Sample : PB135567BSD
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 07 04:37:21 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
Quant Title : GC Extractables
QLast Update : Wed Mar 31 15:57:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

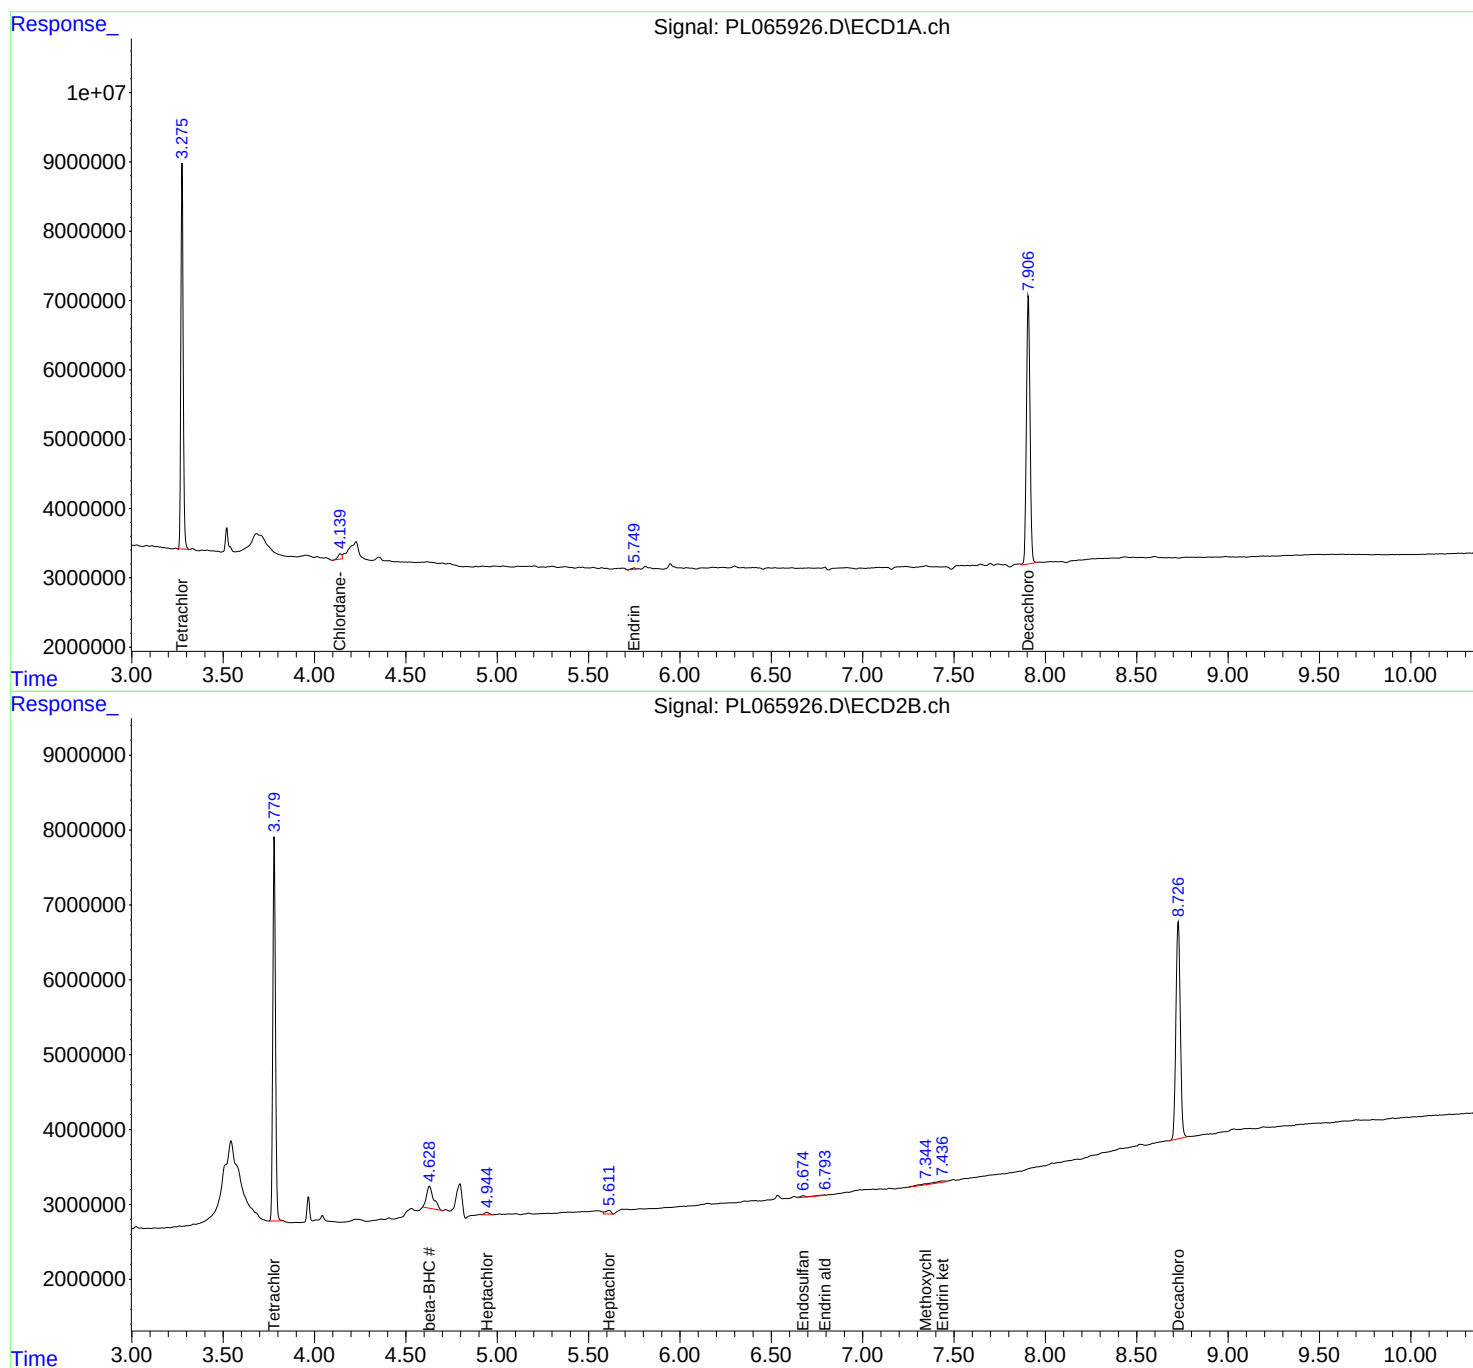


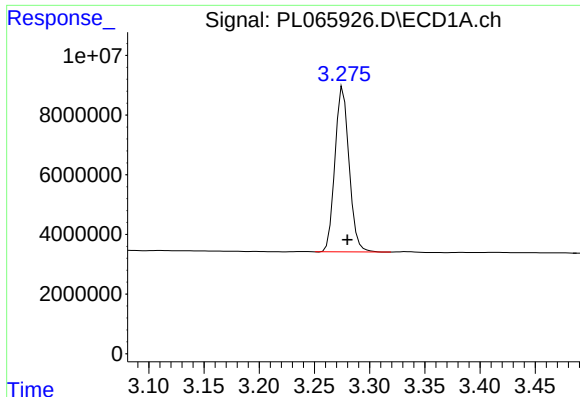

#1 Tetrachloro-m-xylene


R.T.: 3.276 min
Delta R.T.: -0.004 min
Response: 49364506
Conc: 18.95 ng/ml

Instrument :
ECD_L
ClientSampleId :

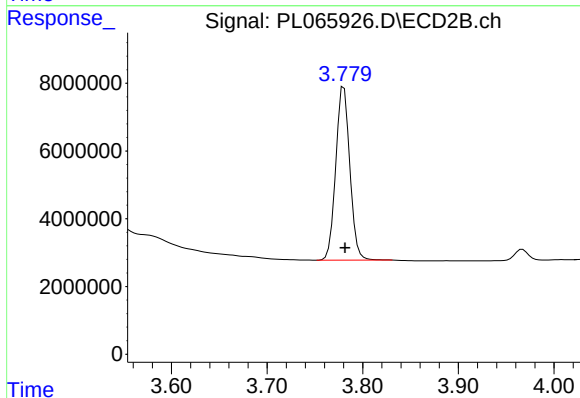


#1 Tetrachloro-m-xylene

R.T.: 3.780 min
Delta R.T.: -0.001 min
Response: 52225240
Conc: 19.03 ng/ml

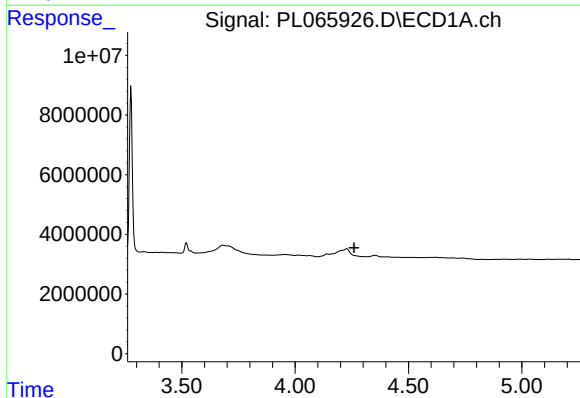


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.260 min
Response: 0
Conc: N.D.

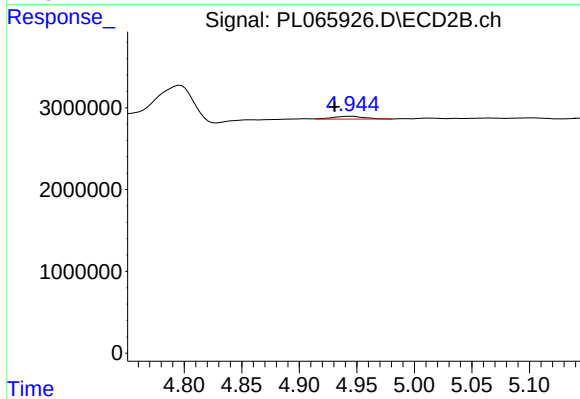

#4 Heptachlor


R.T.: 4.945 min
Delta R.T.: 0.014 min
Response: 623517
Conc: 0.18 ng/ml

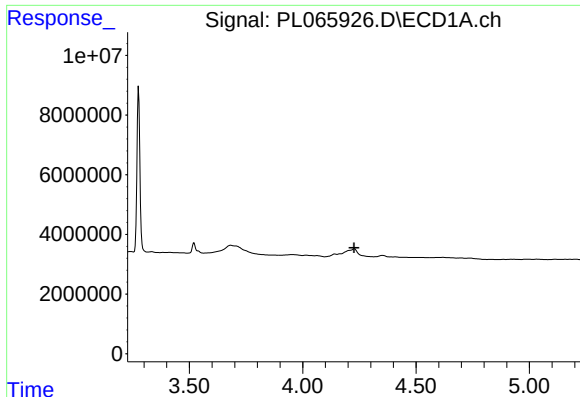

#6 beta-BHC


R.T.: 4.228 min
Delta R.T.: 0.002 min
Response: -148198
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

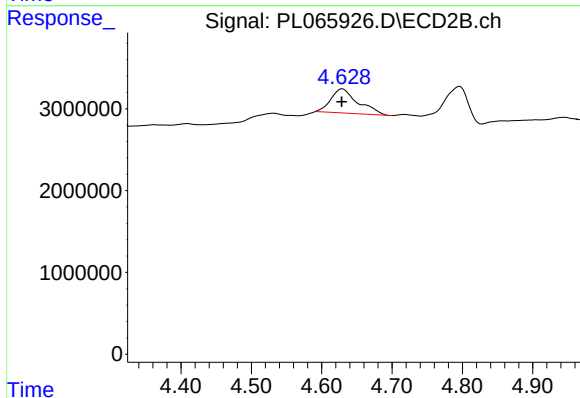


#6 beta-BHC

R.T.: 4.630 min
Delta R.T.: 0.001 min
Response: 7868751
Conc: 4.52 ng/ml

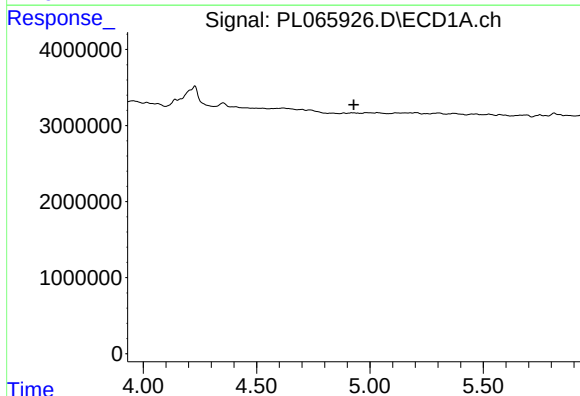


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.929 min
Response: 0
Conc: N.D.

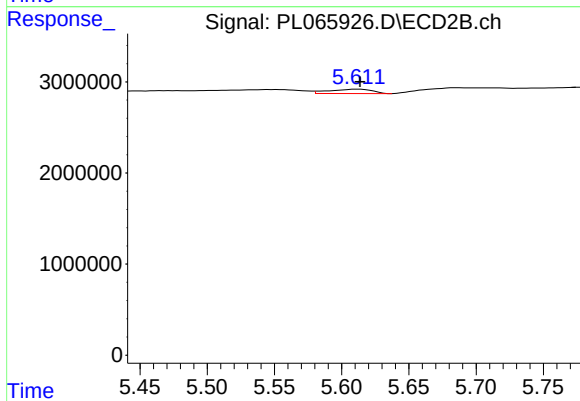

#8 Heptachlor epoxide


R.T.: 5.612 min
Delta R.T.: -0.002 min
Response: 1056217
Conc: 0.34 ng/ml

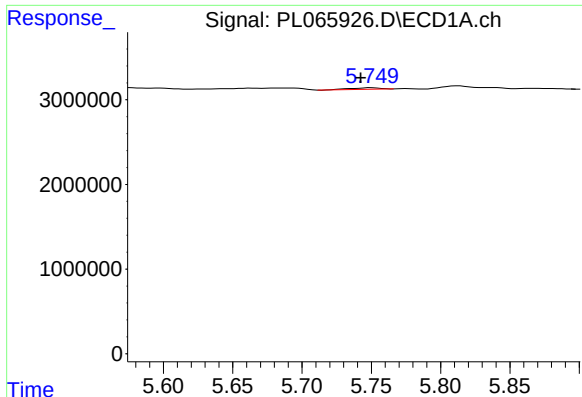

#14 Endrin


R.T.: 5.750 min
Delta R.T.: 0.008 min
Response: 257754
Conc: 0.10 ng/ml

Instrument :
ECD_L
ClientSampleId :

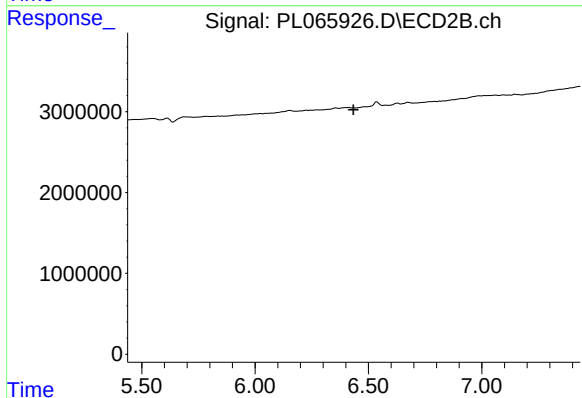


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.434 min
Response: 0
Conc: N.D.

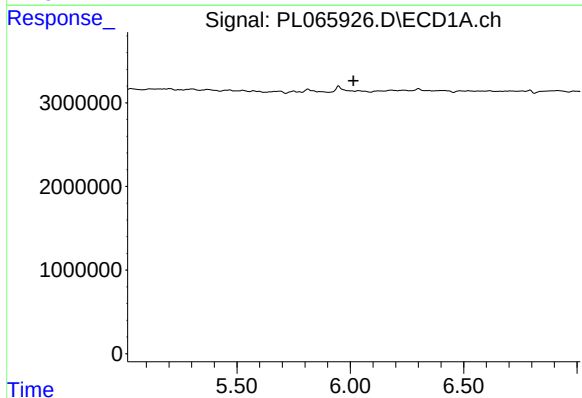


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.015 min
Response: 0
Conc: N.D.

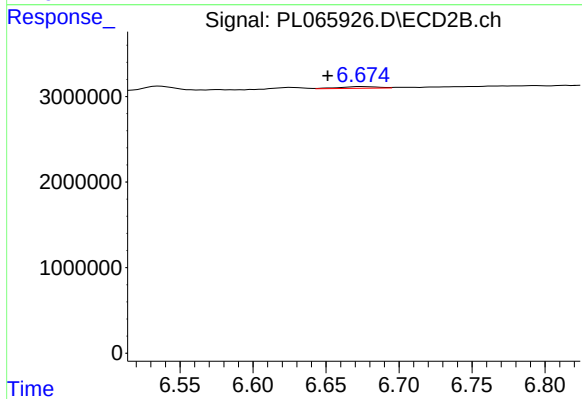

#15 Endosulfan II


R.T.: 6.675 min
Delta R.T.: 0.024 min
Response: 355908
Conc: 0.15 ng/ml

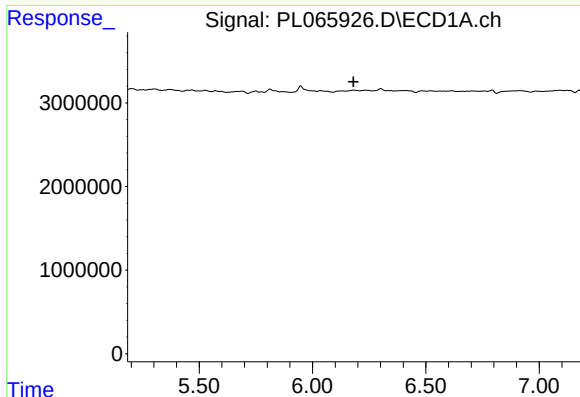

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 6.181 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

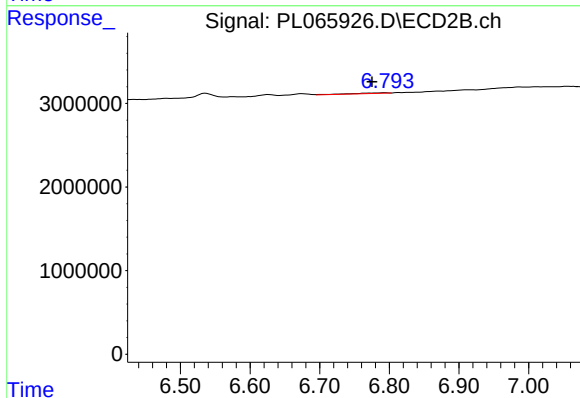


#18 Endrin aldehyde

R.T.: 6.794 min
Delta R.T.: 0.019 min
Response: 285607
Conc: 0.15 ng/ml

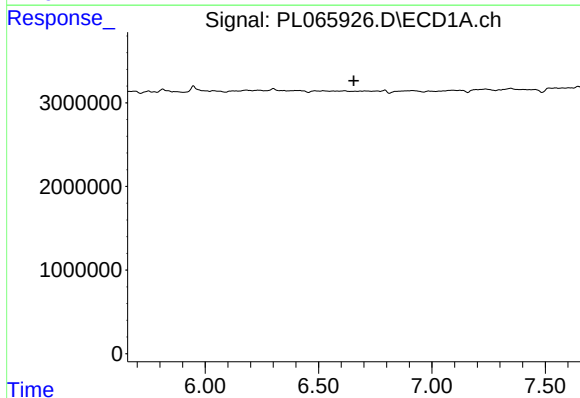


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.656 min
Response: 0
Conc: N.D.

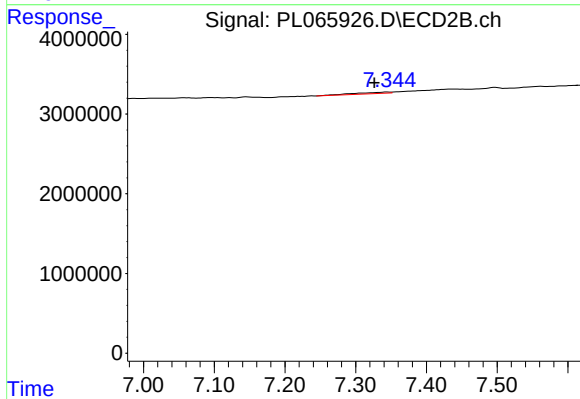

#20 Methoxychlor


R.T.: 7.345 min
Delta R.T.: 0.019 min
Response: 583782
Conc: 0.46 ng/ml

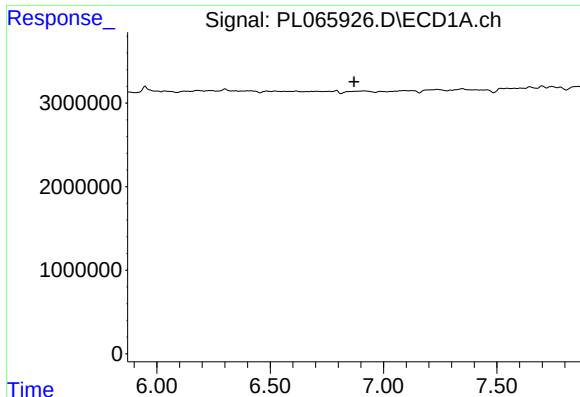

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 6.870 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

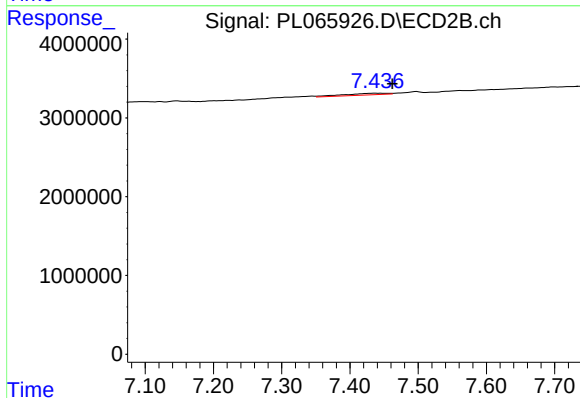


#21 Endrin ketone

R.T.: 7.437 min
Delta R.T.: -0.025 min
Response: 903941
Conc: 0.35 ng/ml

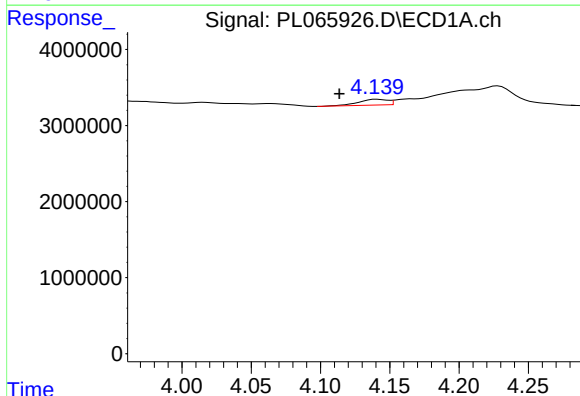


#23 Chlordane-1

R.T.: 4.141 min
Delta R.T.: 0.027 min
Response: 1164035
Conc: 12.90 ng/ml

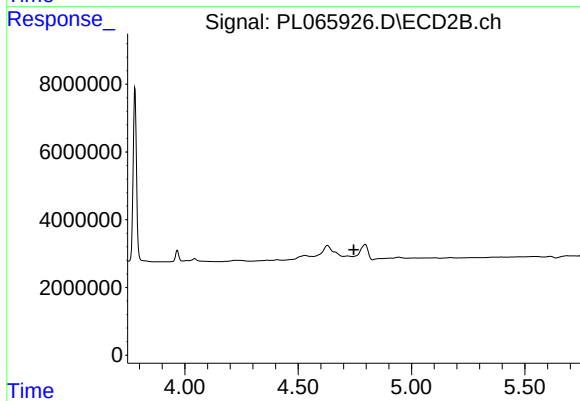

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.745 min
Response: 0
Conc: N.D.

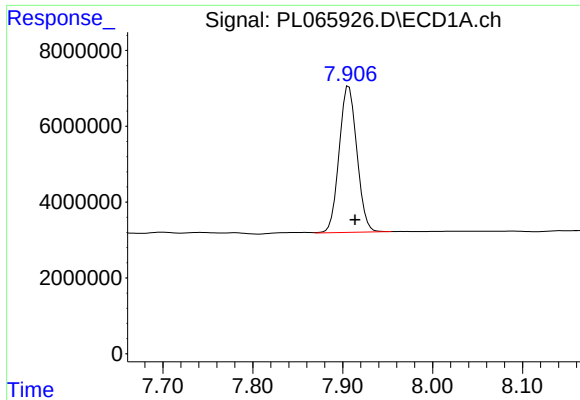

#28 Decachlorobiphenyl

R.T.: 7.907 min
Delta R.T.: -0.007 min
Response: 52892575
Conc: 22.84 ng/ml

Instrument :
ECD_L
ClientSampleId :

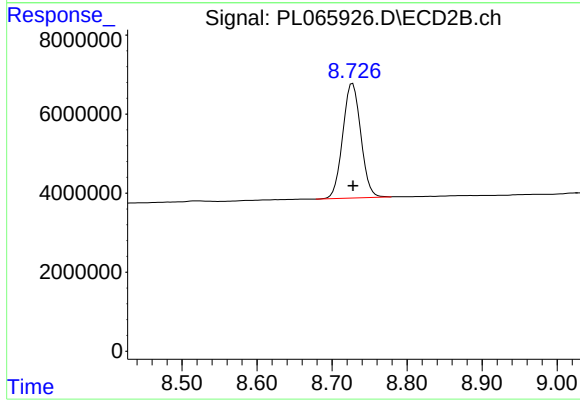

#28 Decachlorobiphenyl

R.T.: 8.727 min
Delta R.T.: 0.000 min
Response: 48493955
Conc: 21.51 ng/ml