

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040621\
 Data File : PL065894.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Apr 2021 10:27
 Operator : AR\AJ
 Sample : M1909-02DL 20X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 FS-SB-10-26-27DL

Manual Integrations
 APPROVED

Ankita
 4/7/2021 4:50:05 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 07 07:37:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 31 15:57:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
12) B	4,4'-DDE	5.385	6.071	338.6E6	127.4E6	122.730m 48.759m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040621\
Data File : PL065894.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Apr 2021 10:27
Operator : AR\AJ
Sample : M1909-02DL 20X
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
FS-SB-10-26-27DL


Manual Integrations
APPROVED

Ankita
4/7/2021 4:50:05 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 07 07:37:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
Quant Title : GC Extractables
QLast Update : Wed Mar 31 15:57:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

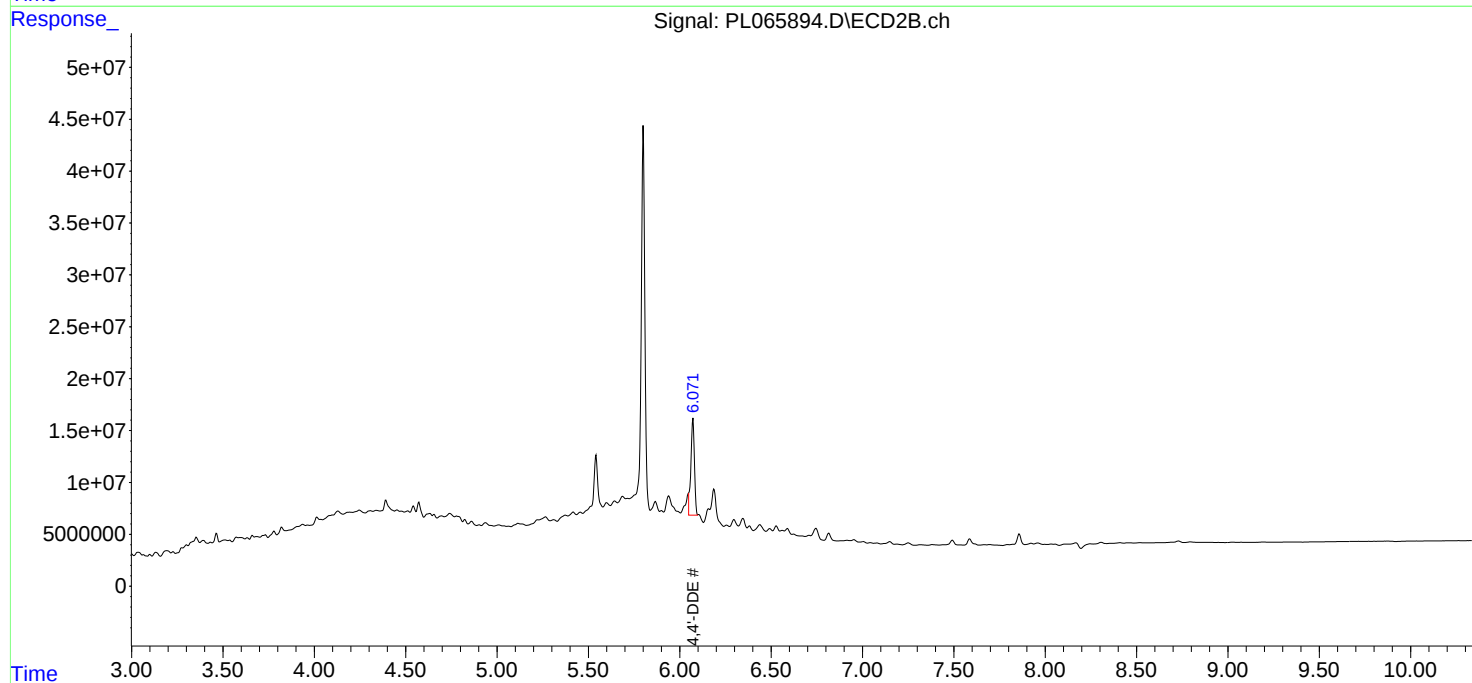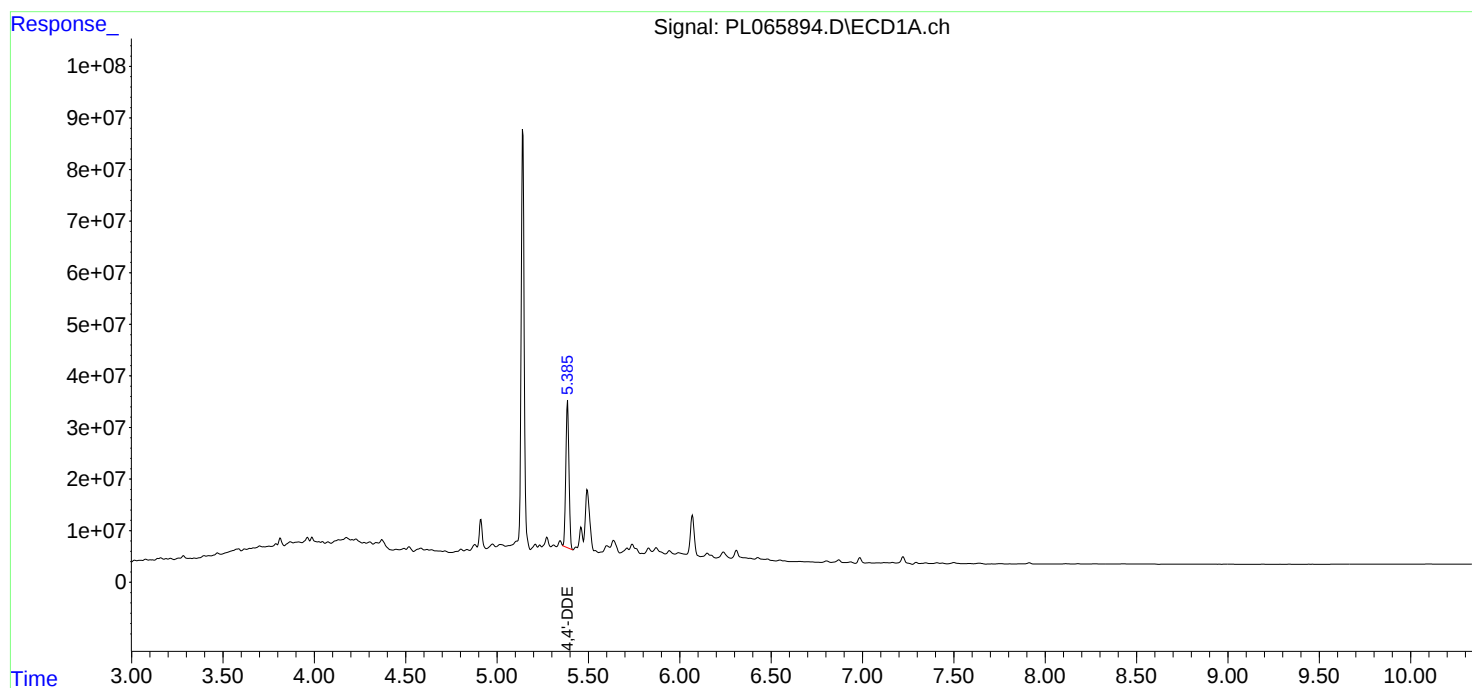

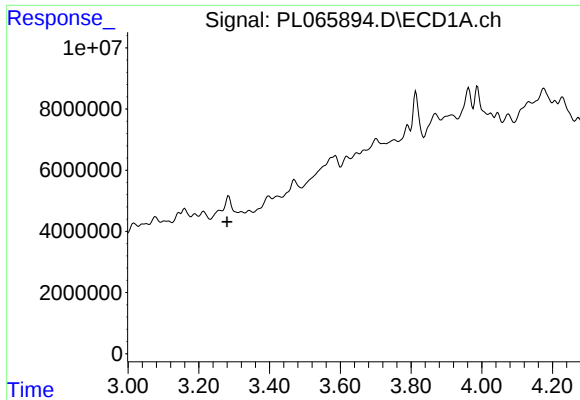


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 3.280 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
FS-SB-10-26-27DL


Manual Integrations
APPROVED

Ankita
4/7/2021 4:50:05 PM

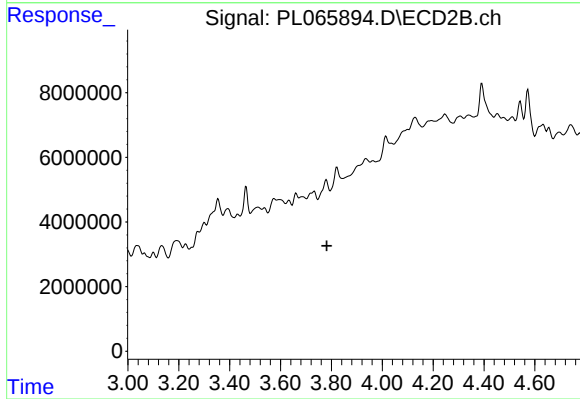


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 3.782 min
Response: 0
Conc: N.D.

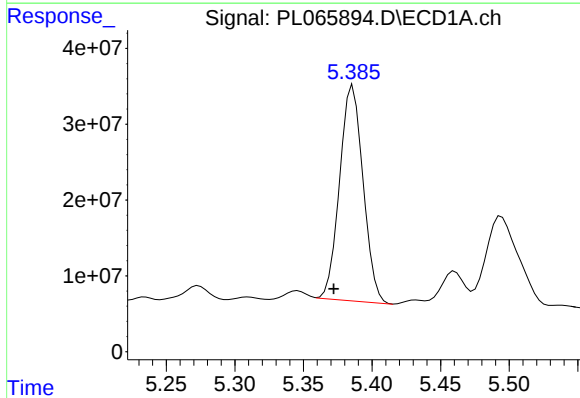


#12 4,4'-DDE

R.T.: 5.385 min
Delta R.T.: 0.013 min
Response: 338616149
Conc: 122.73 ng/ml m

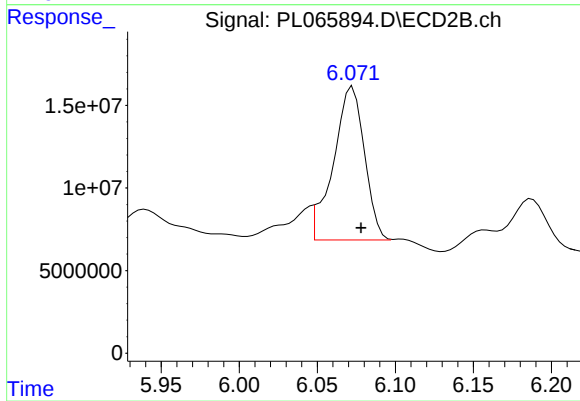

#12 4,4'-DDE

R.T.: 6.071 min
Delta R.T.: -0.007 min
Response: 127383599
Conc: 48.76 ng/ml m

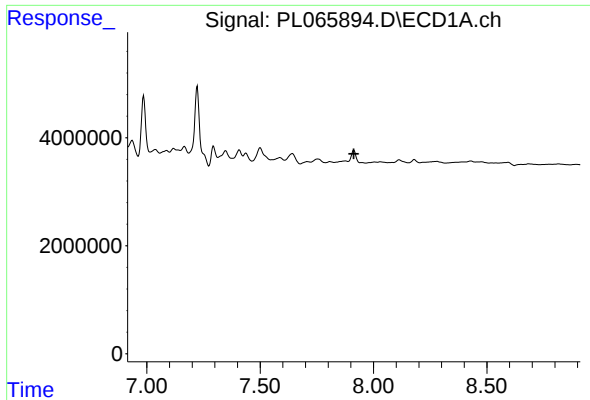


#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.914 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
FS-SB-10-26-27DL

Manual Integrations
APPROVED

Ankita
4/7/2021 4:50:05 PM

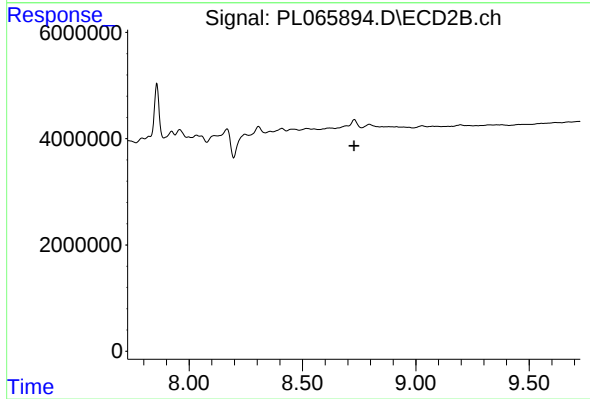

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.728 min
Response: 0
Conc: N.D.