

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040621\
 Data File : PL065915.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Apr 2021 16:02
 Operator : AR\AJ
 Sample : M1894-03
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 0154-FIELD-BLANK

Manual Integrations
 APPROVED

Ankita
 4/7/2021 4:50:40 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 07 04:34:44 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 31 15:57:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.275	3.780	41590655	42940249	15.966	15.643
28) SA Decachlor...	7.906	8.727	26886993	24357490	11.609m	10.804
Target Compounds						
6) B beta-BHC	4.225	4.628	2592392	4698285	1.626m	2.697m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040621\
Data File : PL065915.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Apr 2021 16:02
Operator : AR\AJ
Sample : M1894-03
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
0154-FIELD-BLANK


Manual Integrations
APPROVED

Ankita
4/7/2021 4:50:40 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 07 04:34:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
Quant Title : GC Extractables
QLast Update : Wed Mar 31 15:57:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

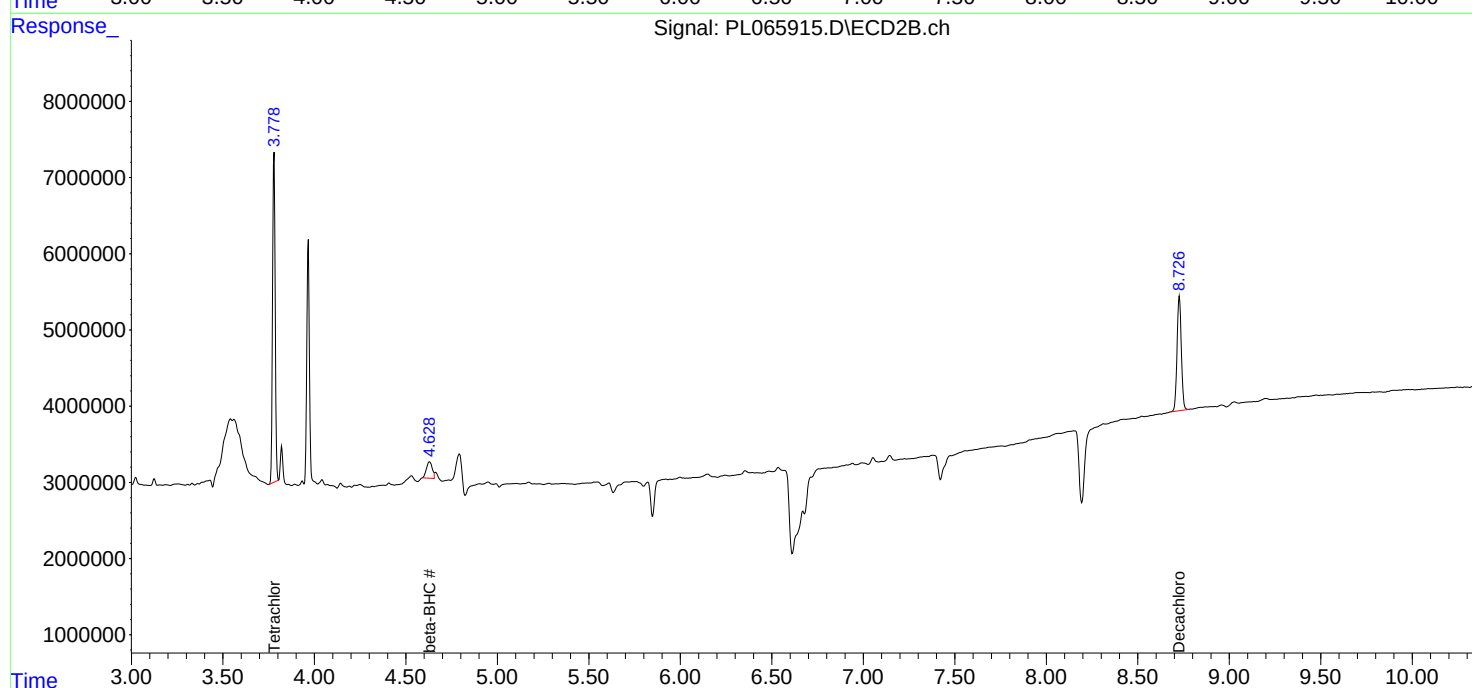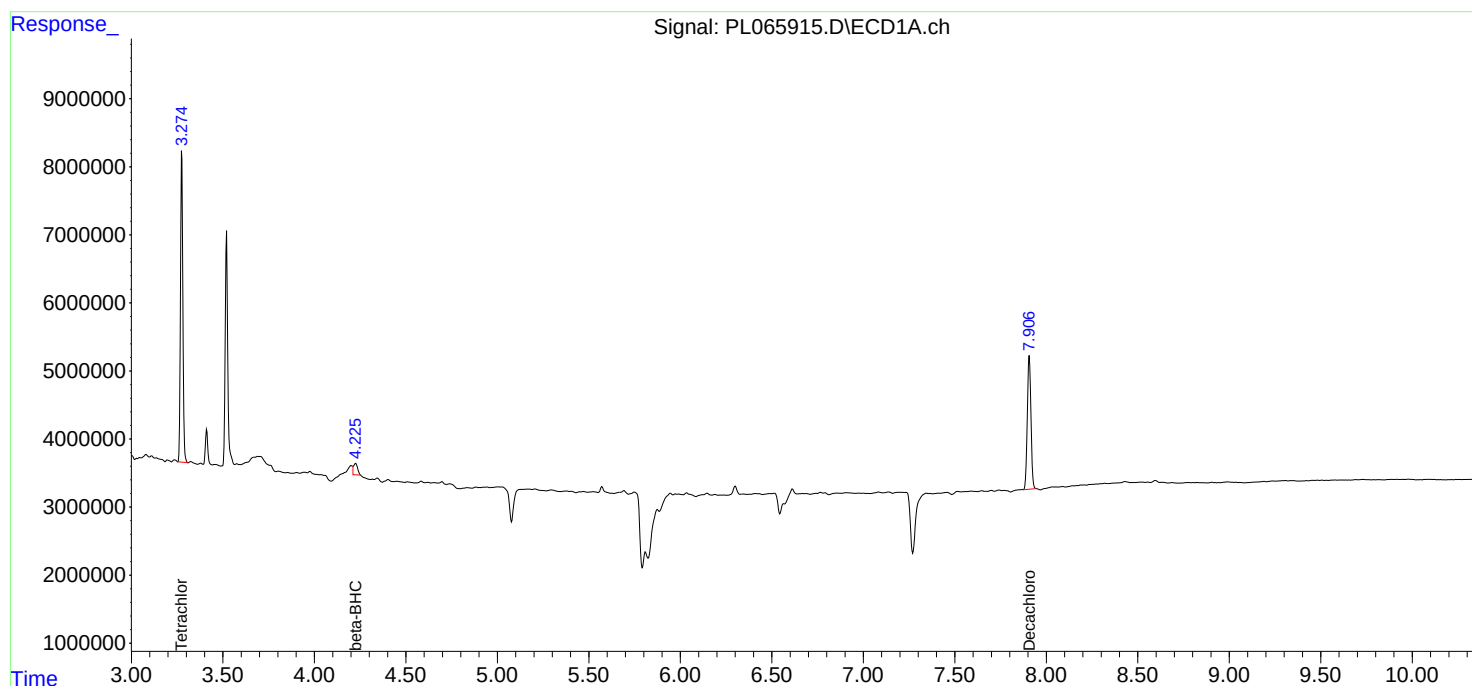

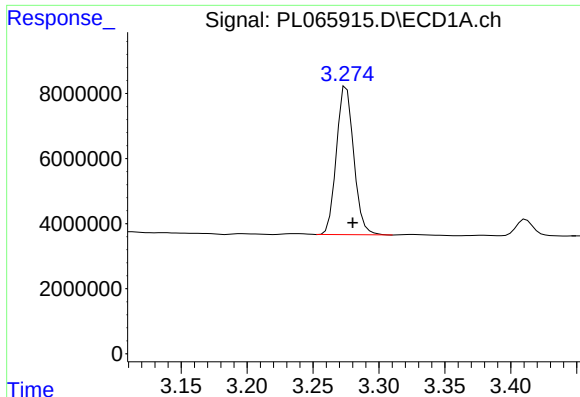


#1 Tetrachloro-m-xylene

R.T.: 3.275 min
Delta R.T.: -0.005 min
Response: 41590655
Conc: 15.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
0154-FIELD-BLANK


Manual Integrations
APPROVED

Ankita
4/7/2021 4:50:40 PM

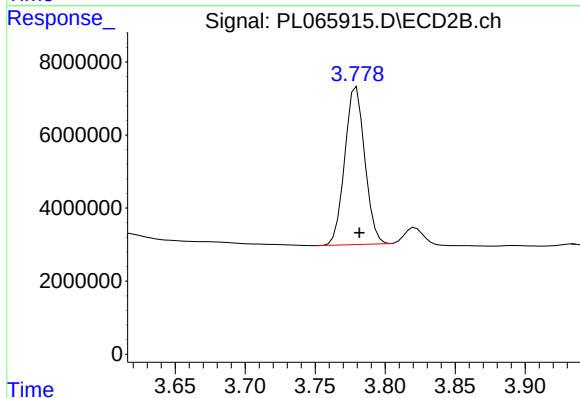


#1 Tetrachloro-m-xylene

R.T.: 3.780 min
Delta R.T.: -0.002 min
Response: 42940249
Conc: 15.64 ng/ml

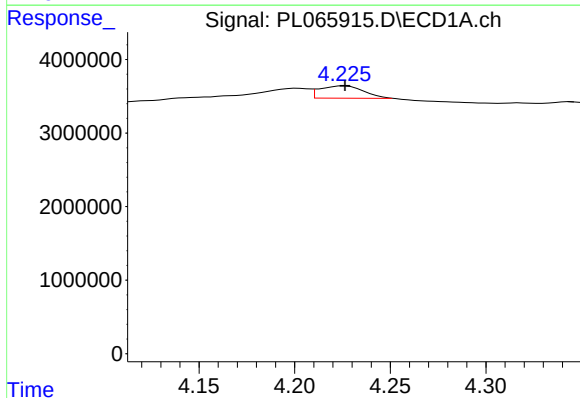


#6 beta-BHC

R.T.: 4.225 min
Delta R.T.: -0.002 min
Response: 2592392
Conc: 1.63 ng/ml m

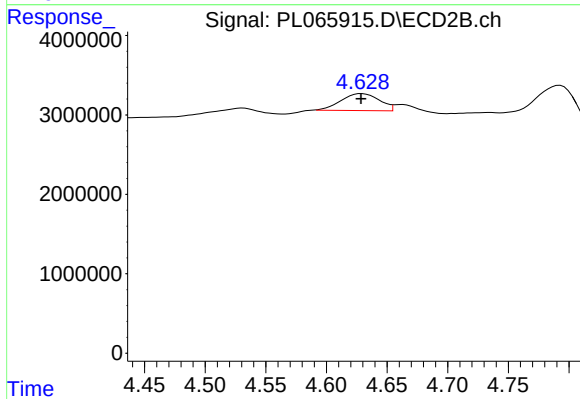

#6 beta-BHC

R.T.: 4.628 min
Delta R.T.: 0.000 min
Response: 4698285
Conc: 2.70 ng/ml m

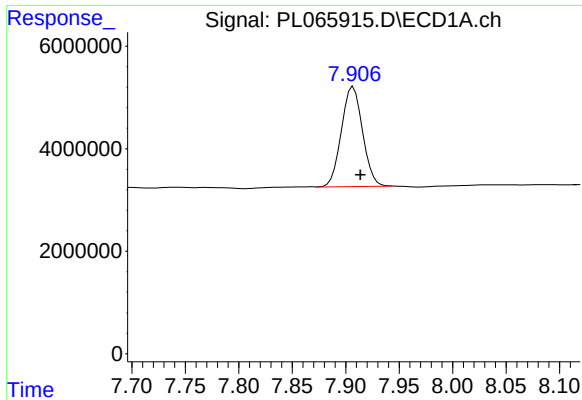


#28 Decachlorobiphenyl

R.T.: 7.906 min
Delta R.T.: -0.008 min
Response: 26886993
Conc: 11.61 ng/ml m

Instrument :
ECD_L
ClientSampleId :
0154-FIELD-BLANK

Manual Integrations
APPROVED

Ankita
4/7/2021 4:50:40 PM

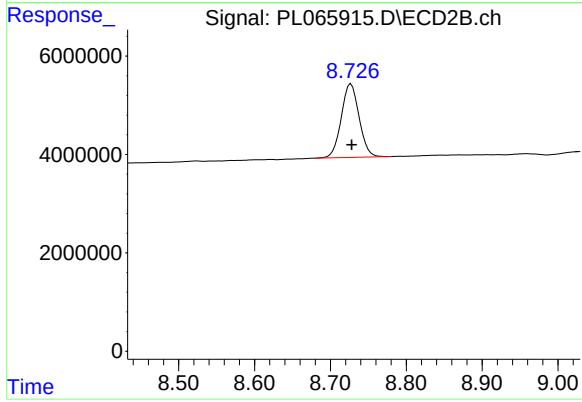

#28 Decachlorobiphenyl

R.T.: 8.727 min
Delta R.T.: 0.000 min
Response: 24357490
Conc: 10.80 ng/ml