

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040621\
 Data File : PL065920.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Apr 2021 17:13
 Operator : AR\AJ
 Sample : M1949-04
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CA-1

Manual Integrations
 APPROVED

Ankita
 4/7/2021 4:50:49 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 07 04:35:51 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 31 15:57:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.276	3.780	52671323	55896158	20.219	20.363
28)	SA Decachlor...	7.906	8.728	50497135	46118554	21.803m	20.456
Target Compounds							
6)	B beta-BHC	4.228	4.627	3938708	7004235	2.471m	4.021m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040621\
Data File : PL065920.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Apr 2021 17:13
Operator : AR\AJ
Sample : M1949-04
Misc :
ALS Vial : 29 Sample Multiplier: 1


Instrument :
ECD_L
ClientSampleId :
CA-1


Manual Integrations
APPROVED

Ankita
4/7/2021 4:50:49 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 07 04:35:51 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
Quant Title : GC Extractables
QLast Update : Wed Mar 31 15:57:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

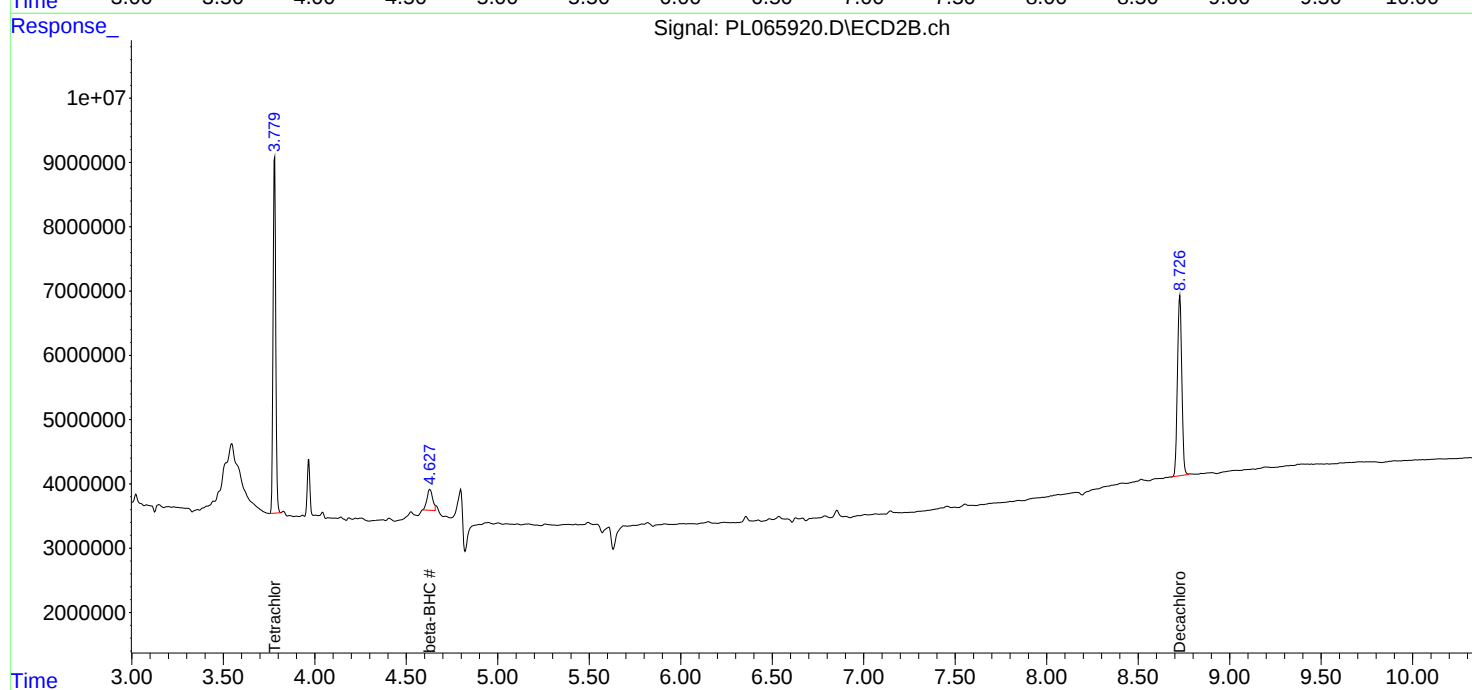

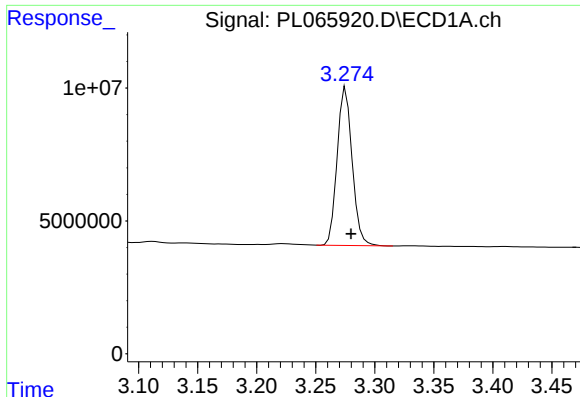


#1 Tetrachloro-m-xylene

R.T.: 3.276 min
Delta R.T.: -0.004 min
Response: 52671323
Conc: 20.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
CA-1


Manual Integrations
APPROVED

Ankita
4/7/2021 4:50:49 PM

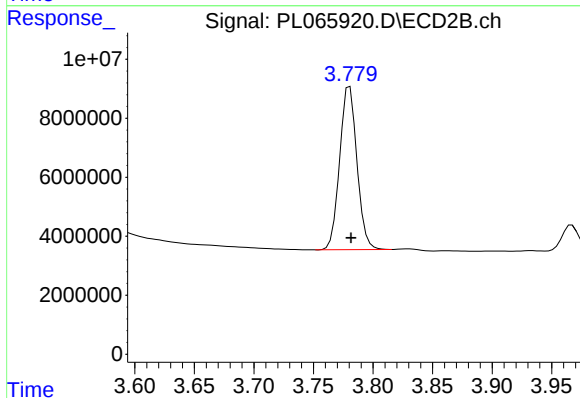


#1 Tetrachloro-m-xylene

R.T.: 3.780 min
Delta R.T.: -0.001 min
Response: 55896158
Conc: 20.36 ng/ml

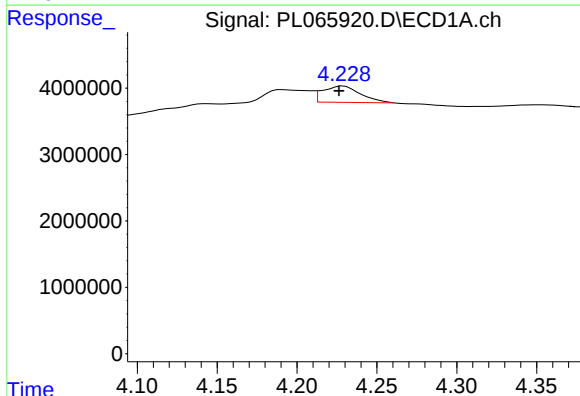


#6 beta-BHC

R.T.: 4.228 min
Delta R.T.: 0.001 min
Response: 3938708
Conc: 2.47 ng/ml m

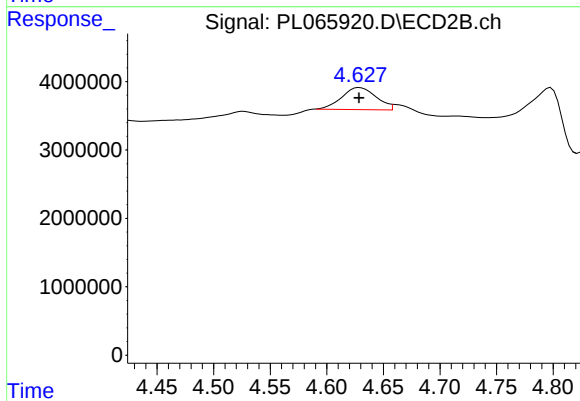

#6 beta-BHC

R.T.: 4.627 min
Delta R.T.: -0.001 min
Response: 7004235
Conc: 4.02 ng/ml m

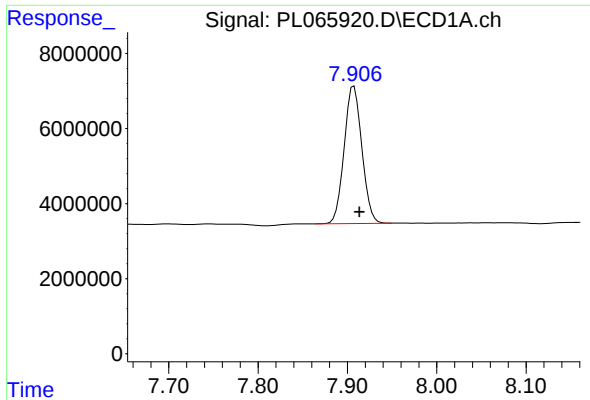


#28 Decachlorobiphenyl

R.T.: 7.906 min
Delta R.T.: -0.008 min
Response: 50497135
Conc: 21.80 ng/ml m

Instrument :
ECD_L
ClientSampleId :
CA-1

Manual Integrations
APPROVED

Ankita
4/7/2021 4:50:49 PM

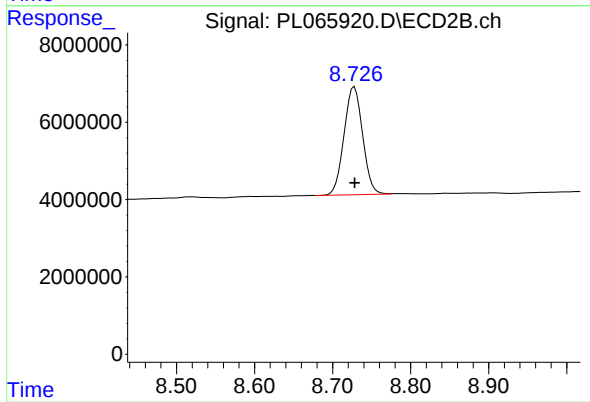

#28 Decachlorobiphenyl

R.T.: 8.728 min
Delta R.T.: 0.000 min
Response: 46118554
Conc: 20.46 ng/ml