

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040621\
 Data File : PL065921.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Apr 2021 17:27
 Operator : AR\AJ
 Sample : M1949-05
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 AB-1

Manual Integrations
 APPROVED

Ankita
 4/7/2021 4:50:51 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 07 04:36:04 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 31 15:57:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.276	3.780	52556280	55465742	20.175	20.206
28) SA Decachlor...	7.907	8.728	49144527	45420879	21.219m	20.147
Target Compounds						
6) B beta-BHC	4.229	4.629	5001047	3808551	3.138m	2.187m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040621\
Data File : PL065921.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Apr 2021 17:27
Operator : AR\AJ
Sample : M1949-05
Misc :
ALS Vial : 30 Sample Multiplier: 1


Instrument :
ECD_L
ClientSampled :
AB-1


Manual Integrations
APPROVED

Ankita
4/7/2021 4:50:51 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 07 04:36:04 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
Quant Title : GC Extractables
QLast Update : Wed Mar 31 15:57:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

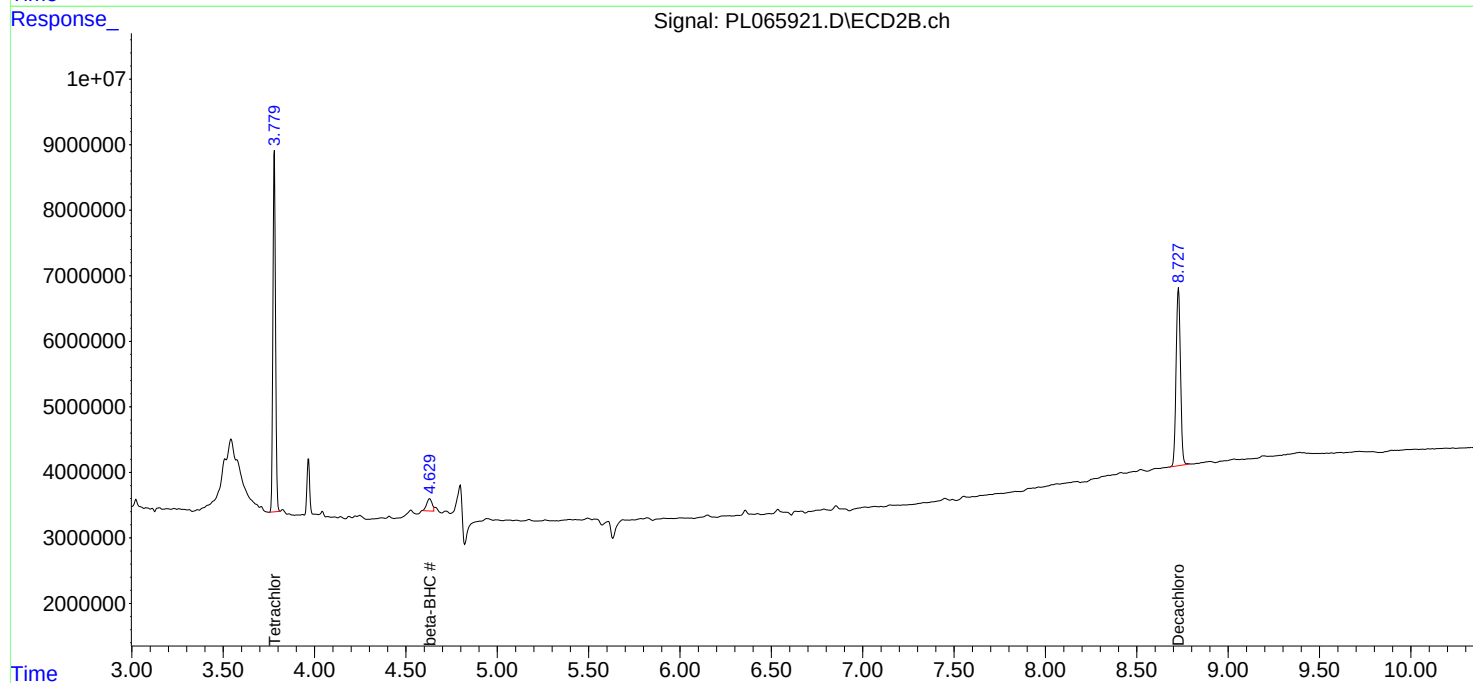

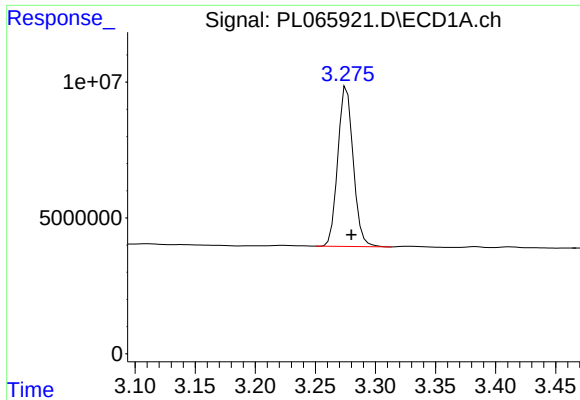


#1 Tetrachloro-m-xylene

R.T.: 3.276 min
Delta R.T.: -0.004 min
Response: 52556280
Conc: 20.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
AB-1


Manual Integrations
APPROVED

Ankita
4/7/2021 4:50:51 PM

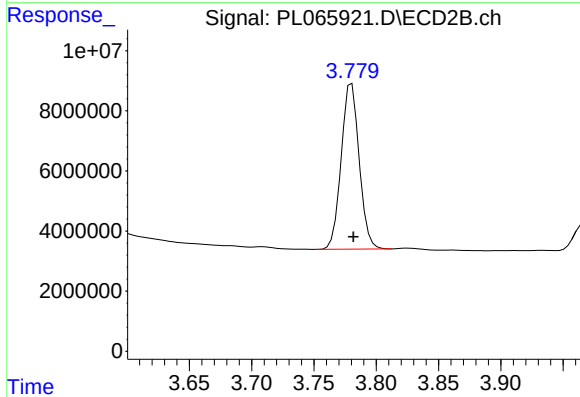


#1 Tetrachloro-m-xylene

R.T.: 3.780 min
Delta R.T.: -0.001 min
Response: 55465742
Conc: 20.21 ng/ml

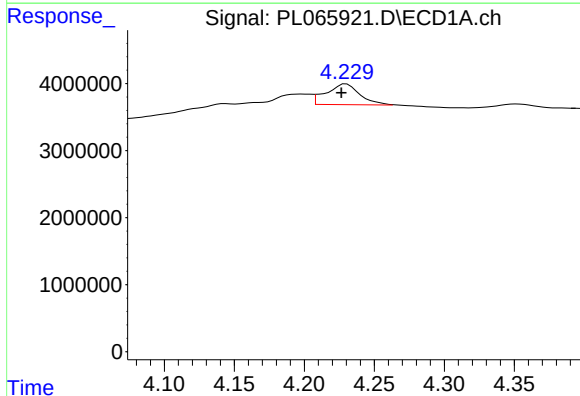


#6 beta-BHC

R.T.: 4.229 min
Delta R.T.: 0.002 min
Response: 5001047
Conc: 3.14 ng/ml m

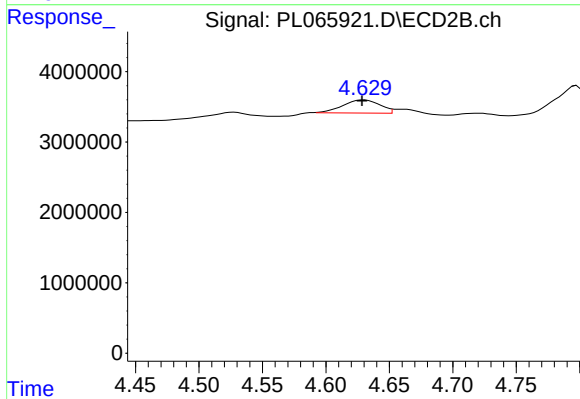

#6 beta-BHC

R.T.: 4.629 min
Delta R.T.: 0.000 min
Response: 3808551
Conc: 2.19 ng/ml m

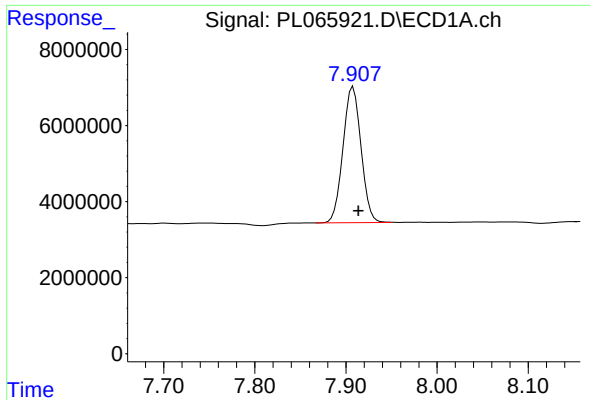


#28 Decachlorobiphenyl

R.T.: 7.907 min
Delta R.T.: -0.007 min
Response: 49144527
Conc: 21.22 ng/ml m

Instrument :
ECD_L
ClientSampleId :
AB-1

Manual Integrations
APPROVED

Ankita
4/7/2021 4:50:51 PM

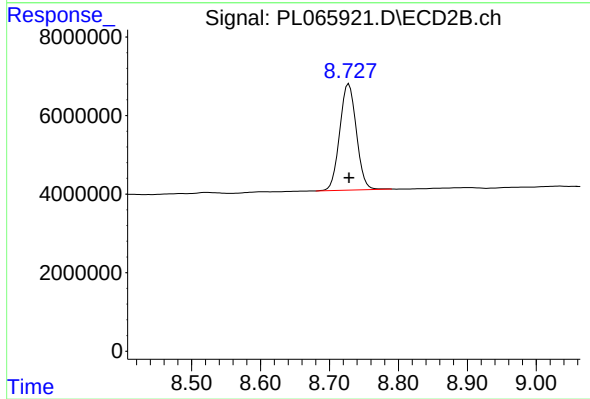

#28 Decachlorobiphenyl

R.T.: 8.728 min
Delta R.T.: 0.000 min
Response: 45420879
Conc: 20.15 ng/ml