

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040622\
 Data File : PL073864.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Apr 2022 18:33
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 07 02:14:21 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 04:12:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.640	5.491	7017286	39976878	21.909	24.358
28)	SA Decachlor...	10.413	11.334	10674773	36512623	20.993	20.419
Target Compounds							
5)	MB Aldrin	0.000	7.464	0	102955	N.D.	0.049 #
6)	B beta-BHC	0.000	6.682	0	646977	N.D.	0.621 #
7)	B delta-BHC	0.000	6.958	0	2240506	N.D.	1.040 #
10)	B gamma-Chl...	0.000	8.209	0	296930	N.D.	0.145 #
14)	MA Endrin	8.088f	0.000	97342	0	0.251	N.D. #
15)	B Endosulfa...	0.000	9.059	0	204528	N.D.	0.133 #
16)	A 4,4'-DDD	0.000	9.011f	0	98644	N.D.	0.068 #
17)	MA 4,4'-DDT	0.000	9.290f	0	122444	N.D.	0.075 #
19)	B Endosulfa...	0.000	9.450	0	40161	N.D.	0.025 #
22)	Mirex	0.000	10.410	0	455772	N.D.	0.336 #
23)	Chlordane-1	0.000	6.855	0	1547367	N.D.	22.651 #
24)	Chlordane-2	0.000	7.464f	0	102955	N.D.	1.432 #
25)	Chlordane-3	0.000	8.209	0	296930	N.D.	1.095 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040622\
Data File : PL073864.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Apr 2022 18:33
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 07 02:14:21 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 04:12:46 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

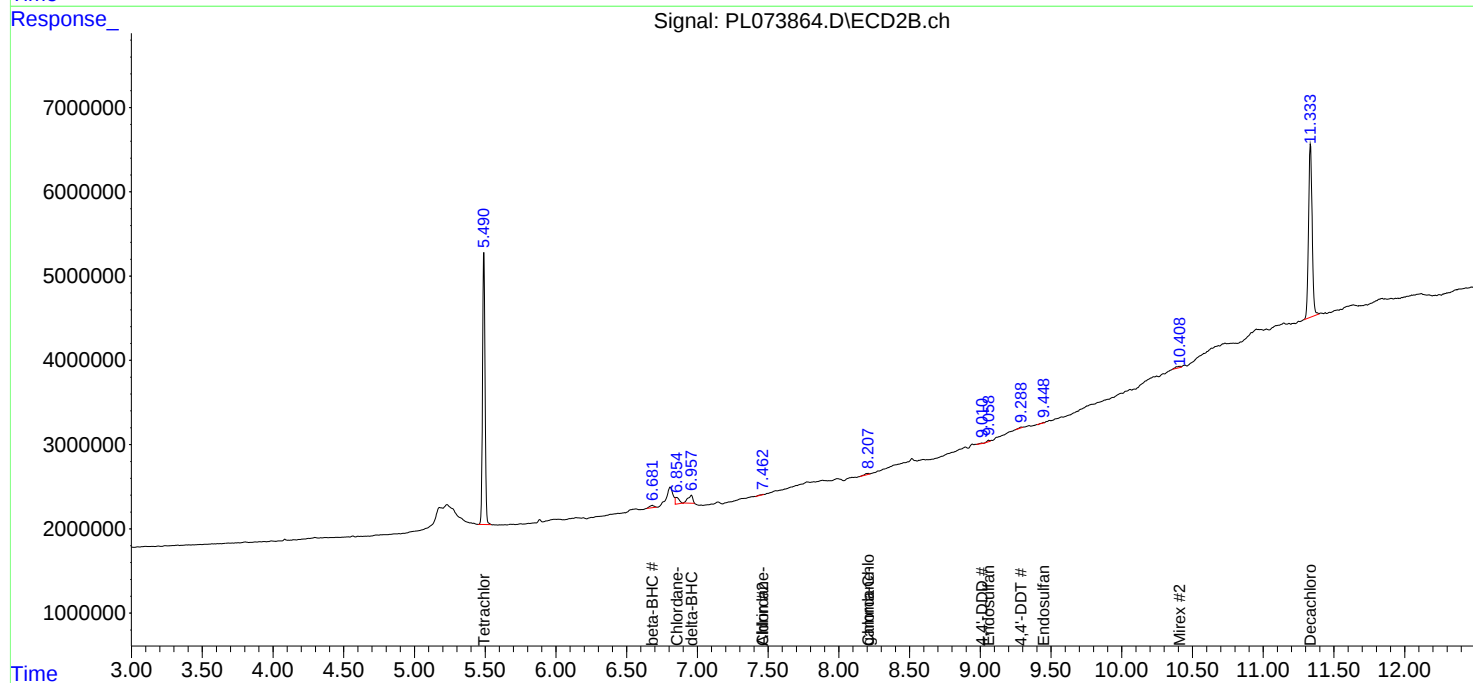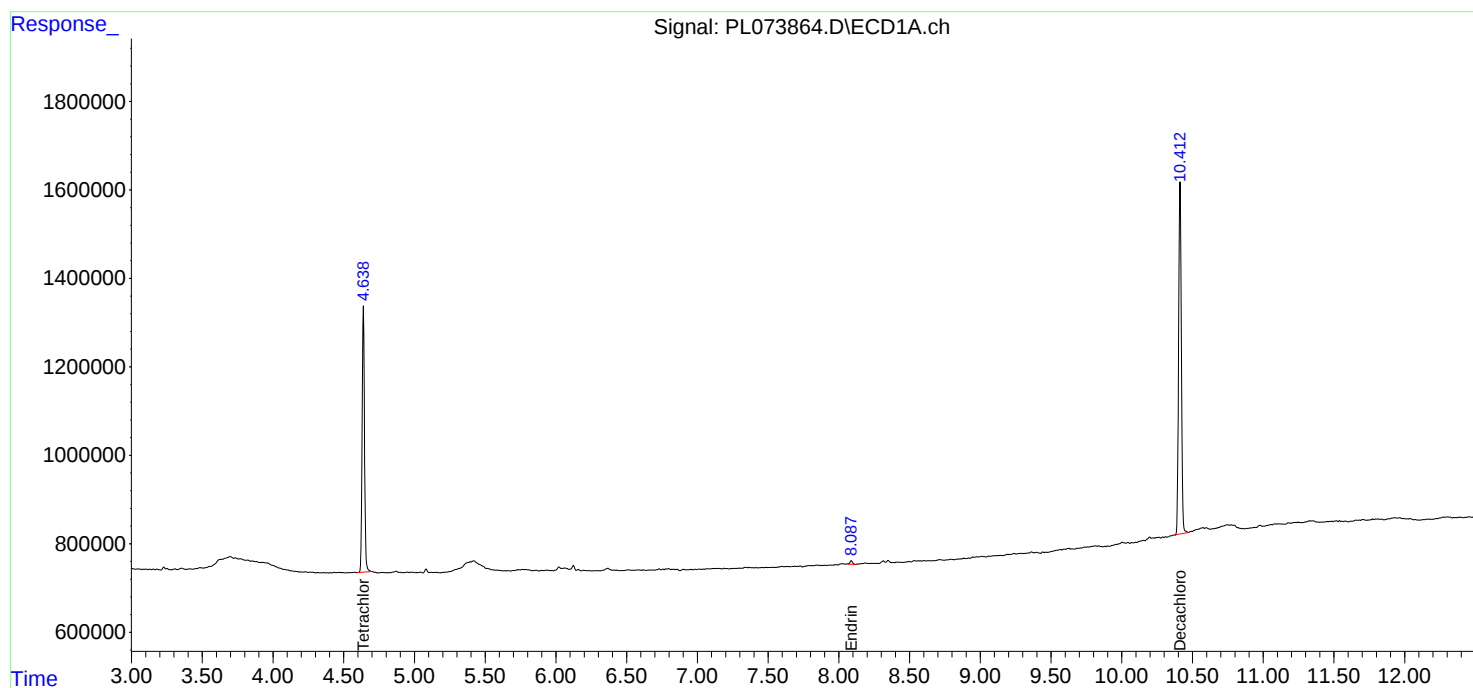


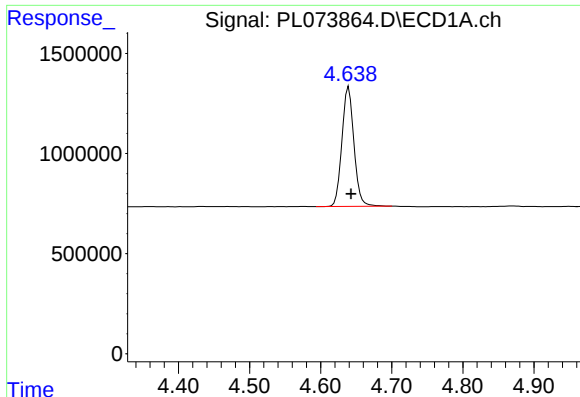

#1 Tetrachloro-m-xylene


R.T.: 4.640 min
Delta R.T.: -0.003 min
Response: 7017286
Conc: 21.91 ng/ml

Instrument :
ECD_L
ClientSampleId :

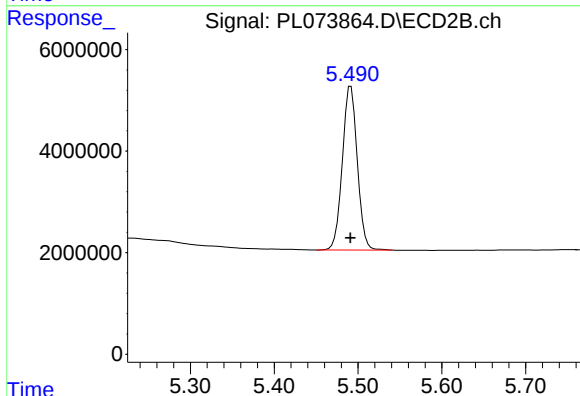


#1 Tetrachloro-m-xylene

R.T.: 5.491 min
Delta R.T.: 0.000 min
Response: 39976878
Conc: 24.36 ng/ml

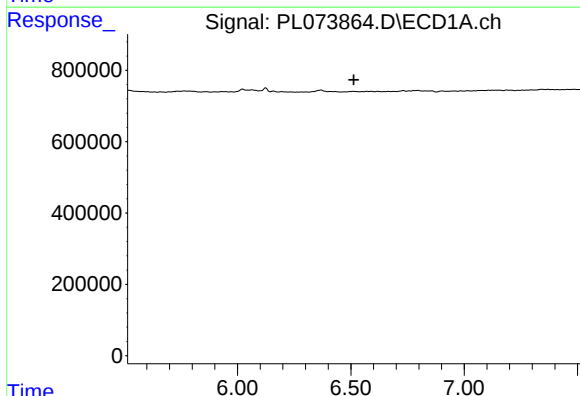


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 6.513 min
Response: 0
Conc: N.D.

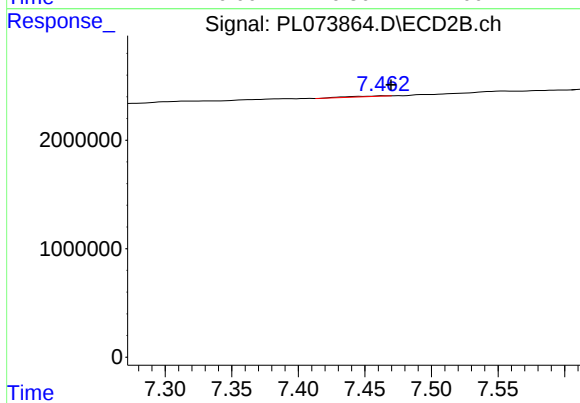

#5 Aldrin


R.T.: 7.464 min
Delta R.T.: -0.006 min
Response: 102955
Conc: 0.05 ng/ml

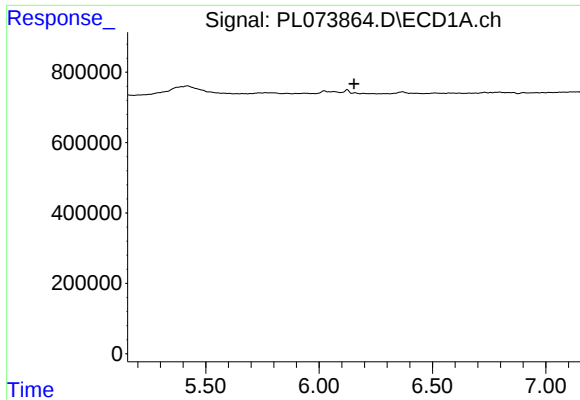

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 6.155 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

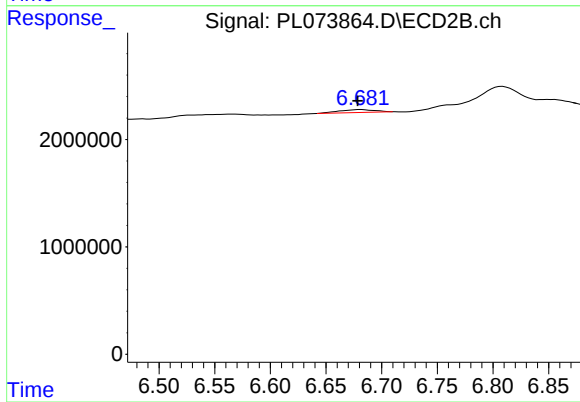


#6 beta-BHC

R.T.: 6.682 min
Delta R.T.: 0.003 min
Response: 646977
Conc: 0.62 ng/ml

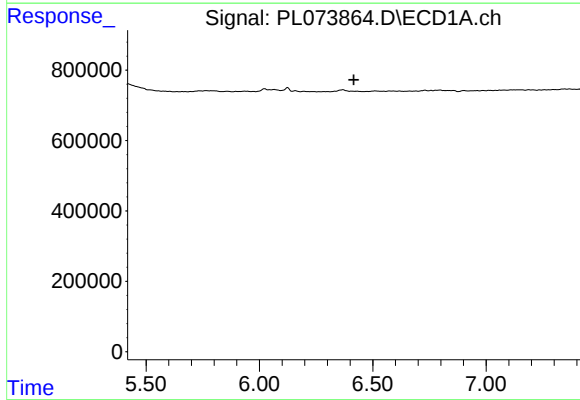


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 6.416 min
Response: 0
Conc: N.D.

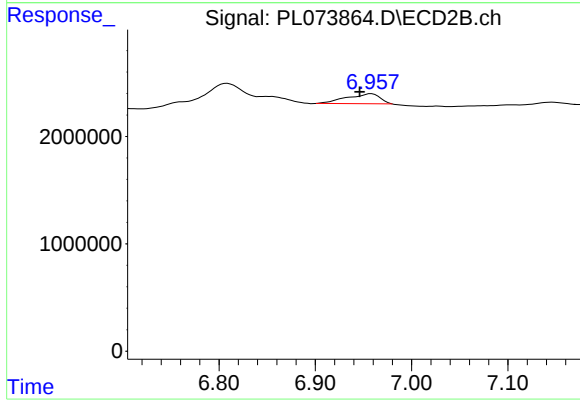

#7 delta-BHC


R.T.: 6.958 min
Delta R.T.: 0.012 min
Response: 2240506
Conc: 1.04 ng/ml

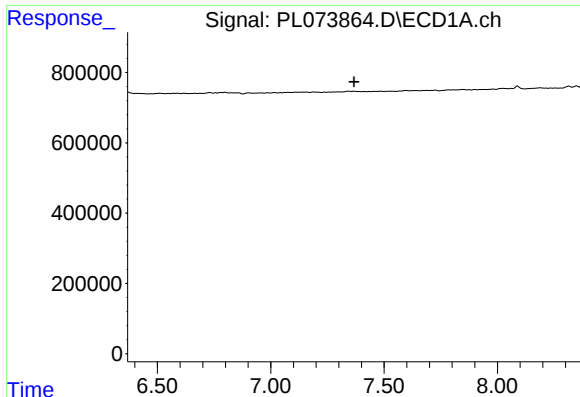

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.368 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

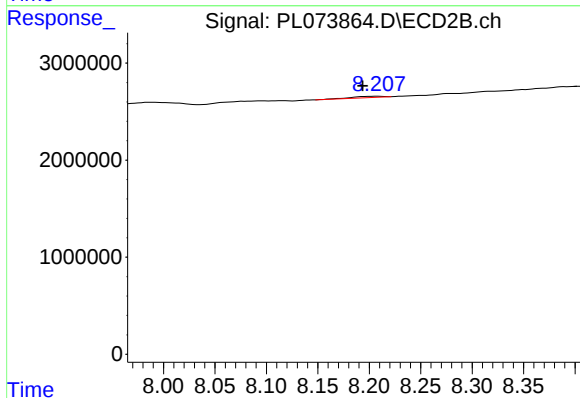


#10 gamma-Chlordane

R.T.: 8.209 min
Delta R.T.: 0.015 min
Response: 296930
Conc: 0.15 ng/ml

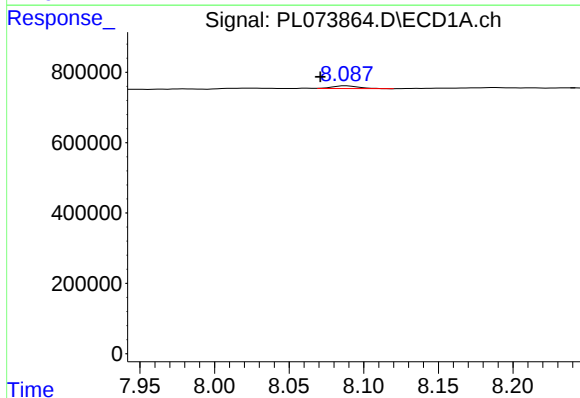


#14 Endrin

R.T.: 8.088 min
Delta R.T.: 0.017 min
Response: 97342
Conc: 0.25 ng/ml

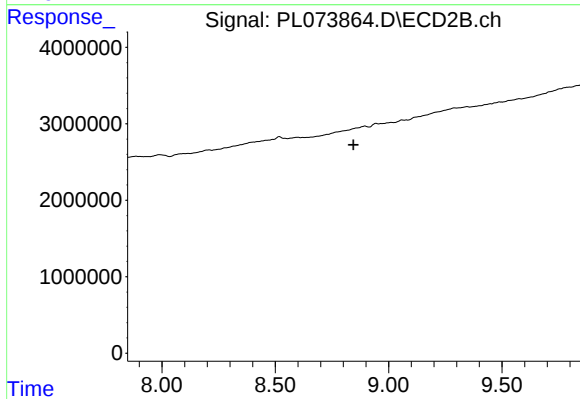

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 8.845 min
Response: 0
Conc: N.D.

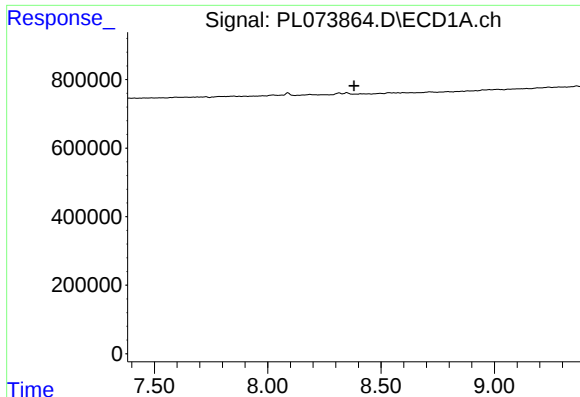

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.382 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

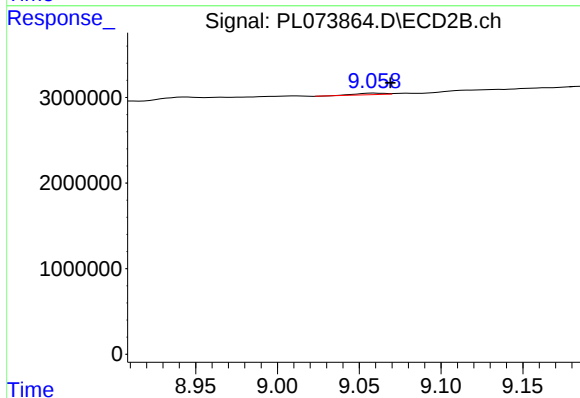


#15 Endosulfan II

R.T.: 9.059 min
Delta R.T.: -0.010 min
Response: 204528
Conc: 0.13 ng/ml

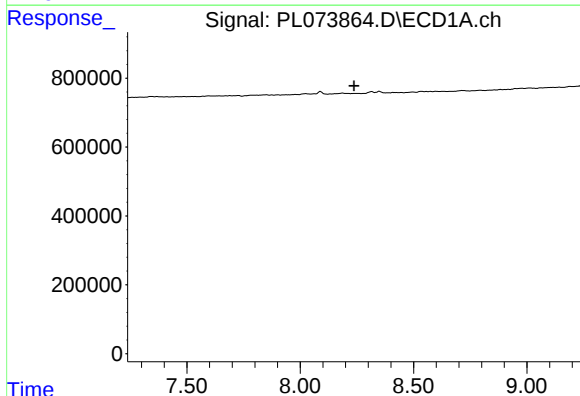


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 8.237 min
Response: 0
Conc: N.D.

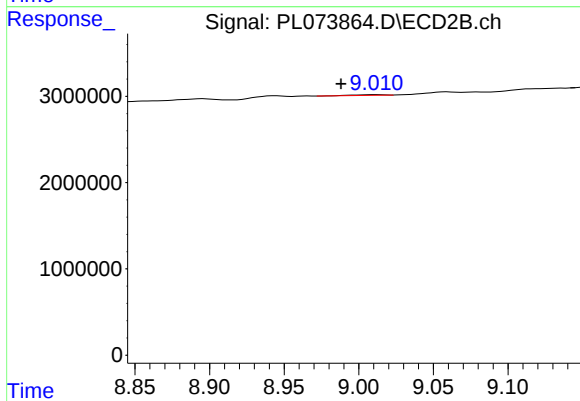

#16 4,4'-DDD


R.T.: 9.011 min
Delta R.T.: 0.023 min
Response: 98644
Conc: 0.07 ng/ml

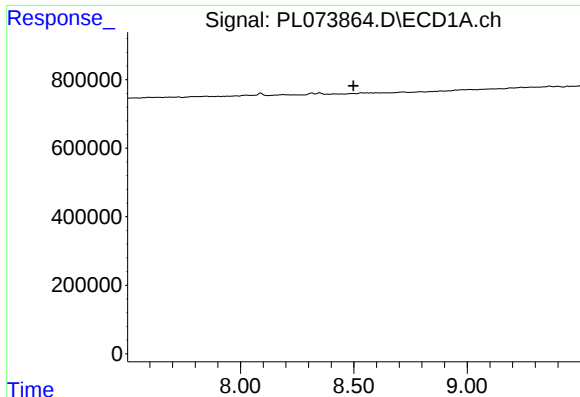

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 8.499 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

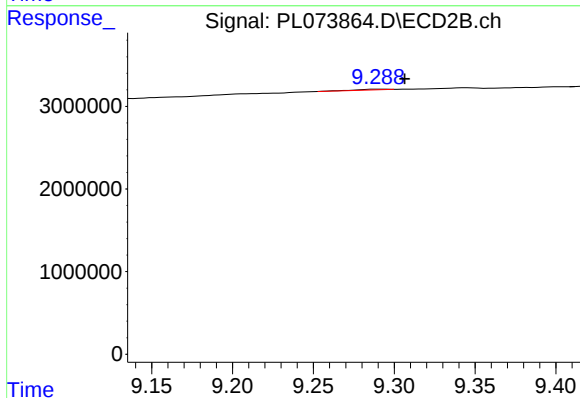


#17 4,4'-DDT

R.T.: 9.290 min
Delta R.T.: -0.016 min
Response: 122444
Conc: 0.07 ng/ml

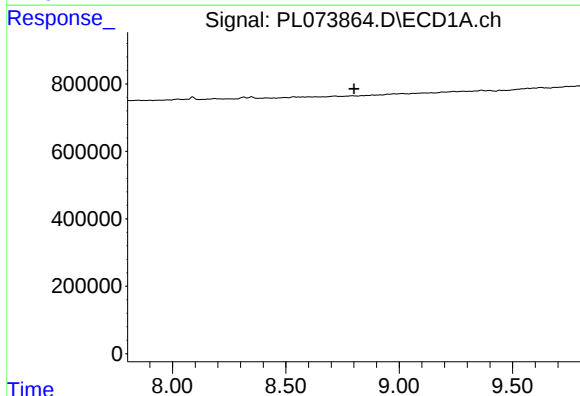


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 8.801 min
Response: 0
Conc: N.D.

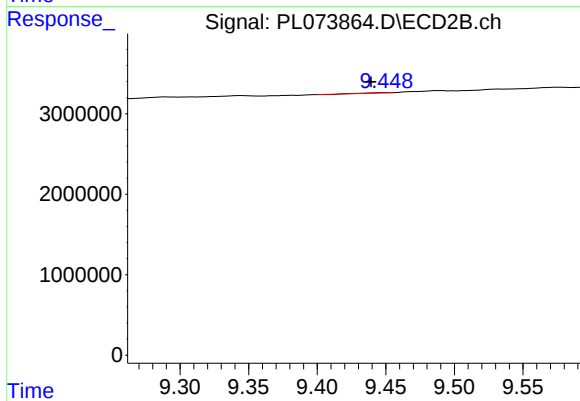

#19 Endosulfan Sulfate


R.T.: 9.450 min
Delta R.T.: 0.011 min
Response: 40161
Conc: 0.03 ng/ml

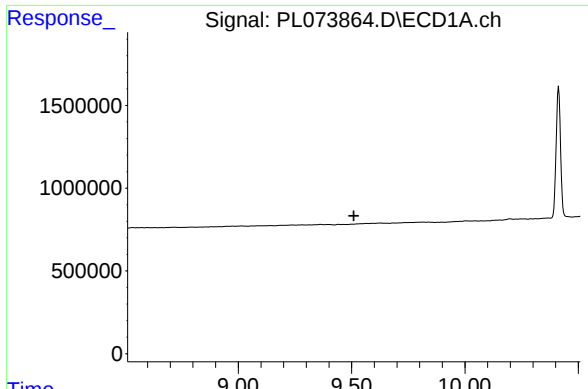

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 9.509 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

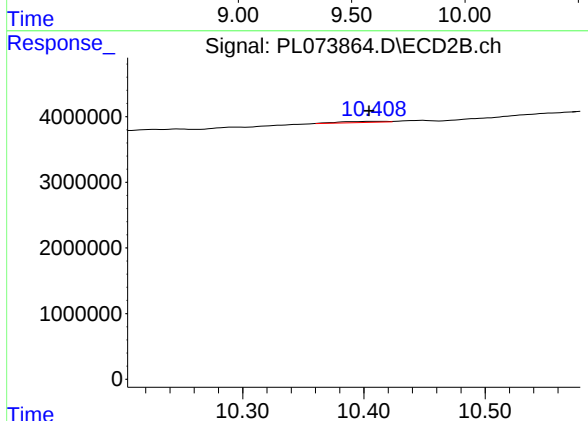


#22 Mirex

R.T.: 10.410 min
Delta R.T.: 0.006 min
Response: 455772
Conc: 0.34 ng/ml

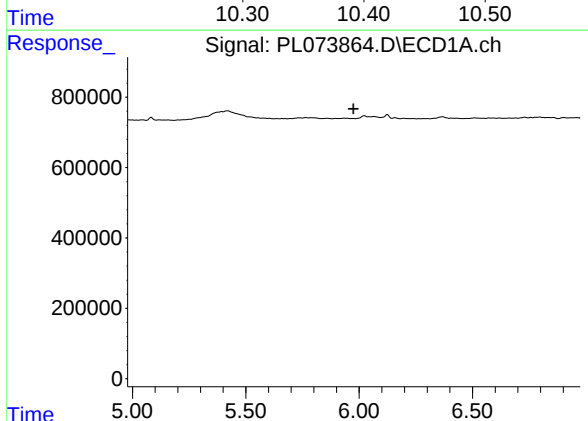


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 5.976 min
Response: 0
Conc: N.D.

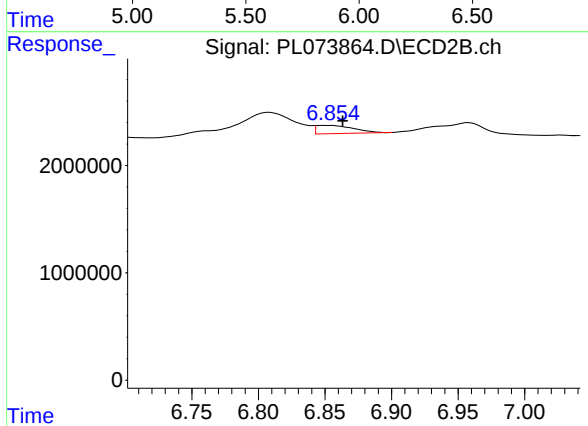

#23 Chlordane-1


R.T.: 6.855 min
Delta R.T.: -0.008 min
Response: 1547367
Conc: 22.65 ng/ml

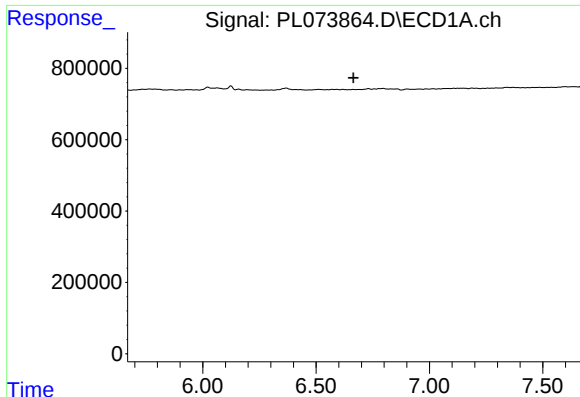

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 6.665 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

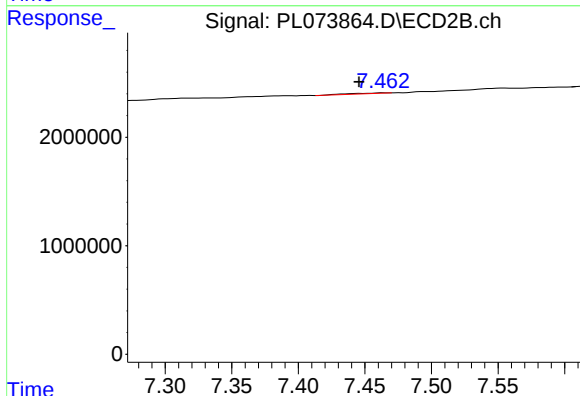


#24 Chlordane-2

R.T.: 7.464 min
Delta R.T.: 0.018 min
Response: 102955
Conc: 1.43 ng/ml

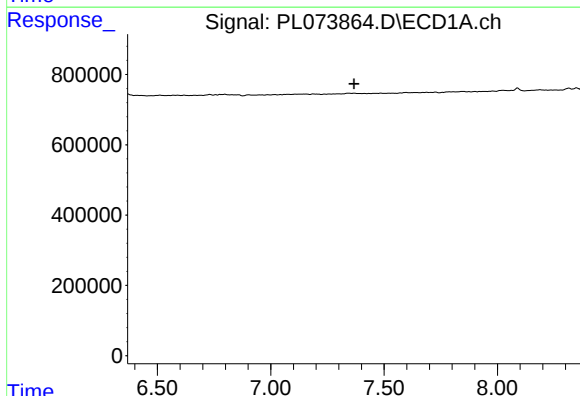


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.368 min
Response: 0
Conc: N.D.

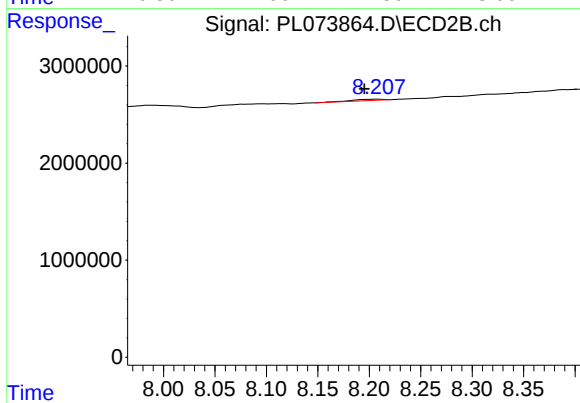

#25 Chlordane-3


R.T.: 8.209 min
Delta R.T.: 0.013 min
Response: 296930
Conc: 1.10 ng/ml

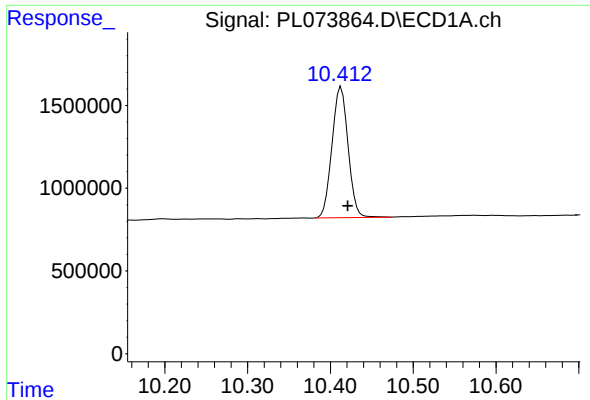

#28 Decachlorobiphenyl

R.T.: 10.413 min
Delta R.T.: -0.008 min
Response: 10674773
Conc: 20.99 ng/ml

Instrument :
ECD_L
ClientSampleId :

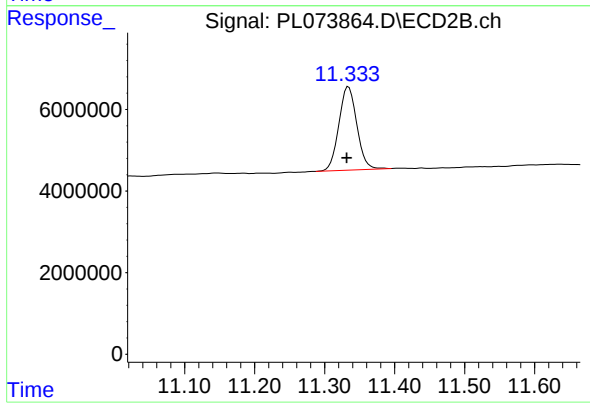

#28 Decachlorobiphenyl

R.T.: 11.334 min
Delta R.T.: 0.003 min
Response: 36512623
Conc: 20.42 ng/ml