

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040622\
 Data File : PL073856.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Apr 2022 16:22
 Operator : AR\AJ
 Sample : N2270-07
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 N2270-07

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 07 02:11:38 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 04:12:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.638	5.491	6523842	34905530	20.369m	21.268
28) SA Decachlor...	10.414	11.335	8354360	29240386	16.429	16.352
Target Compounds						
11) B alpha-Chl...	7.428	8.285	139559	792650	0.316m	0.396 #
12) B 4,4'-DDE	7.645	8.465	205921	823662	0.574	0.460


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040622\
Data File : PL073856.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Apr 2022 16:22
Operator : AR\AJ
Sample : N2270-07
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
N2270-07

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 07 02:11:38 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 04:12:46 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

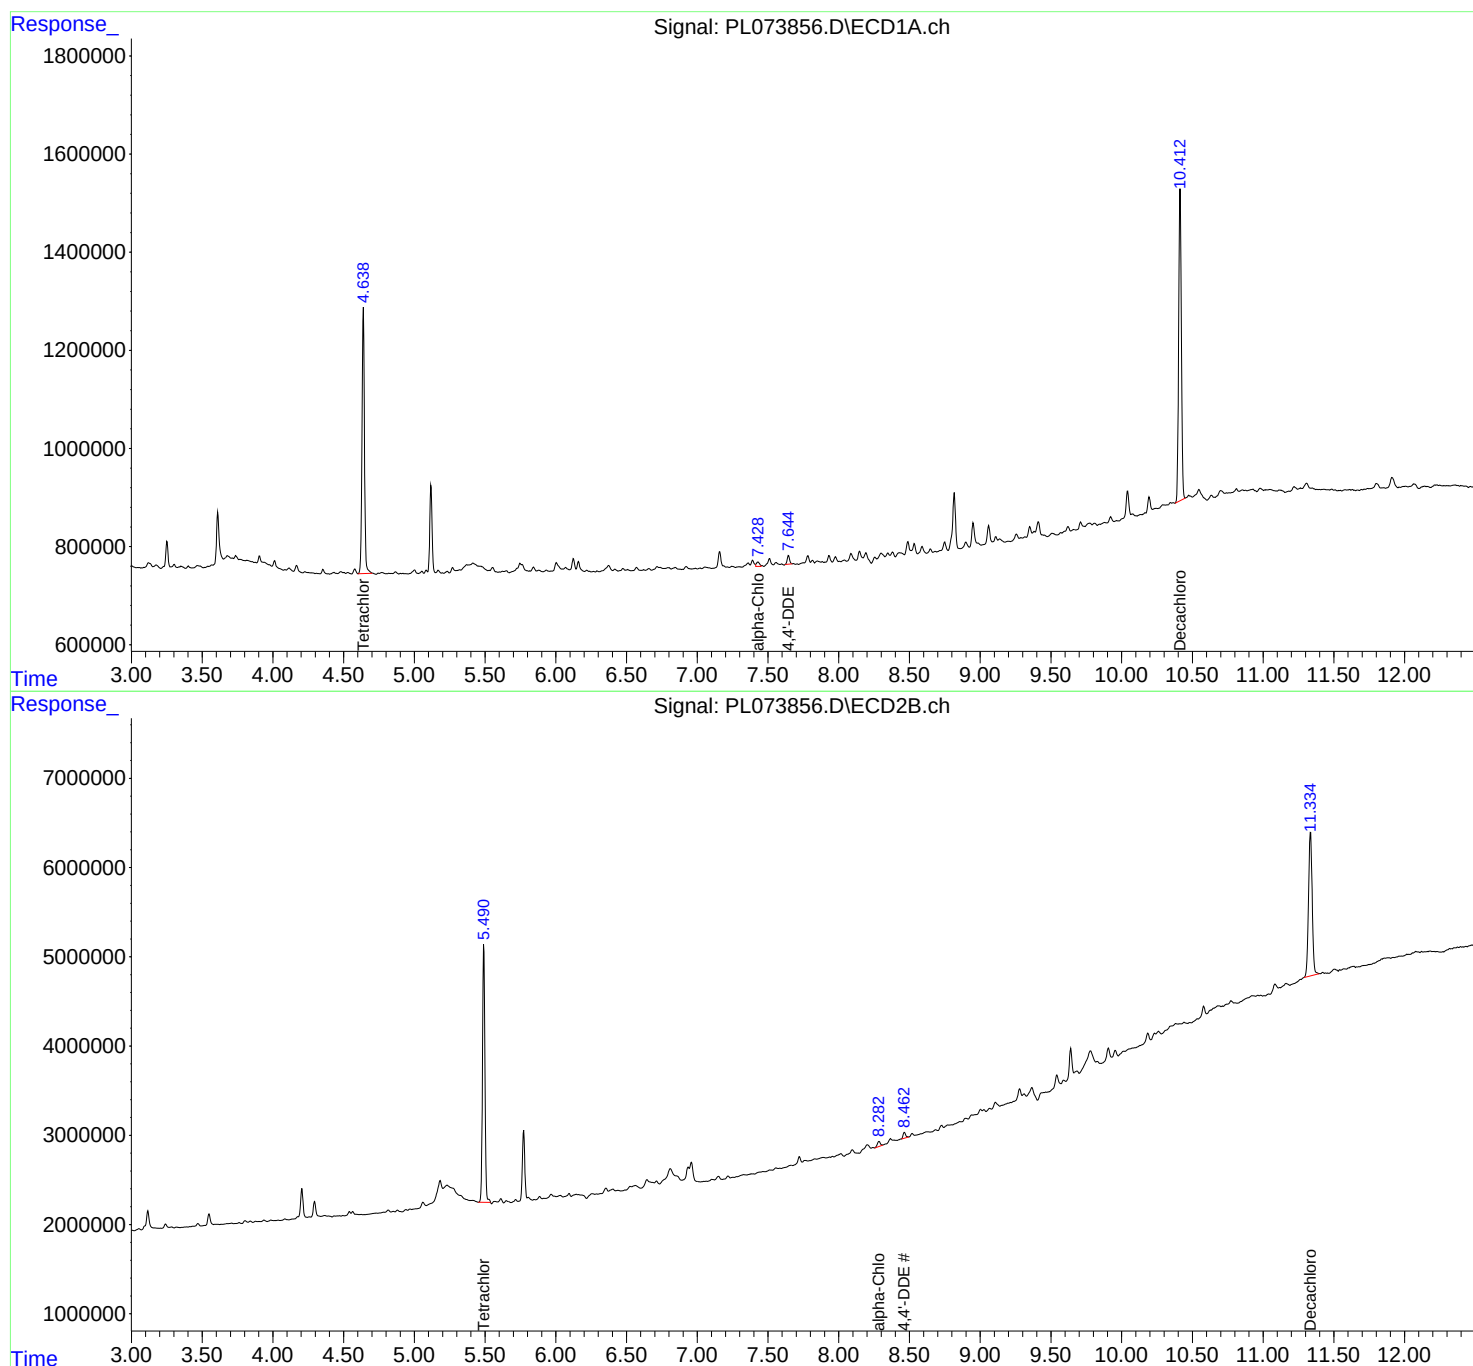


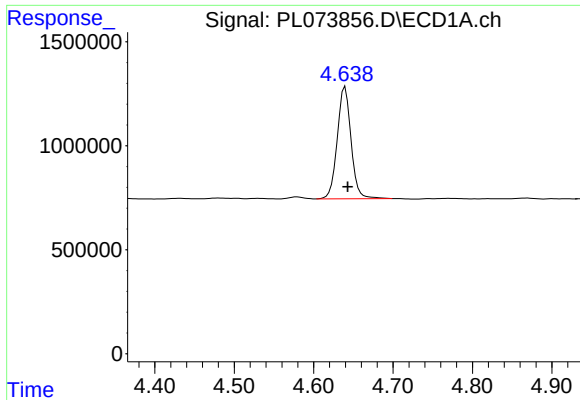

#1 Tetrachloro-m-xylene


R.T.: 4.638 min
Delta R.T.: -0.005 min
Response: 6523842
Conc: 20.37 ng/ml

Instrument :
ECD_L
ClientSampleId :
N2270-07

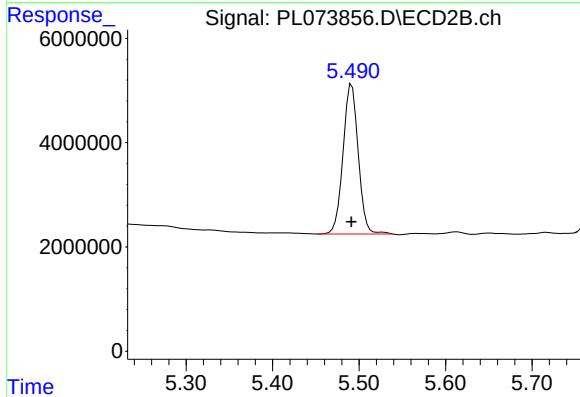


#1 Tetrachloro-m-xylene

R.T.: 5.491 min
Delta R.T.: 0.000 min
Response: 34905530
Conc: 21.27 ng/ml

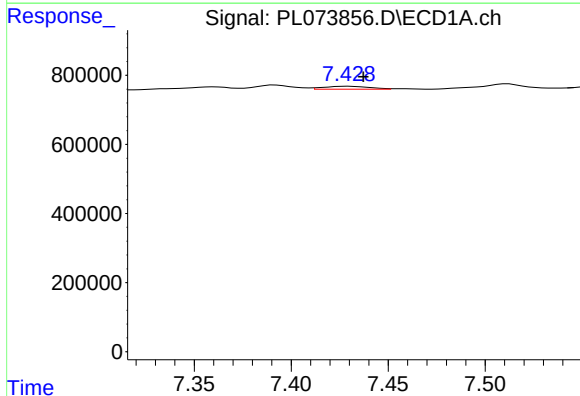


#11 alpha-Chlordane

R.T.: 7.428 min
Delta R.T.: -0.009 min
Response: 139559
Conc: 0.32 ng/ml m

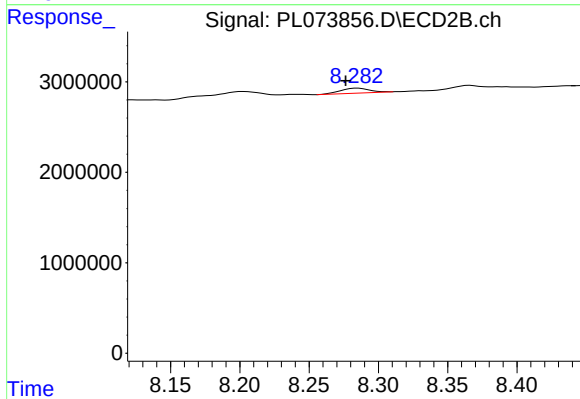

#11 alpha-Chlordane


R.T.: 8.285 min
Delta R.T.: 0.008 min
Response: 792650
Conc: 0.40 ng/ml

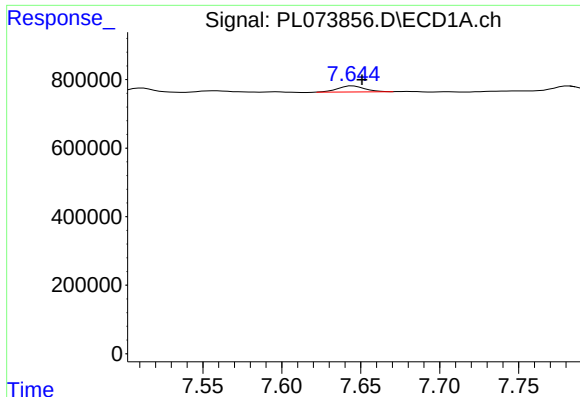

#12 4,4'-DDE


R.T.: 7.645 min
Delta R.T.: -0.006 min
Response: 205921
Conc: 0.57 ng/ml

Instrument :
ECD_L
ClientSampleId :
N2270-07

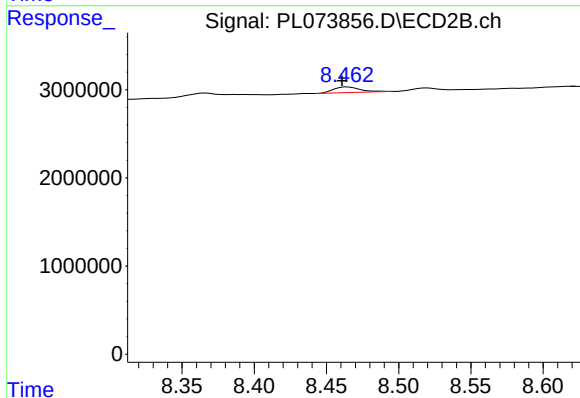


#12 4,4'-DDE

R.T.: 8.465 min
Delta R.T.: 0.004 min
Response: 823662
Conc: 0.46 ng/ml

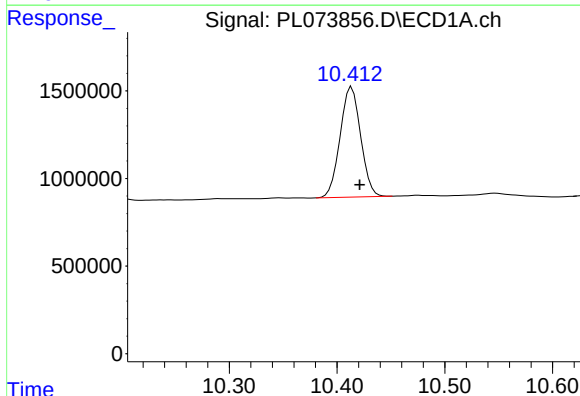

#28 Decachlorobiphenyl

R.T.: 10.414 min
Delta R.T.: -0.007 min
Response: 8354360
Conc: 16.43 ng/ml

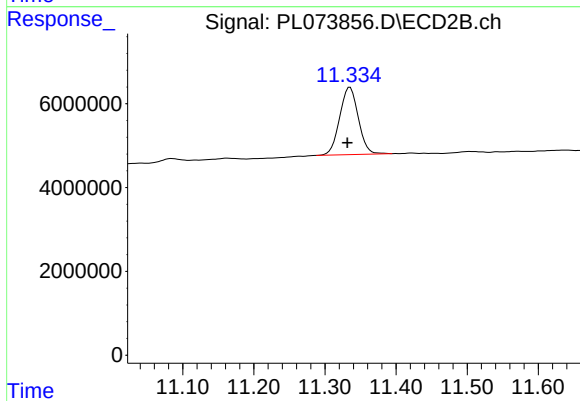

#28 Decachlorobiphenyl

R.T.: 11.335 min
Delta R.T.: 0.004 min
Response: 29240386
Conc: 16.35 ng/ml