

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040721\
 Data File : PL065930.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Apr 2021 09:22
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 08 06:40:49 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 31 15:57:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.276	3.780	48699000	49984470	18.694	18.210
28)	SA Decachlor...	7.907	8.726	44551315	42475521	19.236	18.840
Target Compounds							
2)	A alpha-BHC	3.708	0.000	3256083	0	0.796	N.D. #
4)	MA Heptachlor	4.232f	4.943	1956953	730628	0.543	0.207 #
6)	B beta-BHC	4.232	4.632	1956953	15696349	1.228	9.012 #
14)	MA Endrin	5.750	0.000	320317	0	0.119	N.D. #
18)	B Endrin al...	0.000	6.801f	0	122074	N.D.	0.064 #
20)	A Methoxychlor	0.000	7.335	0	996761	N.D.	0.787 #
21)	B Endrin ke...	6.859	7.434f	633324	524670	0.231	0.204
23)	Chlordane-1	4.137f	0.000	1181257	0	13.092	N.D. #
27)	Chlordane-5	0.000	6.722	0	534622	N.D.	6.412 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040721\
Data File : PL065930.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Apr 2021 09:22
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 08 06:40:49 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
Quant Title : GC Extractables
QLast Update : Wed Mar 31 15:57:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

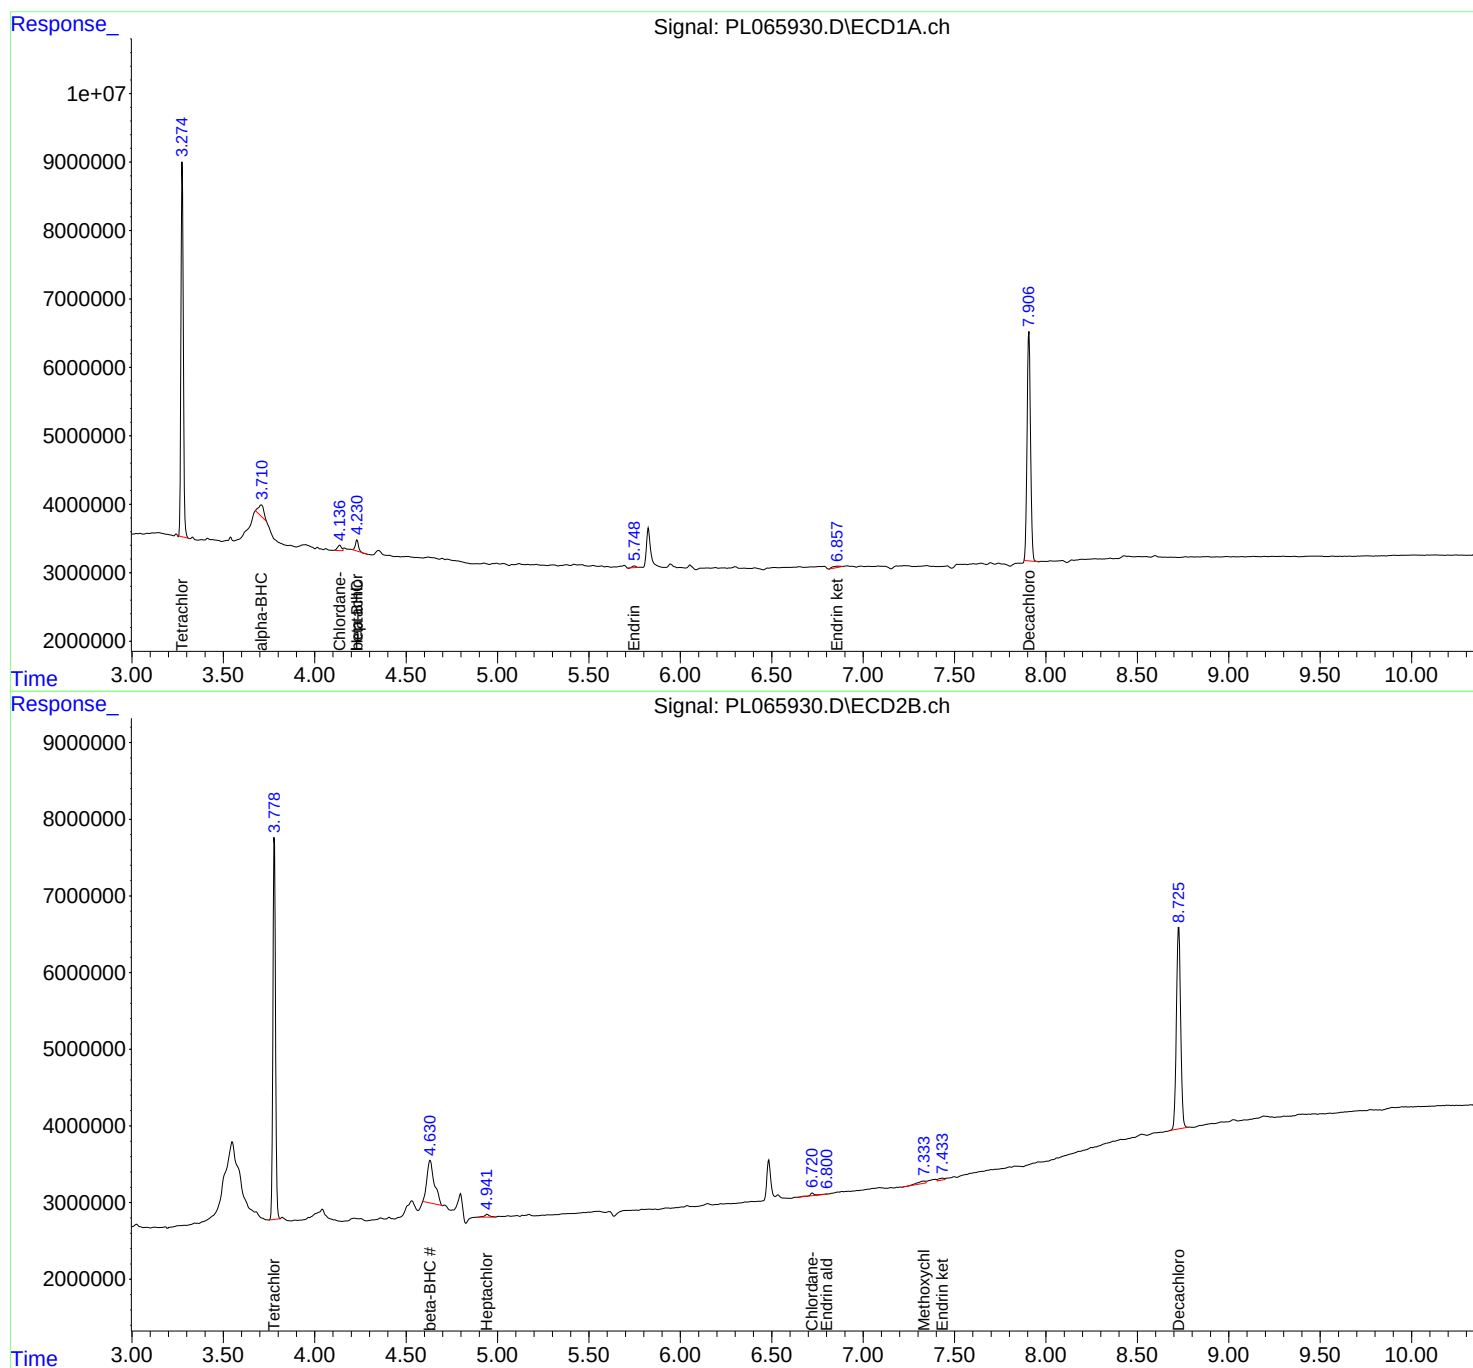


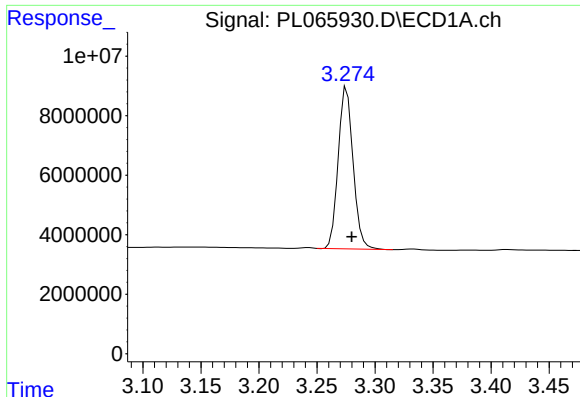

#1 Tetrachloro-m-xylene


R.T.: 3.276 min
Delta R.T.: -0.004 min
Response: 48699000
Conc: 18.69 ng/ml

Instrument :
ECD_L
ClientSampleId :

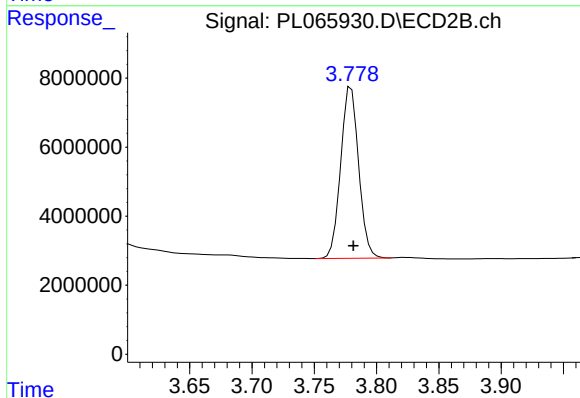


#1 Tetrachloro-m-xylene

R.T.: 3.780 min
Delta R.T.: -0.002 min
Response: 49984470
Conc: 18.21 ng/ml

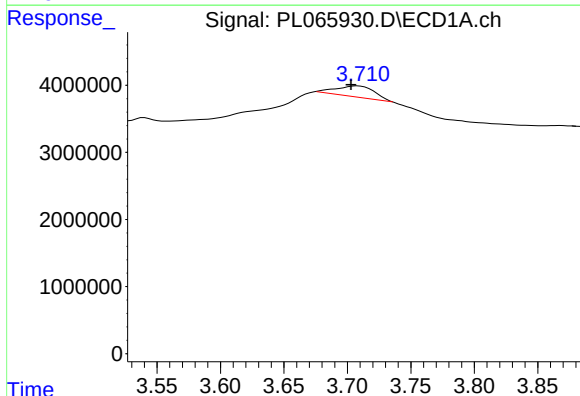


#2 alpha-BHC

R.T.: 3.708 min
Delta R.T.: 0.005 min
Response: 3256083
Conc: 0.80 ng/ml

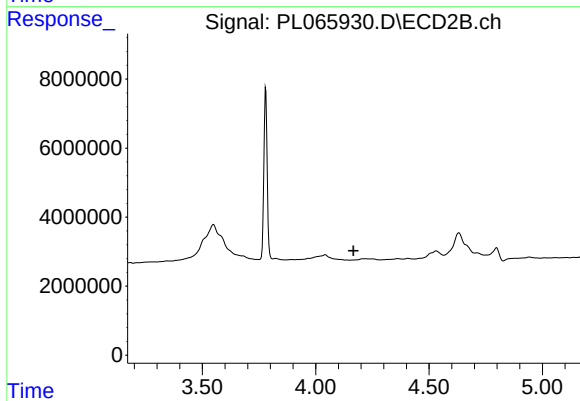

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.167 min
Response: 0
Conc: N.D.

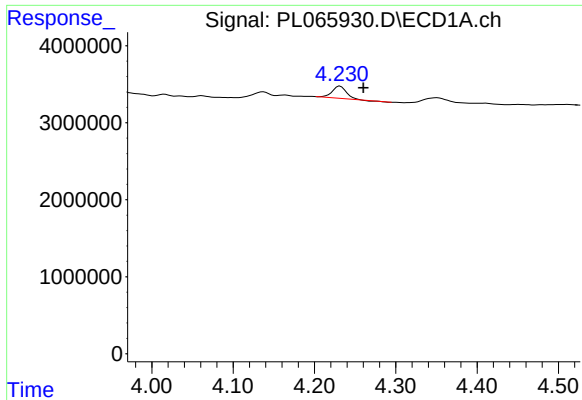

#4 Heptachlor


R.T.: 4.232 min
Delta R.T.: -0.029 min
Response: 1956953
Conc: 0.54 ng/ml

Instrument :
ECD_L
ClientSampleId :

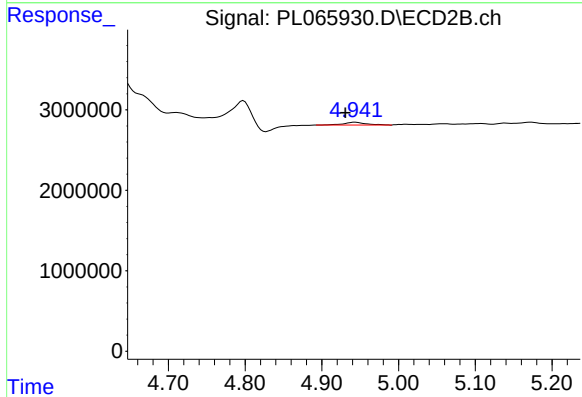


#4 Heptachlor

R.T.: 4.943 min
Delta R.T.: 0.012 min
Response: 730628
Conc: 0.21 ng/ml

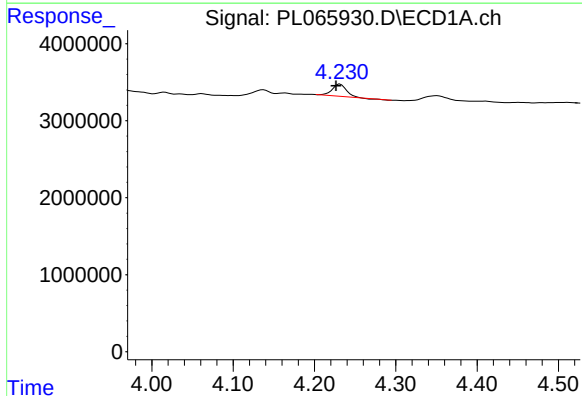


#6 beta-BHC

R.T.: 4.232 min
Delta R.T.: 0.005 min
Response: 1956953
Conc: 1.23 ng/ml

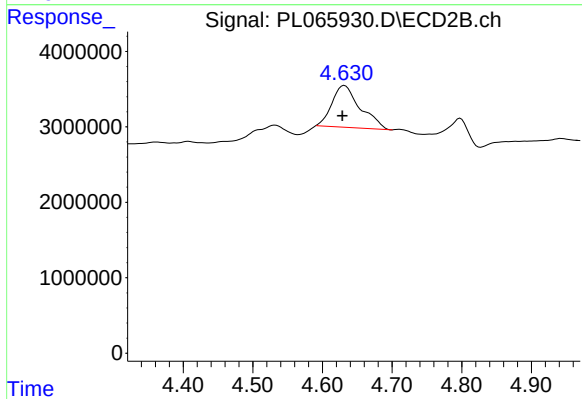

#6 beta-BHC


R.T.: 4.632 min
Delta R.T.: 0.003 min
Response: 15696349
Conc: 9.01 ng/ml

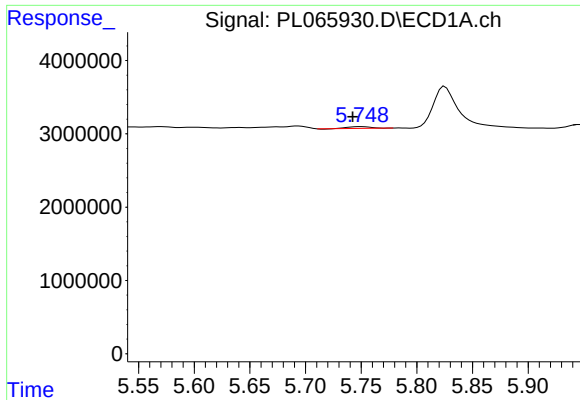

#14 Endrin


R.T.: 5.750 min
Delta R.T.: 0.007 min
Response: 320317
Conc: 0.12 ng/ml

Instrument :
ECD_L
ClientSampleId :

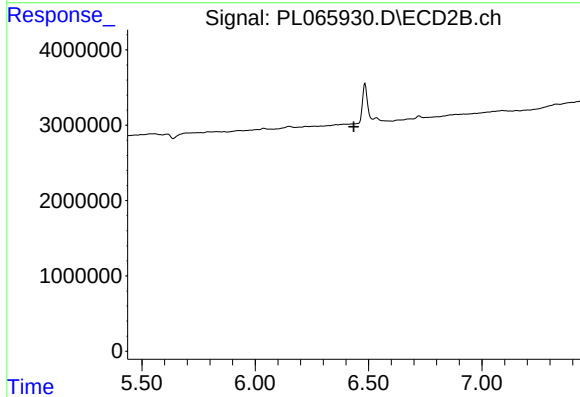


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.434 min
Response: 0
Conc: N.D.

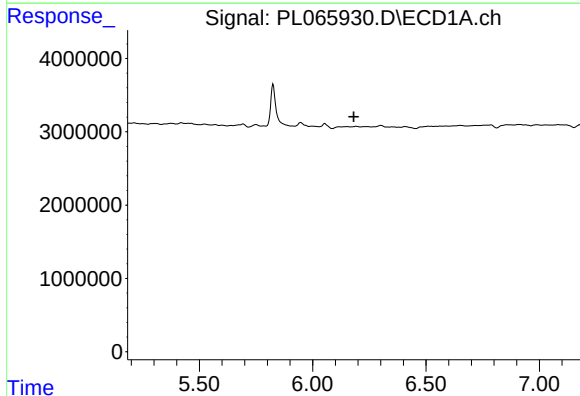


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.181 min
Response: 0
Conc: N.D.

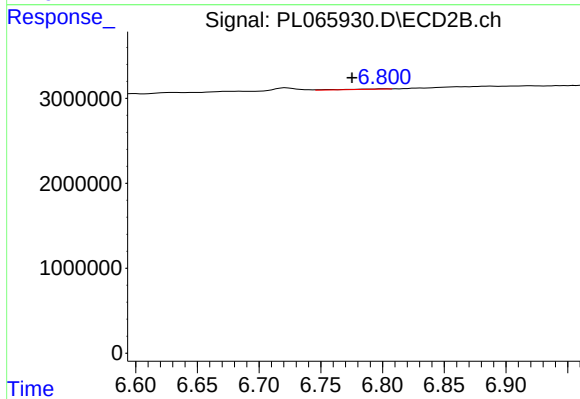

#18 Endrin aldehyde


R.T.: 6.801 min
Delta R.T.: 0.026 min
Response: 122074
Conc: 0.06 ng/ml

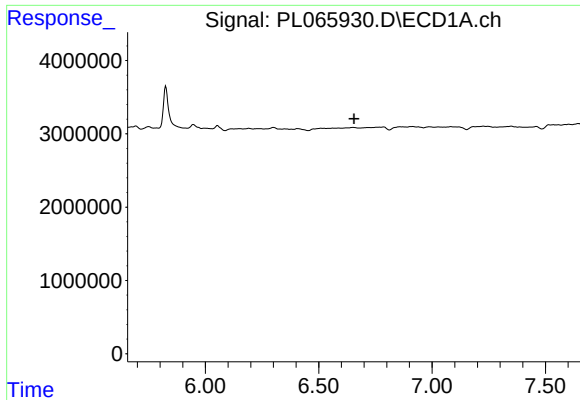

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 6.656 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

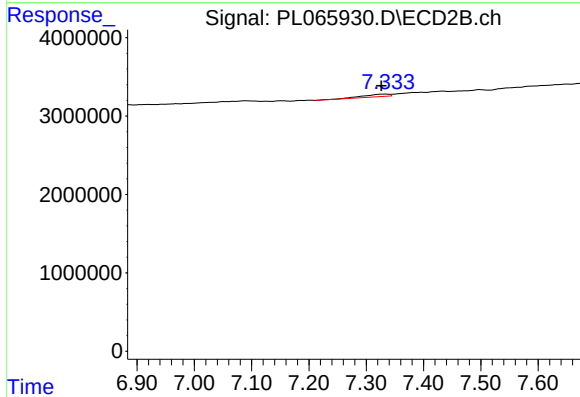


#20 Methoxychlor

R.T.: 7.335 min
Delta R.T.: 0.009 min
Response: 996761
Conc: 0.79 ng/ml

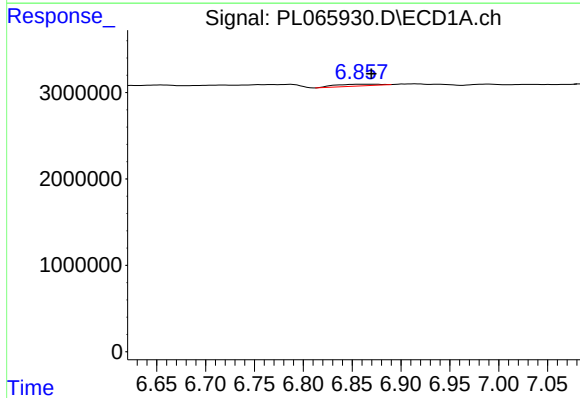


#21 Endrin ketone

R.T.: 6.859 min
Delta R.T.: -0.011 min
Response: 633324
Conc: 0.23 ng/ml

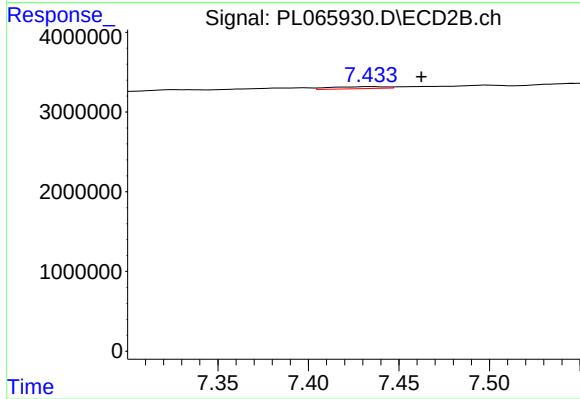

#21 Endrin ketone


R.T.: 7.434 min
Delta R.T.: -0.028 min
Response: 524670
Conc: 0.20 ng/ml

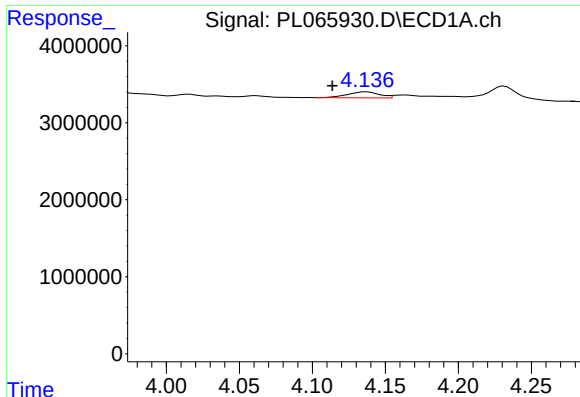

#23 Chlordane-1


R.T.: 4.137 min
Delta R.T.: 0.024 min
Response: 1181257
Conc: 13.09 ng/ml

Instrument :
ECD_L
ClientSampleId :

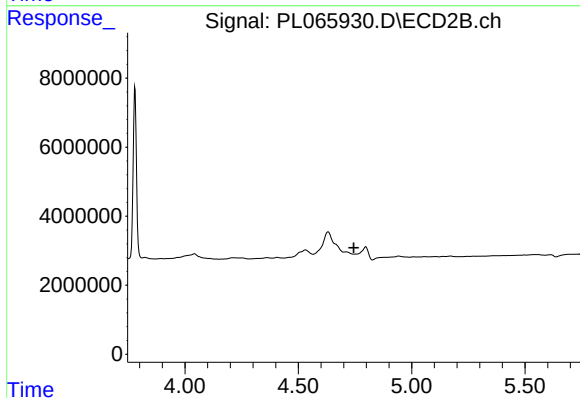


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.745 min
Response: 0
Conc: N.D.

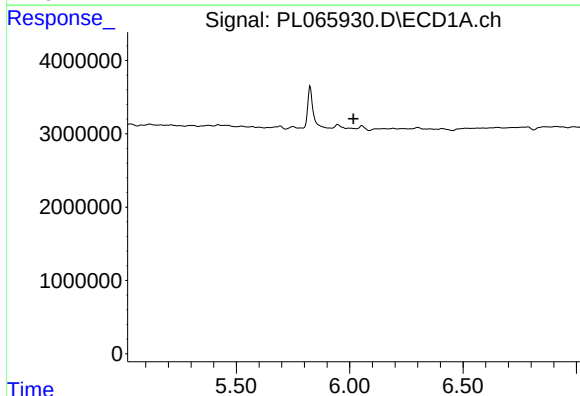


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.017 min
Response: 0
Conc: N.D.

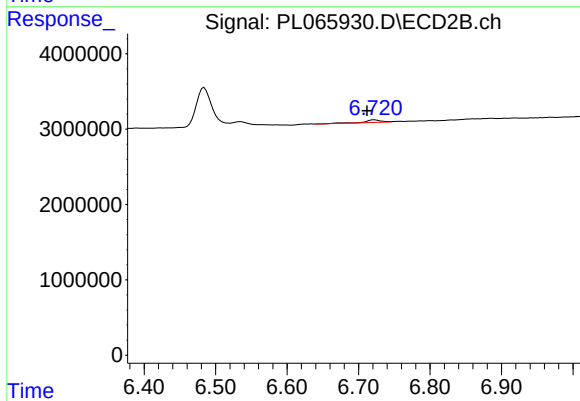

#27 Chlordane-5


R.T.: 6.722 min
Delta R.T.: 0.010 min
Response: 534622
Conc: 6.41 ng/ml

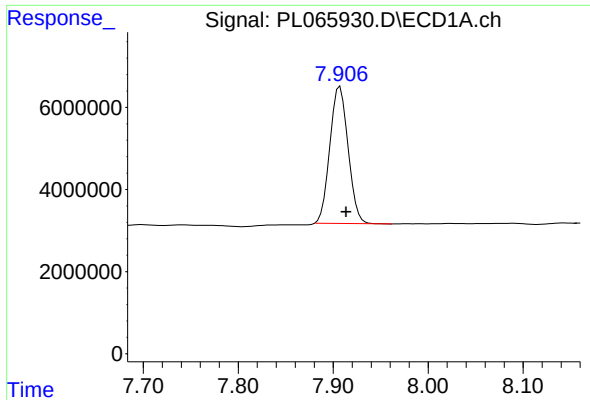

#28 Decachlorobiphenyl

R.T.: 7.907 min
Delta R.T.: -0.006 min
Response: 44551315
Conc: 19.24 ng/ml

Instrument :
ECD_L
ClientSampleId :

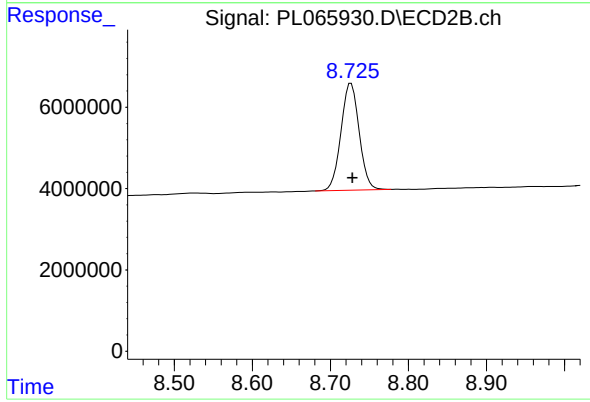

#28 Decachlorobiphenyl

R.T.: 8.726 min
Delta R.T.: -0.002 min
Response: 42475521
Conc: 18.84 ng/ml