

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040721\
 Data File : PL065931.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Apr 2021 09:36
 Operator : AR\AJ
 Sample : PEM
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 08 06:40:58 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 31 15:57:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.276	3.780	50693065	51753278	19.460	18.854
28)	SA Decachlor...	7.906	8.727	46252939	44430725	19.971	19.707
Target Compounds							
2)	A alpha-BHC	3.699	4.164	39010012	37727863	9.538	9.286
3)	MA gamma-BHC...	3.971	4.444	34174149	32826493	9.232	8.966
4)	MA Heptachlor	0.000	4.946	0	624127	N.D.	0.177 #
5)	MB Aldrin	4.500	0.000	323351	0	0.095	N.D. #
6)	B beta-BHC	4.223	4.627	17397741	30969644	10.915	17.780 #
8)	B Heptachlo...	0.000	5.613	0	634913	N.D.	0.204 #
12)	B 4,4'-DDE	5.366	6.077	654414	492690	0.237	0.189
13)	MA Dieldrin	0.000	6.243f	0	1413243	N.D.	0.501 #
14)	MA Endrin	5.736	6.433	126.4E6	114.5E6	46.810	45.966
15)	B Endosulfa...	0.000	6.671f	0	5060425	N.D.	2.141 #
16)	A 4,4'-DDD	5.873	6.567	4847965	3682236	2.137	1.747
17)	MA 4,4'-DDT	6.105	6.860	199.1E6	188.1E6	94.510	84.016
18)	B Endrin al...	6.177	6.774	1474884	871923	0.779	0.460 #
20)	A Methoxychlor	6.650	7.325	276.1E6	259.9E6	219.934	205.226
21)	B Endrin ke...	6.863	7.462	4225133	3746142	1.541	1.457
23)	Chlordane-1	4.111	0.000	771415	0	8.550	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040721\
Data File : PL065931.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Apr 2021 09:36
Operator : AR\AJ
Sample : PEM
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 08 06:40:58 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
Quant Title : GC Extractables
QLast Update : Wed Mar 31 15:57:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

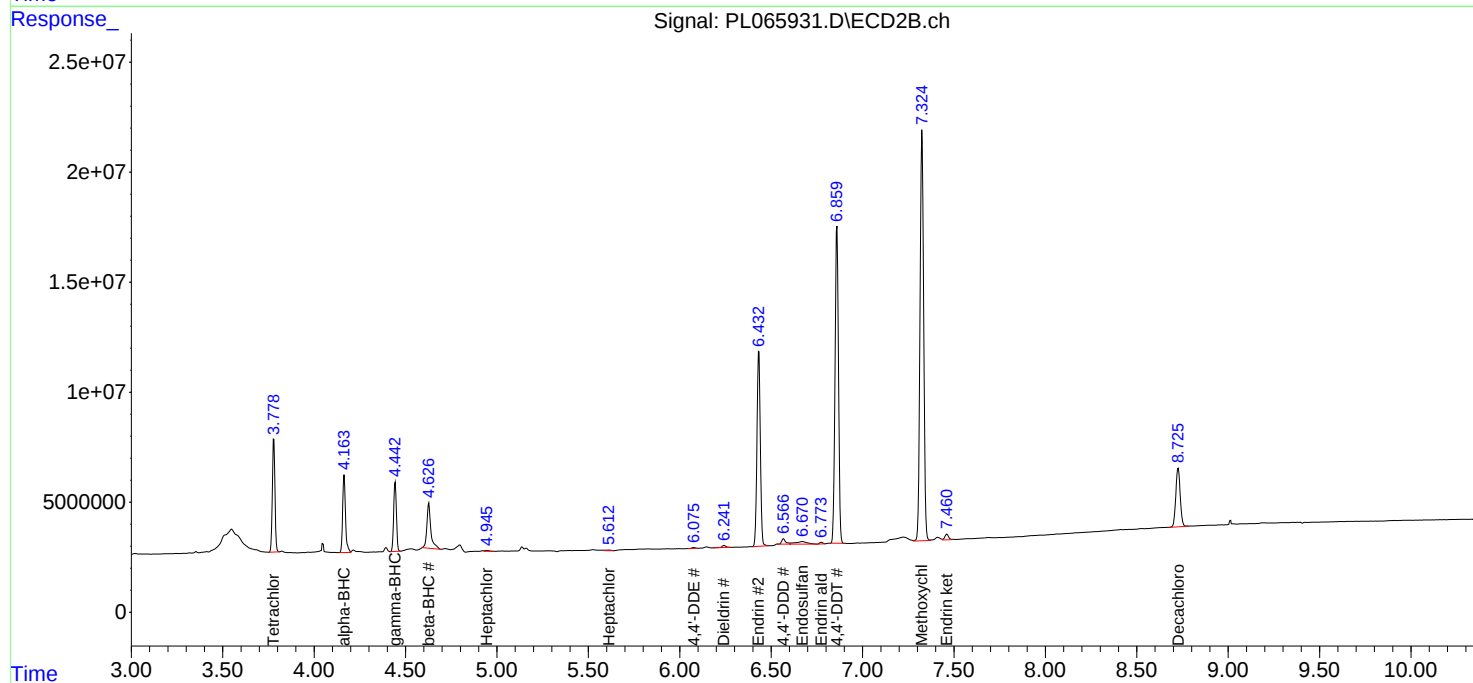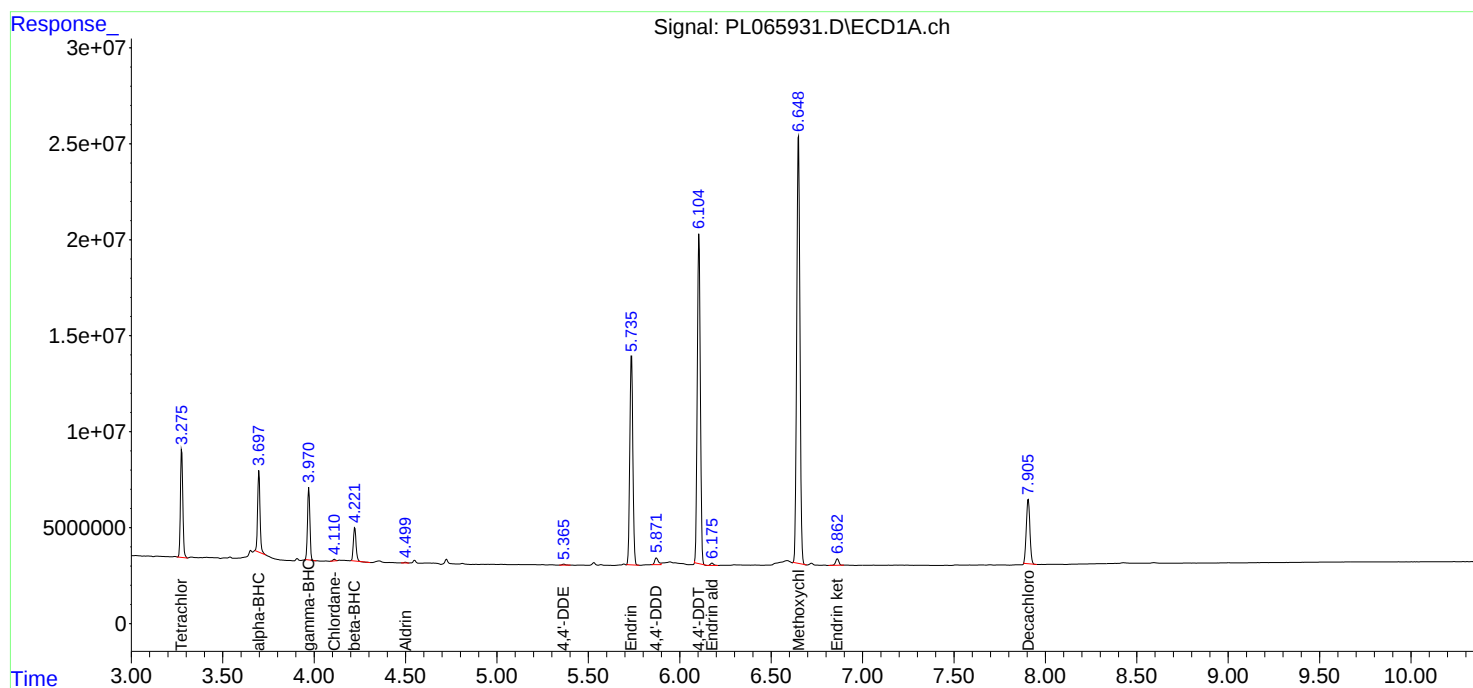


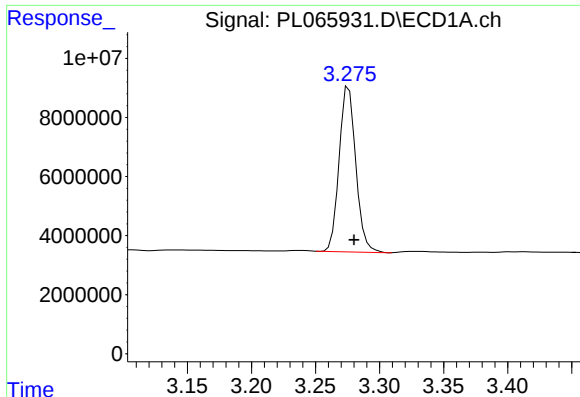

#1 Tetrachloro-m-xylene


R.T.: 3.276 min
Delta R.T.: -0.004 min
Response: 50693065
Conc: 19.46 ng/ml

Instrument :
ECD_L
ClientSampleId :

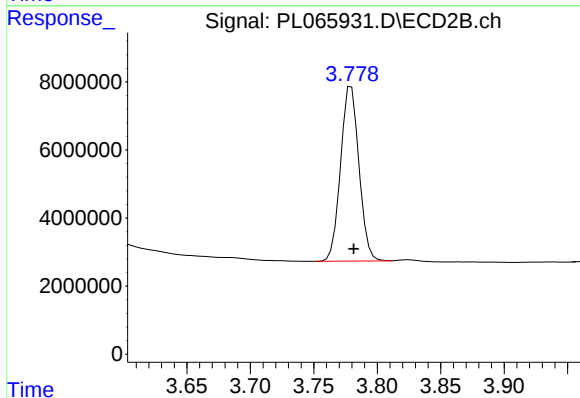


#1 Tetrachloro-m-xylene

R.T.: 3.780 min
Delta R.T.: -0.002 min
Response: 51753278
Conc: 18.85 ng/ml

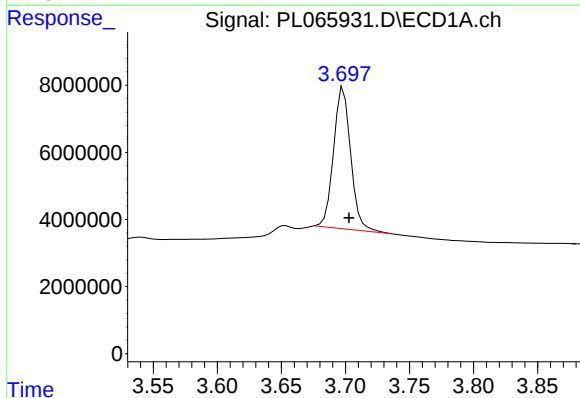


#2 alpha-BHC

R.T.: 3.699 min
Delta R.T.: -0.004 min
Response: 39010012
Conc: 9.54 ng/ml

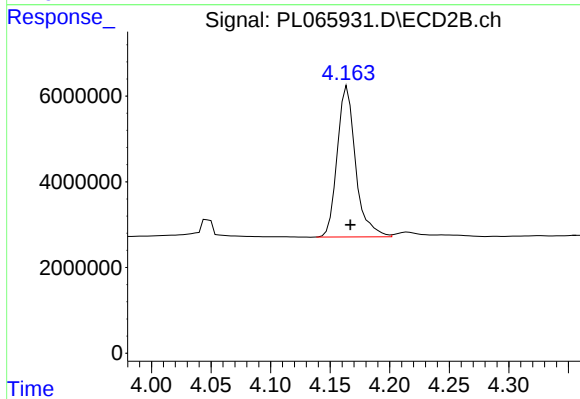

#2 alpha-BHC


R.T.: 4.164 min
Delta R.T.: -0.003 min
Response: 37727863
Conc: 9.29 ng/ml

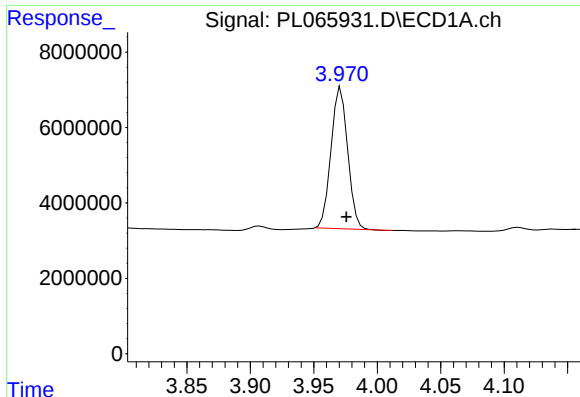

#3 gamma-BHC (Lindane)


R.T.: 3.971 min
Delta R.T.: -0.004 min
Response: 34174149
Conc: 9.23 ng/ml

Instrument :
ECD_L
ClientSampleId :

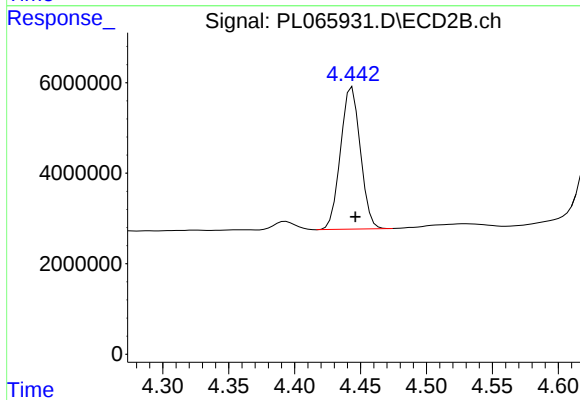


#3 gamma-BHC (Lindane)

R.T.: 4.444 min
Delta R.T.: -0.002 min
Response: 32826493
Conc: 8.97 ng/ml

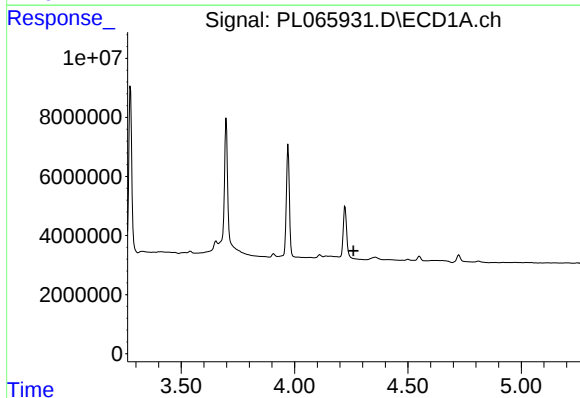


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.260 min
Response: 0
Conc: N.D.

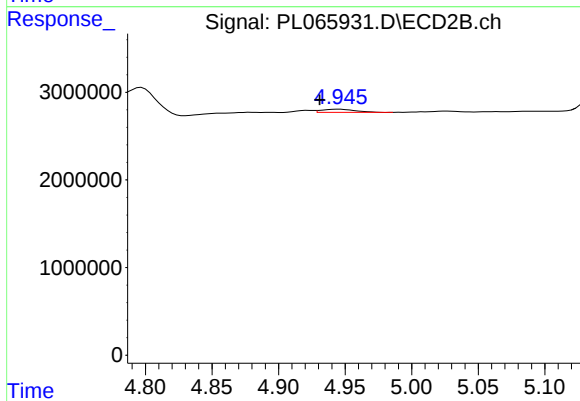

#4 Heptachlor


R.T.: 4.946 min
Delta R.T.: 0.015 min
Response: 624127
Conc: 0.18 ng/ml

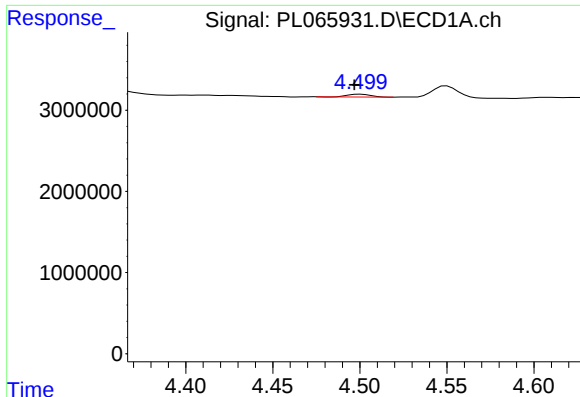

#5 Aldrin


R.T.: 4.500 min
Delta R.T.: 0.003 min
Response: 323351
Conc: 0.09 ng/ml

Instrument :
ECD_L
ClientSampleId :

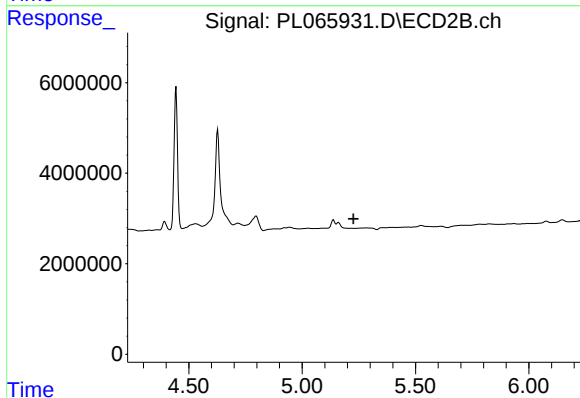


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.227 min
Response: 0
Conc: N.D.

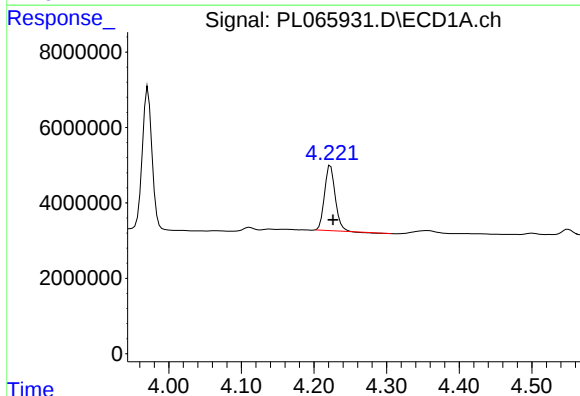


#6 beta-BHC

R.T.: 4.223 min
Delta R.T.: -0.004 min
Response: 17397741
Conc: 10.92 ng/ml

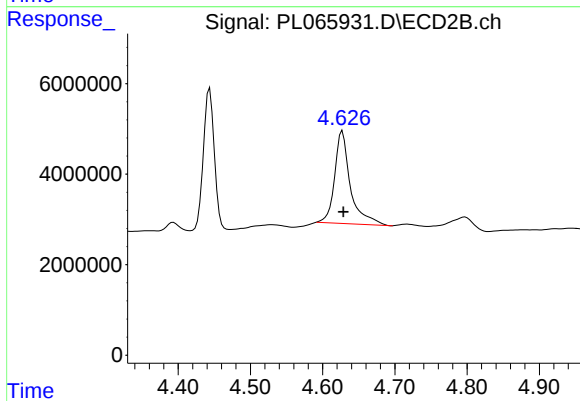

#6 beta-BHC


R.T.: 4.627 min
Delta R.T.: -0.001 min
Response: 30969644
Conc: 17.78 ng/ml

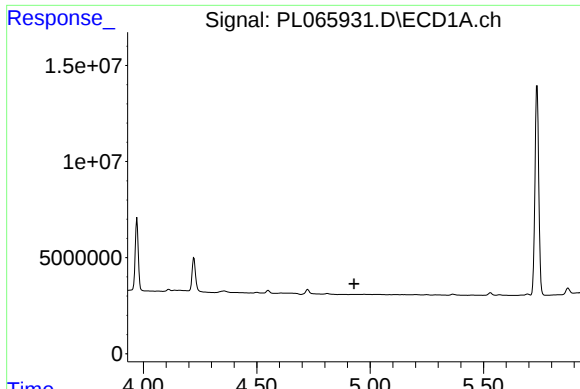

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.929 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

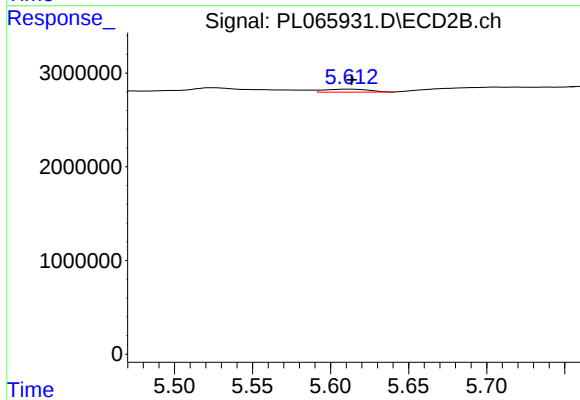


#8 Heptachlor epoxide

R.T.: 5.613 min
Delta R.T.: 0.000 min
Response: 634913
Conc: 0.20 ng/ml

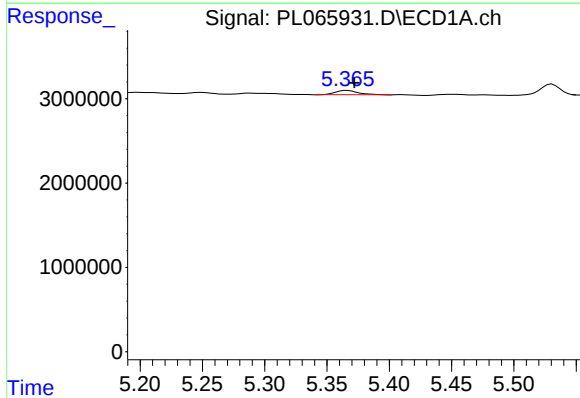


#12 4,4'-DDE

R.T.: 5.366 min
Delta R.T.: -0.006 min
Response: 654414
Conc: 0.24 ng/ml

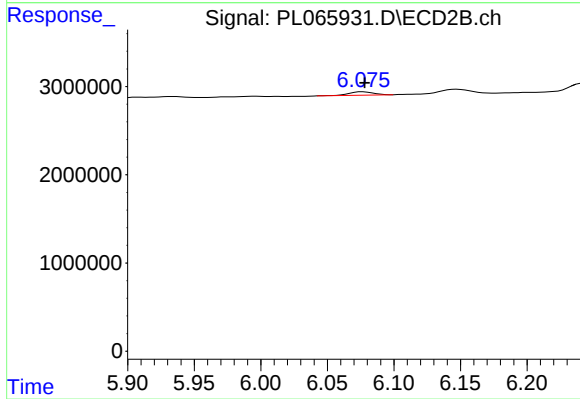

#12 4,4'-DDE


R.T.: 6.077 min
Delta R.T.: -0.001 min
Response: 492690
Conc: 0.19 ng/ml

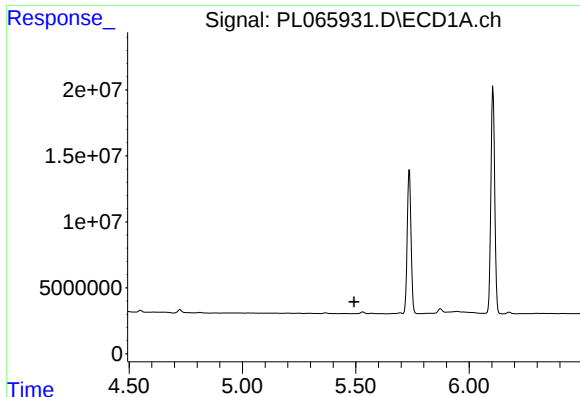

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 5.493 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

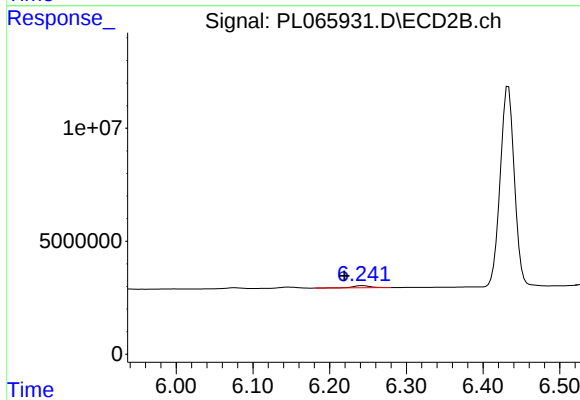


#13 Dieldrin

R.T.: 6.243 min
Delta R.T.: 0.023 min
Response: 1413243
Conc: 0.50 ng/ml

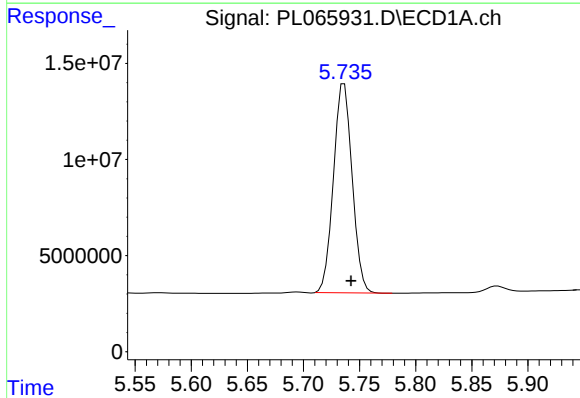


#14 Endrin

R.T.: 5.736 min
Delta R.T.: -0.006 min
Response: 126388095
Conc: 46.81 ng/ml

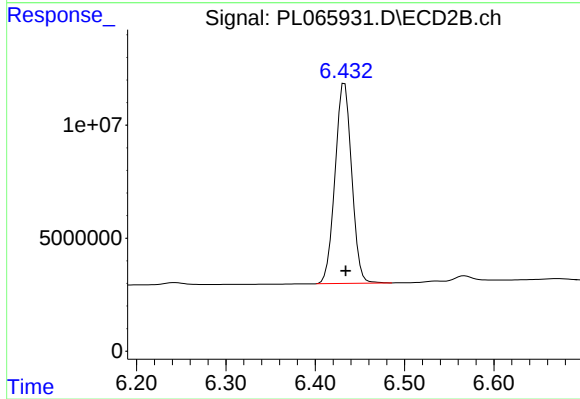

#14 Endrin


R.T.: 6.433 min
Delta R.T.: -0.001 min
Response: 114489907
Conc: 45.97 ng/ml

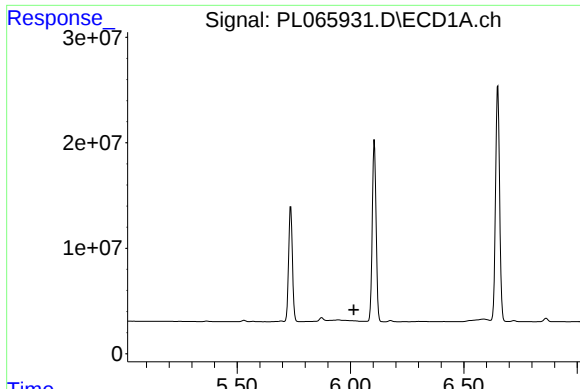

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.015 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

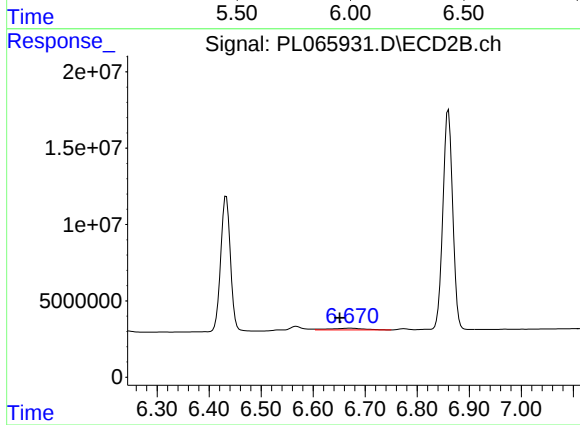


#15 Endosulfan II

R.T.: 6.671 min
Delta R.T.: 0.020 min
Response: 5060425
Conc: 2.14 ng/ml

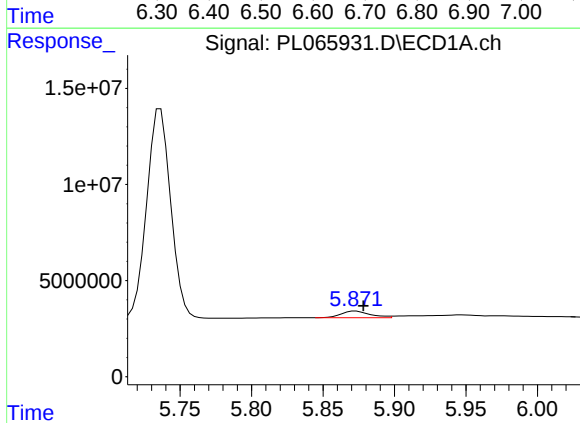


#16 4,4'-DDD

R.T.: 5.873 min
Delta R.T.: -0.005 min
Response: 4847965
Conc: 2.14 ng/ml

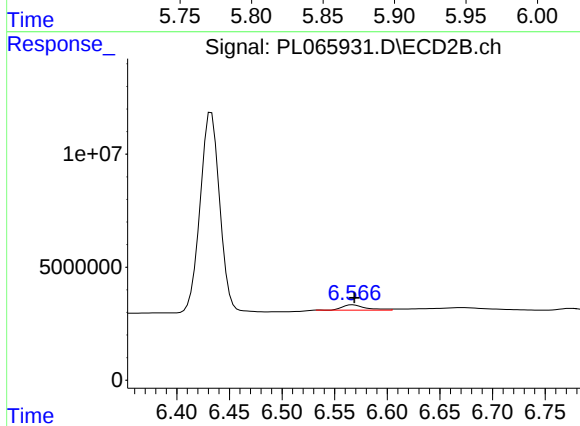

#16 4,4'-DDD


R.T.: 6.567 min
Delta R.T.: -0.001 min
Response: 3682236
Conc: 1.75 ng/ml

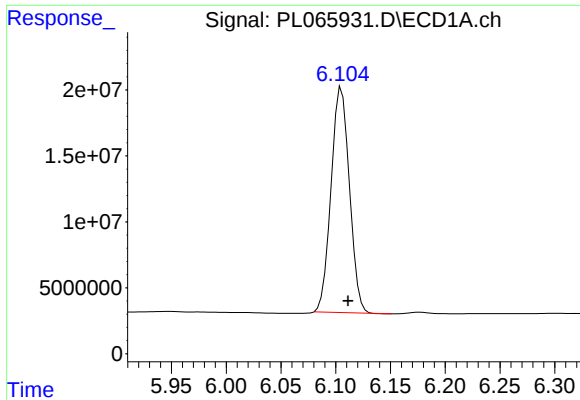

#17 4,4'-DDT


R.T.: 6.105 min
Delta R.T.: -0.006 min
Response: 199115728
Conc: 94.51 ng/ml

Instrument :
ECD_L
ClientSampleId :

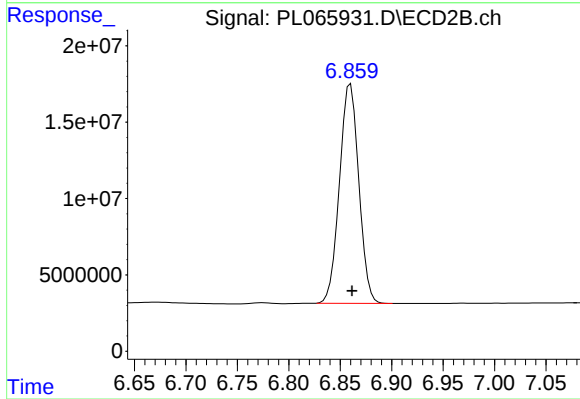


#17 4,4'-DDT

R.T.: 6.860 min
Delta R.T.: -0.001 min
Response: 188118204
Conc: 84.02 ng/ml

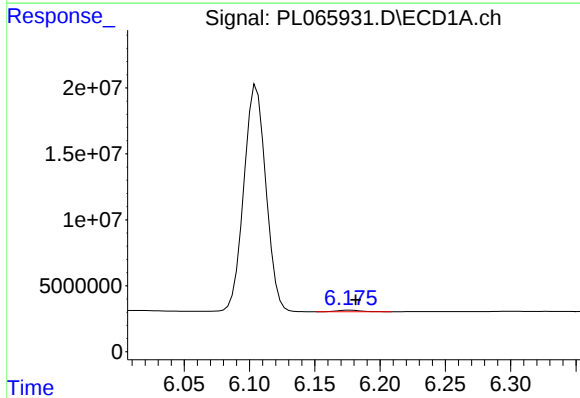


#18 Endrin aldehyde

R.T.: 6.177 min
Delta R.T.: -0.004 min
Response: 1474884
Conc: 0.78 ng/ml

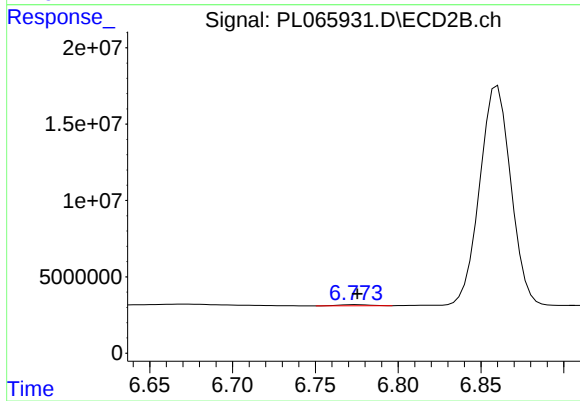

#18 Endrin aldehyde


R.T.: 6.774 min
Delta R.T.: -0.001 min
Response: 871923
Conc: 0.46 ng/ml

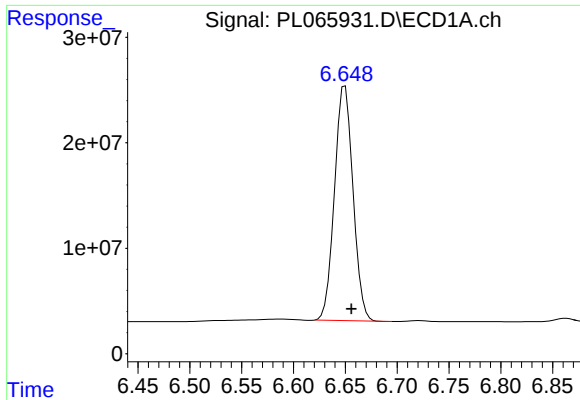

#20 Methoxychlor


R.T.: 6.650 min
Delta R.T.: -0.006 min
Response: 276099887
Conc: 219.93 ng/ml

Instrument :
ECD_L
ClientSampleId :

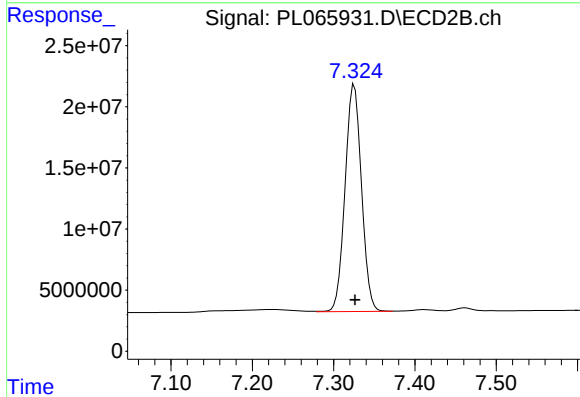


#20 Methoxychlor

R.T.: 7.325 min
Delta R.T.: 0.000 min
Response: 259924013
Conc: 205.23 ng/ml

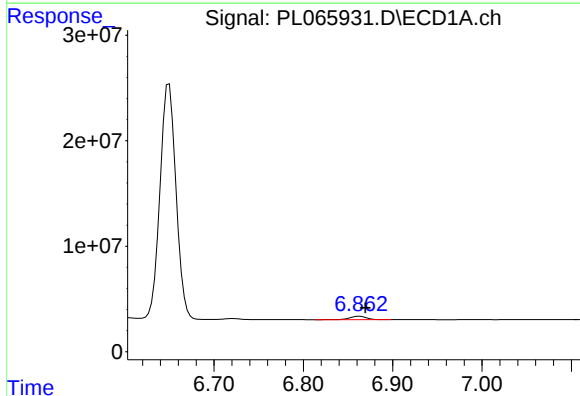


#21 Endrin ketone

R.T.: 6.863 min
Delta R.T.: -0.007 min
Response: 4225133
Conc: 1.54 ng/ml

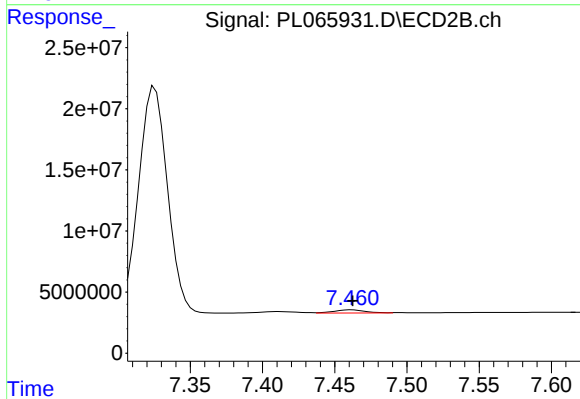

#21 Endrin ketone


R.T.: 7.462 min
Delta R.T.: 0.000 min
Response: 3746142
Conc: 1.46 ng/ml

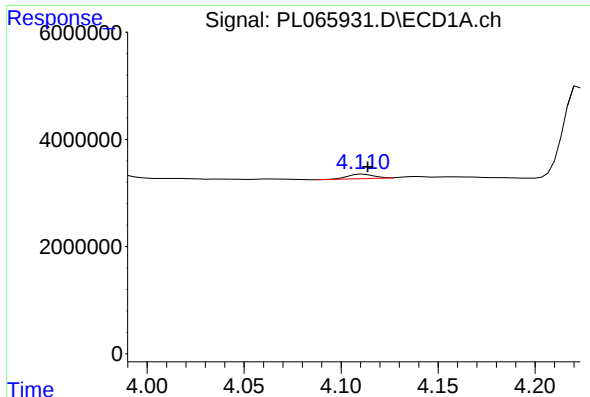

#23 Chlordane-1


R.T.: 4.111 min
Delta R.T.: -0.002 min
Response: 771415
Conc: 8.55 ng/ml

Instrument :
ECD_L
ClientSampleId :

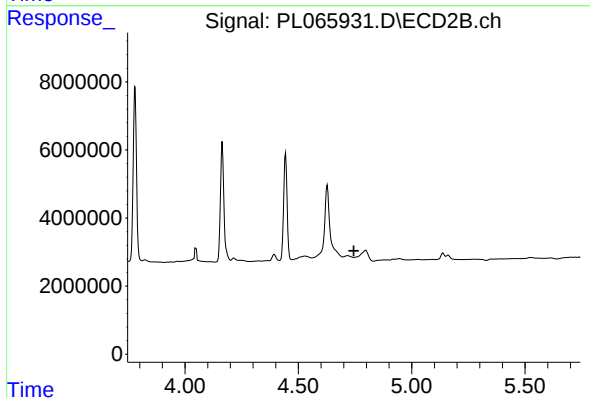


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.745 min
Response: 0
Conc: N.D.

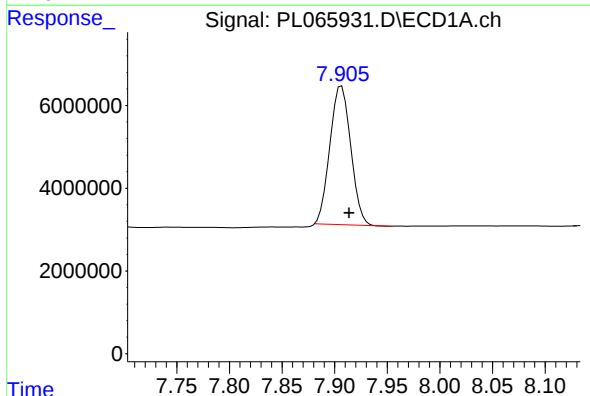

#28 Decachlorobiphenyl

R.T.: 7.906 min
Delta R.T.: -0.007 min
Response: 46252939
Conc: 19.97 ng/ml

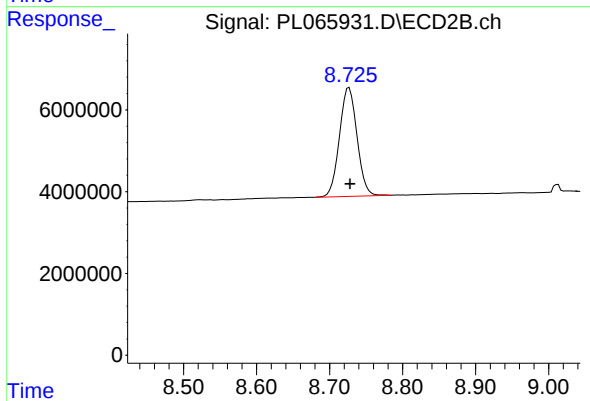

#28 Decachlorobiphenyl

R.T.: 8.727 min
Delta R.T.: -0.002 min
Response: 44430725
Conc: 19.71 ng/ml