

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040721\
 Data File : PL065935.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Apr 2021 11:25
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 08 06:41:44 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 31 15:57:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.276	3.779	48558973	51202013	18.641	18.653
28)	SA Decachlor...	7.906	8.726	45280136	43317287	19.551	19.214
Target Compounds							
4)	MA Heptachlor	4.230f	4.944	1625414	439824	0.451	0.125 #
6)	B beta-BHC	4.230	4.629	1625414	6921929	1.020	3.974 #
8)	B Heptachlo...	0.000	5.612	0	2142161	N.D.	0.690 #
14)	MA Endrin	5.750	0.000	487004	0	0.180	N.D. #
15)	B Endosulfa...	0.000	6.674f	0	507045	N.D.	0.215 #
18)	B Endrin al...	0.000	6.771	0	299968	N.D.	0.158 #
20)	A Methoxychlor	0.000	7.325	0	168051	N.D.	0.133 #
21)	B Endrin ke...	6.860	0.000	801529	0	0.292	N.D. #
23)	Chlordane-1	4.140f	0.000	1039983	0	11.526	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040721\
Data File : PL065935.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Apr 2021 11:25
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 08 06:41:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
Quant Title : GC Extractables
QLast Update : Wed Mar 31 15:57:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

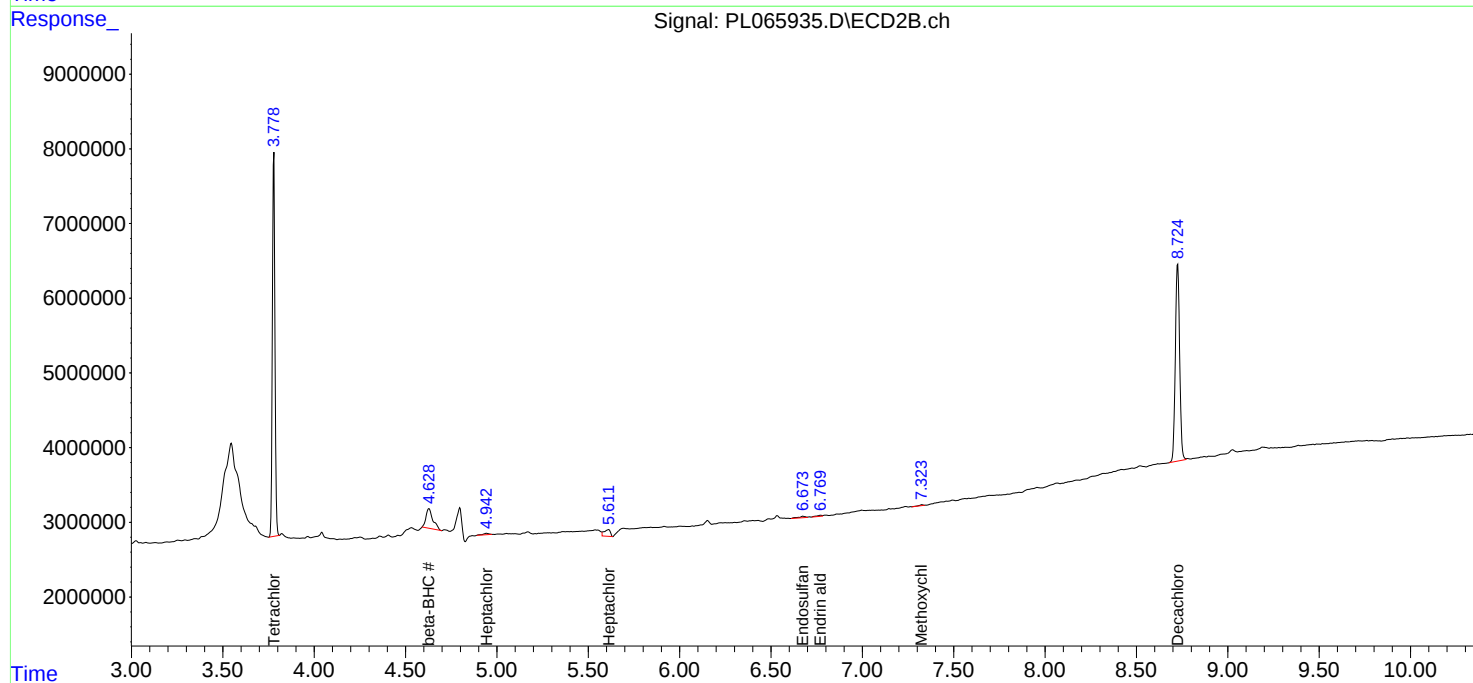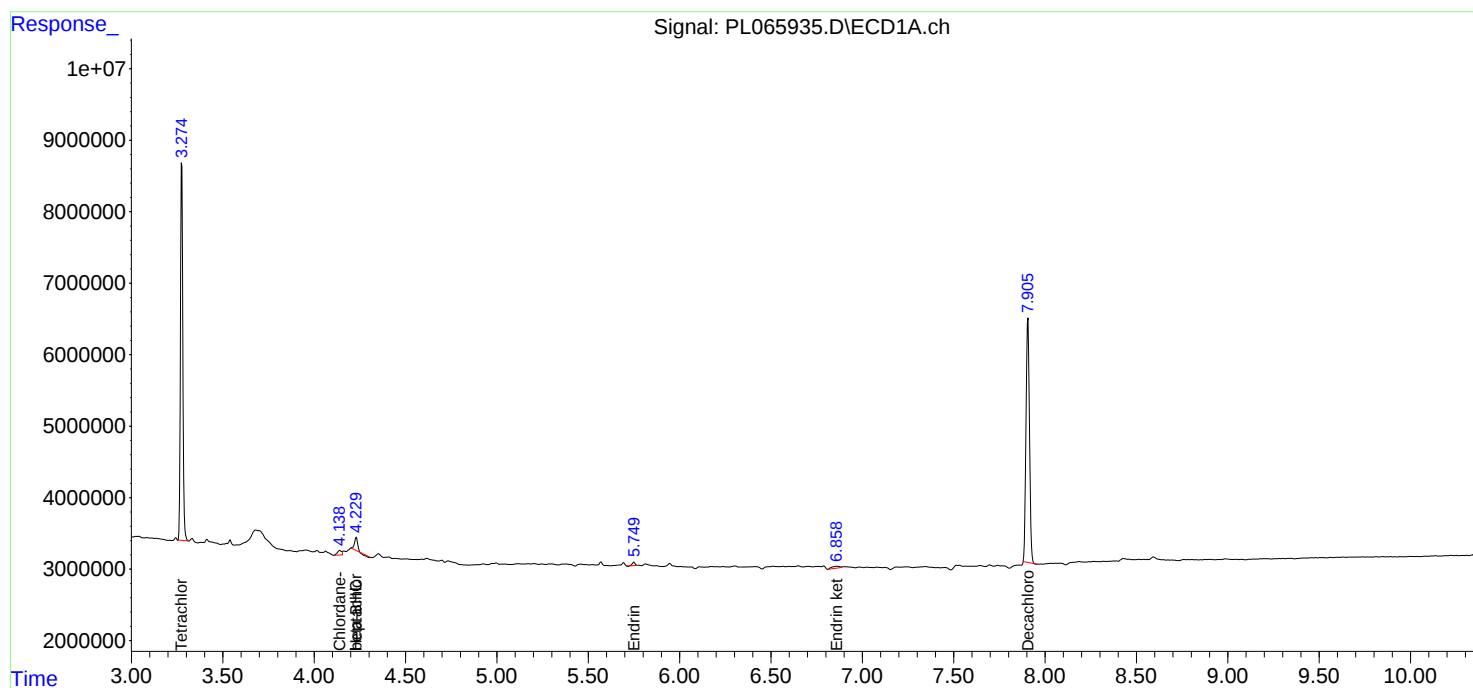


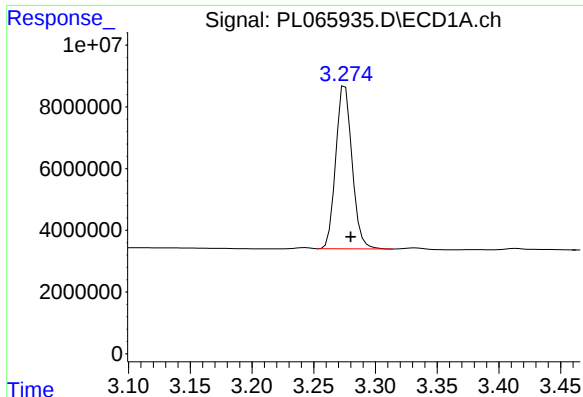

#1 Tetrachloro-m-xylene


R.T.: 3.276 min
Delta R.T.: -0.004 min
Response: 48558973
Conc: 18.64 ng/ml

Instrument :
ECD_L
ClientSampleId :

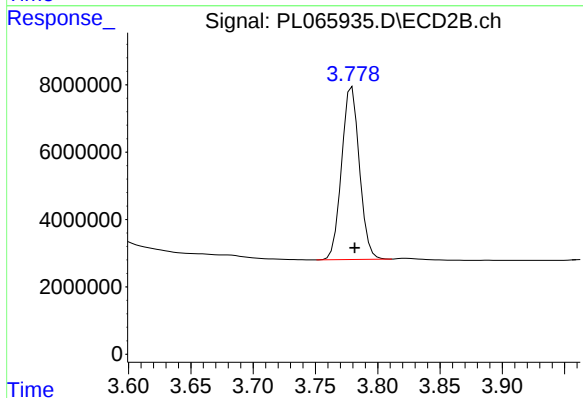


#1 Tetrachloro-m-xylene

R.T.: 3.779 min
Delta R.T.: -0.002 min
Response: 51202013
Conc: 18.65 ng/ml

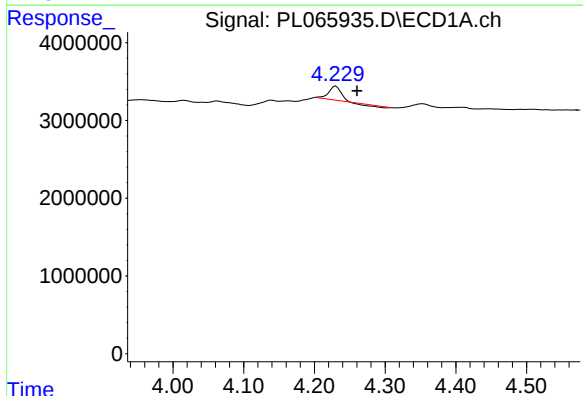


#4 Heptachlor

R.T.: 4.230 min
Delta R.T.: -0.030 min
Response: 1625414
Conc: 0.45 ng/ml

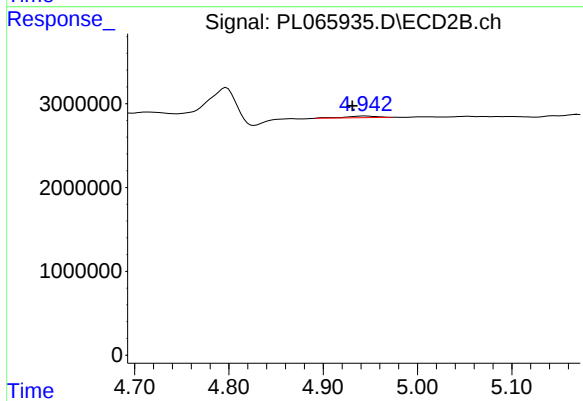

#4 Heptachlor


R.T.: 4.944 min
Delta R.T.: 0.013 min
Response: 439824
Conc: 0.12 ng/ml

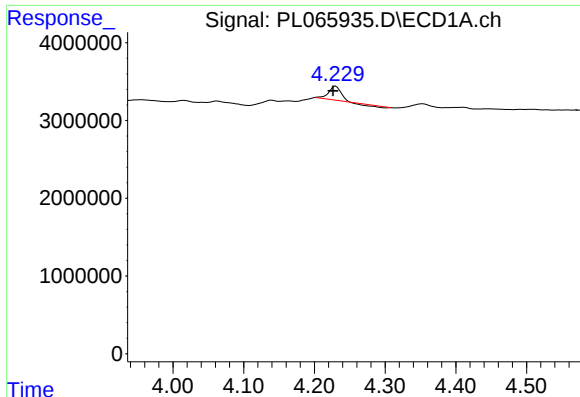

#6 beta-BHC


R.T.: 4.230 min
Delta R.T.: 0.004 min
Response: 1625414
Conc: 1.02 ng/ml

Instrument :
ECD_L
ClientSampleId :

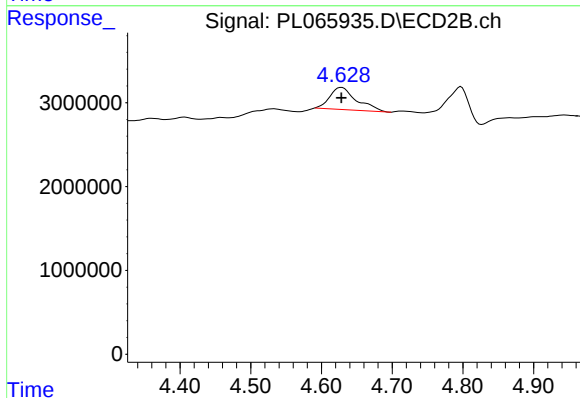


#6 beta-BHC

R.T.: 4.629 min
Delta R.T.: 0.000 min
Response: 6921929
Conc: 3.97 ng/ml

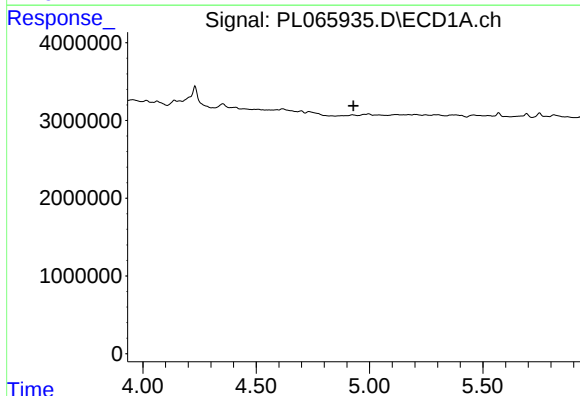


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.929 min
Response: 0
Conc: N.D.

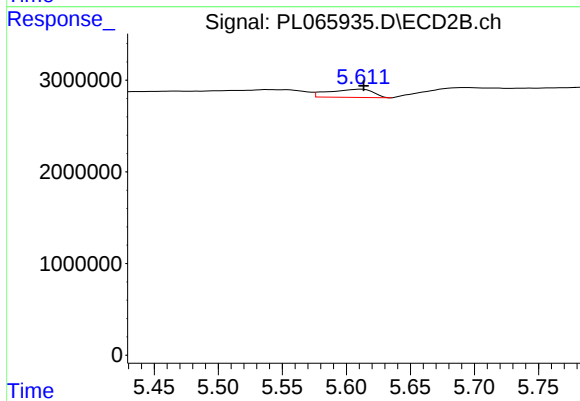

#8 Heptachlor epoxide


R.T.: 5.612 min
Delta R.T.: -0.002 min
Response: 2142161
Conc: 0.69 ng/ml

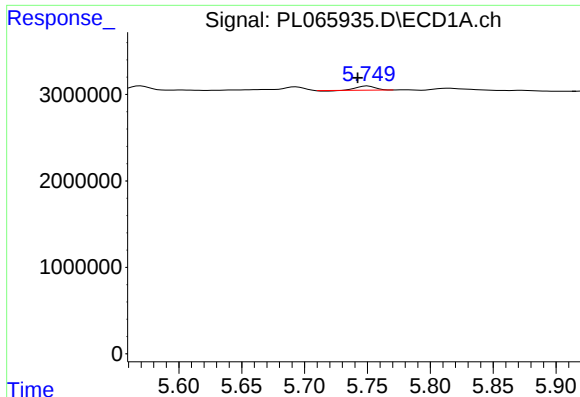

#14 Endrin


R.T.: 5.750 min
Delta R.T.: 0.008 min
Response: 487004
Conc: 0.18 ng/ml

Instrument :
ECD_L
ClientSampleId :

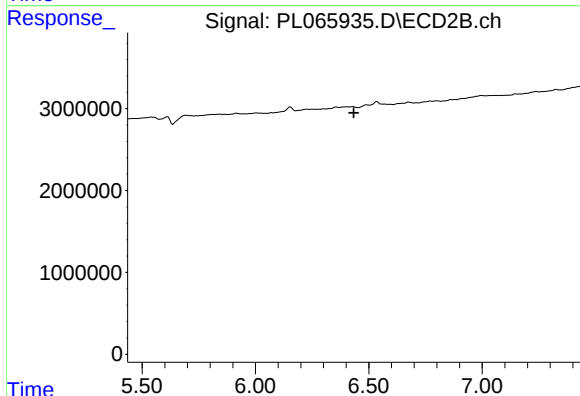


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.434 min
Response: 0
Conc: N.D.

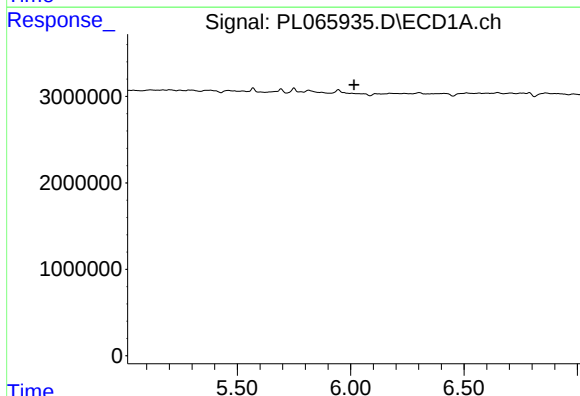


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.015 min
Response: 0
Conc: N.D.

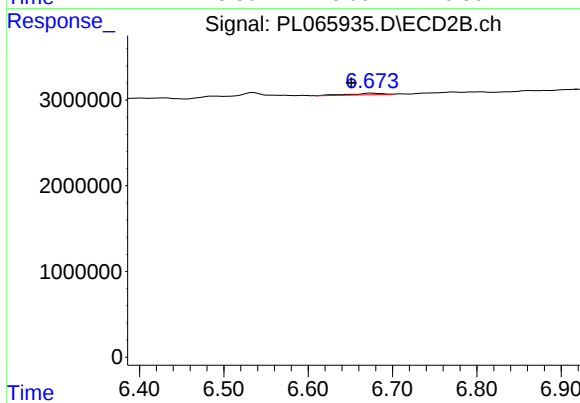

#15 Endosulfan II


R.T.: 6.674 min
Delta R.T.: 0.023 min
Response: 507045
Conc: 0.21 ng/ml

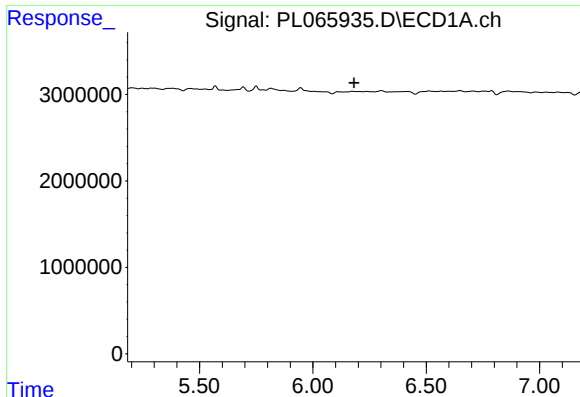

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 6.181 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

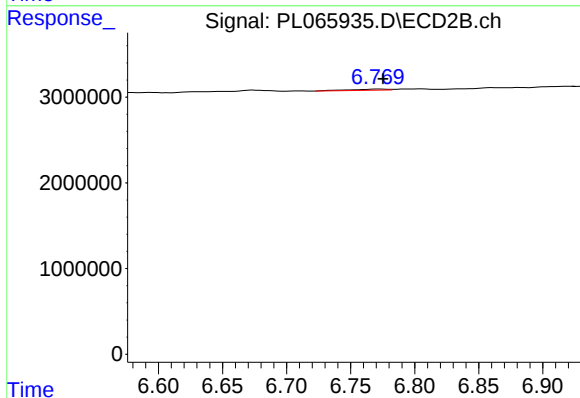


#18 Endrin aldehyde

R.T.: 6.771 min
Delta R.T.: -0.004 min
Response: 299968
Conc: 0.16 ng/ml

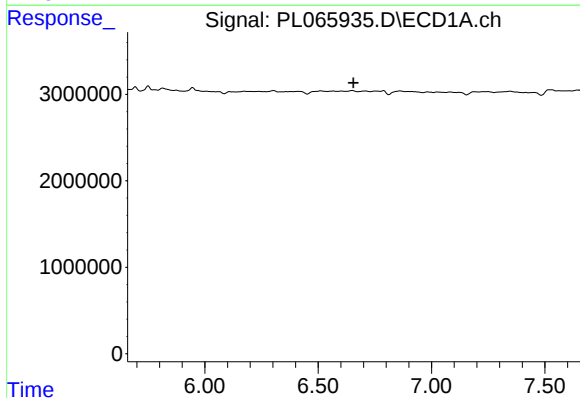


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.656 min
Response: 0
Conc: N.D.

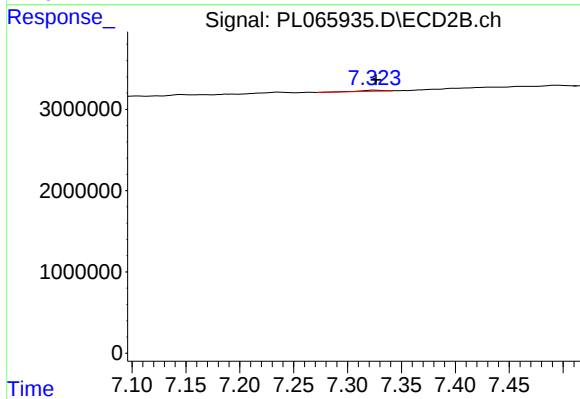

#20 Methoxychlor


R.T.: 7.325 min
Delta R.T.: -0.001 min
Response: 168051
Conc: 0.13 ng/ml

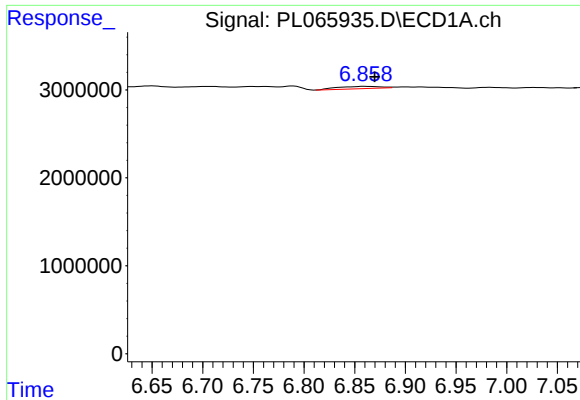

#21 Endrin ketone


R.T.: 6.860 min
Delta R.T.: -0.010 min
Response: 801529
Conc: 0.29 ng/ml

Instrument :
ECD_L
ClientSampleId :

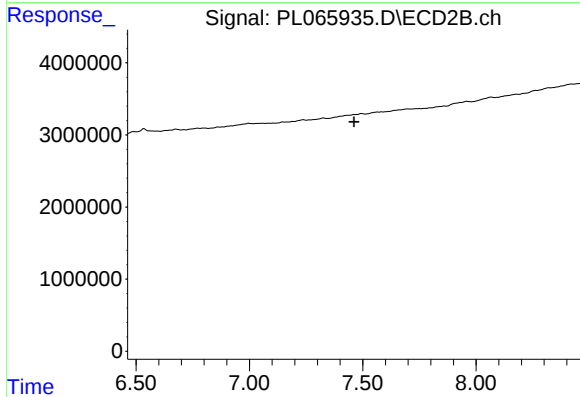


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.462 min
Response: 0
Conc: N.D.

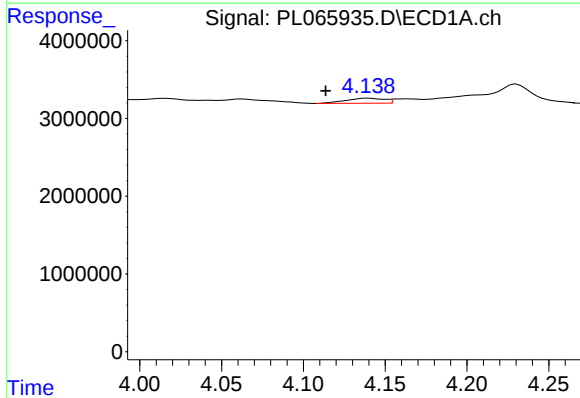


#23 Chlordane-1

R.T.: 4.140 min
Delta R.T.: 0.026 min
Response: 1039983
Conc: 11.53 ng/ml

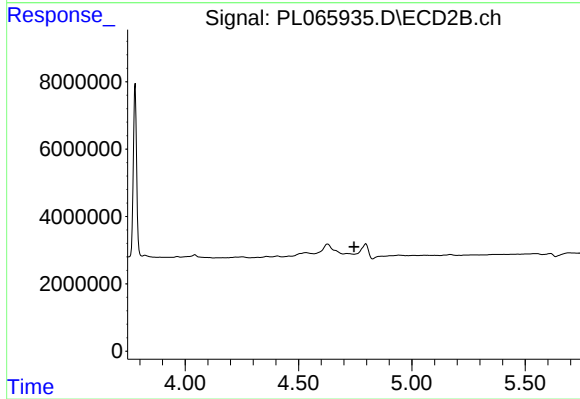

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.745 min
Response: 0
Conc: N.D.

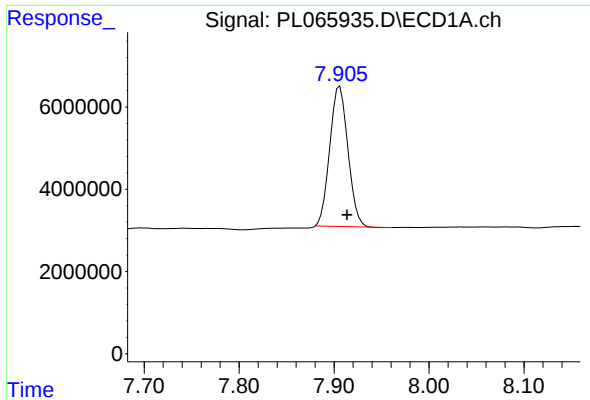

#28 Decachlorobiphenyl

R.T.: 7.906 min
Delta R.T.: -0.008 min
Response: 45280136
Conc: 19.55 ng/ml

Instrument :
ECD_L
ClientSampleId :

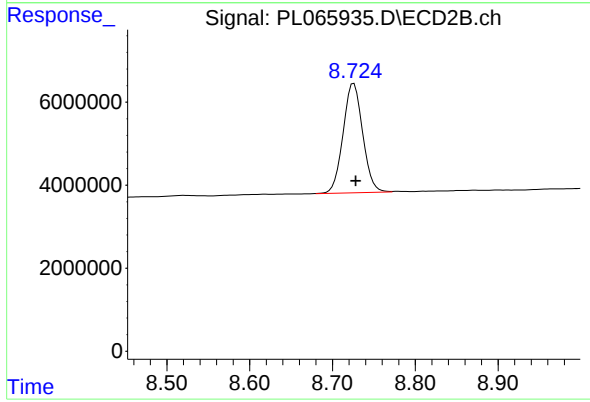

#28 Decachlorobiphenyl

R.T.: 8.726 min
Delta R.T.: -0.002 min
Response: 43317287
Conc: 19.21 ng/ml