

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040725\
 Data File : PL095069.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Apr 2025 19:00
 Operator : AR\AJ
 Sample : Q1730-05
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OU4-VSL-17-040325

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 08 02:21:34 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031125.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 11 17:42:21 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.535	2.769	109.1E6	87663760	38.543	24.561 #
28)	SA Decachlor...	9.051	7.901	56092997	96438566	26.616	23.875
Target Compounds							
15)	B Endosulfa...	6.822f	5.923	9296362	7399646	3.424	1.710 #
23)	Chlordane-1	0.000	3.800f	0	12367477	N.D.	81.887 #
27)	Chlordane-5	0.000	5.923	0	7399646	N.D.	38.573 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040725\
Data File : PL095069.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Apr 2025 19:00
Operator : AR\AJ
Sample : Q1730-05
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
OU4-VSL-17-040325

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 08 02:21:34 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031125.M
Quant Title : GC Extractables
QLast Update : Tue Mar 11 17:42:21 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

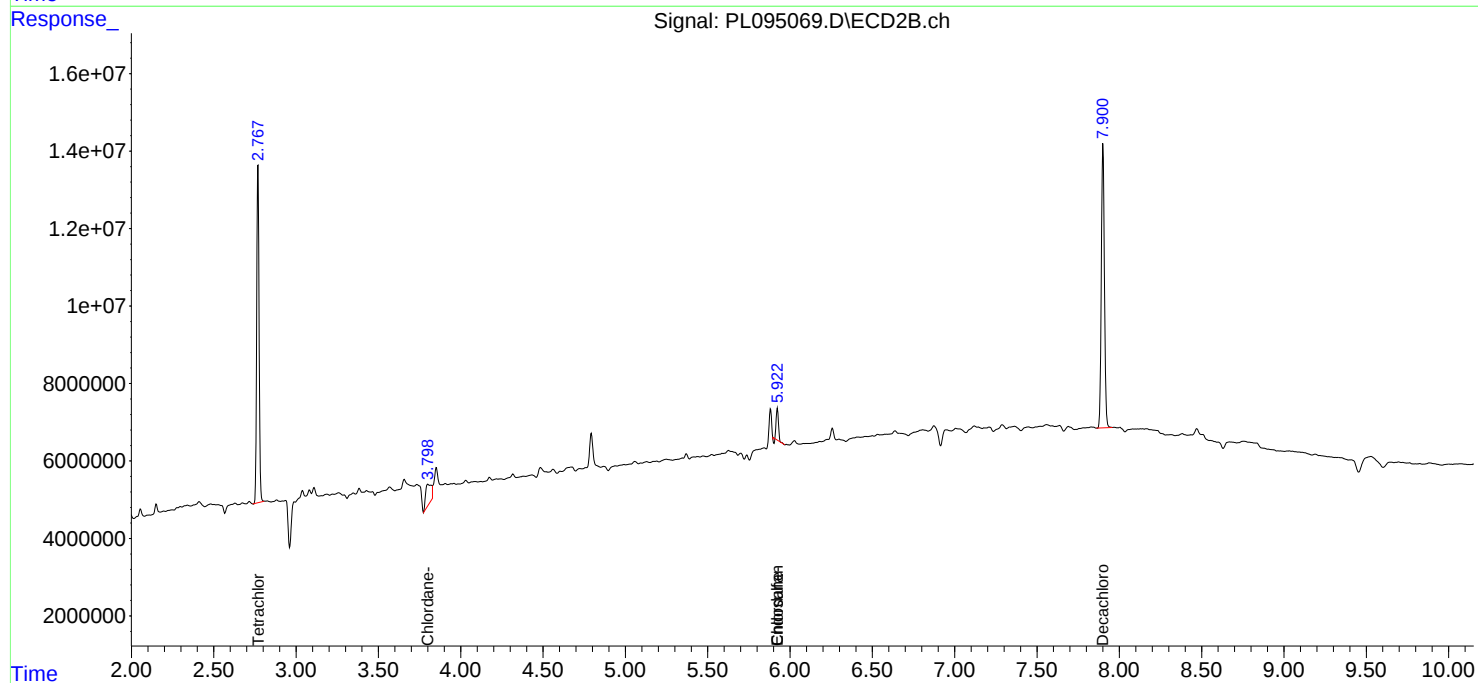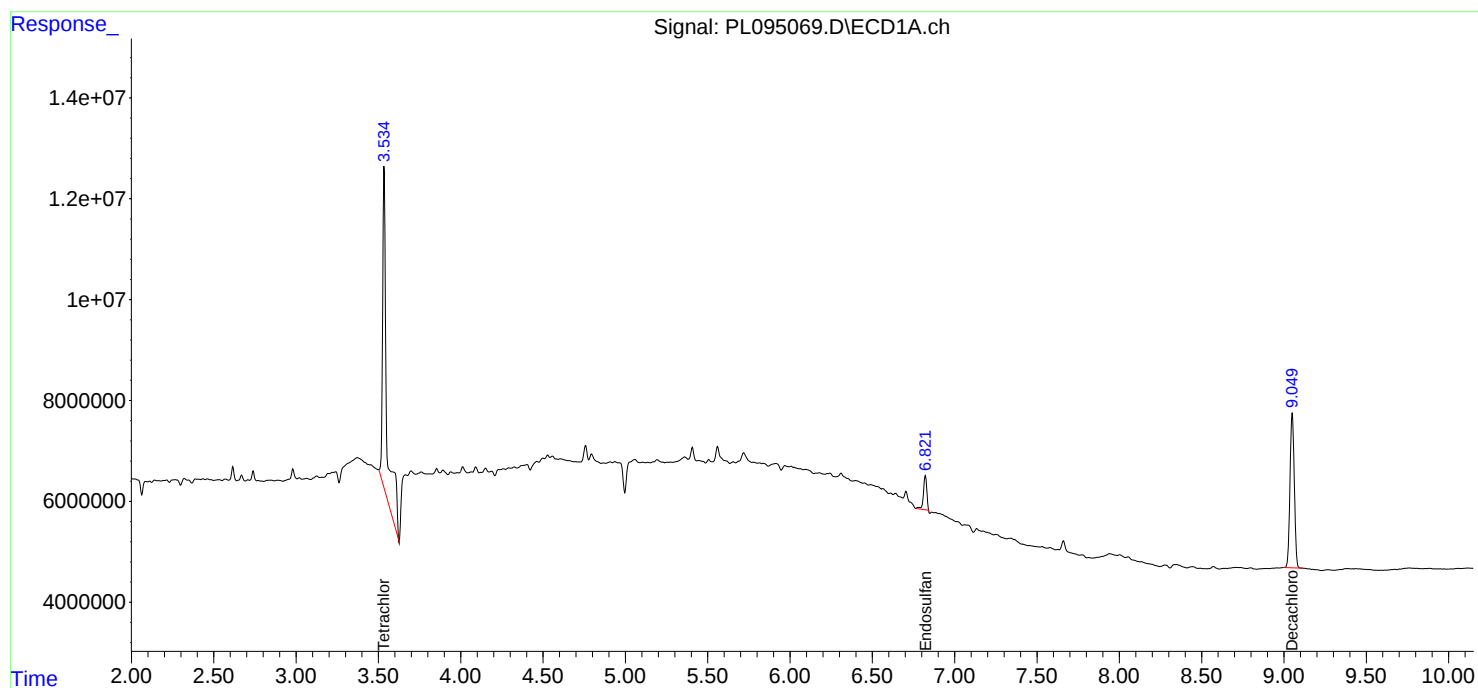


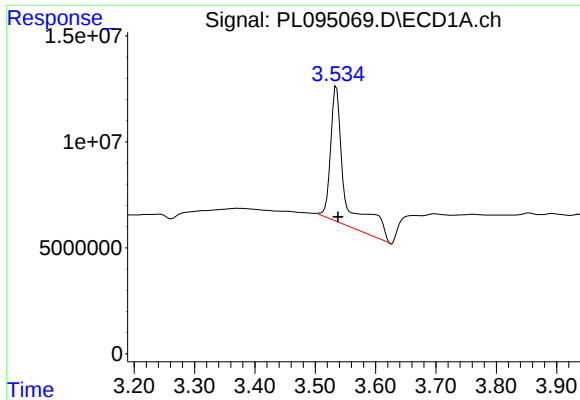

#1 Tetrachloro-m-xylene


R.T.: 3.535 min
Delta R.T.: -0.003 min
Response: 109103629
Conc: 38.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
OU4-VSL-17-040325

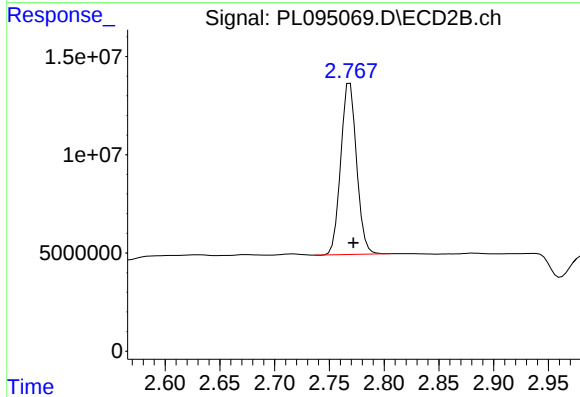


#1 Tetrachloro-m-xylene

R.T.: 2.769 min
Delta R.T.: -0.003 min
Response: 87663760
Conc: 24.56 ng/ml

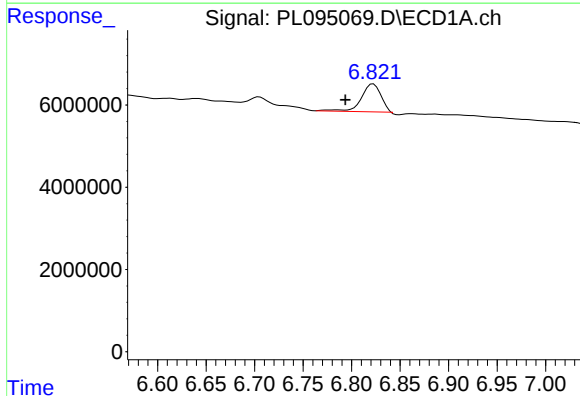


#15 Endosulfan II

R.T.: 6.822 min
Delta R.T.: 0.029 min
Response: 9296362
Conc: 3.42 ng/ml

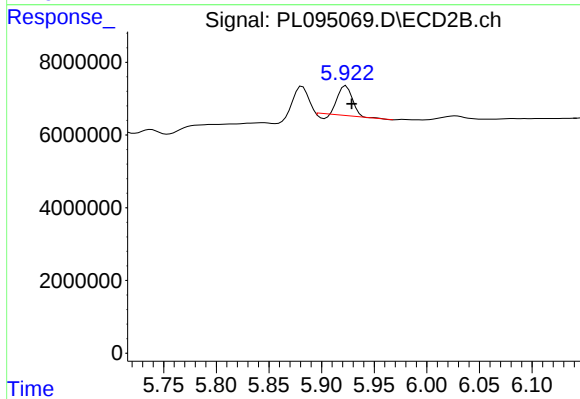

#15 Endosulfan II


R.T.: 5.923 min
Delta R.T.: -0.005 min
Response: 7399646
Conc: 1.71 ng/ml

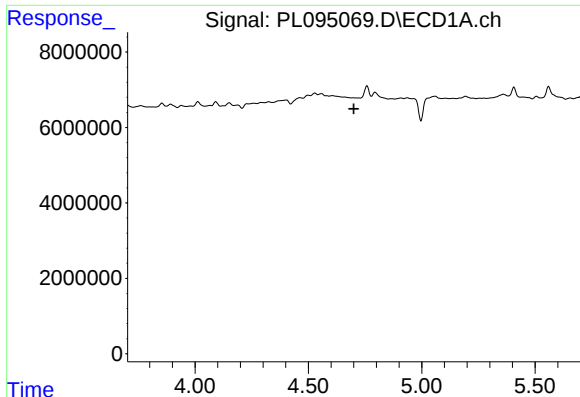

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.700 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
OU4-VSL-17-040325

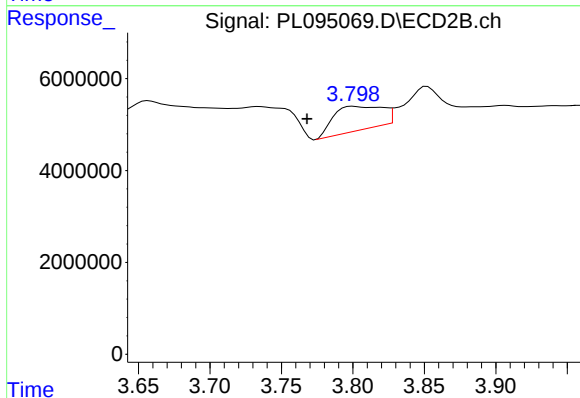


#23 Chlordane-1

R.T.: 3.800 min
Delta R.T.: 0.032 min
Response: 12367477
Conc: 81.89 ng/ml

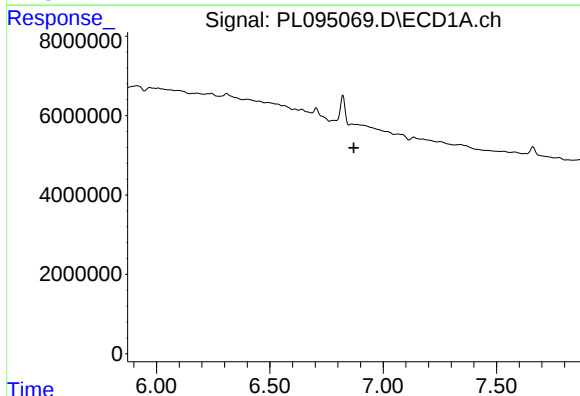


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.871 min
Response: 0
Conc: N.D.

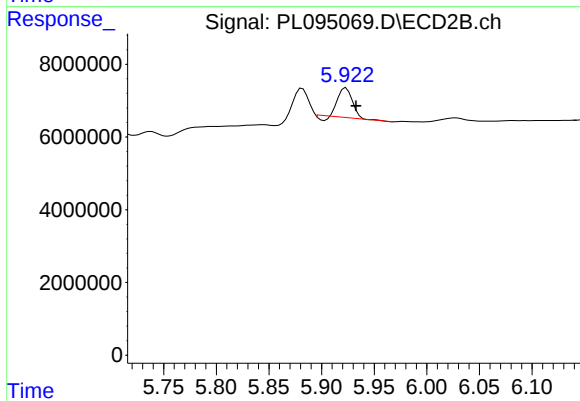

#27 Chlordane-5


R.T.: 5.923 min
Delta R.T.: -0.010 min
Response: 7399646
Conc: 38.57 ng/ml

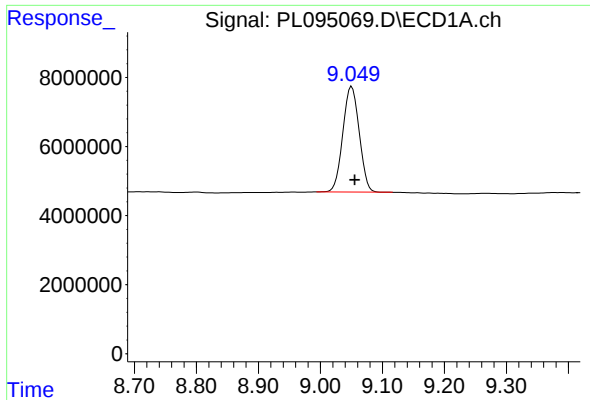

#28 Decachlorobiphenyl

R.T.: 9.051 min
Delta R.T.: -0.005 min
Response: 56092997
Conc: 26.62 ng/ml

Instrument :
ECD_L
ClientSampleId :
OU4-VSL-17-040325

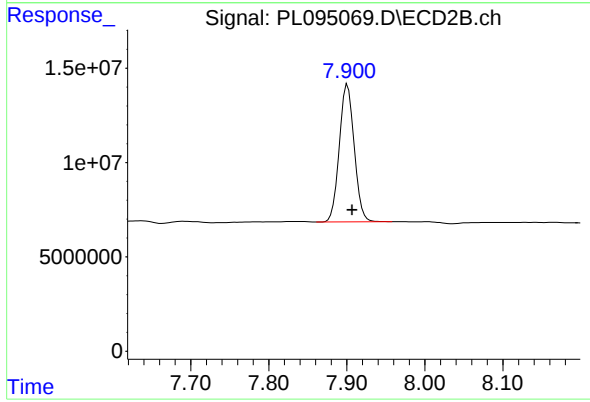

#28 Decachlorobiphenyl

R.T.: 7.901 min
Delta R.T.: -0.006 min
Response: 96438566
Conc: 23.87 ng/ml