

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040819\
 Data File : PL047095.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Apr 2019 14:50
 Operator : AJ\SJ
 Sample : K2294-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-14-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 09 01:02:45 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:40:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.359	3.978	65687965	22951350	9.030	10.024
28)	SA Decachlor...	8.039	9.034	68802273	22349327	8.180	9.640
Target Compounds							
12)	B 4,4'-DDE	0.000	6.311	0	2054773	N.D.	0.828 #
16)	A 4,4'-DDD	0.000	6.808	0	2919164	N.D.	1.451 #
17)	MA 4,4'-DDT	6.218	0.000	4587471	0	0.606	N.D. #
23)	Chlordane-1	4.212	0.000	6100600	0	18.141	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040819\
Data File : PL047095.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Apr 2019 14:50
Operator : AJ\SJ
Sample : K2294-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-14-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 09 01:02:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

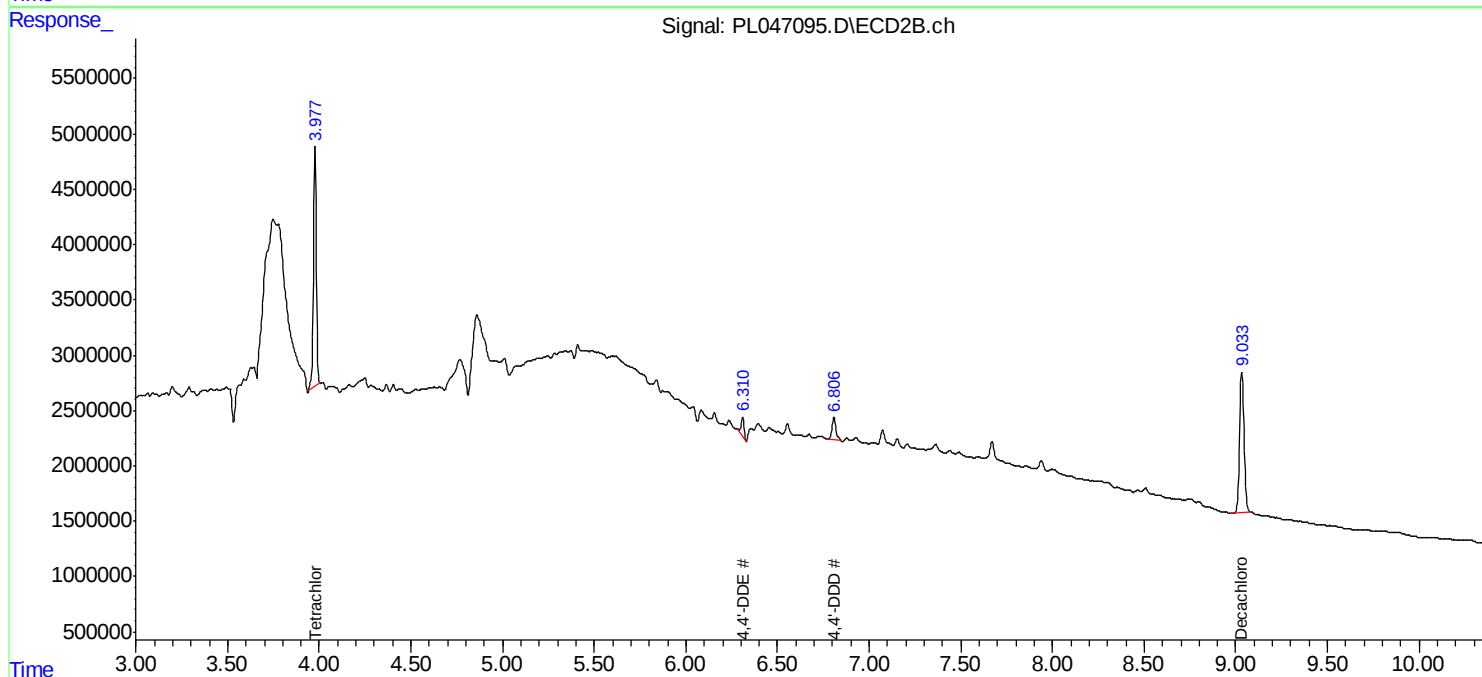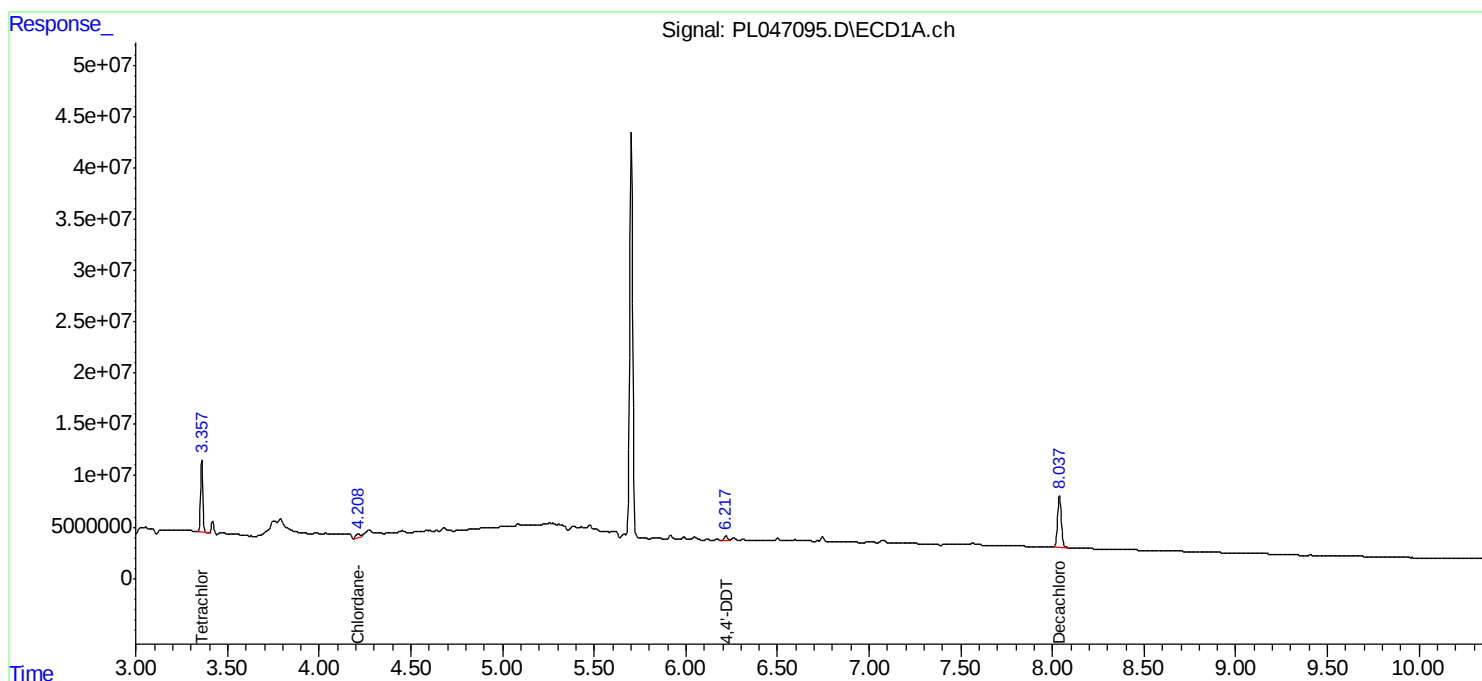


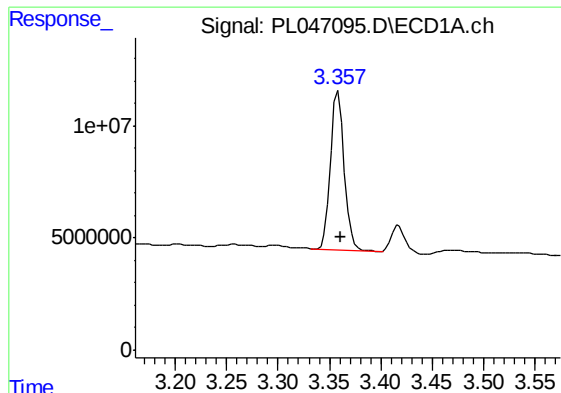

#1 Tetrachloro-m-xylene


R.T.: 3.359 min
Delta R.T.: -0.002 min
Response: 65687965
Conc: 9.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-14-S

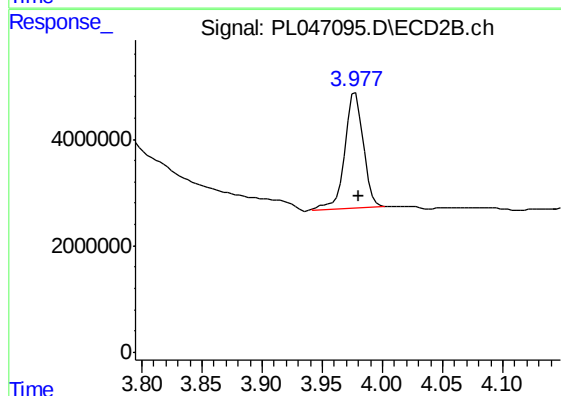


#1 Tetrachloro-m-xylene

R.T.: 3.978 min
Delta R.T.: -0.003 min
Response: 22951350
Conc: 10.02 ng/ml

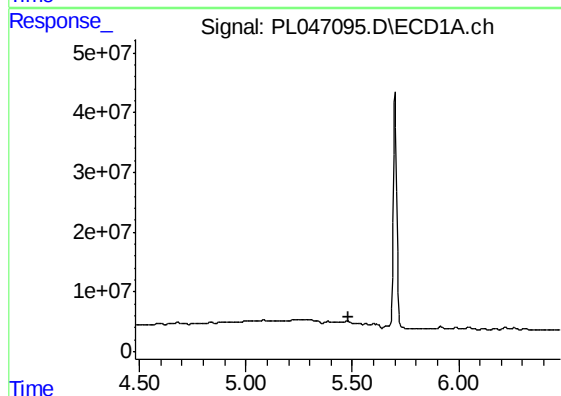


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 5.481 min
Response: 0
Conc: N.D.

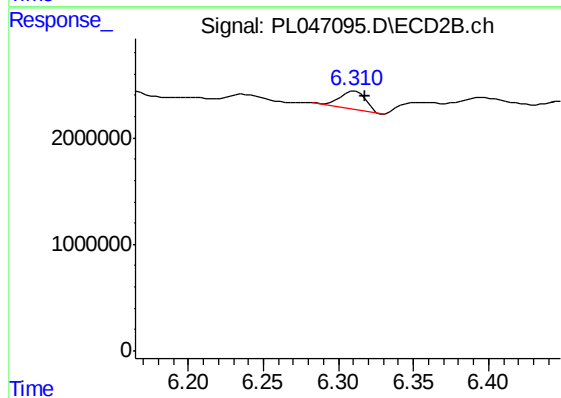

#12 4,4'-DDE


R.T.: 6.311 min
Delta R.T.: -0.007 min
Response: 2054773
Conc: 0.83 ng/ml

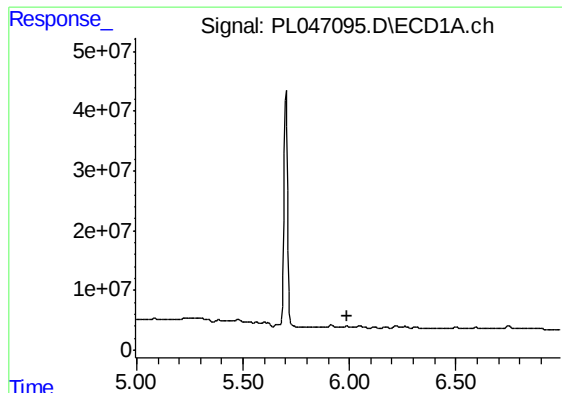

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 5.993 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-14-S

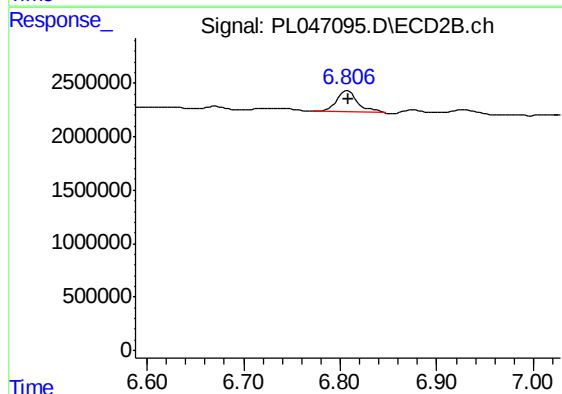


#16 4,4'-DDD

R.T.: 6.808 min
Delta R.T.: -0.001 min
Response: 2919164
Conc: 1.45 ng/ml

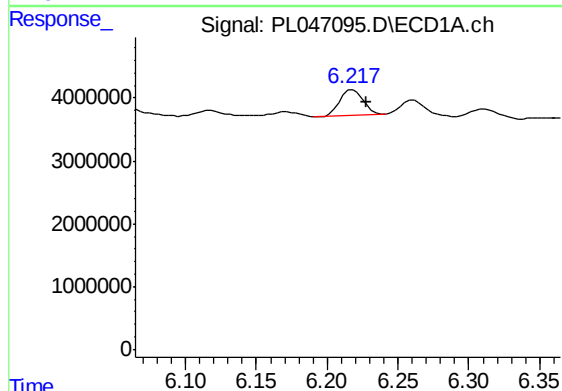


#17 4,4'-DDT

R.T.: 6.218 min
Delta R.T.: -0.009 min
Response: 4587471
Conc: 0.61 ng/ml

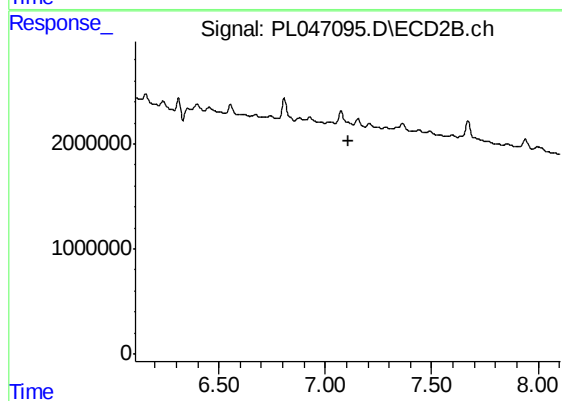

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 7.107 min
Response: 0
Conc: N.D.

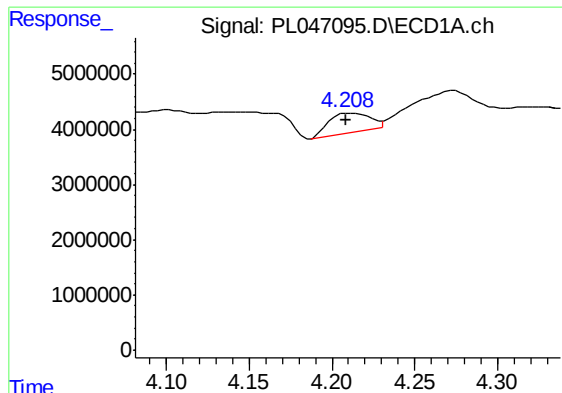

#23 Chlordane-1


R.T.: 4.212 min
Delta R.T.: 0.003 min
Response: 6100600
Conc: 18.14 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-14-S

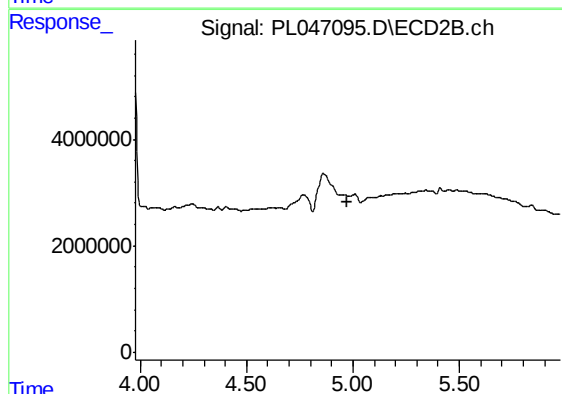


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.975 min
Response: 0
Conc: N.D.

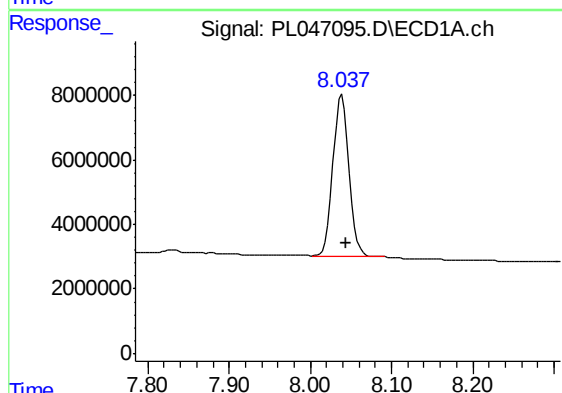

#28 Decachlorobiphenyl

R.T.: 8.039 min
Delta R.T.: -0.006 min
Response: 68802273
Conc: 8.18 ng/ml

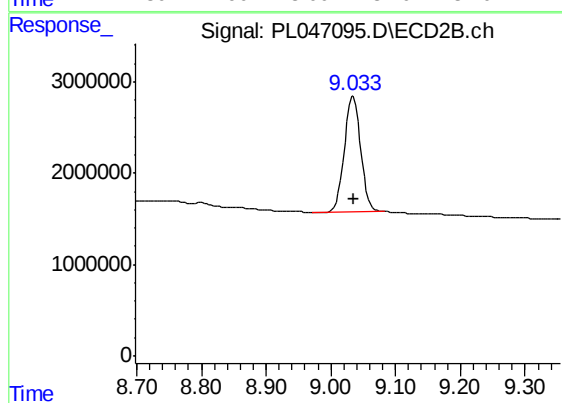

#28 Decachlorobiphenyl

R.T.: 9.034 min
Delta R.T.: 0.000 min
Response: 22349327
Conc: 9.64 ng/ml