

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040820\
 Data File : PL057848.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Apr 2020 13:58
 Operator : AJ\MA
 Sample : PB128067BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB128067BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 09 01:06:58 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 04 06:41:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.458	3.956	217.6E6	46930159	21.583	21.625
28)	SA Decachlor...	8.207	8.979	215.4E6	50003253	20.896	22.385
Target Compounds							
2)	A alpha-BHC	3.895	0.000	7768629	0	0.447	N.D. #
4)	MA Heptachlor	0.000	5.137	0	823865	N.D.	0.245 #
7)	B delta-BHC	0.000	4.985f	0	4279801	N.D.	3.668 #
8)	B Heptachlo...	0.000	5.805	0	2475603	N.D.	0.917 #
11)	B alpha-Chl...	5.450	0.000	2270901	0	0.171	N.D. #
15)	B Endosulfa...	0.000	6.870f	0	752392	N.D.	0.290 #
23)	Chlordane-1	4.355f	4.927	3637871	1615513	9.836	18.320 #
26)	Chlordane-4	5.450	0.000	2270901	0	2.183	N.D. #
27)	Chlordane-5	6.320f	0.000	193921	0	0.513	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040820\
Data File : PL057848.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Apr 2020 13:58
Operator : AJ\MA
Sample : PB128067BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleID :
PB128067BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 09 01:06:58 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
Quant Title : GC Extractables
QLast Update : Sat Apr 04 06:41:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

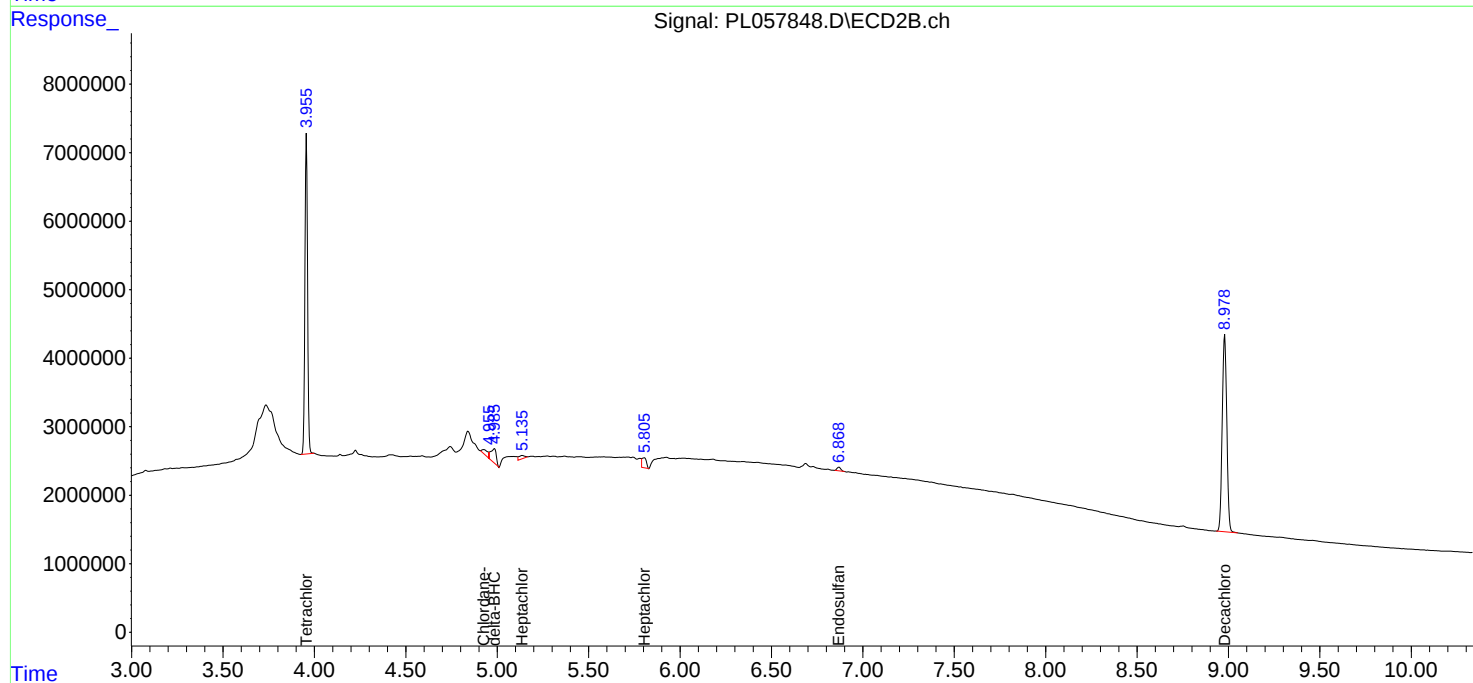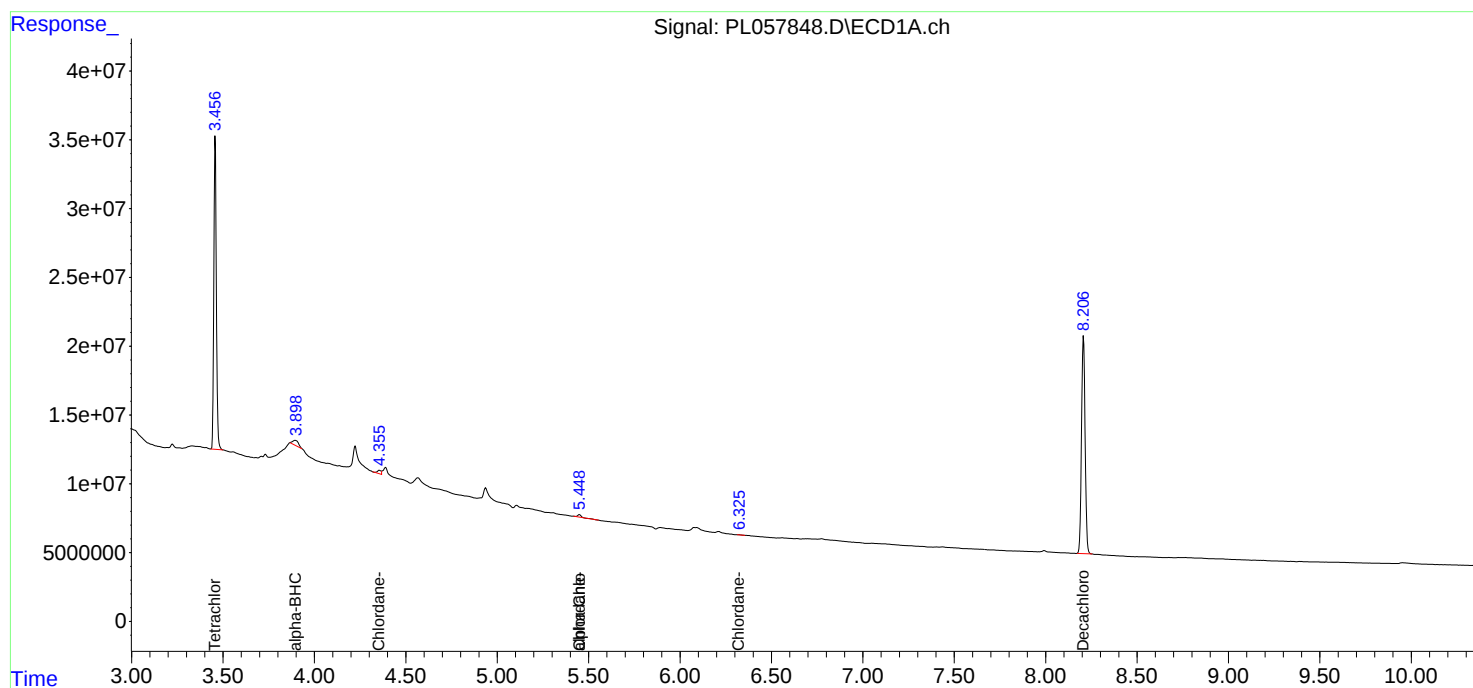


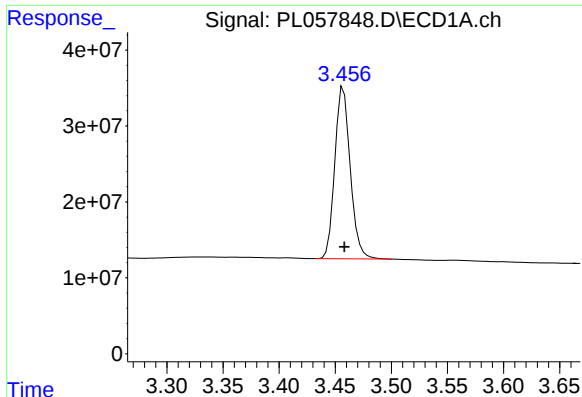

#1 Tetrachloro-m-xylene


R.T.: 3.458 min
Delta R.T.: 0.000 min
Response: 217577863
Conc: 21.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB128067BL

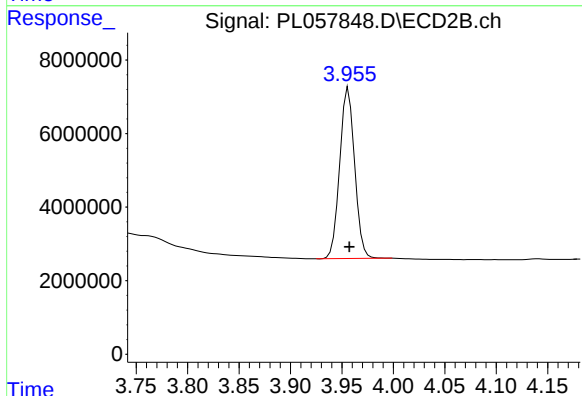


#1 Tetrachloro-m-xylene

R.T.: 3.956 min
Delta R.T.: -0.001 min
Response: 46930159
Conc: 21.63 ng/ml

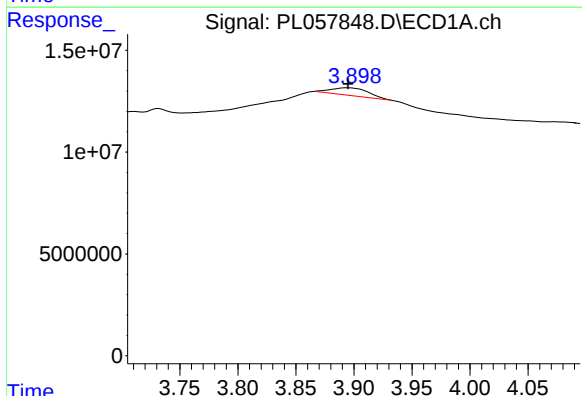


#2 alpha-BHC

R.T.: 3.895 min
Delta R.T.: 0.000 min
Response: 7768629
Conc: 0.45 ng/ml

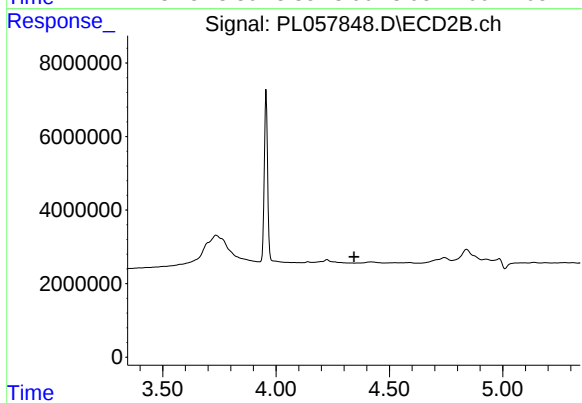

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.345 min
Response: 0
Conc: N.D.

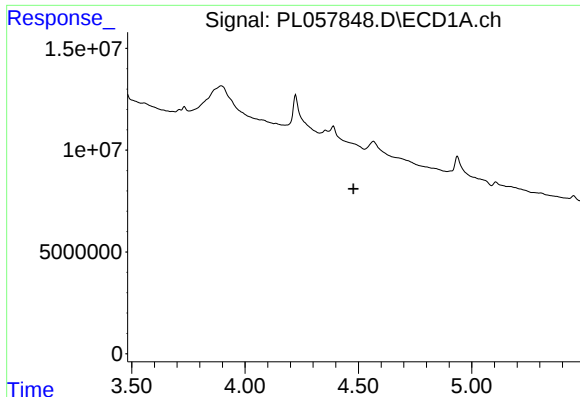

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.479 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB128067BL

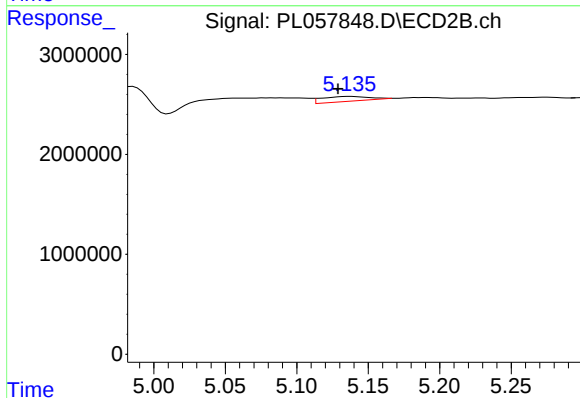


#4 Heptachlor

R.T.: 5.137 min
Delta R.T.: 0.008 min
Response: 823865
Conc: 0.25 ng/ml

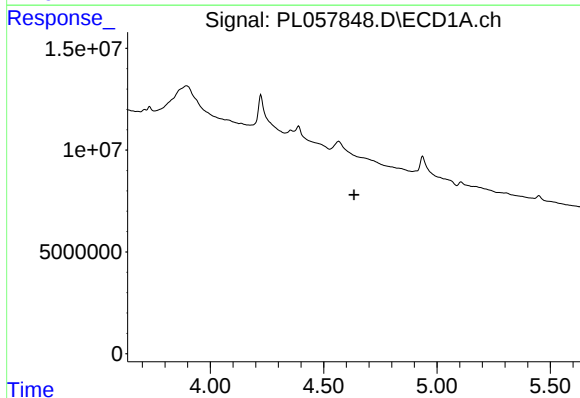


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.634 min
Response: 0
Conc: N.D.

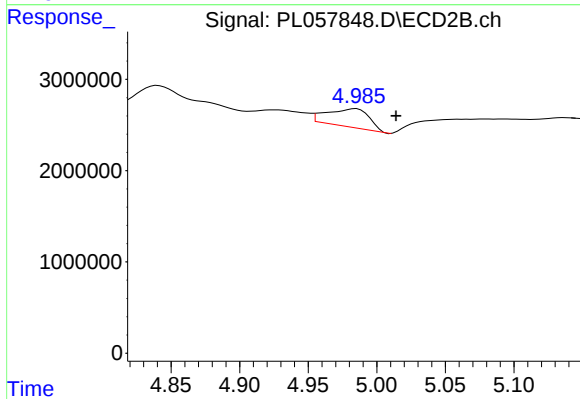

#7 delta-BHC


R.T.: 4.985 min
Delta R.T.: -0.029 min
Response: 4279801
Conc: 3.67 ng/ml

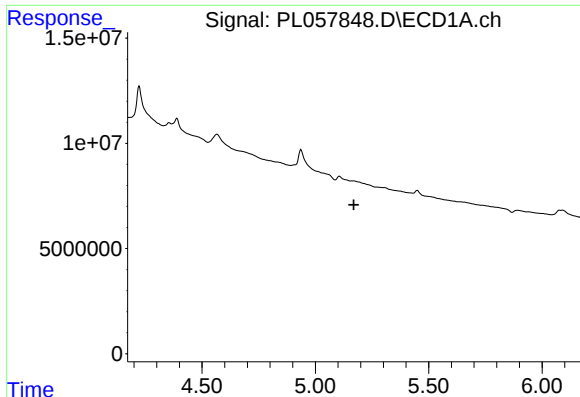

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.169 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB128067BL

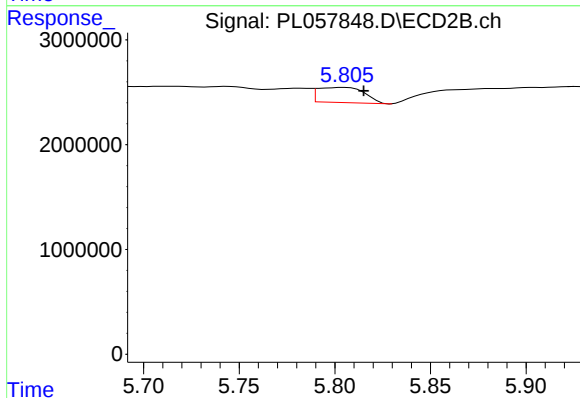


#8 Heptachlor epoxide

R.T.: 5.805 min
Delta R.T.: -0.010 min
Response: 2475603
Conc: 0.92 ng/ml

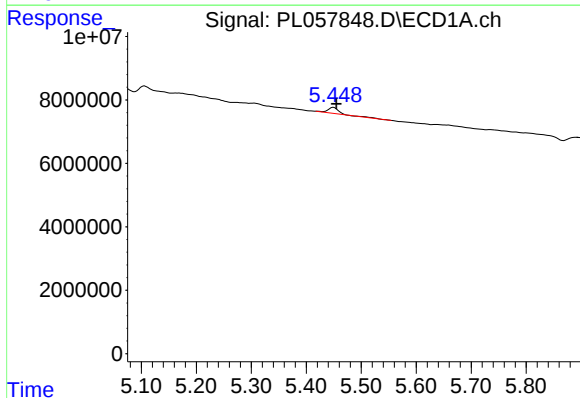


#11 alpha-Chlordane

R.T.: 5.450 min
Delta R.T.: -0.005 min
Response: 2270901
Conc: 0.17 ng/ml

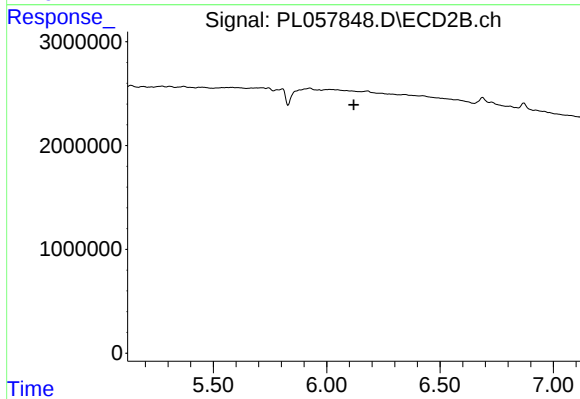

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.120 min
Response: 0
Conc: N.D.

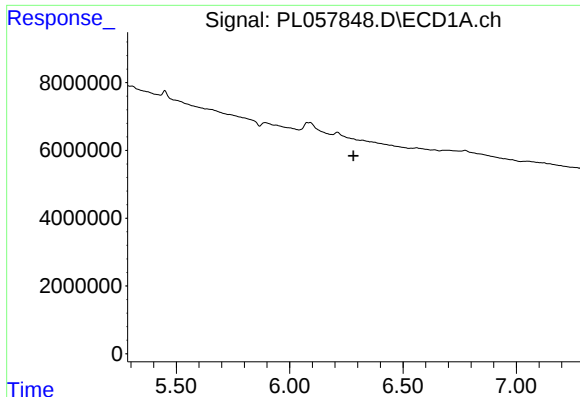

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.282 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB128067BL

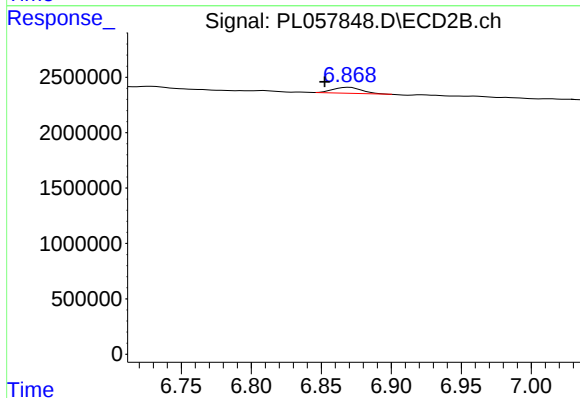


#15 Endosulfan II

R.T.: 6.870 min
Delta R.T.: 0.017 min
Response: 752392
Conc: 0.29 ng/ml

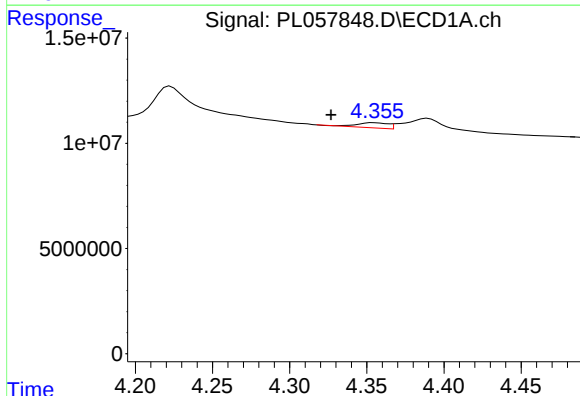


#23 Chlordane-1

R.T.: 4.355 min
Delta R.T.: 0.028 min
Response: 3637871
Conc: 9.84 ng/ml

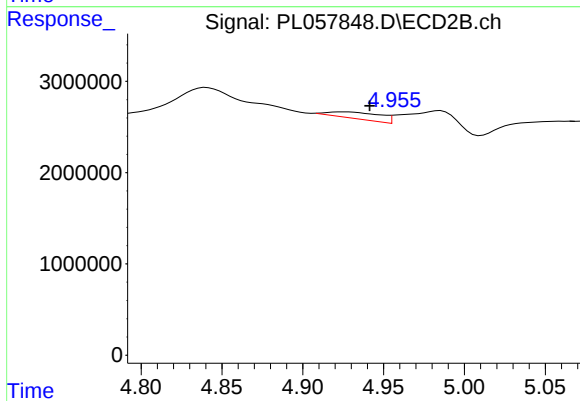

#23 Chlordane-1


R.T.: 4.927 min
Delta R.T.: -0.015 min
Response: 1615513
Conc: 18.32 ng/ml

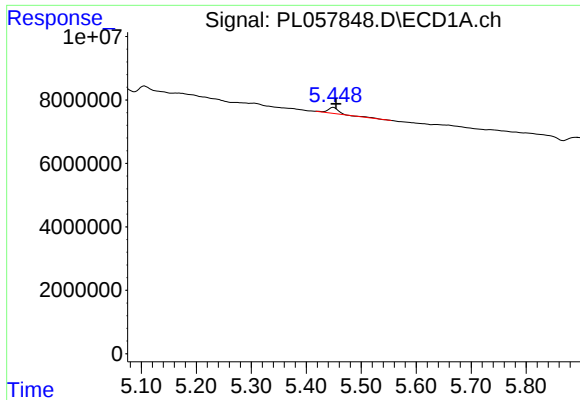

#26 Chlordane-4


R.T.: 5.450 min
Delta R.T.: -0.005 min
Response: 2270901
Conc: 2.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB128067BL

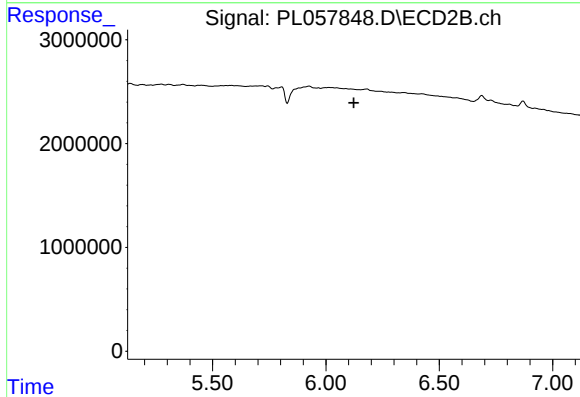


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.123 min
Response: 0
Conc: N.D.

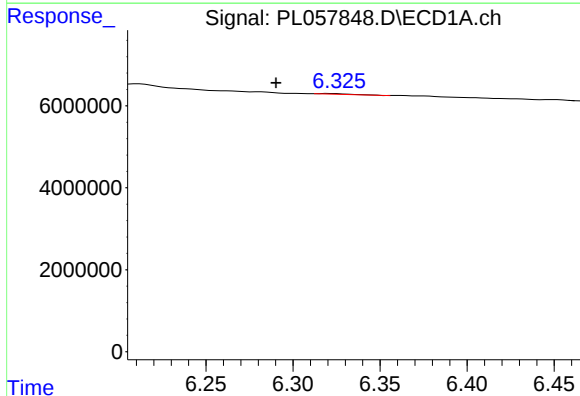


#27 Chlordane-5

R.T.: 6.320 min
Delta R.T.: 0.030 min
Response: 193921
Conc: 0.51 ng/ml

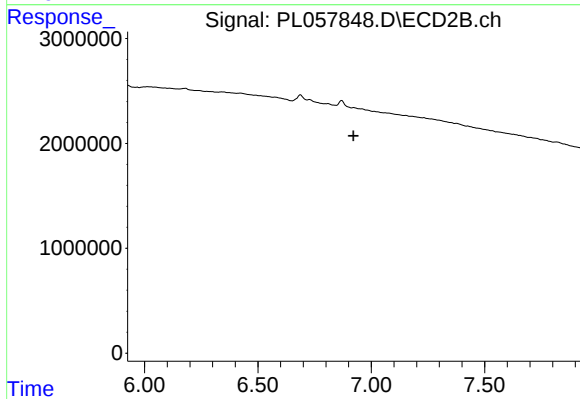

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T. : 6.922 min
Response: 0
Conc: N.D.

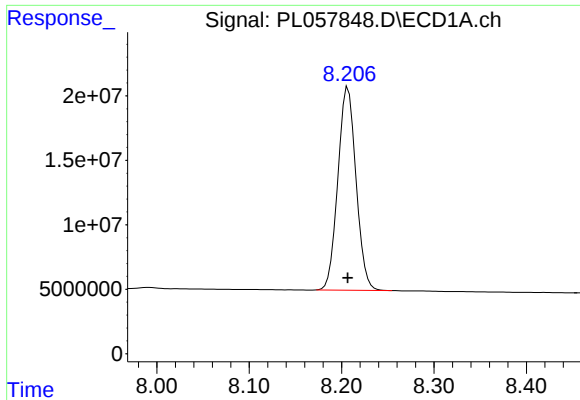

#28 Decachlorobiphenyl

R.T.: 8.207 min
Delta R.T.: 0.000 min
Response: 215409247
Conc: 20.90 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB128067BL

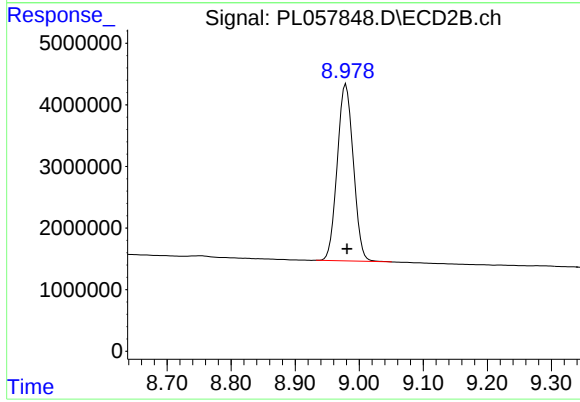

#28 Decachlorobiphenyl

R.T.: 8.979 min
Delta R.T.: -0.002 min
Response: 50003253
Conc: 22.39 ng/ml