

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040822\
 Data File : PL073887.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Apr 2022 11:33
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 08 15:40:10 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040822.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 08 15:38:55 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.638	5.491	21481045	98082924	56.762	50.000
28)	SA Decachlor...	10.413	11.335	27342840	95825454	50.000	50.000
Target Compounds							
23)	Chlordane-1	5.971	6.864	6138212	37874849	500.000	500.000
24)	Chlordane-2	6.660	7.447	8377795	41373479	500.000	500.000
25)	Chlordane-3	7.362	8.197	21285765	158.2E6	500.000	500.000
26)	Chlordane-4	7.431	8.283	22848553	189.6E6	500.000	500.000
27)	Chlordane-5	8.381	9.152	8432339	30799539	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040822\
Data File : PL073887.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Apr 2022 11:33
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 08 15:40:10 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040822.M
Quant Title : GC Extractables
QLast Update : Fri Apr 08 15:38:55 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

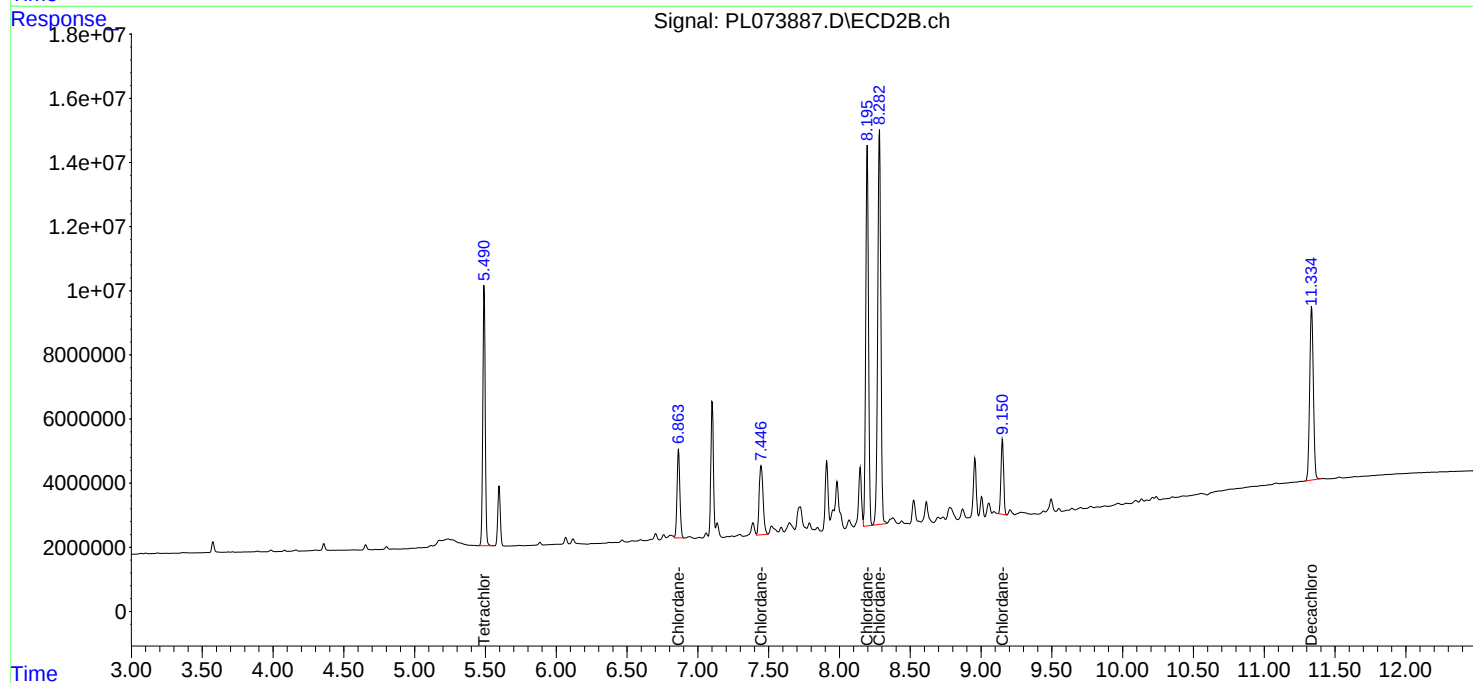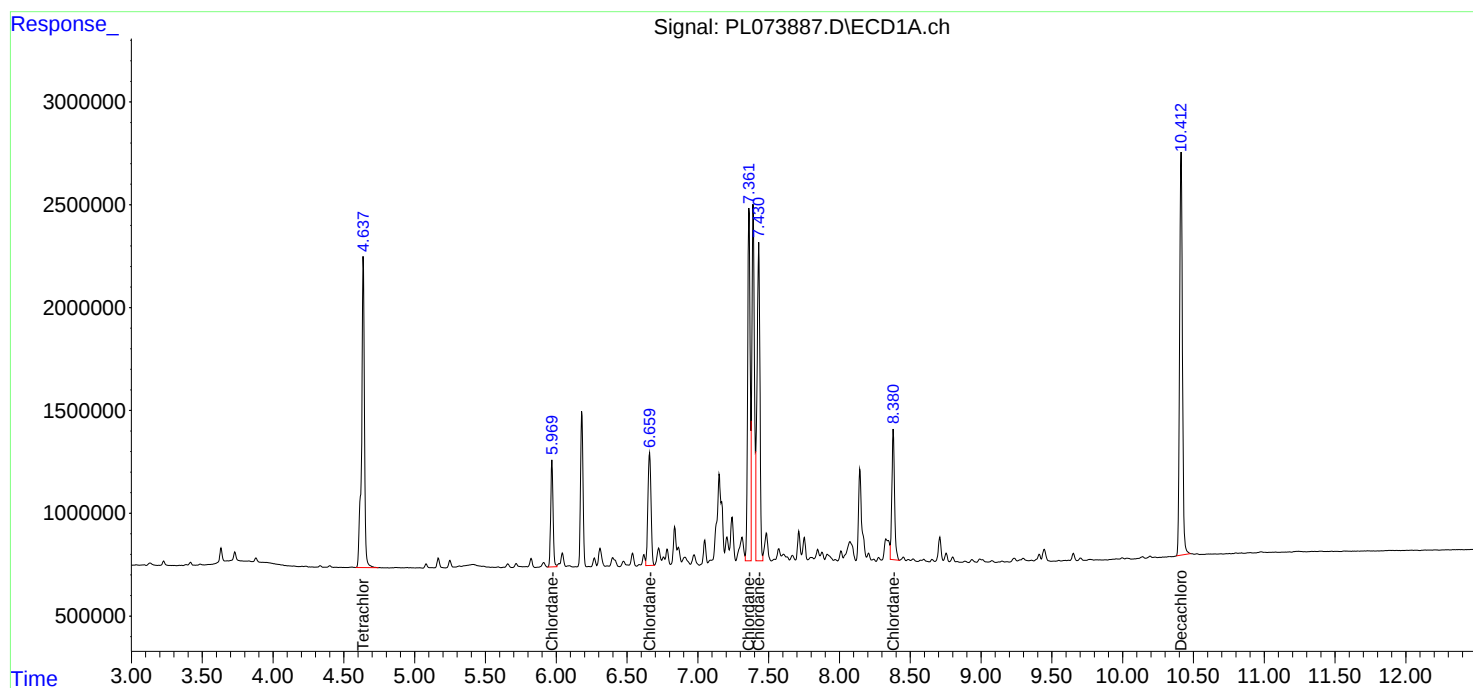


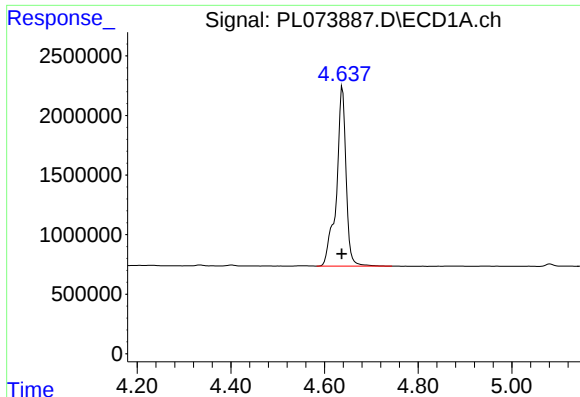

#1 Tetrachloro-m-xylene


R.T.: 4.638 min
Delta R.T.: 0.001 min
Response: 21481045
Conc: 56.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

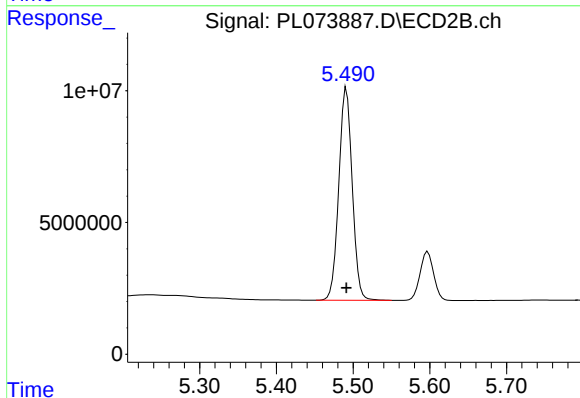


#1 Tetrachloro-m-xylene

R.T.: 5.491 min
Delta R.T.: 0.000 min
Response: 98082924
Conc: 50.00 ng/ml

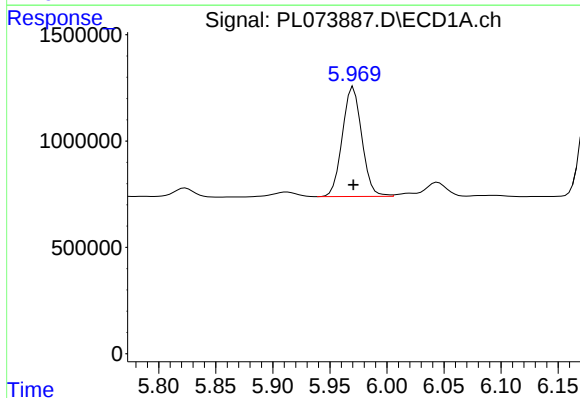


#23 Chlordane-1

R.T.: 5.971 min
Delta R.T.: 0.000 min
Response: 6138212
Conc: 500.00 ng/ml

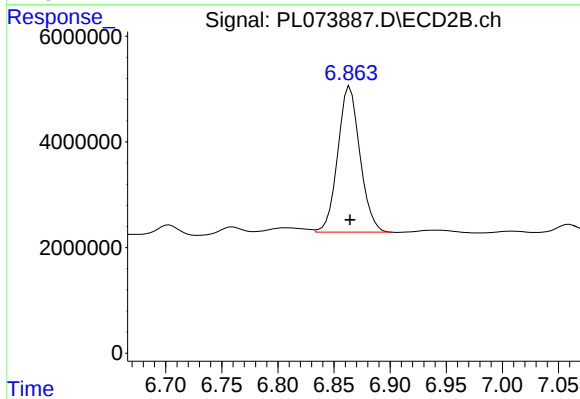

#23 Chlordane-1


R.T.: 6.864 min
Delta R.T.: 0.000 min
Response: 37874849
Conc: 500.00 ng/ml

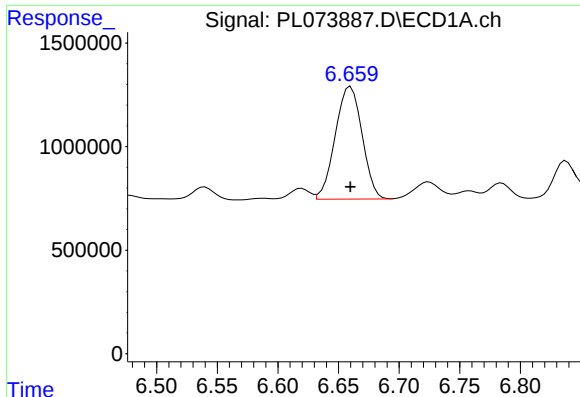

#24 Chlordane-2


R.T.: 6.660 min
Delta R.T.: 0.000 min
Response: 8377795
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

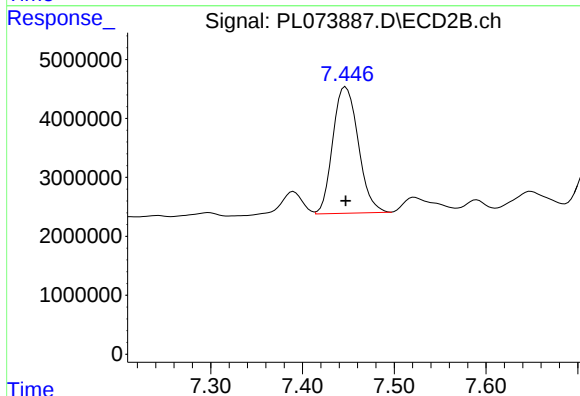


#24 Chlordane-2

R.T.: 7.447 min
Delta R.T.: 0.000 min
Response: 41373479
Conc: 500.00 ng/ml

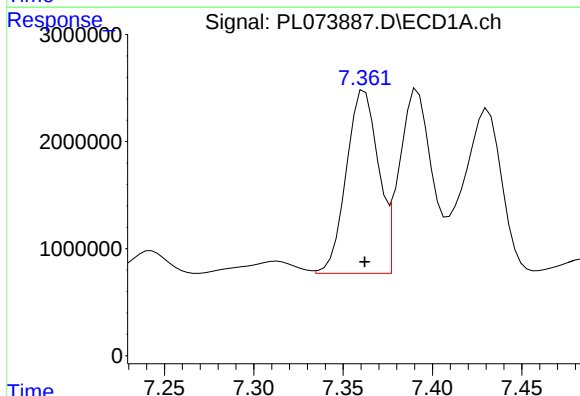


#25 Chlordane-3

R.T.: 7.362 min
Delta R.T.: 0.000 min
Response: 21285765
Conc: 500.00 ng/ml

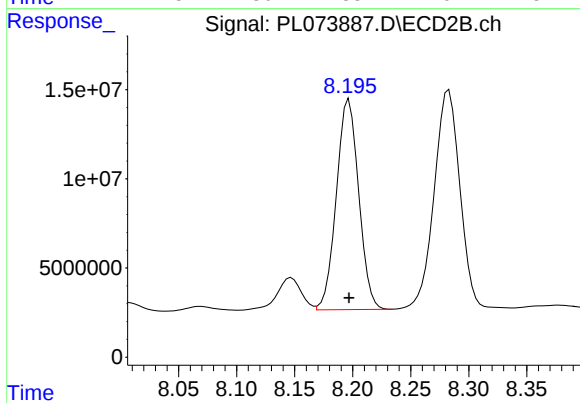

#25 Chlordane-3


R.T.: 8.197 min
Delta R.T.: 0.000 min
Response: 158215280
Conc: 500.00 ng/ml

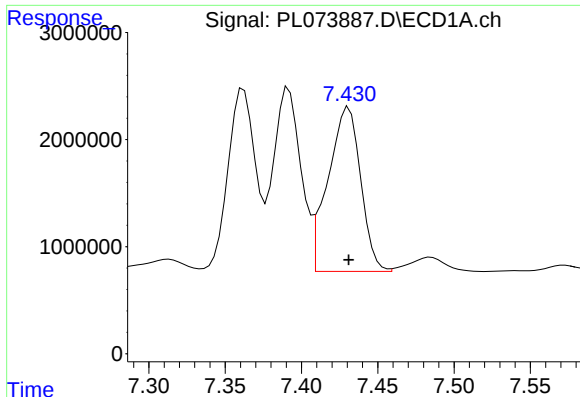

#26 Chlordane-4


R.T.: 7.431 min
Delta R.T.: 0.000 min
Response: 22848553
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

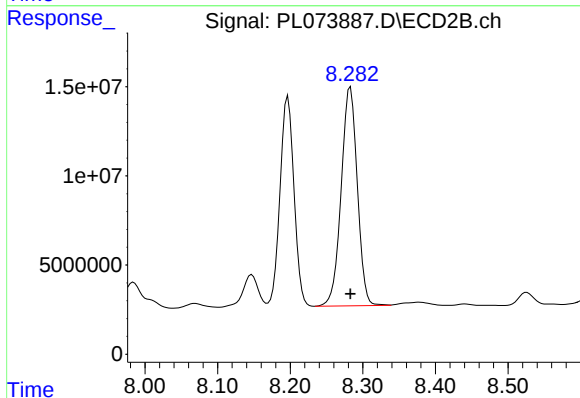


#26 Chlordane-4

R.T.: 8.283 min
Delta R.T.: 0.000 min
Response: 189621732
Conc: 500.00 ng/ml

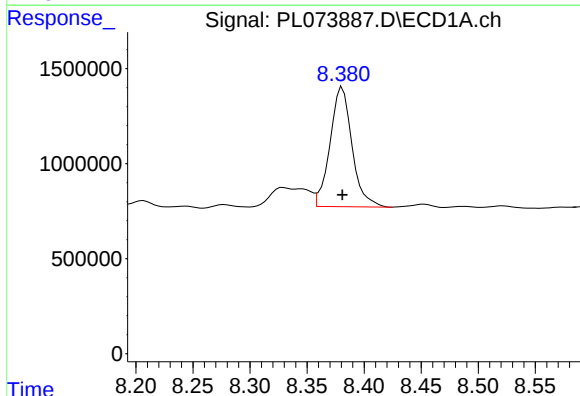


#27 Chlordane-5

R.T.: 8.381 min
Delta R.T.: 0.000 min
Response: 8432339
Conc: 500.00 ng/ml

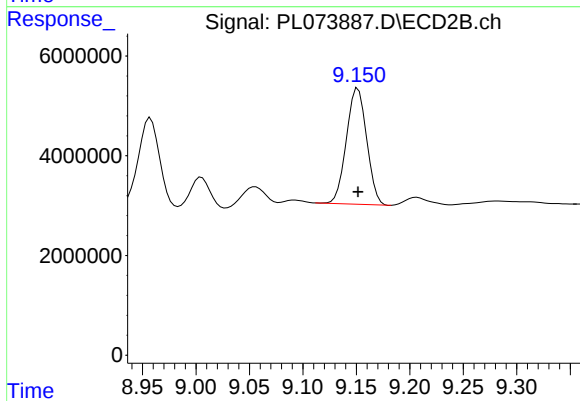

#27 Chlordane-5


R.T.: 9.152 min
Delta R.T.: 0.000 min
Response: 30799539
Conc: 500.00 ng/ml

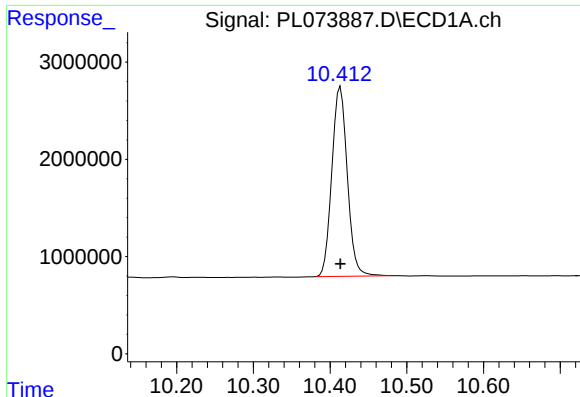

#28 Decachlorobiphenyl

R.T.: 10.413 min
Delta R.T.: 0.000 min
Response: 27342840
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

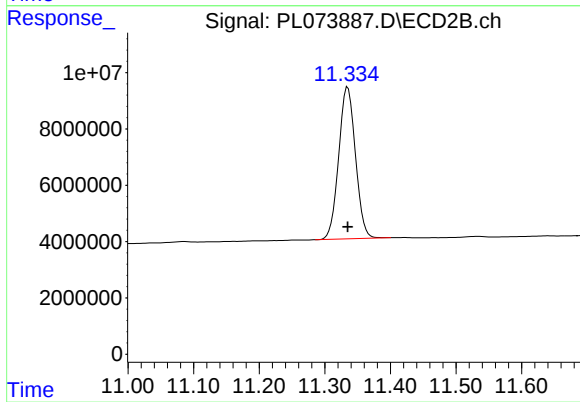

#28 Decachlorobiphenyl

R.T.: 11.335 min
Delta R.T.: 0.000 min
Response: 95825454
Conc: 50.00 ng/ml