

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040822\
 Data File : PL073900.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Apr 2022 15:58
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 08 17:03:36 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040822.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 08 15:48:40 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.639	5.491	21370493	98744681	66.140	55.382
28)	SA Decachlor...	10.414	11.335	27510915	97394242	52.902	55.140
Target Compounds							
23)	Chlordane-1	5.971	6.864	6186724	38940071	496.666	487.966
24)	Chlordane-2	6.660	7.446	8415868	41419835	482.942	501.225
25)	Chlordane-3	7.361	8.197	21267424	158.9E6	491.596	469.821
26)	Chlordane-4	7.431	8.283	22890893	191.1E6	493.208	481.782
27)	Chlordane-5	8.381	9.151	8373412	30943543	480.108	514.206



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040822\
Data File : PL073900.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Apr 2022 15:58
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 08 17:03:36 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040822.M
Quant Title : GC Extractables
QLast Update : Fri Apr 08 15:48:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

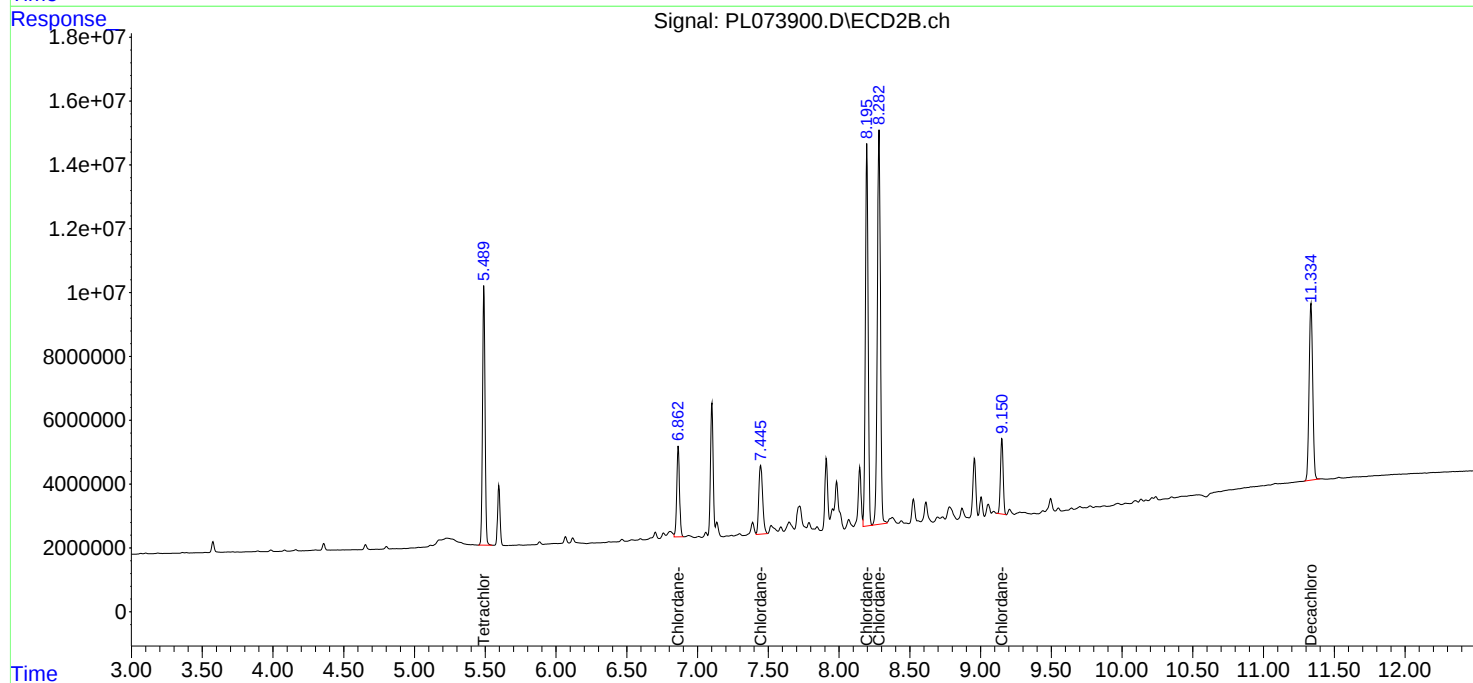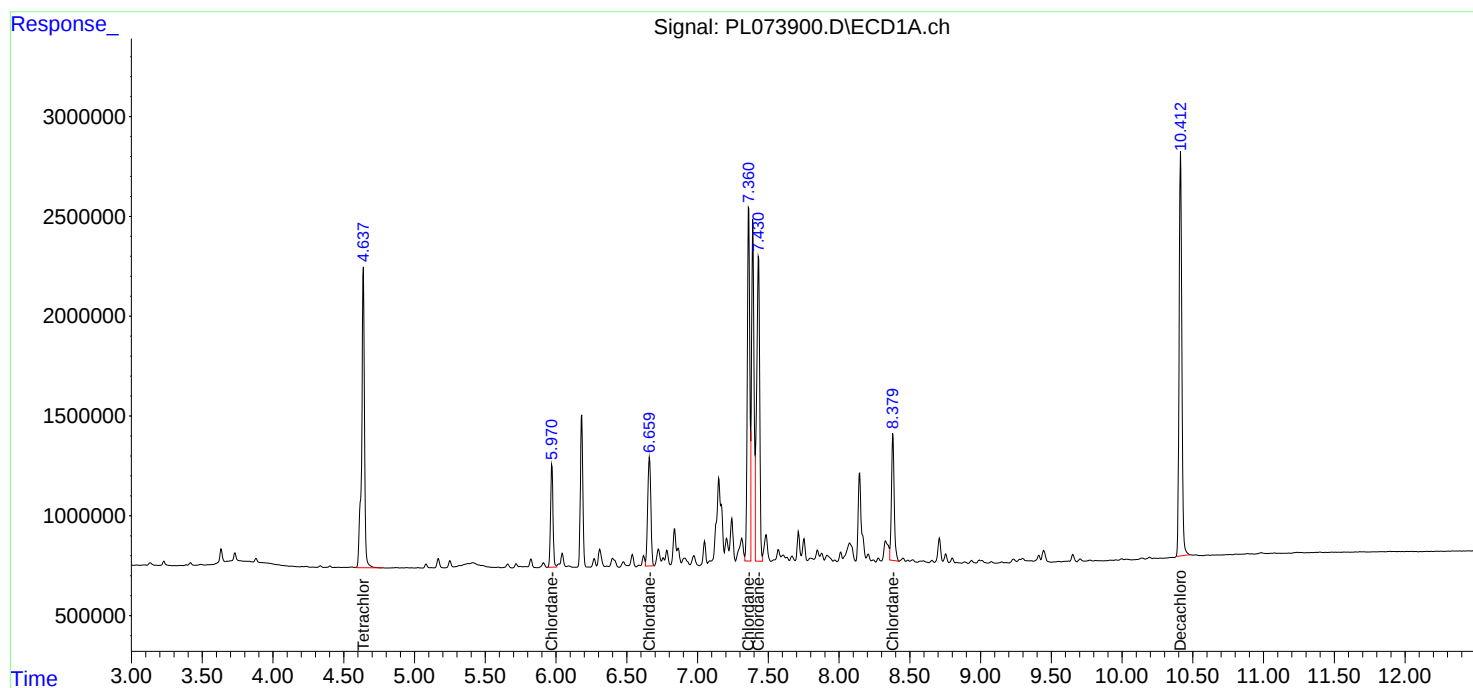


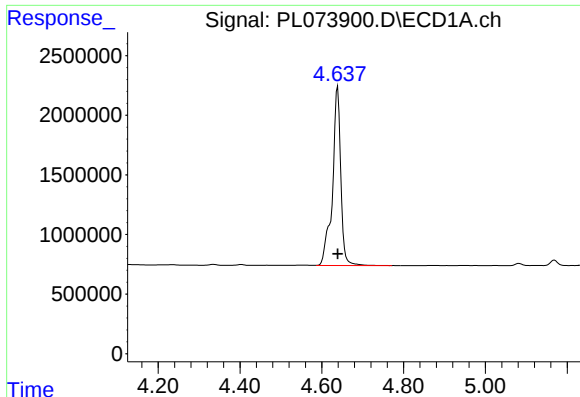

#1 Tetrachloro-m-xylene


R.T.: 4.639 min
Delta R.T.: 0.000 min
Response: 21370493
Conc: 66.14 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

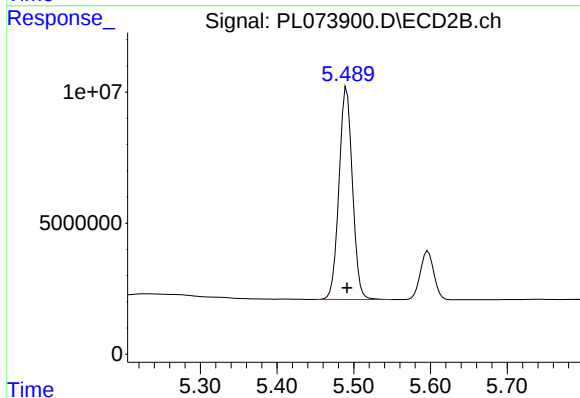


#1 Tetrachloro-m-xylene

R.T.: 5.491 min
Delta R.T.: 0.000 min
Response: 98744681
Conc: 55.38 ng/ml

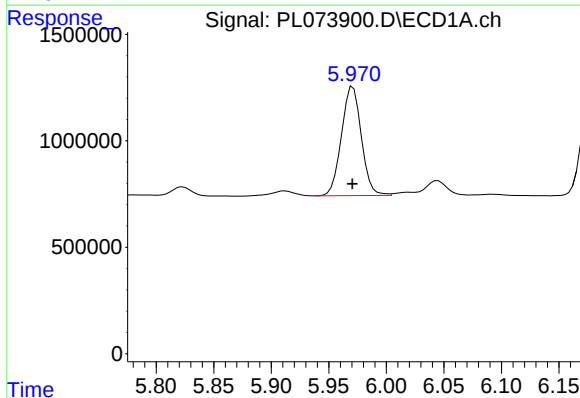


#23 Chlordane-1

R.T.: 5.971 min
Delta R.T.: 0.000 min
Response: 6186724
Conc: 496.67 ng/ml

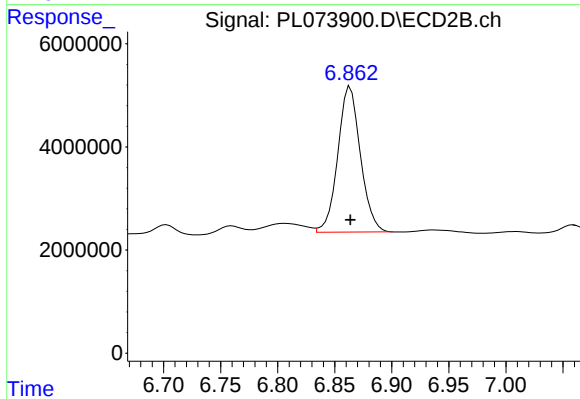

#23 Chlordane-1


R.T.: 6.864 min
Delta R.T.: 0.000 min
Response: 38940071
Conc: 487.97 ng/ml

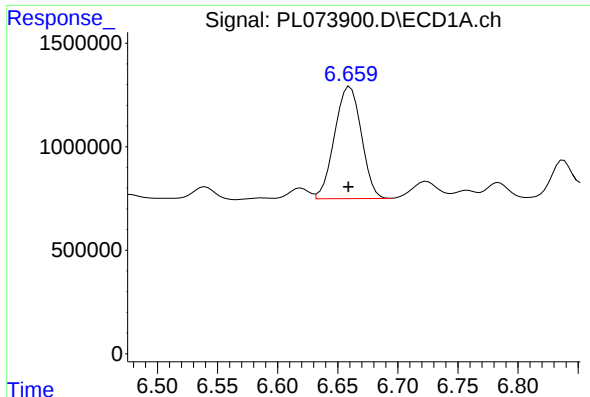

#24 Chlordane-2


R.T.: 6.660 min
Delta R.T.: 0.001 min
Response: 8415868
Conc: 482.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

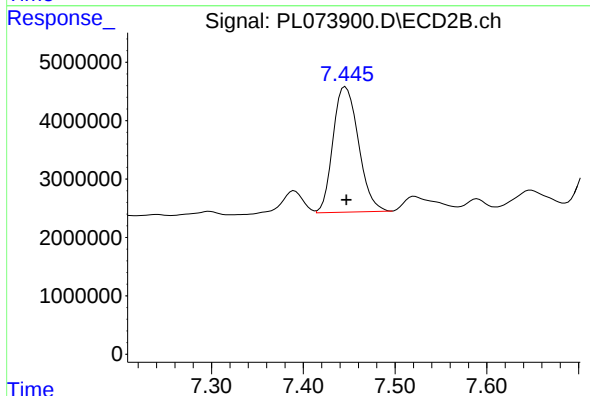


#24 Chlordane-2

R.T.: 7.446 min
Delta R.T.: 0.000 min
Response: 41419835
Conc: 501.23 ng/ml

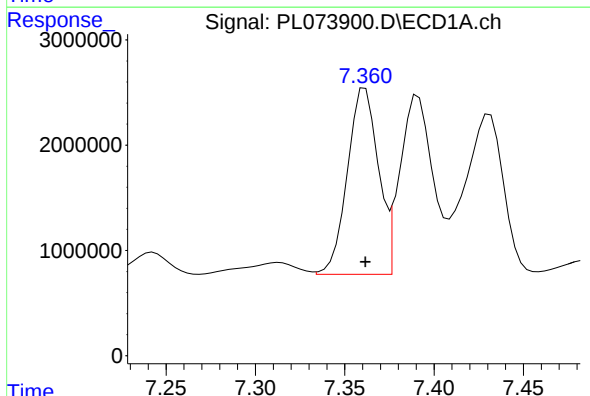


#25 Chlordane-3

R.T.: 7.361 min
Delta R.T.: 0.000 min
Response: 21267424
Conc: 491.60 ng/ml

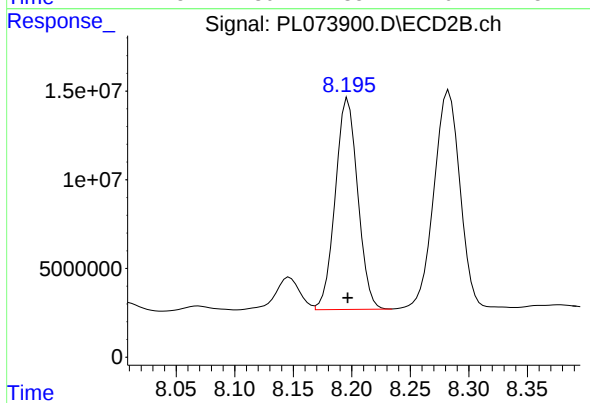

#25 Chlordane-3


R.T.: 8.197 min
Delta R.T.: 0.000 min
Response: 158940680
Conc: 469.82 ng/ml

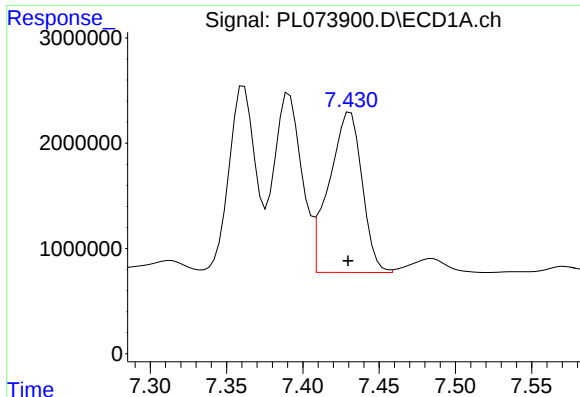

#26 Chlordane-4


R.T.: 7.431 min
Delta R.T.: 0.002 min
Response: 22890893
Conc: 493.21 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

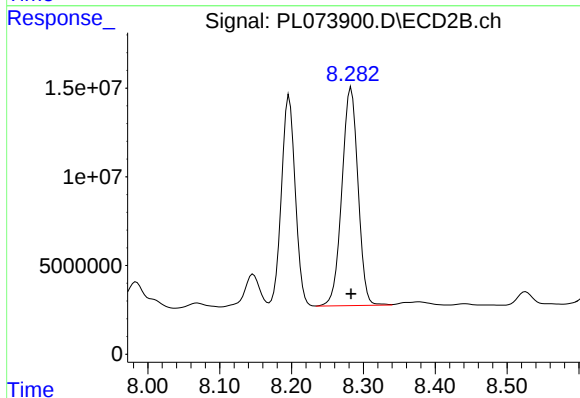


#26 Chlordane-4

R.T.: 8.283 min
Delta R.T.: 0.000 min
Response: 191085222
Conc: 481.78 ng/ml

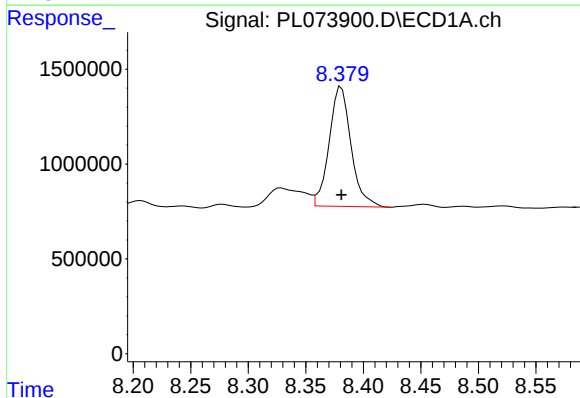


#27 Chlordane-5

R.T.: 8.381 min
Delta R.T.: 0.000 min
Response: 8373412
Conc: 480.11 ng/ml

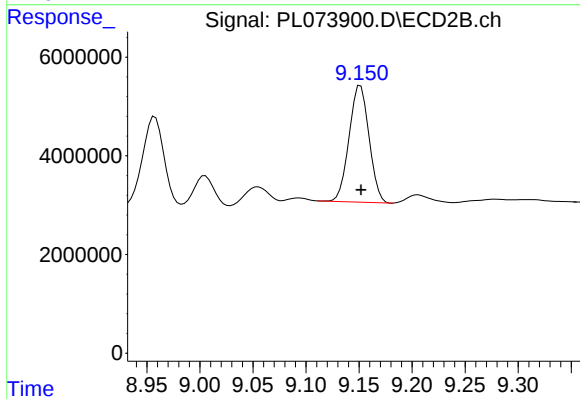

#27 Chlordane-5


R.T.: 9.151 min
Delta R.T.: 0.000 min
Response: 30943543
Conc: 514.21 ng/ml

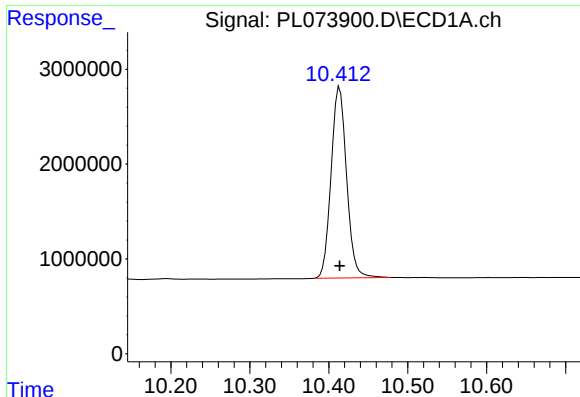

#28 Decachlorobiphenyl

R.T.: 10.414 min
Delta R.T.: 0.000 min
Response: 27510915
Conc: 52.90 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

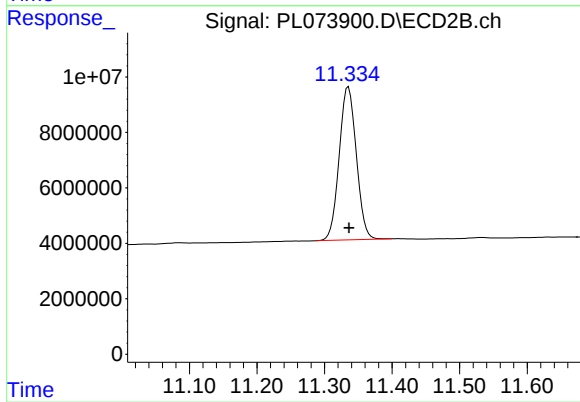

#28 Decachlorobiphenyl

R.T.: 11.335 min
Delta R.T.: 0.000 min
Response: 97394242
Conc: 55.14 ng/ml