

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040825\
 Data File : PL095121.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Apr 2025 17:19
 Operator : AR\AJ
 Sample : Q1745-01
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 IB-6A-WC

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 08 22:43:57 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031125.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 11 17:42:21 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.535	2.768	98804200	91170165	34.905	25.543 #
28)	SA Decachlor...	9.051	7.901	35787257	55705722	16.981	13.791
Target Compounds							
4)	MA Heptachlor	0.000	3.924f	0	10849365	N.D.	2.059 #
6)	B beta-BHC	4.535	3.924f	4301410	10849365	2.331	4.884 #
7)	B delta-BHC	4.760	0.000	3218172	0	0.826	N.D. #
9)	A Endosulfan I	0.000	5.121f	0	38108600	N.D.	8.683 #
10)	B gamma-Chl...	5.924f	0.000	14779209	0	4.386	N.D. #
12)	B 4,4'-DDE	0.000	5.241	0	39946970	N.D.	8.593 #
13)	MA Dieldrin	0.000	5.365	0	26354582	N.D.	5.432 #
14)	MA Endrin	0.000	5.643	0	24870912	N.D.	5.700 #
21)	B Endrin ke...	7.618f	0.000	4736801	0	1.792	N.D. #
23)	Chlordane-1	0.000	3.766	0	16939390	N.D.	112.158 #
24)	Chlordane-2	0.000	4.373f	0	18098767	N.D.	102.492 #
25)	Chlordane-3	5.924	0.000	14779209	0	29.569	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040825\
Data File : PL095121.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Apr 2025 17:19
Operator : AR\AJ
Sample : Q1745-01
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
IB-6A-WC

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 08 22:43:57 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031125.M
Quant Title : GC Extractables
QLast Update : Tue Mar 11 17:42:21 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

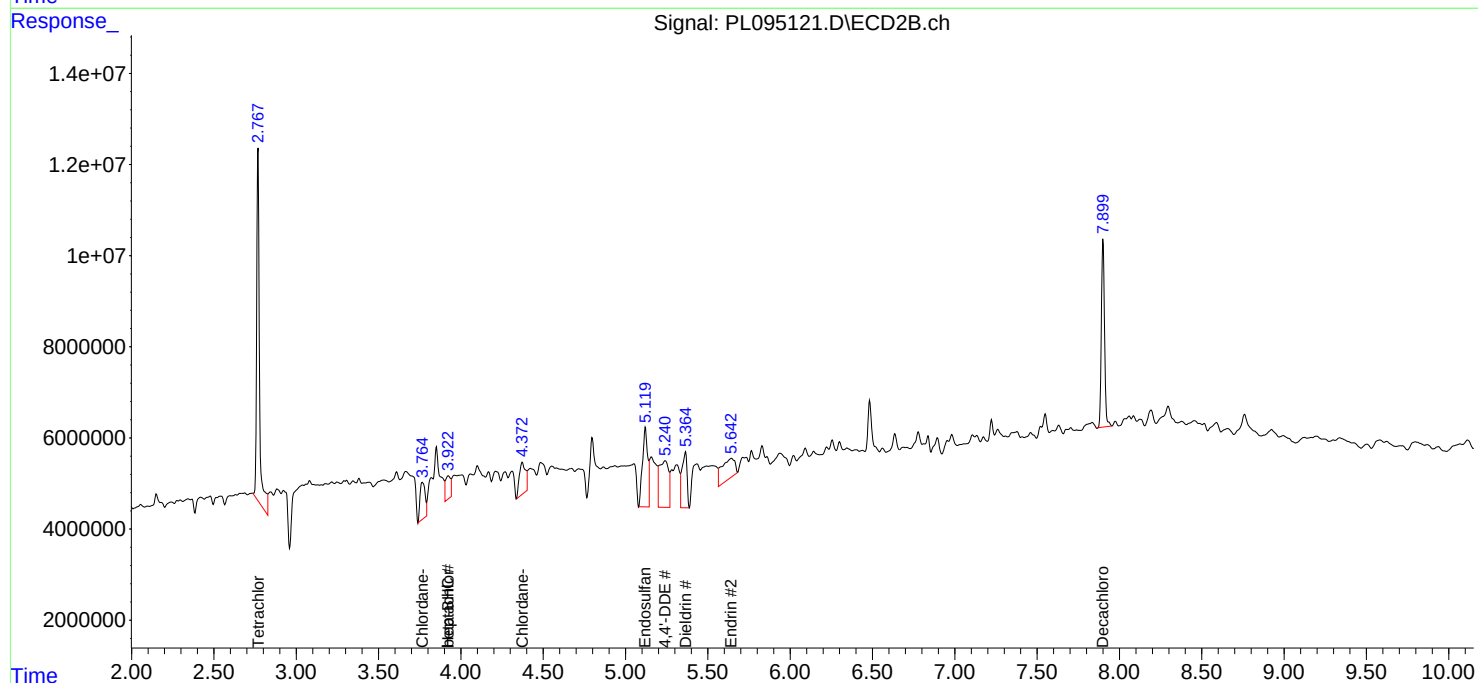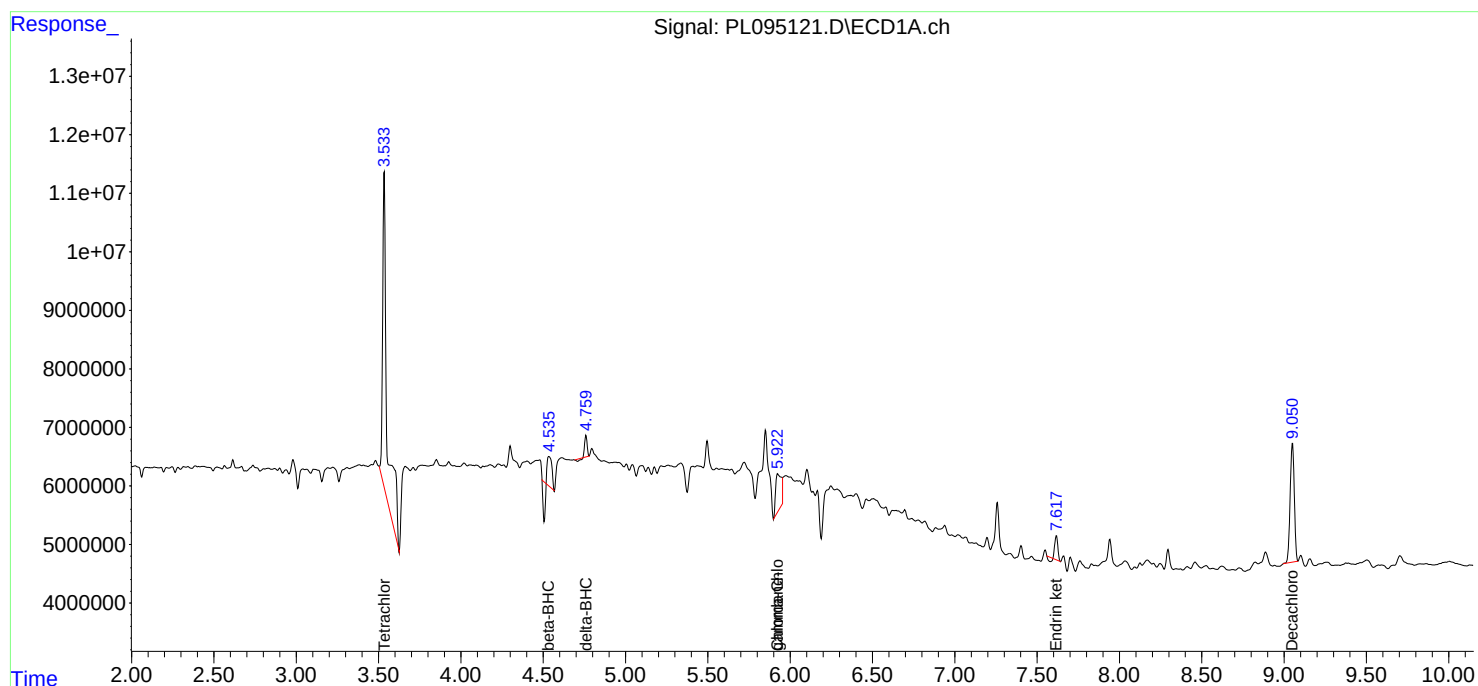


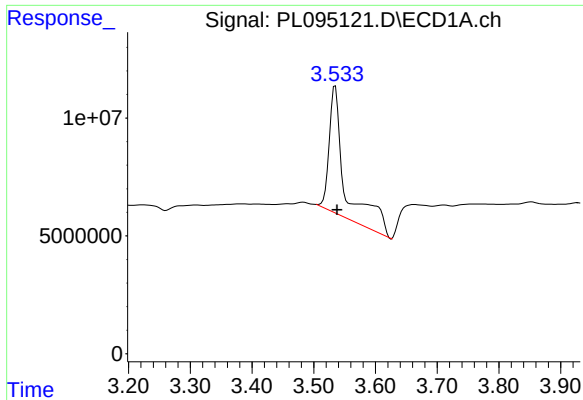

#1 Tetrachloro-m-xylene


R.T.: 3.535 min
Delta R.T.: -0.003 min
Response: 98804200
Conc: 34.90 ng/ml

Instrument :
ECD_L
ClientSampleId :
IB-6A-WC

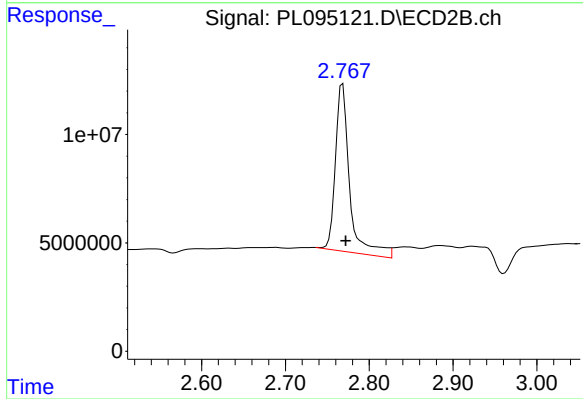


#1 Tetrachloro-m-xylene

R.T.: 2.768 min
Delta R.T.: -0.004 min
Response: 91170165
Conc: 25.54 ng/ml

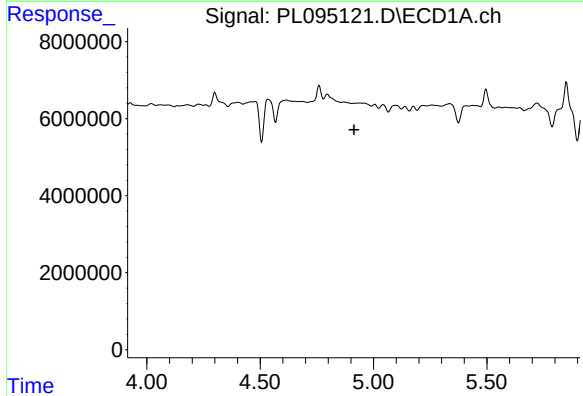


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.915 min
Response: 0
Conc: N.D.

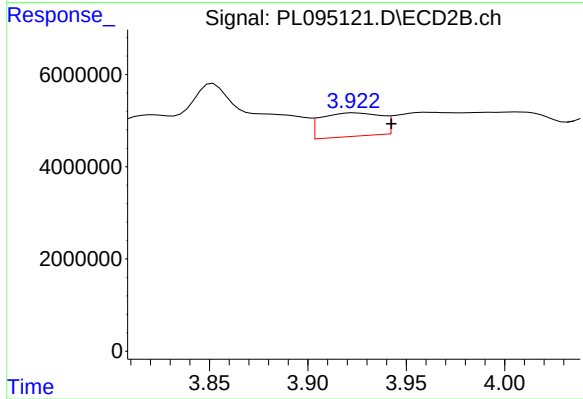

#4 Heptachlor


R.T.: 3.924 min
Delta R.T.: -0.018 min
Response: 10849365
Conc: 2.06 ng/ml

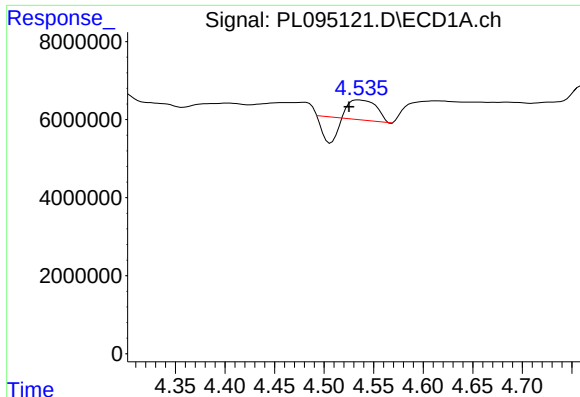

#6 beta-BHC


R.T.: 4.535 min
Delta R.T.: 0.010 min
Response: 4301410
Conc: 2.33 ng/ml

Instrument :
ECD_L
ClientSampleId :
IB-6A-WC

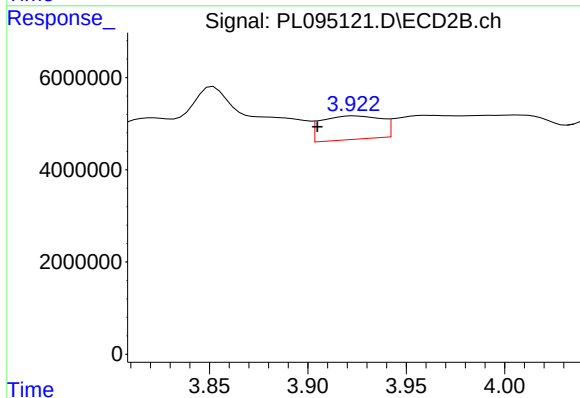


#6 beta-BHC

R.T.: 3.924 min
Delta R.T.: 0.019 min
Response: 10849365
Conc: 4.88 ng/ml

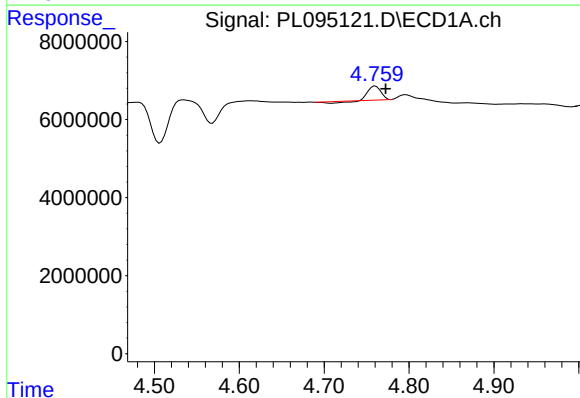


#7 delta-BHC

R.T.: 4.760 min
Delta R.T.: -0.012 min
Response: 3218172
Conc: 0.83 ng/ml

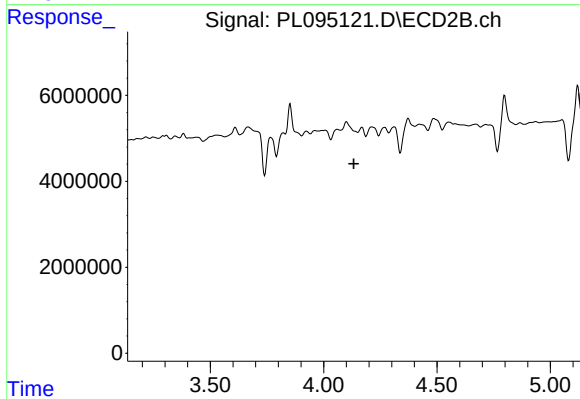

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.133 min
Response: 0
Conc: N.D.

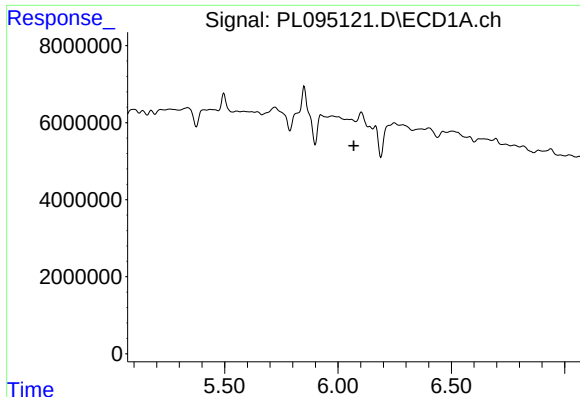

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.069 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
IB-6A-WC

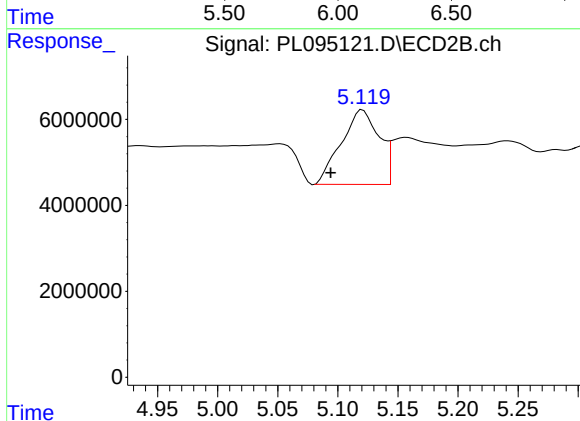


#9 Endosulfan I

R.T.: 5.121 min
Delta R.T.: 0.027 min
Response: 38108600
Conc: 8.68 ng/ml

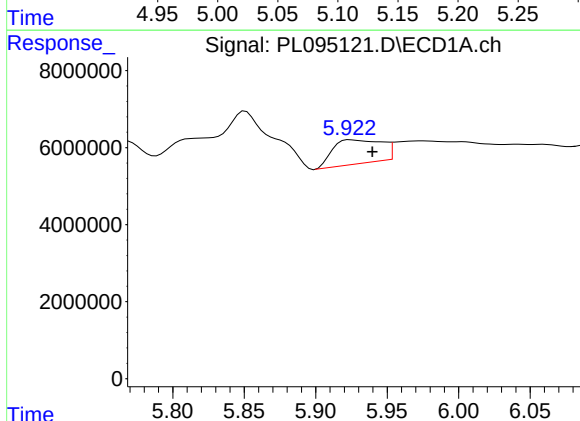


#10 gamma-Chlordane

R.T.: 5.924 min
Delta R.T.: -0.015 min
Response: 14779209
Conc: 4.39 ng/ml

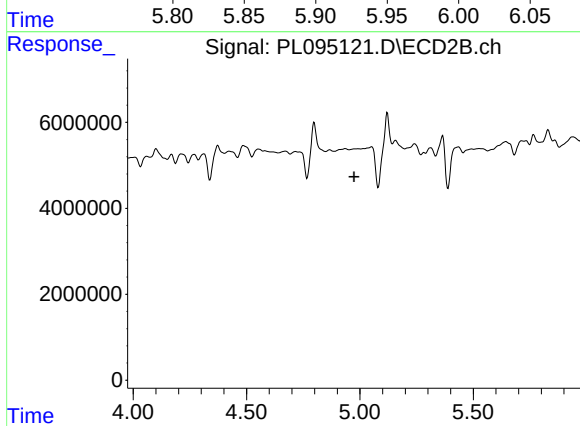

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 4.974 min
Response: 0
Conc: N.D.

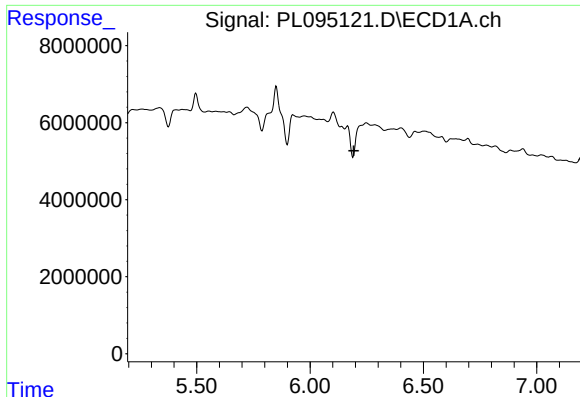

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 6.193 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
IB-6A-WC

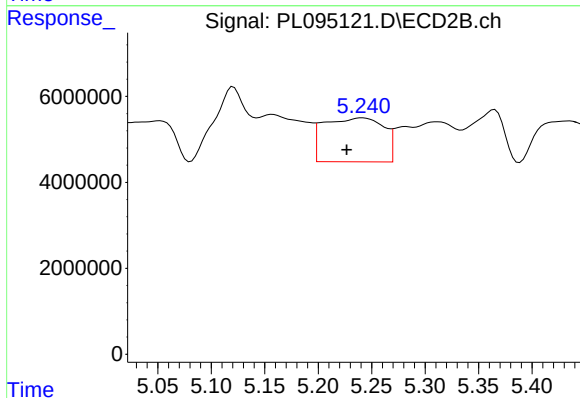


#12 4,4'-DDE

R.T.: 5.241 min
Delta R.T.: 0.015 min
Response: 39946970
Conc: 8.59 ng/ml

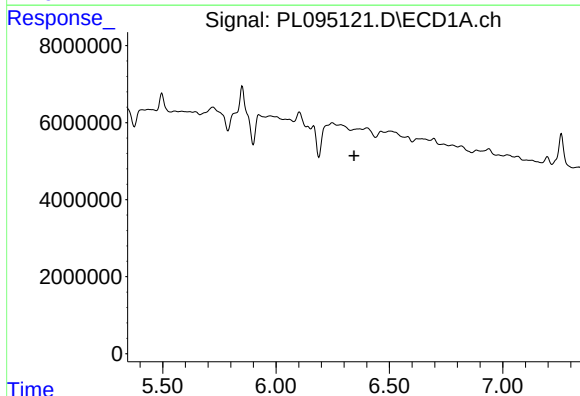


#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 6.344 min
Response: 0
Conc: N.D.

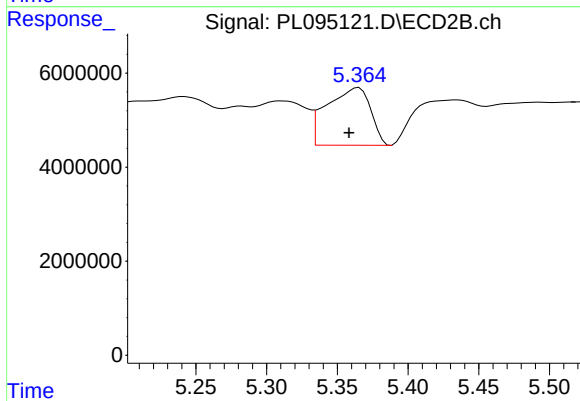

#13 Dieldrin


R.T.: 5.365 min
Delta R.T.: 0.007 min
Response: 26354582
Conc: 5.43 ng/ml

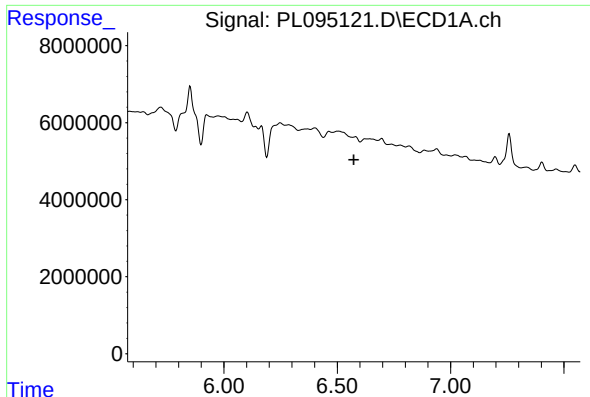

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.574 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
IB-6A-WC

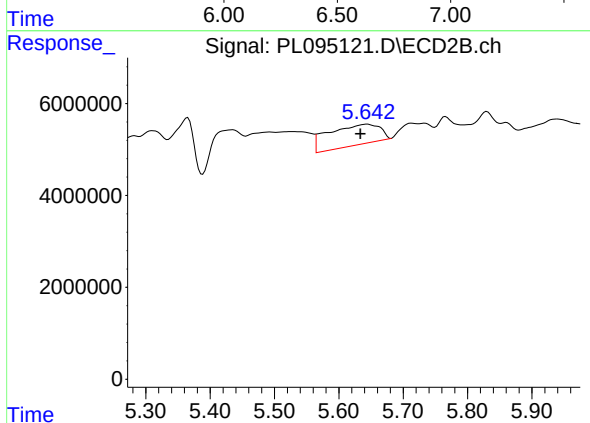


#14 Endrin

R.T.: 5.643 min
Delta R.T.: 0.010 min
Response: 24870912
Conc: 5.70 ng/ml

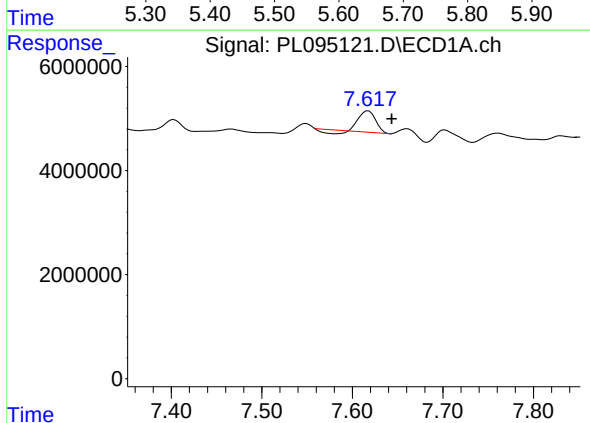


#21 Endrin ketone

R.T.: 7.618 min
Delta R.T.: -0.026 min
Response: 4736801
Conc: 1.79 ng/ml

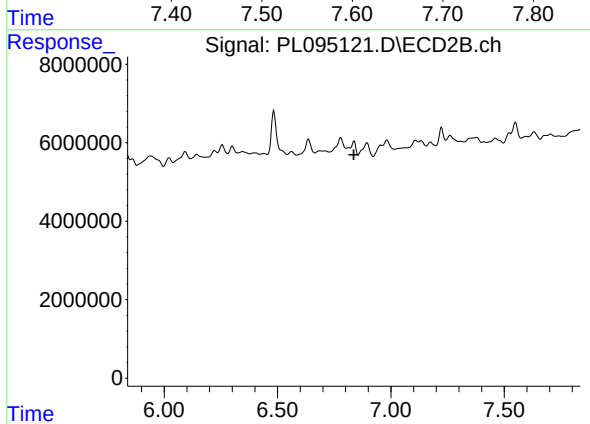

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 6.836 min
Response: 0
Conc: N.D.

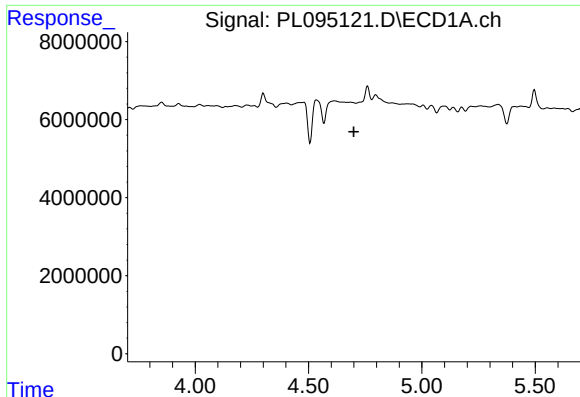

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.700 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
IB-6A-WC

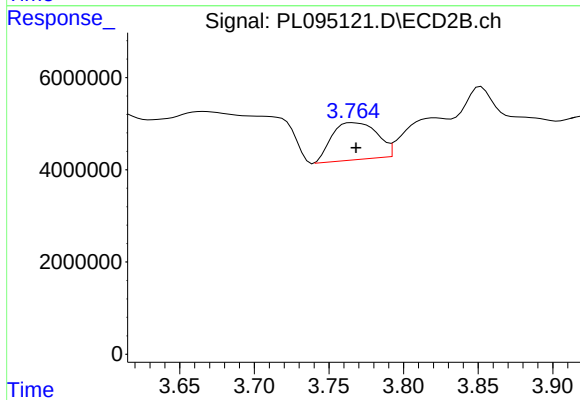


#23 Chlordane-1

R.T.: 3.766 min
Delta R.T.: -0.002 min
Response: 16939390
Conc: 112.16 ng/ml

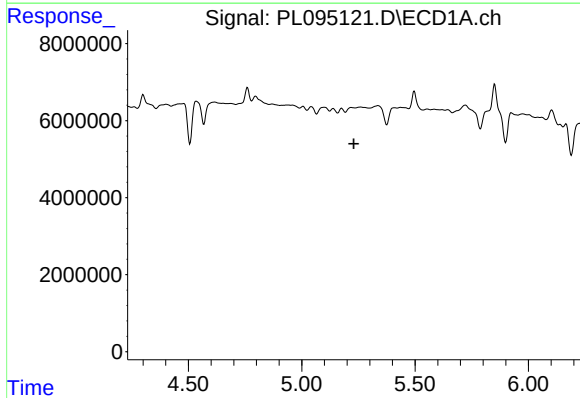


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T.: 5.230 min
Response: 0
Conc: N.D.

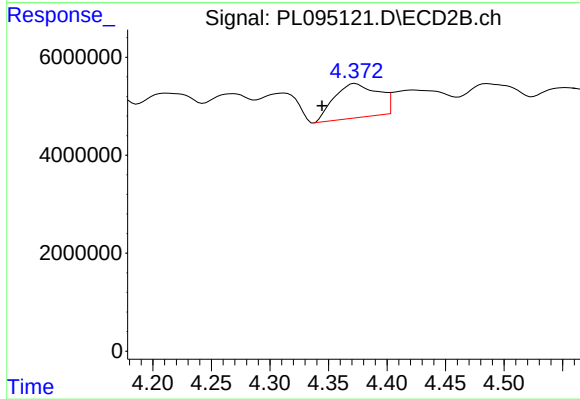

#24 Chlordane-2


R.T.: 4.373 min
Delta R.T.: 0.029 min
Response: 18098767
Conc: 102.49 ng/ml

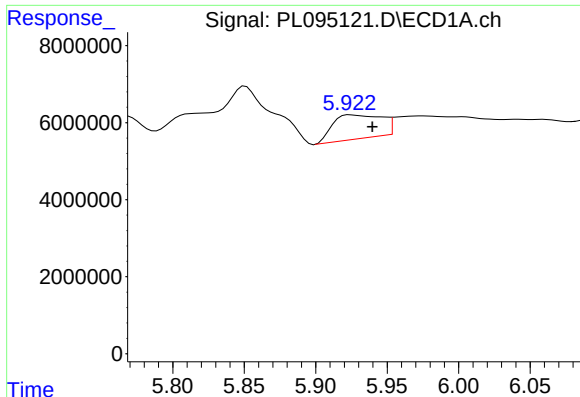

#25 Chlordane-3


R.T.: 5.924 min
Delta R.T.: -0.016 min
Response: 14779209
Conc: 29.57 ng/ml

Instrument :
ECD_L
ClientSampleId :
IB-6A-WC

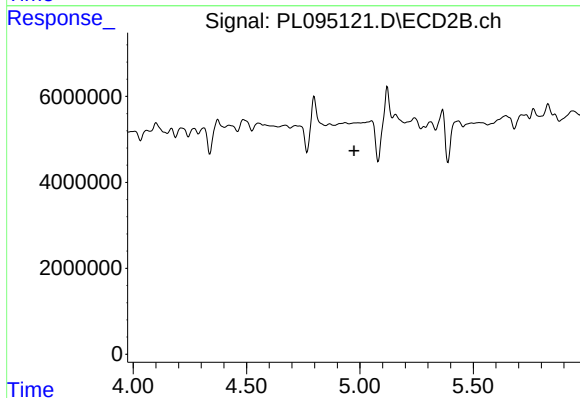


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 4.975 min
Response: 0
Conc: N.D.

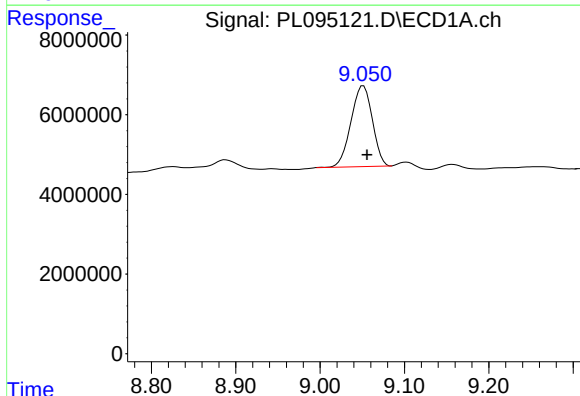

#28 Decachlorobiphenyl

R.T.: 9.051 min
Delta R.T.: -0.004 min
Response: 35787257
Conc: 16.98 ng/ml

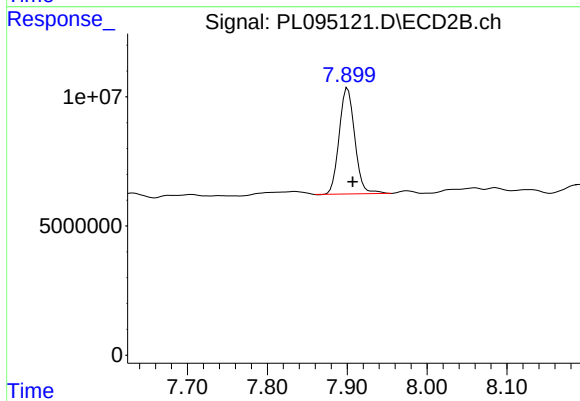

#28 Decachlorobiphenyl

R.T.: 7.901 min
Delta R.T.: -0.006 min
Response: 55705722
Conc: 13.79 ng/ml