

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040919\
 Data File : PL047128.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Apr 2019 17:46
 Operator : AJ\SJ
 Sample : K2294-04
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-14-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 10 01:04:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:40:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.358	3.978	147.6E6	48170255	20.288	21.039
28) SA Decachlor...	8.038	9.035	125.8E6	37982588	14.951	16.383
Target Compounds						
2) A alpha-BHC	3.793	0.000	11966306	0	1.026	N.D. #
6) B beta-BHC	4.322	0.000	15513291	0	3.446	N.D. #
23) Chlordane-1	4.215	0.000	7940416	0	23.611	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040919\
Data File : PL047128.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Apr 2019 17:46
Operator : AJ\SJ
Sample : K2294-04
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-14-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 10 01:04:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

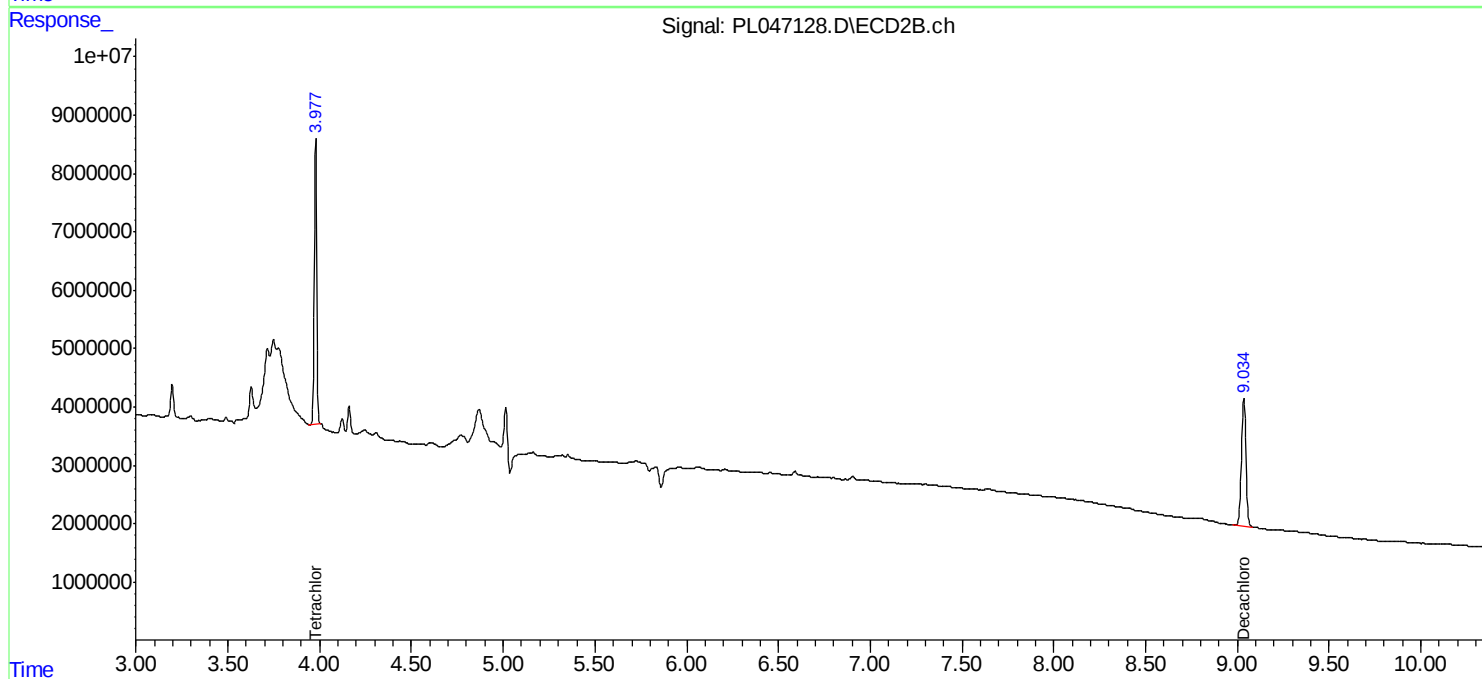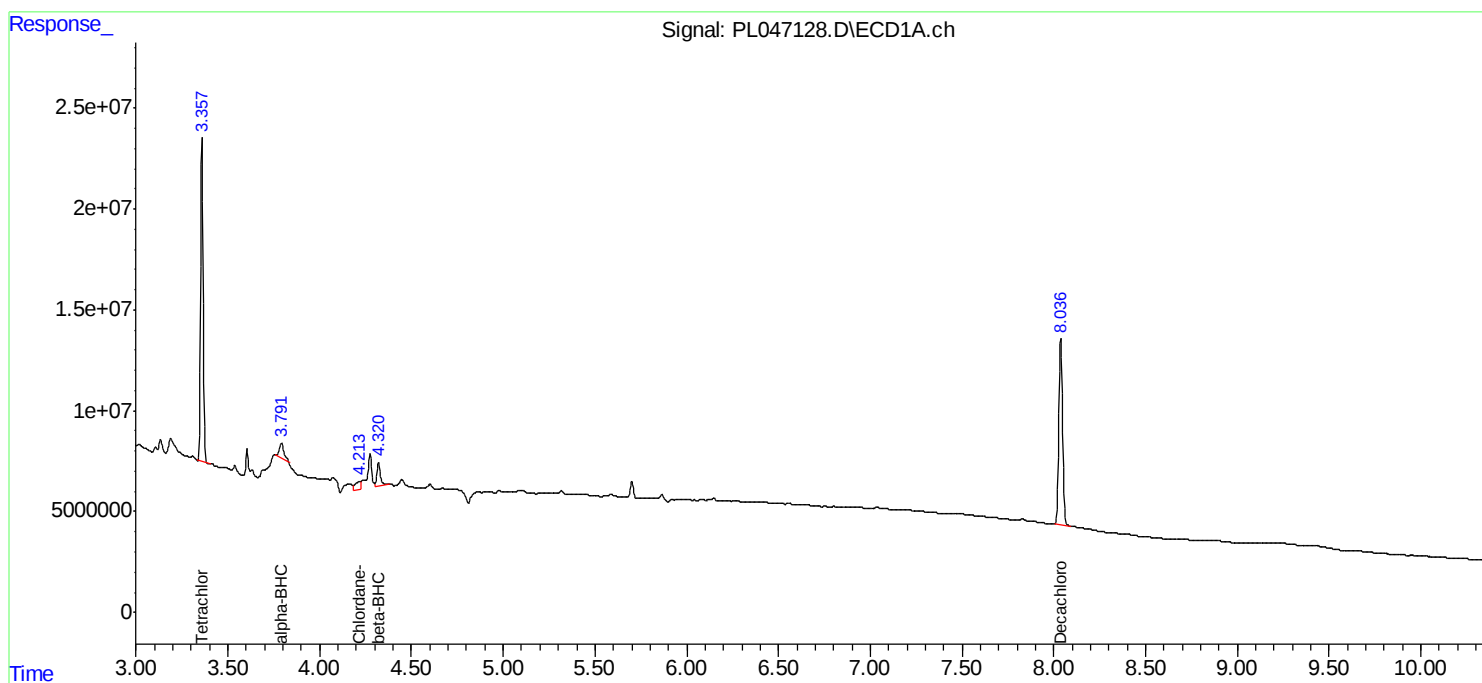


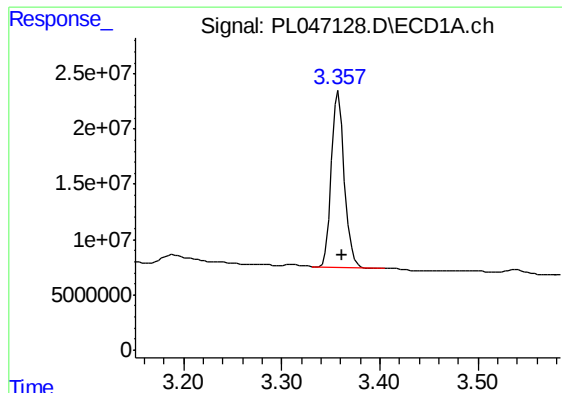

#1 Tetrachloro-m-xylene


R.T.: 3.358 min
Delta R.T.: -0.003 min
Response: 147584707
Conc: 20.29 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-14-S

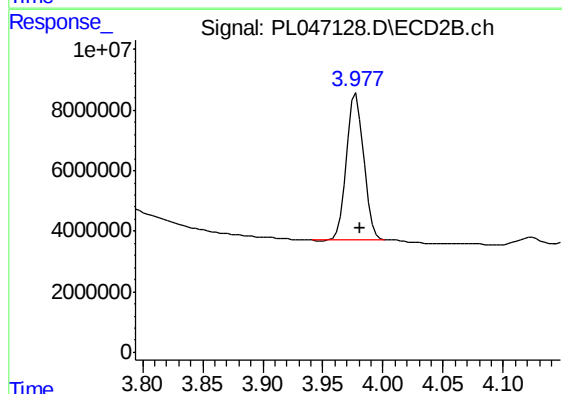


#1 Tetrachloro-m-xylene

R.T.: 3.978 min
Delta R.T.: -0.003 min
Response: 48170255
Conc: 21.04 ng/ml

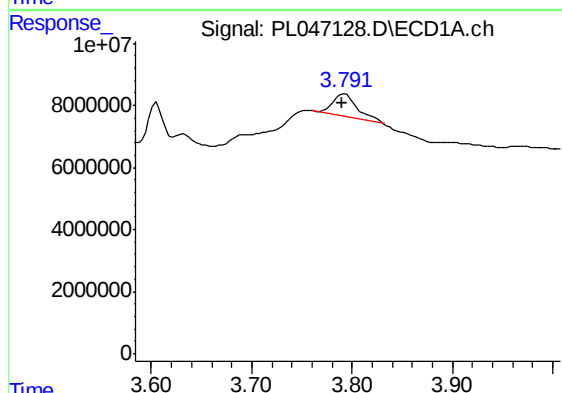


#2 alpha-BHC

R.T.: 3.793 min
Delta R.T.: 0.002 min
Response: 11966306
Conc: 1.03 ng/ml

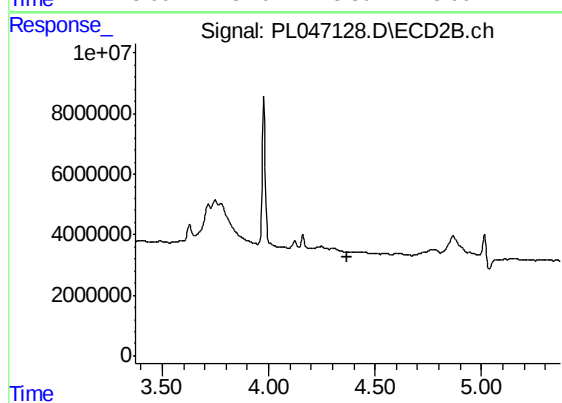

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.371 min
Response: 0
Conc: N.D.

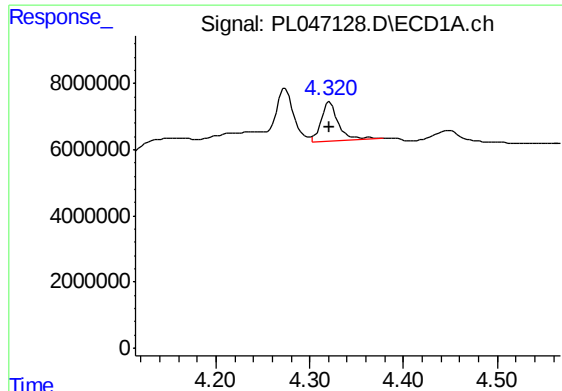

#6 beta-BHC


R.T.: 4.322 min
Delta R.T.: 0.000 min
Response: 15513291
Conc: 3.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-14-S

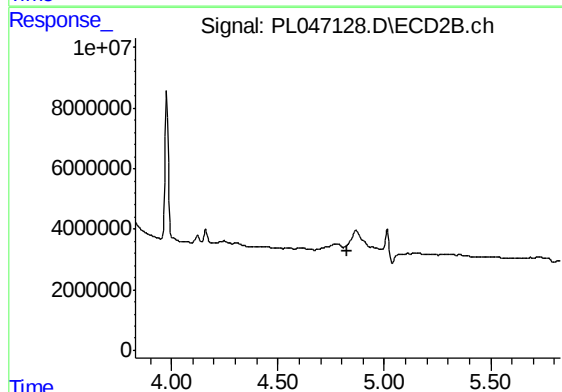


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.828 min
Response: 0
Conc: N.D.

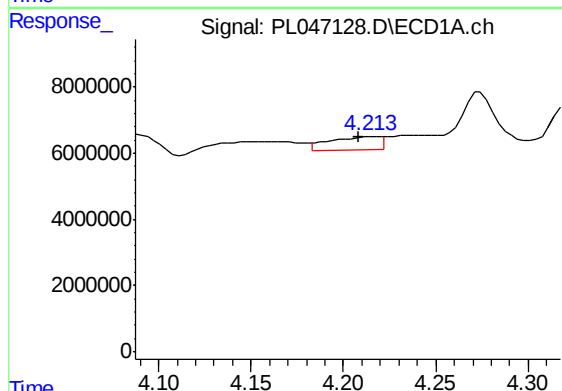


#23 Chlordane-1

R.T.: 4.215 min
Delta R.T.: 0.006 min
Response: 7940416
Conc: 23.61 ng/ml

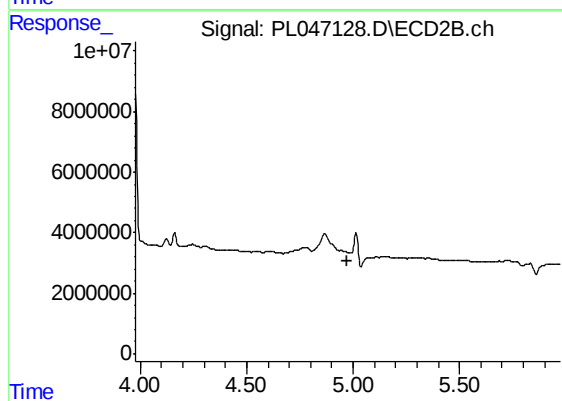

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.975 min
Response: 0
Conc: N.D.

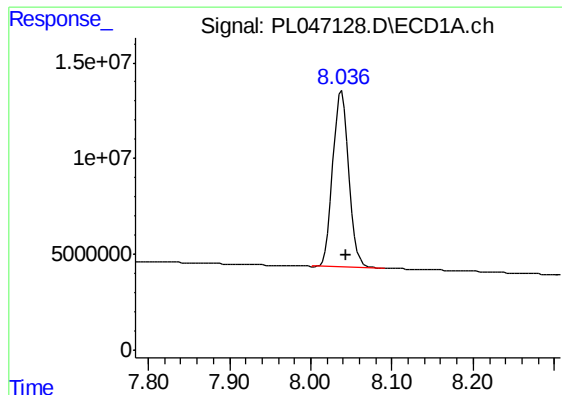

#28 Decachlorobiphenyl

R.T.: 8.038 min
Delta R.T.: -0.006 min
Response: 125751951
Conc: 14.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-14-S

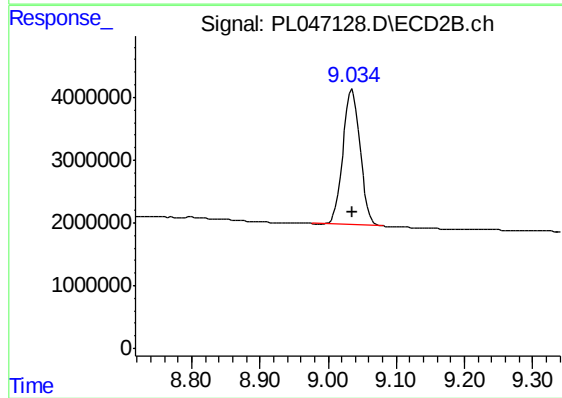

#28 Decachlorobiphenyl

R.T.: 9.035 min
Delta R.T.: 0.000 min
Response: 37982588
Conc: 16.38 ng/ml