

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040919\
 Data File : PL047119.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Apr 2019 15:36
 Operator : AJ\SJ
 Sample : K2316-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 20190169-COMP-CS-1

Manual Integrations
 APPROVED

mohammad
 4/10/2019 3:44:33 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 10 01:02:25 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:40:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.358	3.978	66487263	21033462	9.140	9.186
28) SA Decachlor...	8.038	9.034	64673125	19819665	7.689	8.549
Target Compounds						
12) B 4,4'-DDE	5.474	6.313	2962959	1238195	0.322m	0.499m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040919\
Data File : PL047119.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Apr 2019 15:36
Operator : AJ\SJ
Sample : K2316-01
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
20190169-COMP-CS-1


Manual Integrations
APPROVED

mohammad
4/10/2019 3:44:33 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 10 01:02:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

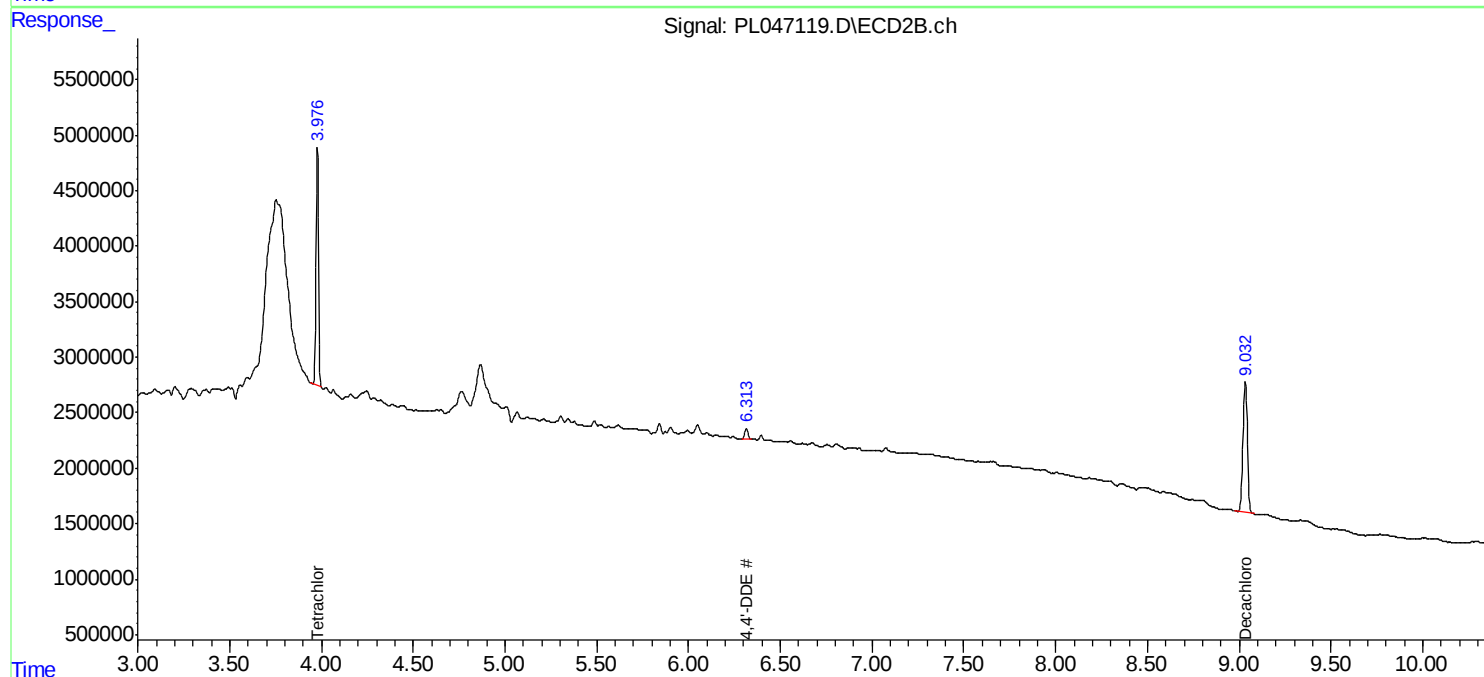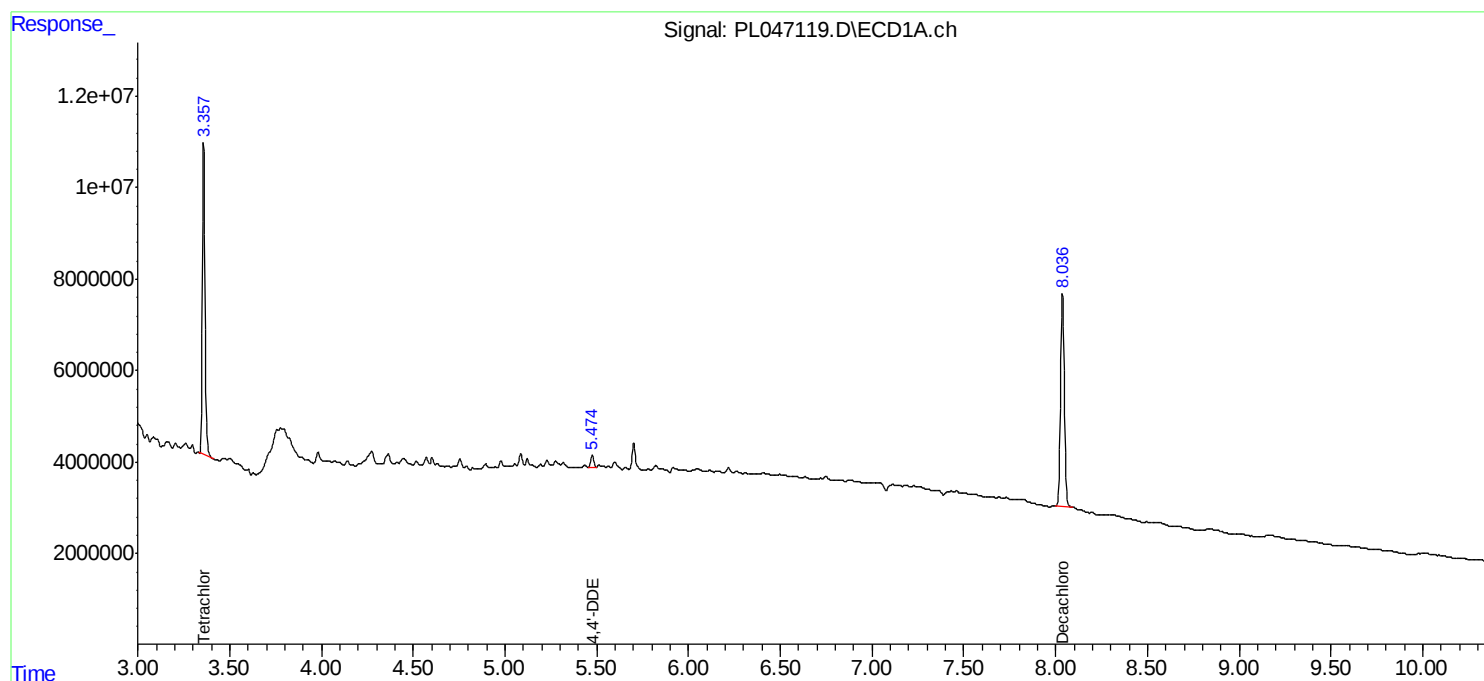

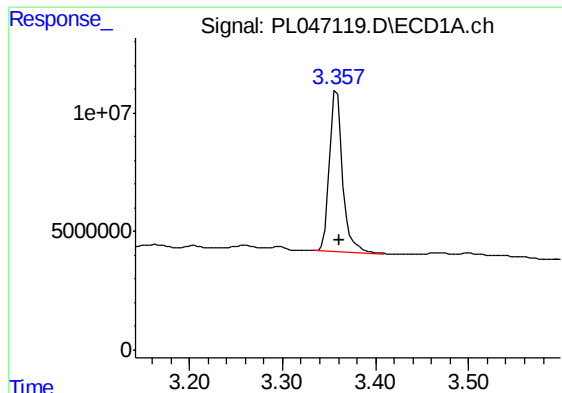


#1 Tetrachloro-m-xylene

R.T.: 3.358 min
Delta R.T.: -0.003 min
Response: 66487263
Conc: 9.14 ng/ml

Instrument :
ECD_L
ClientSampleId :
20190169-COMP-CS-1


Manual Integrations
APPROVED

mohammad
4/10/2019 3:44:33 PM

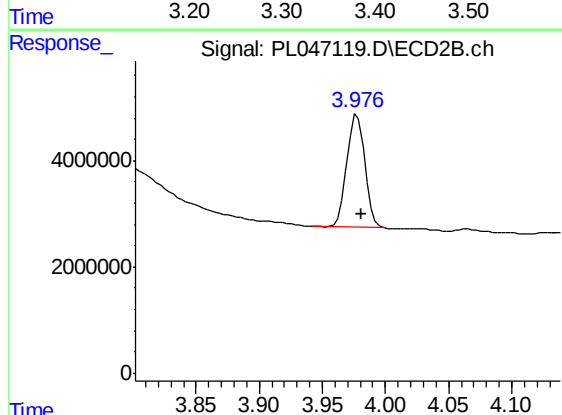


#1 Tetrachloro-m-xylene

R.T.: 3.978 min
Delta R.T.: -0.003 min
Response: 21033462
Conc: 9.19 ng/ml

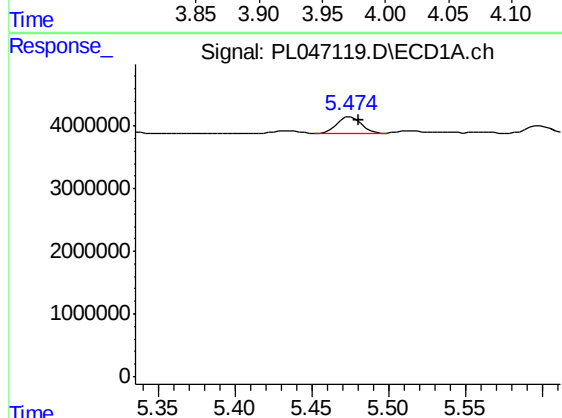


#12 4,4'-DDE

R.T.: 5.474 min
Delta R.T.: -0.006 min
Response: 2962959
Conc: 0.32 ng/ml m

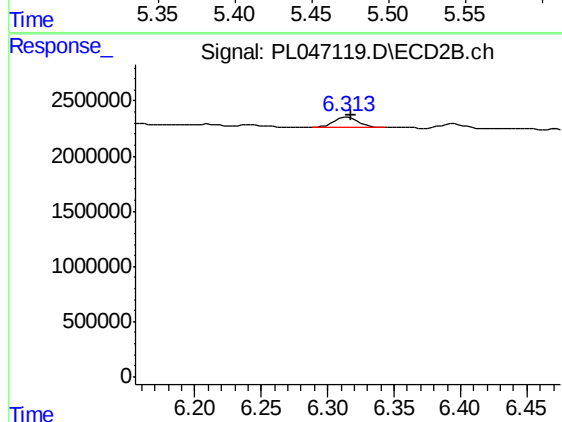

#12 4,4'-DDE

R.T.: 6.313 min
Delta R.T.: -0.005 min
Response: 1238195
Conc: 0.50 ng/ml m

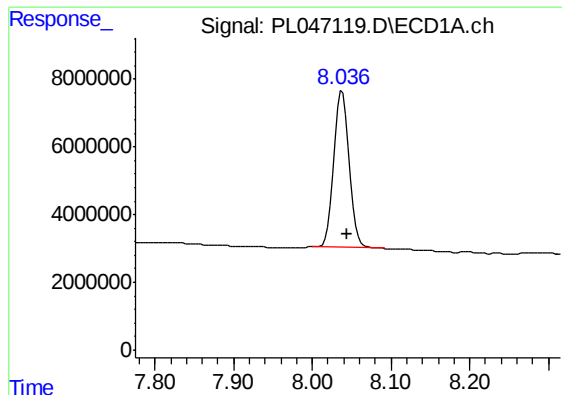


#28 Decachlorobiphenyl

R.T.: 8.038 min
Delta R.T.: -0.006 min
Response: 64673125
Conc: 7.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
20190169-COMP-CS-1

Manual Integrations
APPROVED

mohammad
4/10/2019 3:44:33 PM

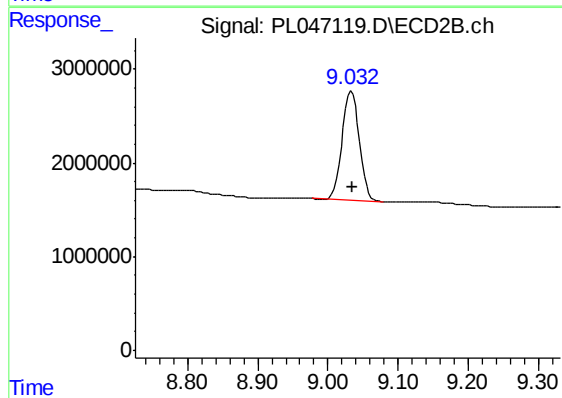

#28 Decachlorobiphenyl

R.T.: 9.034 min
Delta R.T.: -0.001 min
Response: 19819665
Conc: 8.55 ng/ml