

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040919\
 Data File : PL047161.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Apr 2019 02:09
 Operator : AJ\SJ
 Sample : K2316-08
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 20190176-AMND-COMP-CS-3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 10 04:02:01 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:40:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.358	3.977	55392638	18473386	7.614	8.068
28)	SA Decachlor...	8.036	9.032	49273051	14562778	5.858	6.281
Target Compounds							
12)	B 4,4'-DDE	5.474	6.313	7172324	3140364	0.779	1.265 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040919\
Data File : PL047161.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Apr 2019 02:09
Operator : AJ\SJ
Sample : K2316-08
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
20190176-AMND-COMP-CS-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 10 04:02:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

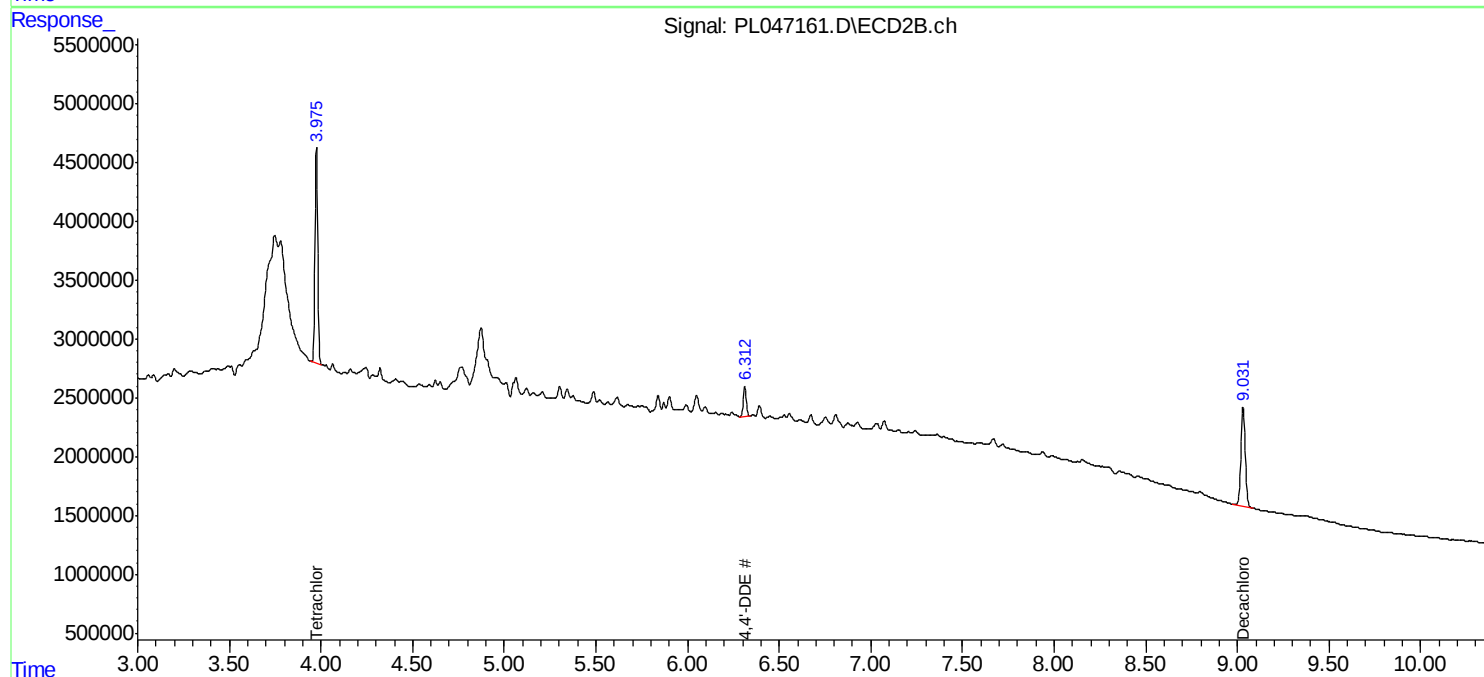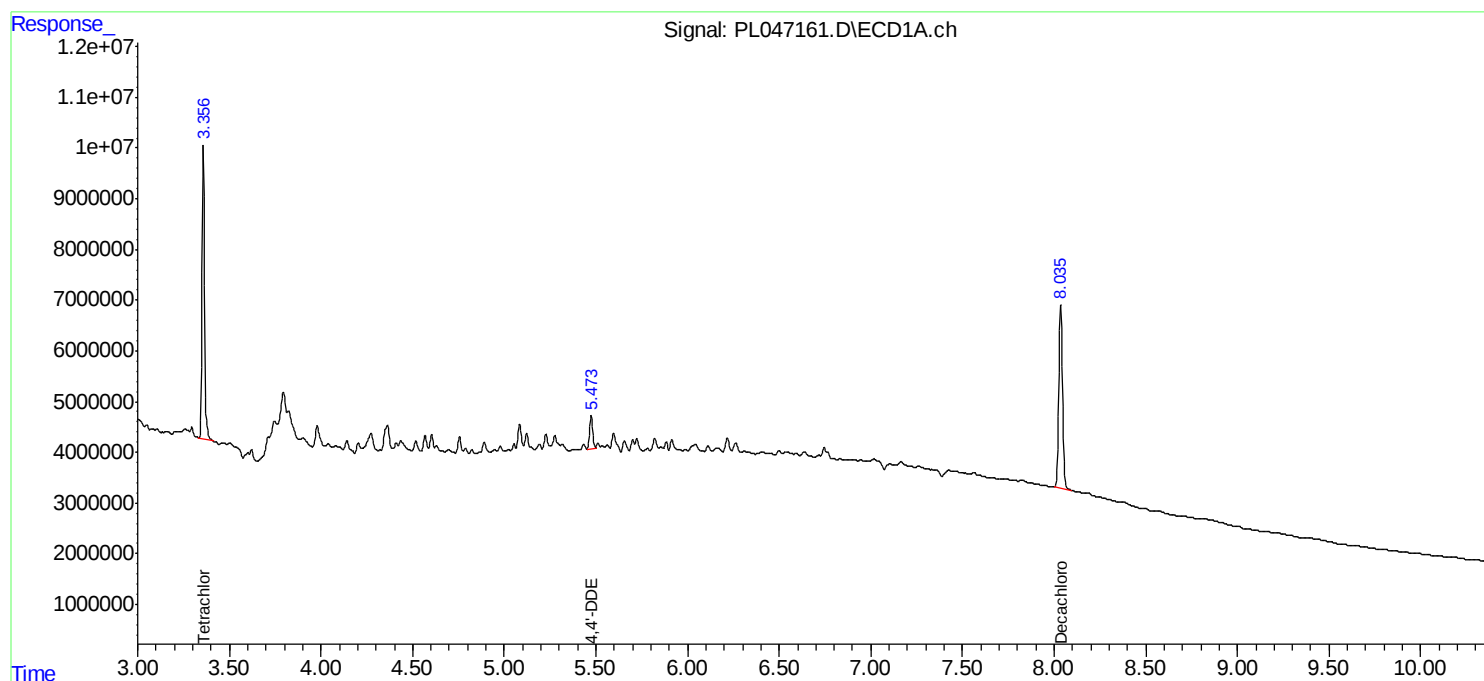


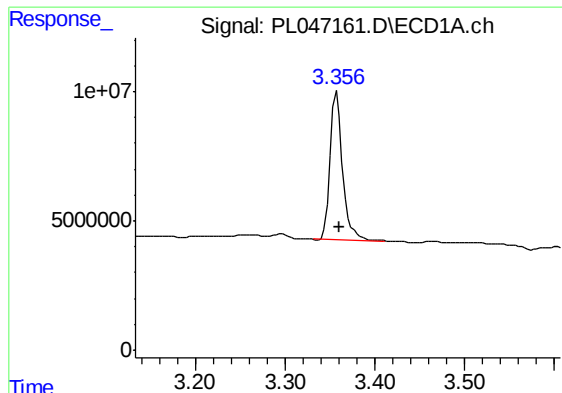

#1 Tetrachloro-m-xylene


R.T.: 3.358 min
Delta R.T.: -0.003 min
Response: 55392638
Conc: 7.61 ng/ml

Instrument :
ECD_L
ClientSampleId :
20190176-AMND-COMP-CS-3

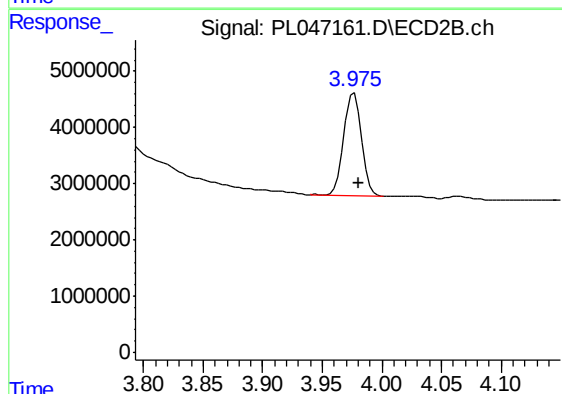


#1 Tetrachloro-m-xylene

R.T.: 3.977 min
Delta R.T.: -0.004 min
Response: 18473386
Conc: 8.07 ng/ml

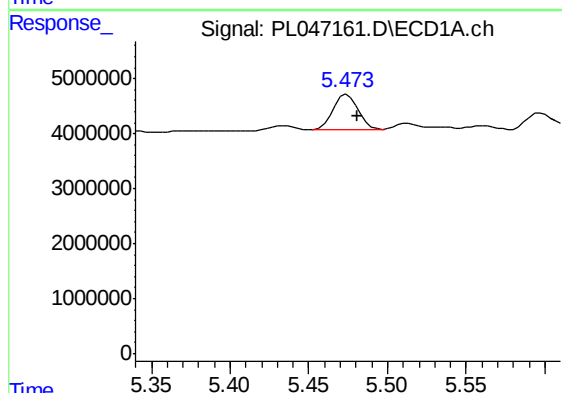


#12 4,4'-DDE

R.T.: 5.474 min
Delta R.T.: -0.006 min
Response: 7172324
Conc: 0.78 ng/ml

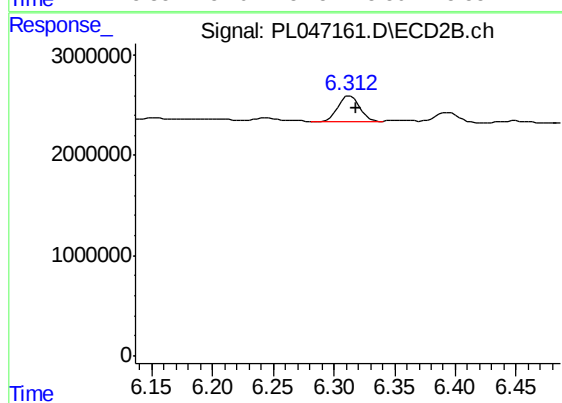

#12 4,4'-DDE


R.T.: 6.313 min
Delta R.T.: -0.005 min
Response: 3140364
Conc: 1.27 ng/ml

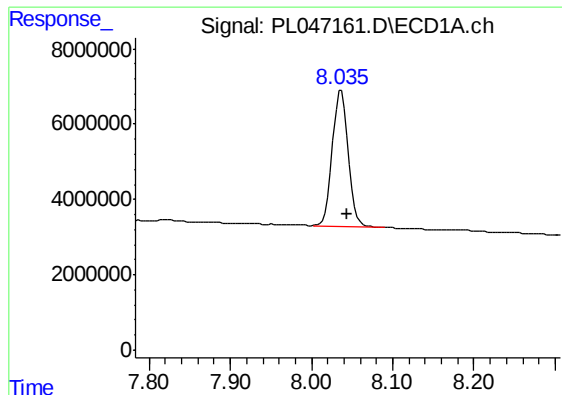

#28 Decachlorobiphenyl

R.T.: 8.036 min
Delta R.T.: -0.008 min
Response: 49273051
Conc: 5.86 ng/ml

Instrument :
ECD_L
ClientSampleId :
20190176-AMND-COMP-CS-3

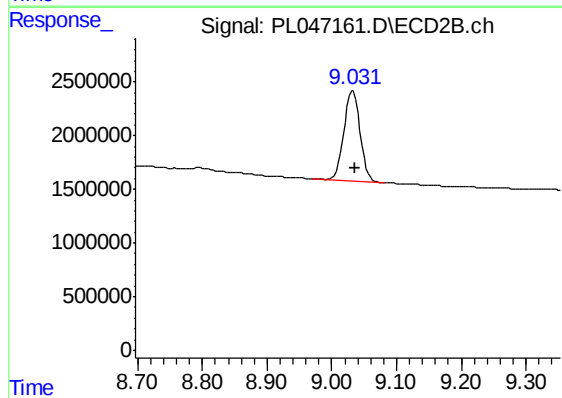

#28 Decachlorobiphenyl

R.T.: 9.032 min
Delta R.T.: -0.003 min
Response: 14562778
Conc: 6.28 ng/ml