

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040921\
 Data File : PL065960.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Apr 2021 18:24
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 10 08:51:10 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040921.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 10 02:10:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.448	4.154	45306516	52969820	18.656	19.217
28)	SA Decachlor...	8.177	9.353	41063224	38170592	19.035	20.137
Target Compounds							
2)	A alpha-BHC	3.873	0.000	3130795	0	0.819	N.D. #
4)	MA Heptachlor	0.000	5.355	0	3074019	N.D.	0.892 #
6)	B beta-BHC	4.425	5.034	4927417	8394601	2.860	1.993 #
8)	B Heptachlo...	0.000	6.072	0	969493	N.D.	0.341 #
12)	B 4,4'-DDE	0.000	6.510f	0	644068	N.D.	0.259 #
14)	MA Endrin	5.979	0.000	841192	0	0.285	N.D. #
15)	B Endosulfa...	0.000	7.123	0	670652	N.D.	0.315 #
19)	B Endosulfa...	6.635	0.000	833416	0	0.271	N.D. #
21)	B Endrin ke...	7.114	7.975	41181379	3292552	12.773	1.458 #
22)	Mirex	0.000	8.443f	0	619252	N.D.	0.368 #
23)	Chlordane-1	4.339f	0.000	2537975	0	24.249	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040921\
Data File : PL065960.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Apr 2021 18:24
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 10 08:51:10 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040921.M
Quant Title : GC Extractables
QLast Update : Sat Apr 10 02:10:31 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

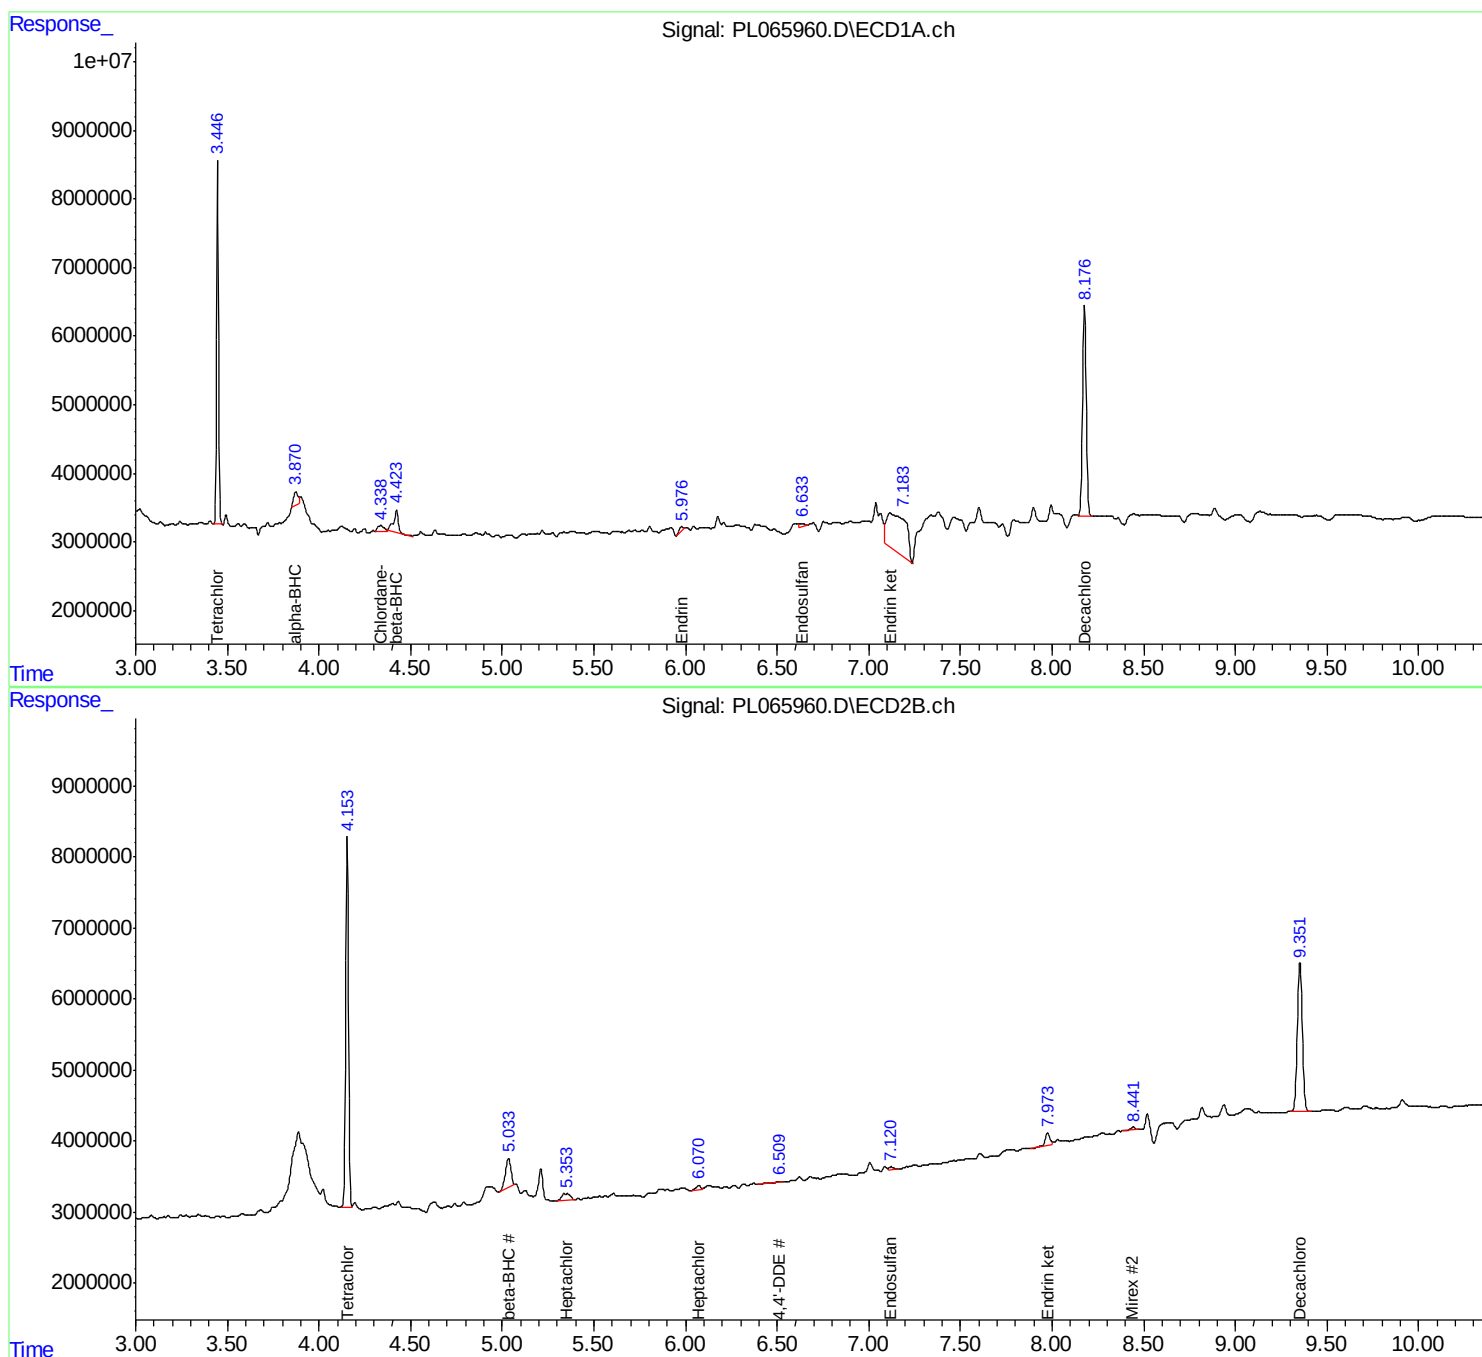

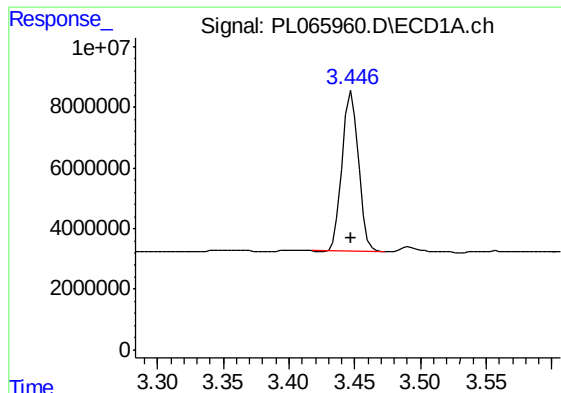


#1 Tetrachloro-m-xylene

R.T.: 3.448 min
Delta R.T.: 0.000 min
Response: 45306516
Conc: 18.66 ng/ml

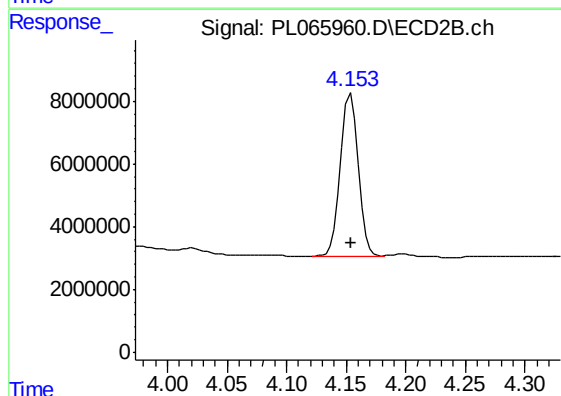


#1 Tetrachloro-m-xylene

R.T.: 4.154 min
Delta R.T.: 0.000 min
Response: 52969820
Conc: 19.22 ng/ml

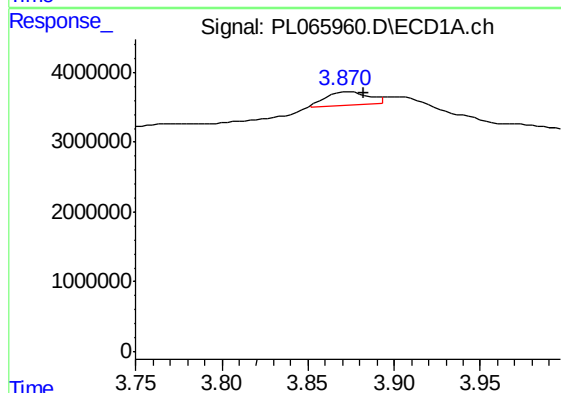


#2 alpha-BHC

R.T.: 3.873 min
Delta R.T.: -0.009 min
Response: 3130795
Conc: 0.82 ng/ml

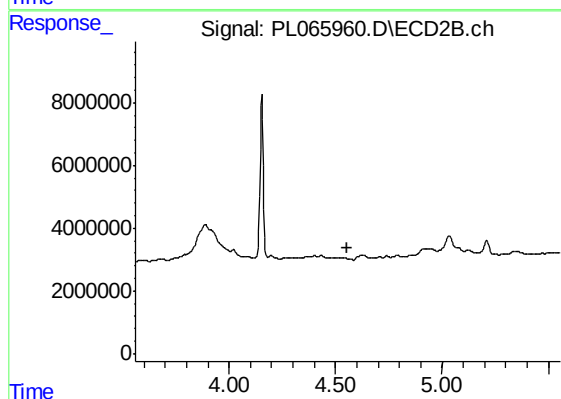


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 4.558 min
Response: 0
Conc: N.D.

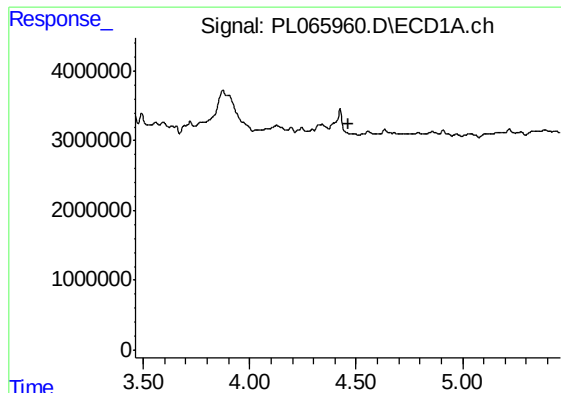


#4 Heptachlor

R.T.: 0.000 min
Exp R.T.: 4.462 min
Response: 0
Conc: N.D.

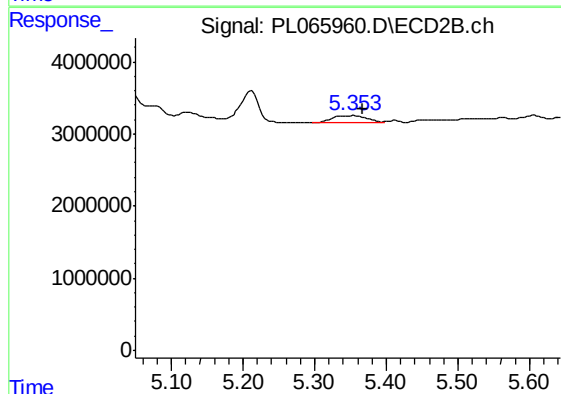


#4 Heptachlor

R.T.: 5.355 min
Delta R.T.: -0.012 min
Response: 3074019
Conc: 0.89 ng/ml

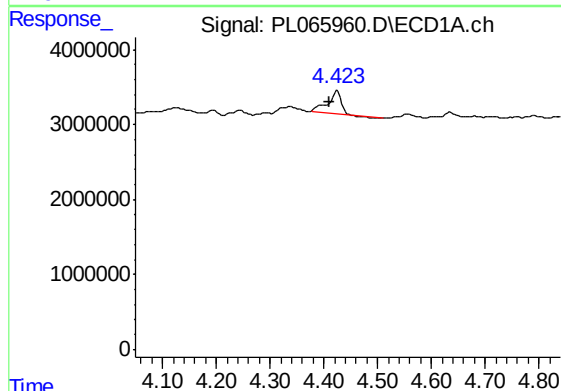


#6 beta-BHC

R.T.: 4.425 min
Delta R.T.: 0.015 min
Response: 4927417
Conc: 2.86 ng/ml

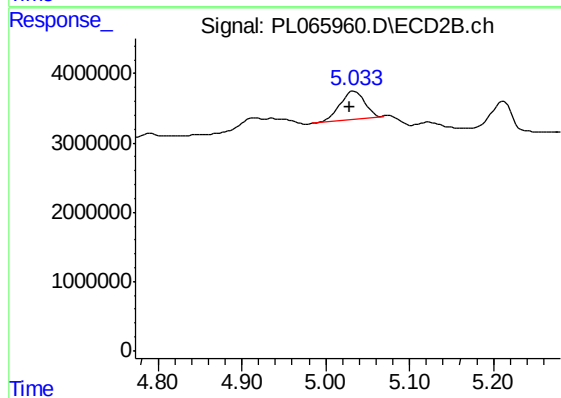


#6 beta-BHC

R.T.: 5.034 min
Delta R.T.: 0.006 min
Response: 8394601
Conc: 1.99 ng/ml

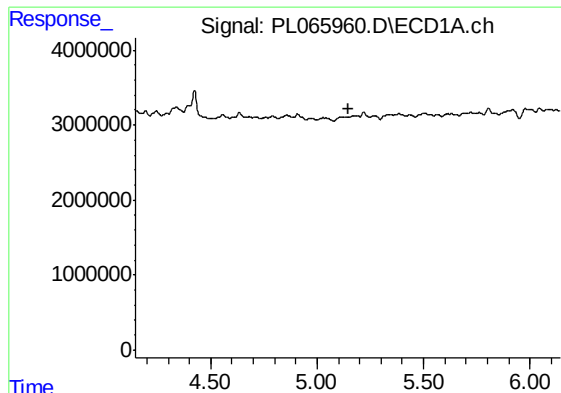


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.146 min
Response: 0
Conc: N.D.

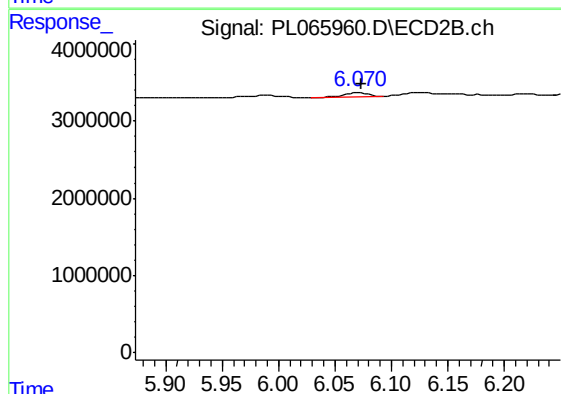


#8 Heptachlor epoxide

R.T.: 6.072 min
Delta R.T.: -0.002 min
Response: 969493
Conc: 0.34 ng/ml

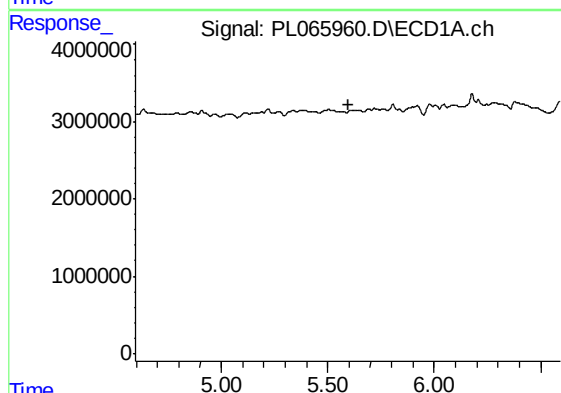


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 5.595 min
Response: 0
Conc: N.D.

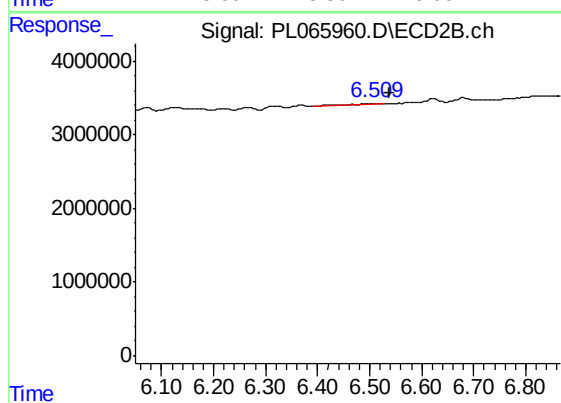


#12 4,4'-DDE

R.T.: 6.510 min
Delta R.T.: -0.029 min
Response: 644068
Conc: 0.26 ng/ml

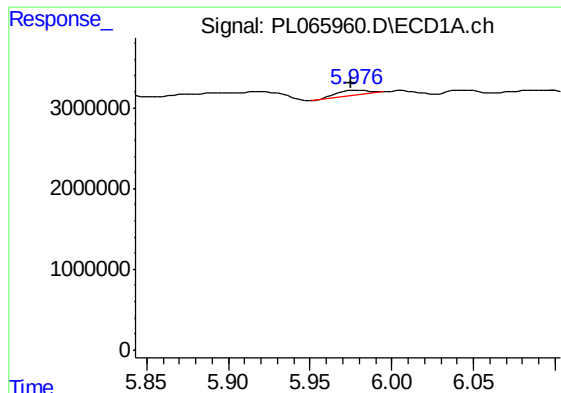


#14 Endrin

R.T.: 5.979 min
Delta R.T.: 0.004 min
Response: 841192
Conc: 0.29 ng/ml

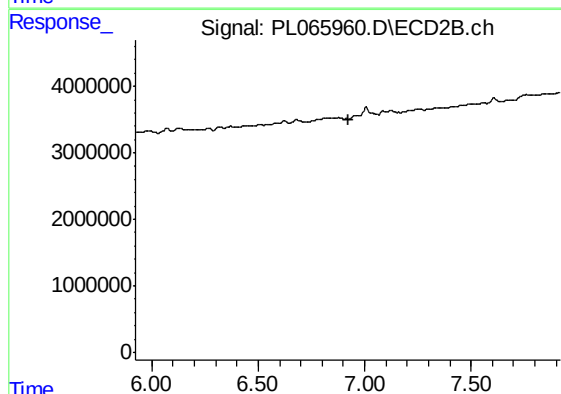


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.922 min
Response: 0
Conc: N.D.

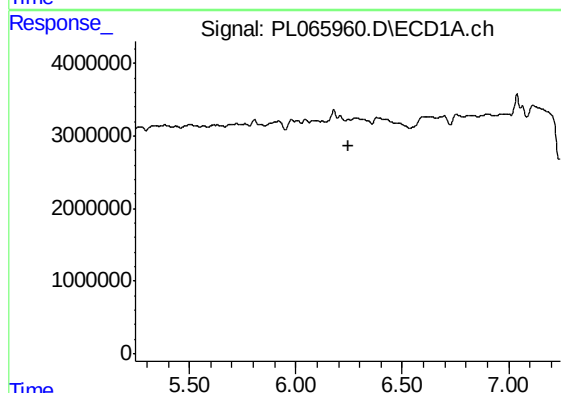


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.246 min
Response: 0
Conc: N.D.

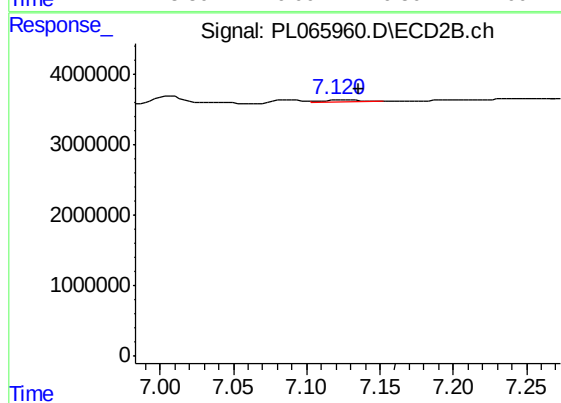


#15 Endosulfan II

R.T.: 7.123 min
Delta R.T.: -0.013 min
Response: 670652
Conc: 0.31 ng/ml

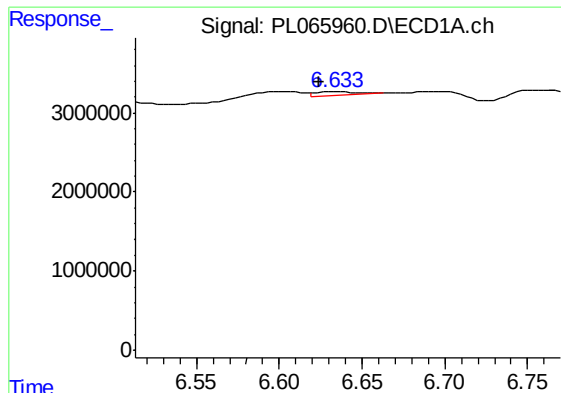


#19 Endosulfan Sulfate

R.T.: 6.635 min
Delta R.T.: 0.010 min
Response: 833416
Conc: 0.27 ng/ml

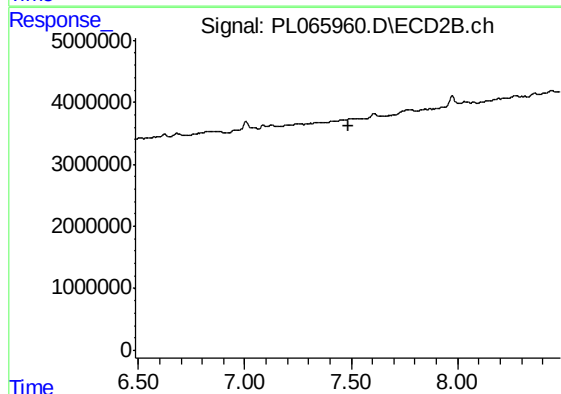


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.486 min
Response: 0
Conc: N.D.

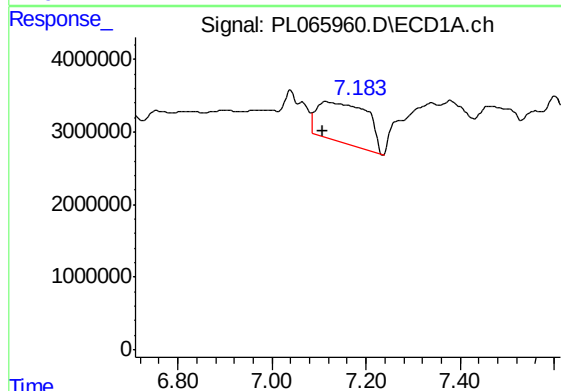


#21 Endrin ketone

R.T.: 7.114 min
Delta R.T.: 0.005 min
Response: 41181379
Conc: 12.77 ng/ml

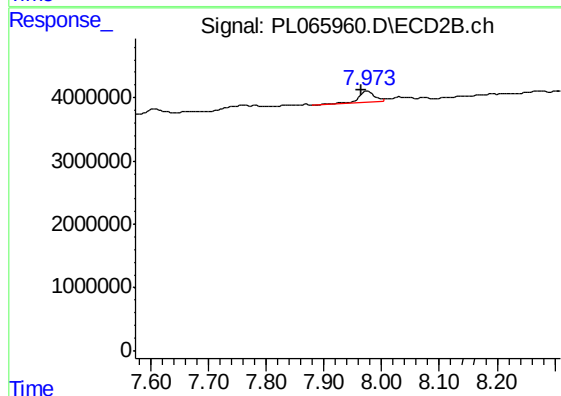


#21 Endrin ketone

R.T.: 7.975 min
Delta R.T.: 0.009 min
Response: 3292552
Conc: 1.46 ng/ml

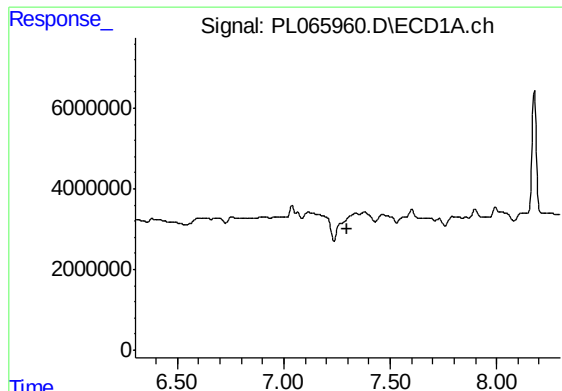


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 7.301 min
Response: 0
Conc: N.D.

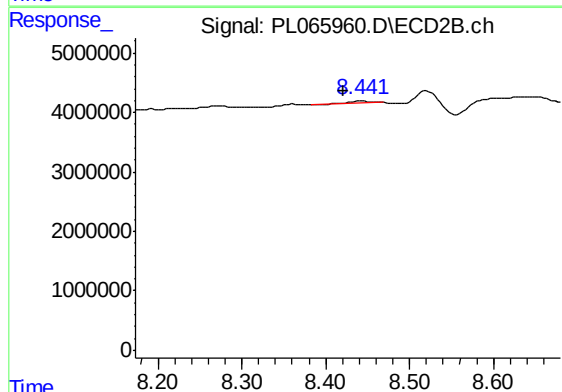


#22 Mirex

R.T.: 8.443 min
Delta R.T.: 0.021 min
Response: 619252
Conc: 0.37 ng/ml

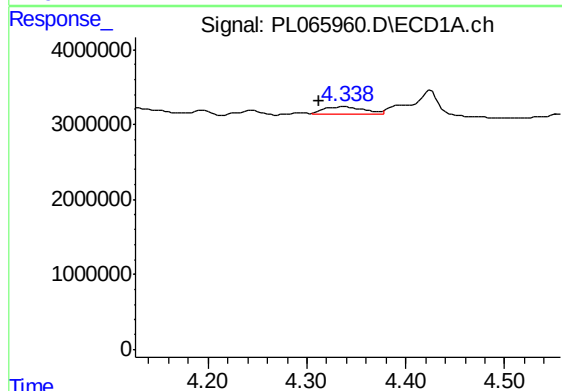


#23 Chlordane-1

R.T.: 4.339 min
Delta R.T.: 0.028 min
Response: 2537975
Conc: 24.25 ng/ml

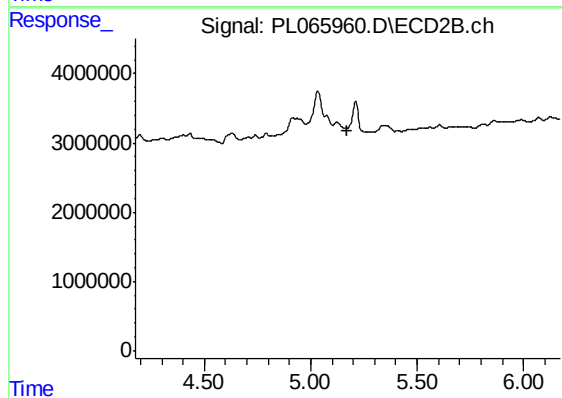


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.175 min
Response: 0
Conc: N.D.

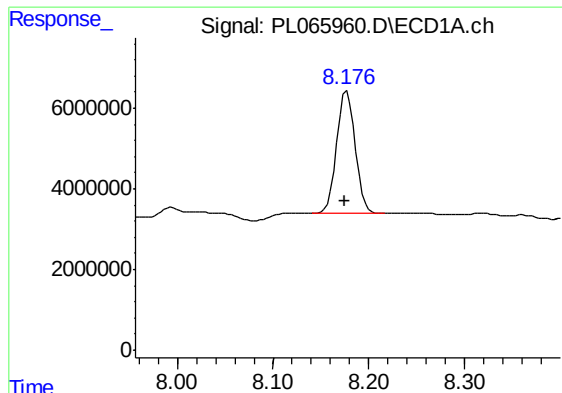

#28 Decachlorobiphenyl

R.T.: 8.177 min
Delta R.T.: 0.002 min
Response: 41063224
Conc: 19.04 ng/ml

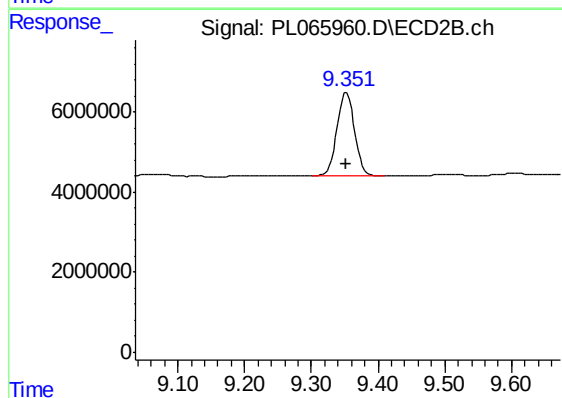

#28 Decachlorobiphenyl

R.T.: 9.353 min
Delta R.T.: 0.001 min
Response: 38170592
Conc: 20.14 ng/ml