

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040921\
 Data File : PL065969.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Apr 2021 20:33
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 10 01:51:37 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040921.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 10 01:51:03 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	3.447	4.154	216.9E6	187.7E6	74.391	67.231
28)	SA Decachlor...	8.175	9.352	152.5E6	138.6E6	71.356	71.763
Target Compounds							
23)	Chlordane-1	4.311	5.175	75874990	76004171	723.916	651.110
24)	Chlordane-2	4.808	5.652	87046135	76495890	718.192	652.210
25)	Chlordane-3	5.372	6.311	249.9E6	272.5E6	747.222	656.641
26)	Chlordane-4	5.430	6.385	206.5E6	349.3E6	741.125	708.202
27)	Chlordane-5	6.255	7.207	93300016	61644913	726.887	724.792


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040921\
Data File : PL065969.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Apr 2021 20:33
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 10 01:51:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040921.M
Quant Title : GC Extractables
QLast Update : Sat Apr 10 01:51:03 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

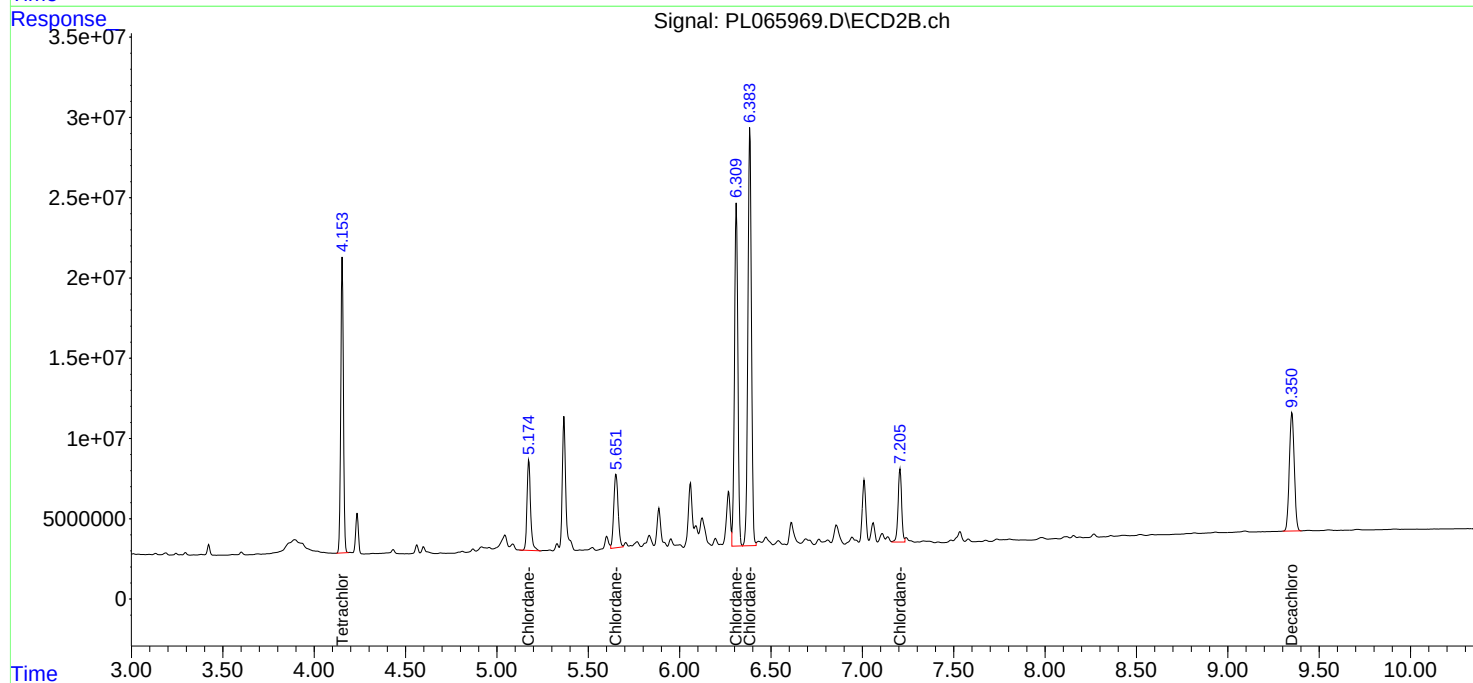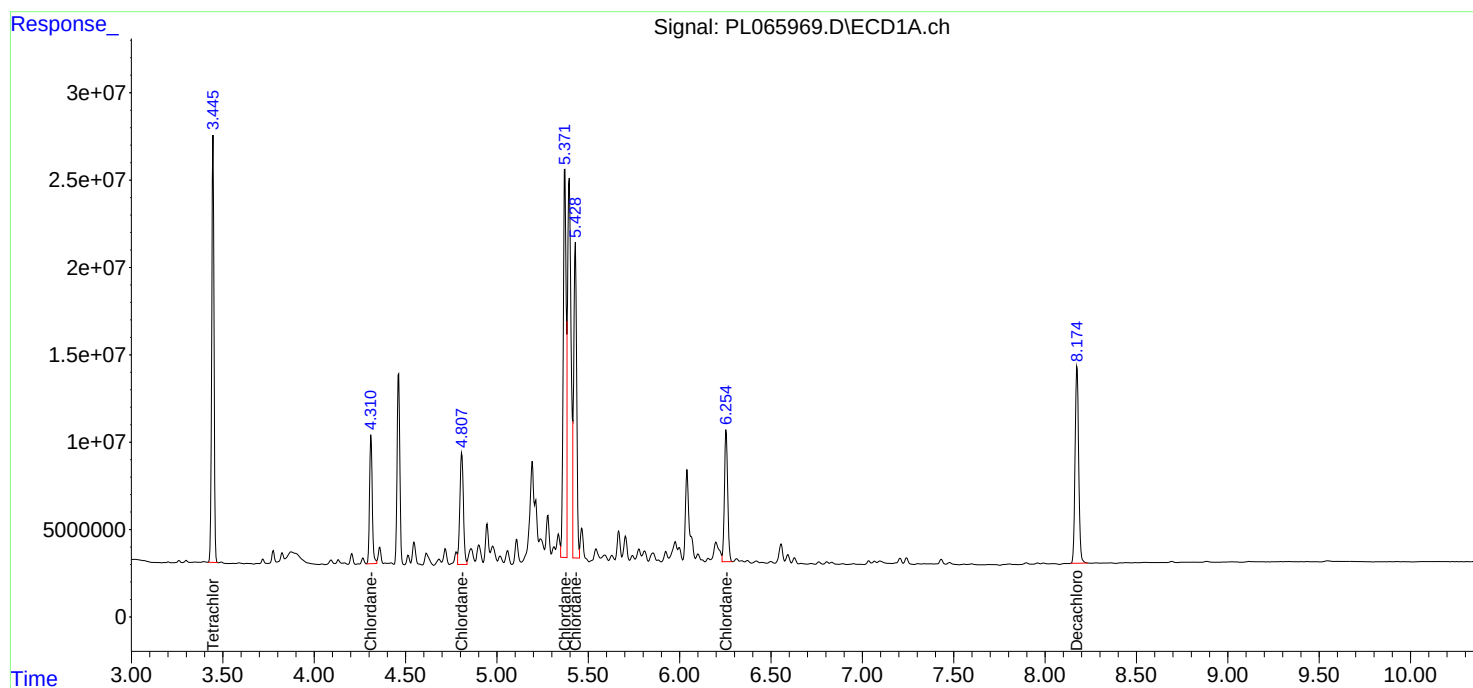

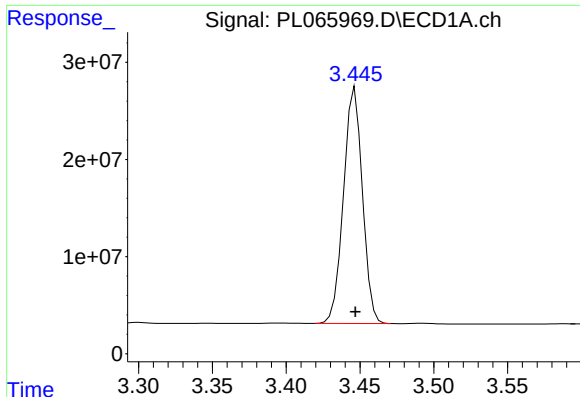


#1 Tetrachloro-m-xylene

R.T.: 3.447 min
Delta R.T.: 0.000 min
Response: 216872118
Conc: 74.39 ng/ml

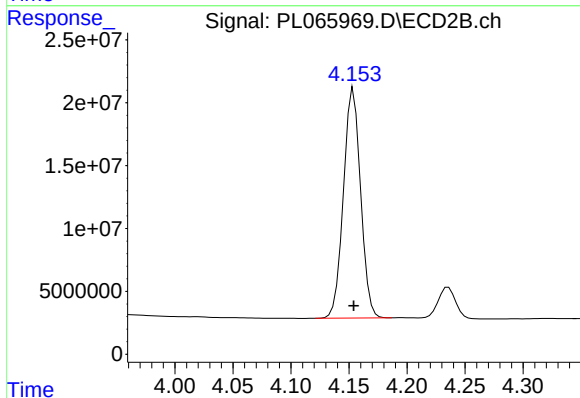


#1 Tetrachloro-m-xylene

R.T.: 4.154 min
Delta R.T.: 0.000 min
Response: 187674249
Conc: 67.23 ng/ml

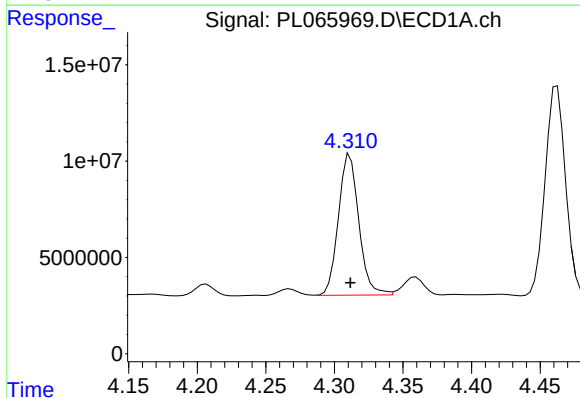


#23 Chlordane-1

R.T.: 4.311 min
Delta R.T.: 0.000 min
Response: 75874990
Conc: 723.92 ng/ml

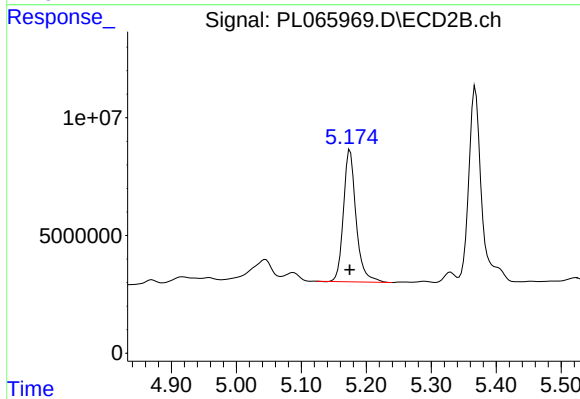


#23 Chlordane-1

R.T.: 5.175 min
Delta R.T.: 0.000 min
Response: 76004171
Conc: 651.11 ng/ml

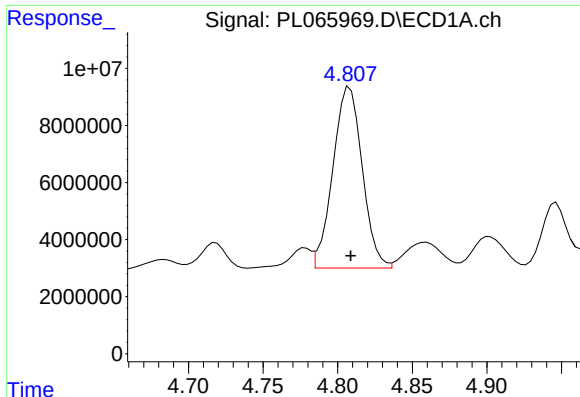


#24 Chlordane-2

R.T.: 4.808 min
Delta R.T.: 0.000 min
Response: 87046135
Conc: 718.19 ng/ml

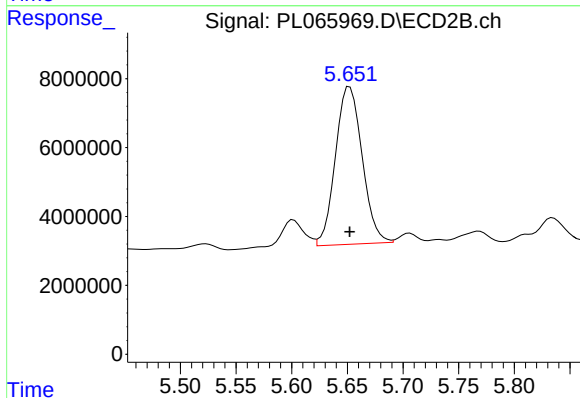


#24 Chlordane-2

R.T.: 5.652 min
Delta R.T.: 0.000 min
Response: 76495890
Conc: 652.21 ng/ml

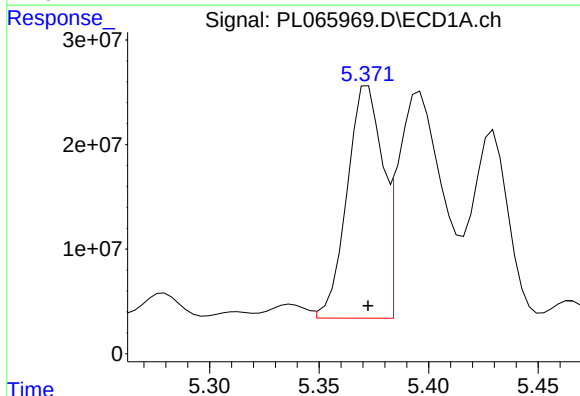


#25 Chlordane-3

R.T.: 5.372 min
Delta R.T.: 0.000 min
Response: 249905352
Conc: 747.22 ng/ml

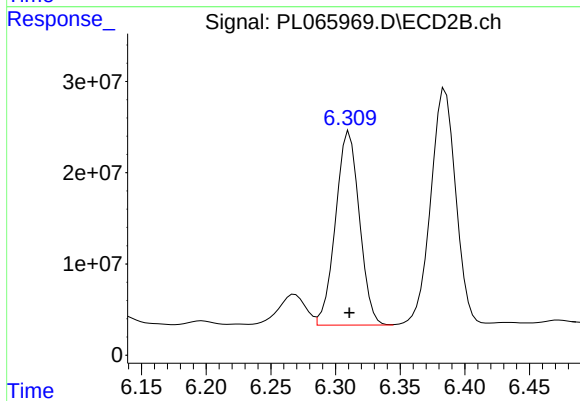


#25 Chlordane-3

R.T.: 6.311 min
Delta R.T.: 0.000 min
Response: 272475405
Conc: 656.64 ng/ml

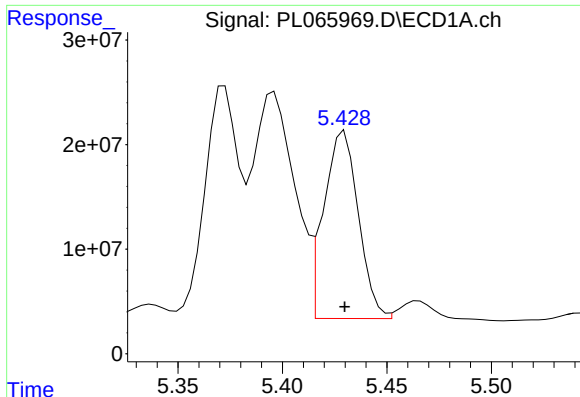


#26 Chlordane-4

R.T.: 5.430 min
Delta R.T.: 0.000 min
Response: 206549550
Conc: 741.13 ng/ml

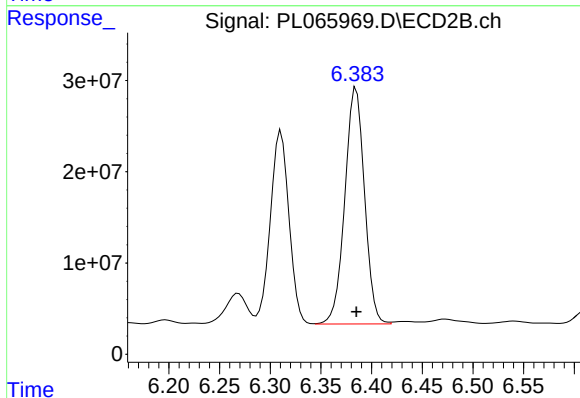


#26 Chlordane-4

R.T.: 6.385 min
Delta R.T.: 0.000 min
Response: 349265828
Conc: 708.20 ng/ml

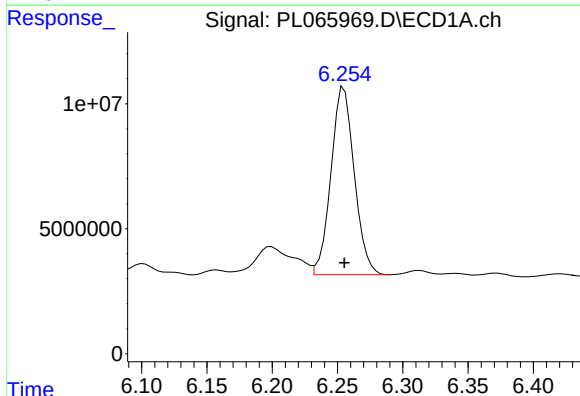


#27 Chlordane-5

R.T.: 6.255 min
Delta R.T.: 0.000 min
Response: 93300016
Conc: 726.89 ng/ml

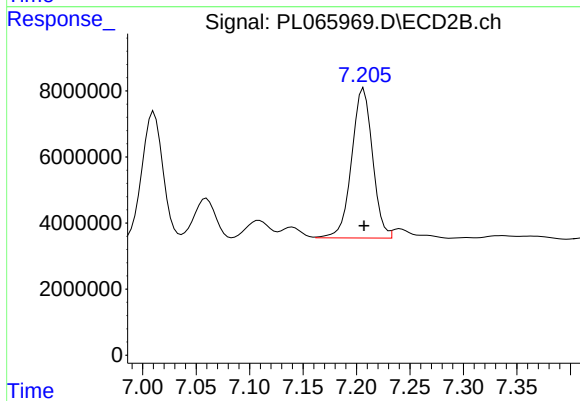

#27 Chlordane-5

R.T.: 7.207 min
Delta R.T.: 0.000 min
Response: 61644913
Conc: 724.79 ng/ml

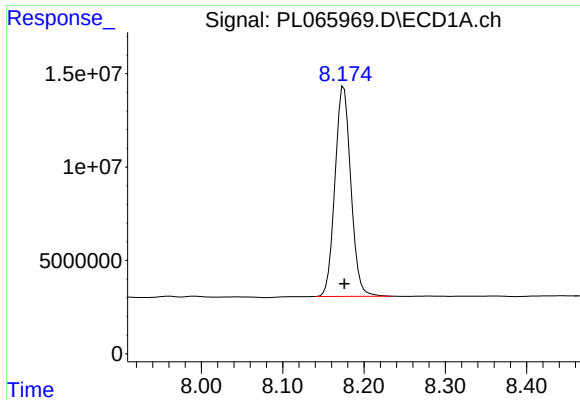


#28 Decachlorobiphenyl

R.T.: 8.175 min

Delta R.T.: 0.000 min

Response: 152461758

Conc: 71.36 ng/ml

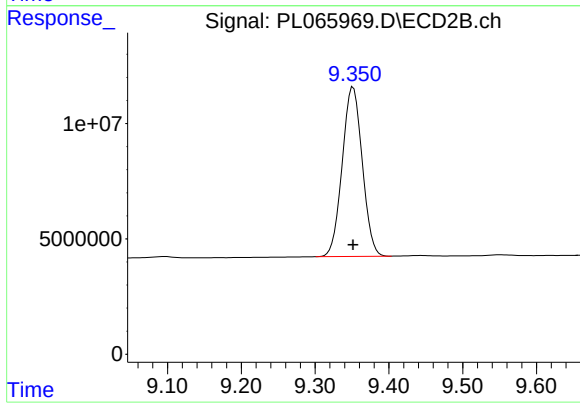

#28 Decachlorobiphenyl

R.T.: 9.352 min

Delta R.T.: 0.000 min

Response: 138566446

Conc: 71.76 ng/ml