

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040921\
 Data File : PL065971.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Apr 2021 21:02
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 10 01:52:07 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040921.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 10 01:51:03 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	3.446	4.154	69948713	68042876	23.994	24.375
28)	SA Decachlor...	8.175	9.351	55447324	50716785	25.951	26.266
Target Compounds							
23)	Chlordane-1	4.311	5.174	26383622	30121594	251.724	258.045
24)	Chlordane-2	4.808	5.652	31626714	29908393	260.943	255.001
25)	Chlordane-3	5.372	6.310	80383996	101.0E6	240.350	243.467
26)	Chlordane-4	5.430	6.384	68146678	122.1E6	244.519	247.520
27)	Chlordane-5	6.254	7.206	32187115	19612279	250.765	230.592


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040921\
Data File : PL065971.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Apr 2021 21:02
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 10 01:52:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040921.M
Quant Title : GC Extractables
QLast Update : Sat Apr 10 01:51:03 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

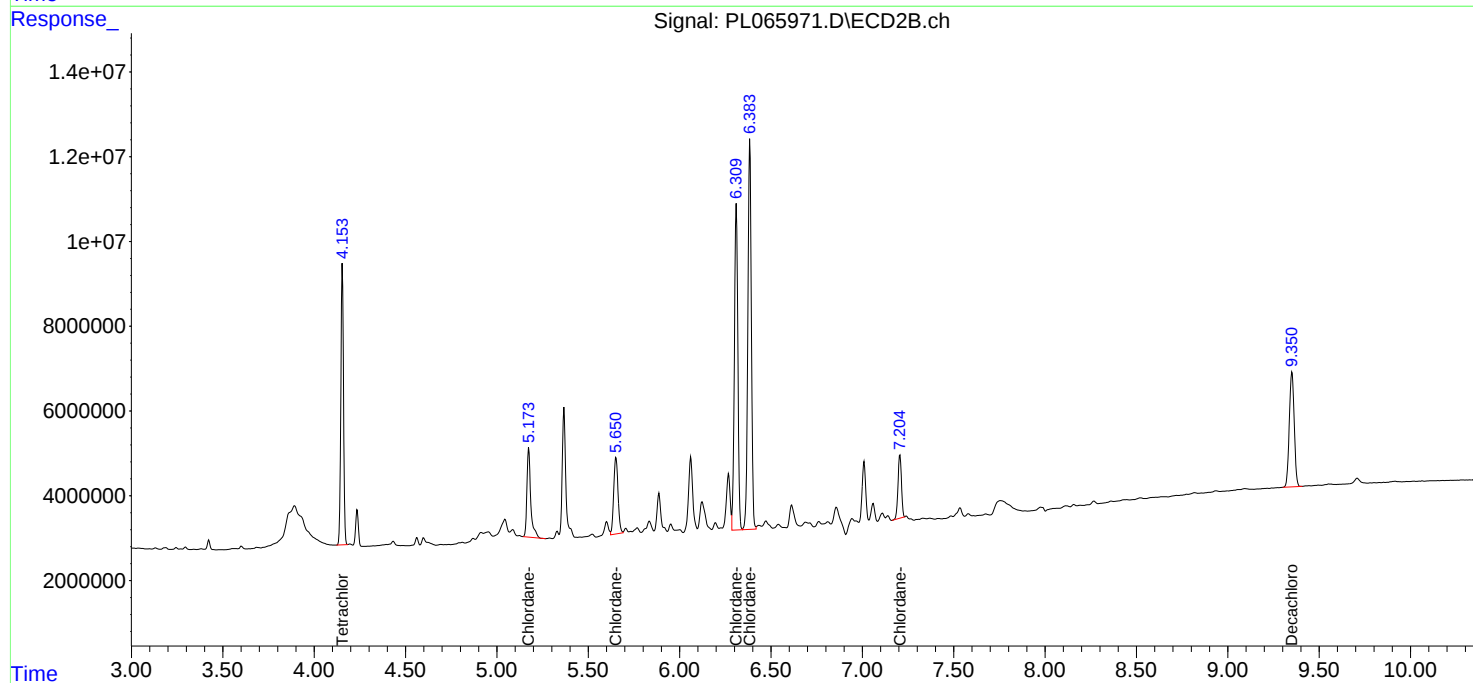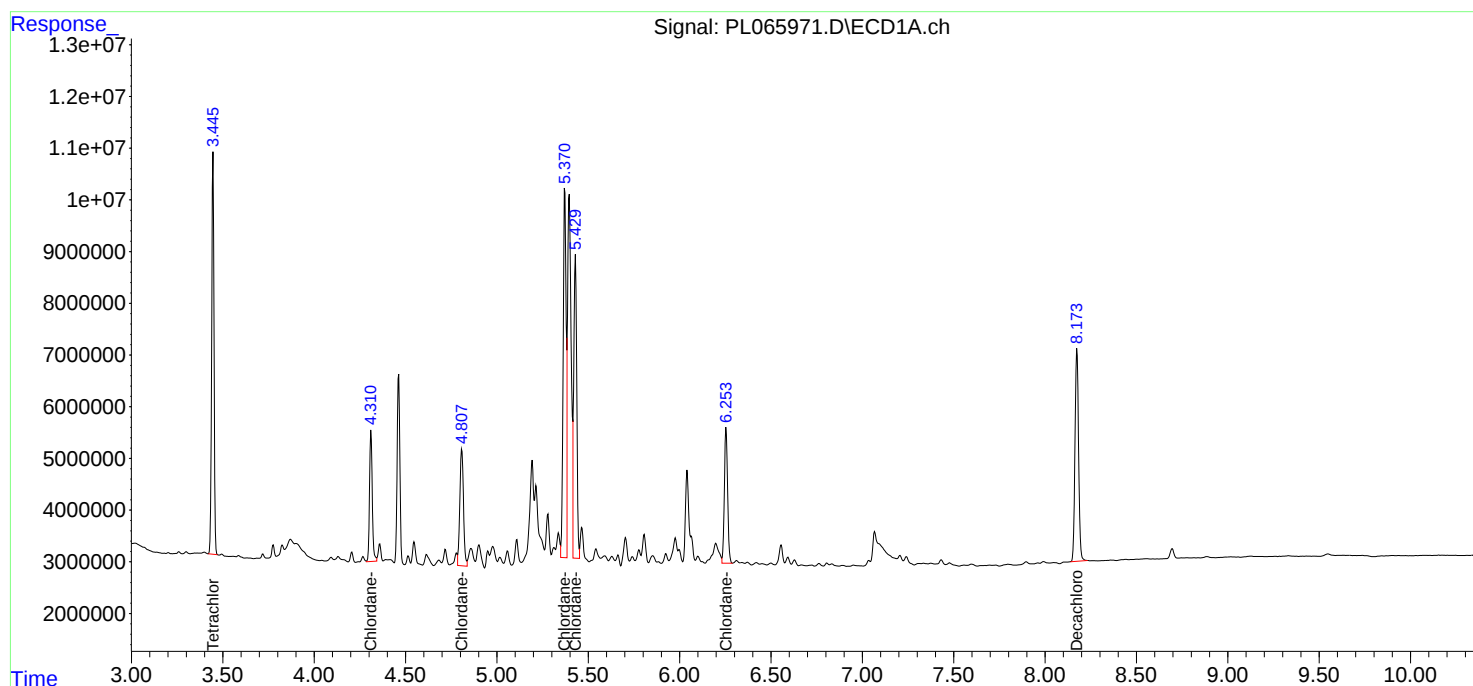

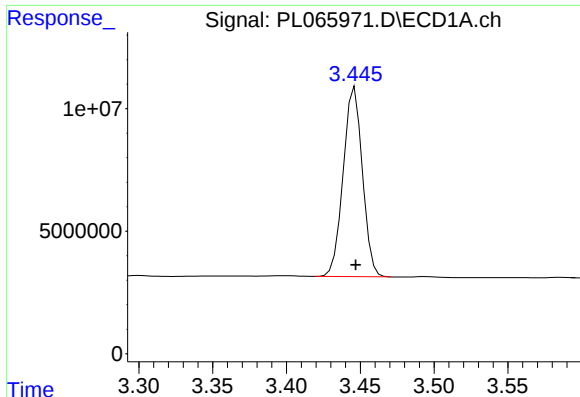


#1 Tetrachloro-m-xylene

R.T.: 3.446 min
Delta R.T.: 0.000 min
Response: 69948713
Conc: 23.99 ng/ml

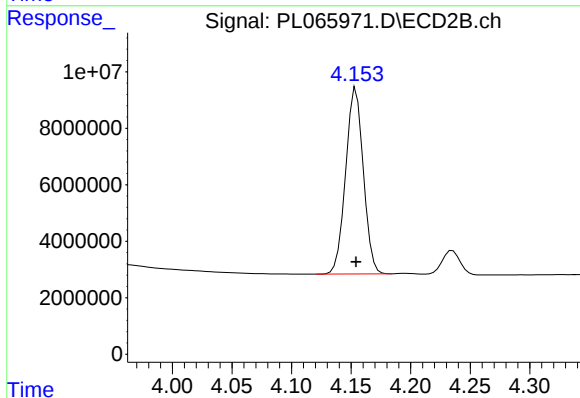


#1 Tetrachloro-m-xylene

R.T.: 4.154 min
Delta R.T.: 0.000 min
Response: 68042876
Conc: 24.38 ng/ml

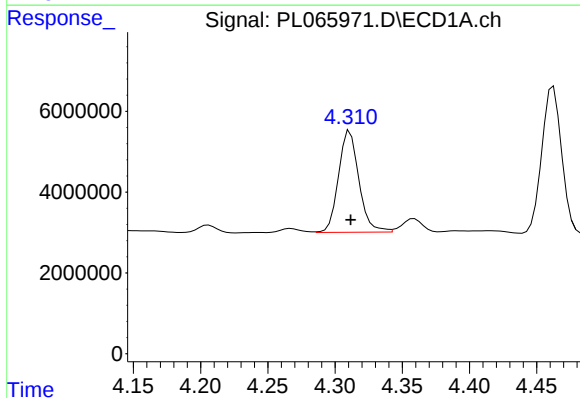


#23 Chlordane-1

R.T.: 4.311 min
Delta R.T.: 0.000 min
Response: 26383622
Conc: 251.72 ng/ml

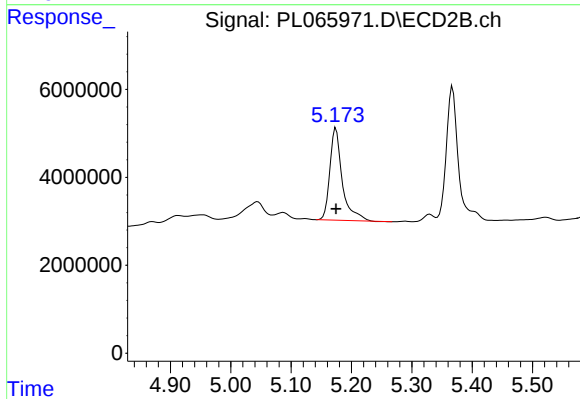


#23 Chlordane-1

R.T.: 5.174 min
Delta R.T.: 0.000 min
Response: 30121594
Conc: 258.04 ng/ml

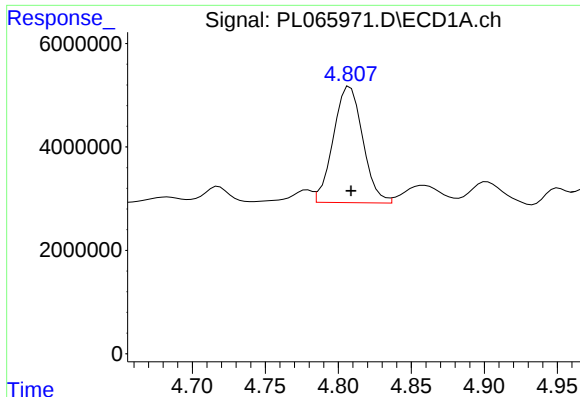


#24 Chlordane-2

R.T.: 4.808 min
Delta R.T.: 0.000 min
Response: 31626714
Conc: 260.94 ng/ml

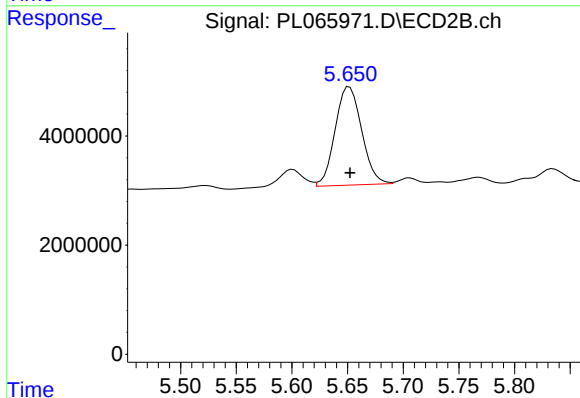


#24 Chlordane-2

R.T.: 5.652 min
Delta R.T.: 0.000 min
Response: 29908393
Conc: 255.00 ng/ml

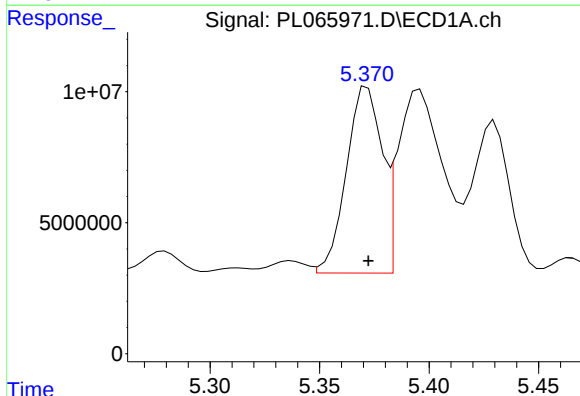


#25 Chlordane-3

R.T.: 5.372 min
Delta R.T.: 0.000 min
Response: 80383996
Conc: 240.35 ng/ml

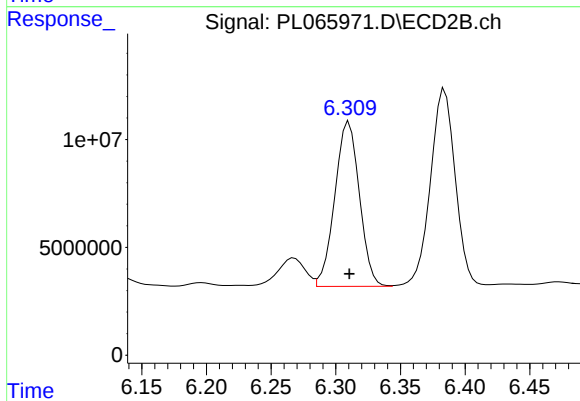


#25 Chlordane-3

R.T.: 6.310 min
Delta R.T.: 0.000 min
Response: 101027551
Conc: 243.47 ng/ml

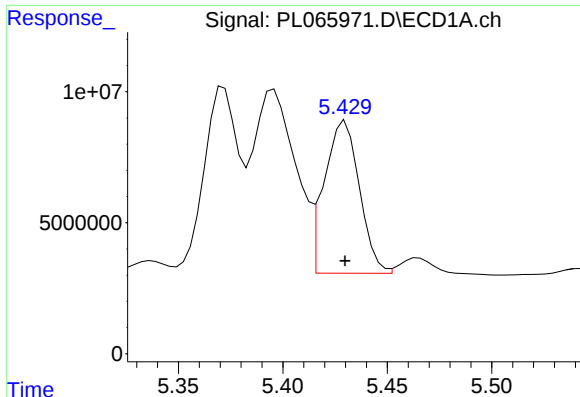


#26 Chlordane-4

R.T.: 5.430 min
Delta R.T.: 0.000 min
Response: 68146678
Conc: 244.52 ng/ml

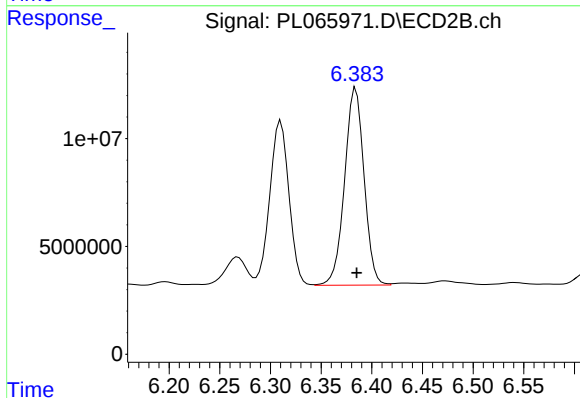


#26 Chlordane-4

R.T.: 6.384 min
Delta R.T.: 0.000 min
Response: 122070170
Conc: 247.52 ng/ml

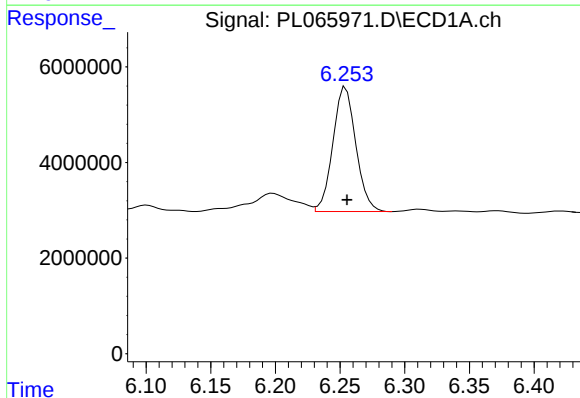


#27 Chlordane-5

R.T.: 6.254 min
Delta R.T.: 0.000 min
Response: 32187115
Conc: 250.77 ng/ml

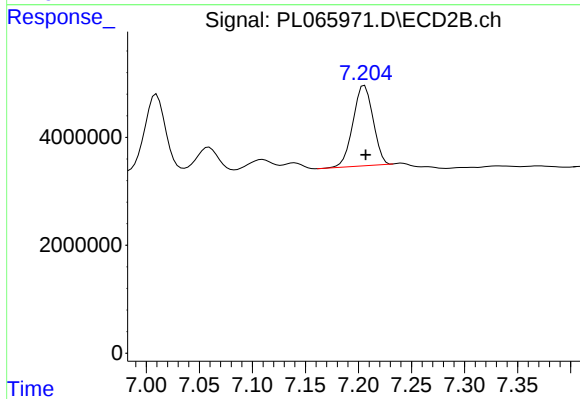


#27 Chlordane-5

R.T.: 7.206 min
Delta R.T.: -0.001 min
Response: 19612279
Conc: 230.59 ng/ml

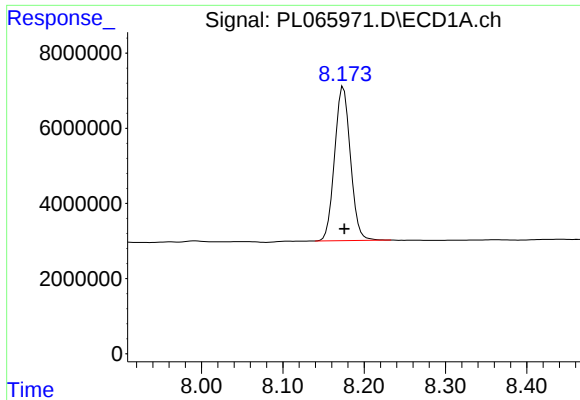

#28 Decachlorobiphenyl

R.T.: 8.175 min
Delta R.T.: -0.001 min
Response: 55447324
Conc: 25.95 ng/ml

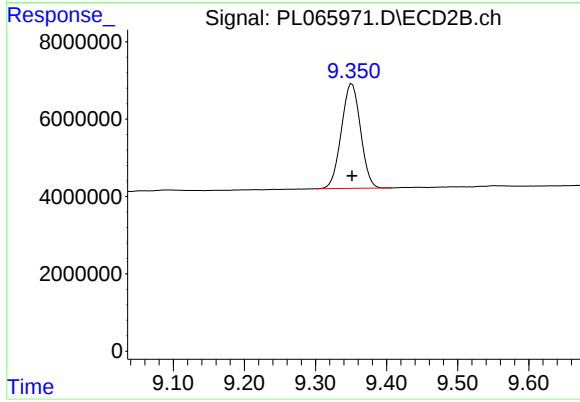

#28 Decachlorobiphenyl

R.T.: 9.351 min
Delta R.T.: 0.000 min
Response: 50716785
Conc: 26.27 ng/ml