

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040921\
 Data File : PL065987.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Apr 2021 04:12
 Operator : AR\AJ
 Sample : M1874-01
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 10 08:54:45 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040921.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 10 02:10:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	3.448	4.154	54182046	65544996	22.311	23.780
28)	SA Decachlor...	8.175	9.352	49208700	48245827	22.811	25.453
Target Compounds							
4)	MA Heptachlor	0.000	5.352	0	1417769	N.D.	0.412 #
8)	B Heptachlo...	0.000	6.068	0	995465	N.D.	0.350 #
12)	B 4,4'-DDE	0.000	6.544	0	1359328	N.D.	0.546 #
15)	B Endosulfa...	0.000	7.127	0	482962	N.D.	0.227 #
17)	MA 4,4'-DDT	0.000	7.337	0	2014831	N.D.	1.063 #
21)	B Endrin ke...	0.000	7.973	0	901337	N.D.	0.399 #
23)	Chlordane-1	4.329f	0.000	2723033	0	26.017	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040921\
Data File : PL065987.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Apr 2021 04:12
Operator : AR\AJ
Sample : M1874-01
Misc :
ALS Vial : 25 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 10 08:54:45 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040921.M
Quant Title : GC Extractables
QLast Update : Sat Apr 10 02:10:31 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

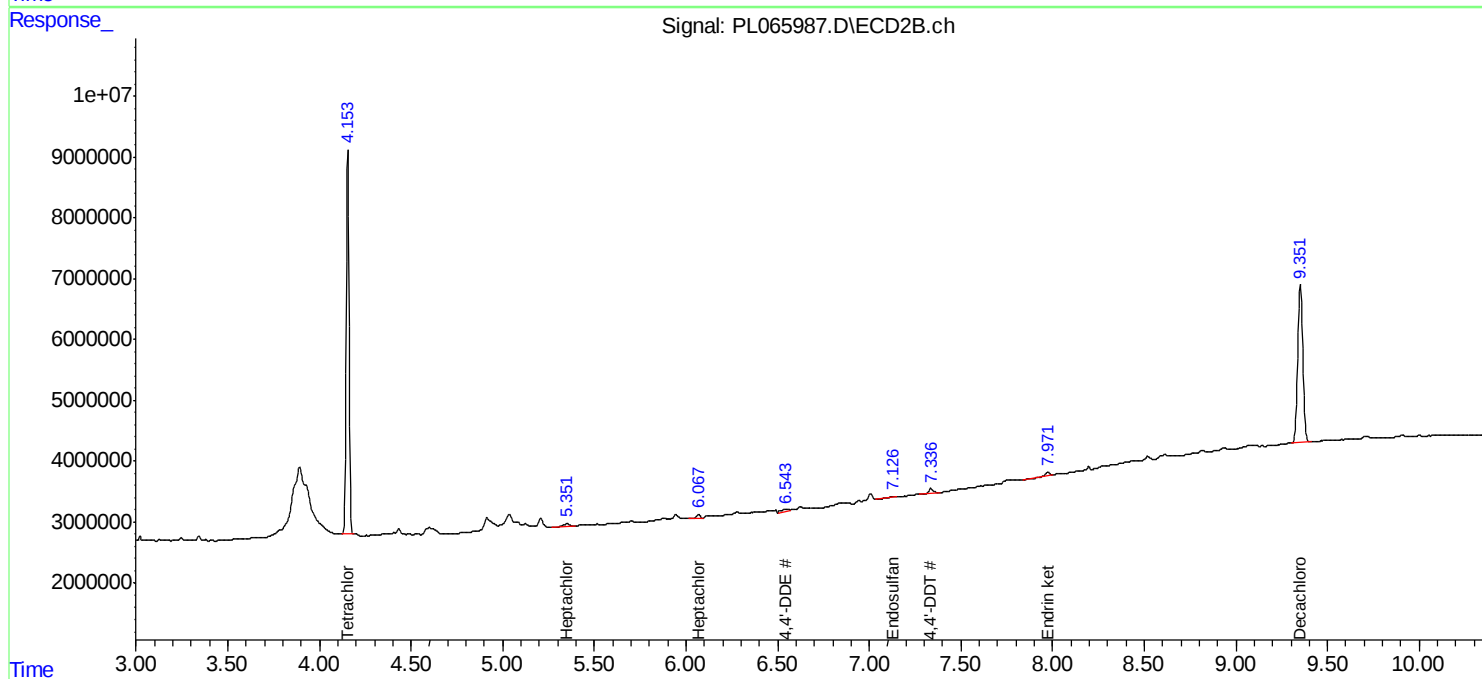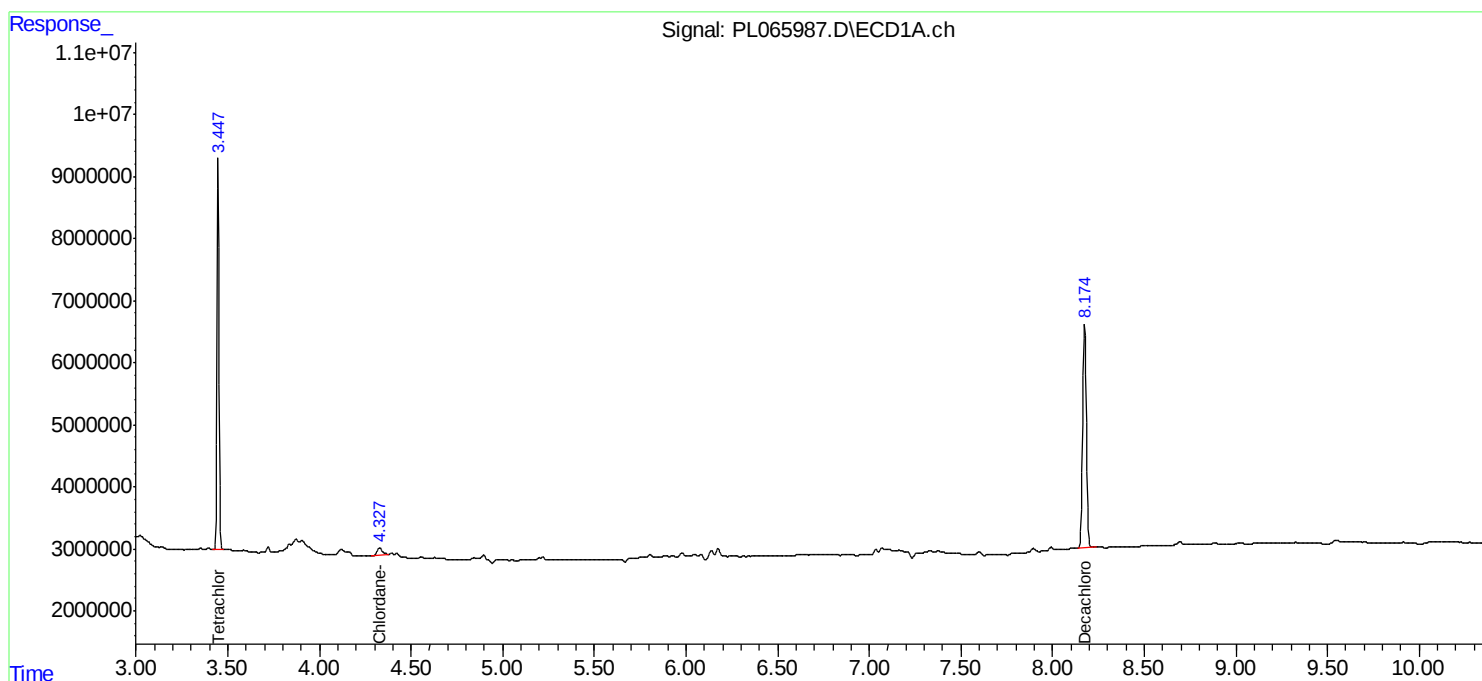

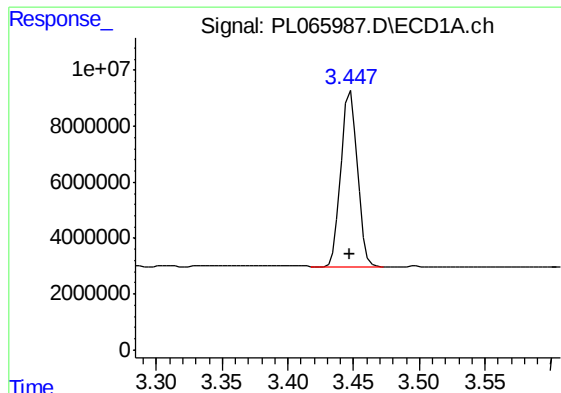


#1 Tetrachloro-m-xylene

R.T.: 3.448 min
Delta R.T.: 0.000 min
Response: 54182046
Conc: 22.31 ng/ml

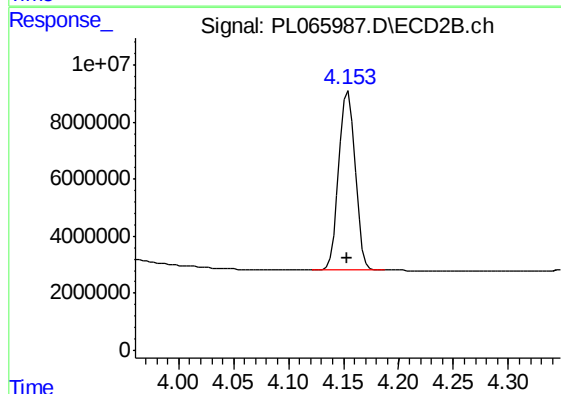


#1 Tetrachloro-m-xylene

R.T.: 4.154 min
Delta R.T.: 0.000 min
Response: 65544996
Conc: 23.78 ng/ml

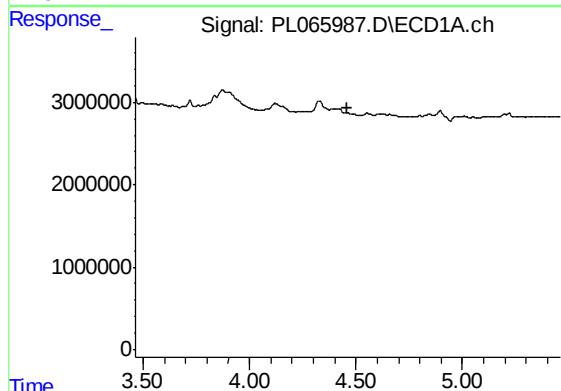


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.462 min
Response: 0
Conc: N.D.

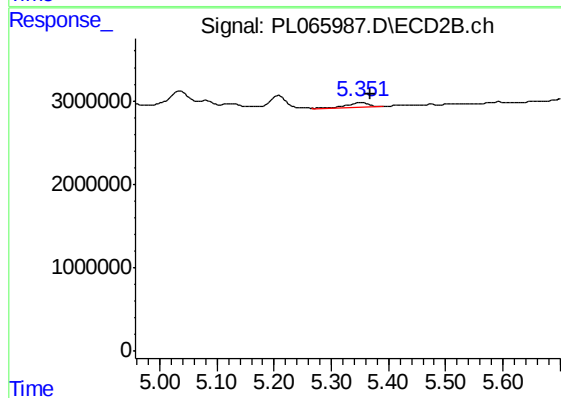


#4 Heptachlor

R.T.: 5.352 min
Delta R.T.: -0.015 min
Response: 1417769
Conc: 0.41 ng/ml

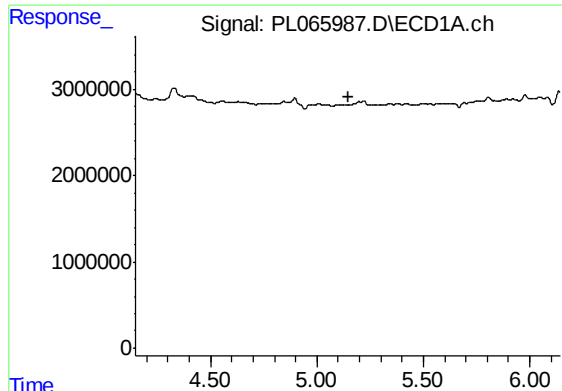


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.146 min
Response: 0
Conc: N.D.

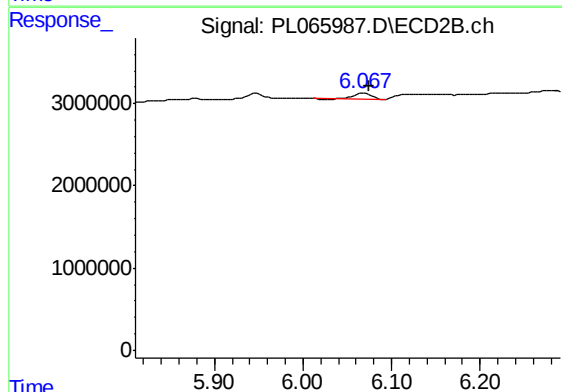


#8 Heptachlor epoxide

R.T.: 6.068 min
Delta R.T.: -0.006 min
Response: 995465
Conc: 0.35 ng/ml

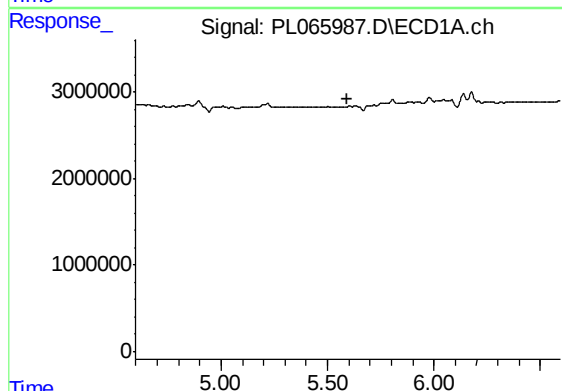


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 5.595 min
Response: 0
Conc: N.D.

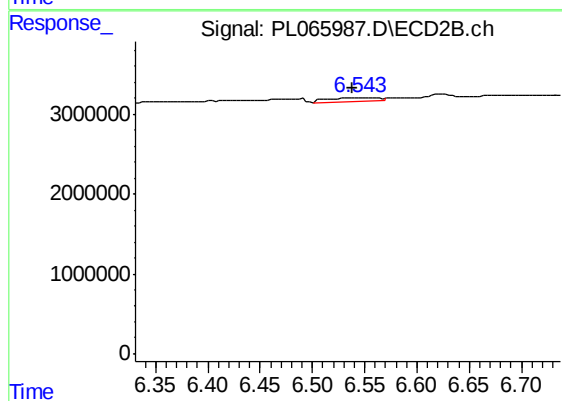


#12 4,4'-DDE

R.T.: 6.544 min
Delta R.T.: 0.006 min
Response: 1359328
Conc: 0.55 ng/ml

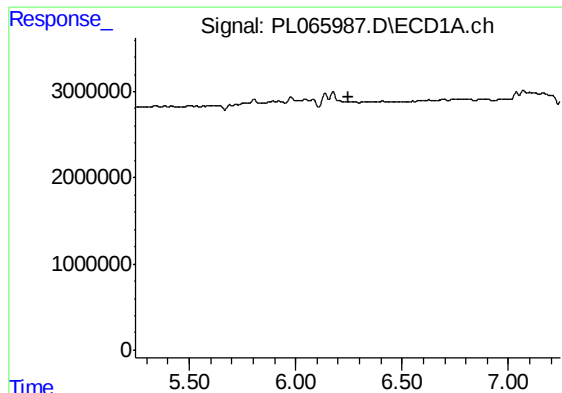


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.246 min
Response: 0
Conc: N.D.

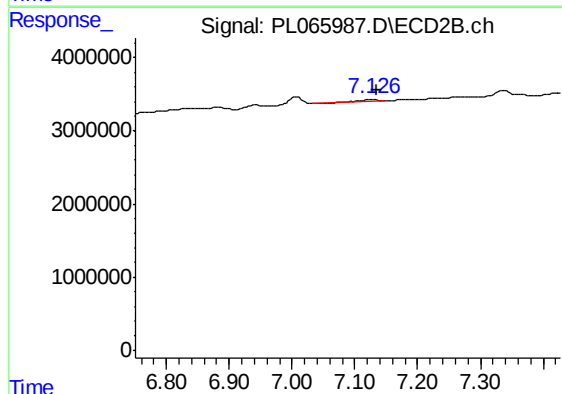


#15 Endosulfan II

R.T.: 7.127 min
Delta R.T.: -0.008 min
Response: 482962
Conc: 0.23 ng/ml

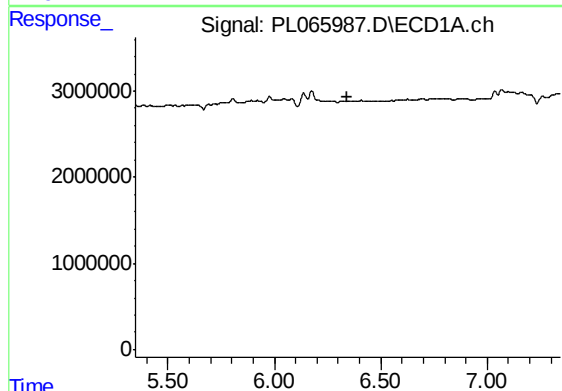


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.346 min
Response: 0
Conc: N.D.

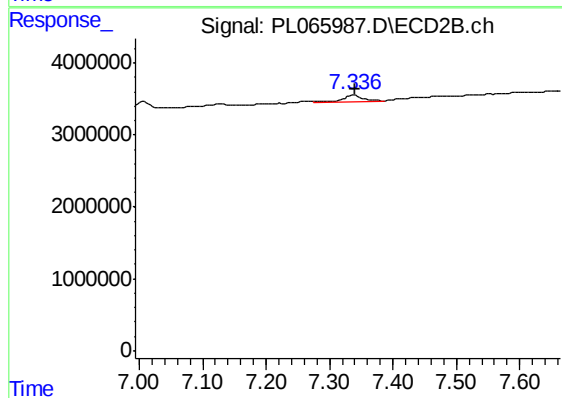


#17 4,4'-DDT

R.T.: 7.337 min
Delta R.T.: -0.003 min
Response: 2014831
Conc: 1.06 ng/ml

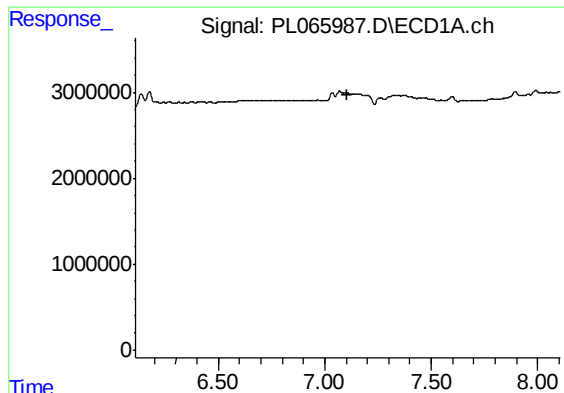


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.109 min
Response: 0
Conc: N.D.

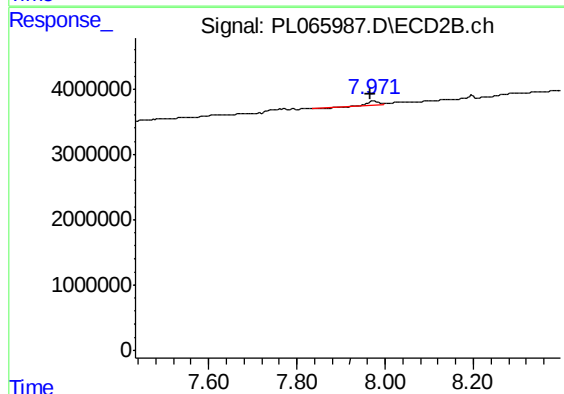


#21 Endrin ketone

R.T.: 7.973 min
Delta R.T.: 0.008 min
Response: 901337
Conc: 0.40 ng/ml

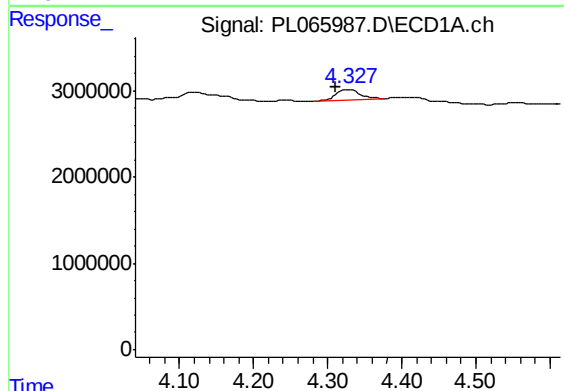


#23 Chlordane-1

R.T.: 4.329 min
Delta R.T.: 0.017 min
Response: 2723033
Conc: 26.02 ng/ml

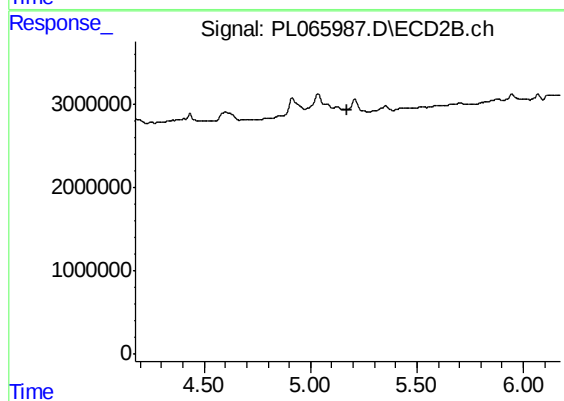


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.175 min
Response: 0
Conc: N.D.

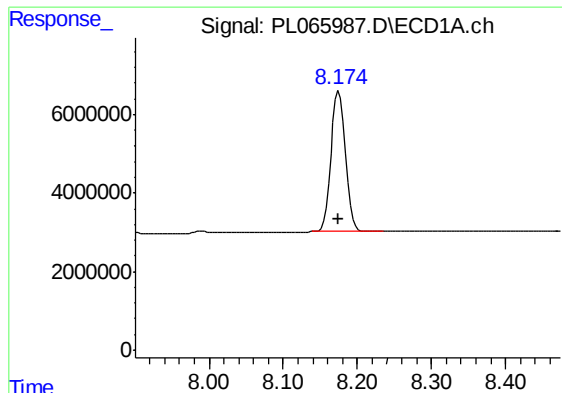

#28 Decachlorobiphenyl

R.T.: 8.175 min
Delta R.T.: 0.000 min
Response: 49208700
Conc: 22.81 ng/ml

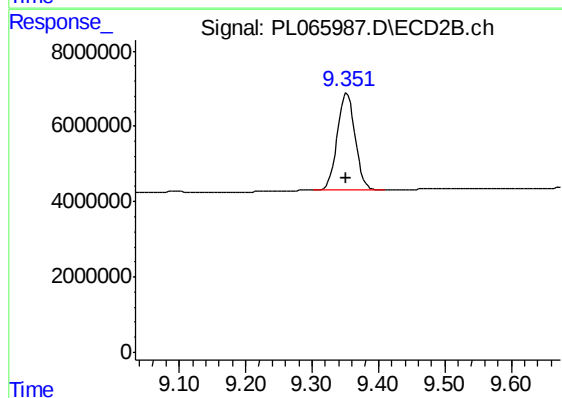

#28 Decachlorobiphenyl

R.T.: 9.352 min
Delta R.T.: 0.001 min
Response: 48245827
Conc: 25.45 ng/ml