

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040921\
 Data File : PL065968.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Apr 2021 20:19
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 10 01:51:24 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040921.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 10 01:51:03 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.447	4.154	288.0E6	250.6E6	98.789	89.770
28)	SA Decachlor...	8.176	9.352	199.7E6	179.0E6	93.461	92.709
Target Compounds							
23)	Chlordane-1	4.312	5.175	99014871	99805589	944.692	855.011
24)	Chlordane-2	4.809	5.652	112.8E6	99168612	931.059	845.520
25)	Chlordane-3	5.373	6.311	330.4E6	376.3E6	987.814	906.792
26)	Chlordane-4	5.430	6.385	273.3E6	442.6E6	980.616	897.445
27)	Chlordane-5	6.255	7.207	123.0E6	81340891	958.290	956.368



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040921\
Data File : PL065968.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Apr 2021 20:19
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 10 01:51:24 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040921.M
Quant Title : GC Extractables
QLast Update : Sat Apr 10 01:51:03 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

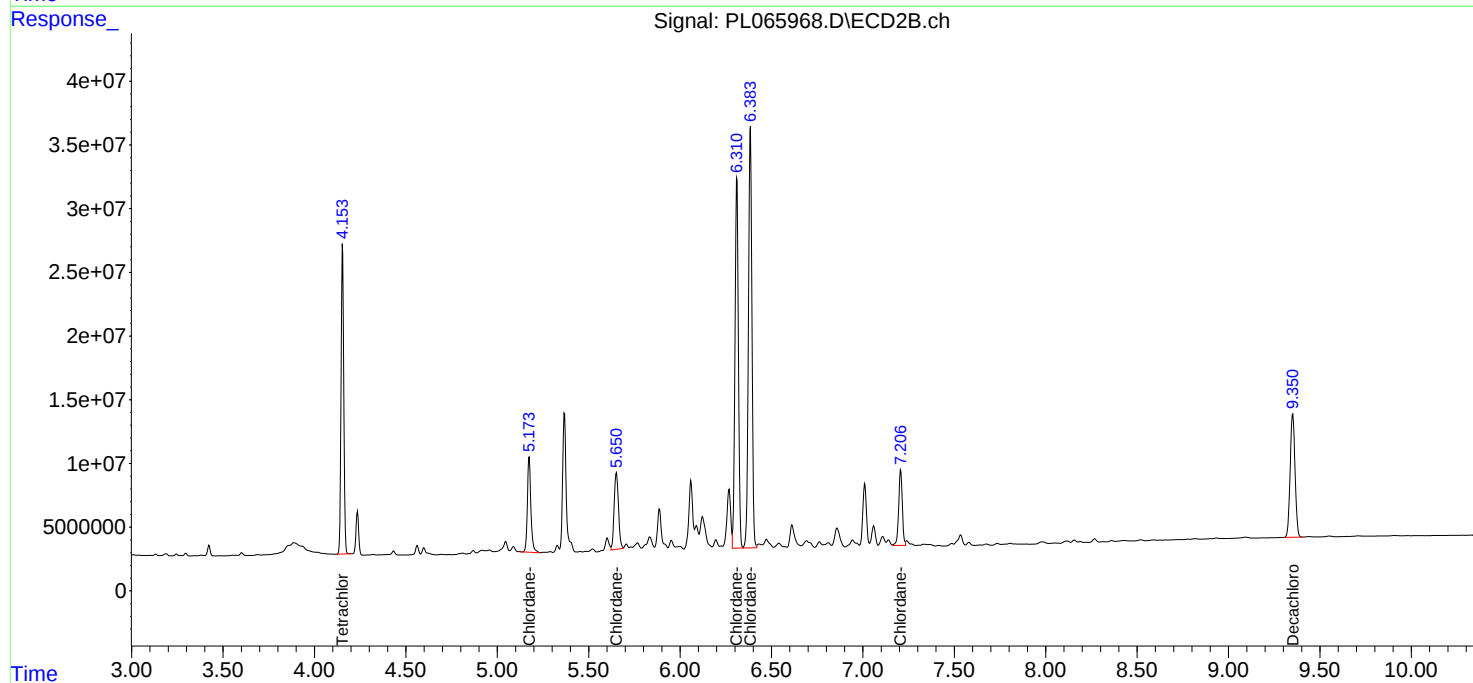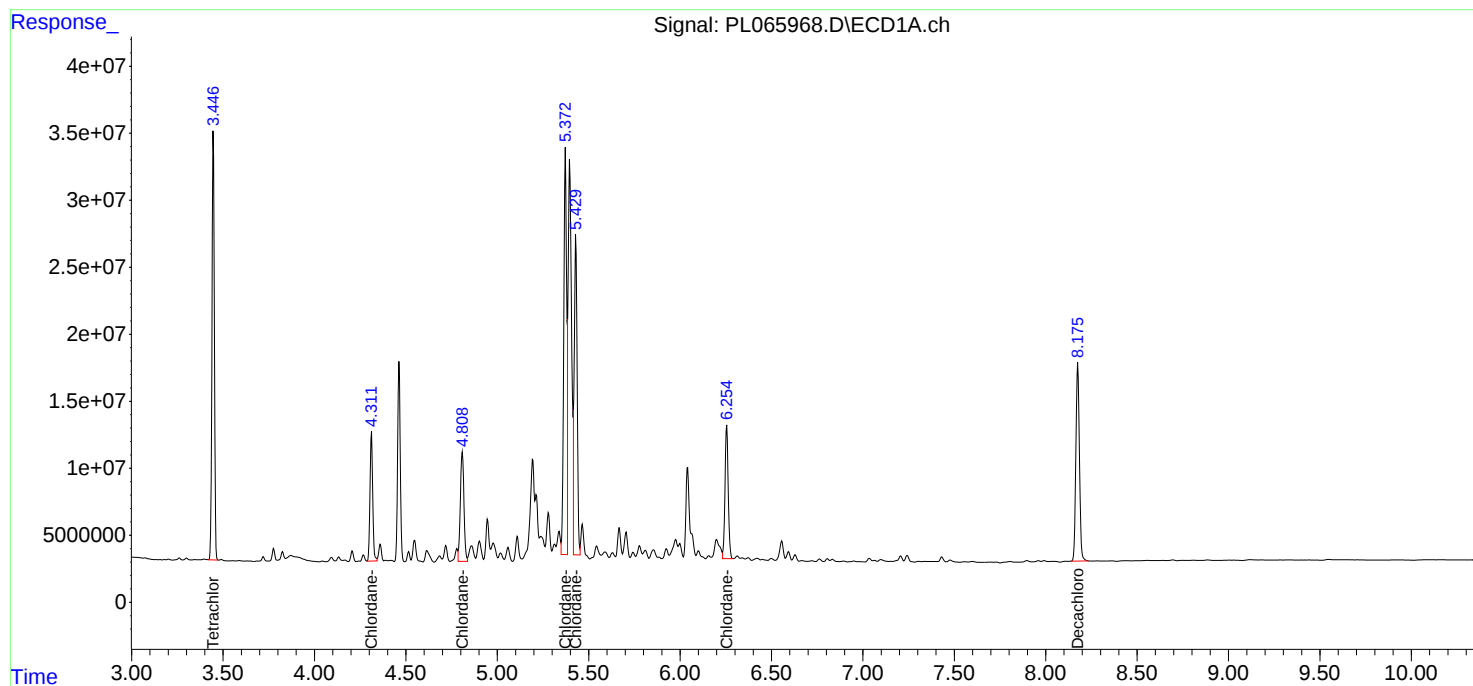


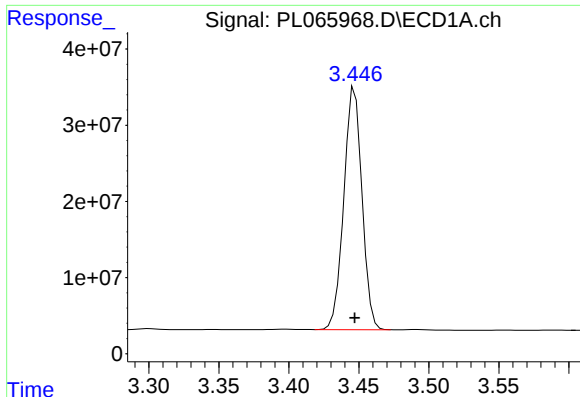

#1 Tetrachloro-m-xylene


R.T.: 3.447 min
Delta R.T.: 0.000 min
Response: 287997458
Conc: 98.79 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

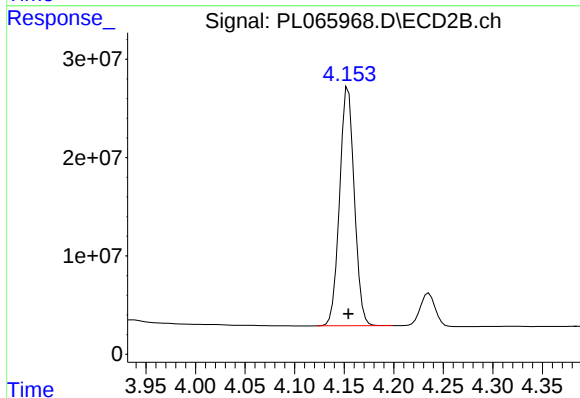


#1 Tetrachloro-m-xylene

R.T.: 4.154 min
Delta R.T.: 0.000 min
Response: 250590758
Conc: 89.77 ng/ml

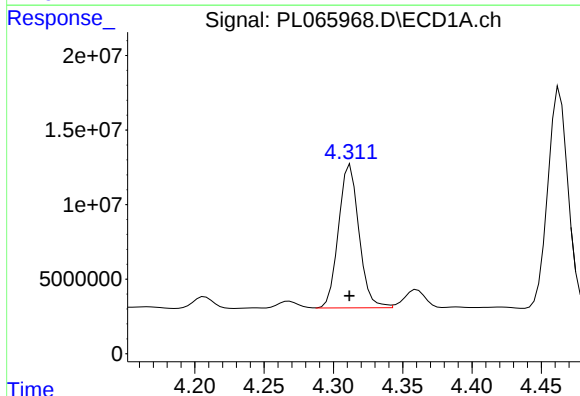


#23 Chlordane-1

R.T.: 4.312 min
Delta R.T.: 0.000 min
Response: 99014871
Conc: 944.69 ng/ml

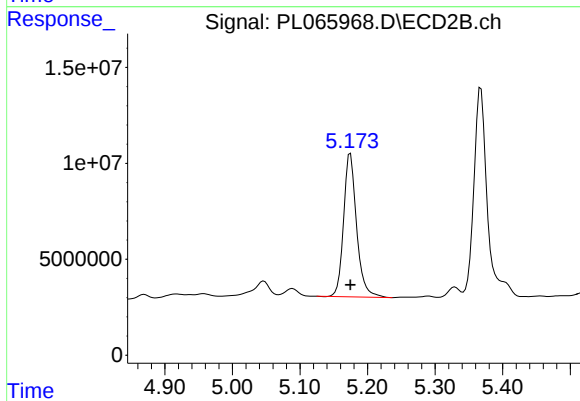

#23 Chlordane-1


R.T.: 5.175 min
Delta R.T.: 0.000 min
Response: 99805589
Conc: 855.01 ng/ml

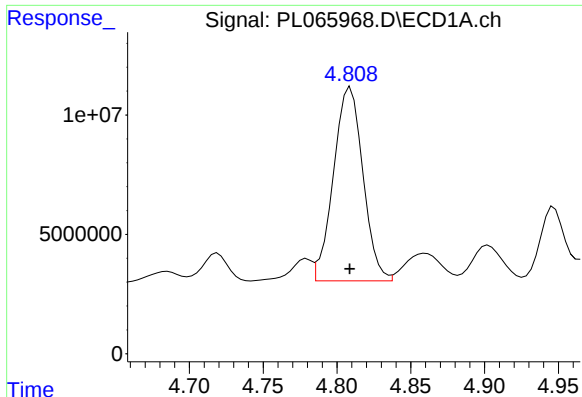

#24 Chlordane-2


R.T.: 4.809 min
Delta R.T.: 0.000 min
Response: 112845993
Conc: 931.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

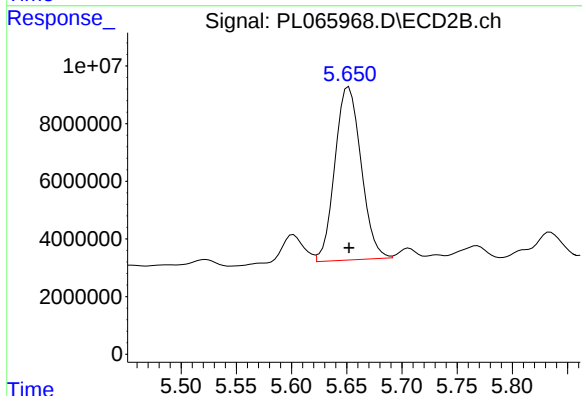


#24 Chlordane-2

R.T.: 5.652 min
Delta R.T.: 0.000 min
Response: 99168612
Conc: 845.52 ng/ml

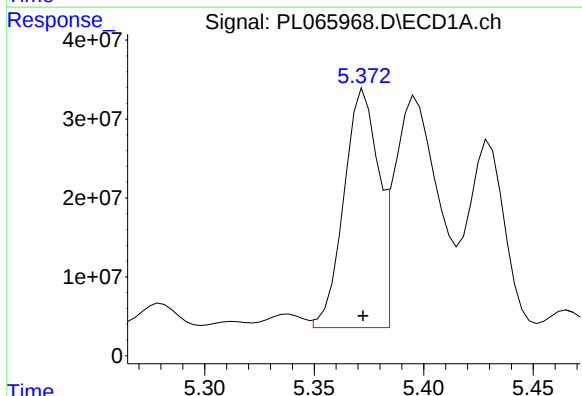


#25 Chlordane-3

R.T.: 5.373 min
Delta R.T.: 0.000 min
Response: 330370401
Conc: 987.81 ng/ml

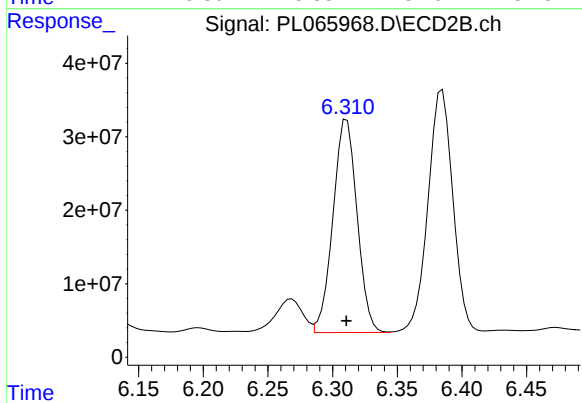

#25 Chlordane-3


R.T.: 6.311 min
Delta R.T.: 0.000 min
Response: 376276177
Conc: 906.79 ng/ml

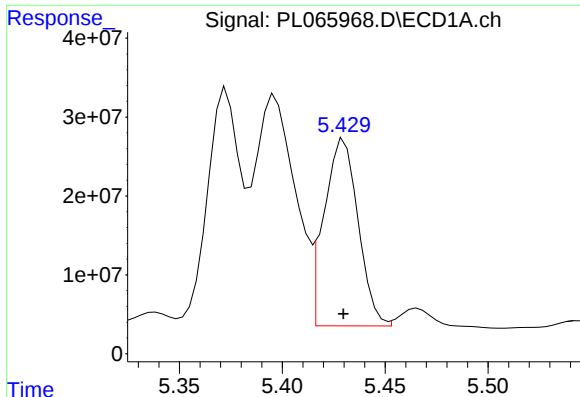

#26 Chlordane-4


R.T.: 5.430 min
Delta R.T.: 0.000 min
Response: 273294937
Conc: 980.62 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

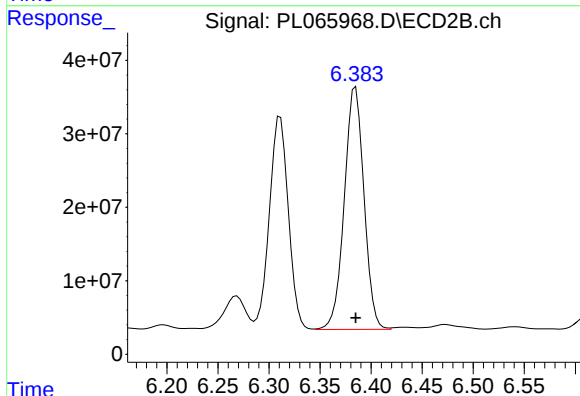


#26 Chlordane-4

R.T.: 6.385 min
Delta R.T.: 0.000 min
Response: 442595272
Conc: 897.44 ng/ml

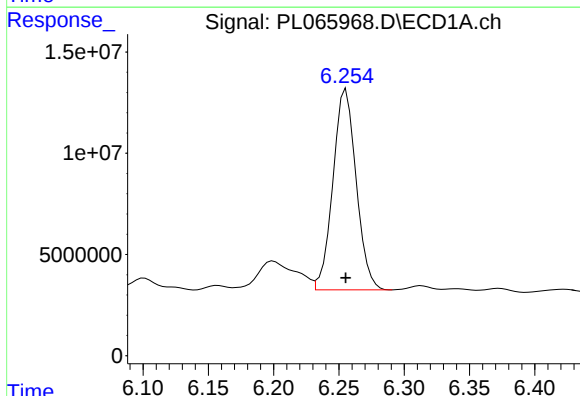


#27 Chlordane-5

R.T.: 6.255 min
Delta R.T.: 0.000 min
Response: 123001939
Conc: 958.29 ng/ml

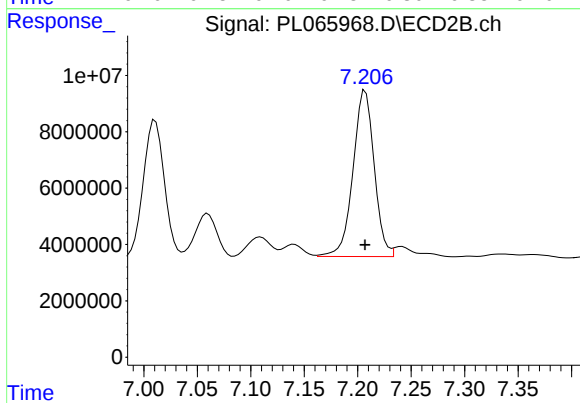

#27 Chlordane-5


R.T.: 7.207 min
Delta R.T.: 0.000 min
Response: 81340891
Conc: 956.37 ng/ml

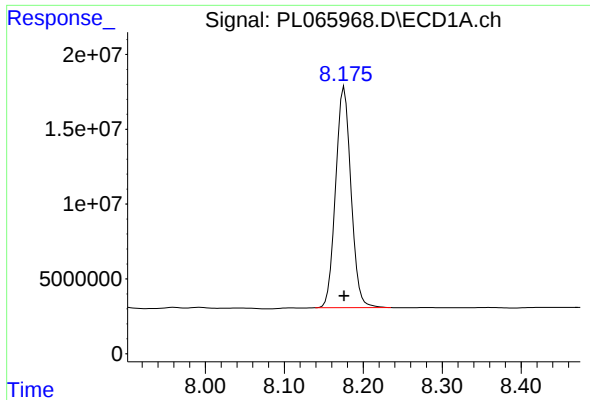

#28 Decachlorobiphenyl

R.T.: 8.176 min
Delta R.T.: 0.000 min
Response: 199692268
Conc: 93.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

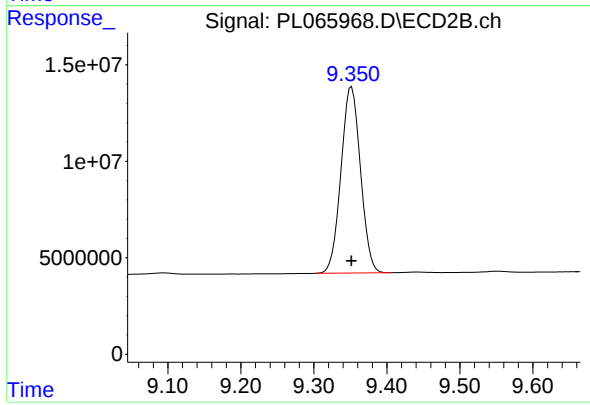

#28 Decachlorobiphenyl

R.T.: 9.352 min
Delta R.T.: 0.000 min
Response: 179011913
Conc: 92.71 ng/ml