

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040921\
 Data File : PL065970.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Apr 2021 20:47
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 10 01:51:52 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040921.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 10 01:51:03 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.447	4.154	145.8E6	139.6E6	50.000	50.000
28)	SA Decachlor...	8.176	9.351	106.8E6	96544933	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.312	5.175	52405920	58365100	500.000	500.000
24)	Chlordane-2	4.809	5.652	60600870	58643595	500.000	500.000
25)	Chlordane-3	5.372	6.311	167.2E6	207.5E6	500.000	500.000
26)	Chlordane-4	5.430	6.385	139.3E6	246.6E6	500.000	500.000
27)	Chlordane-5	6.255	7.207	64177814	42525952	500.000	500.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040921\
Data File : PL065970.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Apr 2021 20:47
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 10 01:51:52 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040921.M
Quant Title : GC Extractables
QLast Update : Sat Apr 10 01:51:03 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

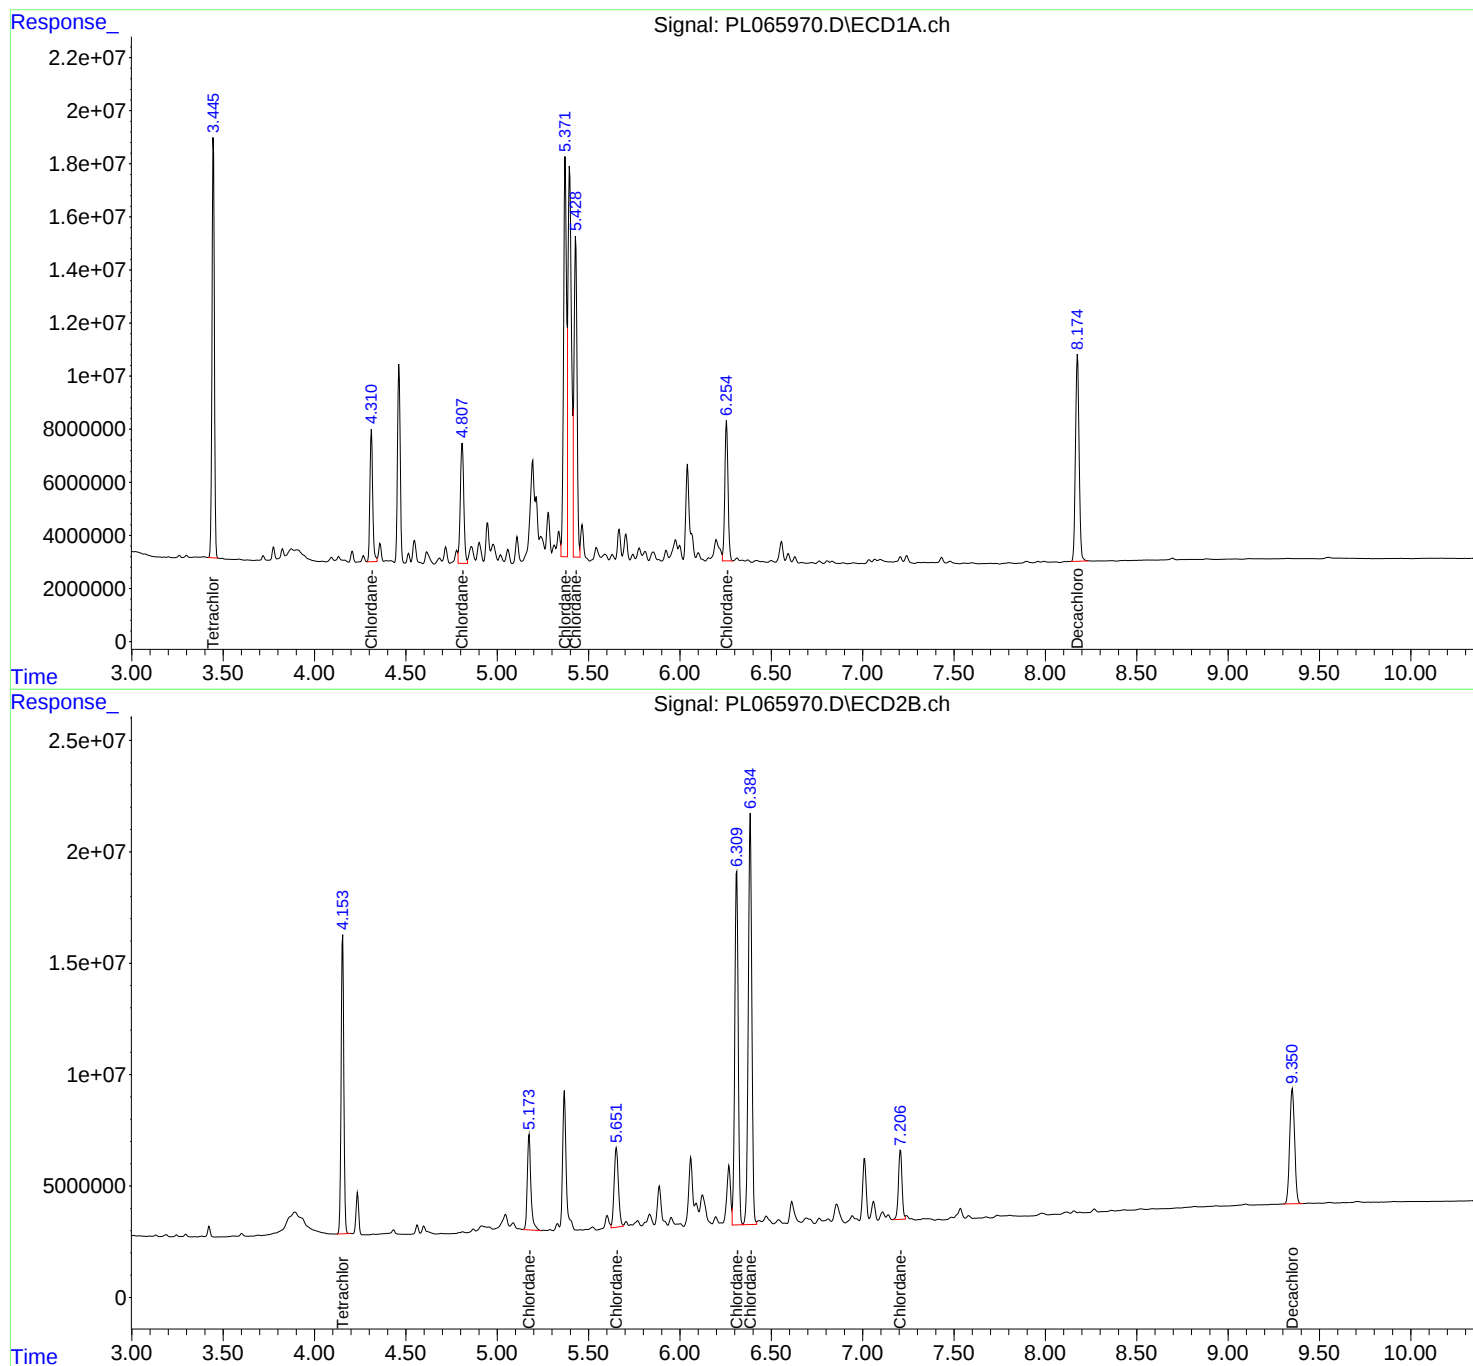


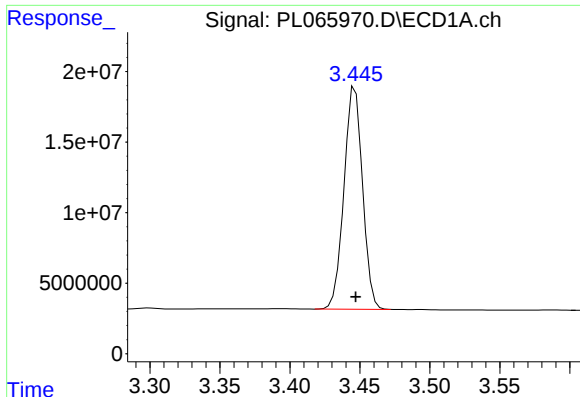

#1 Tetrachloro-m-xylene


R.T.: 3.447 min
Delta R.T.: 0.000 min
Response: 145764382
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

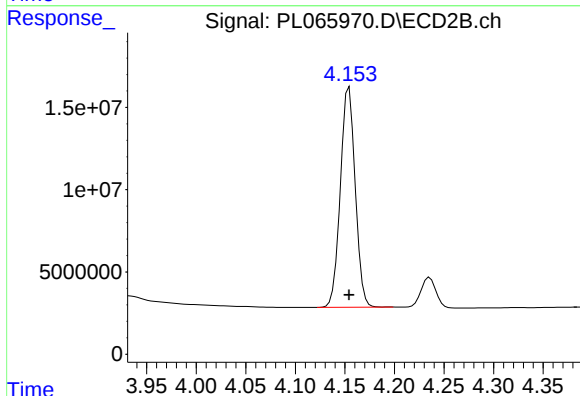


#1 Tetrachloro-m-xylene

R.T.: 4.154 min
Delta R.T.: 0.000 min
Response: 139573512
Conc: 50.00 ng/ml

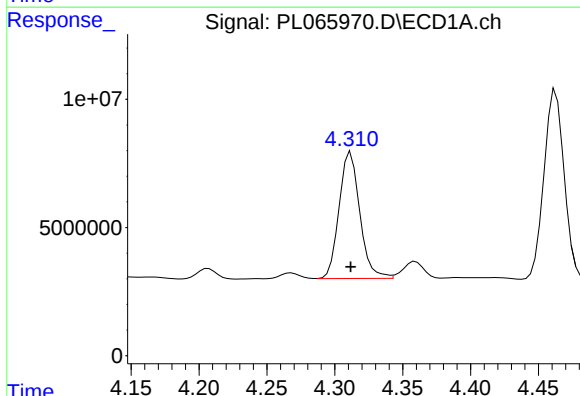


#23 Chlordane-1

R.T.: 4.312 min
Delta R.T.: 0.000 min
Response: 52405920
Conc: 500.00 ng/ml

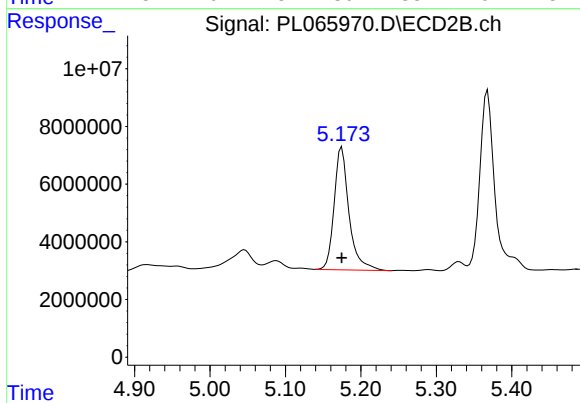

#23 Chlordane-1


R.T.: 5.175 min
Delta R.T.: 0.000 min
Response: 58365100
Conc: 500.00 ng/ml

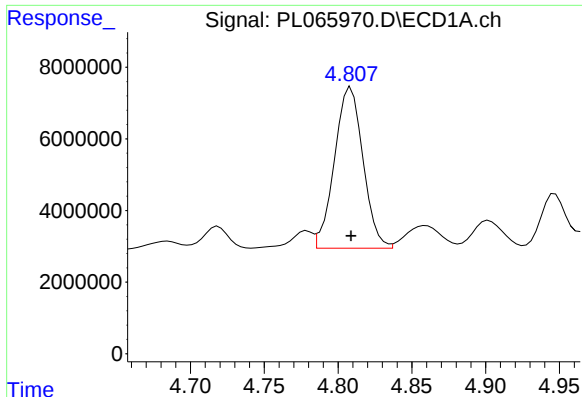

#24 Chlordane-2


R.T.: 4.809 min
Delta R.T.: 0.000 min
Response: 60600870
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

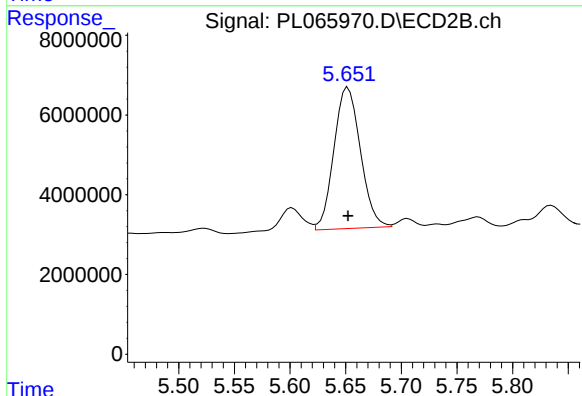


#24 Chlordane-2

R.T.: 5.652 min
Delta R.T.: 0.000 min
Response: 58643595
Conc: 500.00 ng/ml

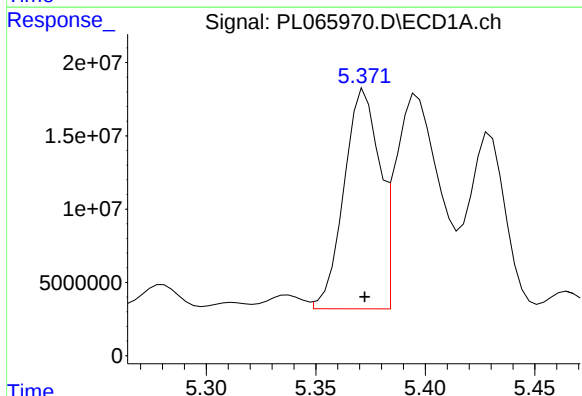


#25 Chlordane-3

R.T.: 5.372 min
Delta R.T.: 0.000 min
Response: 167223009
Conc: 500.00 ng/ml

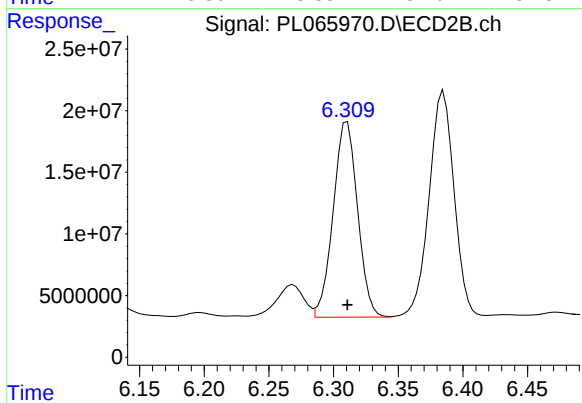

#25 Chlordane-3


R.T.: 6.311 min
Delta R.T.: 0.000 min
Response: 207476557
Conc: 500.00 ng/ml

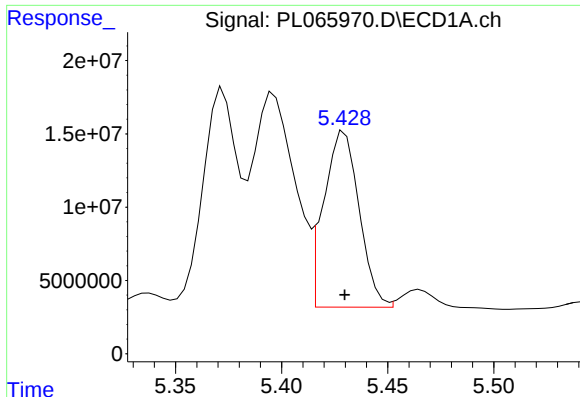

#26 Chlordane-4


R.T.: 5.430 min
Delta R.T.: 0.000 min
Response: 139348658
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

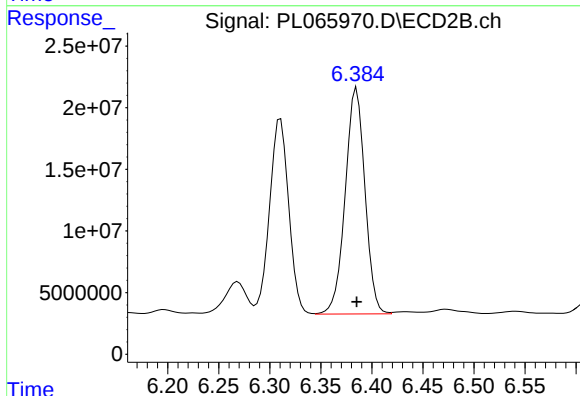


#26 Chlordane-4

R.T.: 6.385 min
Delta R.T.: 0.000 min
Response: 246586371
Conc: 500.00 ng/ml

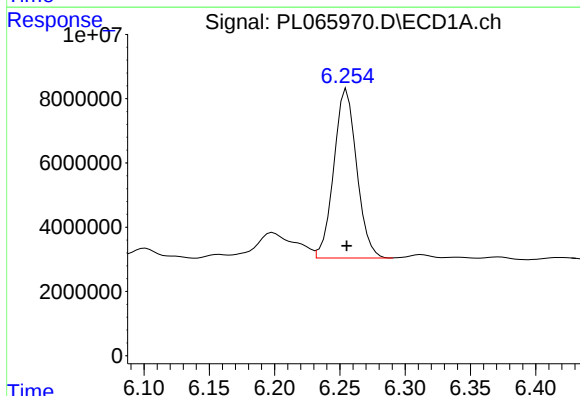


#27 Chlordane-5

R.T.: 6.255 min
Delta R.T.: 0.000 min
Response: 64177814
Conc: 500.00 ng/ml

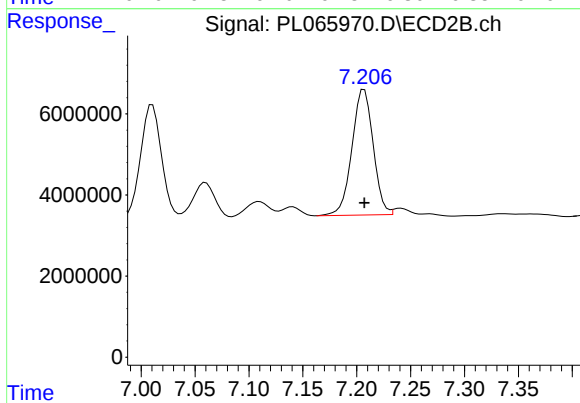

#27 Chlordane-5

R.T.: 7.207 min
Delta R.T.: 0.000 min
Response: 42525952
Conc: 500.00 ng/ml

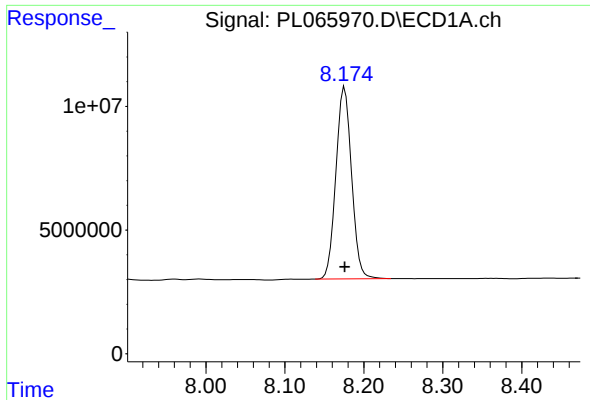

#28 Decachlorobiphenyl


R.T.: 8.176 min

Delta R.T.: 0.000 min

Response: 106831357

Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

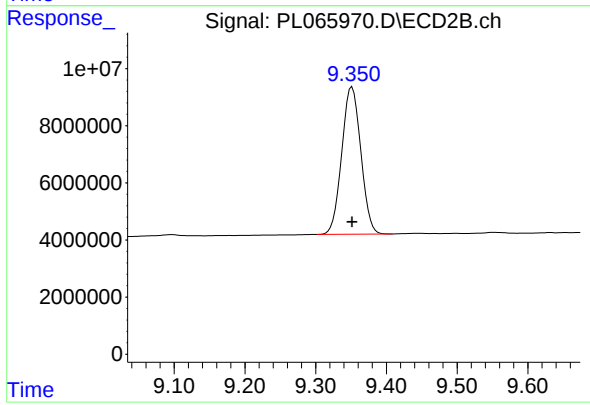

#28 Decachlorobiphenyl

R.T.: 9.351 min

Delta R.T.: 0.000 min

Response: 96544933

Conc: 50.00 ng/ml