

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040921\
 Data File : PL065979.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Apr 2021 22:56
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL040921CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 10 08:37:22 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040921.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 10 02:10:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.447	4.154	139.3E6	131.7E6	57.359	47.768
28)	SA Decachlor...	8.175	9.352	102.5E6	96626790	47.534	50.977
Target Compounds							
23)	Chlordane-1	4.311	5.175	49756796	54739867	475.401	498.158
24)	Chlordane-2	4.808	5.652	58076711	55263950	478.532	494.488
25)	Chlordane-3	5.372	6.311	160.0E6	195.6E6	488.750	497.048
26)	Chlordane-4	5.429	6.385	134.7E6	233.6E6	491.933	489.602
27)	Chlordane-5	6.254	7.207	60823970	41293938	478.032	505.517



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040921\
Data File : PL065979.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Apr 2021 22:56
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL040921CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 10 08:37:22 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040921.M
Quant Title : GC Extractables
QLast Update : Sat Apr 10 02:10:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

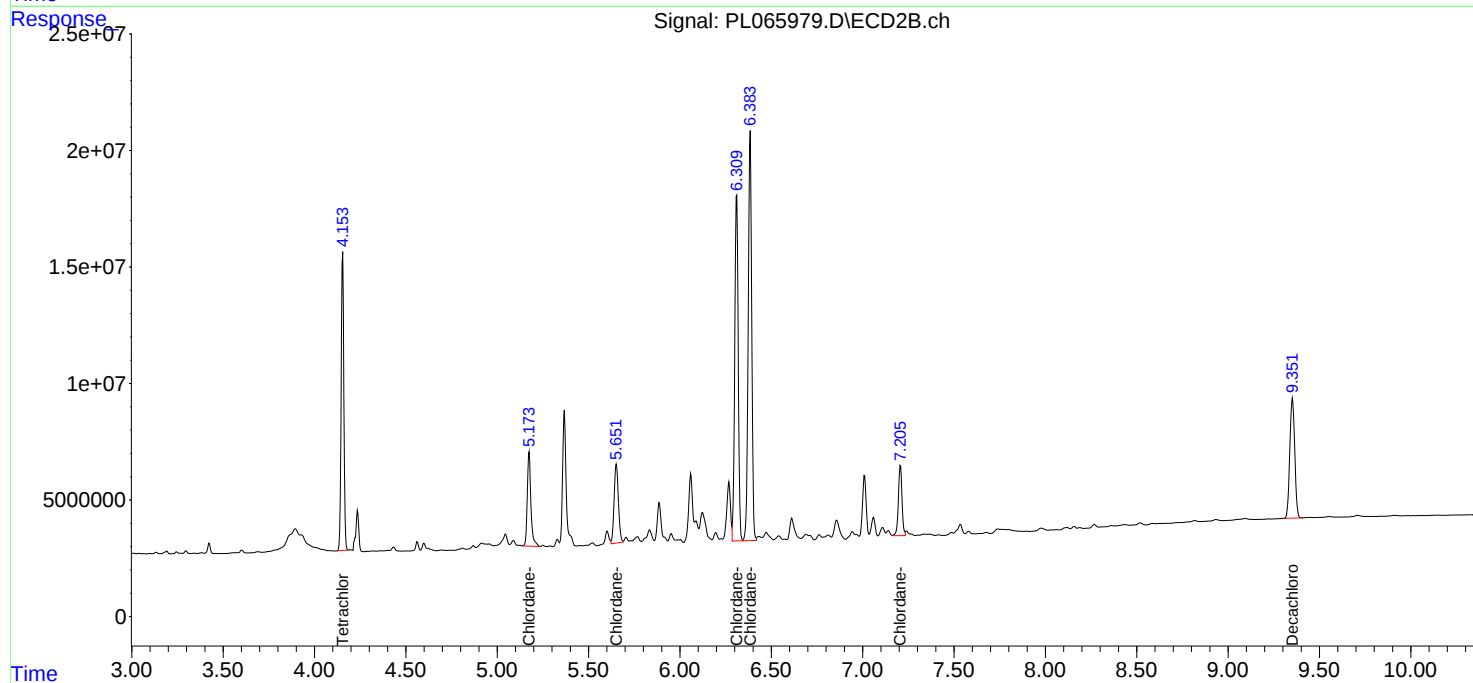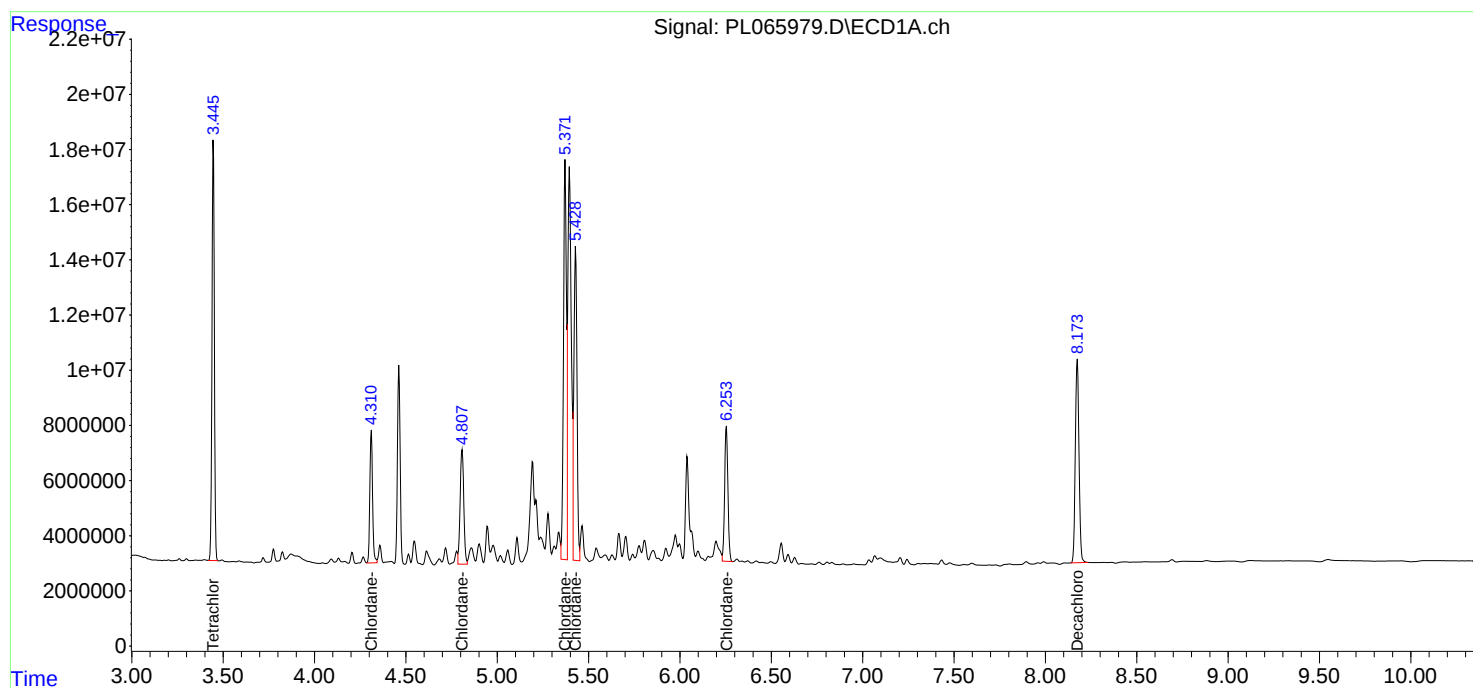


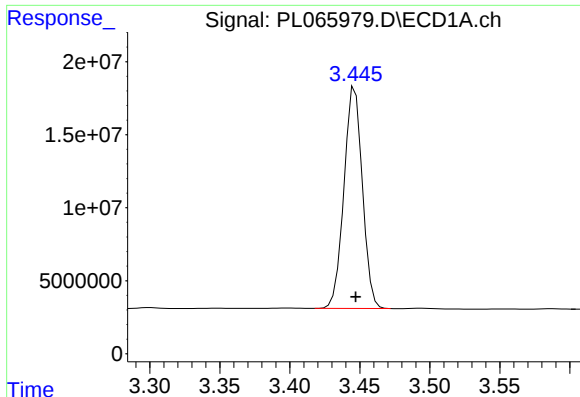

#1 Tetrachloro-m-xylene


R.T.: 3.447 min
Delta R.T.: 0.000 min
Response: 139294424
Conc: 57.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL040921CHLOR

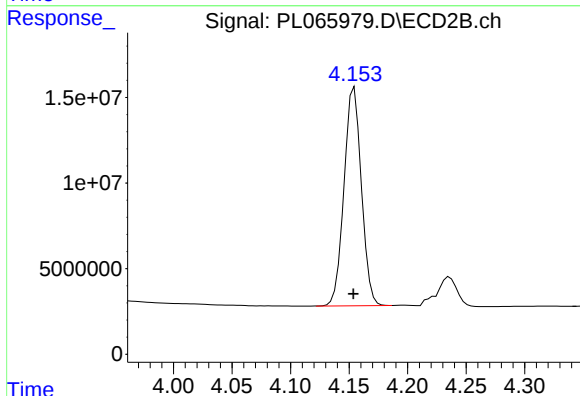


#1 Tetrachloro-m-xylene

R.T.: 4.154 min
Delta R.T.: 0.000 min
Response: 131666041
Conc: 47.77 ng/ml

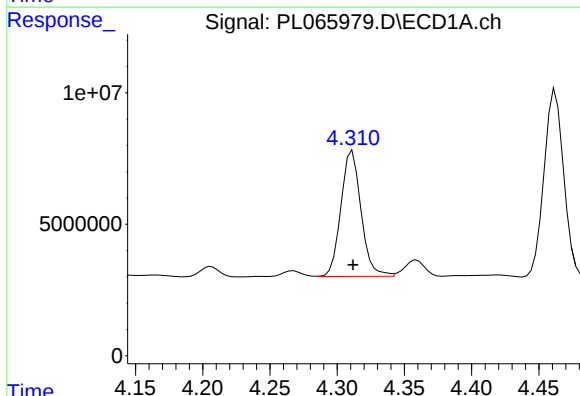


#23 Chlordane-1

R.T.: 4.311 min
Delta R.T.: 0.000 min
Response: 49756796
Conc: 475.40 ng/ml

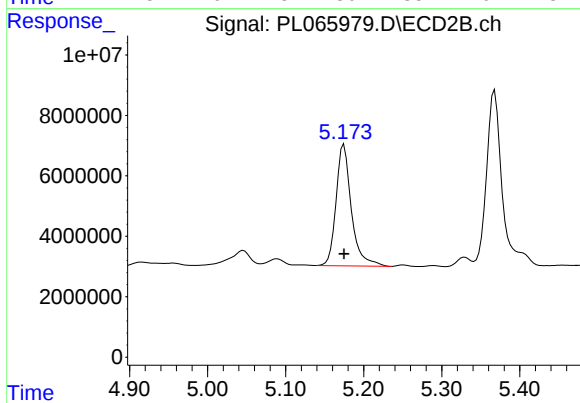

#23 Chlordane-1


R.T.: 5.175 min
Delta R.T.: 0.000 min
Response: 54739867
Conc: 498.16 ng/ml

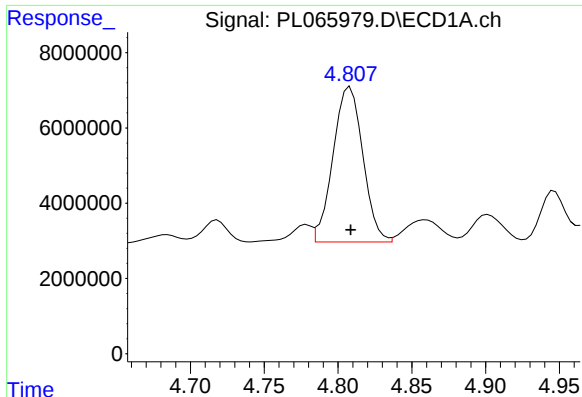

#24 Chlordane-2


R.T.: 4.808 min
Delta R.T.: 0.000 min
Response: 58076711
Conc: 478.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL040921CHLOR

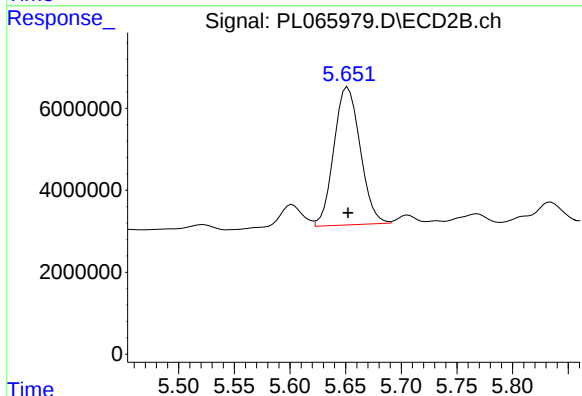


#24 Chlordane-2

R.T.: 5.652 min
Delta R.T.: 0.000 min
Response: 55263950
Conc: 494.49 ng/ml

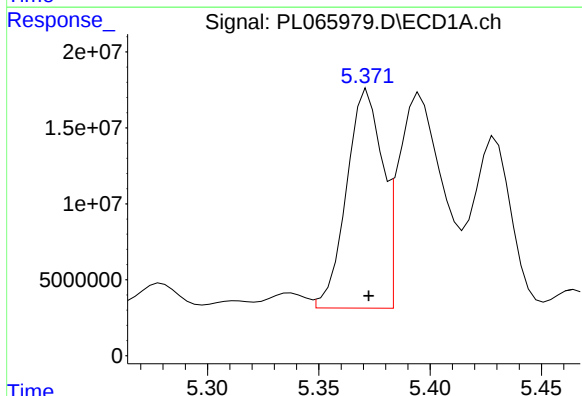


#25 Chlordane-3

R.T.: 5.372 min
Delta R.T.: 0.000 min
Response: 159964361
Conc: 488.75 ng/ml

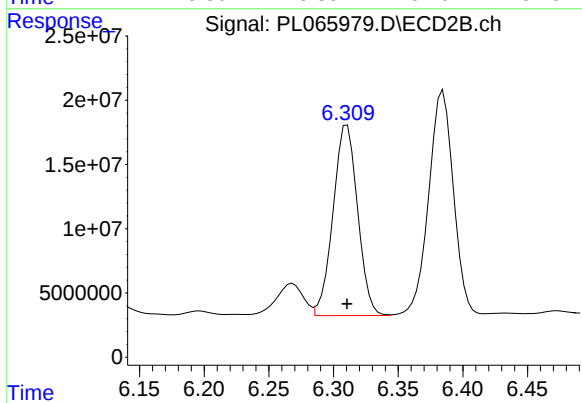

#25 Chlordane-3


R.T.: 6.311 min
Delta R.T.: 0.000 min
Response: 195626876
Conc: 497.05 ng/ml

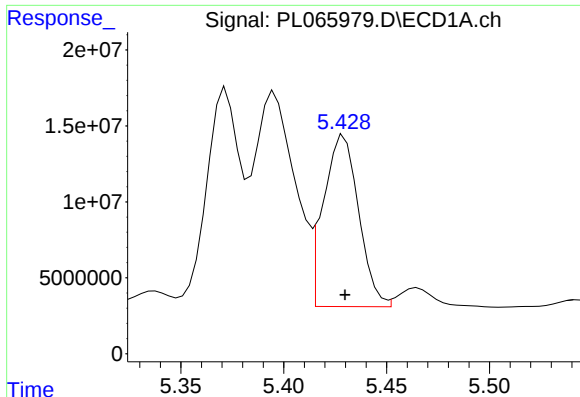

#26 Chlordane-4


R.T.: 5.429 min
Delta R.T.: 0.000 min
Response: 134695215
Conc: 491.93 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL040921CHLOR

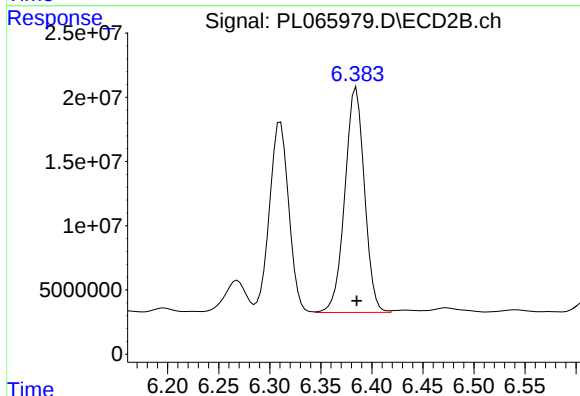


#26 Chlordane-4

R.T.: 6.385 min
Delta R.T.: 0.000 min
Response: 233634543
Conc: 489.60 ng/ml

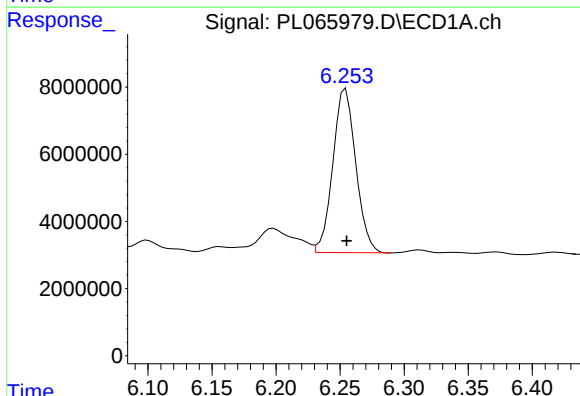


#27 Chlordane-5

R.T.: 6.254 min
Delta R.T.: 0.000 min
Response: 60823970
Conc: 478.03 ng/ml

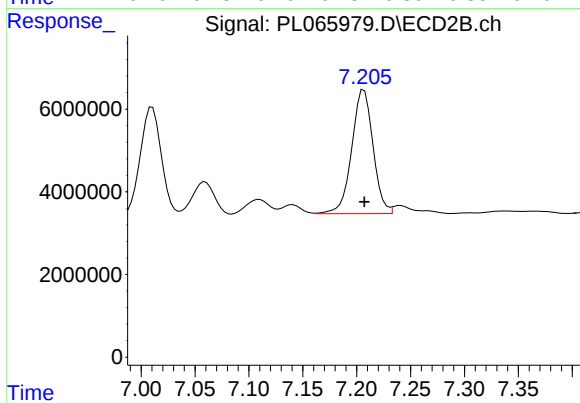

#27 Chlordane-5

R.T.: 7.207 min
Delta R.T.: 0.000 min
Response: 41293938
Conc: 505.52 ng/ml

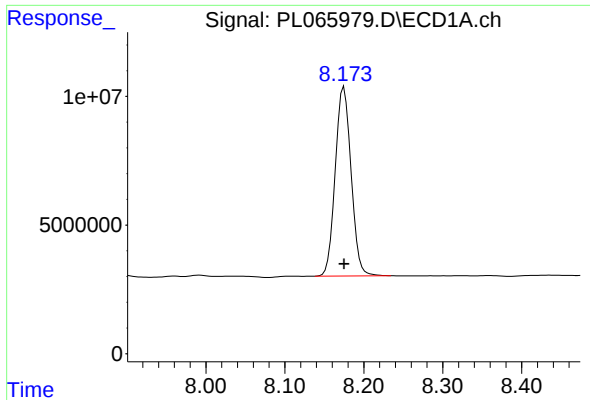

#28 Decachlorobiphenyl


R.T.: 8.175 min

Delta R.T.: 0.000 min

Response: 102543327

Conc: 47.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL040921CHLOR

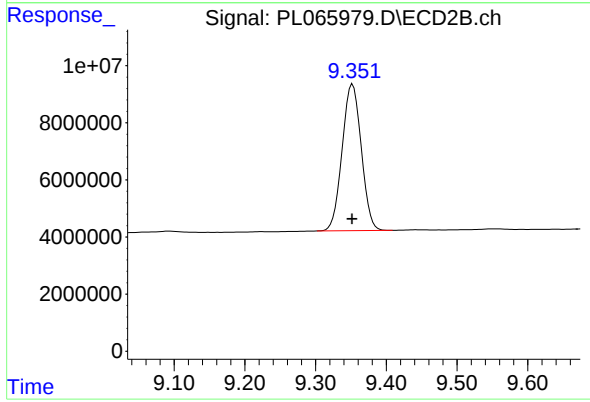

#28 Decachlorobiphenyl

R.T.: 9.352 min

Delta R.T.: 0.000 min

Response: 96626790

Conc: 50.98 ng/ml