

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040921\
 Data File : PL065988.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Apr 2021 04:26
 Operator : AR\AJ
 Sample : M1947-01
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 FS-SB19B(6-7)

Manual Integrations
 APPROVED

Ankita
 4/12/2021 2:41:37 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 10 08:55:01 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040921.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 10 02:10:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.447	4.154	53180991	63493618	21.899	23.035
28)	SA Decachlor...	8.175	9.353	49529947	51013142	22.960	26.913
Target Compounds							
15)	B Endosulfa...	6.247	7.131	2832131	2656499	0.962	1.247m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040921\
Data File : PL065988.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Apr 2021 04:26
Operator : AR\AJ
Sample : M1947-01
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
FS-SB19B(6-7)


Manual Integrations
APPROVED

Ankita
4/12/2021 2:41:37 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 10 08:55:01 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040921.M
Quant Title : GC Extractables
QLast Update : Sat Apr 10 02:10:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

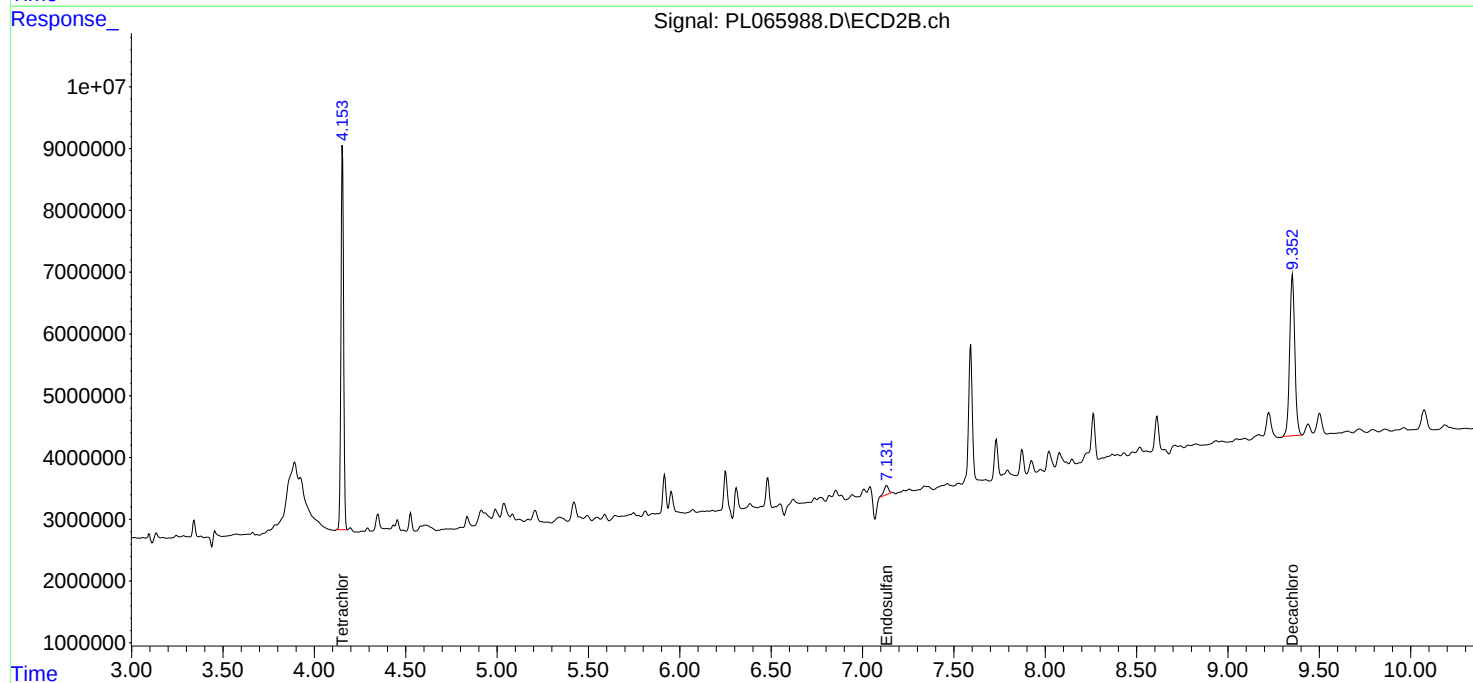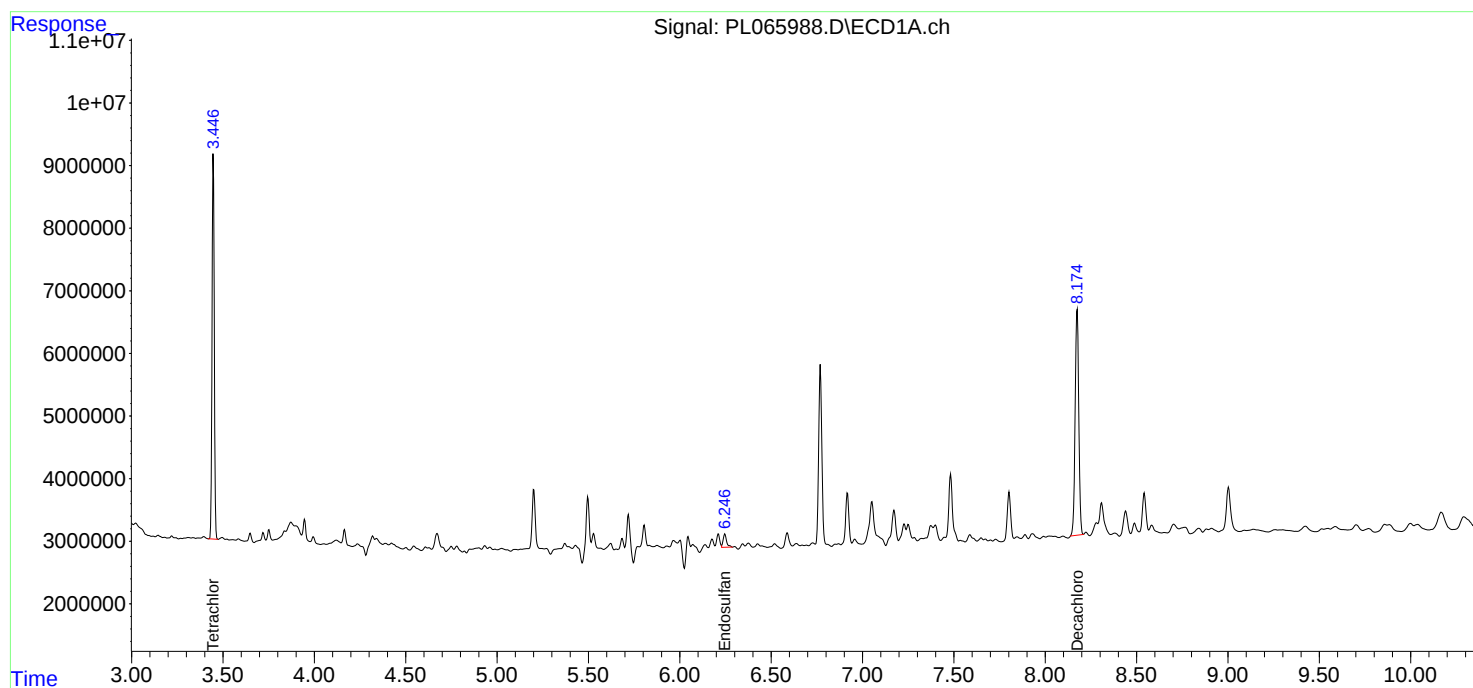

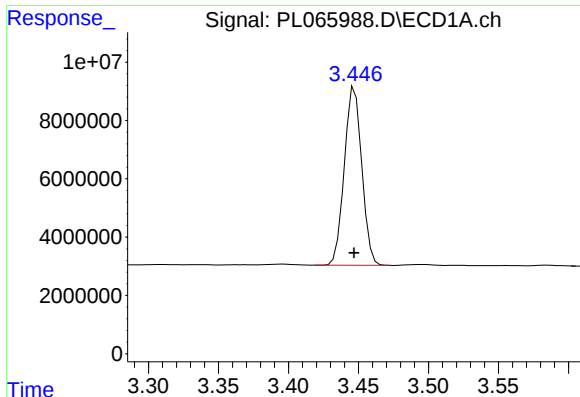


#1 Tetrachloro-m-xylene

R.T.: 3.447 min
Delta R.T.: 0.000 min
Response: 53180991
Conc: 21.90 ng/ml

Instrument :
ECD_L
ClientSampleId :
FS-SB19B(6-7)


Manual Integrations
APPROVED

Ankita
4/12/2021 2:41:37 PM

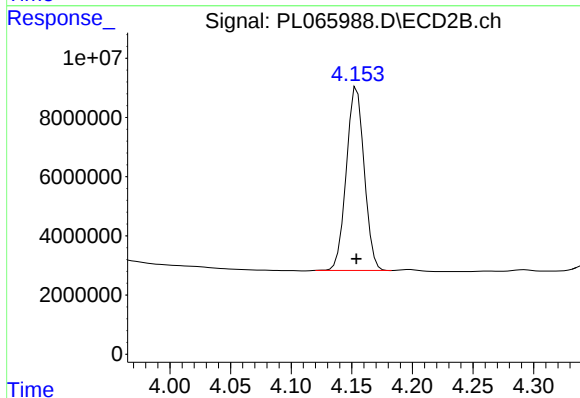


#1 Tetrachloro-m-xylene

R.T.: 4.154 min
Delta R.T.: 0.000 min
Response: 63493618
Conc: 23.04 ng/ml

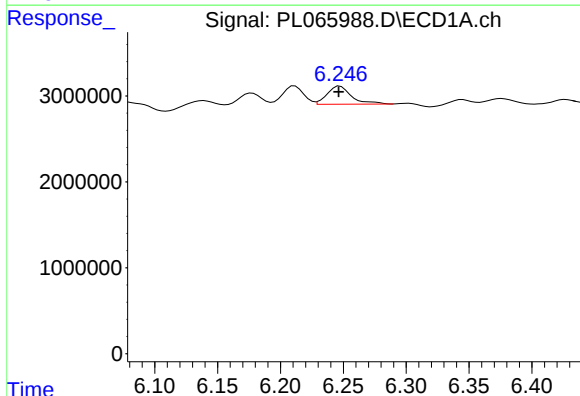


#15 Endosulfan II

R.T.: 6.247 min
Delta R.T.: 0.000 min
Response: 2832131
Conc: 0.96 ng/ml

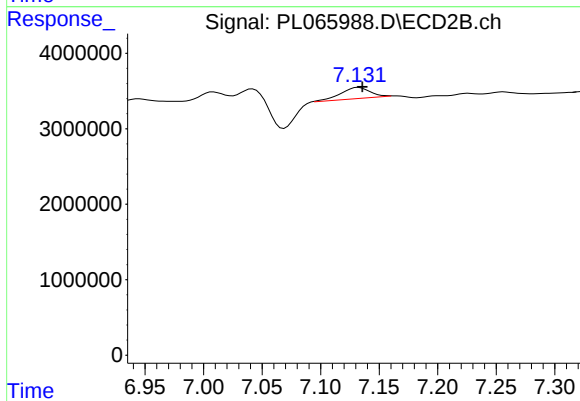

#15 Endosulfan II

R.T.: 7.131 min
Delta R.T.: -0.005 min
Response: 2656499
Conc: 1.25 ng/ml m

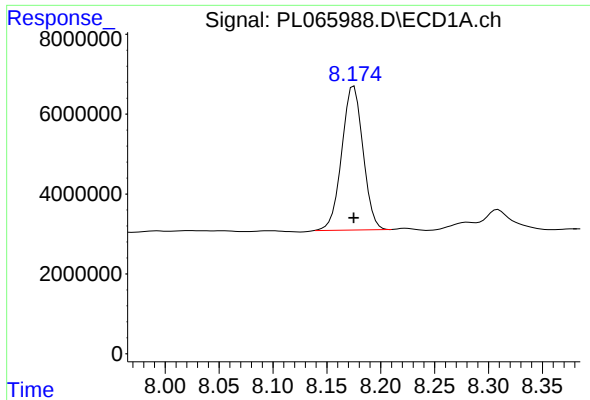


#28 Decachlorobiphenyl

R.T.: 8.175 min
Delta R.T.: 0.000 min
Response: 49529947
Conc: 22.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
FS-SB19B(6-7)

Manual Integrations
APPROVED

Ankita
4/12/2021 2:41:37 PM

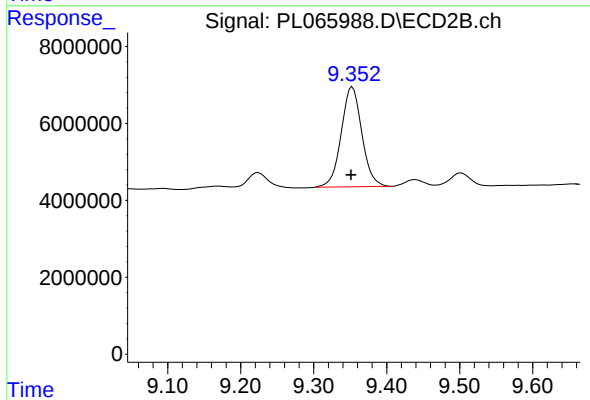

#28 Decachlorobiphenyl

R.T.: 9.353 min
Delta R.T.: 0.002 min
Response: 51013142
Conc: 26.91 ng/ml