

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040921\
 Data File : PL065995.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Apr 2021 06:06
 Operator : AR\AJ
 Sample : M1967-04
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SED-1B

Manual Integrations
 APPROVED

Ankita
 4/12/2021 2:41:40 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 10 08:58:04 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040921.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 10 02:10:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.447	4.155	49875650	59815210	20.538	21.701
28)	SA Decachlor...	8.174	9.353	35116376	35638931	16.278	18.802
Target Compounds							
11)	B alpha-Chl...	5.428	6.383	1771059	2739450	0.546m	0.999m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040921\
Data File : PL065995.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Apr 2021 06:06
Operator : AR\AJ
Sample : M1967-04
Misc :
ALS Vial : 33 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SED-1B


Manual Integrations
APPROVED

Ankita
4/12/2021 2:41:40 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 10 08:58:04 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040921.M
Quant Title : GC Extractables
QLast Update : Sat Apr 10 02:10:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

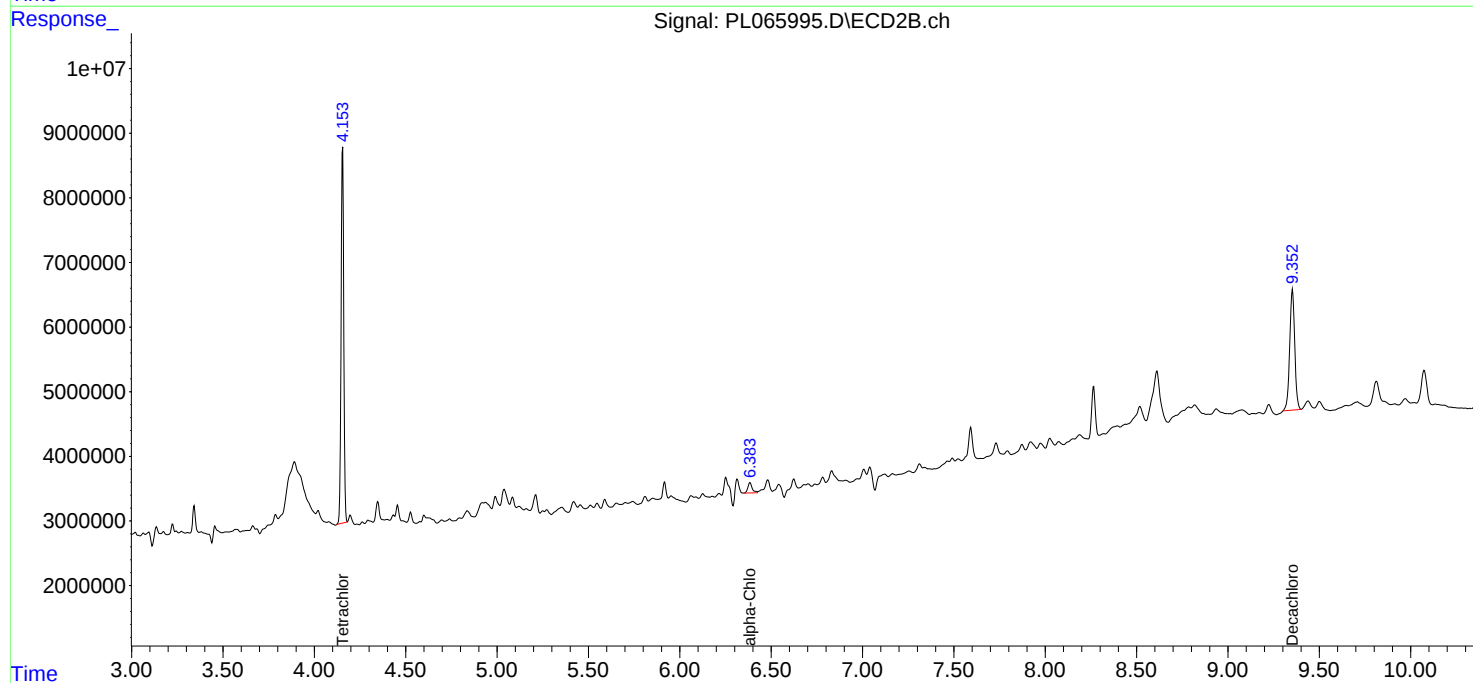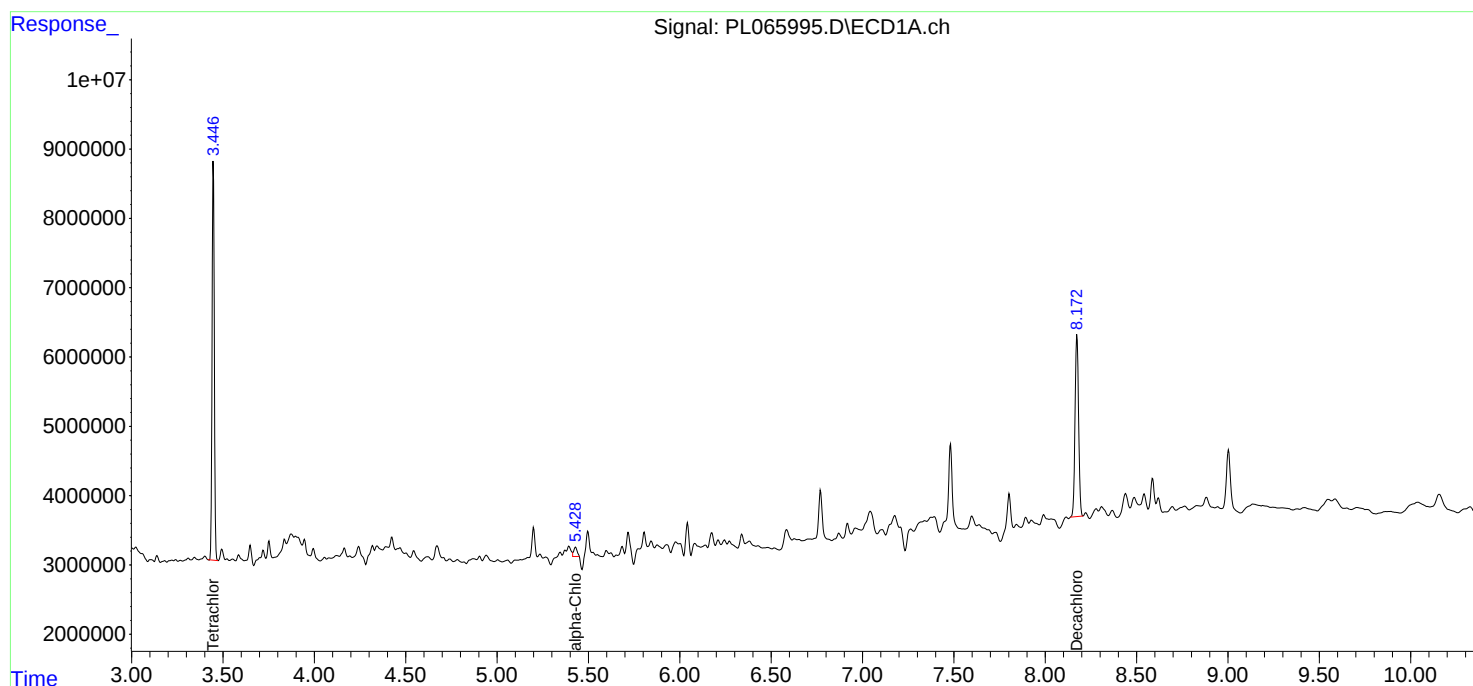

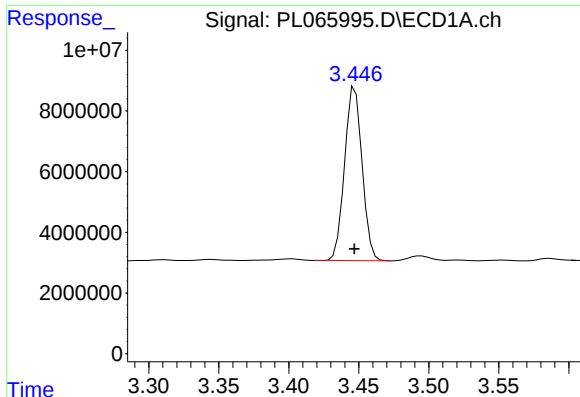


#1 Tetrachloro-m-xylene

R.T.: 3.447 min
Delta R.T.: 0.000 min
Response: 49875650
Conc: 20.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
SED-1B


Manual Integrations
APPROVED

Ankita
4/12/2021 2:41:40 PM

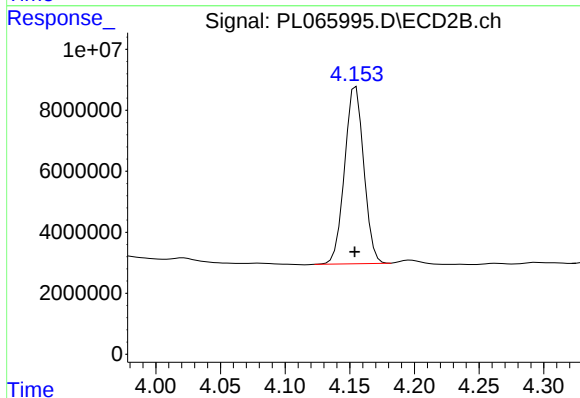


#1 Tetrachloro-m-xylene

R.T.: 4.155 min
Delta R.T.: 0.001 min
Response: 59815210
Conc: 21.70 ng/ml

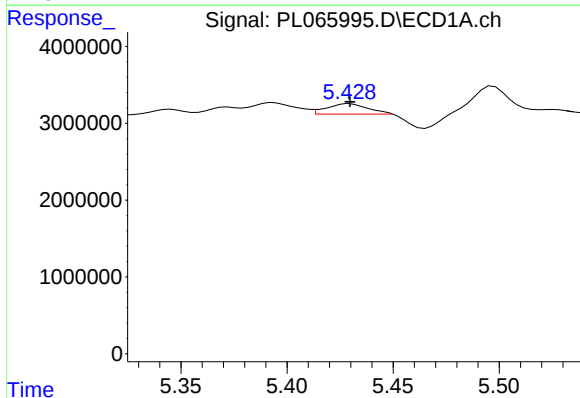


#11 alpha-Chlordane

R.T.: 5.428 min
Delta R.T.: -0.002 min
Response: 1771059
Conc: 0.55 ng/ml m

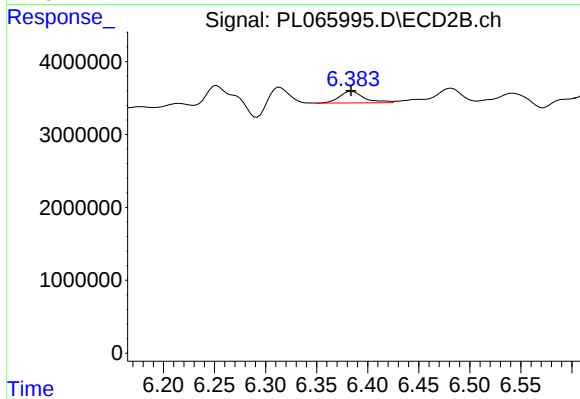

#11 alpha-Chlordane

R.T.: 6.383 min
Delta R.T.: 0.000 min
Response: 2739450
Conc: 1.00 ng/ml m

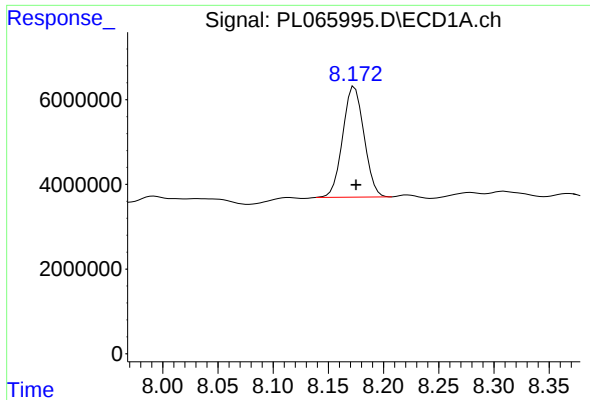


#28 Decachlorobiphenyl

R.T.: 8.174 min
Delta R.T.: -0.001 min
Response: 35116376
Conc: 16.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
SED-1B

Manual Integrations
APPROVED

Ankita
4/12/2021 2:41:40 PM

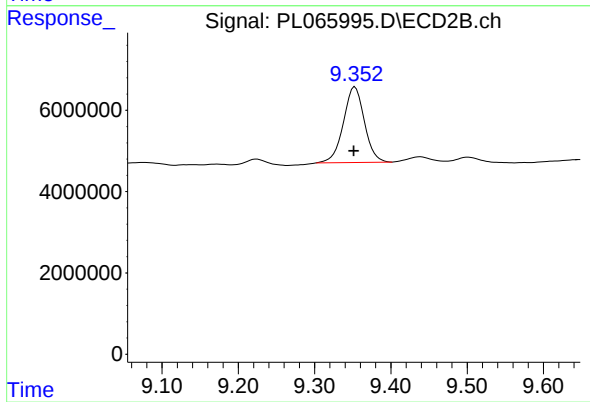

#28 Decachlorobiphenyl

R.T.: 9.353 min
Delta R.T.: 0.002 min
Response: 35638931
Conc: 18.80 ng/ml