

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040925\
 Data File : PL095135.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Apr 2025 16:08
 Operator : AR\AJ
 Sample : Q1754-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 10 01:23:58 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031125.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 11 17:42:21 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.535	2.768	51534805	73926648	18.206	20.712
28)	SA Decachlor...	9.047	7.899	38687741	56070034	18.358	13.881
Target Compounds							
7)	B delta-BHC	4.760	0.000	10575517	0	2.716	N.D. #
9)	A Endosulfan I	0.000	5.121f	0	15574338	N.D.	3.549 #
10)	B gamma-Chl...	5.933	0.000	7845076	0	2.328	N.D. #
13)	MA Dieldrin	0.000	5.365	0	27160443	N.D.	5.598 #
20)	A Methoxychlor	0.000	6.636f	0	8175114	N.D.	3.854 #
25)	Chlordane-3	5.933	0.000	7845076	0	15.696	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040925\
Data File : PL095135.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Apr 2025 16:08
Operator : AR\AJ
Sample : Q1754-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 10 01:23:58 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031125.M
Quant Title : GC Extractables
QLast Update : Tue Mar 11 17:42:21 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

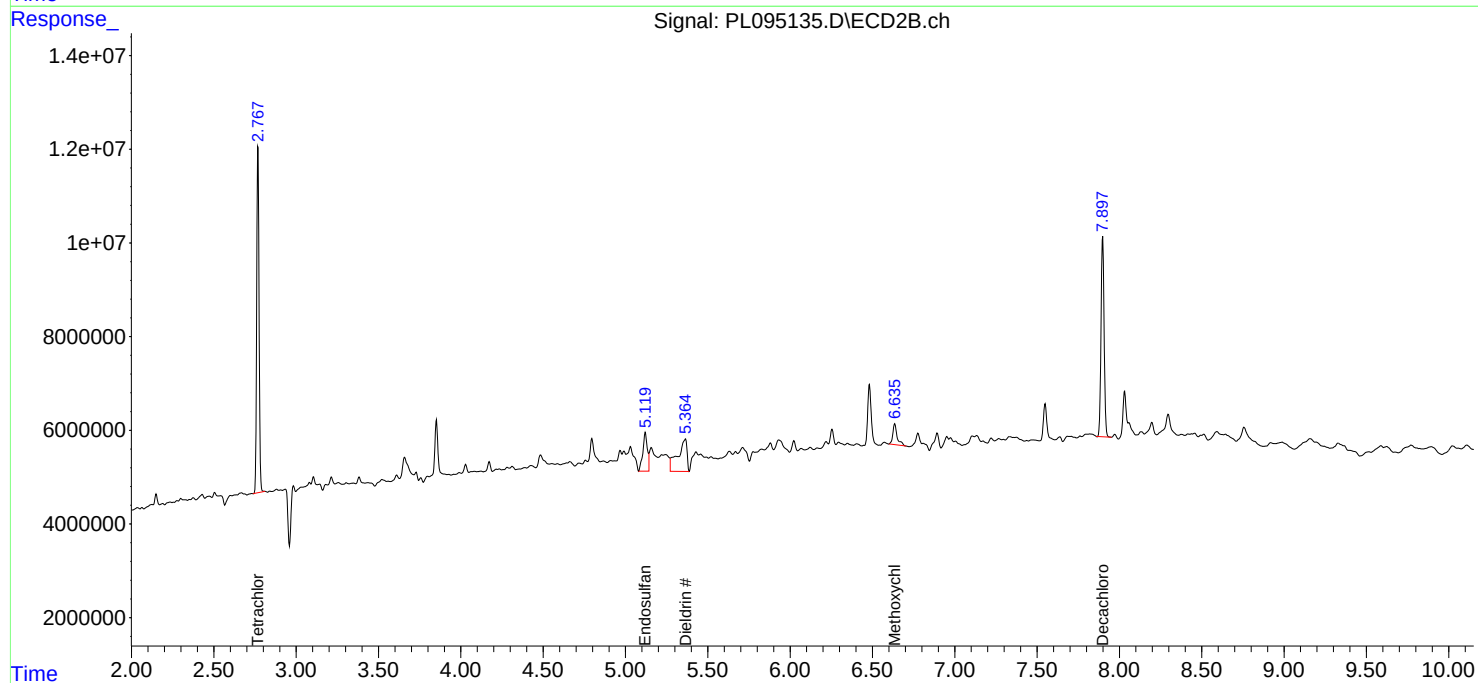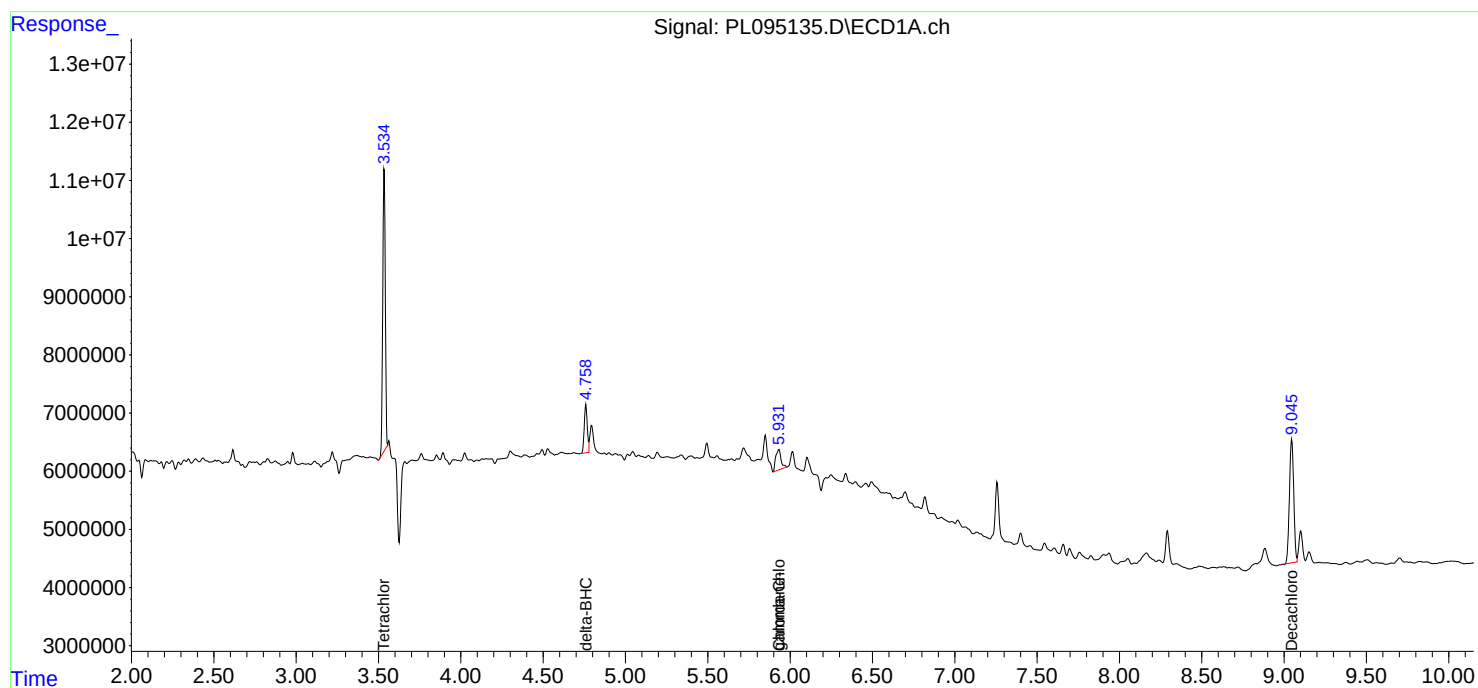


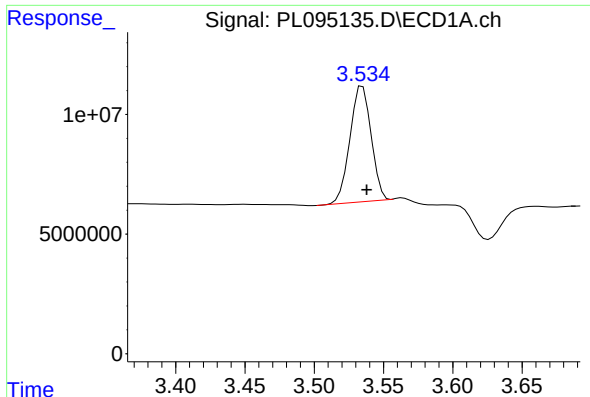

#1 Tetrachloro-m-xylene


R.T.: 3.535 min
Delta R.T.: -0.003 min
Response: 51534805
Conc: 18.21 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1

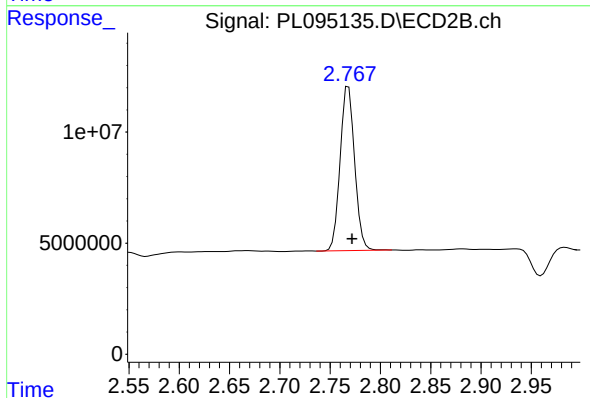


#1 Tetrachloro-m-xylene

R.T.: 2.768 min
Delta R.T.: -0.004 min
Response: 73926648
Conc: 20.71 ng/ml

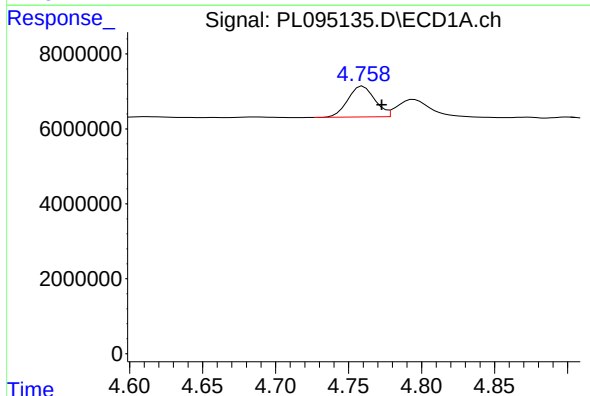


#7 delta-BHC

R.T.: 4.760 min
Delta R.T.: -0.013 min
Response: 10575517
Conc: 2.72 ng/ml

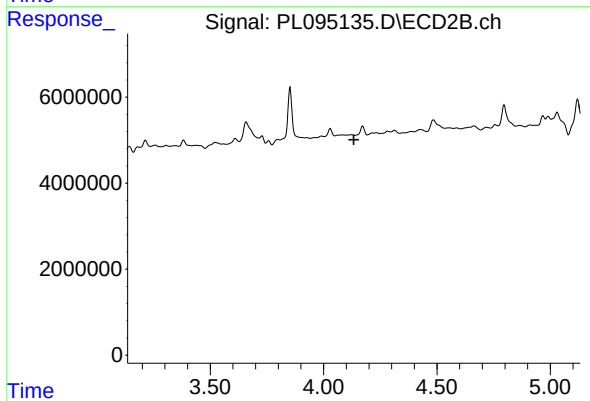

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.133 min
Response: 0
Conc: N.D.

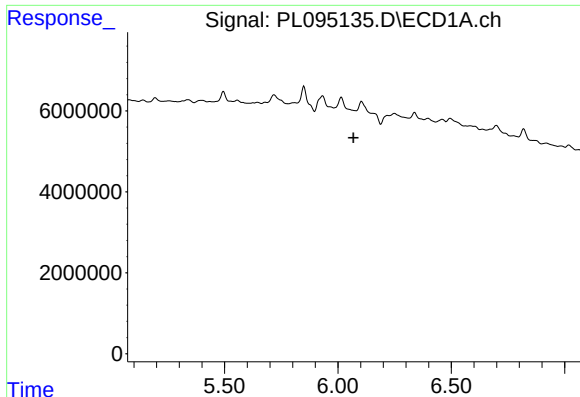

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.069 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-1

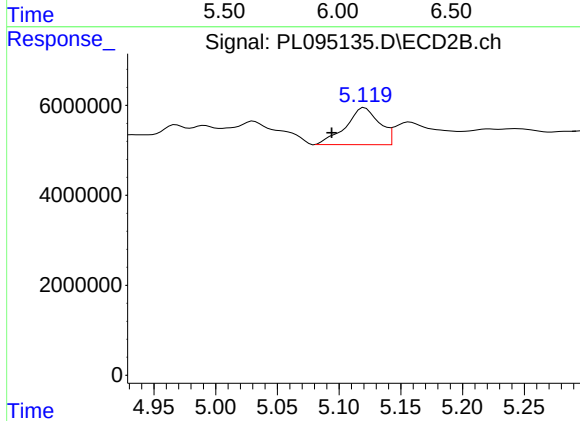


#9 Endosulfan I

R.T.: 5.121 min
Delta R.T.: 0.027 min
Response: 15574338
Conc: 3.55 ng/ml

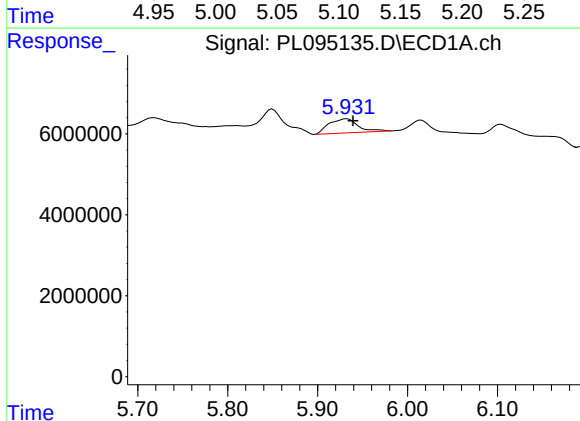


#10 gamma-Chlordane

R.T.: 5.933 min
Delta R.T.: -0.007 min
Response: 7845076
Conc: 2.33 ng/ml

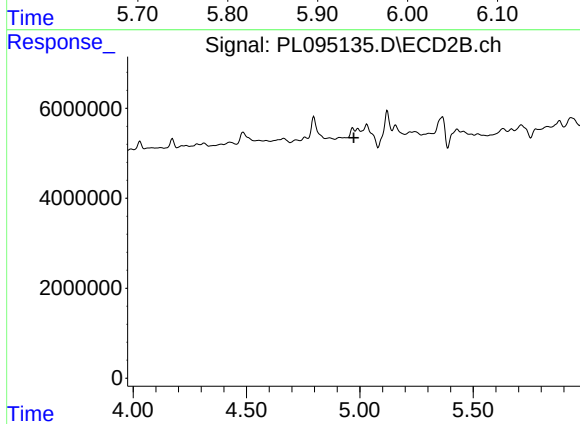

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 4.974 min
Response: 0
Conc: N.D.

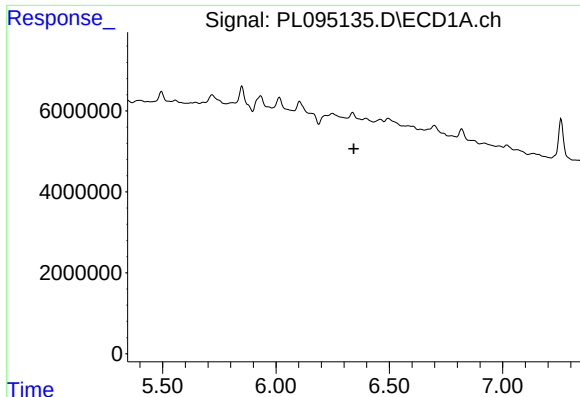

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 6.344 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-1

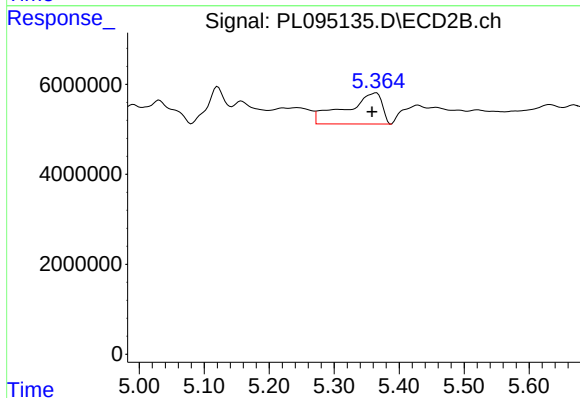


#13 Dieldrin

R.T.: 5.365 min
Delta R.T.: 0.007 min
Response: 27160443
Conc: 5.60 ng/ml

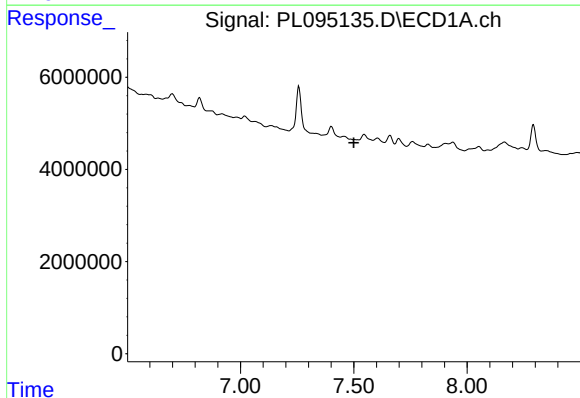


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.500 min
Response: 0
Conc: N.D.

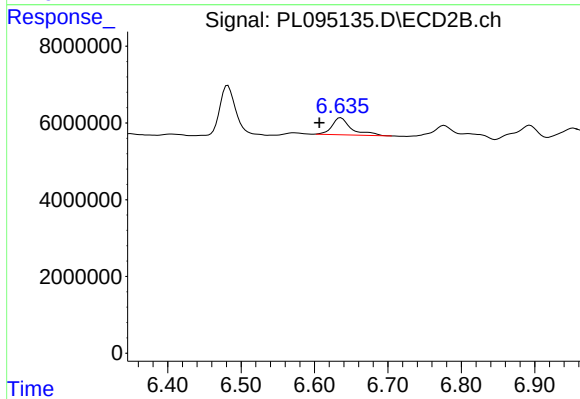

#20 Methoxychlor


R.T.: 6.636 min
Delta R.T.: 0.029 min
Response: 8175114
Conc: 3.85 ng/ml

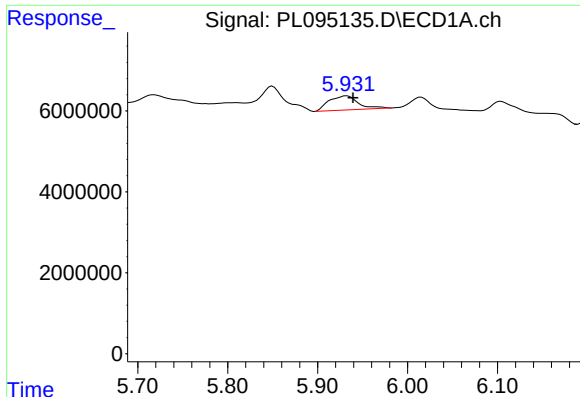

#25 Chlordane-3


R.T.: 5.933 min
Delta R.T.: -0.007 min
Response: 7845076
Conc: 15.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1

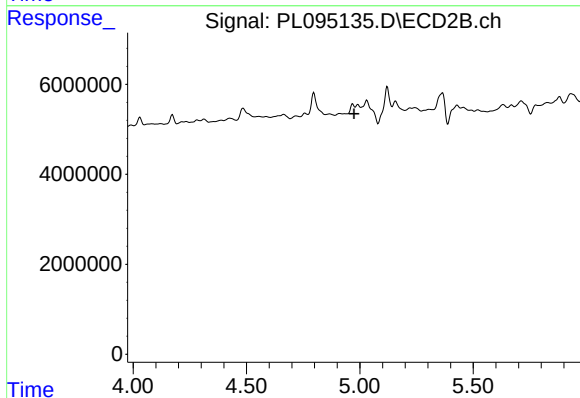


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 4.975 min
Response: 0
Conc: N.D.

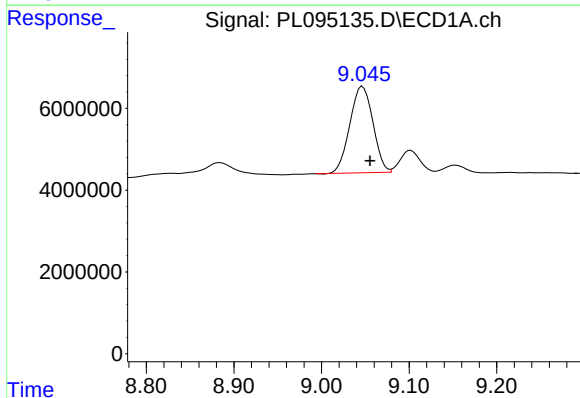

#28 Decachlorobiphenyl

R.T.: 9.047 min
Delta R.T.: -0.009 min
Response: 38687741
Conc: 18.36 ng/ml

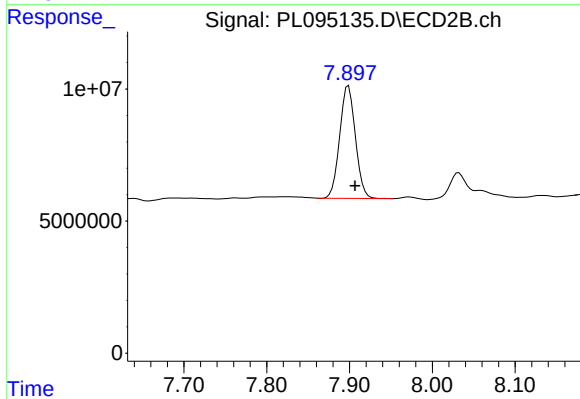

#28 Decachlorobiphenyl

R.T.: 7.899 min
Delta R.T.: -0.008 min
Response: 56070034
Conc: 13.88 ng/ml