

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040925\
 Data File : PL095141.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Apr 2025 18:03
 Operator : AR\AJ
 Sample : Q1752-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 10 01:24:41 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031125.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 11 17:42:21 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.535	2.768	100.9E6	76865913	35.648	21.535 #
28)	SA Decachlor...	9.050	7.899	42597380	69859429	20.213	17.295
Target Compounds							
6)	B beta-BHC	0.000	3.902	0	1837147	N.D.	0.827 #
7)	B delta-BHC	4.760	0.000	3780740	0	0.971	N.D. #
10)	B gamma-Chl...	5.935	4.969	8984595	8140029	2.667	1.686 #
11)	B alpha-Chl...	6.018	5.030	13396393	13533791	4.063	2.836 #
12)	B 4,4'-DDE	0.000	5.219	0	5715085	N.D.	1.229 #
17)	MA 4,4'-DDT	0.000	6.024	0	10309514	N.D.	2.557 #
25)	Chlordane-3	5.935	4.969	8984595	8140029	17.976	15.301
26)	Chlordane-4	6.018	5.030	13396393	13533791	22.741	25.999



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040925\
Data File : PL095141.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Apr 2025 18:03
Operator : AR\AJ
Sample : Q1752-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 10 01:24:41 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031125.M
Quant Title : GC Extractables
QLast Update : Tue Mar 11 17:42:21 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

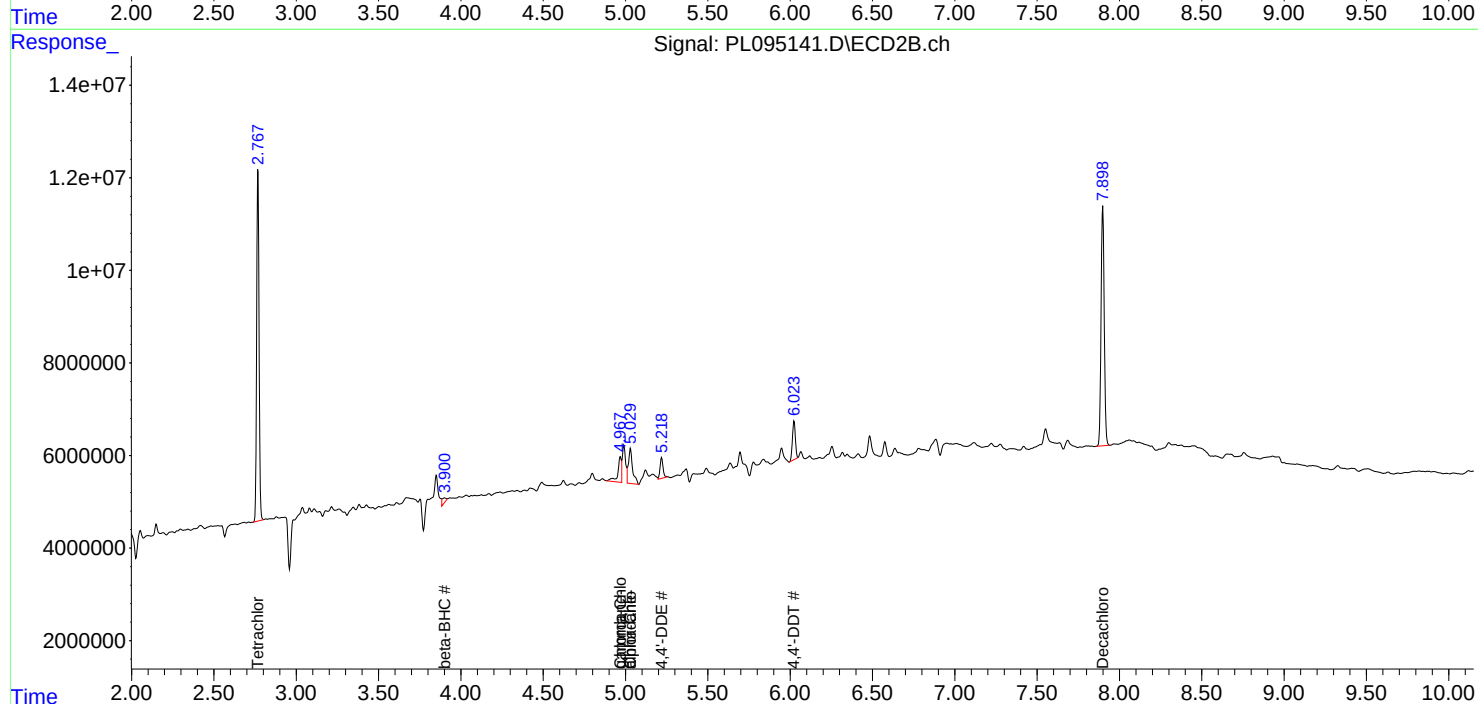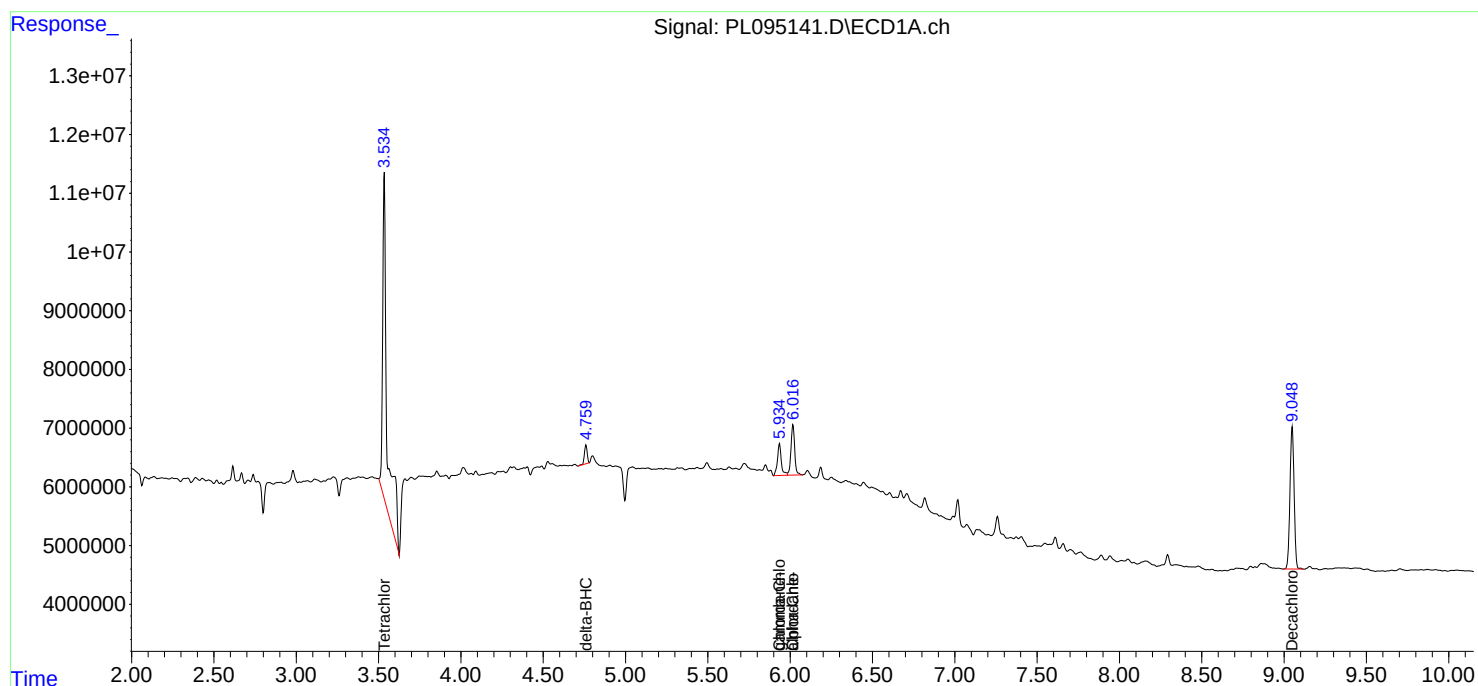


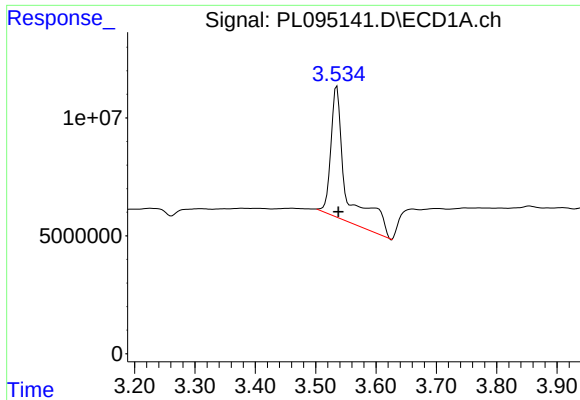

#1 Tetrachloro-m-xylene


R.T.: 3.535 min
Delta R.T.: -0.003 min
Response: 100908638
Conc: 35.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-2

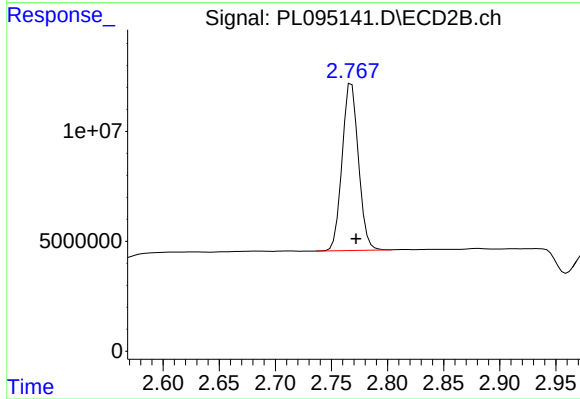


#1 Tetrachloro-m-xylene

R.T.: 2.768 min
Delta R.T.: -0.004 min
Response: 76865913
Conc: 21.54 ng/ml

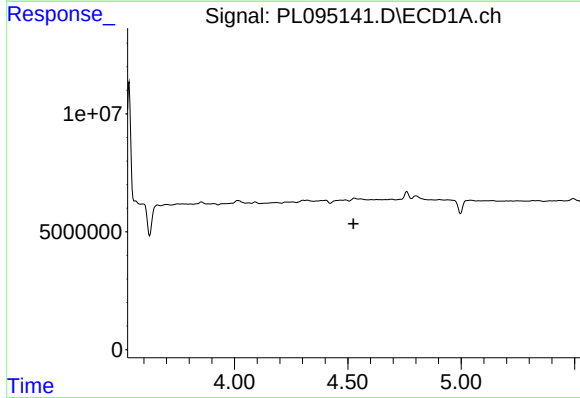


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.525 min
Response: 0
Conc: N.D.

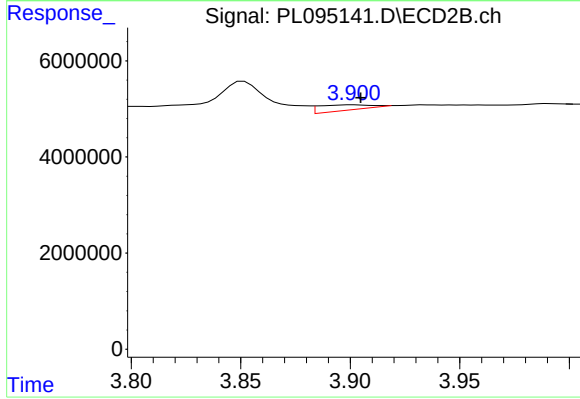

#6 beta-BHC


R.T.: 3.902 min
Delta R.T.: -0.003 min
Response: 1837147
Conc: 0.83 ng/ml

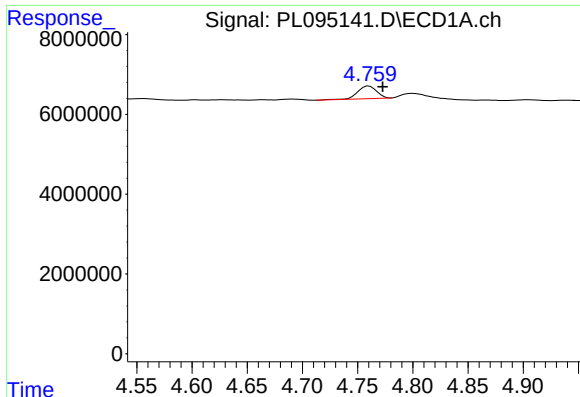

#7 delta-BHC


R.T.: 4.760 min
Delta R.T.: -0.012 min
Response: 3780740
Conc: 0.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-2

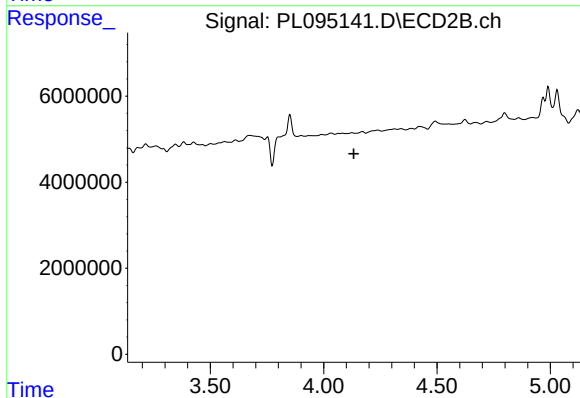


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.133 min
Response: 0
Conc: N.D.

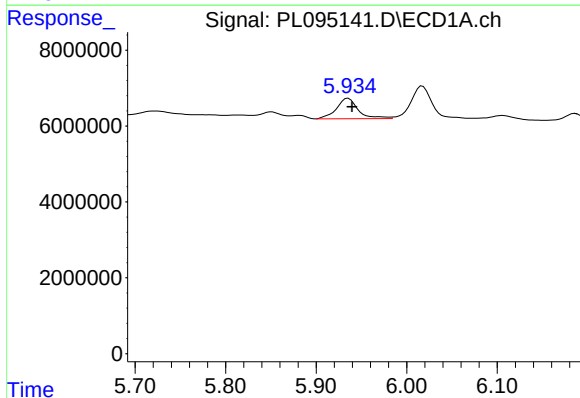


#10 gamma-Chlordane

R.T.: 5.935 min
Delta R.T.: -0.004 min
Response: 8984595
Conc: 2.67 ng/ml

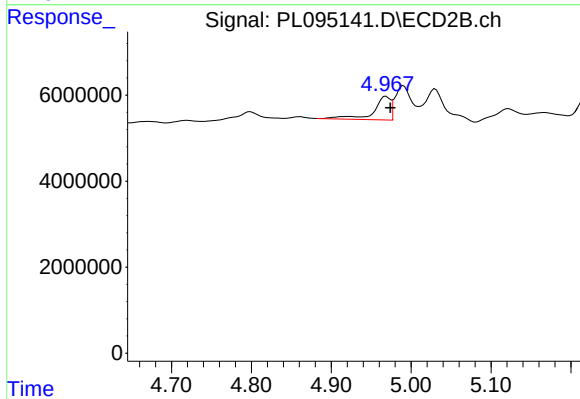

#10 gamma-Chlordane


R.T.: 4.969 min
Delta R.T.: -0.005 min
Response: 8140029
Conc: 1.69 ng/ml

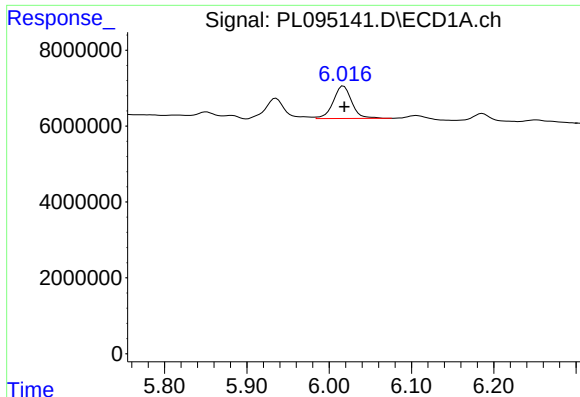

#11 alpha-Chlordane


R.T.: 6.018 min
Delta R.T.: 0.000 min
Response: 13396393
Conc: 4.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-2

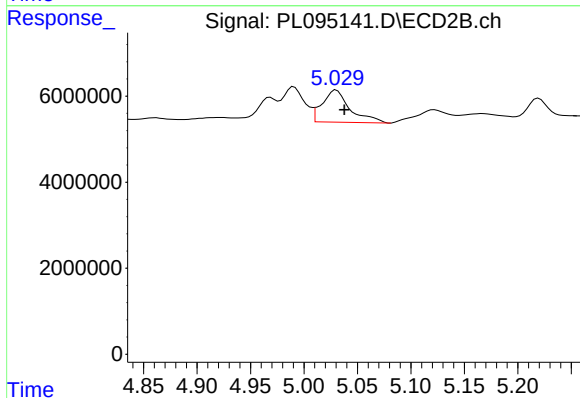


#11 alpha-Chlordane

R.T.: 5.030 min
Delta R.T.: -0.007 min
Response: 13533791
Conc: 2.84 ng/ml

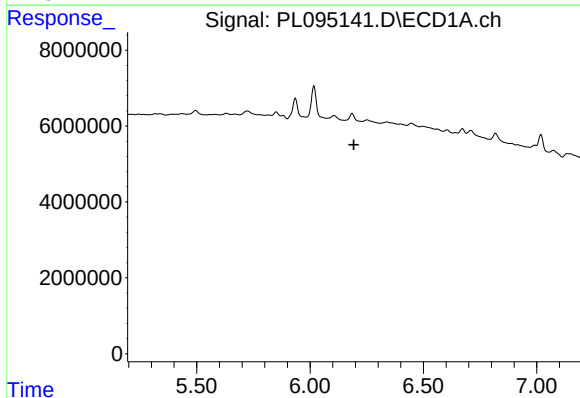


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 6.193 min
Response: 0
Conc: N.D.

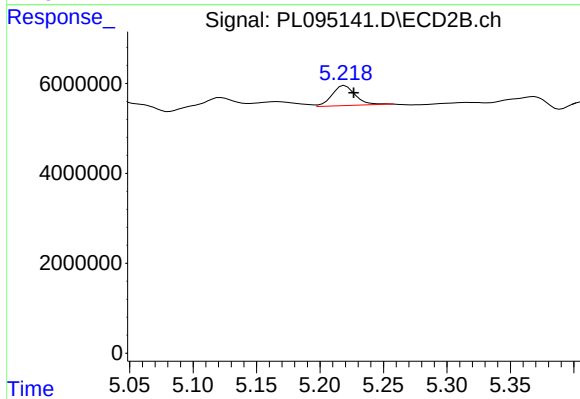

#12 4,4'-DDE


R.T.: 5.219 min
Delta R.T.: -0.007 min
Response: 5715085
Conc: 1.23 ng/ml

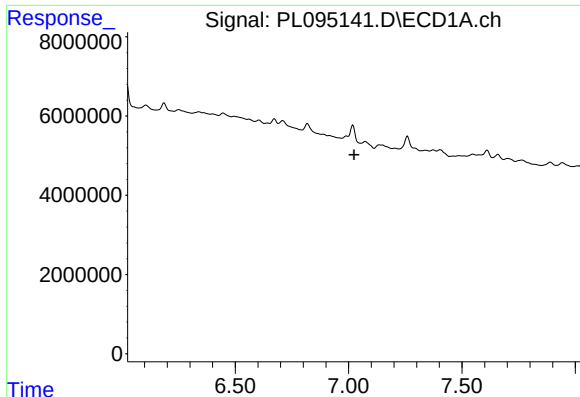

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 7.024 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-2

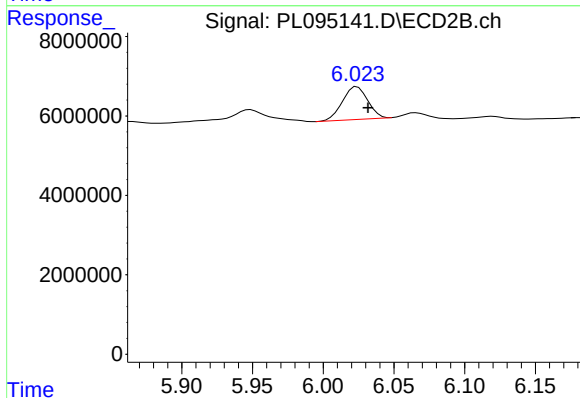


#17 4,4'-DDT

R.T.: 6.024 min
Delta R.T.: -0.008 min
Response: 10309514
Conc: 2.56 ng/ml

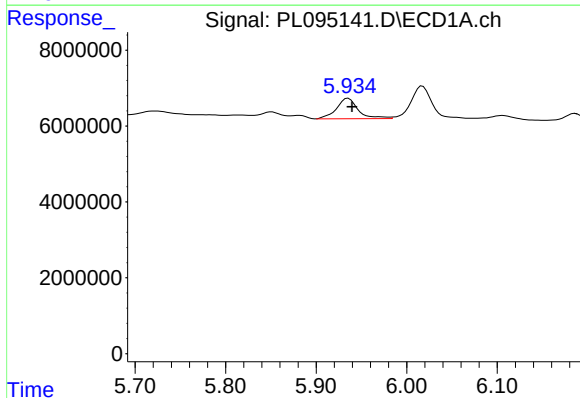


#25 Chlordane-3

R.T.: 5.935 min
Delta R.T.: -0.004 min
Response: 8984595
Conc: 17.98 ng/ml

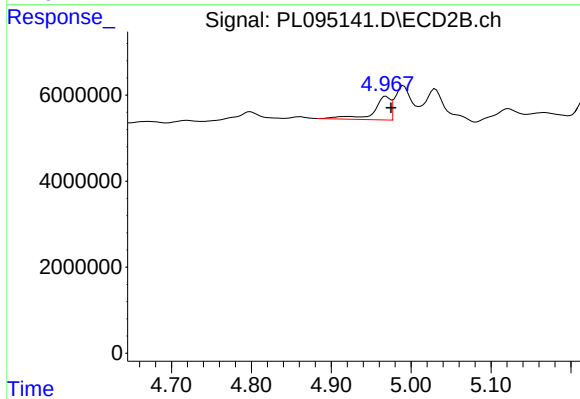

#25 Chlordane-3


R.T.: 4.969 min
Delta R.T.: -0.006 min
Response: 8140029
Conc: 15.30 ng/ml

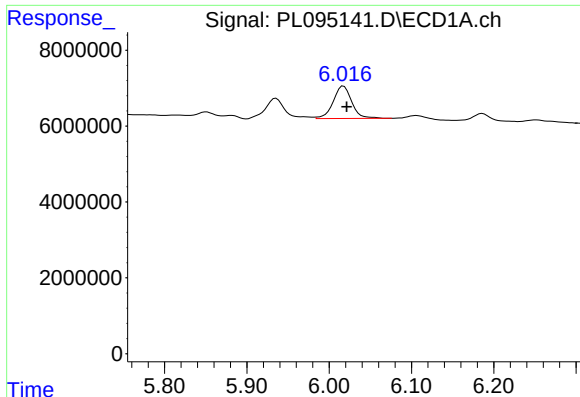

#26 Chlordane-4


R.T.: 6.018 min
Delta R.T.: -0.004 min
Response: 13396393
Conc: 22.74 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-2

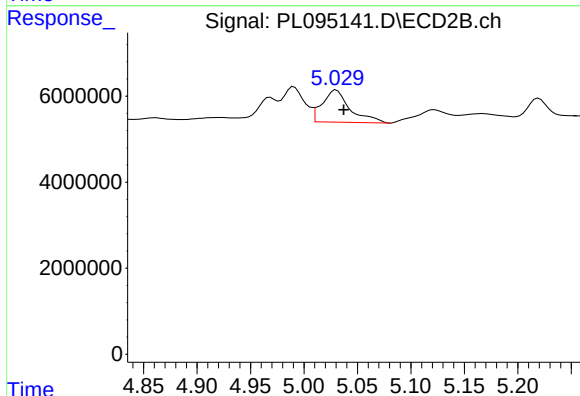


#26 Chlordane-4

R.T.: 5.030 min
Delta R.T.: -0.007 min
Response: 13533791
Conc: 26.00 ng/ml

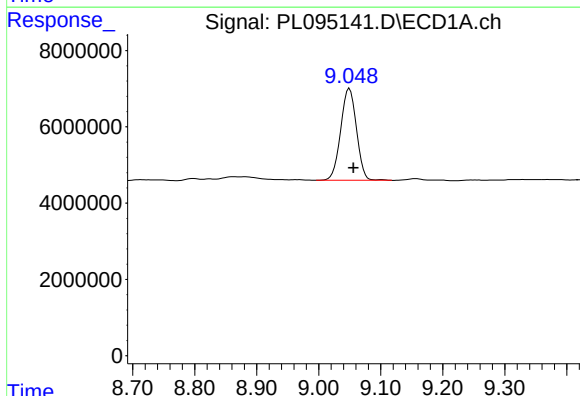

#28 Decachlorobiphenyl

R.T.: 9.050 min
Delta R.T.: -0.006 min
Response: 42597380
Conc: 20.21 ng/ml

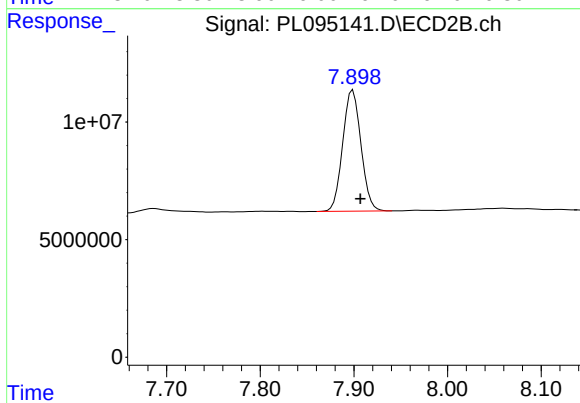

#28 Decachlorobiphenyl

R.T.: 7.899 min
Delta R.T.: -0.008 min
Response: 69859429
Conc: 17.29 ng/ml