

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040925\
 Data File : PL095151.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Apr 2025 20:48
 Operator : AR\AJ
 Sample : Q1752-07
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 10 01:26:40 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031125.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 11 17:42:21 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.534	2.768	57135400	76043962	20.184	21.305
28)	SA Decachlor...	9.045	7.897	38795431	70398952	18.409	17.428
Target Compounds							
2)	A alpha-BHC	0.000	3.258f	0	4191927	N.D.	0.778 #
8)	B Heptachlo...	0.000	4.717	0	7307784	N.D.	1.596 #
9)	A Endosulfan I	0.000	5.119f	0	13261321	N.D.	3.022 #
10)	B gamma-Chl...	5.934	4.990f	28706635	126.4E6	8.520	26.180 #
11)	B alpha-Chl...	6.018	5.028	82806797	36444394	25.117	7.636 #
12)	B 4,4'-DDE	0.000	5.219	0	7227337	N.D.	1.555 #
14)	MA Endrin	0.000	5.629	0	15583829	N.D.	3.571 #
15)	B Endosulfa...	0.000	5.925	0	10768569	N.D.	2.488 #
17)	MA 4,4'-DDT	0.000	6.021	0	6146582	N.D.	1.524 #
25)	Chlordane-3	5.934	4.990	28706635	126.4E6	57.434	237.607 #
26)	Chlordane-4	6.018	5.028	82806797	36444394	140.567	70.010 #
27)	Chlordane-5	0.000	5.925	0	10768569	N.D.	56.134 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040925\
Data File : PL095151.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Apr 2025 20:48
Operator : AR\AJ
Sample : Q1752-07
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 10 01:26:40 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031125.M
Quant Title : GC Extractables
QLast Update : Tue Mar 11 17:42:21 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

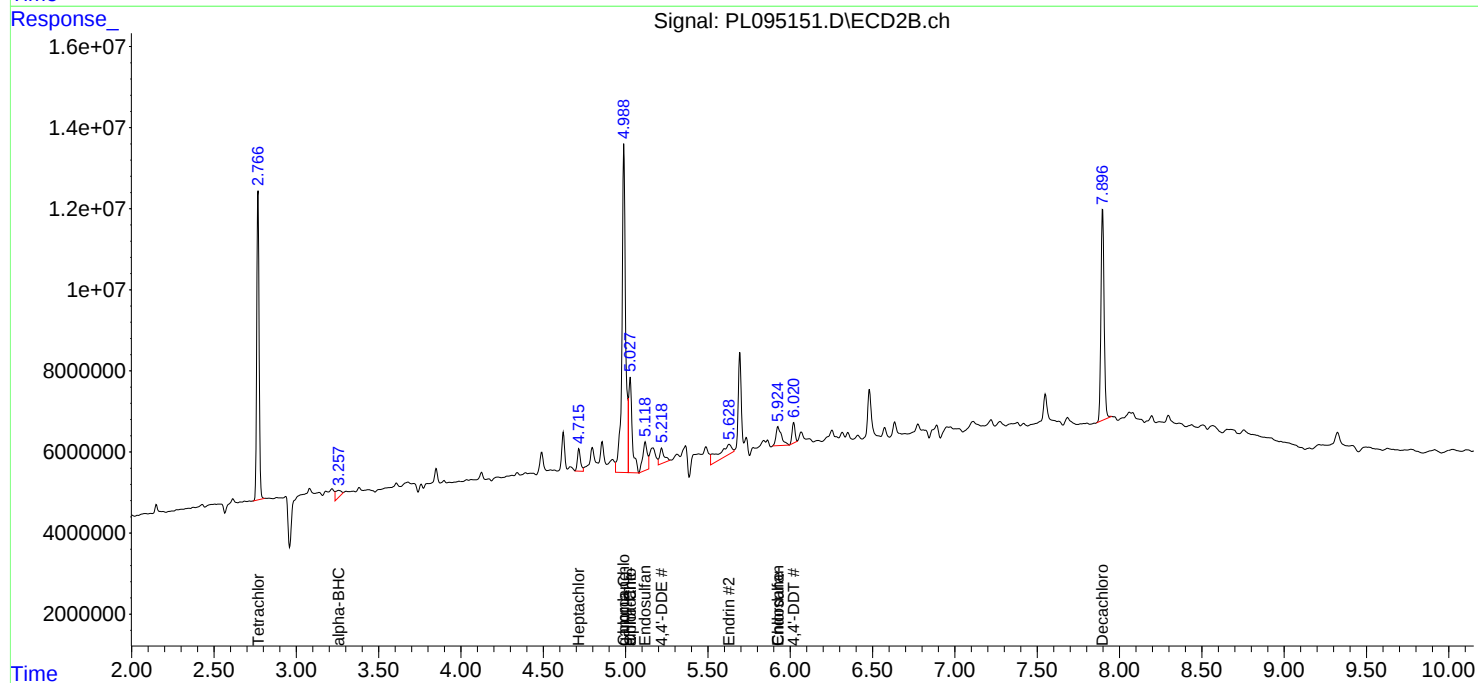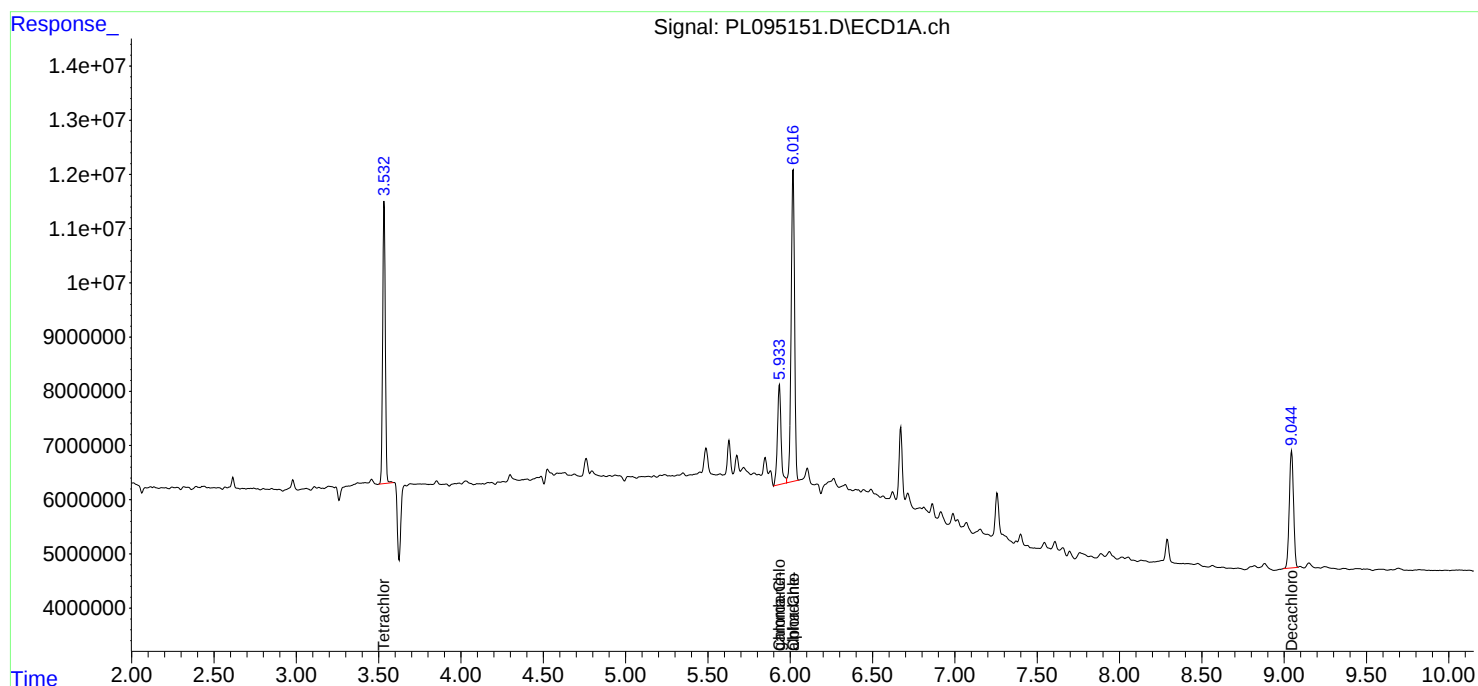


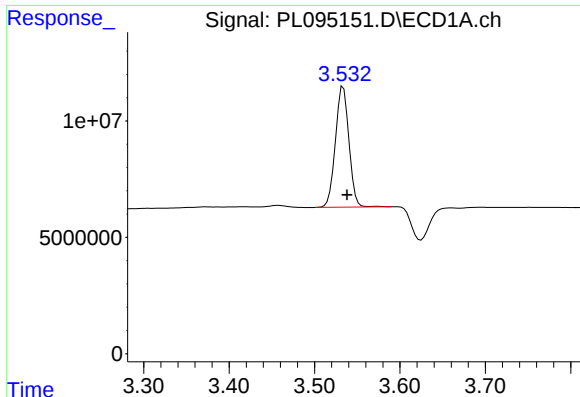

#1 Tetrachloro-m-xylene


R.T.: 3.534 min
Delta R.T.: -0.004 min
Response: 57135400
Conc: 20.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-3

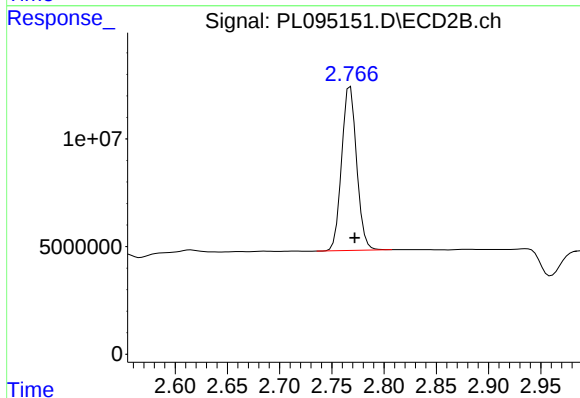


#1 Tetrachloro-m-xylene

R.T.: 2.768 min
Delta R.T.: -0.004 min
Response: 76043962
Conc: 21.31 ng/ml

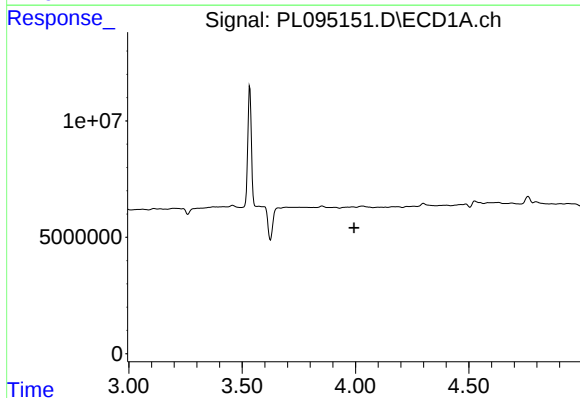


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.994 min
Response: 0
Conc: N.D.

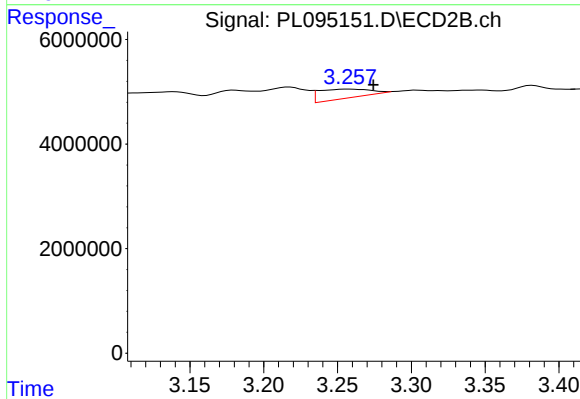

#2 alpha-BHC


R.T.: 3.258 min
Delta R.T.: -0.016 min
Response: 4191927
Conc: 0.78 ng/ml

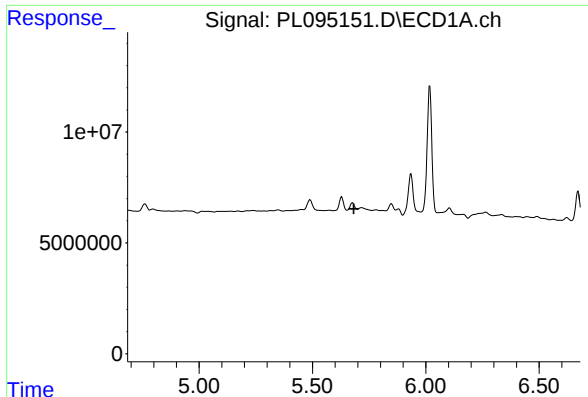

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.683 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-3

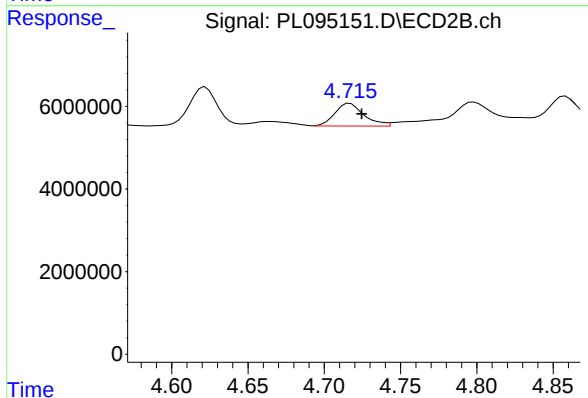


#8 Heptachlor epoxide

R.T.: 4.717 min
Delta R.T.: -0.008 min
Response: 7307784
Conc: 1.60 ng/ml

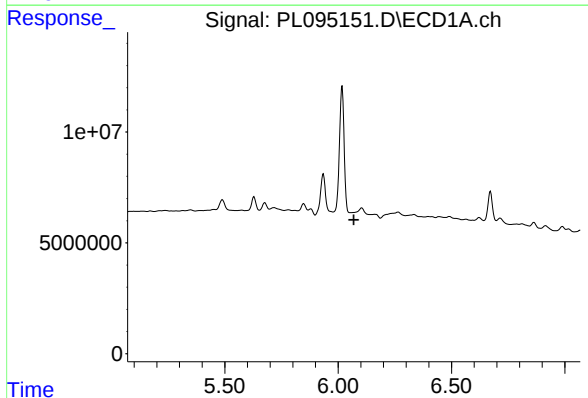


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 6.069 min
Response: 0
Conc: N.D.

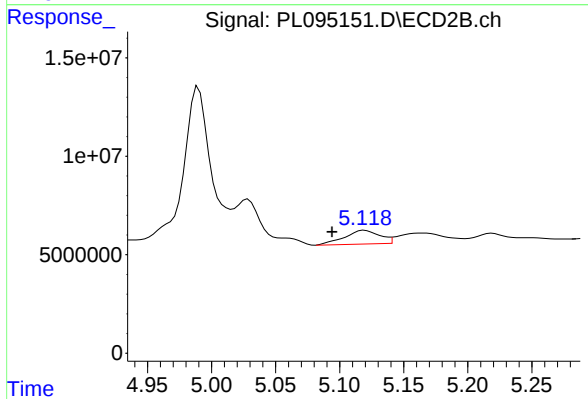

#9 Endosulfan I


R.T.: 5.119 min
Delta R.T.: 0.025 min
Response: 13261321
Conc: 3.02 ng/ml

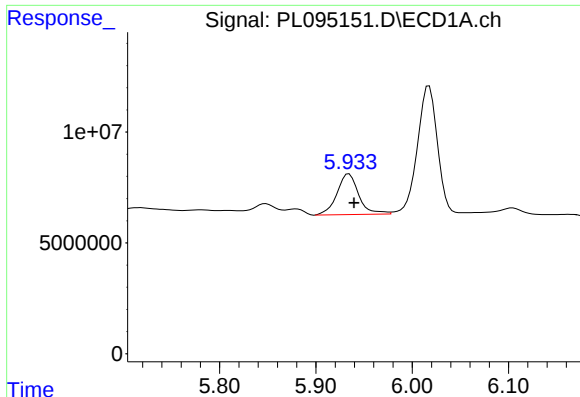

#10 gamma-Chlordane


R.T.: 5.934 min
Delta R.T.: -0.005 min
Response: 28706635
Conc: 8.52 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-3

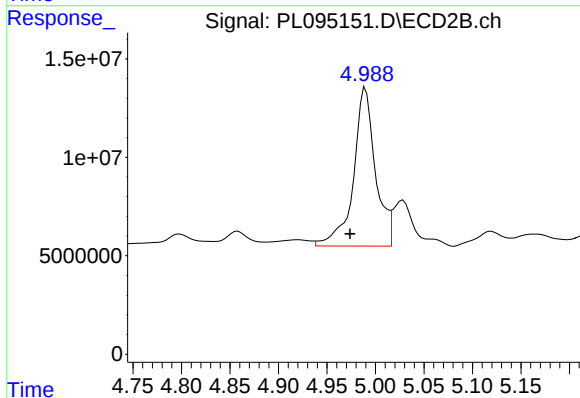


#10 gamma-Chlordane

R.T.: 4.990 min
Delta R.T.: 0.016 min
Response: 126406322
Conc: 26.18 ng/ml

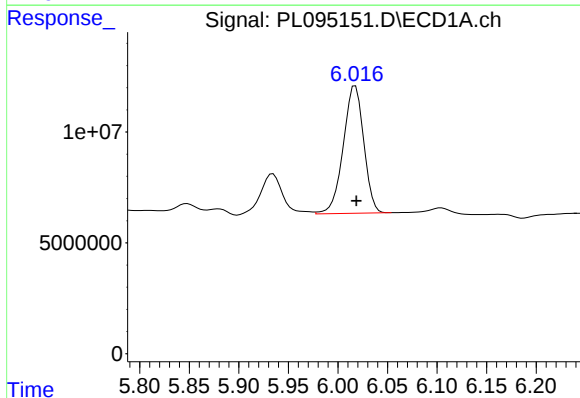


#11 alpha-Chlordane

R.T.: 6.018 min
Delta R.T.: 0.000 min
Response: 82806797
Conc: 25.12 ng/ml

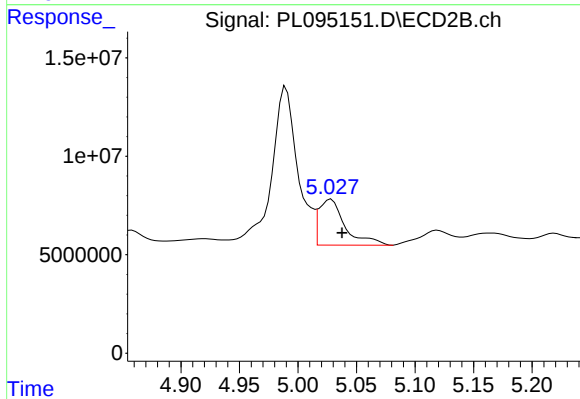

#11 alpha-Chlordane


R.T.: 5.028 min
Delta R.T.: -0.009 min
Response: 36444394
Conc: 7.64 ng/ml

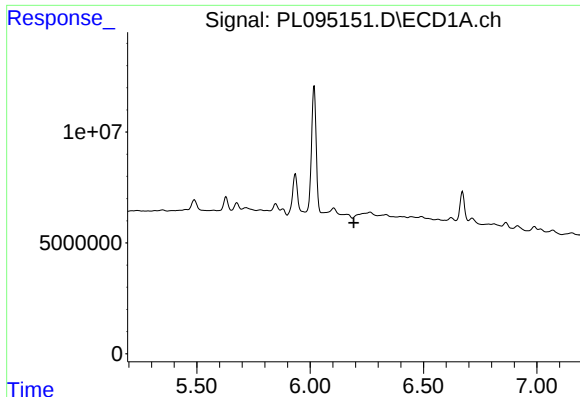

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 6.193 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-3

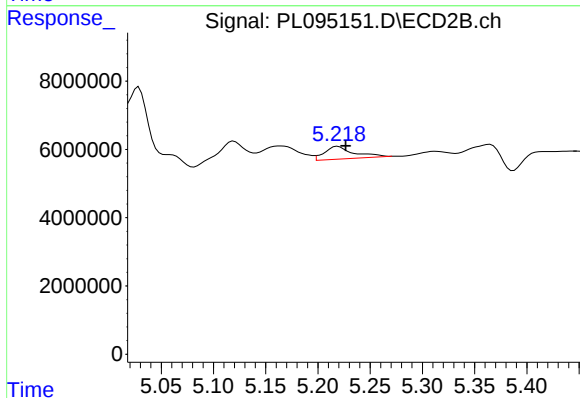


#12 4,4'-DDE

R.T.: 5.219 min
Delta R.T.: -0.008 min
Response: 7227337
Conc: 1.55 ng/ml

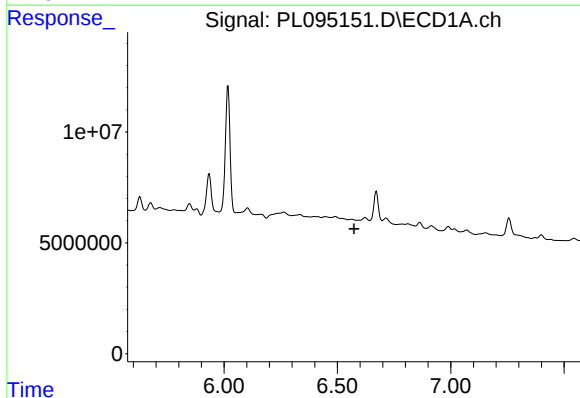


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.574 min
Response: 0
Conc: N.D.

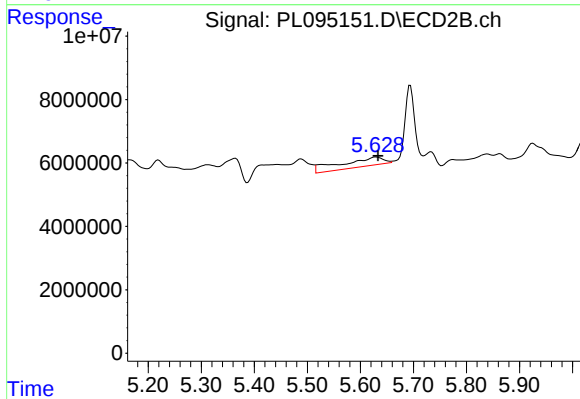

#14 Endrin


R.T.: 5.629 min
Delta R.T.: -0.004 min
Response: 15583829
Conc: 3.57 ng/ml

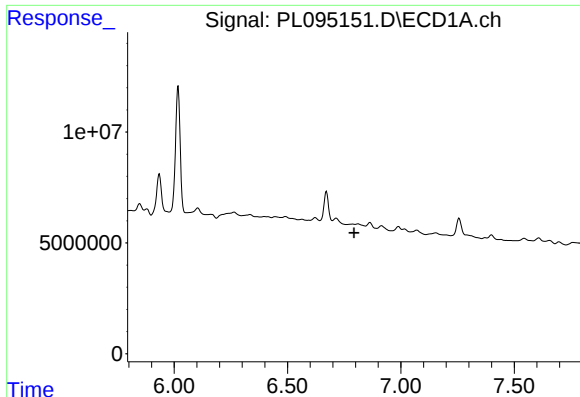

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.794 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-3

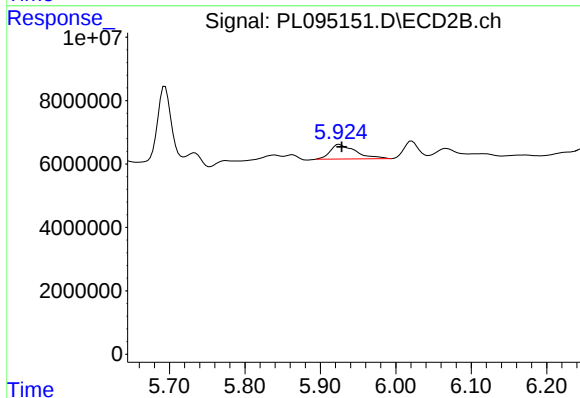


#15 Endosulfan II

R.T.: 5.925 min
Delta R.T.: -0.003 min
Response: 10768569
Conc: 2.49 ng/ml

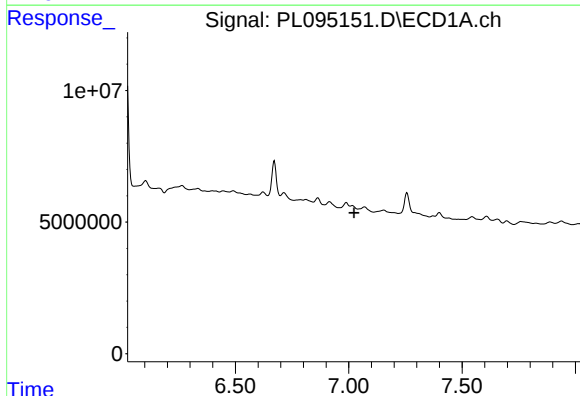


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 7.024 min
Response: 0
Conc: N.D.

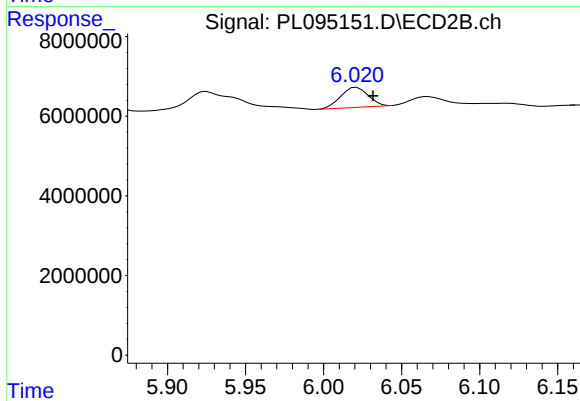

#17 4,4'-DDT


R.T.: 6.021 min
Delta R.T.: -0.010 min
Response: 6146582
Conc: 1.52 ng/ml

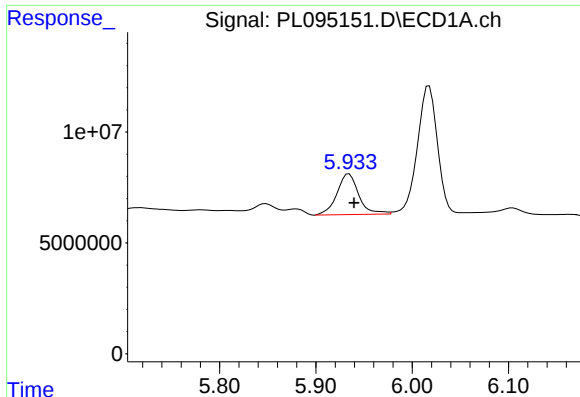

#25 Chlordane-3


R.T.: 5.934 min
Delta R.T.: -0.005 min
Response: 28706635
Conc: 57.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-3

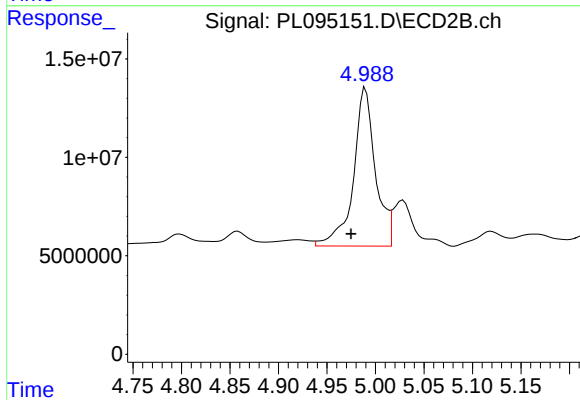


#25 Chlordane-3

R.T.: 4.990 min
Delta R.T.: 0.015 min
Response: 126406322
Conc: 237.61 ng/ml

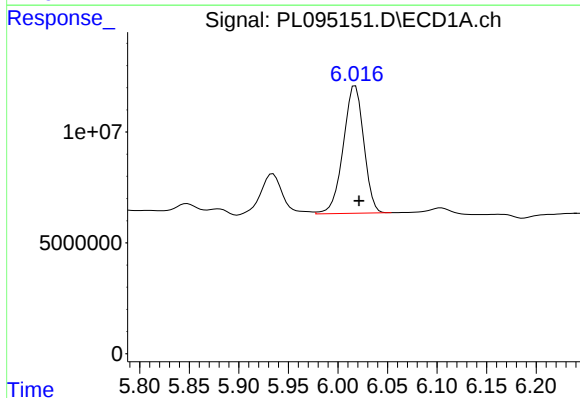


#26 Chlordane-4

R.T.: 6.018 min
Delta R.T.: -0.004 min
Response: 82806797
Conc: 140.57 ng/ml

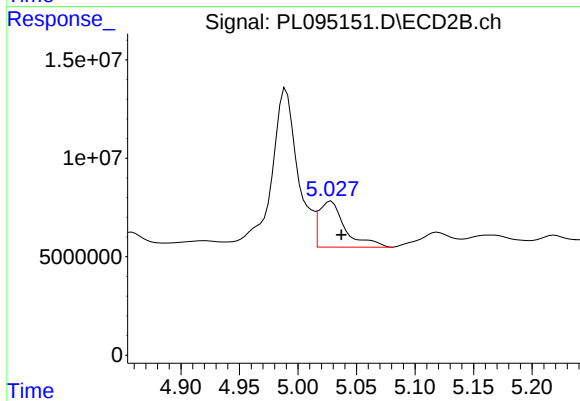

#26 Chlordane-4


R.T.: 5.028 min
Delta R.T.: -0.009 min
Response: 36444394
Conc: 70.01 ng/ml

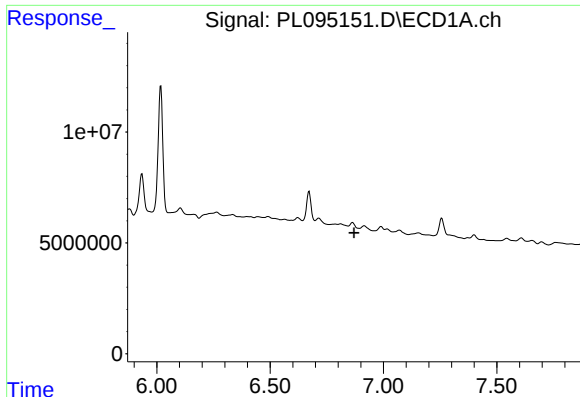

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.871 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-3

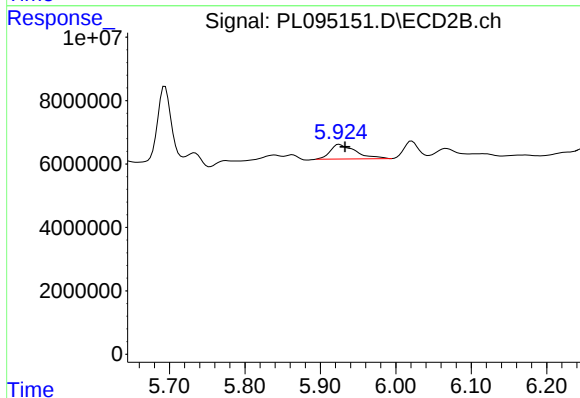


#27 Chlordane-5

R.T.: 5.925 min
Delta R.T.: -0.008 min
Response: 10768569
Conc: 56.13 ng/ml

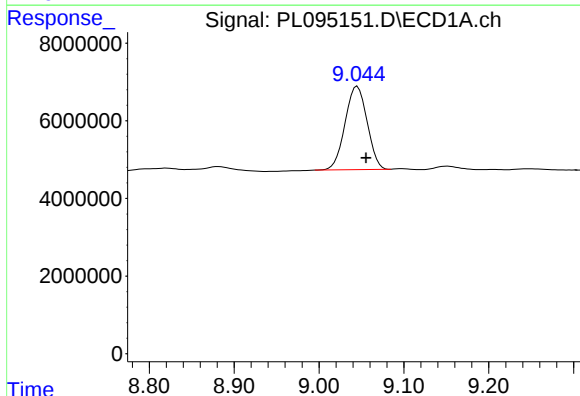

#28 Decachlorobiphenyl

R.T.: 9.045 min
Delta R.T.: -0.010 min
Response: 38795431
Conc: 18.41 ng/ml

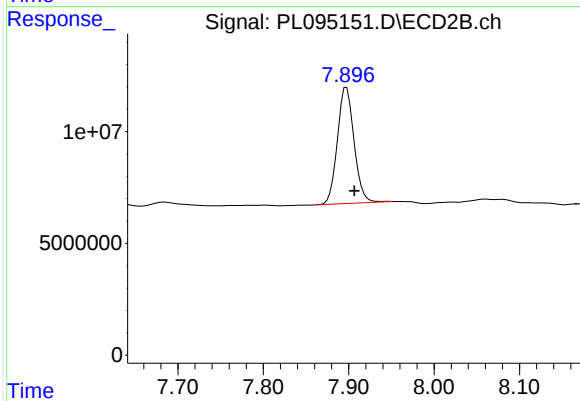

#28 Decachlorobiphenyl

R.T.: 7.897 min
Delta R.T.: -0.009 min
Response: 70398952
Conc: 17.43 ng/ml