

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041019\
 Data File : PL047236.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Apr 2019 01:50
 Operator : AJ\SJ
 Sample : PSTDCCC050
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 11 11:59:36 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:40:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.357	3.976	351.8E6	114.7E6	48.362	50.103
28)	SA Decachlor...	8.033	9.028	387.6E6	113.9E6	46.079	49.133
Target Compounds							
2)	A alpha-BHC	3.786	4.365	576.7E6	166.5E6	49.447	51.814
3)	MA gamma-BHC...	4.063	4.650	522.6E6	154.2E6	48.643	51.518
4)	MA Heptachlor	4.350	5.156	521.1E6	151.1E6	47.265	49.138
5)	MB Aldrin	4.590	5.460	505.7E6	147.0E6	49.024	51.314
6)	B beta-BHC	4.317	4.823	214.4E6	69034815	47.620	52.075
7)	B delta-BHC	4.512	5.039	506.3E6	131.1E6	50.019	56.524
8)	B Heptachlo...	5.027	5.846	474.0E6	137.8E6	48.596	52.244
9)	A Endosulfan I	5.359	6.202	448.2E6	132.7E6	47.667	50.856
10)	B gamma-Chl...	5.250	6.081	491.9E6	153.7E6	47.889	54.145
11)	B alpha-Chl...	5.306	6.153	479.3E6	144.9E6	47.277	51.090
12)	B 4,4'-DDE	5.474	6.311	417.4E6	125.2E6	45.333	50.426
13)	MA Dieldrin	5.599	6.459	484.1E6	134.6E6	48.243	49.653
14)	MA Endrin	5.852	6.677	410.2E6	109.2E6	43.544	45.705
15)	B Endosulfa...	6.127	6.887	426.5E6	121.1E6	47.599	50.202
16)	A 4,4'-DDD	5.985	6.801	406.2E6	111.9E6	53.738	55.592
17)	MA 4,4'-DDT	6.219	7.099	303.5E6	86015536	40.074	41.019
18)	B Endrin al...	6.293	7.011	353.7E6	104.6E6	47.194	49.234
19)	B Endosulfa...	6.505	7.233	392.8E6	113.4E6	47.839	48.073
20)	A Methoxychlor	6.764	7.557	146.3E6	51321571	34.415	40.259
21)	B Endrin ke...	6.987	7.703	458.6E6	129.2E6	49.594	52.019
22)	Mirex	7.163	8.154	326.6E6	97059411	44.827	48.526
24)	Chlordane-2	0.000	5.460f	0	147.0E6	N.D.	1258.583 #
25)	Chlordane-3	5.250	6.081	491.9E6	153.7E6	441.729	403.046
26)	Chlordane-4	5.306	6.153	479.3E6	144.9E6	463.558	314.081 #
27)	Chlordane-5	6.127	0.000	426.5E6	0	1249.658	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041019\
Data File : PL047236.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Apr 2019 01:50
Operator : AJ\SJ
Sample : PSTDCCC050
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 11 11:59:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

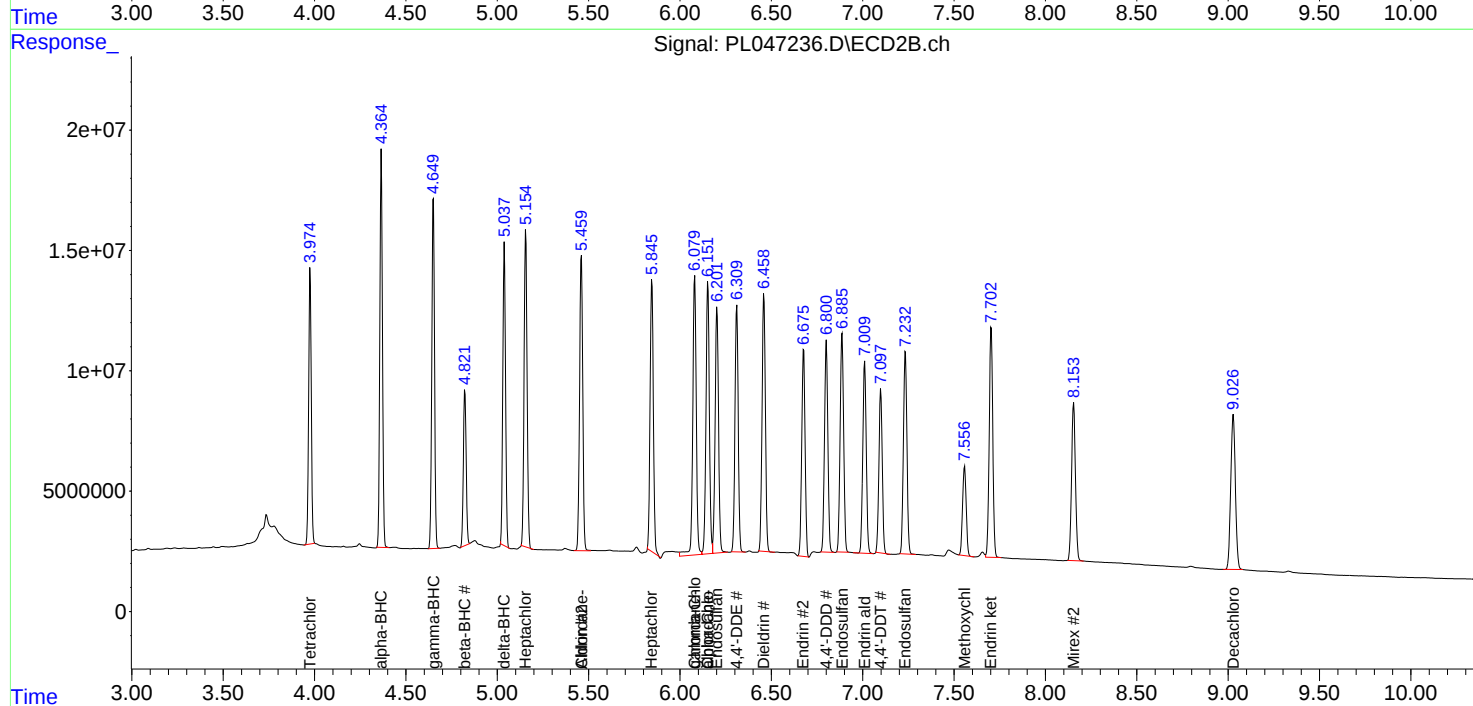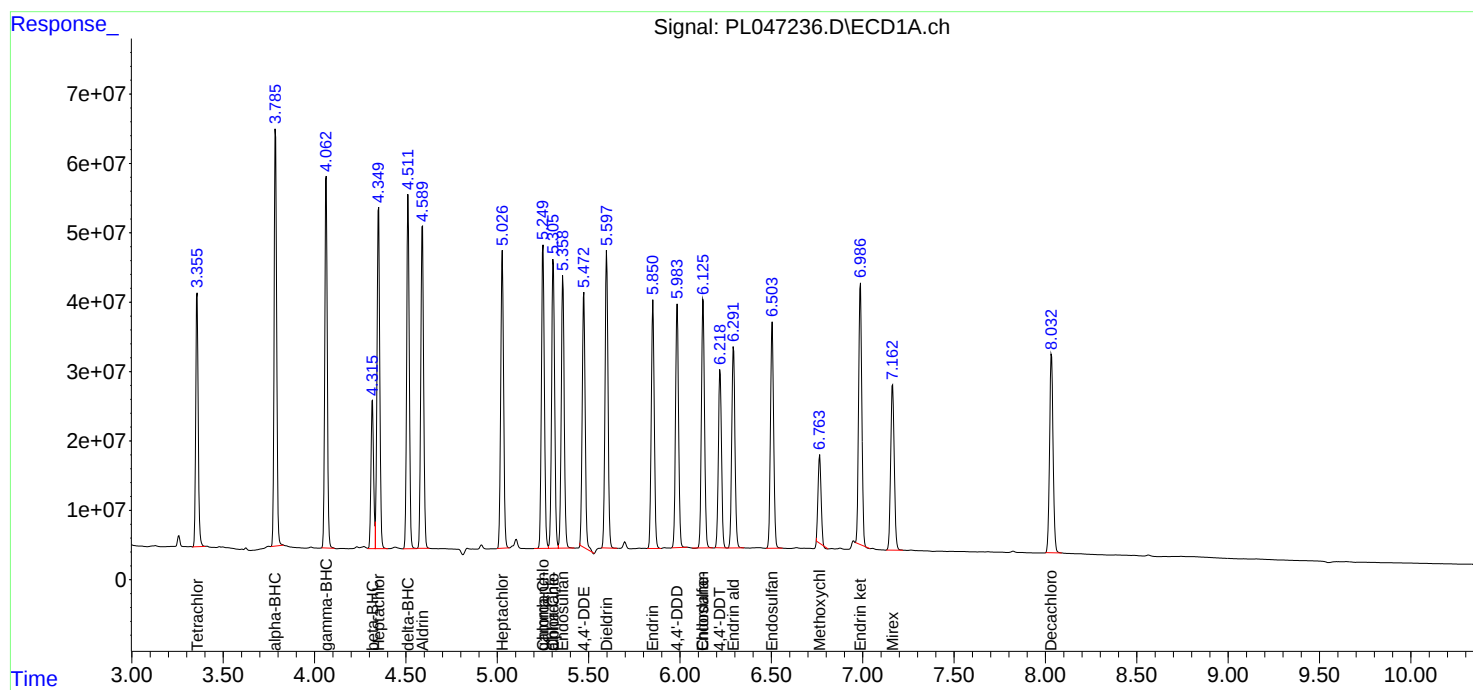


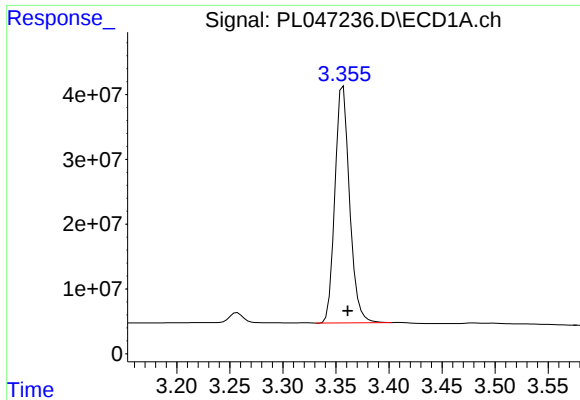

#1 Tetrachloro-m-xylene


R.T.: 3.357 min
Delta R.T.: -0.004 min
Response: 351814528
Conc: 48.36 ng/ml

Instrument :
ECD_L
ClientSampleId :

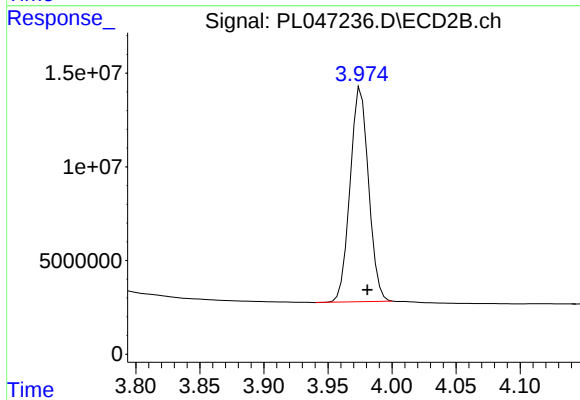


#1 Tetrachloro-m-xylene

R.T.: 3.976 min
Delta R.T.: -0.005 min
Response: 114715645
Conc: 50.10 ng/ml

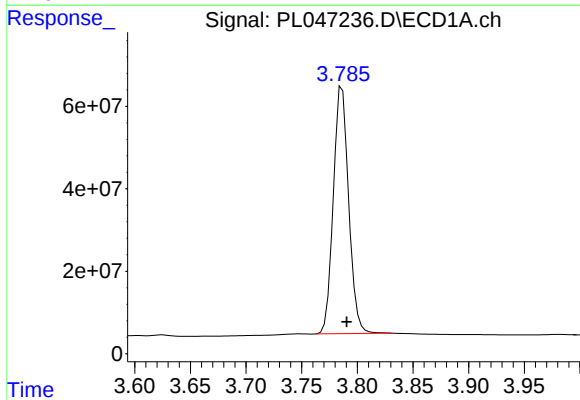


#2 alpha-BHC

R.T.: 3.786 min
Delta R.T.: -0.004 min
Response: 576656507
Conc: 49.45 ng/ml

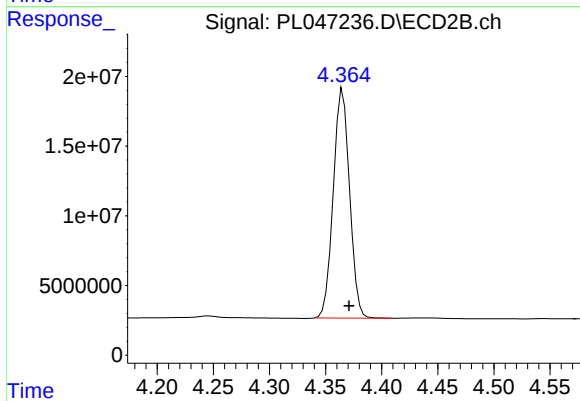

#2 alpha-BHC


R.T.: 4.365 min
Delta R.T.: -0.005 min
Response: 166495057
Conc: 51.81 ng/ml

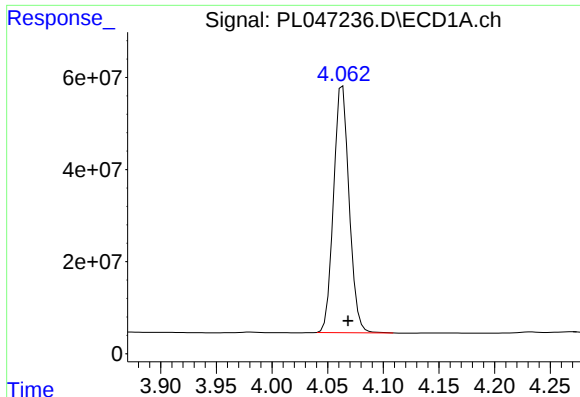

#3 gamma-BHC (Lindane)


R.T.: 4.063 min
Delta R.T.: -0.005 min
Response: 522640703
Conc: 48.64 ng/ml

Instrument :
ECD_L
ClientSampleId :

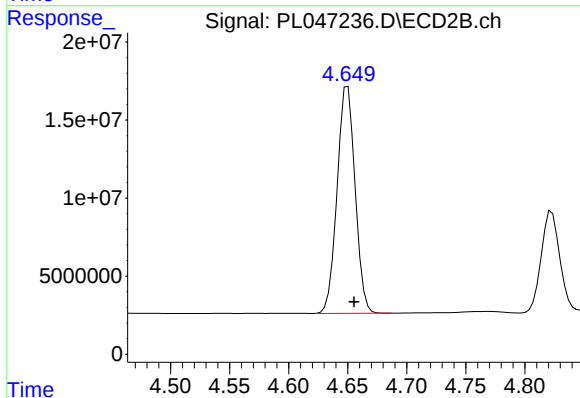


#3 gamma-BHC (Lindane)

R.T.: 4.650 min
Delta R.T.: -0.006 min
Response: 154195108
Conc: 51.52 ng/ml

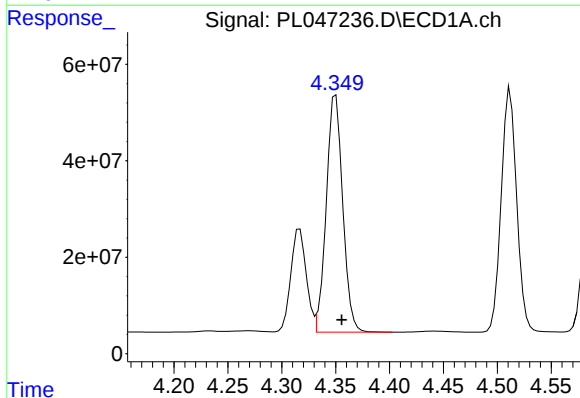


#4 Heptachlor

R.T.: 4.350 min
Delta R.T.: -0.006 min
Response: 521103601
Conc: 47.26 ng/ml

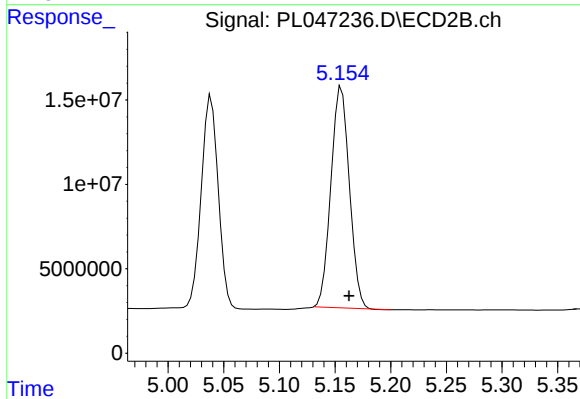

#4 Heptachlor


R.T.: 5.156 min
Delta R.T.: -0.007 min
Response: 151141261
Conc: 49.14 ng/ml

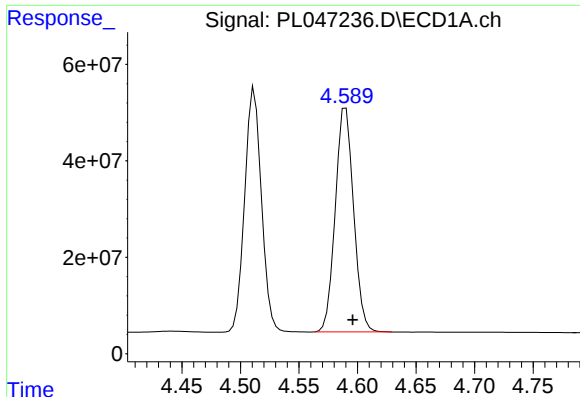

#5 Aldrin


R.T.: 4.590 min
Delta R.T.: -0.006 min
Response: 505685884
Conc: 49.02 ng/ml

Instrument :
ECD_L
ClientSampleId :

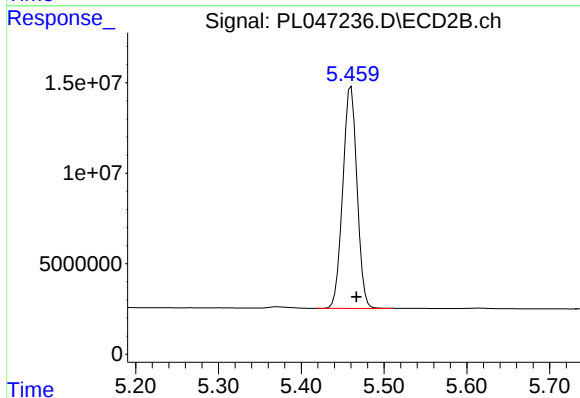


#5 Aldrin

R.T.: 5.460 min
Delta R.T.: -0.006 min
Response: 147014102
Conc: 51.31 ng/ml

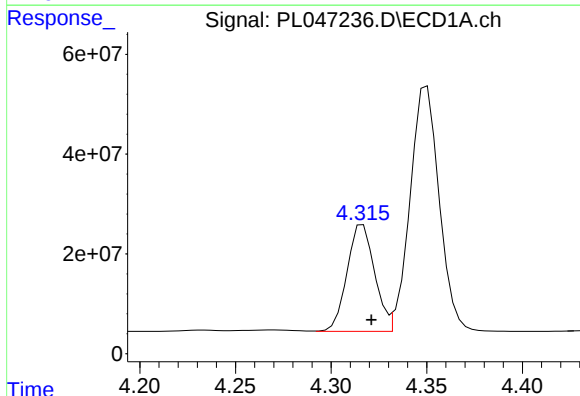


#6 beta-BHC

R.T.: 4.317 min
Delta R.T.: -0.004 min
Response: 214402989
Conc: 47.62 ng/ml

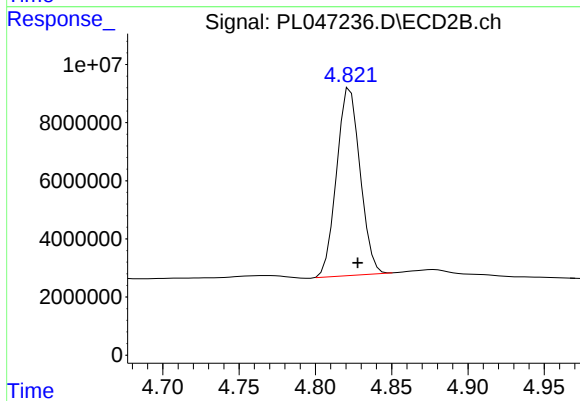

#6 beta-BHC


R.T.: 4.823 min
Delta R.T.: -0.005 min
Response: 69034815
Conc: 52.07 ng/ml

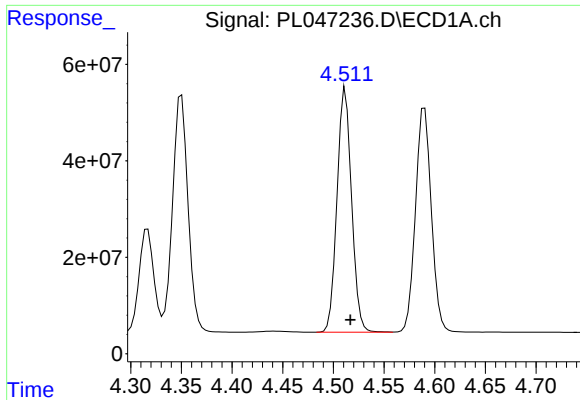

#7 delta-BHC


R.T.: 4.512 min
Delta R.T.: -0.005 min
Response: 506343102
Conc: 50.02 ng/ml

Instrument :
ECD_L
ClientSampleId :

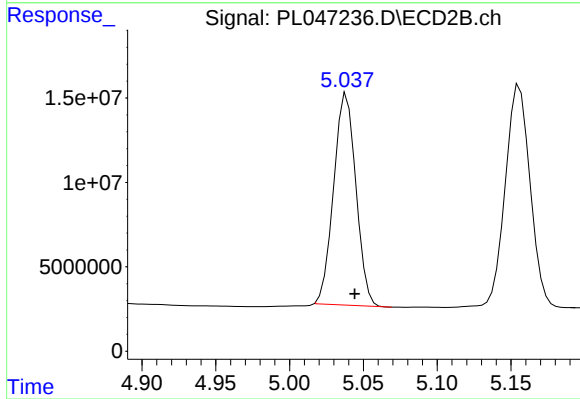


#7 delta-BHC

R.T.: 5.039 min
Delta R.T.: -0.005 min
Response: 131144594
Conc: 56.52 ng/ml

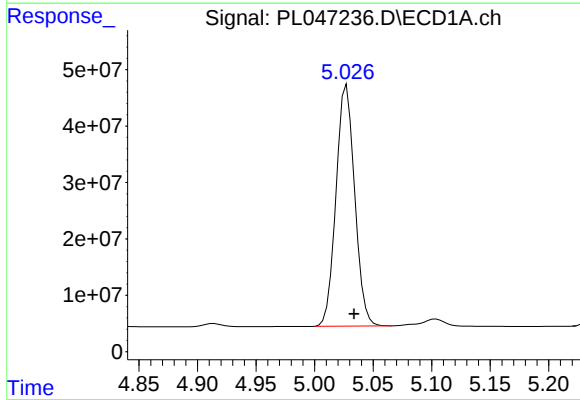


#8 Heptachlor epoxide

R.T.: 5.027 min
Delta R.T.: -0.006 min
Response: 473979762
Conc: 48.60 ng/ml

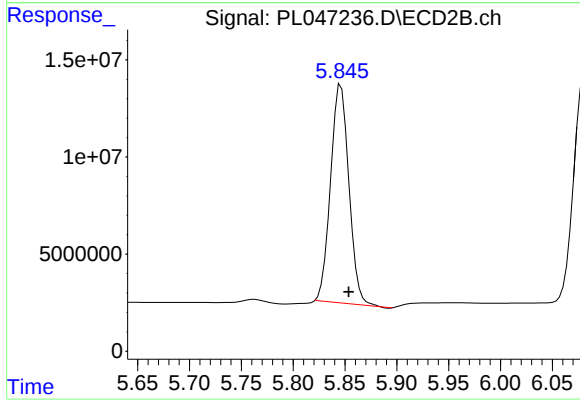

#8 Heptachlor epoxide


R.T.: 5.846 min
Delta R.T.: -0.008 min
Response: 137778162
Conc: 52.24 ng/ml

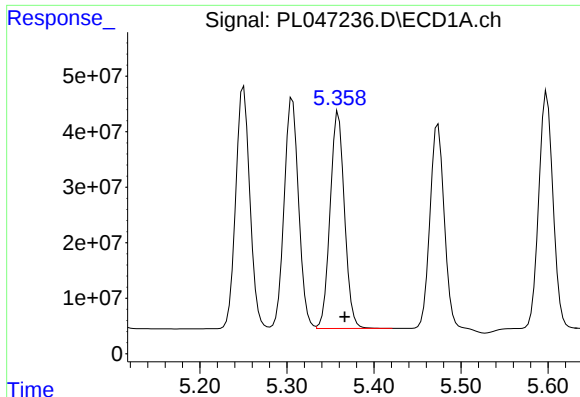

#9 Endosulfan I


R.T.: 5.359 min
Delta R.T.: -0.007 min
Response: 448181171
Conc: 47.67 ng/ml

Instrument :
ECD_L
ClientSampleId :

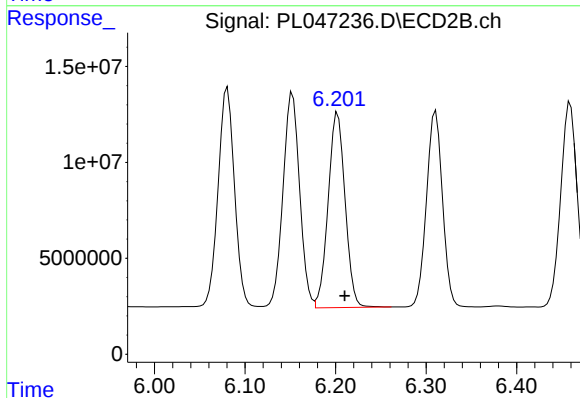


#9 Endosulfan I

R.T.: 6.202 min
Delta R.T.: -0.008 min
Response: 132728827
Conc: 50.86 ng/ml

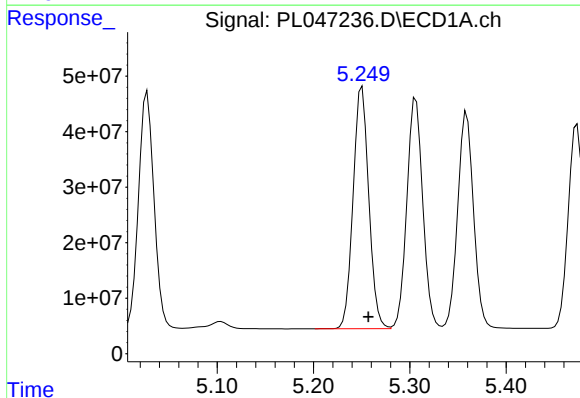


#10 gamma-Chlordane

R.T.: 5.250 min
Delta R.T.: -0.007 min
Response: 491941398
Conc: 47.89 ng/ml

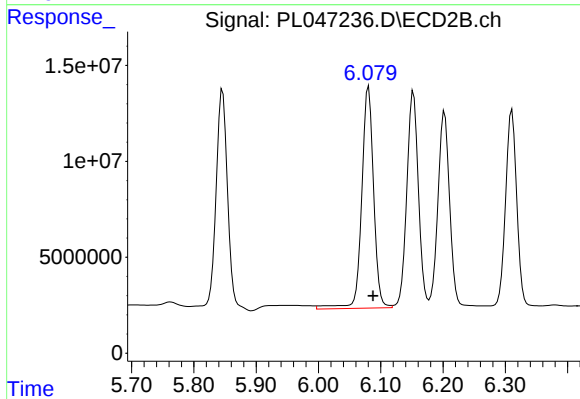

#10 gamma-Chlordane


R.T.: 6.081 min
Delta R.T.: -0.007 min
Response: 153668406
Conc: 54.15 ng/ml

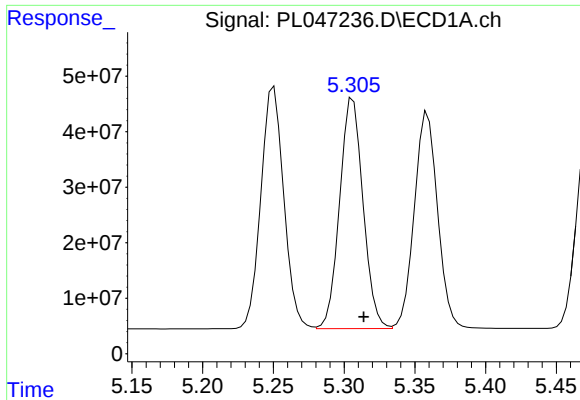

#11 alpha-Chlordane


R.T.: 5.306 min
Delta R.T.: -0.008 min
Response: 479346992
Conc: 47.28 ng/ml

Instrument :
ECD_L
ClientSampleId :

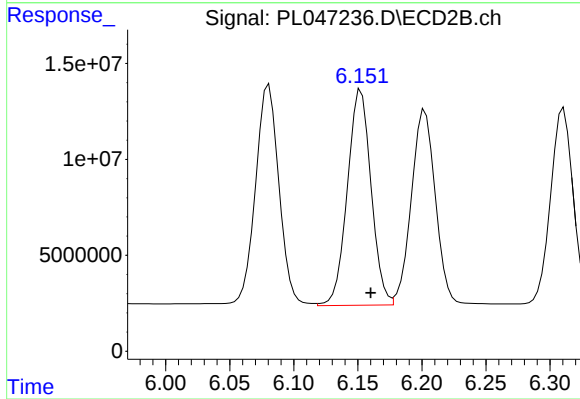


#11 alpha-Chlordane

R.T.: 6.153 min
Delta R.T.: -0.008 min
Response: 144924935
Conc: 51.09 ng/ml

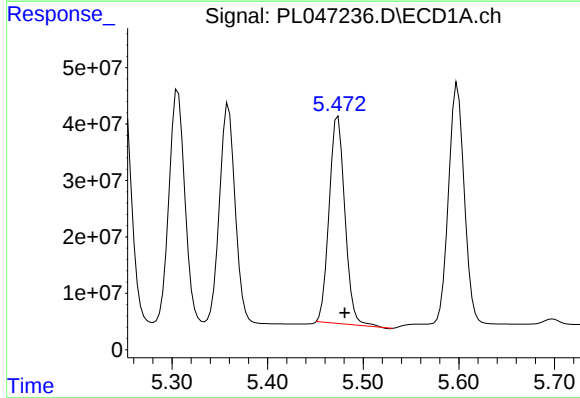


#12 4,4'-DDE

R.T.: 5.474 min
Delta R.T.: -0.007 min
Response: 417381778
Conc: 45.33 ng/ml

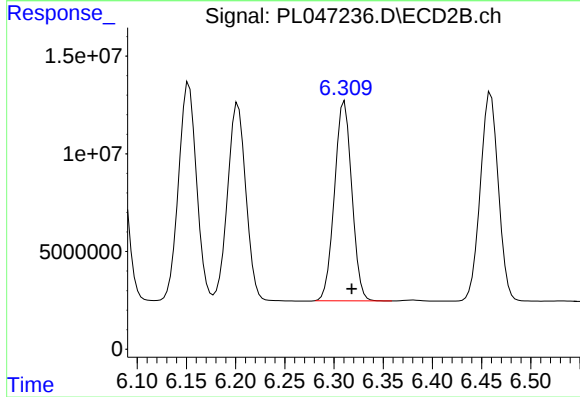

#12 4,4'-DDE


R.T.: 6.311 min
Delta R.T.: -0.007 min
Response: 125172933
Conc: 50.43 ng/ml

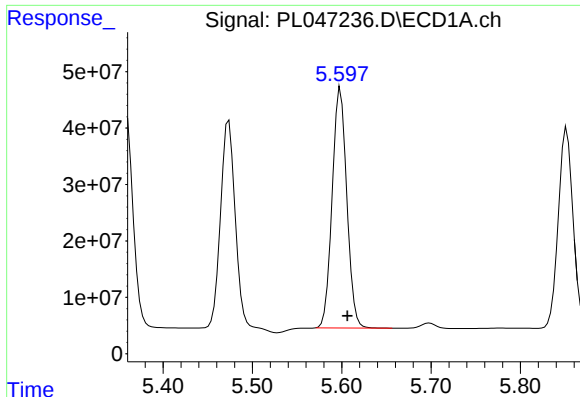

#13 Dieldrin


R.T.: 5.599 min
Delta R.T.: -0.008 min
Response: 484149204
Conc: 48.24 ng/ml

Instrument :
ECD_L
ClientSampleId :

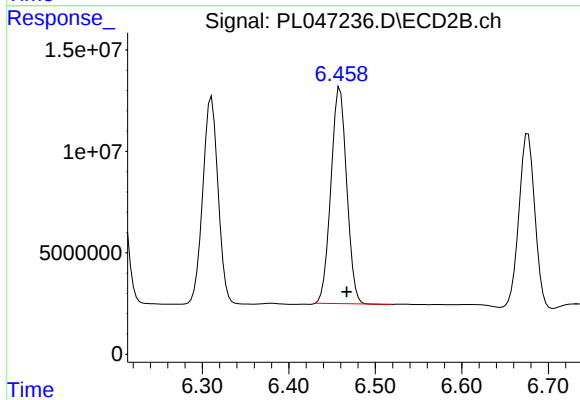


#13 Dieldrin

R.T.: 6.459 min
Delta R.T.: -0.008 min
Response: 134593198
Conc: 49.65 ng/ml

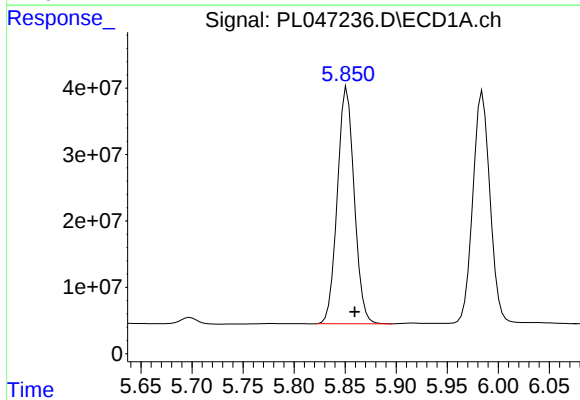


#14 Endrin

R.T.: 5.852 min
Delta R.T.: -0.008 min
Response: 410154612
Conc: 43.54 ng/ml

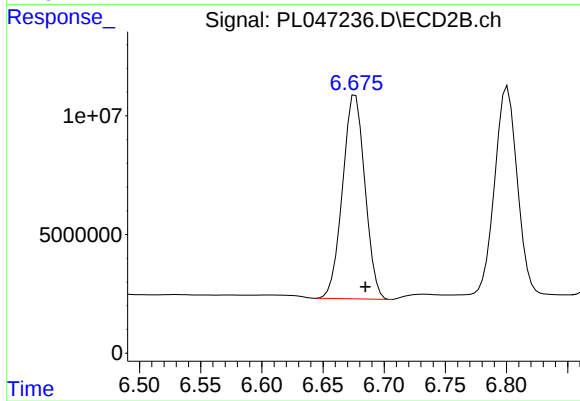

#14 Endrin


R.T.: 6.677 min
Delta R.T.: -0.008 min
Response: 109223462
Conc: 45.70 ng/ml

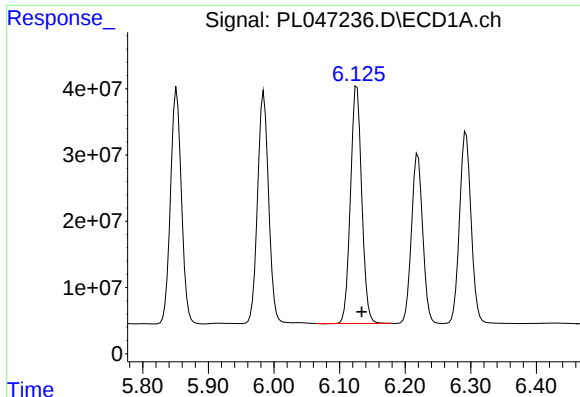

#15 Endosulfan II


R.T.: 6.127 min
Delta R.T.: -0.008 min
Response: 426467121
Conc: 47.60 ng/ml

Instrument :
ECD_L
ClientSampleId :

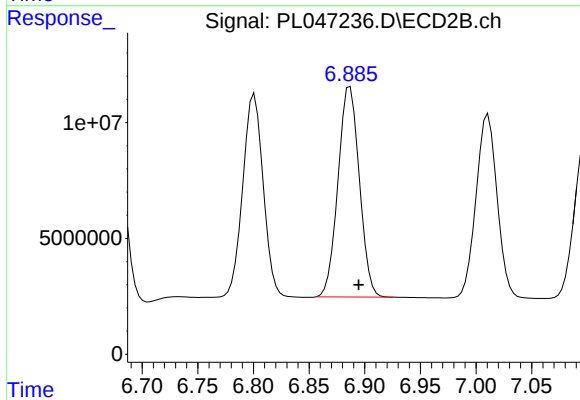


#15 Endosulfan II

R.T.: 6.887 min
Delta R.T.: -0.008 min
Response: 121130886
Conc: 50.20 ng/ml

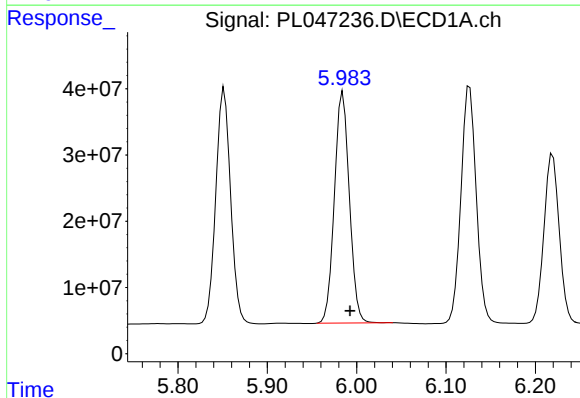


#16 4,4'-DDD

R.T.: 5.985 min
Delta R.T.: -0.008 min
Response: 406205329
Conc: 53.74 ng/ml

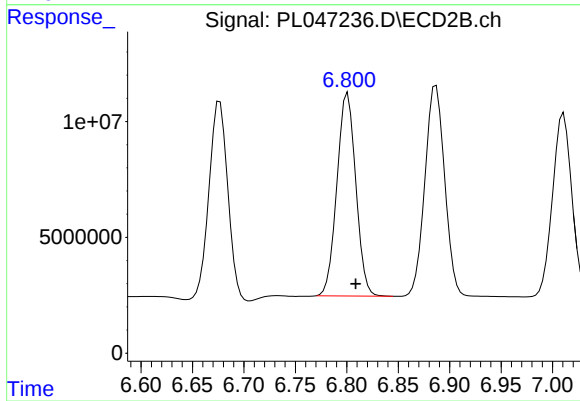

#16 4,4'-DDD


R.T.: 6.801 min
Delta R.T.: -0.008 min
Response: 111852608
Conc: 55.59 ng/ml

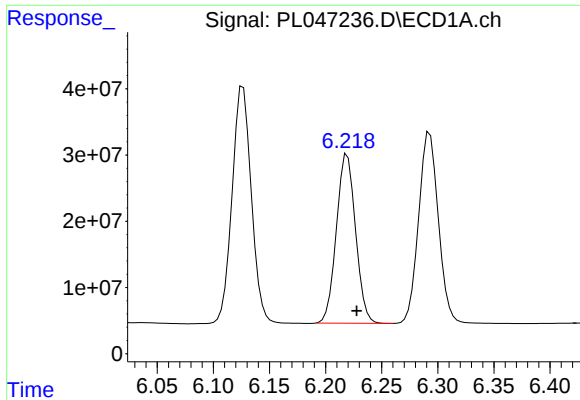

#17 4,4'-DDT


R.T.: 6.219 min
Delta R.T.: -0.008 min
Response: 303537605
Conc: 40.07 ng/ml

Instrument :
ECD_L
ClientSampleId :

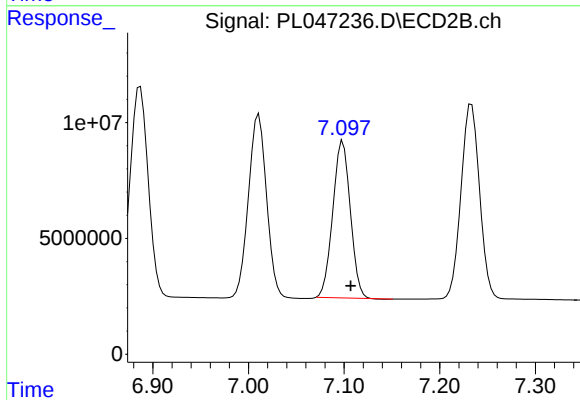


#17 4,4'-DDT

R.T.: 7.099 min
Delta R.T.: -0.008 min
Response: 86015536
Conc: 41.02 ng/ml

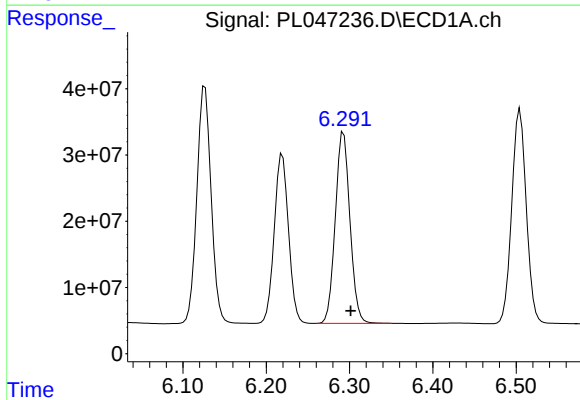


#18 Endrin aldehyde

R.T.: 6.293 min
Delta R.T.: -0.009 min
Response: 353725455
Conc: 47.19 ng/ml

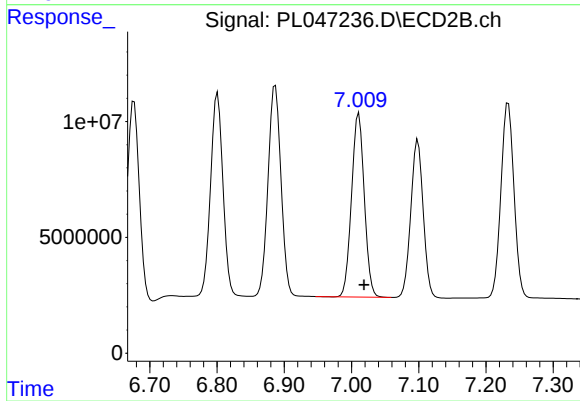

#18 Endrin aldehyde


R.T.: 7.011 min
Delta R.T.: -0.008 min
Response: 104572874
Conc: 49.23 ng/ml

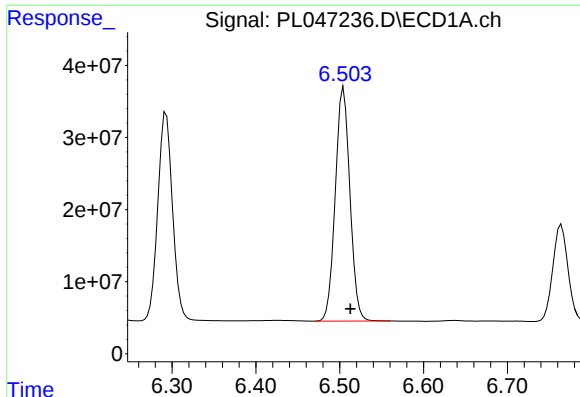

#19 Endosulfan Sulfate


R.T.: 6.505 min
Delta R.T.: -0.008 min
Response: 392811734
Conc: 47.84 ng/ml

Instrument :
ECD_L
ClientSampleId :

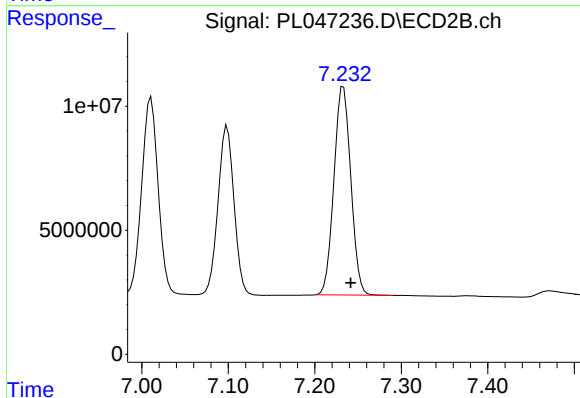


#19 Endosulfan Sulfate

R.T.: 7.233 min
Delta R.T.: -0.008 min
Response: 113404355
Conc: 48.07 ng/ml

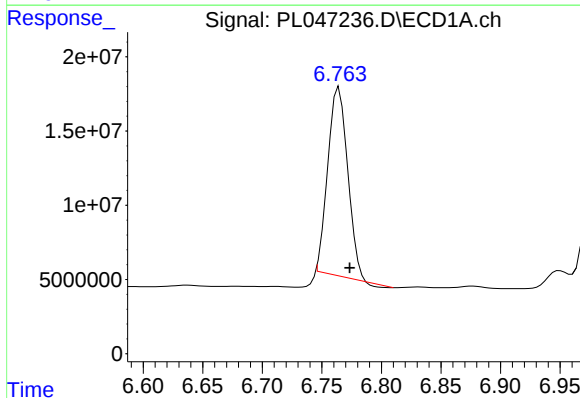


#20 Methoxychlor

R.T.: 6.764 min
Delta R.T.: -0.009 min
Response: 146260922
Conc: 34.42 ng/ml

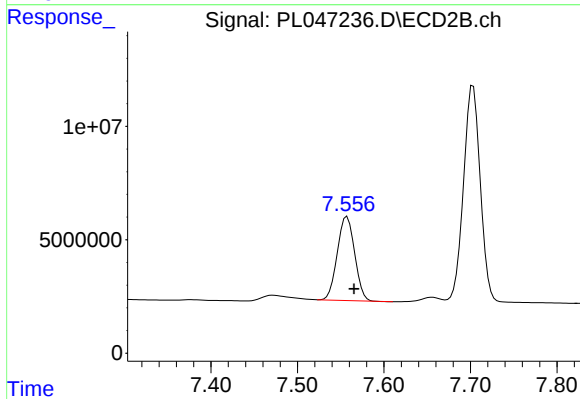

#20 Methoxychlor


R.T.: 7.557 min
Delta R.T.: -0.008 min
Response: 51321571
Conc: 40.26 ng/ml

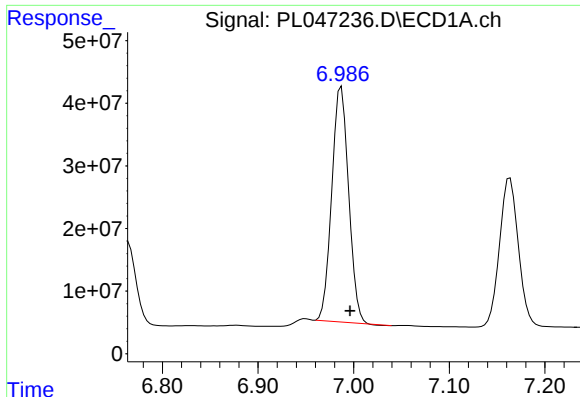

#21 Endrin ketone


R.T.: 6.987 min
Delta R.T.: -0.009 min
Response: 458585792
Conc: 49.59 ng/ml

Instrument :
ECD_L
ClientSampleId :

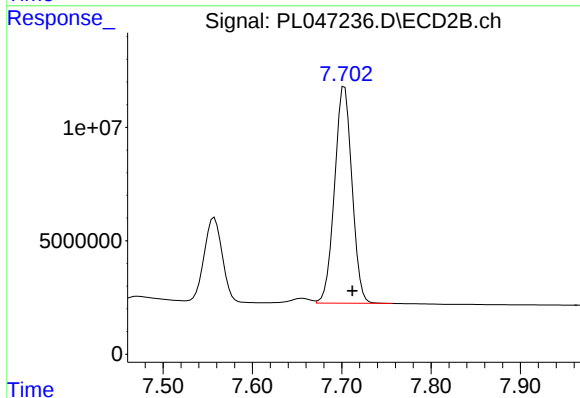


#21 Endrin ketone

R.T.: 7.703 min
Delta R.T.: -0.009 min
Response: 129243573
Conc: 52.02 ng/ml

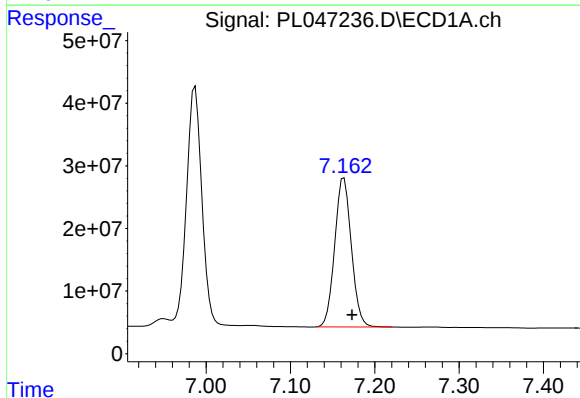


#22 Mirex

R.T.: 7.163 min
Delta R.T.: -0.010 min
Response: 326586405
Conc: 44.83 ng/ml

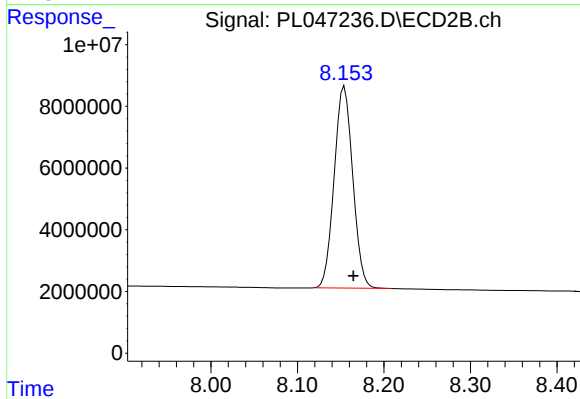

#22 Mirex


R.T.: 8.154 min
Delta R.T.: -0.010 min
Response: 97059411
Conc: 48.53 ng/ml

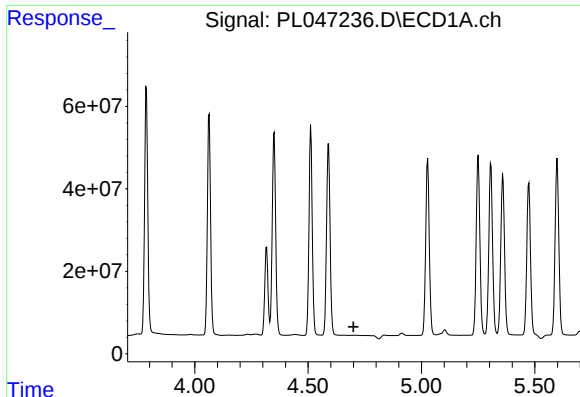

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 4.701 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

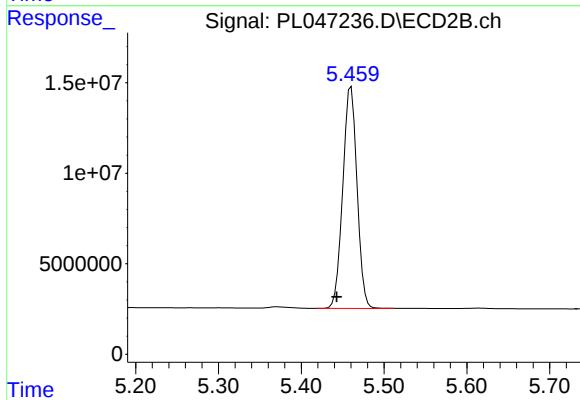


#24 Chlordane-2

R.T.: 5.460 min
Delta R.T.: 0.017 min
Response: 147014102
Conc: 1258.58 ng/ml

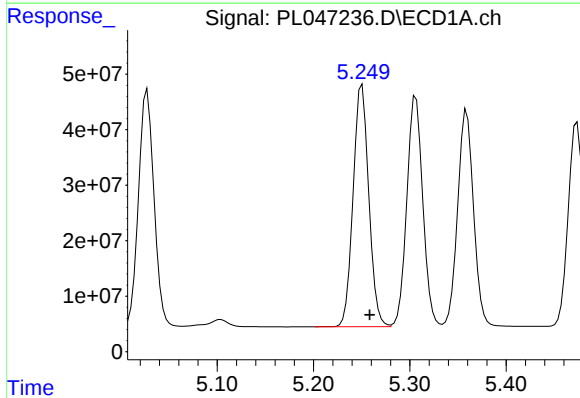


#25 Chlordane-3

R.T.: 5.250 min
Delta R.T.: -0.008 min
Response: 491941398
Conc: 441.73 ng/ml

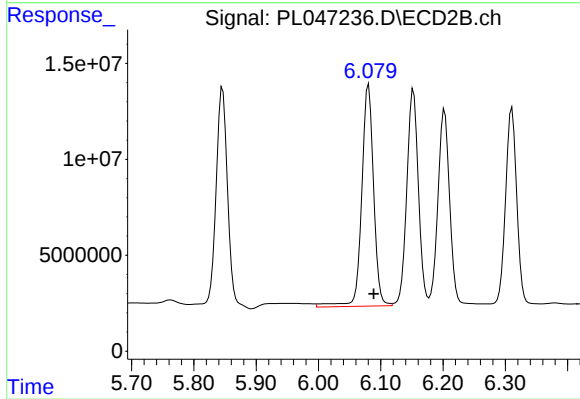

#25 Chlordane-3


R.T.: 6.081 min
Delta R.T.: -0.008 min
Response: 153668406
Conc: 403.05 ng/ml

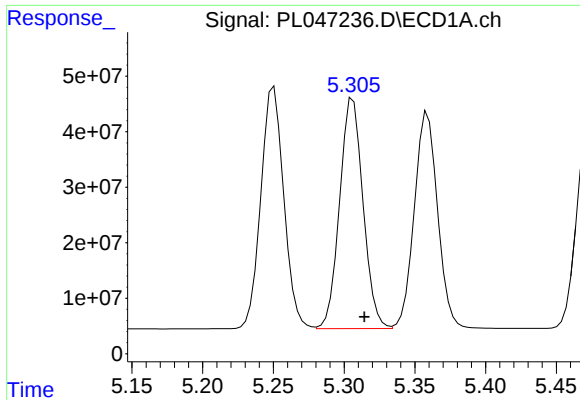

#26 Chlordane-4


R.T.: 5.306 min
Delta R.T.: -0.008 min
Response: 479346992
Conc: 463.56 ng/ml

Instrument :
ECD_L
ClientSampleId :

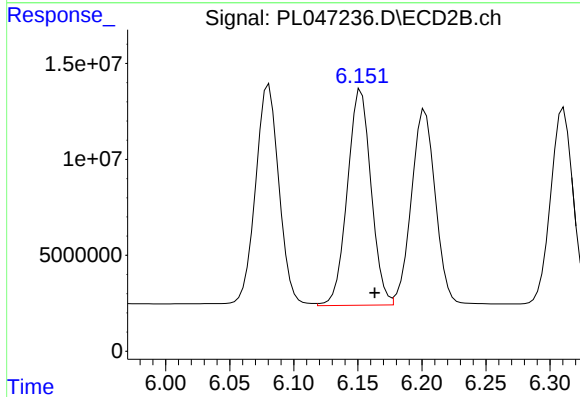


#26 Chlordane-4

R.T.: 6.153 min
Delta R.T.: -0.011 min
Response: 144924935
Conc: 314.08 ng/ml

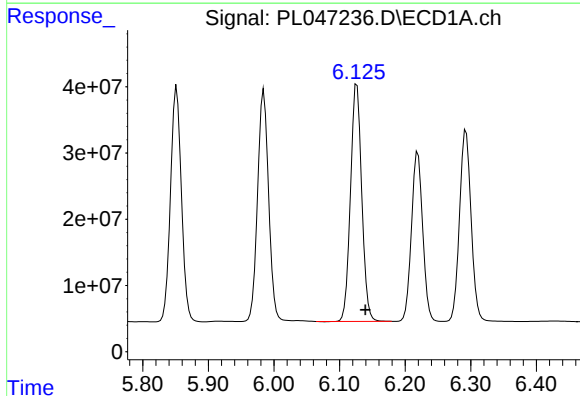


#27 Chlordane-5

R.T.: 6.127 min
Delta R.T.: -0.013 min
Response: 426467121
Conc: 1249.66 ng/ml

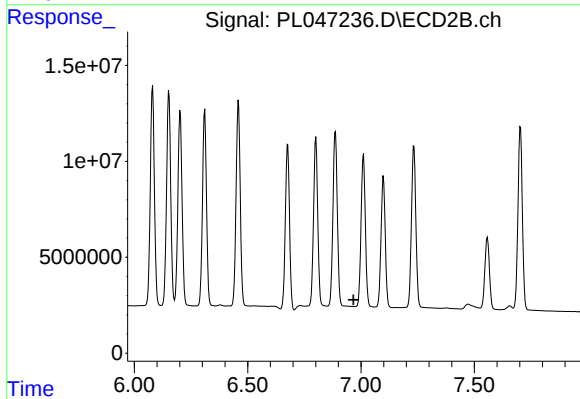

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.967 min
Response: 0
Conc: N.D.

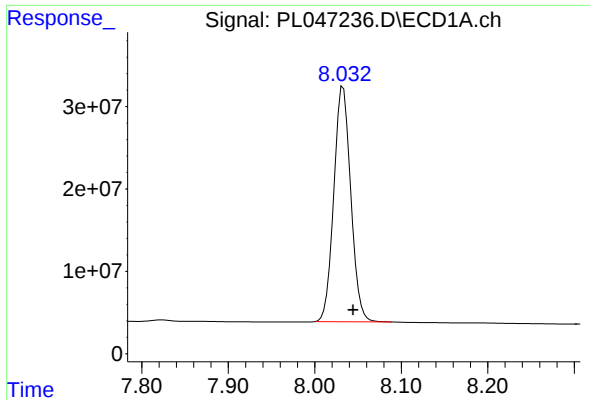

#28 Decachlorobiphenyl

R.T.: 8.033 min
Delta R.T.: -0.011 min
Response: 387570416
Conc: 46.08 ng/ml

Instrument :
ECD_L
ClientSampleId :

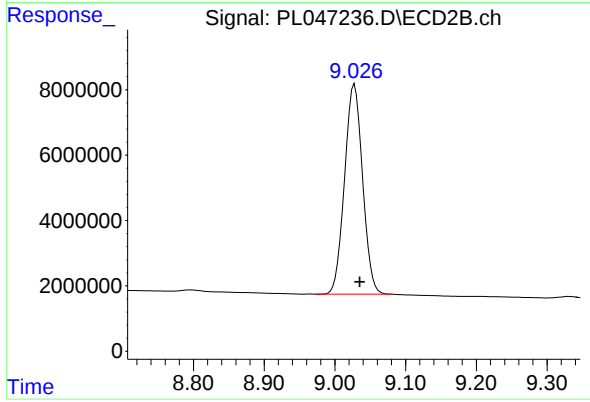

#28 Decachlorobiphenyl

R.T.: 9.028 min
Delta R.T.: -0.007 min
Response: 113914311
Conc: 49.13 ng/ml