

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041019\
 Data File : PL047241.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Apr 2019 03:16
 Operator : AJ\SJ
 Sample : K2311-02
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 0168-SITE-WATER

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 11 04:54:43 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:40:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.357	3.976	133.6E6	44771273	18.363	19.554
28)	SA Decachlor...	8.033	9.028	165.9E6	48868892	19.719	21.078
Target Compounds							
2)	A alpha-BHC	3.777	4.393f	11521387	3707217	0.988	1.154
3)	MA gamma-BHC...	4.073	4.666	3631429	2956208	0.338	0.988 #
4)	MA Heptachlor	0.000	5.146f	0	2518990	N.D.	0.819 #
9)	A Endosulfan I	0.000	6.239f	0	3671671	N.D.	1.407 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041019\
Data File : PL047241.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Apr 2019 03:16
Operator : AJ\SJ
Sample : K2311-02
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
0168-SITE-WATER

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 11 04:54:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

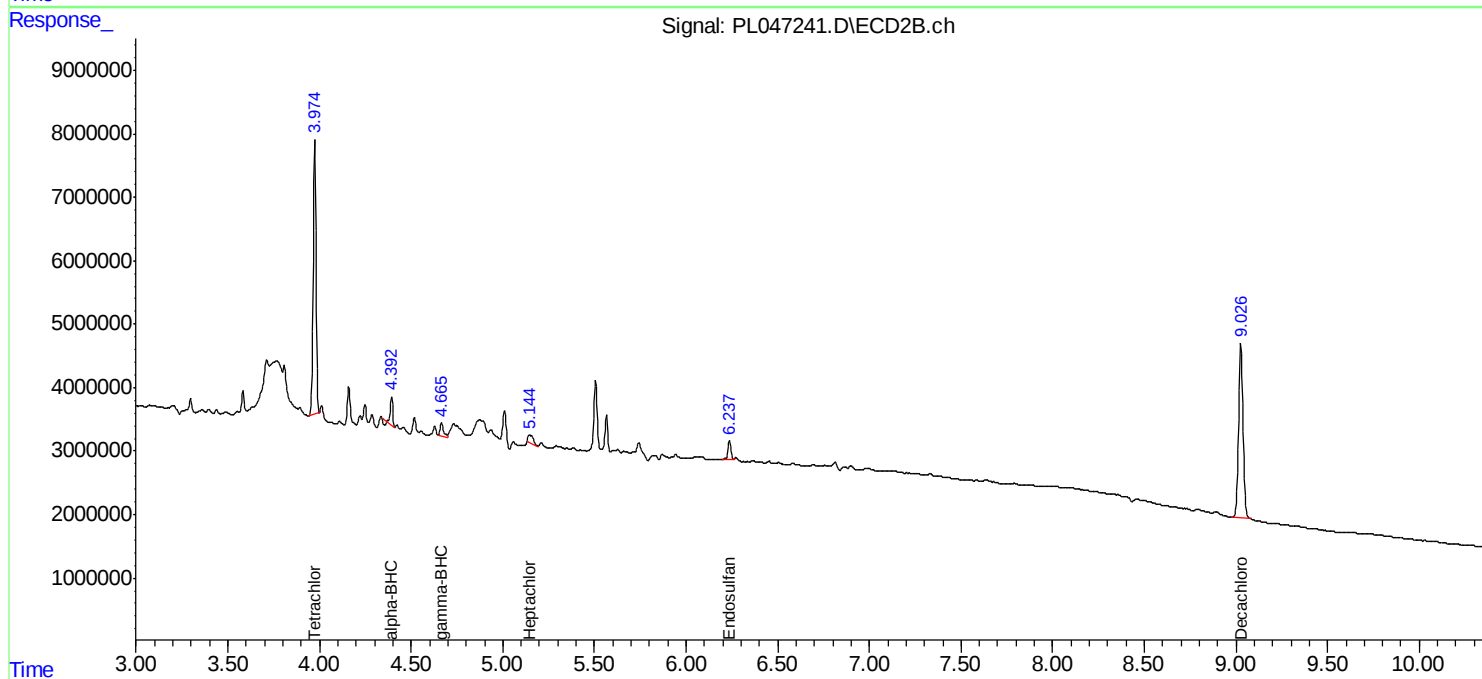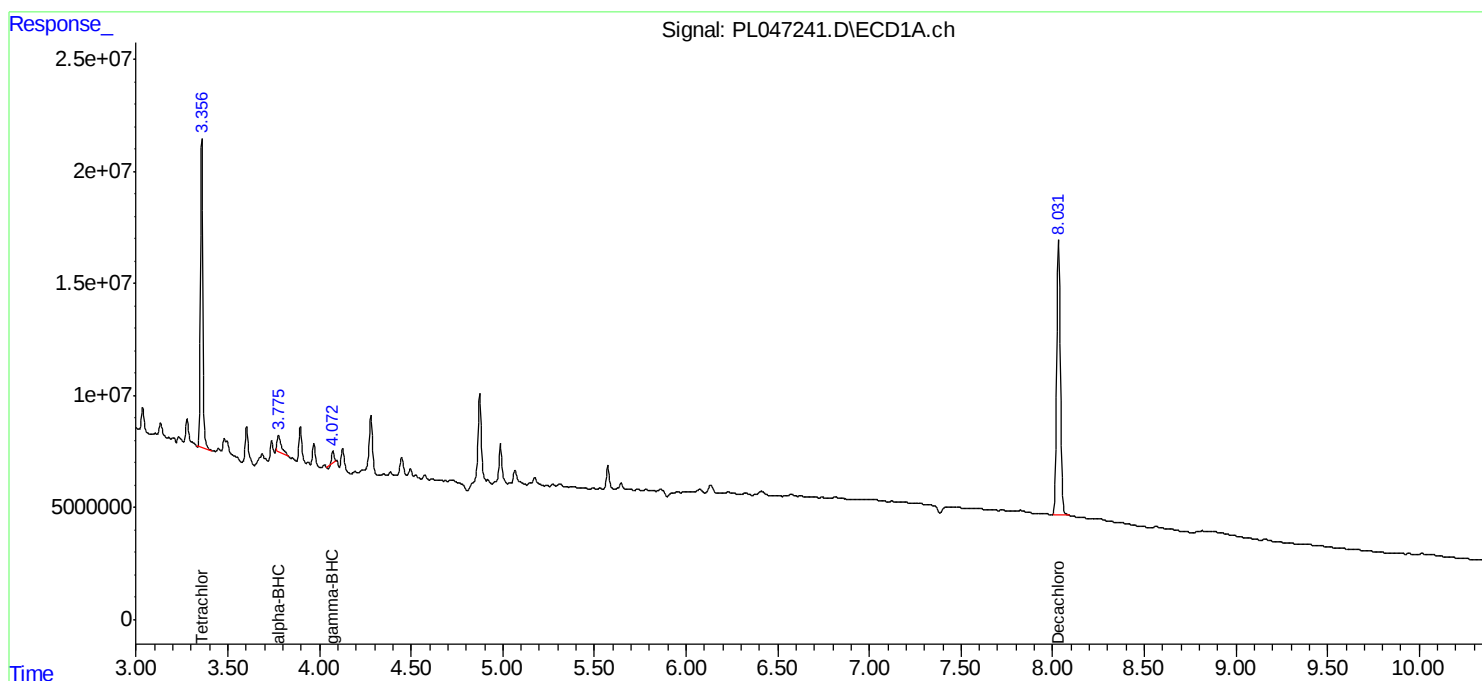


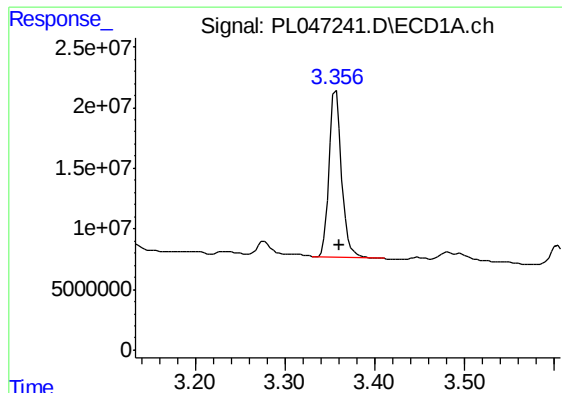

#1 Tetrachloro-m-xylene


R.T.: 3.357 min
Delta R.T.: -0.004 min
Response: 133582840
Conc: 18.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
0168-SITE-WATER

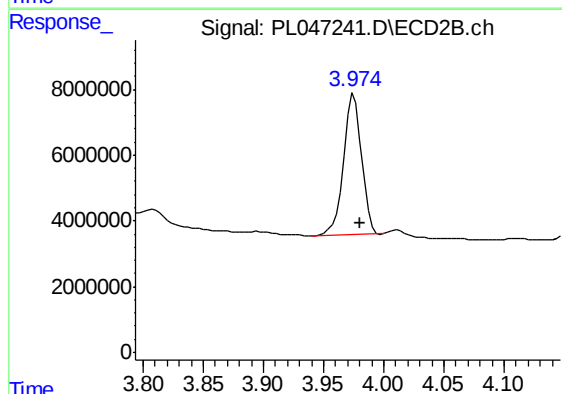


#1 Tetrachloro-m-xylene

R.T.: 3.976 min
Delta R.T.: -0.005 min
Response: 44771273
Conc: 19.55 ng/ml

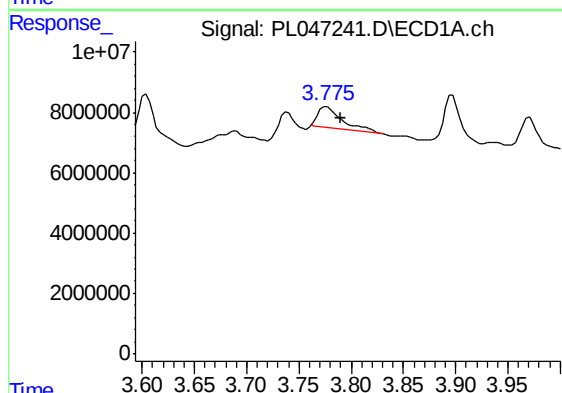


#2 alpha-BHC

R.T.: 3.777 min
Delta R.T.: -0.014 min
Response: 11521387
Conc: 0.99 ng/ml

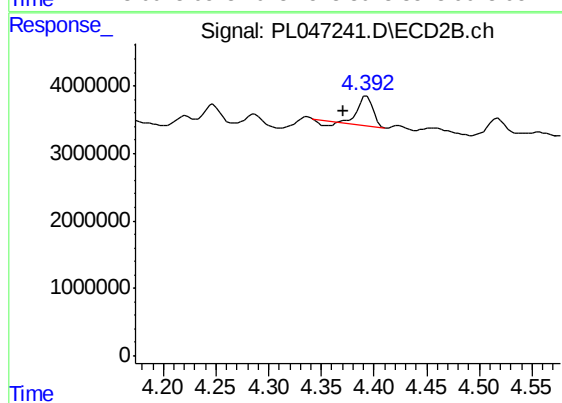

#2 alpha-BHC


R.T.: 4.393 min
Delta R.T.: 0.022 min
Response: 3707217
Conc: 1.15 ng/ml

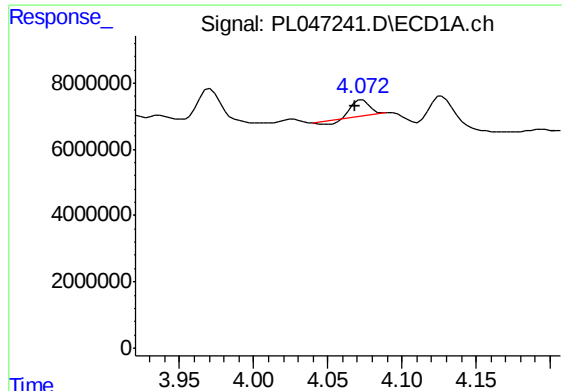

#3 gamma-BHC (Lindane)


R.T.: 4.073 min
Delta R.T.: 0.005 min
Response: 3631429
Conc: 0.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
0168-SITE-WATER

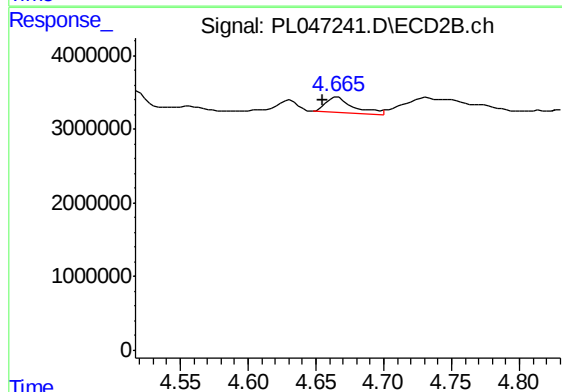


#3 gamma-BHC (Lindane)

R.T.: 4.666 min
Delta R.T.: 0.011 min
Response: 2956208
Conc: 0.99 ng/ml

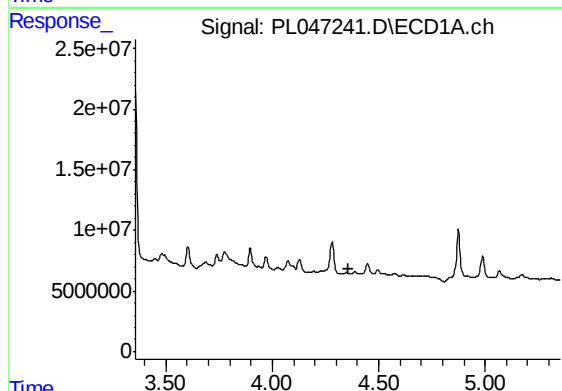


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.356 min
Response: 0
Conc: N.D.

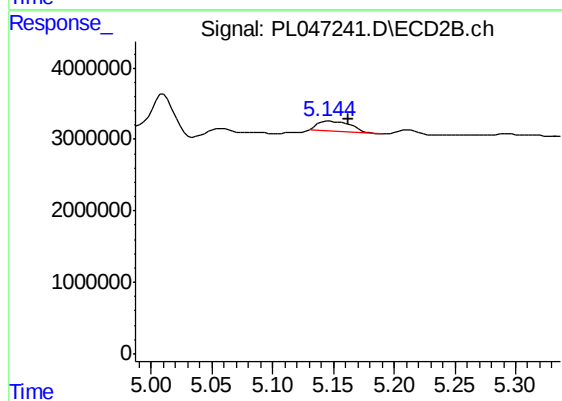

#4 Heptachlor


R.T.: 5.146 min
Delta R.T.: -0.017 min
Response: 2518990
Conc: 0.82 ng/ml

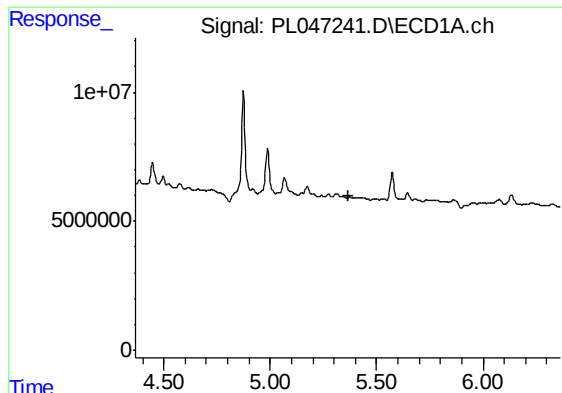

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.366 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
0168-SITE-WATER

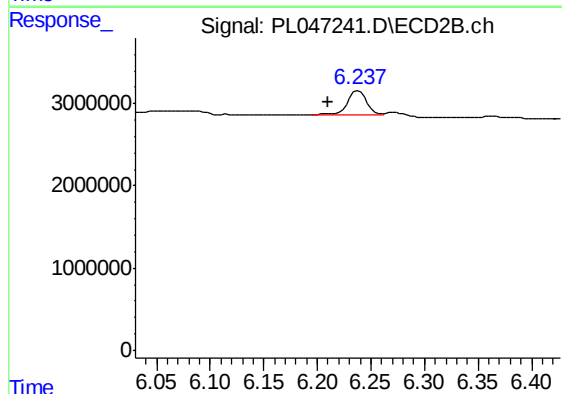


#9 Endosulfan I

R.T.: 6.239 min
Delta R.T.: 0.028 min
Response: 3671671
Conc: 1.41 ng/ml

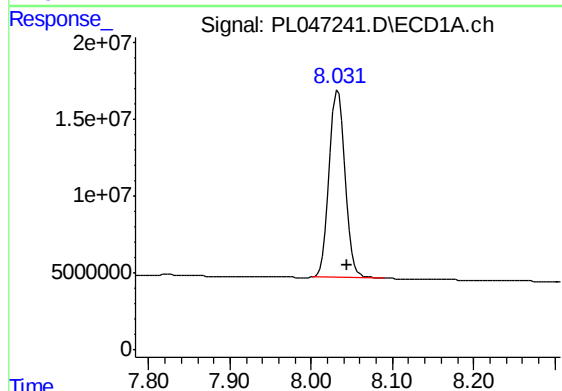

#28 Decachlorobiphenyl

R.T.: 8.033 min
Delta R.T.: -0.011 min
Response: 165856496
Conc: 19.72 ng/ml

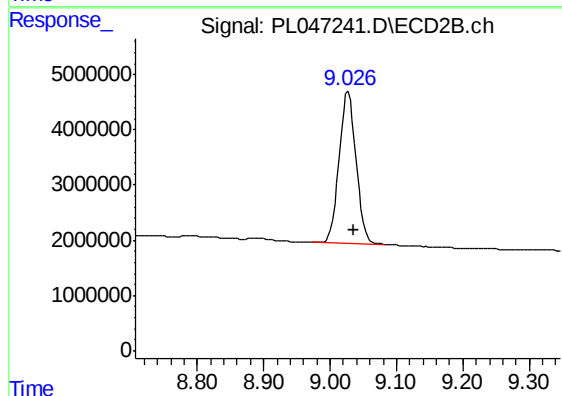

#28 Decachlorobiphenyl

R.T.: 9.028 min
Delta R.T.: -0.007 min
Response: 48868892
Conc: 21.08 ng/ml