

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041019\
 Data File : PL047249.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Apr 2019 05:10
 Operator : AJ\SJ
 Sample : K2343-03
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-7-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 11 05:58:09 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:40:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.357	3.975	141.9E6	45872996	19.501	20.035
28)	SA Decachlor...	8.033	9.028	134.3E6	42384490	15.964	18.281
Target Compounds							
3)	MA gamma-BHC...	4.071	0.000	9635007	0	0.897	N.D. #
9)	A Endosulfan I	5.389f	0.000	26737101	0	2.844	N.D. #
10)	B gamma-Chl...	0.000	6.069f	0	4573357	N.D.	1.611 #
20)	A Methoxychlor	6.802f	0.000	9018429	0	2.122	N.D. #
25)	Chlordane-3	0.000	6.069f	0	4573357	N.D.	11.995 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041019\
Data File : PL047249.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Apr 2019 05:10
Operator : AJ\SJ
Sample : K2343-03
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-7-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 11 05:58:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

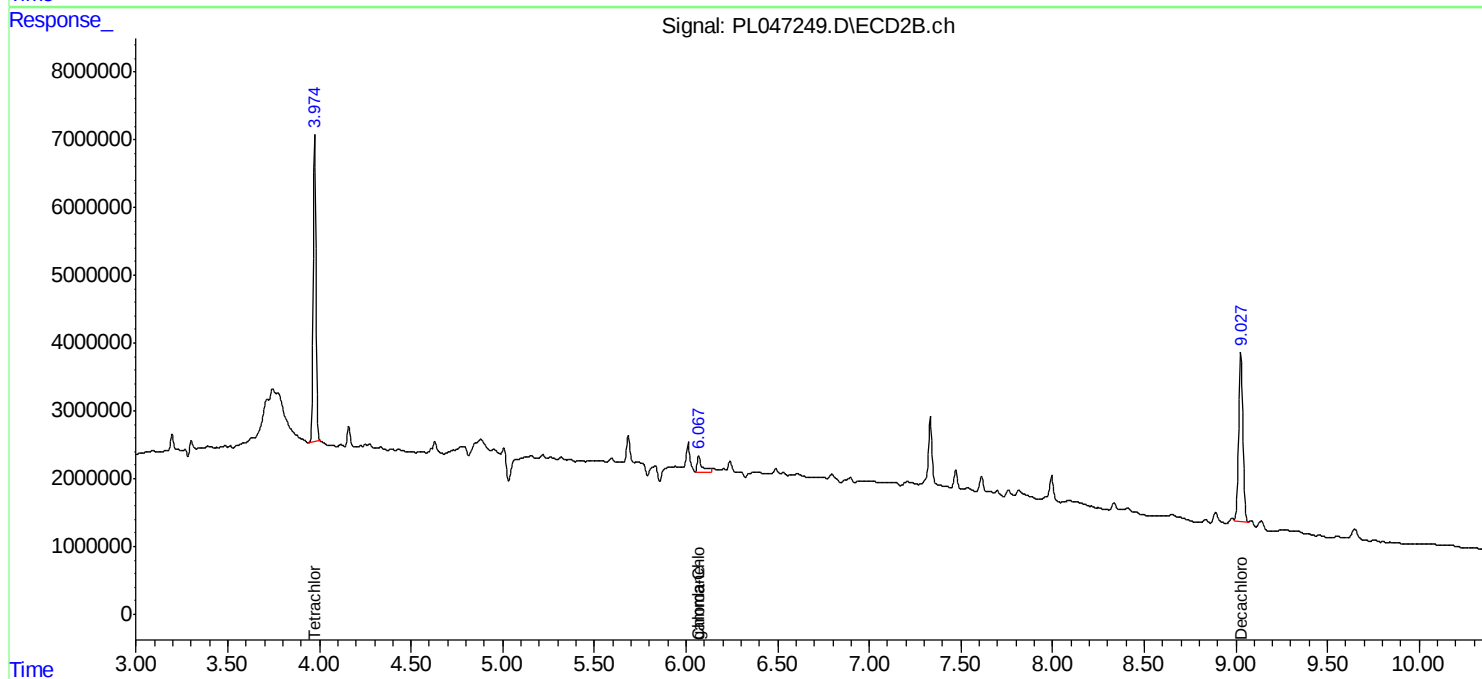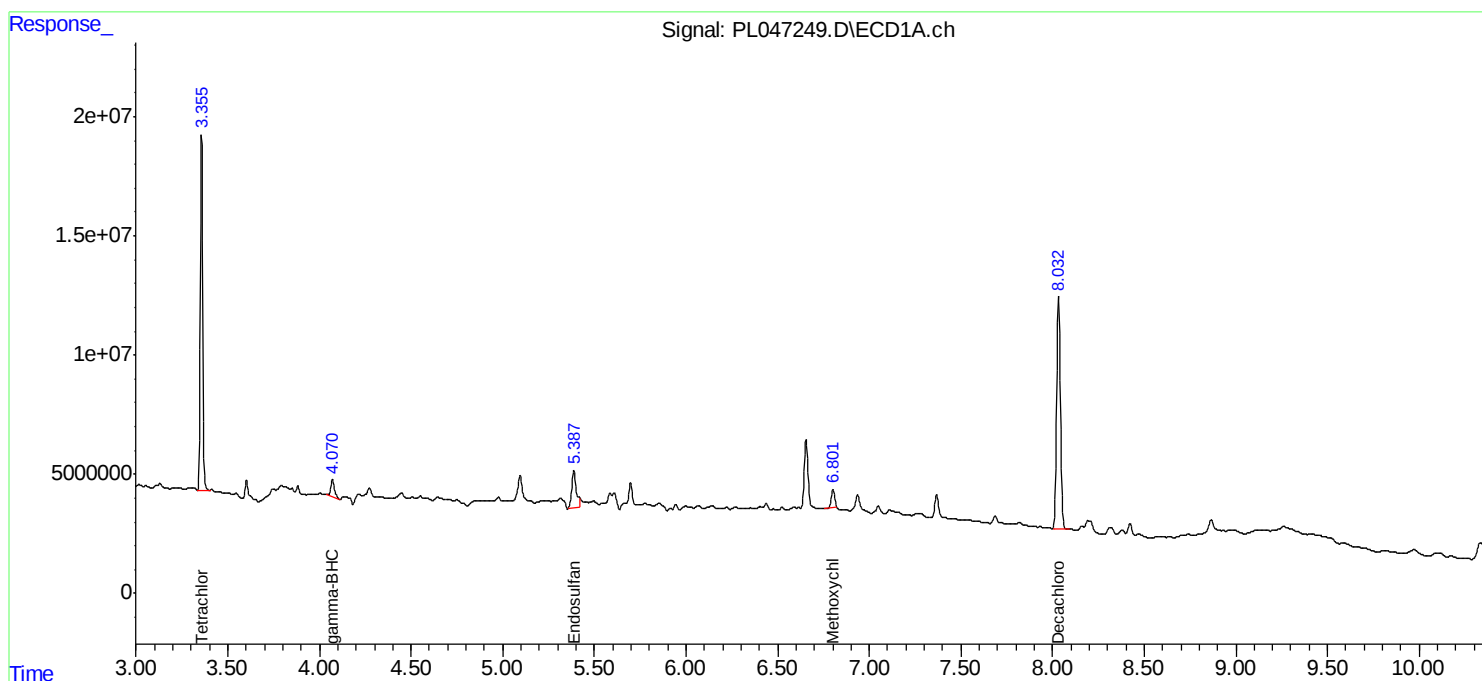


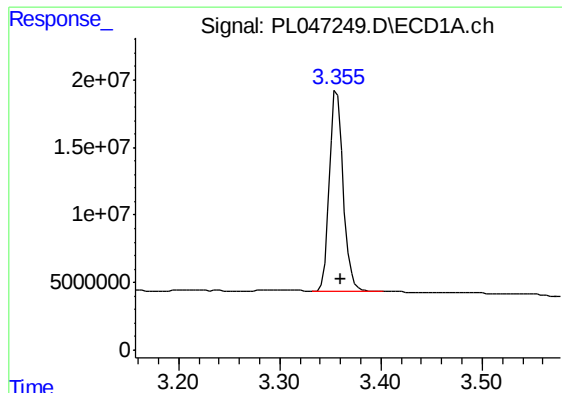

#1 Tetrachloro-m-xylene


R.T.: 3.357 min
Delta R.T.: -0.004 min
Response: 141861261
Conc: 19.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-7-S

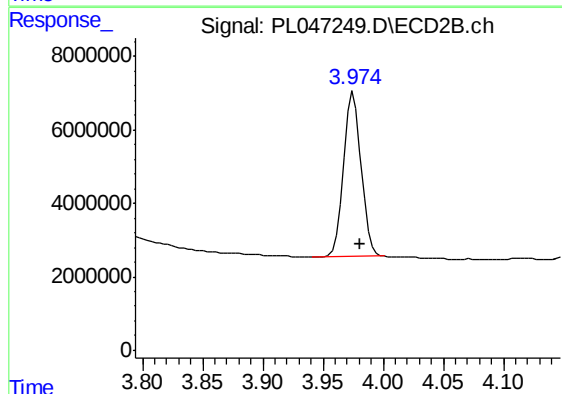


#1 Tetrachloro-m-xylene

R.T.: 3.975 min
Delta R.T.: -0.005 min
Response: 45872996
Conc: 20.04 ng/ml

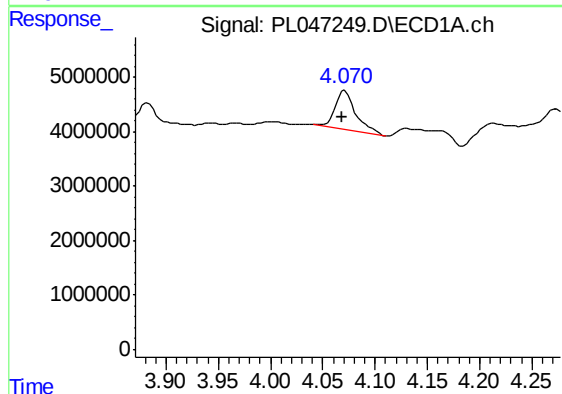


#3 gamma-BHC (Lindane)

R.T.: 4.071 min
Delta R.T.: 0.003 min
Response: 9635007
Conc: 0.90 ng/ml

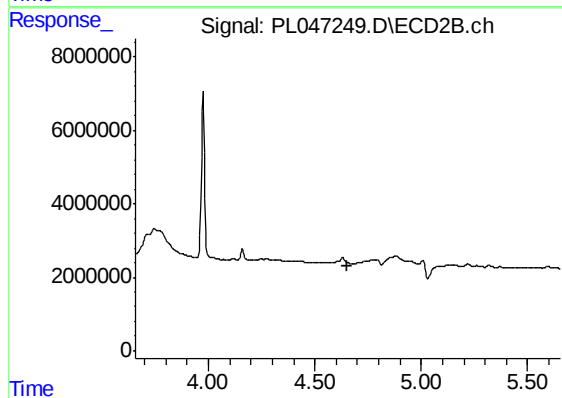

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.656 min
Response: 0
Conc: N.D.

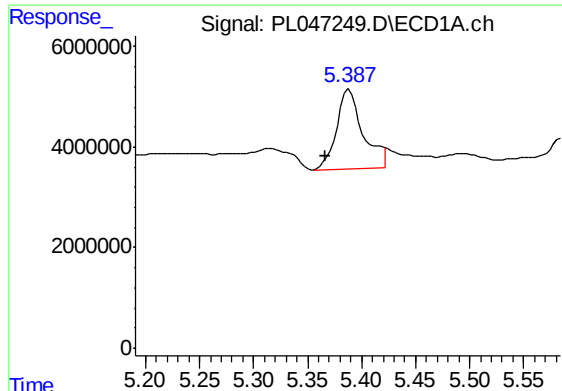

#9 Endosulfan I


R.T.: 5.389 min
Delta R.T.: 0.022 min
Response: 26737101
Conc: 2.84 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-7-S

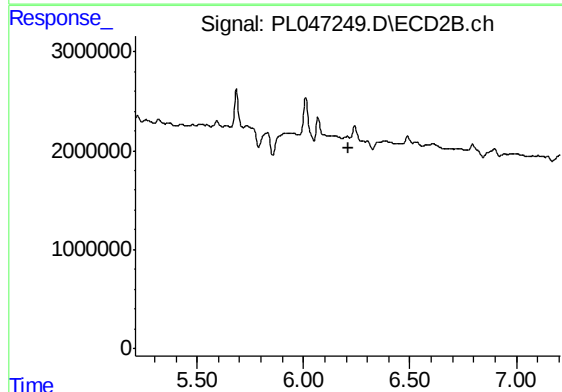


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.210 min
Response: 0
Conc: N.D.

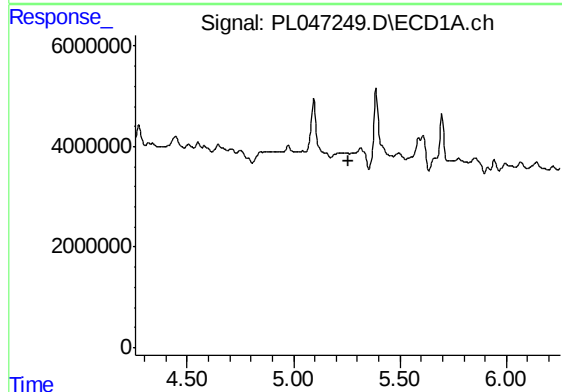


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.257 min
Response: 0
Conc: N.D.

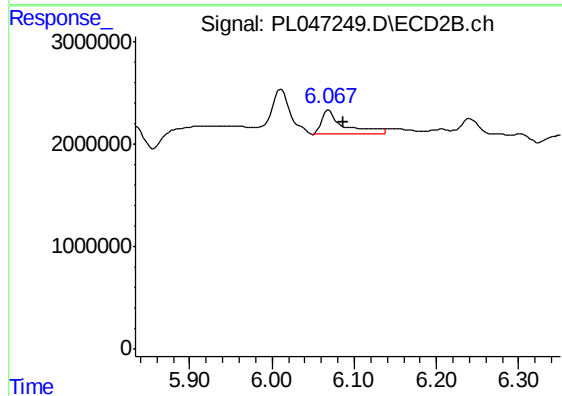

#10 gamma-Chlordane


R.T.: 6.069 min
Delta R.T.: -0.019 min
Response: 4573357
Conc: 1.61 ng/ml

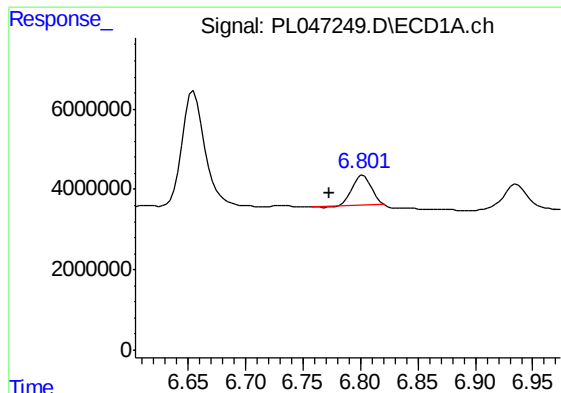

#20 Methoxychlor


R.T.: 6.802 min
Delta R.T.: 0.029 min
Response: 9018429
Conc: 2.12 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-7-S

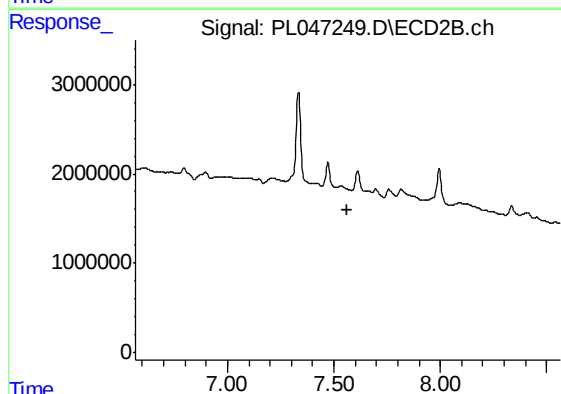


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.565 min
Response: 0
Conc: N.D.

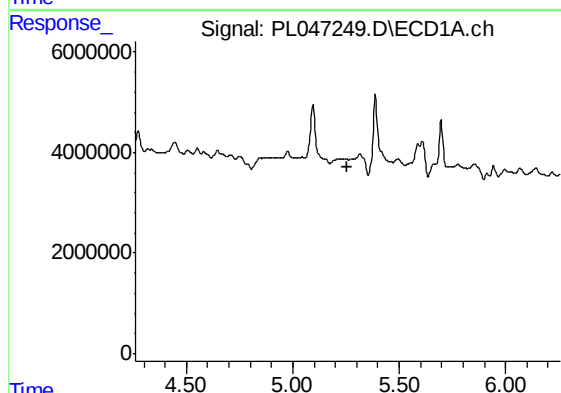


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.258 min
Response: 0
Conc: N.D.

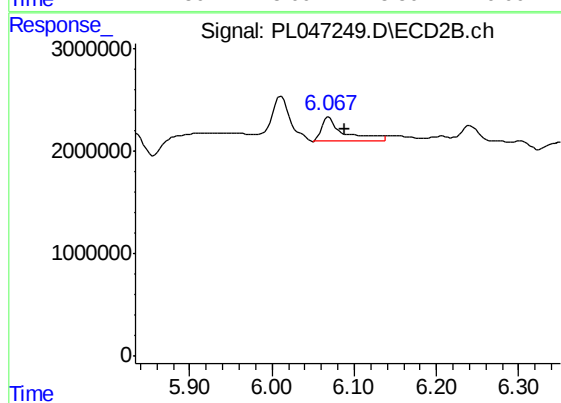

#25 Chlordane-3


R.T.: 6.069 min
Delta R.T.: -0.020 min
Response: 4573357
Conc: 12.00 ng/ml

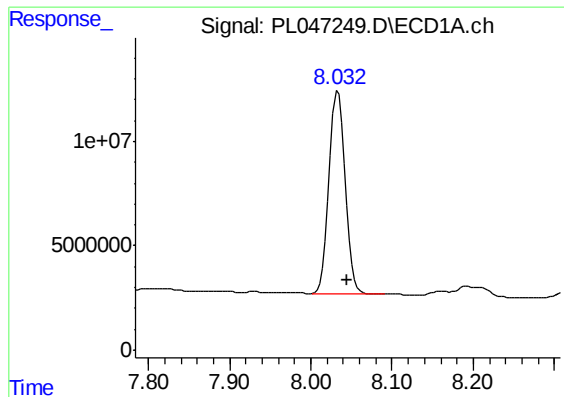

#28 Decachlorobiphenyl

R.T.: 8.033 min
Delta R.T.: -0.011 min
Response: 134272494
Conc: 15.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-7-S

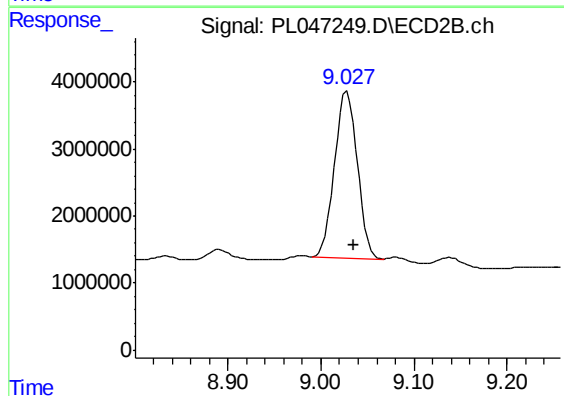

#28 Decachlorobiphenyl

R.T.: 9.028 min
Delta R.T.: -0.007 min
Response: 42384490
Conc: 18.28 ng/ml