

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041019\
 Data File : PL047183.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Apr 2019 10:57
 Operator : AJ\SJ
 Sample : K2316-14
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SPLP-LEACHATE-AMND-CS-4

Manual Integrations
 APPROVED

mohammad
 4/11/2019 3:55:13 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 11 01:01:58 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:40:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.358	3.977	120.2E6	51801668	16.524	22.625 #
28)	SA Decachlor...	8.036	9.031	119.3E6	31948369	14.187	13.780m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041019\
Data File : PL047183.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Apr 2019 10:57
Operator : AJ\SJ
Sample : K2316-14
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SPLP-LEACHATE-AMND-CS-4


Manual Integrations
APPROVED

mohammad
4/11/2019 3:55:13 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 11 01:01:58 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

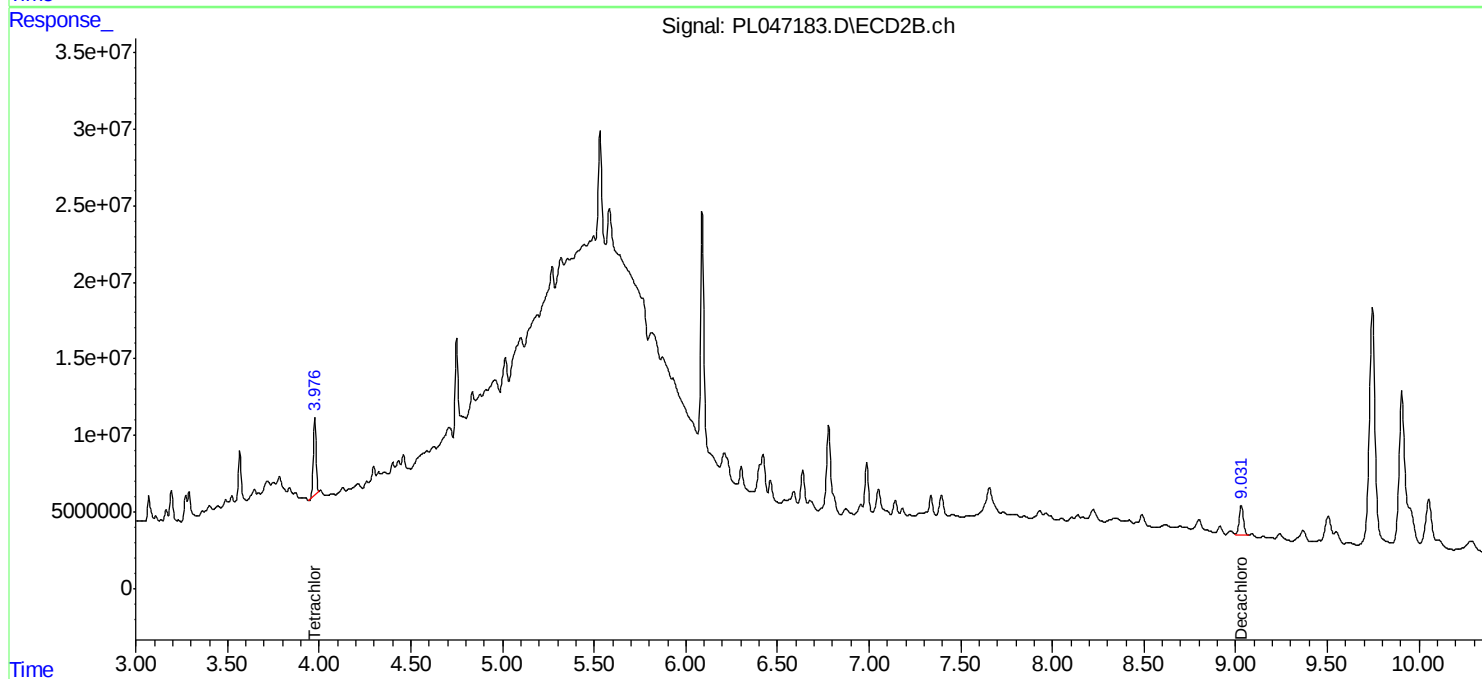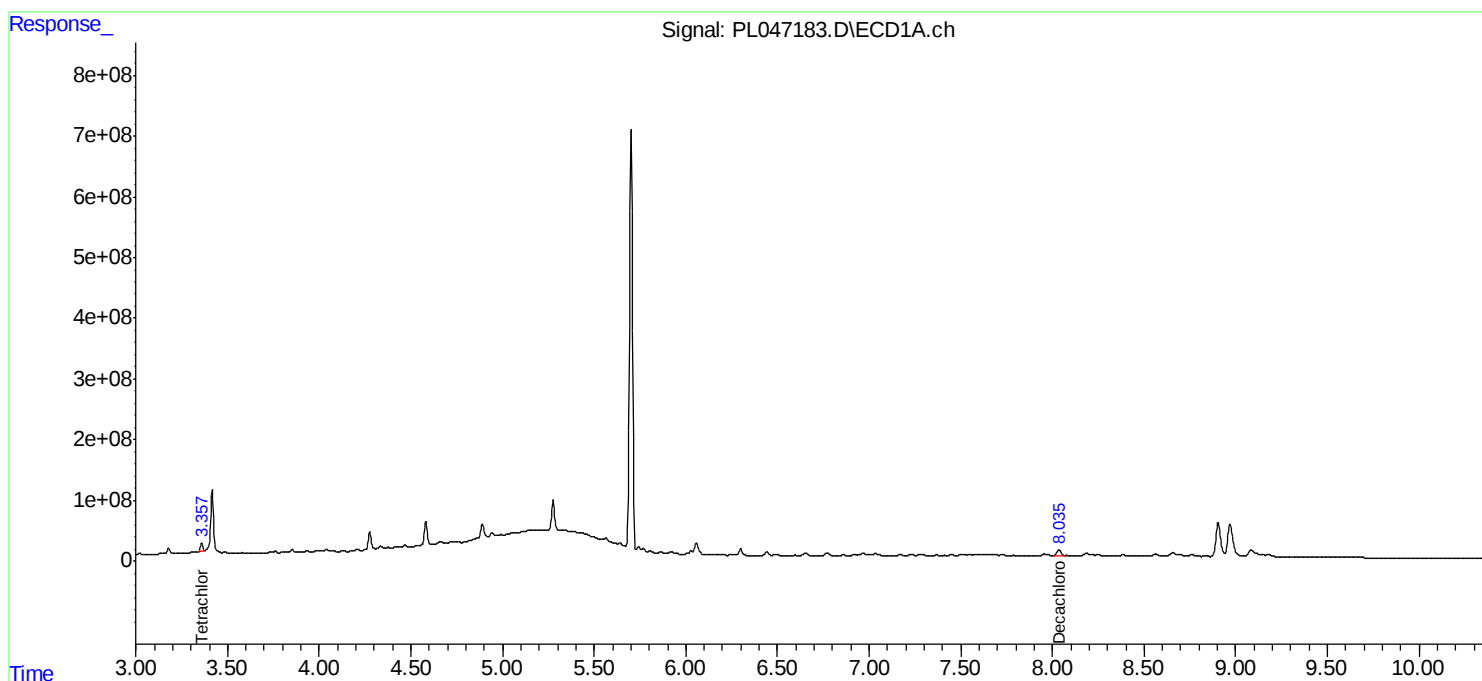

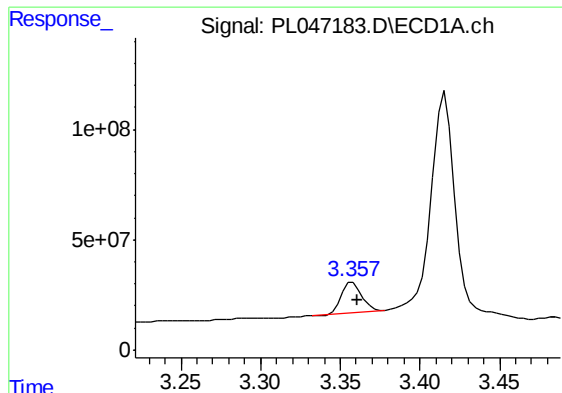


#1 Tetrachloro-m-xylene

R.T.: 3.358 min
Delta R.T.: -0.003 min
Response: 120206744
Conc: 16.52 ng/ml

Instrument :
ECD_L
ClientSampleId :
SPLP-LEACHATE-AMND-CS-4


Manual Integrations
APPROVED

mohammad
4/11/2019 3:55:13 PM

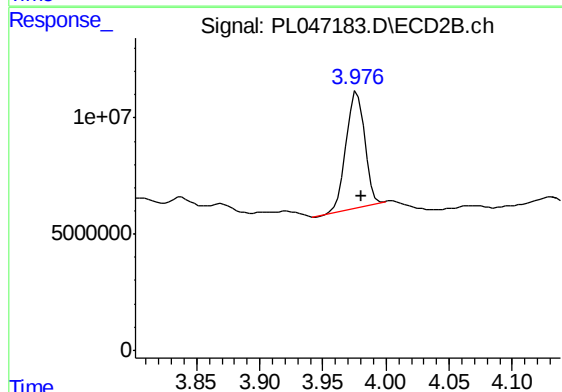


#1 Tetrachloro-m-xylene

R.T.: 3.977 min
Delta R.T.: -0.004 min
Response: 51801668
Conc: 22.62 ng/ml

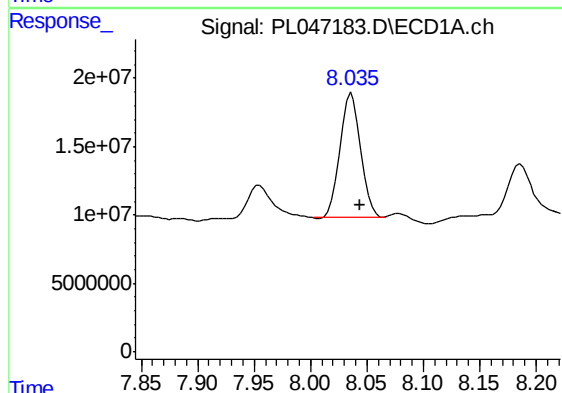

#28 Decachlorobiphenyl

R.T.: 8.036 min
Delta R.T.: -0.008 min
Response: 119326530
Conc: 14.19 ng/ml

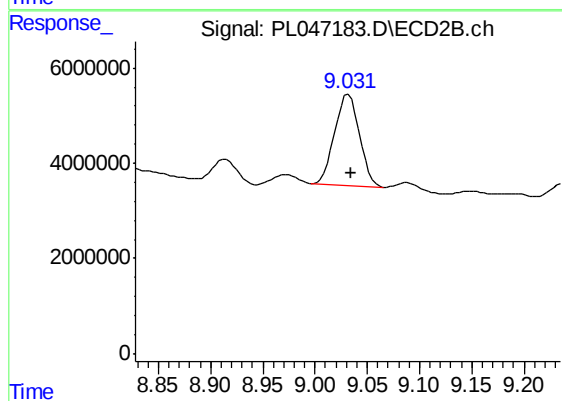

#28 Decachlorobiphenyl

R.T.: 9.031 min
Delta R.T.: -0.004 min
Response: 31948369
Conc: 13.78 ng/ml m